

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ122223\
 Data File : PQ064738.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2023 13:39
 Operator : YP\AJ
 Sample : 05897-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 GHL-SS-35aRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/26/2023
 Supervised By :Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 22:23:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ122123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 22 03:53:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.459	2.772	49574508	60566933	11.622	11.734
2) SA Decachlor...	8.696	7.568	11707415	15391764	3.360m	3.166

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ122223\
Data File : PQ064738.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2023 13:39
Operator : YP\AJ
Sample : 05897-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
GHL-SS-35aRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 22:23:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ122123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 22 03:53:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

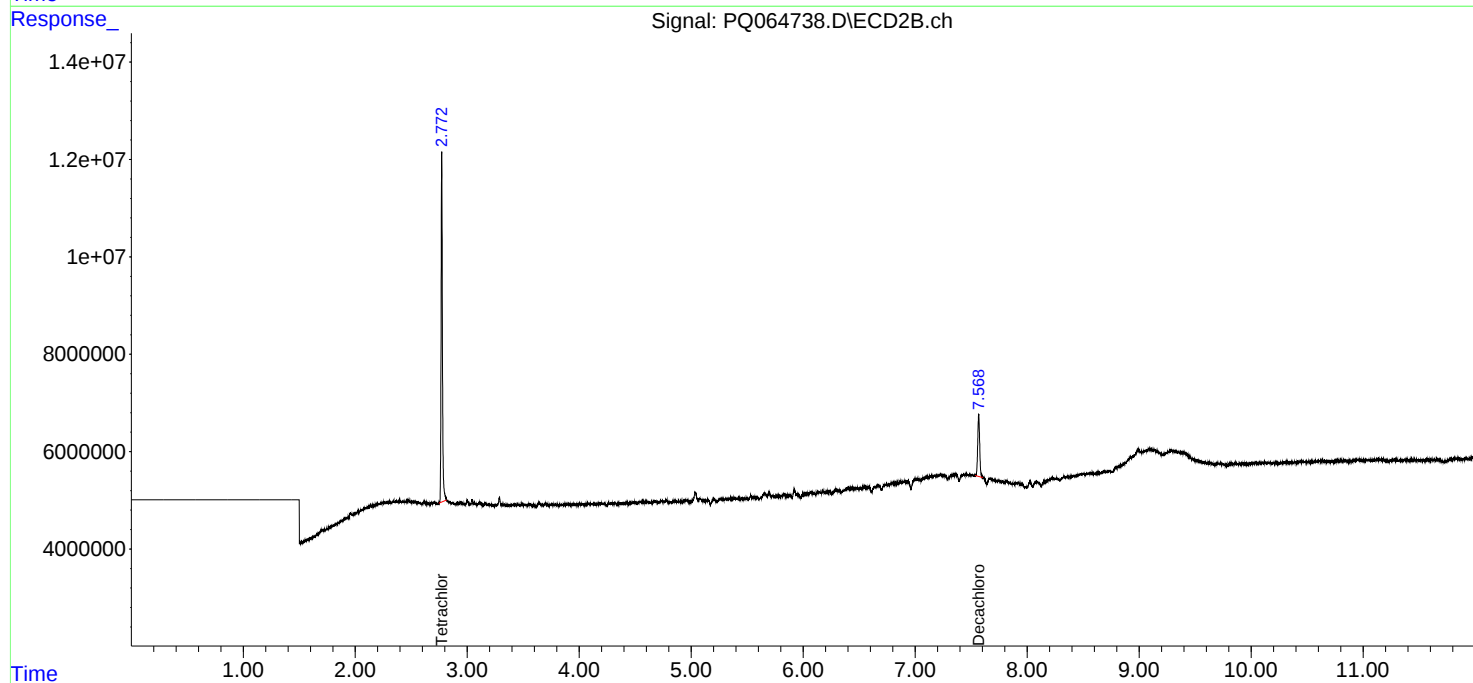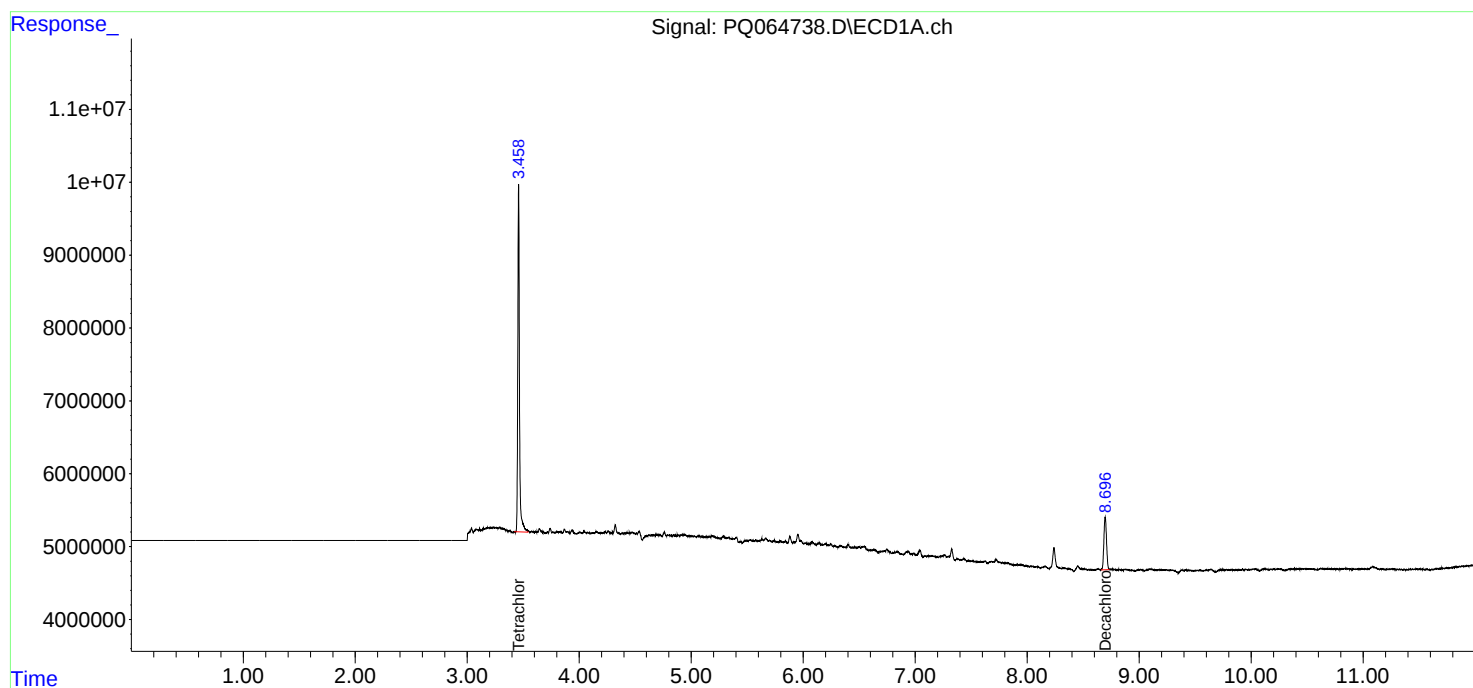

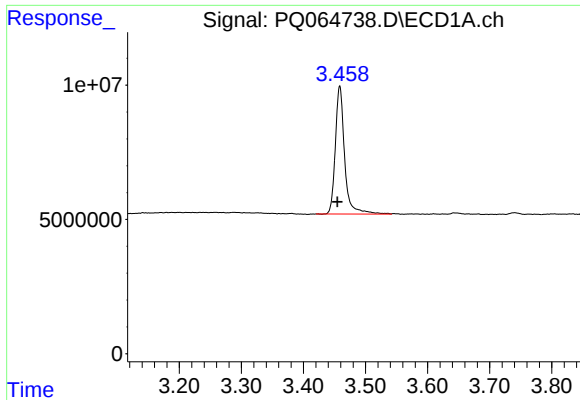


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.004 min
Response: 49574508
Conc: 11.62 ng/ml

Instrument :
ECD_Q
ClientSampleId :
GHL-SS-35aRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2023
Supervised By :Ankita Jodhani 12/26/2023

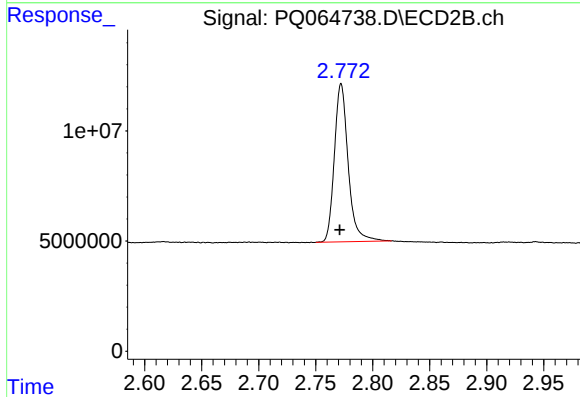


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.001 min
Response: 60566933
Conc: 11.73 ng/ml

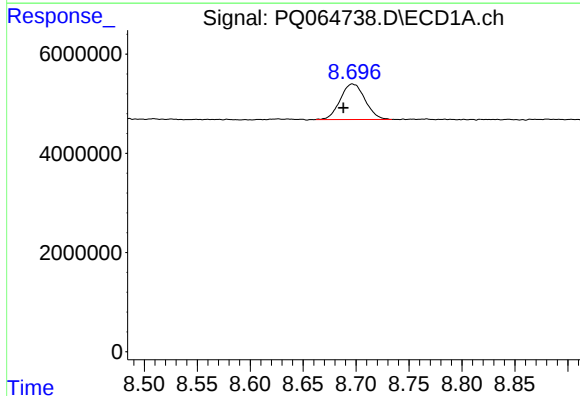

#2 Decachlorobiphenyl

R.T.: 8.696 min
Delta R.T.: 0.008 min
Response: 11707415
Conc: 3.36 ng/ml m

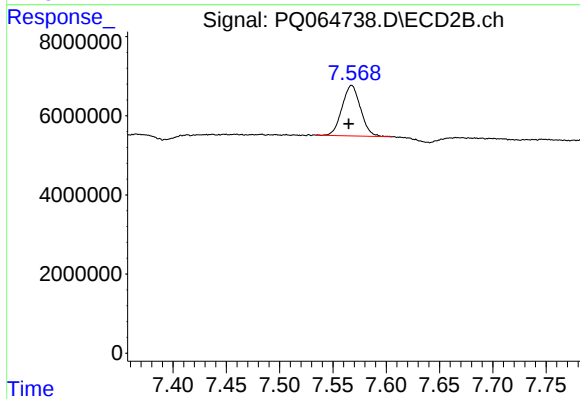

#2 Decachlorobiphenyl

R.T.: 7.568 min
Delta R.T.: 0.003 min
Response: 15391764
Conc: 3.17 ng/ml