



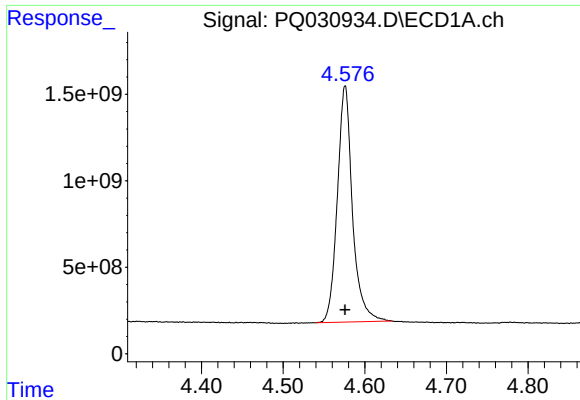

#1 Tetrachloro-m-xylene

R.T.: 4.576 min
Delta R.T.: 0.000 min
Response: 17628034174
Conc: 85.30 ng/ml

Instrument :
ECD_Q
ClientSampleId :

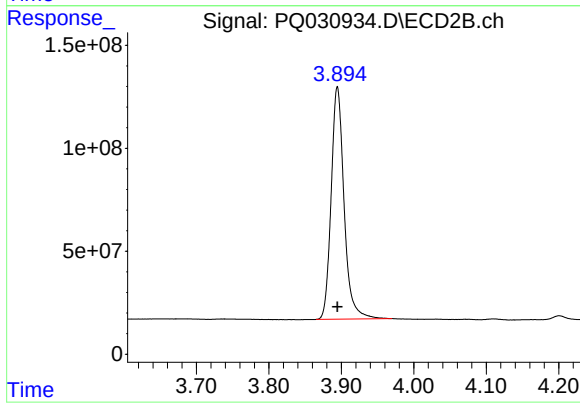

#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 1396477673
Conc: 84.01 ng/ml