



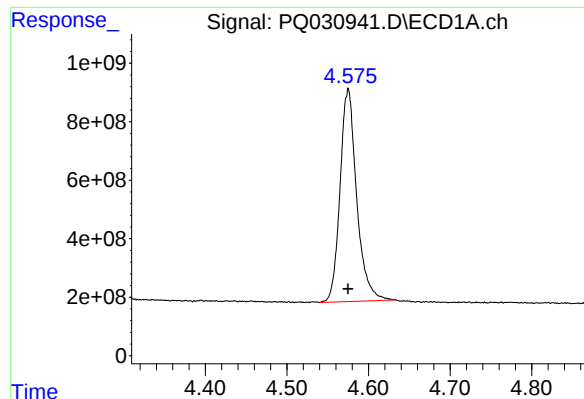

#1 Tetrachloro-m-xylene

R.T.: 4.575 min  
Delta R.T.: 0.000 min  
Response: 10310435770  
Conc: 49.39 ng/ml

Instrument :  
ECD\_Q  
ClientSampleId :

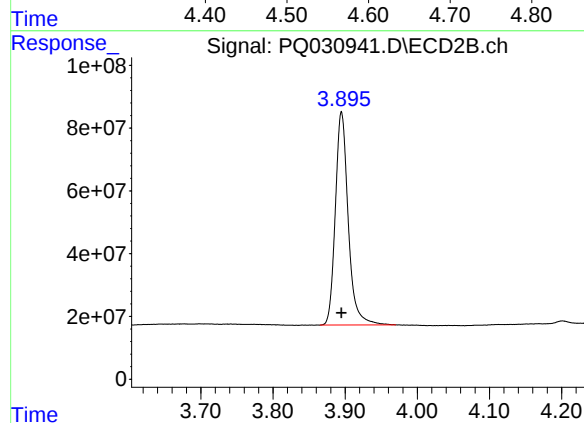

#1 Tetrachloro-m-xylene

R.T.: 3.895 min  
Delta R.T.: 0.000 min  
Response: 842545471  
Conc: 54.35 ng/ml