

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010319\
 Data File : PQ036217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2019 14:44
 Operator : SM\SJ
 Sample : K1022-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 107-PCB-25-ST-SIDEDOOR-GLAZIN

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 00:36:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ122918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 31 04:01:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.725	94365416	44931368	18.440	15.990
2) SA Decachlor...	10.063	8.692	54298982	31619538	15.567	15.841

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010319\
Data File : PQ036217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2019 14:44
Operator : SM\SJ
Sample : K1022-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
107-PCB-25-ST-SIDEDOOR-GLAZIN

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 00:36:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ122918.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 31 04:01:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

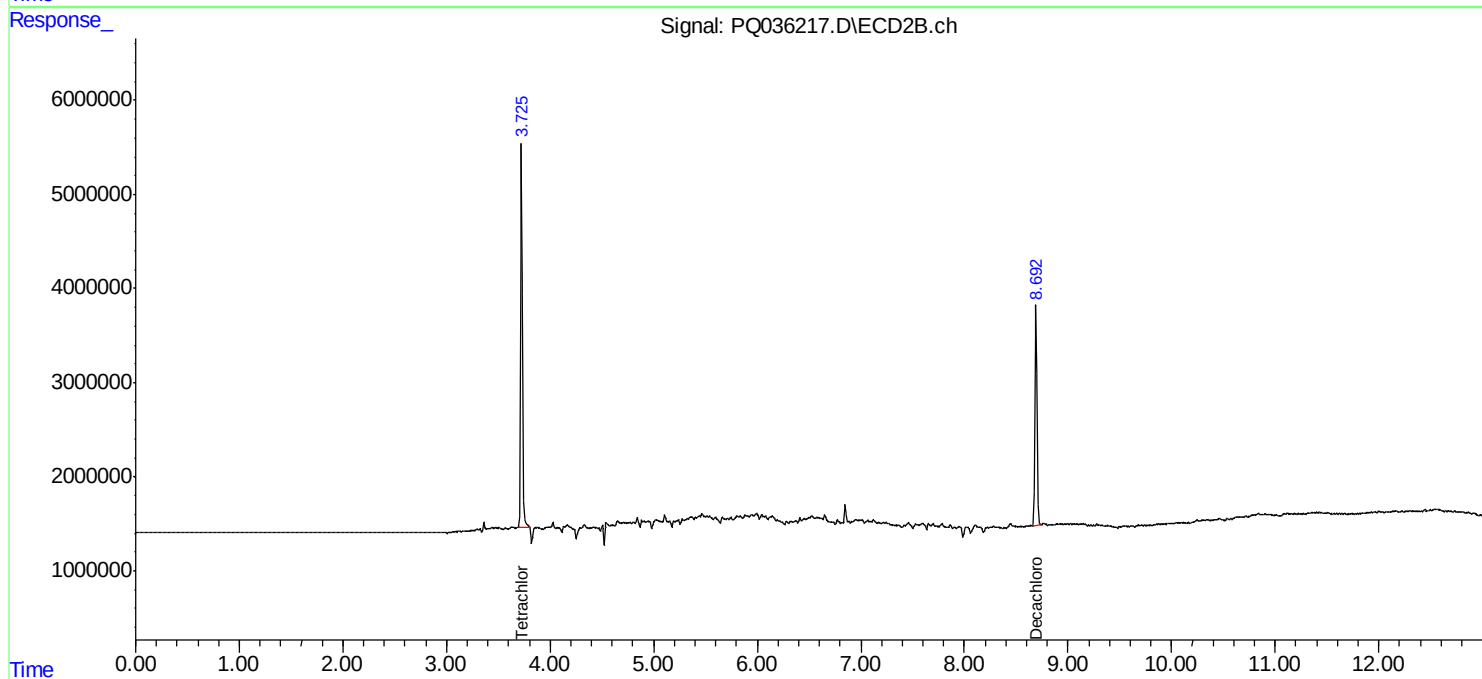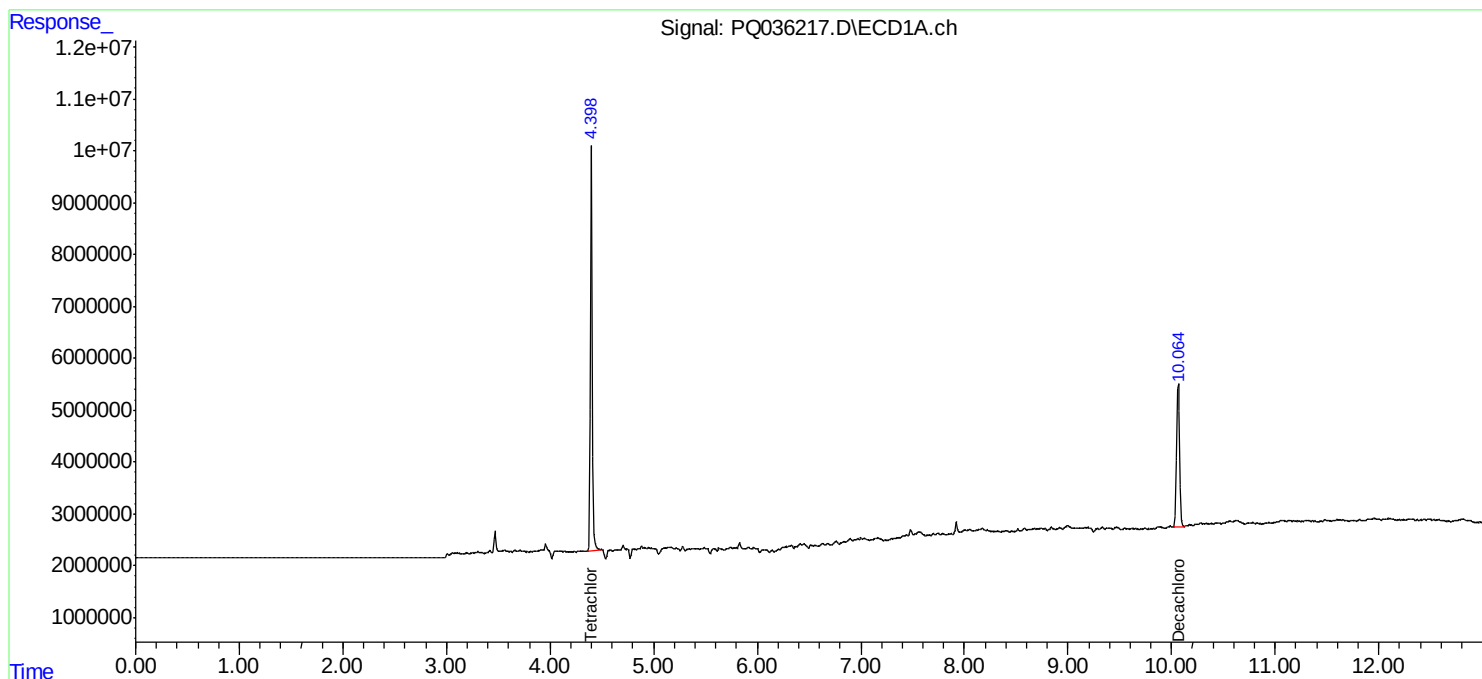


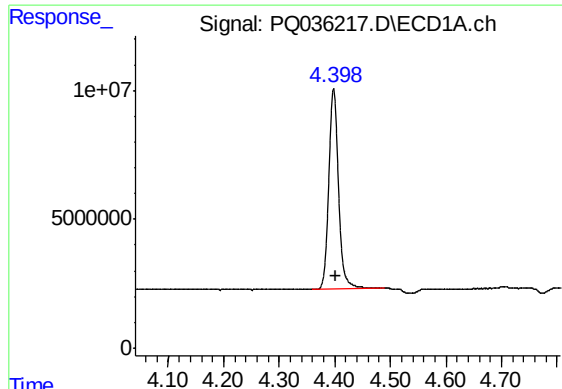

#1 Tetrachloro-m-xylene


R.T.: 4.398 min
Delta R.T.: -0.003 min
Response: 94365416
Conc: 18.44 ng/ml

Instrument :
ECD_Q
ClientSampleId :
107-PCB-25-ST-SIDEDOOR-GLAZIN

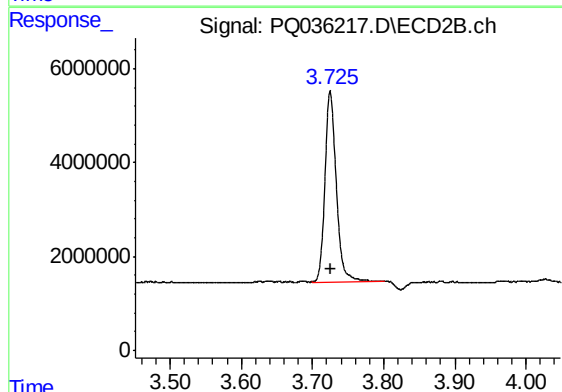


#1 Tetrachloro-m-xylene

R.T.: 3.725 min
Delta R.T.: -0.001 min
Response: 44931368
Conc: 15.99 ng/ml

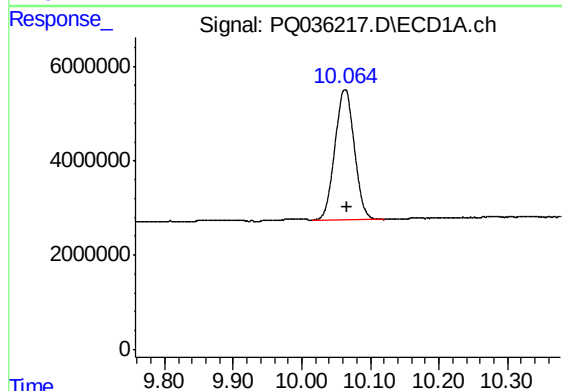

#2 Decachlorobiphenyl

R.T.: 10.063 min
Delta R.T.: -0.004 min
Response: 54298982
Conc: 15.57 ng/ml

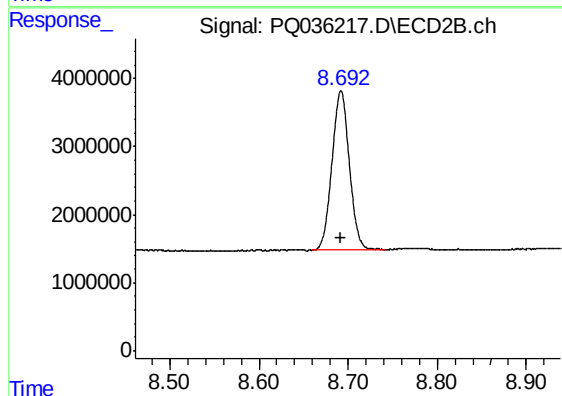

#2 Decachlorobiphenyl

R.T.: 8.692 min
Delta R.T.: 0.000 min
Response: 31619538
Conc: 15.84 ng/ml