

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010319\
 Data File : PQ036226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2019 17:04
 Operator : SM\SJ
 Sample : K1022-03 (Sig #1); J1022-03 (Sig #2)
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 105-PCB-25-ST-REVOLVING-DOOR

Manual Integrations
 APPROVED

Sohil
 1/4/2019 10:16:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 08:12:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ122918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 31 04:01:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.396	3.726	104.7E6	57041251	20.450	20.300
2)	SA Decachlor...	10.060	8.690	83894021	112.5E6	24.051m	56.359m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ010319\
Data File : PQ036226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2019 17:04
Operator : SM\SJ
Sample : K1022-03 (Sig #1); J1022-03 (Sig #2)
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
105-PCB-25-ST-REVOLVING-DOOR


Manual Integrations
APPROVED

Sohil
1/4/2019 10:16:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 08:12:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ122918.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 31 04:01:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

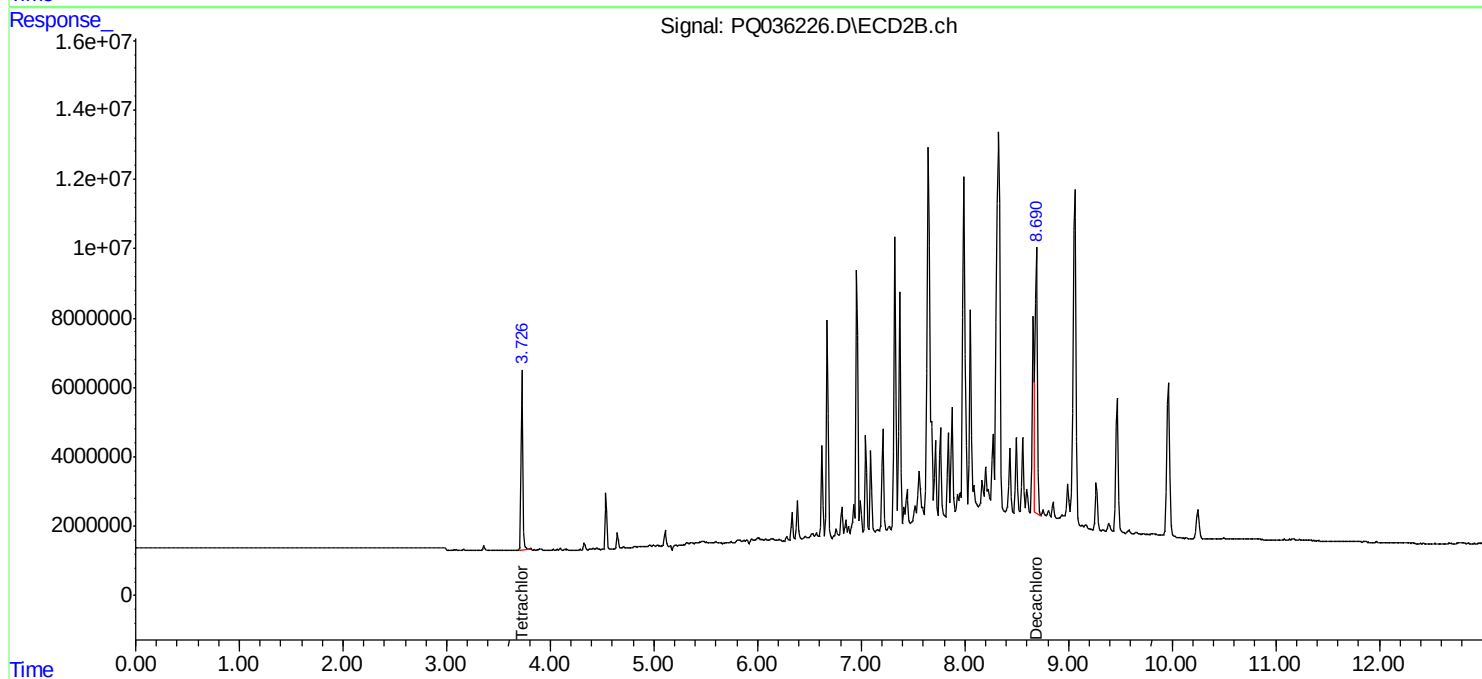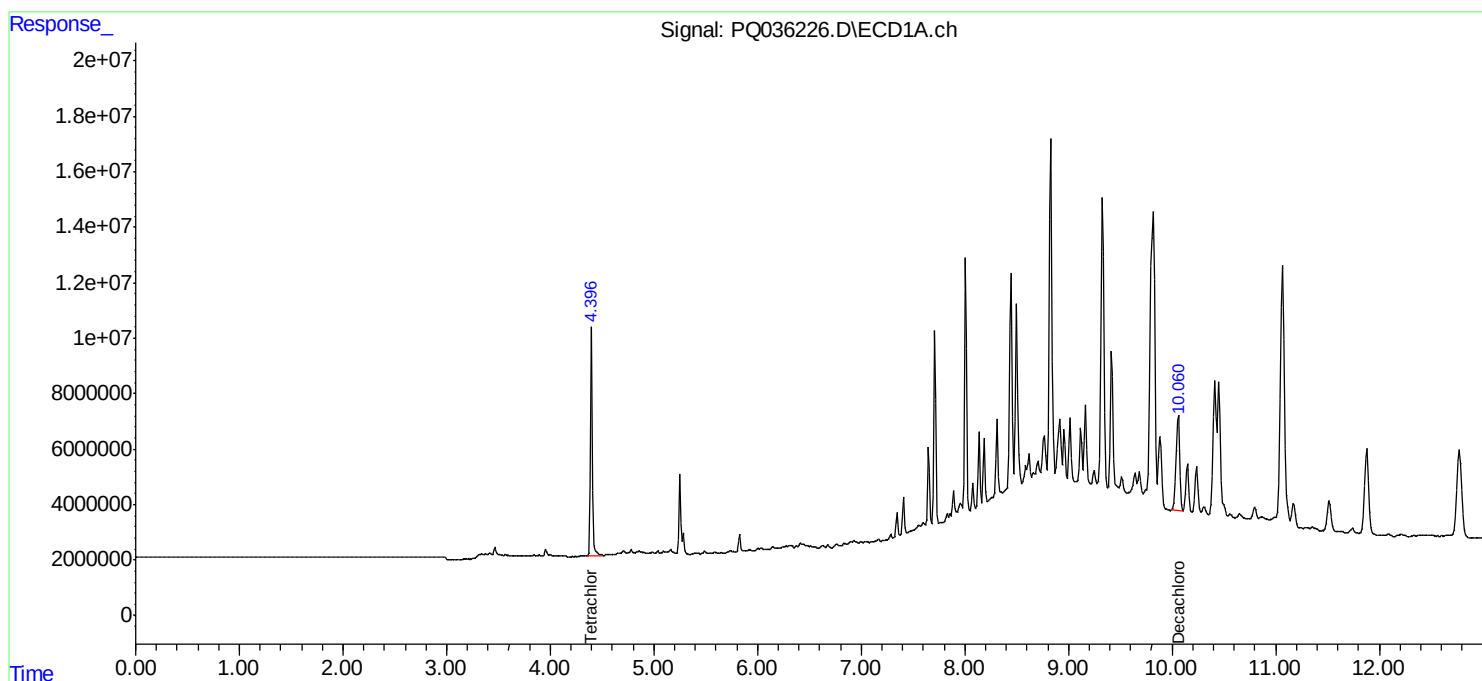

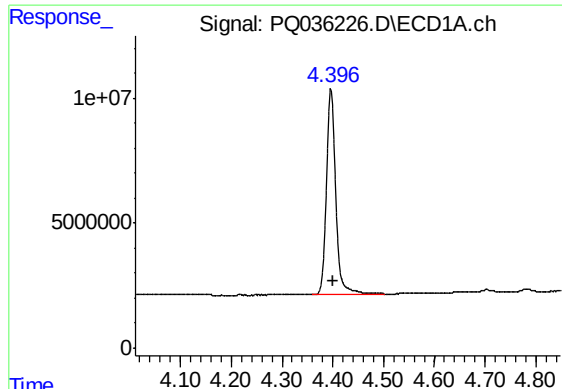


#1 Tetrachloro-m-xylene

R.T.: 4.396 min
Delta R.T.: -0.005 min
Response: 104655880
Conc: 20.45 ng/ml

Instrument :
ECD_Q
ClientSampleId :
105-PCB-25-ST-REVOLVING-DOOR


Manual Integrations
APPROVED

Sohil
1/4/2019 10:16:35 AM

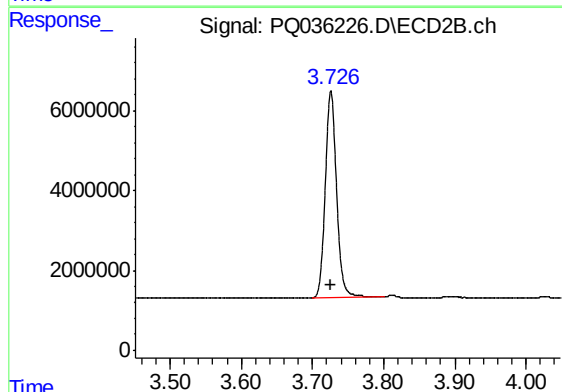


#1 Tetrachloro-m-xylene

R.T.: 3.726 min
Delta R.T.: 0.000 min
Response: 57041251
Conc: 20.30 ng/ml

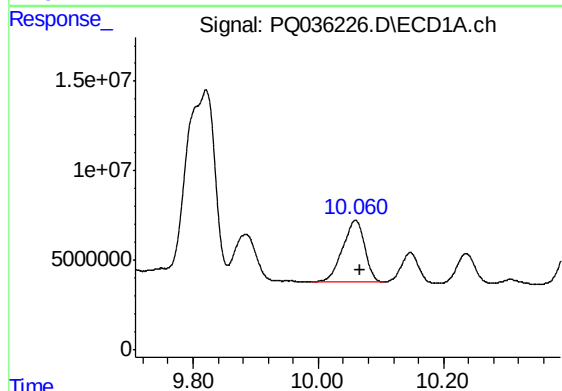

#2 Decachlorobiphenyl

R.T.: 10.060 min
Delta R.T.: -0.007 min
Response: 83894021
Conc: 24.05 ng/ml m

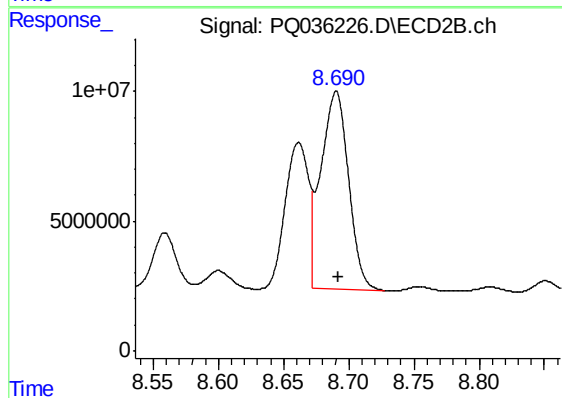

#2 Decachlorobiphenyl

R.T.: 8.690 min
Delta R.T.: -0.002 min
Response: 112495394
Conc: 56.36 ng/ml m