

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ012519\
 Data File : PQ036682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2019 10:01
 Operator : SM\SJ
 Sample : K1166-01 (Sig #1); K1166-01RE (Sig #2)
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 D-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 23:44:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ012419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 24 06:01:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.705	79139606	39200079	17.194	16.361
2) SA Decachlor...	9.961	8.650	31175006	16435700	8.551	8.737

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ012519\
Data File : PQ036682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2019 10:01
Operator : SM\SJ
Sample : K1166-01 (Sig #1); K1166-01RE (Sig #2)
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
D-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 23:44:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ012419.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 24 06:01:26 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

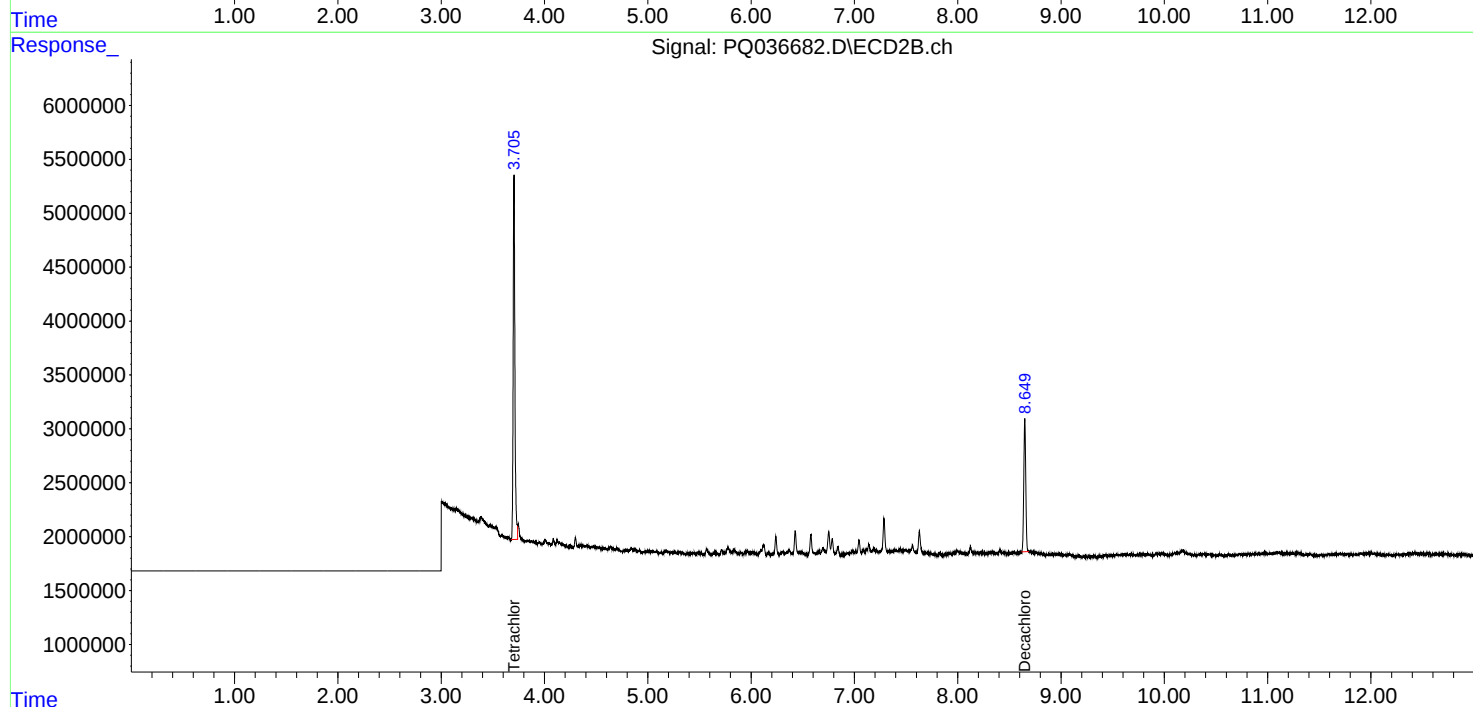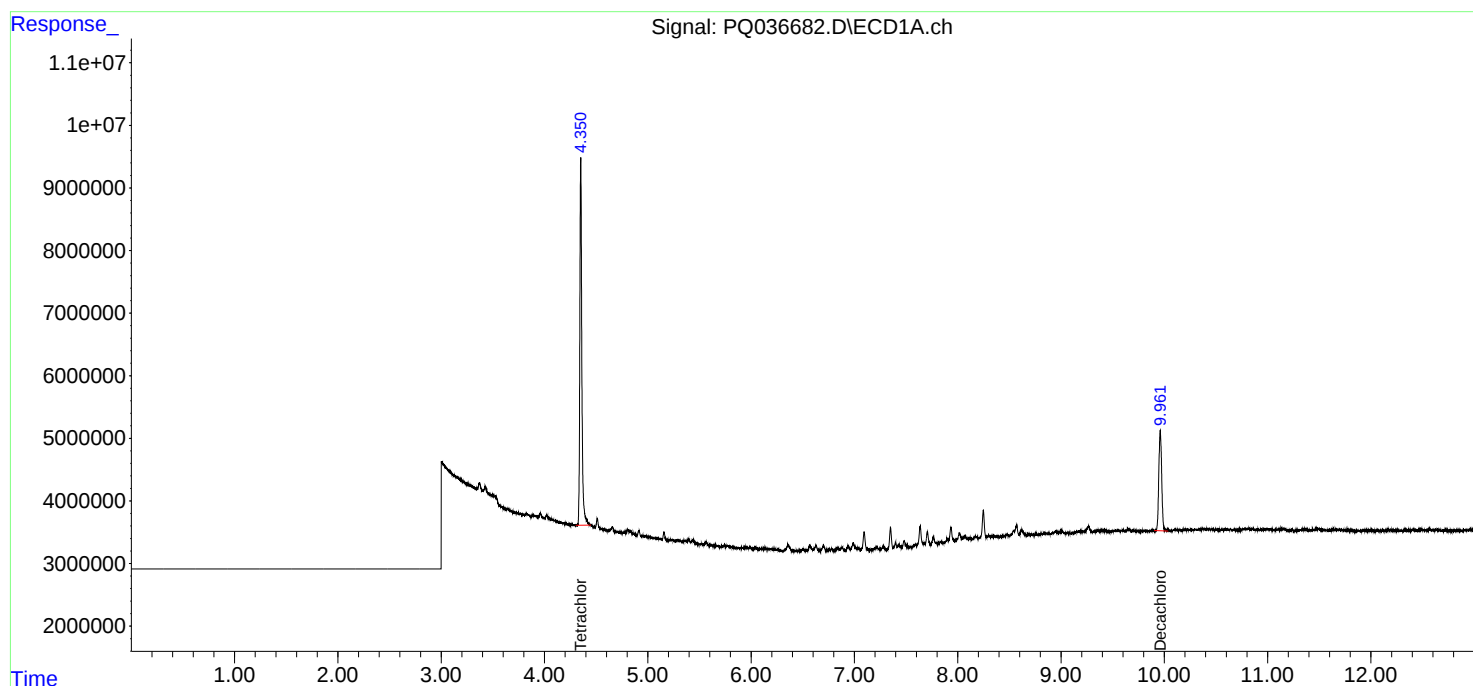


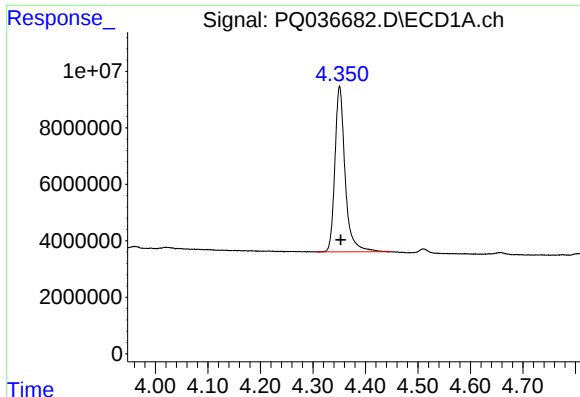

#1 Tetrachloro-m-xylene


R.T.: 4.351 min
Delta R.T.: -0.002 min
Response: 79139606
Conc: 17.19 ng/ml

Instrument :
ECD_Q
ClientSampleId :
D-10

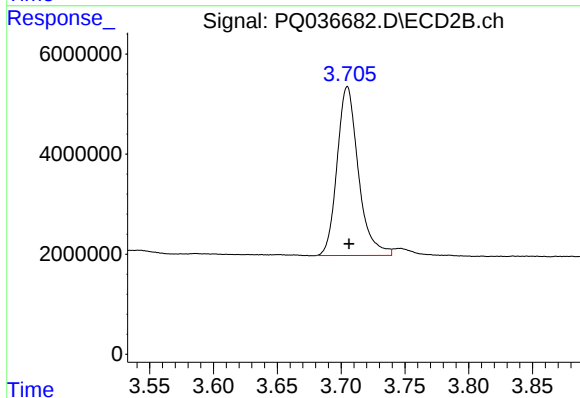


#1 Tetrachloro-m-xylene

R.T.: 3.705 min
Delta R.T.: -0.001 min
Response: 39200079
Conc: 16.36 ng/ml

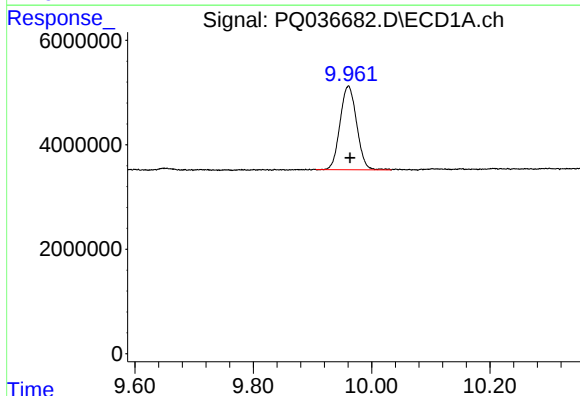

#2 Decachlorobiphenyl

R.T.: 9.961 min
Delta R.T.: -0.003 min
Response: 31175006
Conc: 8.55 ng/ml

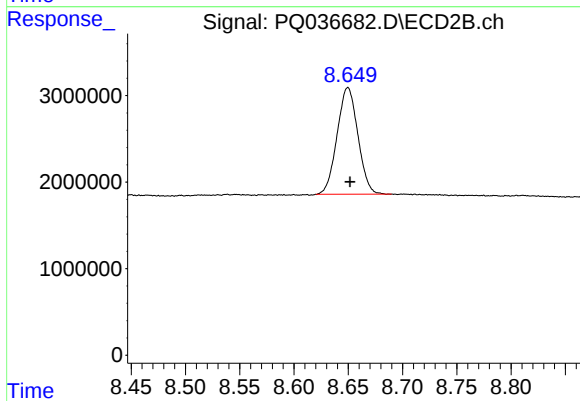

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: -0.002 min
Response: 16435700
Conc: 8.74 ng/ml