

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ013120\
 Data File : PQ046333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2020 01:26
 Operator : AJ\MA
 Sample : L1332-01
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 KIT-SINK-1ST-DRAW

Manual Integrations
 APPROVED

mohammad
 2/4/2020 12:26:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 04:58:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 06:56:17 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.196	4.345	219.7E6	110.2E6	36.531m	37.422
2) SA Decachlor...	11.327	9.764	134.2E6	128.1E6	26.080	25.127

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ013120\
Data File : PQ046333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2020 01:26
Operator : AJ\MA
Sample : L1332-01
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
KIT-SINK-1ST-DRAW


Manual Integrations
APPROVED

mohammad
2/4/2020 12:26:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 04:58:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 06:56:17 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

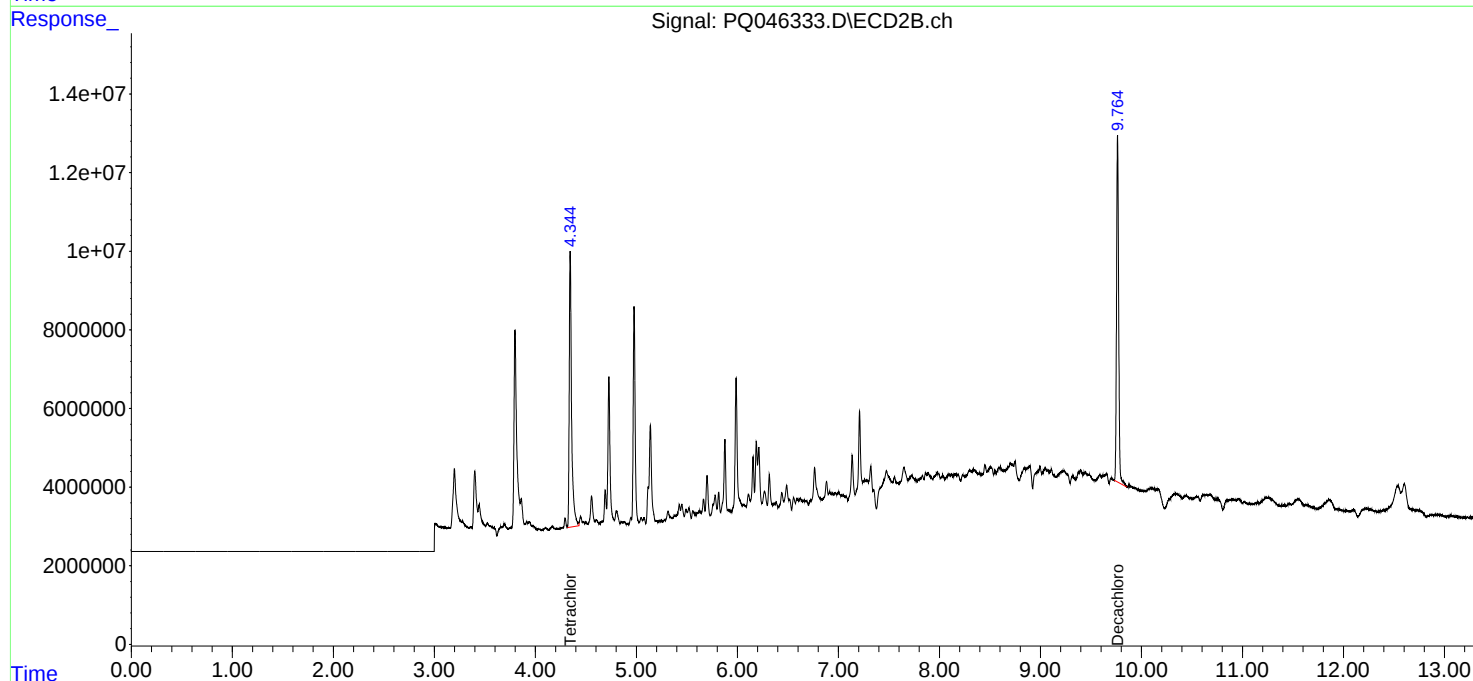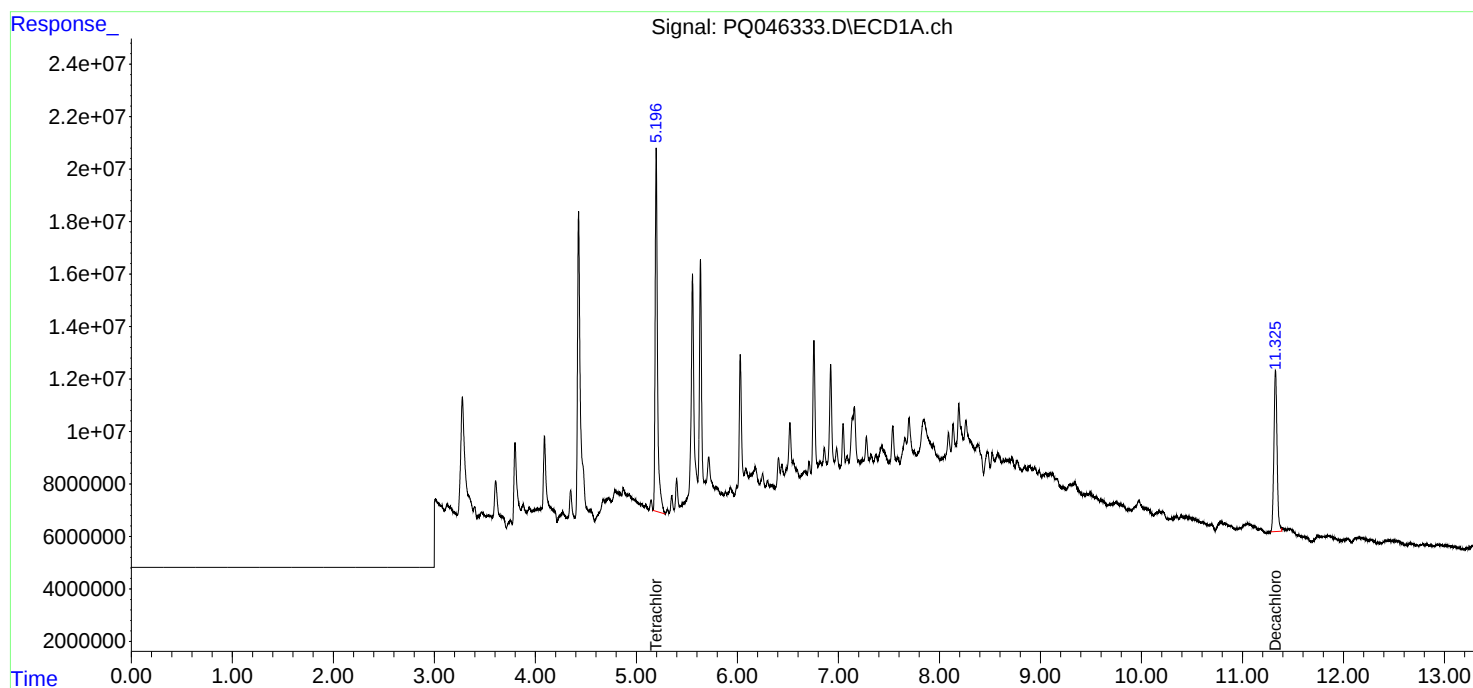

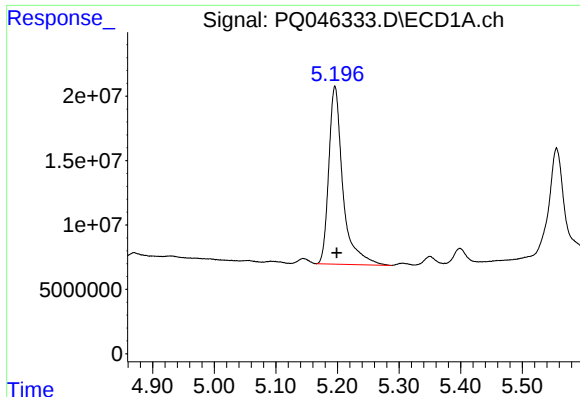


#1 Tetrachloro-m-xylene

R.T.: 5.196 min
Delta R.T.: -0.003 min
Response: 219717170
Conc: 36.53 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
KIT-SINK-1ST-DRAW


Manual Integrations
APPROVED

mohammad
2/4/2020 12:26:08 PM

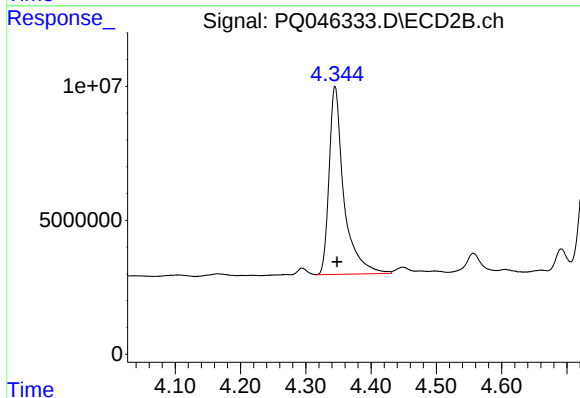


#1 Tetrachloro-m-xylene

R.T.: 4.345 min
Delta R.T.: -0.003 min
Response: 110197362
Conc: 37.42 ng/ml

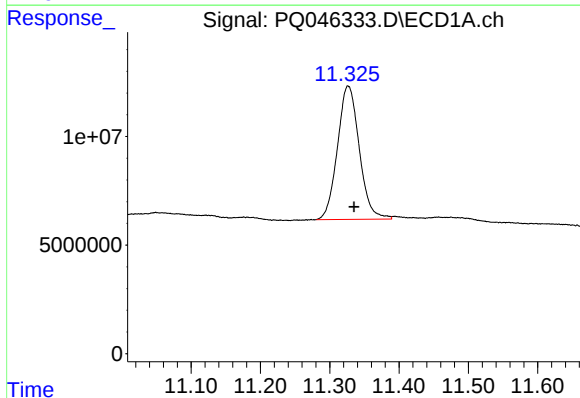

#2 Decachlorobiphenyl

R.T.: 11.327 min
Delta R.T.: -0.009 min
Response: 134197412
Conc: 26.08 ng/ml

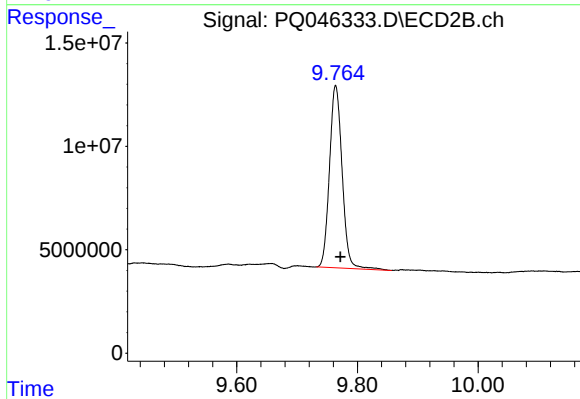

#2 Decachlorobiphenyl

R.T.: 9.764 min
Delta R.T.: -0.008 min
Response: 128135752
Conc: 25.13 ng/ml