

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ021119\
 Data File : PQ037144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Feb 2019 16:23
 Operator : SM\SJ
 Sample : SURR TEST
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SURR TEST

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 12 07:52:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ020619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 06 18:32:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.301	3.682	-14049871	56709892	N.D.	24.556
2) SA Decachlor...	0.000	8.609	0	32688357	N.D.	17.398 #
Target Compounds						
26) L6 AR-1254-1	6.264	0.000	2861543	0	6.565	N.D. #
28) L6 AR-1254-3	6.925	0.000	1661807	0	2.369	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ021119\
Data File : PQ037144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Feb 2019 16:23
Operator : SM\SJ
Sample : SURR TEST
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
SURR TEST

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 12 07:52:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ020619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 06 18:32:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

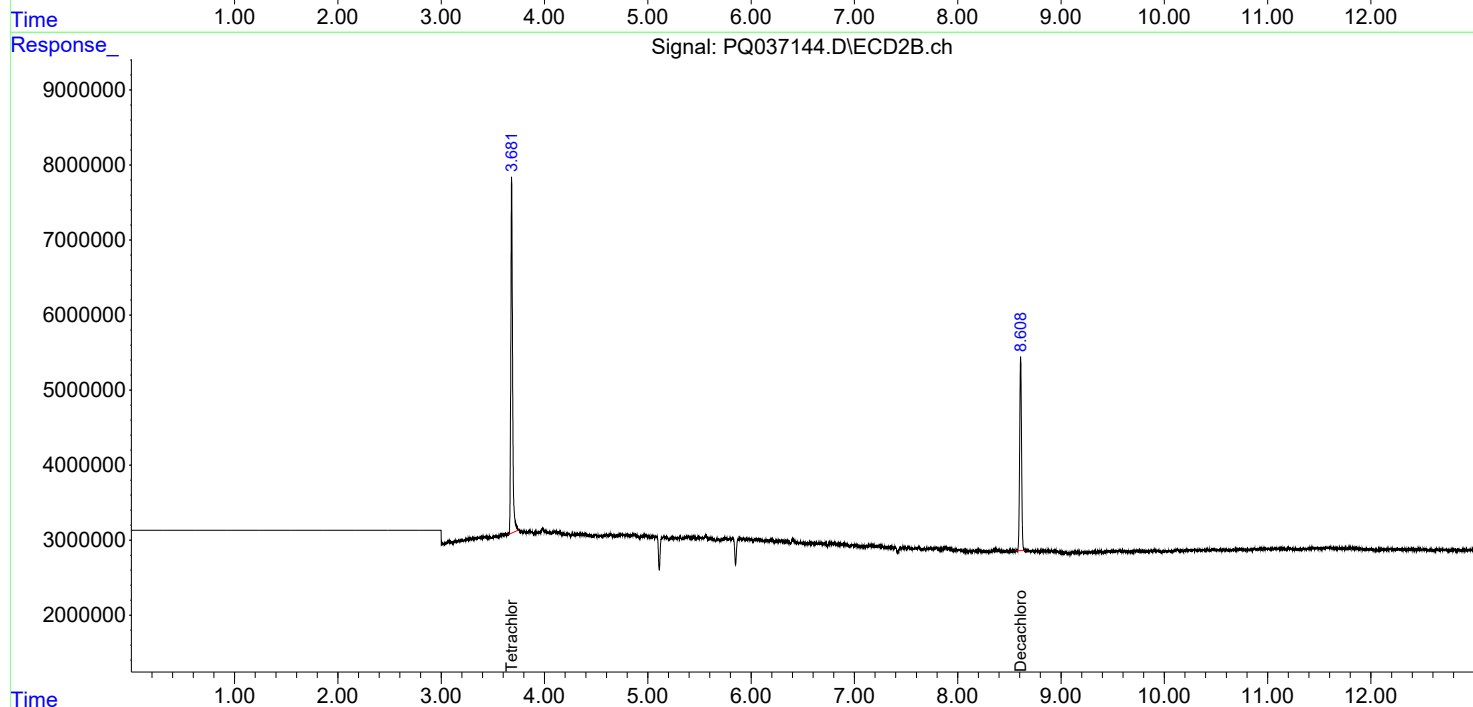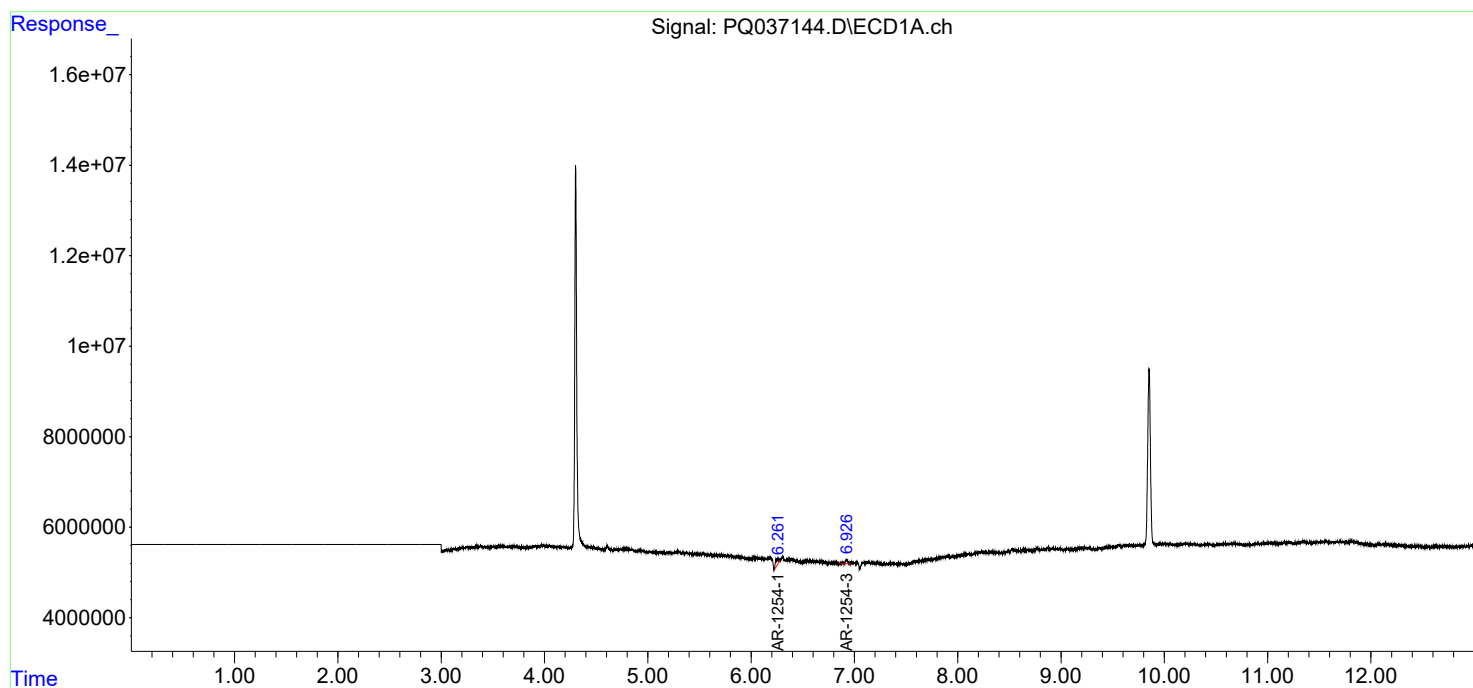


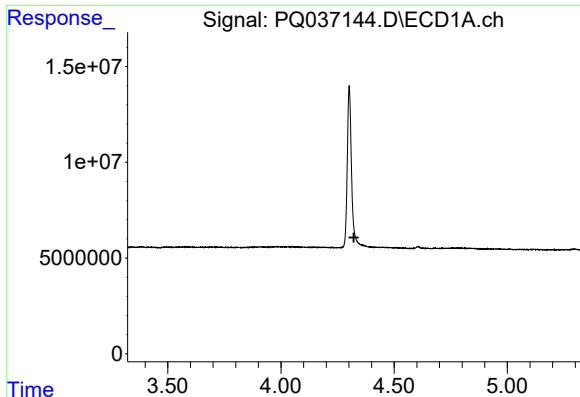

#1 Tetrachloro-m-xylene


R.T.: 4.301 min
Delta R.T.: -0.021 min
Response: -14049871
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
SURR TEST

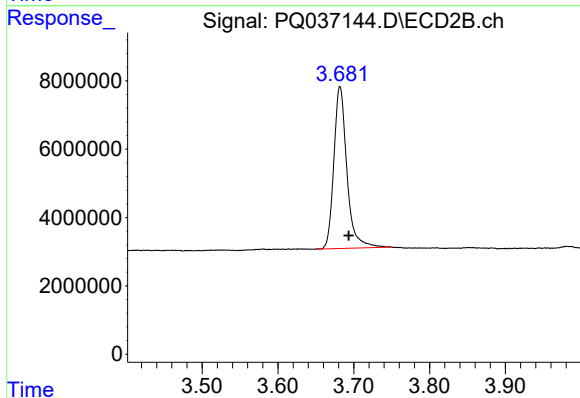


#1 Tetrachloro-m-xylene

R.T.: 3.682 min
Delta R.T.: -0.011 min
Response: 56709892
Conc: 24.56 ng/ml

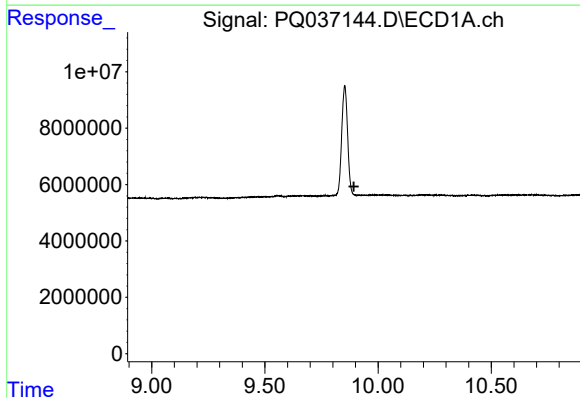


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.893 min
Response: 0
Conc: N.D.

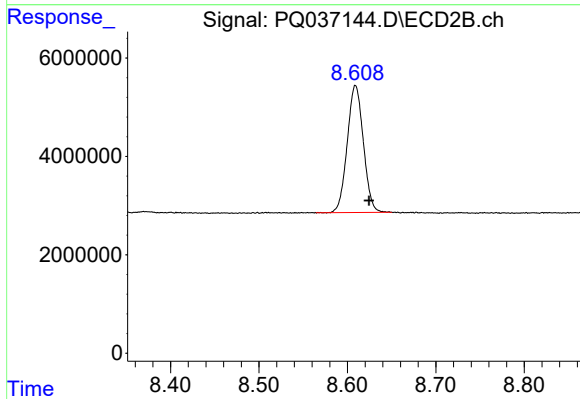

#2 Decachlorobiphenyl


R.T.: 8.609 min
Delta R.T.: -0.015 min
Response: 32688357
Conc: 17.40 ng/ml

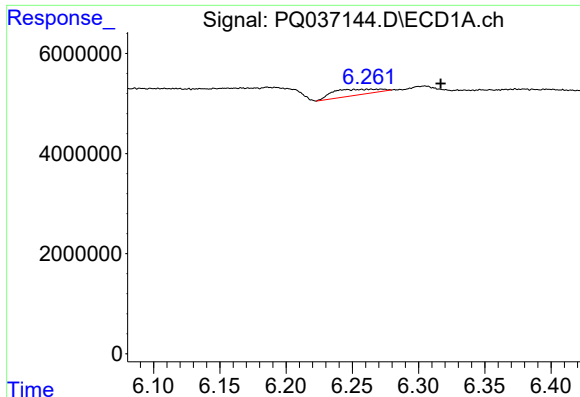

#26 AR-1254-1


R.T.: 6.264 min
Delta R.T.: -0.053 min
Response: 2861543
Conc: 6.56 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SURR TEST

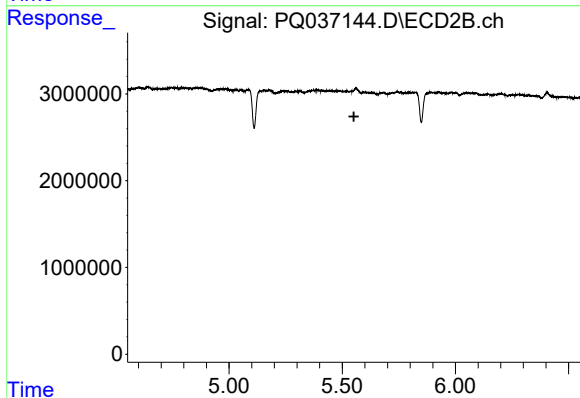


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.551 min
Response: 0
Conc: N.D.

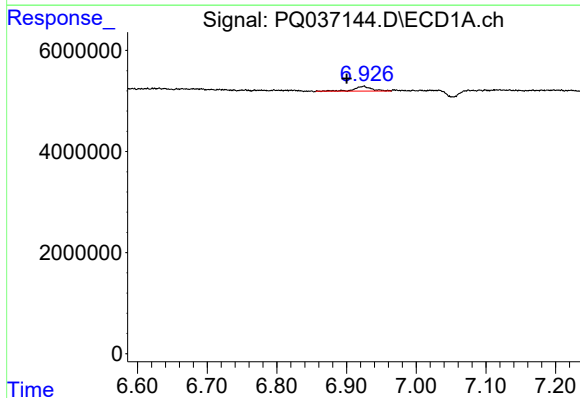

#28 AR-1254-3

R.T.: 6.925 min
Delta R.T.: 0.025 min
Response: 1661807
Conc: 2.37 ng/ml

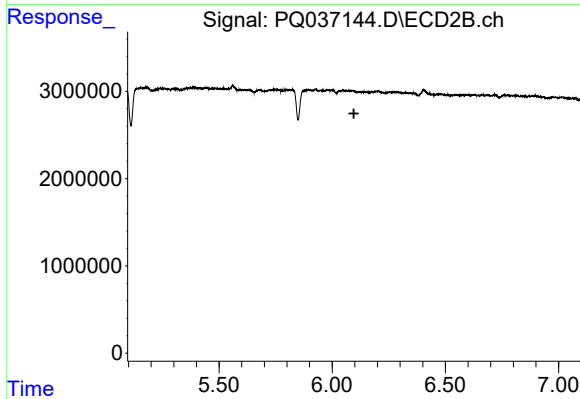

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.096 min
Response: 0
Conc: N.D.