

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ021919\
 Data File : PQ037404.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Feb 2019 16:51
 Operator : SM\SJ
 Sample : K1514-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 FK-BPM-004-CLEARBROOK-PILE-1

Manual Integrations
 APPROVED

Sohil
 2/20/2019 8:15:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 23:35:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ021319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 13 16:51:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.256	3.666	120.8E6	62043942	20.711	20.476
2) SA Decachlor...	9.753	8.570	75373342	34115259	15.389m	15.697

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ021919\
Data File : PQ037404.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Feb 2019 16:51
Operator : SM\SJ
Sample : K1514-01
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1


Manual Integrations
APPROVED

Sohil
2/20/2019 8:15:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 23:35:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ021319.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 13 16:51:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

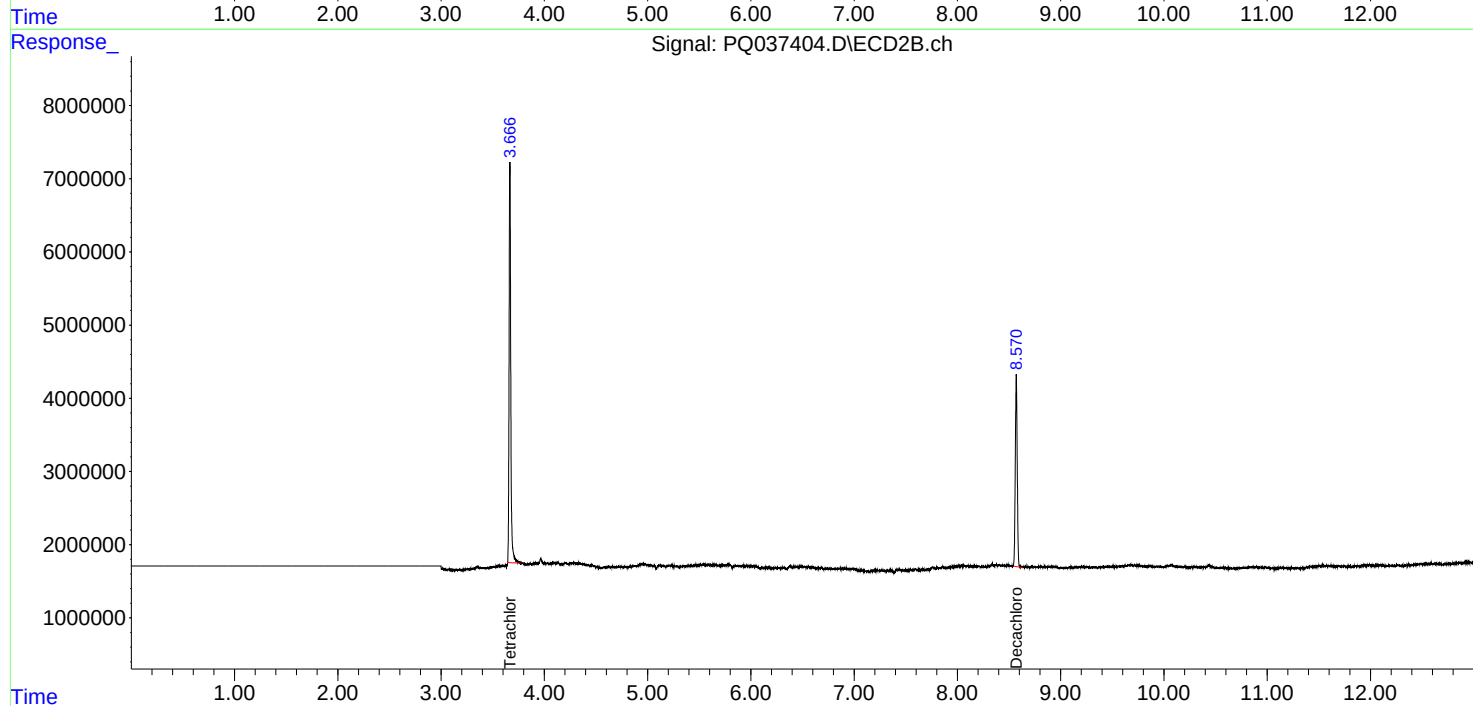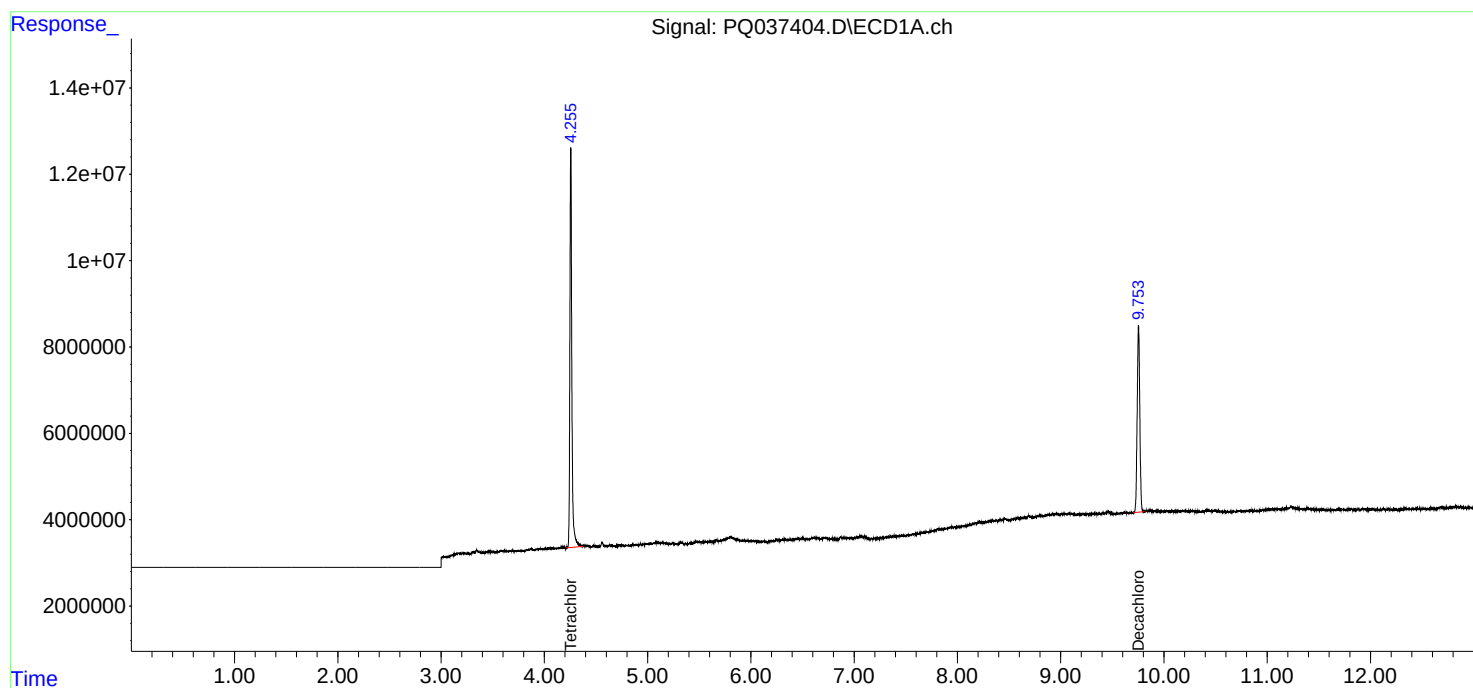

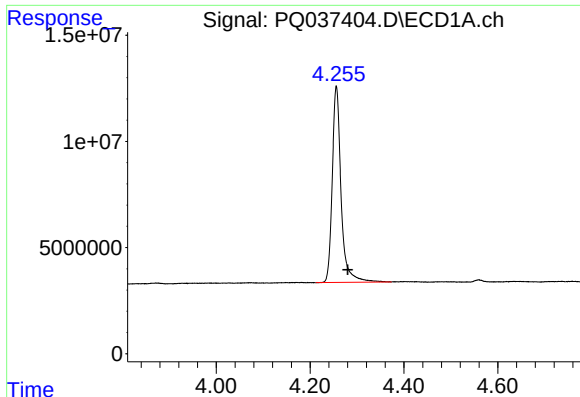


#1 Tetrachloro-m-xylene

R.T.: 4.256 min
Delta R.T.: -0.024 min
Response: 120790491
Conc: 20.71 ng/ml

Instrument :
ECD_Q
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1


Manual Integrations
APPROVED

Sohil
2/20/2019 8:15:46 AM

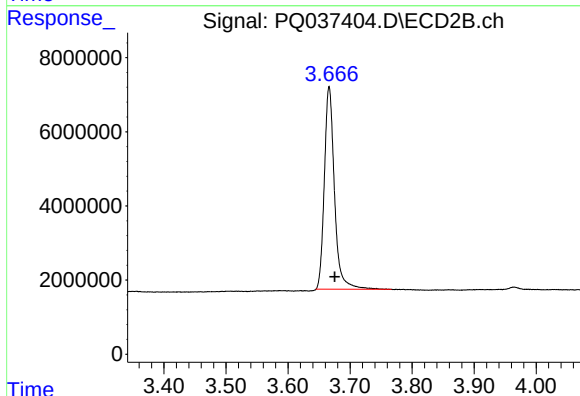


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: -0.009 min
Response: 62043942
Conc: 20.48 ng/ml

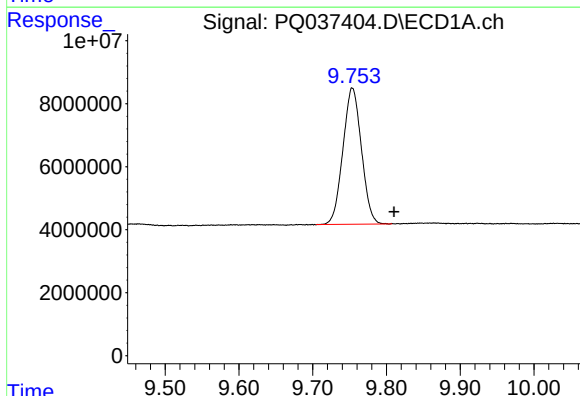

#2 Decachlorobiphenyl

R.T.: 9.753 min
Delta R.T.: -0.058 min
Response: 75373342
Conc: 15.39 ng/ml m

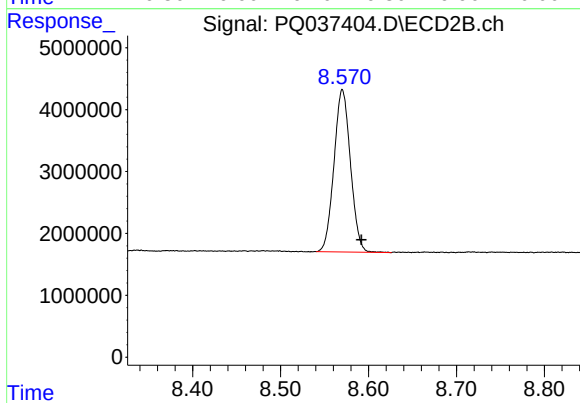

#2 Decachlorobiphenyl

R.T.: 8.570 min
Delta R.T.: -0.022 min
Response: 34115259
Conc: 15.70 ng/ml