

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ022019\
 Data File : PQ037411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2019 09:58
 Operator : SM\SJ
 Sample : SPIKE TEST
 Misc :
 ALS Vial : 141 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SPIKE TEST

Manual Integrations
 APPROVED

Sohil
 2/22/2019 8:14:22 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 20 13:25:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ021319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 13 16:51:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.259	3.670	139.5E6	57276865	23.925	18.903
2) SA Decachlor...	9.752	8.569	67469340	30311506	13.775m	13.947

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ022019\
Data File : PQ037411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2019 09:58
Operator : SM\SJ
Sample : SPIKE TEST
Misc :
ALS Vial : 141 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
SPIKE TEST


Manual Integrations
APPROVED

Sohil
2/22/2019 8:14:22 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 20 13:25:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ021319.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 13 16:51:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

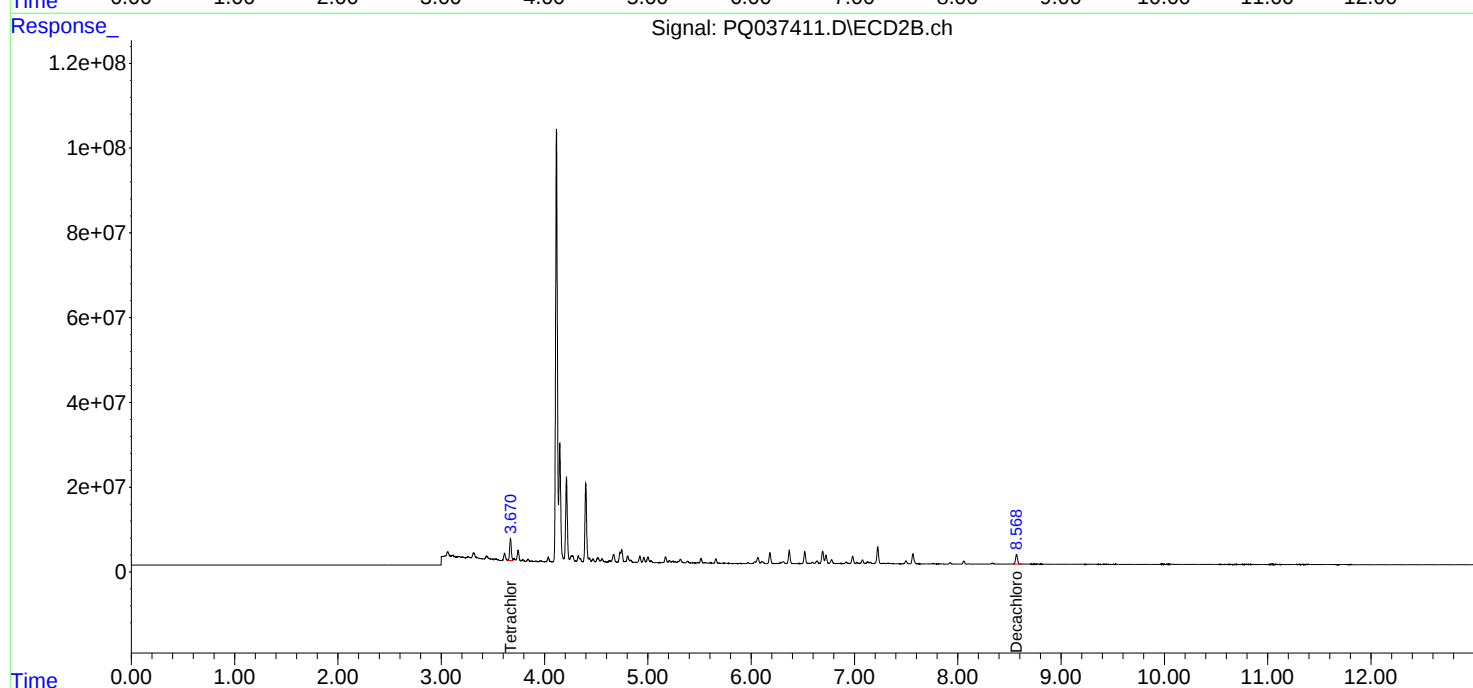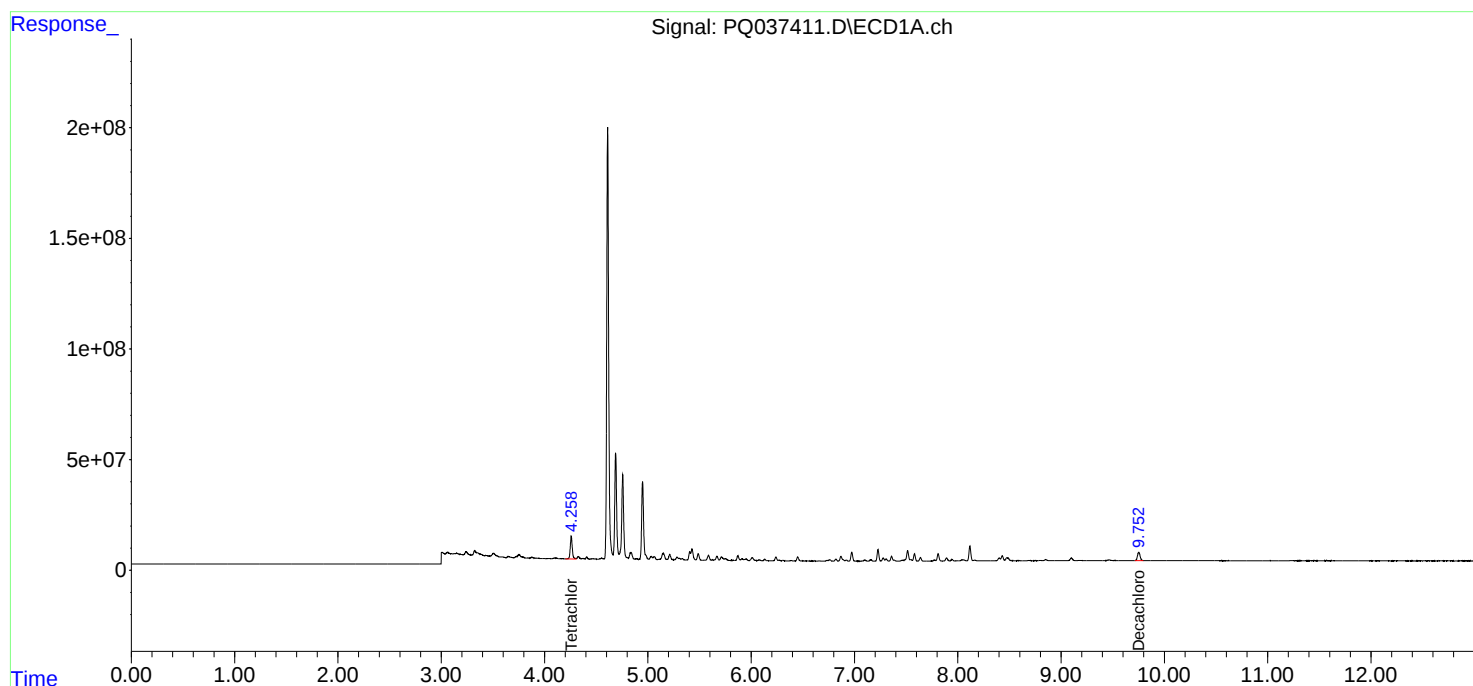

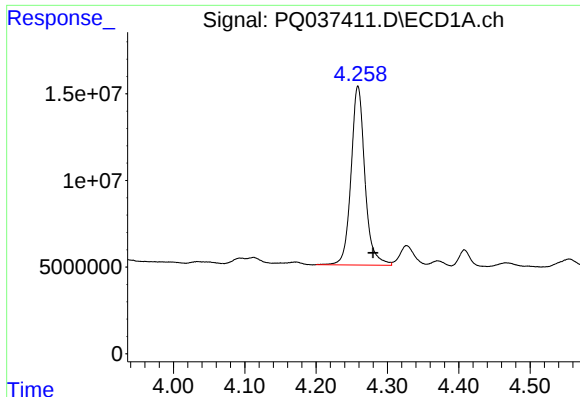


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: -0.021 min
Response: 139533824
Conc: 23.93 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SPIKE TEST


Manual Integrations
APPROVED

Sohil
2/22/2019 8:14:22 AM

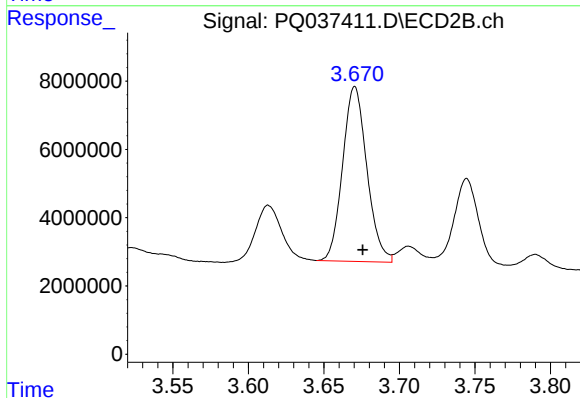


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: -0.005 min
Response: 57276865
Conc: 18.90 ng/ml

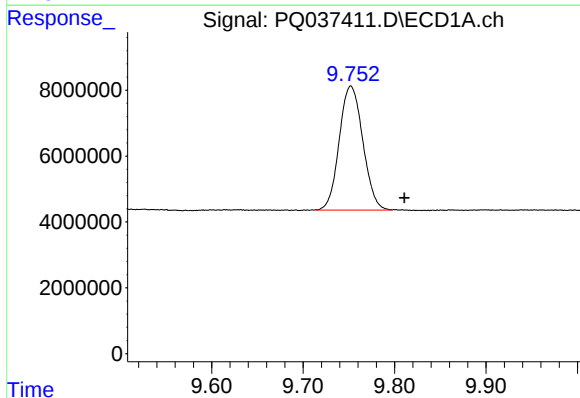

#2 Decachlorobiphenyl

R.T.: 9.752 min
Delta R.T.: -0.059 min
Response: 67469340
Conc: 13.77 ng/ml m

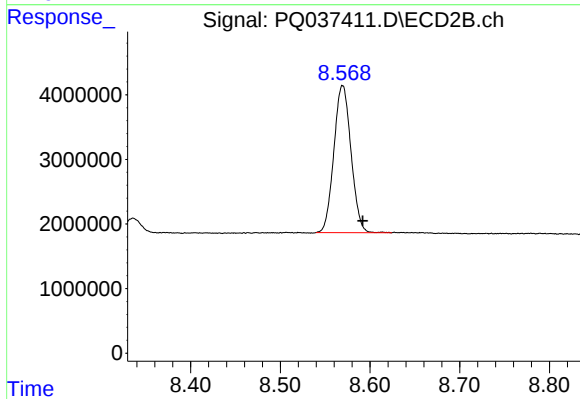

#2 Decachlorobiphenyl

R.T.: 8.569 min
Delta R.T.: -0.023 min
Response: 30311506
Conc: 13.95 ng/ml