

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ030920\
 Data File : PQ046808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2020 19:42
 Operator : AJ\MA
 Sample : L1841-38 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 WALL-FLASHING-A

Manual Integrations
 APPROVED

Sohil
 3/11/2020 11:00:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 05:48:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ030920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 10 04:56:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.178	4.323	82731143	40778001	4.427m	4.520
2) SA Decachlor...	11.304	9.740	40628888	33538751	4.274	4.579

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ030920\
Data File : PQ046808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2020 19:42
Operator : AJ\MA
Sample : L1841-38 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
WALL-FLASHING-A


Manual Integrations
APPROVED

Sohil
3/11/2020 11:00:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 05:48:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ030920.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 10 04:56:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

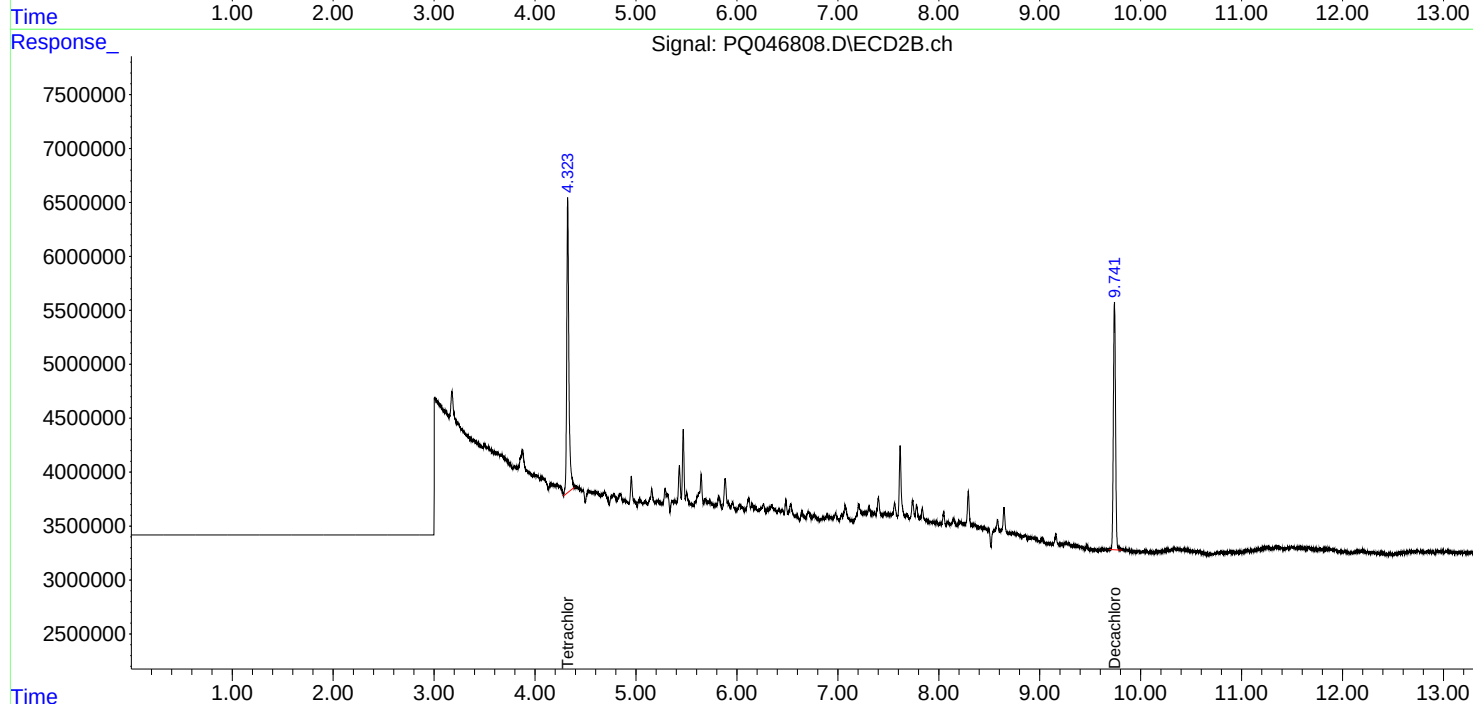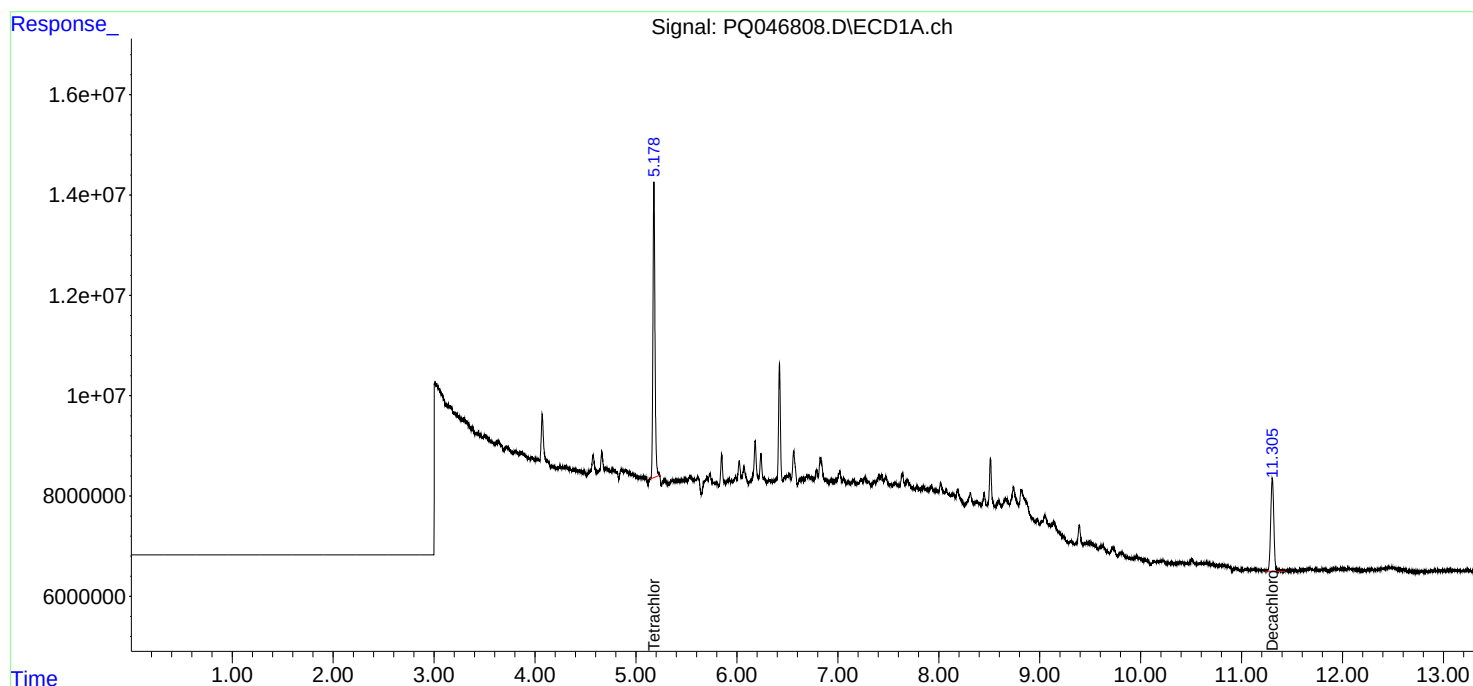

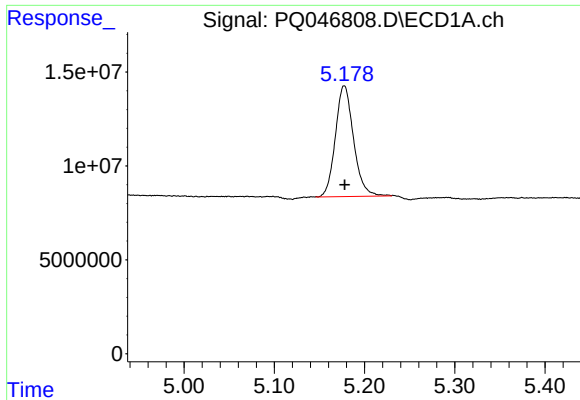


#1 Tetrachloro-m-xylene

R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 82731143
Conc: 4.43 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
WALL-FLASHING-A


Manual Integrations
APPROVED

Sohil
3/11/2020 11:00:28 AM

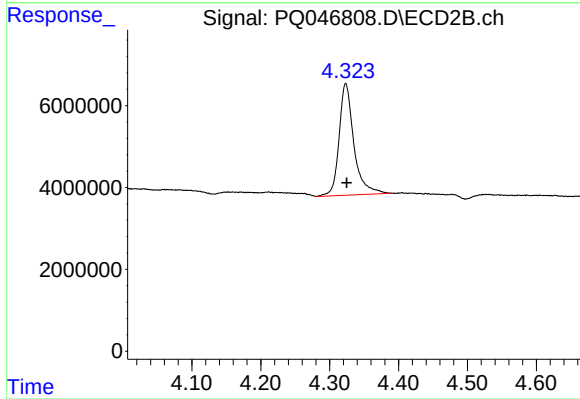


#1 Tetrachloro-m-xylene

R.T.: 4.323 min
Delta R.T.: -0.002 min
Response: 40778001
Conc: 4.52 ng/ml

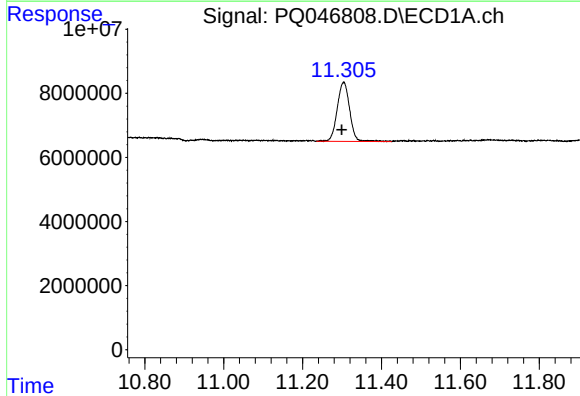

#2 Decachlorobiphenyl

R.T.: 11.304 min
Delta R.T.: 0.005 min
Response: 40628888
Conc: 4.27 ng/ml

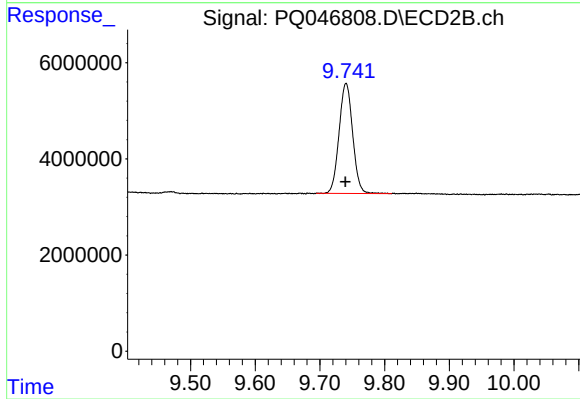

#2 Decachlorobiphenyl

R.T.: 9.740 min
Delta R.T.: 0.001 min
Response: 33538751
Conc: 4.58 ng/ml