

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ041420\
 Data File : PQ047377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2020 10:38
 Operator : AJ\MA
 Sample : L2225-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 FK-BPM-01-C3-D3-C3A-D3A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 13:25:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 07 06:16:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.103	4.262	193.4E6	31063083	11.718	12.690
2)	SA Decachlor...	11.171	9.644	116.4E6	37439386	13.701	14.041

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ041420\
Data File : PQ047377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2020 10:38
Operator : AJ\MA
Sample : L2225-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
FK-BPM-01-C3-D3-C3A-D3A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 13:25:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040720.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 07 06:16:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

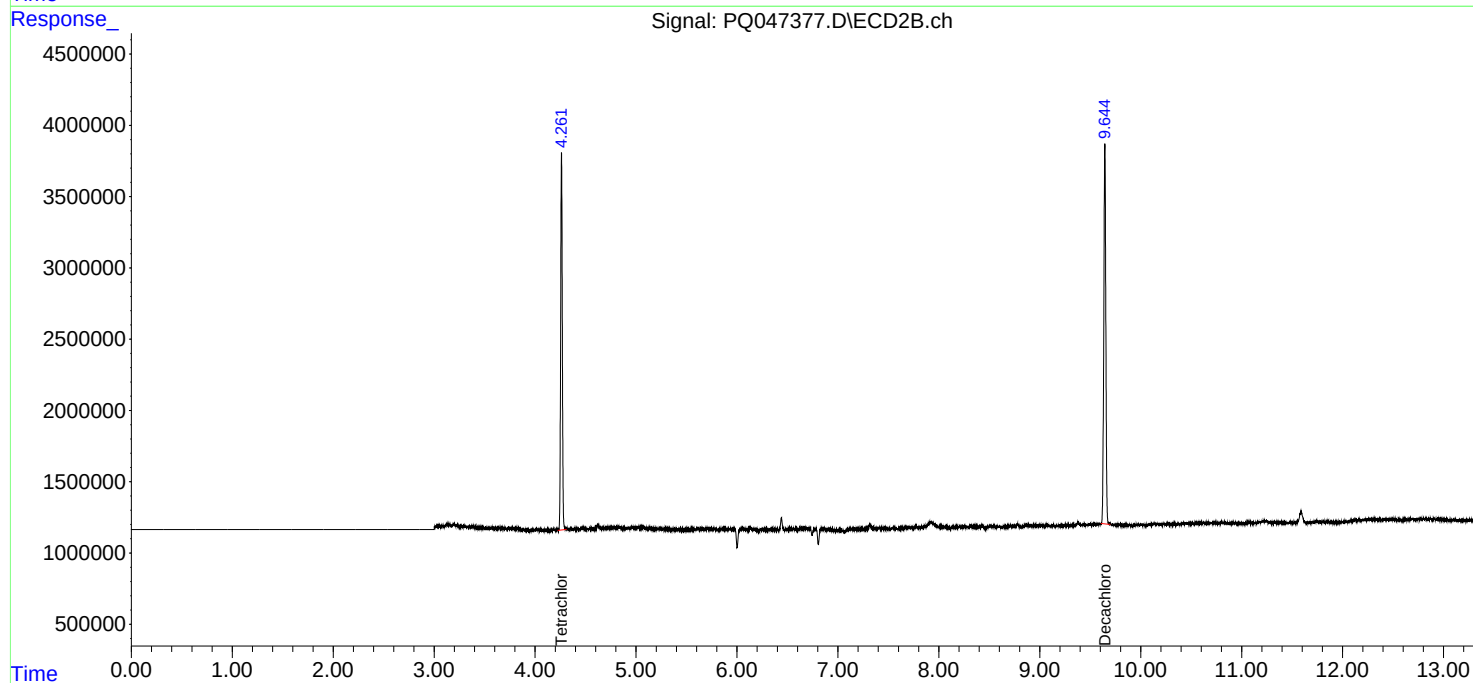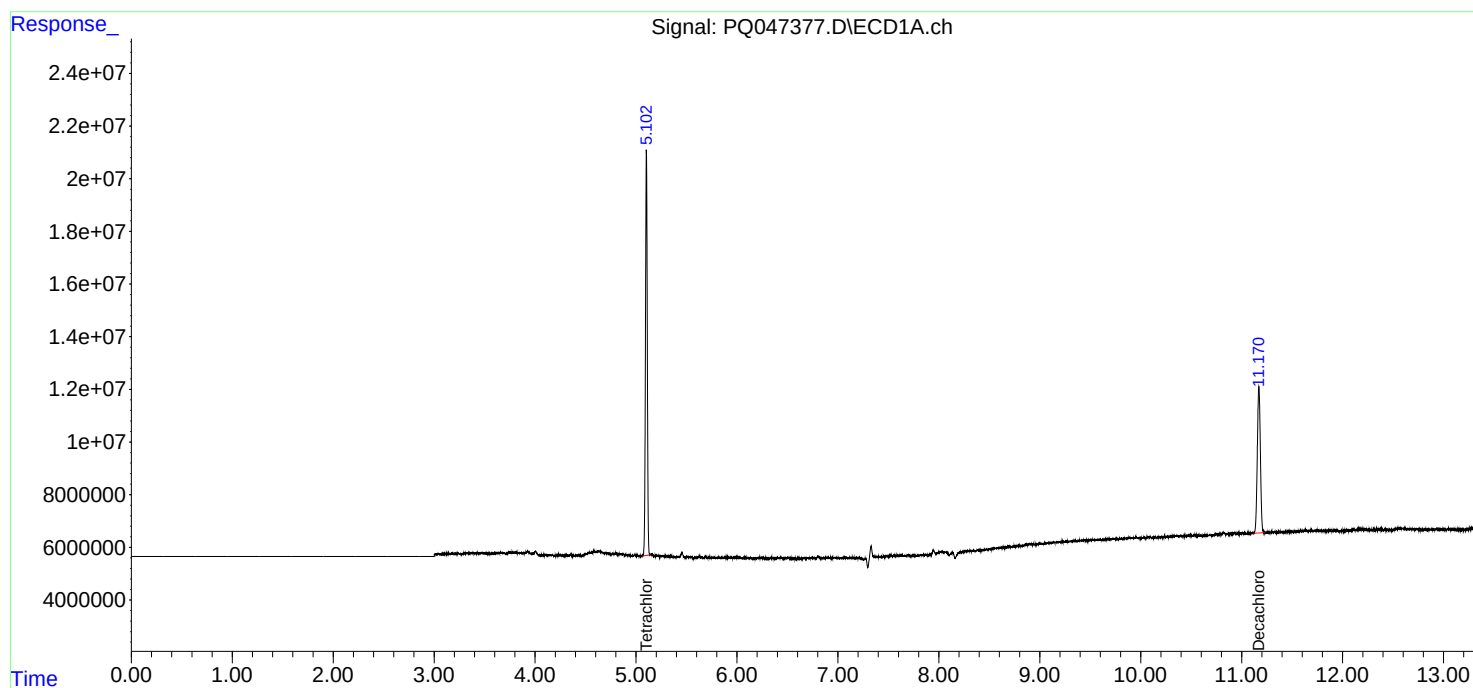


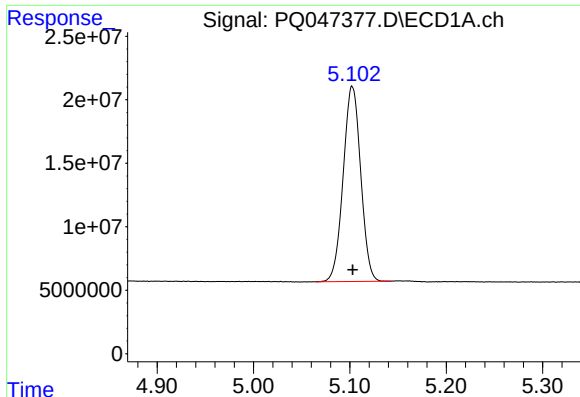

#1 Tetrachloro-m-xylene


R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 193395724
Conc: 11.72 ng/ml

Instrument :
ECD_Q
ClientSampleId :
FK-BPM-01-C3-D3-C3A-D3A

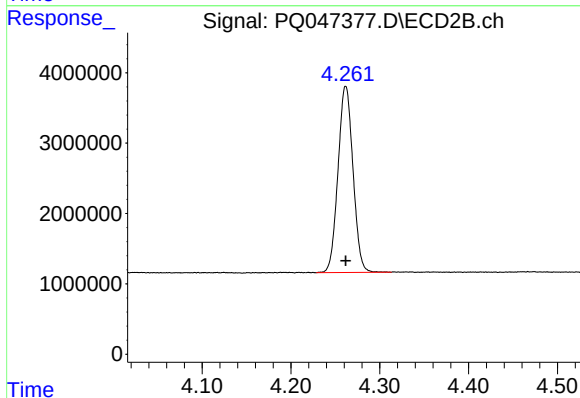


#1 Tetrachloro-m-xylene

R.T.: 4.262 min
Delta R.T.: 0.000 min
Response: 31063083
Conc: 12.69 ng/ml

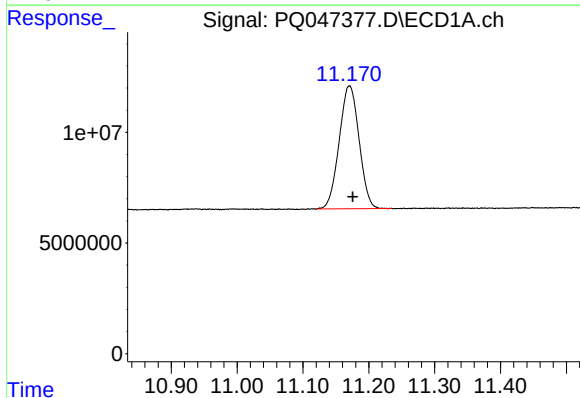

#2 Decachlorobiphenyl

R.T.: 11.171 min
Delta R.T.: -0.005 min
Response: 116390100
Conc: 13.70 ng/ml

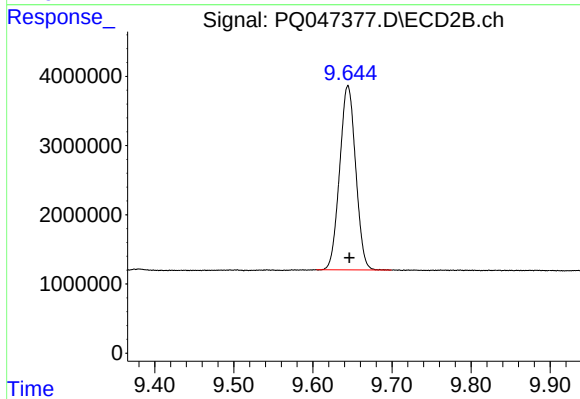

#2 Decachlorobiphenyl

R.T.: 9.644 min
Delta R.T.: -0.002 min
Response: 37439386
Conc: 14.04 ng/ml