

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ042120\
 Data File : PQ047517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 10:43
 Operator : AJ\MA
 Sample : L2342-19
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 TP-15-COMP

Manual Integrations
 APPROVED

Sohil
 4/22/2020 4:32:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 11:23:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ041620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 17 08:20:56 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.106	4.262	290.1E6	54859834	15.782m	18.434
2) SA Decachlor...	11.186	9.646	425.2E6	52123978	19.920	16.673

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ042120\
Data File : PQ047517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 10:43
Operator : AJ\MA
Sample : L2342-19
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
TP-15-COMP


Manual Integrations
APPROVED

Sohil
4/22/2020 4:32:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 11:23:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ041620.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 17 08:20:56 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

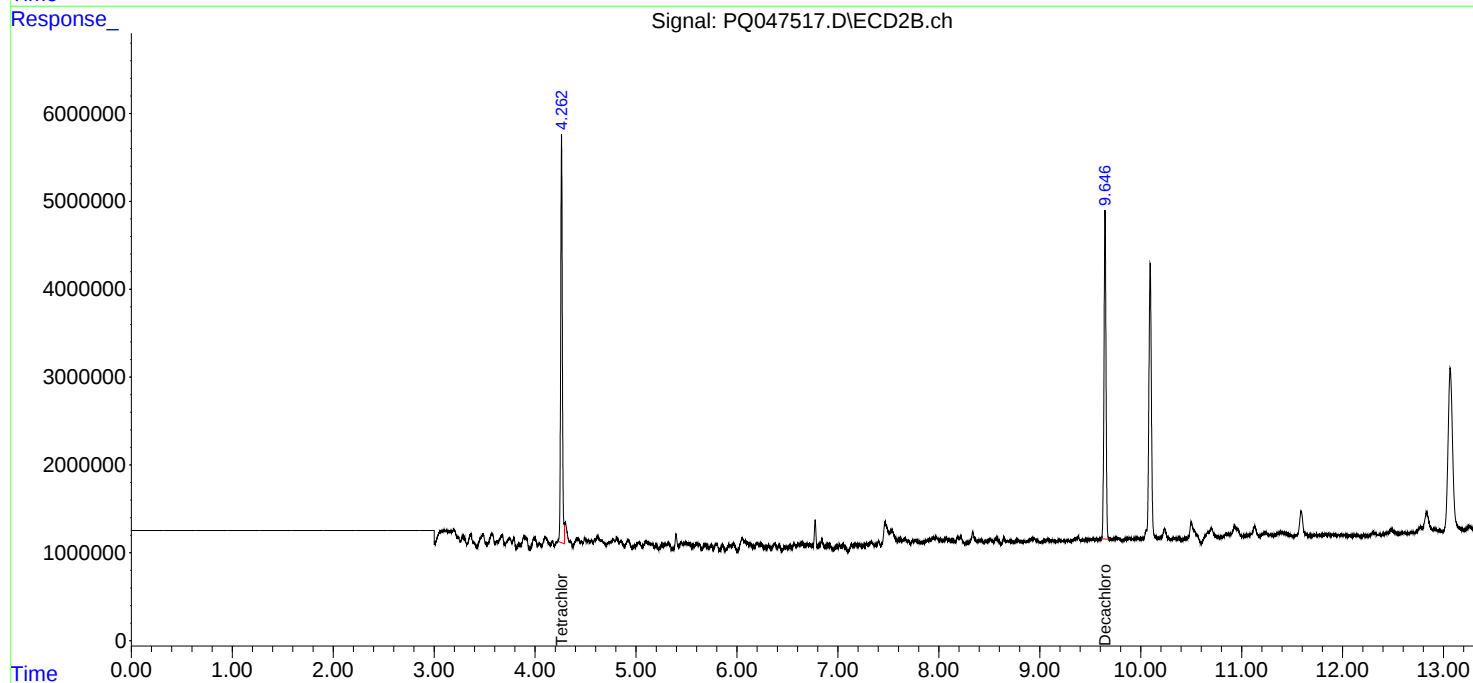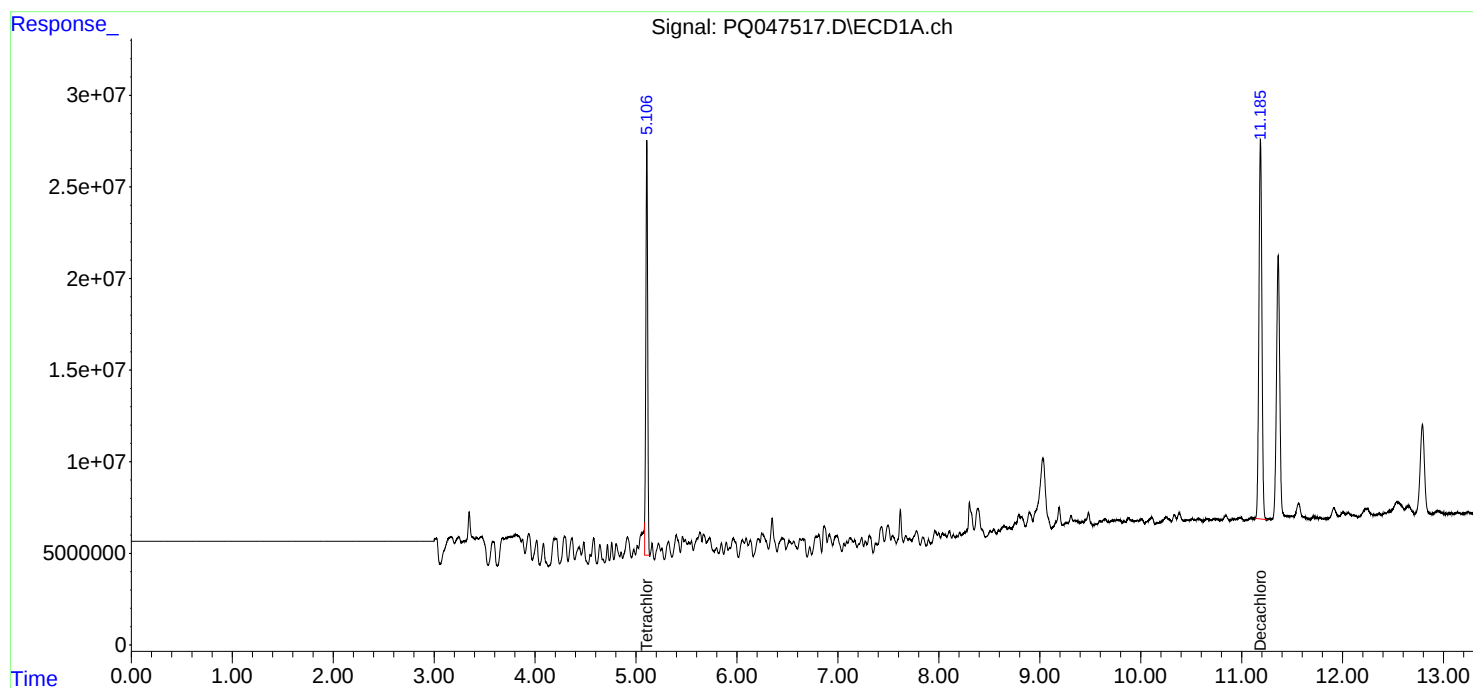

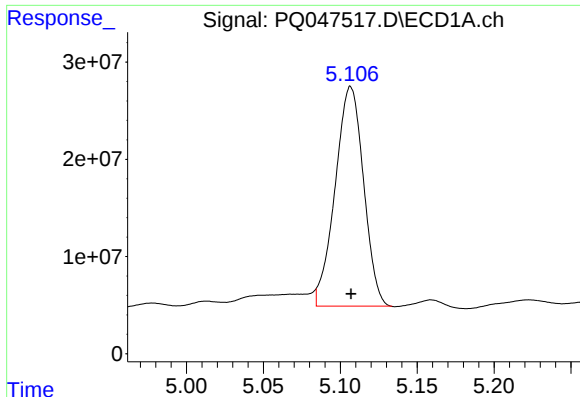


#1 Tetrachloro-m-xylene

R.T.: 5.106 min
Delta R.T.: 0.000 min
Response: 290068556
Conc: 15.78 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
TP-15-COMP


Manual Integrations
APPROVED

Sohil
4/22/2020 4:32:51 PM

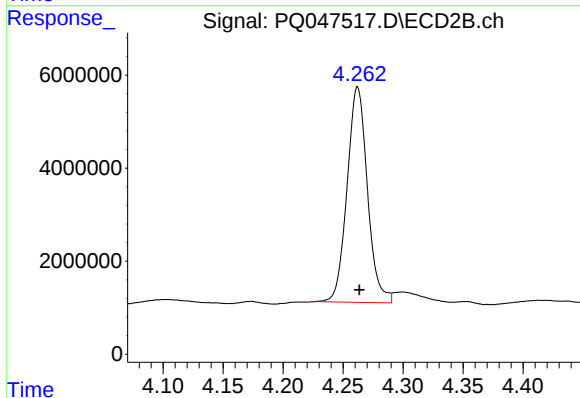


#1 Tetrachloro-m-xylene

R.T.: 4.262 min
Delta R.T.: -0.001 min
Response: 54859834
Conc: 18.43 ng/ml

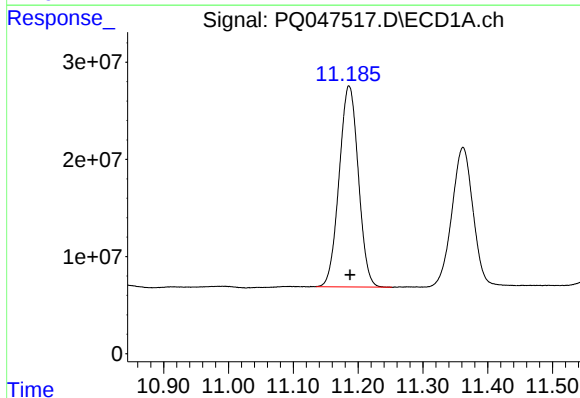

#2 Decachlorobiphenyl

R.T.: 11.186 min
Delta R.T.: -0.002 min
Response: 425249333
Conc: 19.92 ng/ml

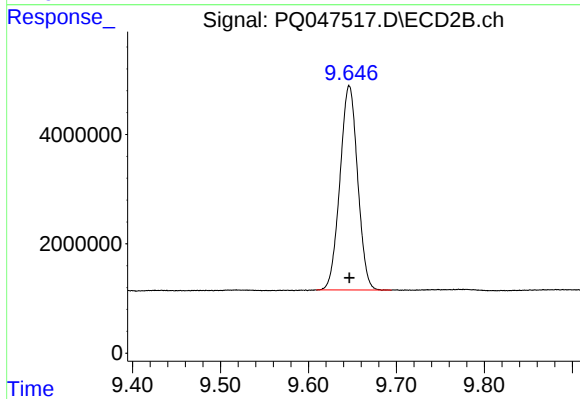

#2 Decachlorobiphenyl

R.T.: 9.646 min
Delta R.T.: 0.000 min
Response: 52123978
Conc: 16.67 ng/ml