

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ042220\
 Data File : PQ047547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2020 15:33
 Operator : AJ\MA
 Sample : L2375-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 TP-16A

Manual Integrations
 APPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 15:59:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ041620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 17 08:20:56 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.108	4.264	226.5E6	40325267	12.321m	13.550
2) SA Decachlor...	11.184	9.646	324.3E6	41496528	15.193	13.273

Sohil

4/23/2020 3:24:54 PM

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ042220\
Data File : PQ047547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2020 15:33
Operator : AJ\MA
Sample : L2375-02
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
TP-16A

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 15:59:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ041620.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 17 08:20:56 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

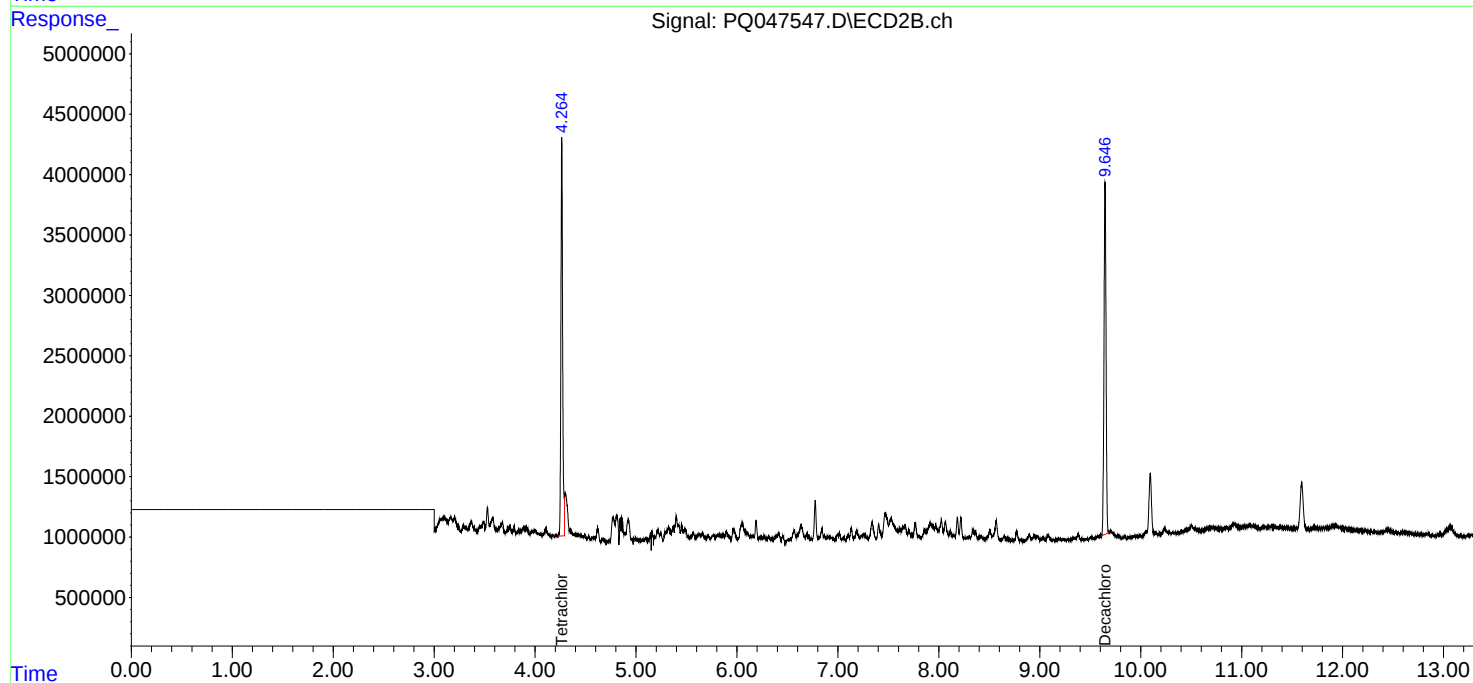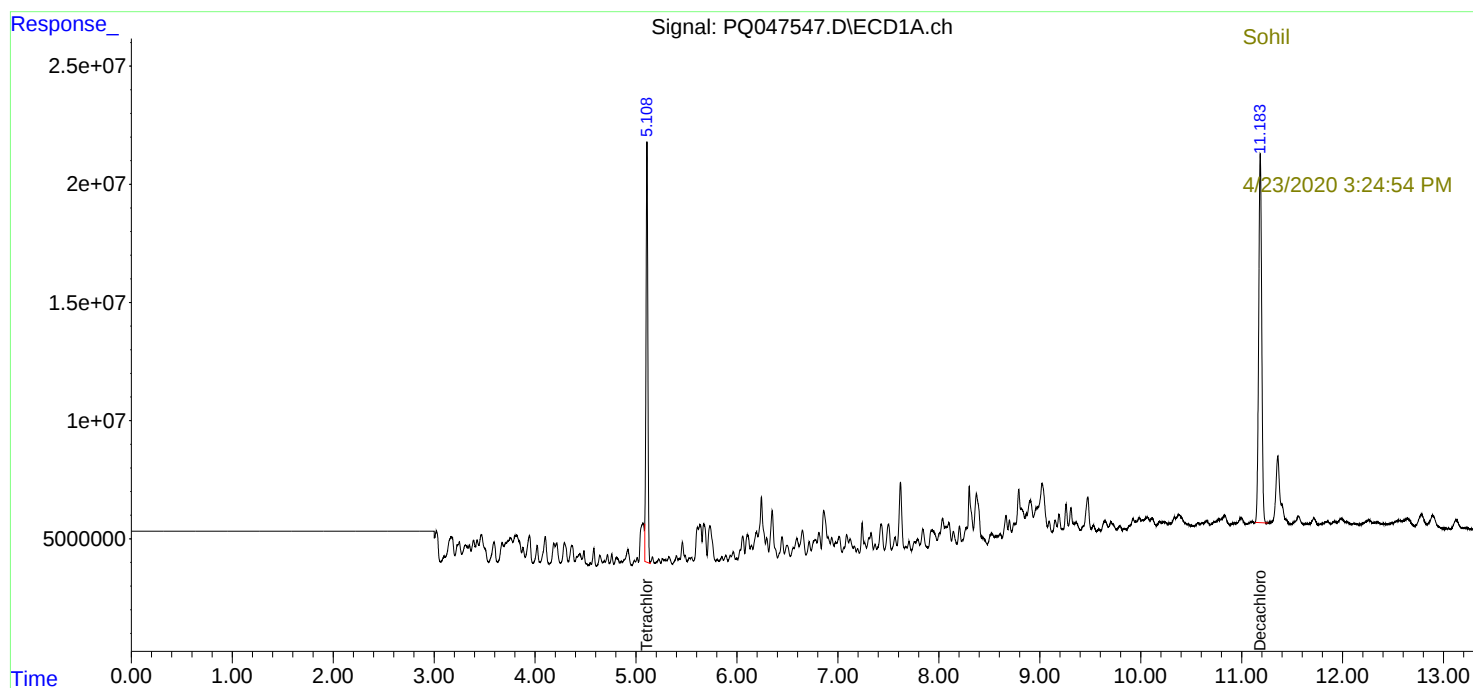

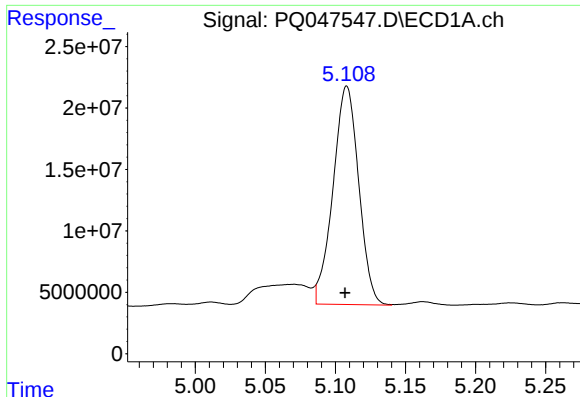


#1 Tetrachloro-m-xylene

R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 226459917
Conc: 12.32 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
TP-16A


Manual Integrations
APPROVED

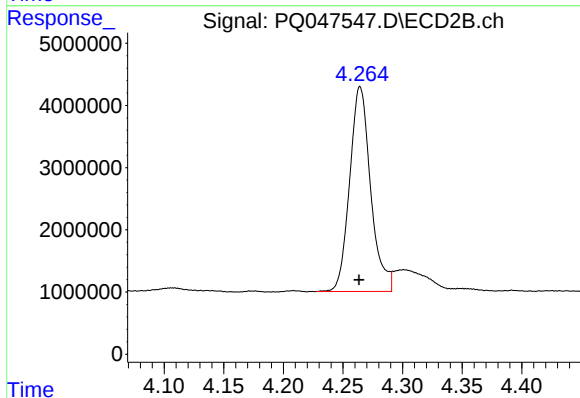

#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 40325267
Conc: 13.55 ng/ml


Sohil

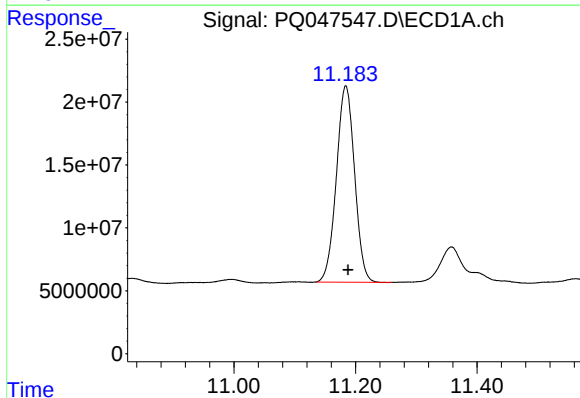

#2 Decachlorobiphenyl

R.T.: 11.184 min
Delta R.T.: -0.004 min
Response: 324341944
Conc: 15.19 ng/ml

4/23/2020 3:24:54 PM

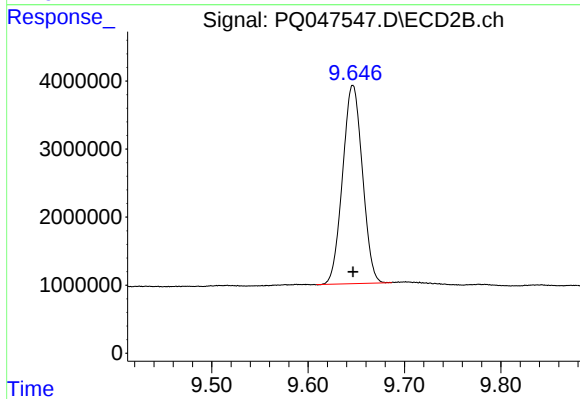

#2 Decachlorobiphenyl

R.T.: 9.646 min
Delta R.T.: 0.000 min
Response: 41496528
Conc: 13.27 ng/ml