

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ051019\
 Data File : PQ039574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 May 2019 14:22
 Operator : AJ\MA
 Sample : K2762-16RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 P021-SS003-0612-01RE

Manual Integrations
 APPROVED

Ankita
 5/13/2019 4:16:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 10 23:02:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ050919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 10 01:55:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	5.663	4.765	83687678	54160649	14.640	14.758
2) SA Decachlor...	12.043	10.519	51838164	26280424	8.023m	7.932

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ051019\
Data File : PQ039574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 May 2019 14:22
Operator : AJ\MA
Sample : K2762-16RE
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
P021-SS003-0612-01RE


Manual Integrations
APPROVED

Ankita
5/13/2019 4:16:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 10 23:02:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ050919.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 10 01:55:02 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

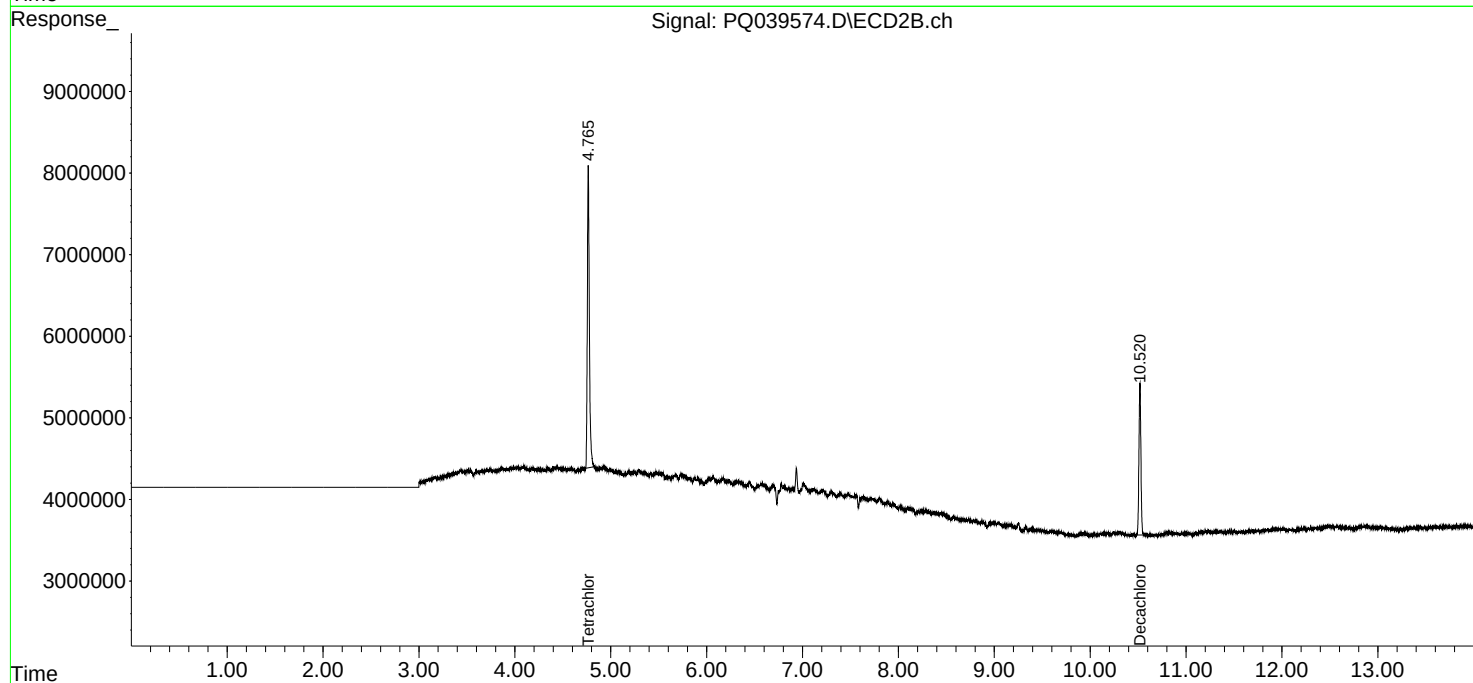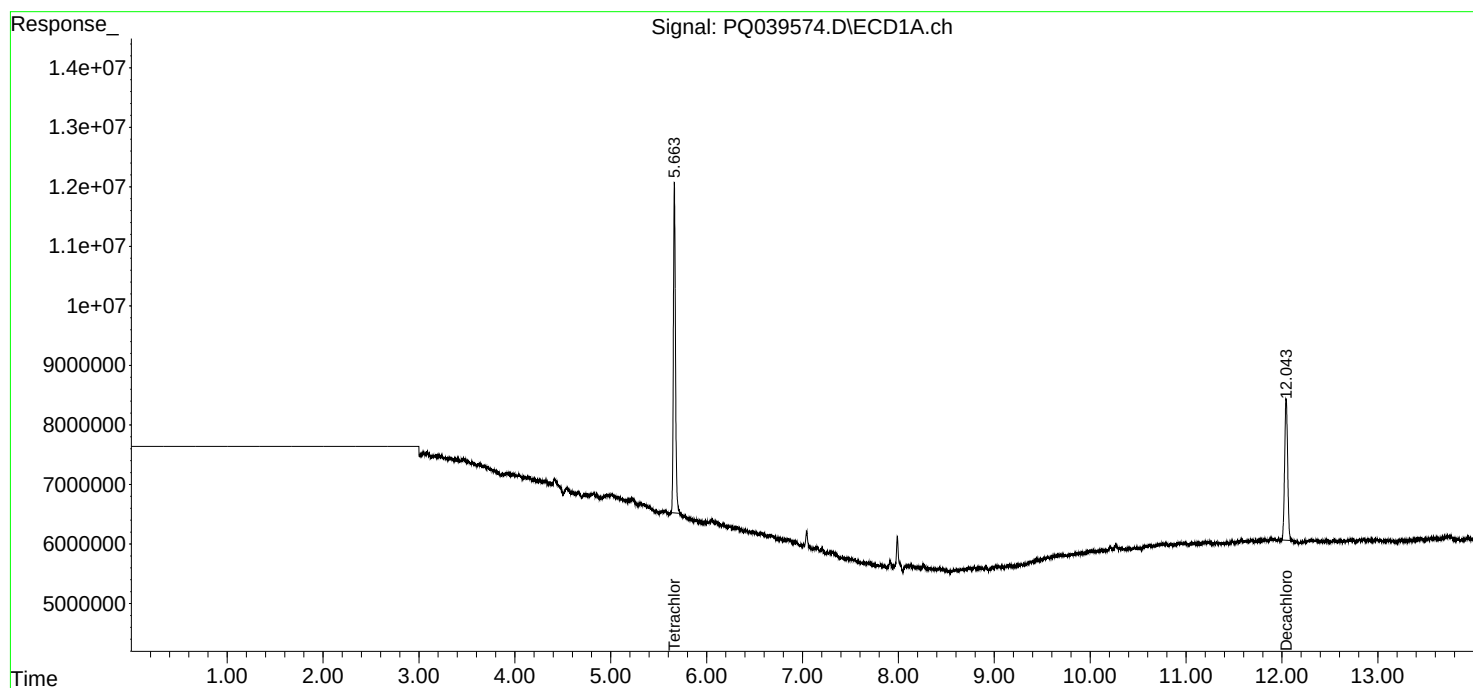

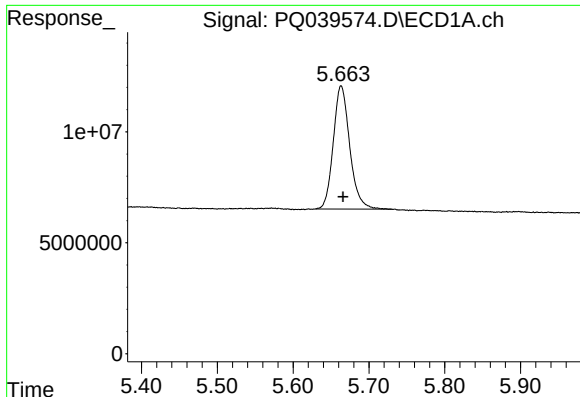


#1 Tetrachloro-m-xylene

R.T.: 5.663 min
Delta R.T.: -0.003 min
Response: 83687678
Conc: 14.64 ng/ml

Instrument :
ECD_Q
ClientSampleId :
P021-SS003-0612-01RE


Manual Integrations
APPROVED

Ankita
5/13/2019 4:16:48 PM

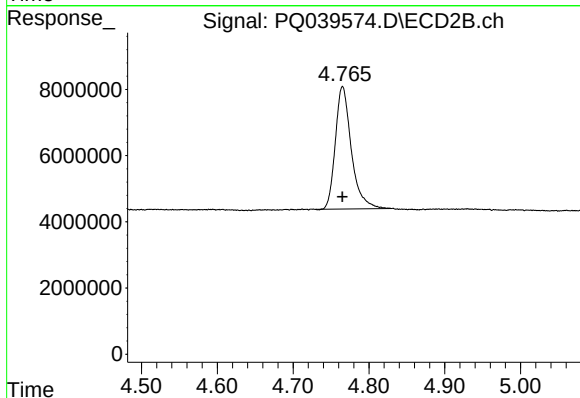


#1 Tetrachloro-m-xylene

R.T.: 4.765 min
Delta R.T.: 0.000 min
Response: 54160649
Conc: 14.76 ng/ml

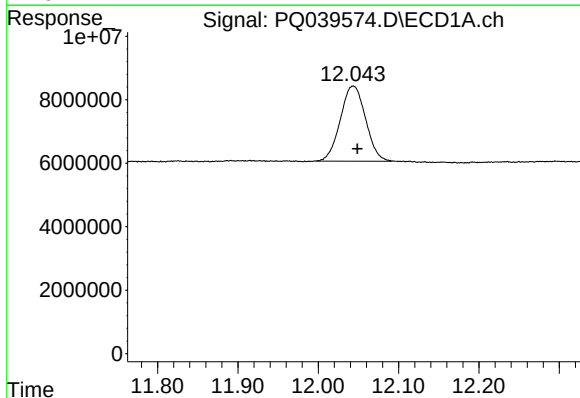

#2 Decachlorobiphenyl

R.T.: 12.043 min
Delta R.T.: -0.005 min
Response: 51838164
Conc: 8.02 ng/ml m

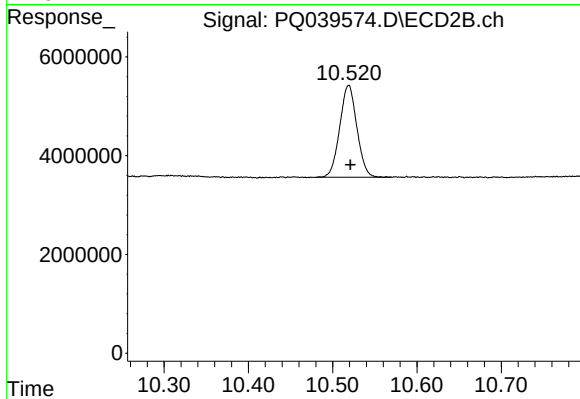

#2 Decachlorobiphenyl

R.T.: 10.519 min
Delta R.T.: -0.002 min
Response: 26280424
Conc: 7.93 ng/ml