

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ052623\
 Data File : PQ061300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2023 20:43
 Operator : YP\AJ
 Sample : 02908-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 TWP02

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/30/2023
 Supervised By :Ankita Jodhani 05/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 21:57:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 25 13:25:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.760	101.9E6	57394009	20.331m	19.867
2) SA Decachlor...	8.584	7.534	55595508	55237161	14.373	15.169

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ052623\
Data File : PQ061300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2023 20:43
Operator : YP\AJ
Sample : 02908-13
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
TWP02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2023
Supervised By :Ankita Jodhani 05/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 21:57:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052523.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 25 13:25:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

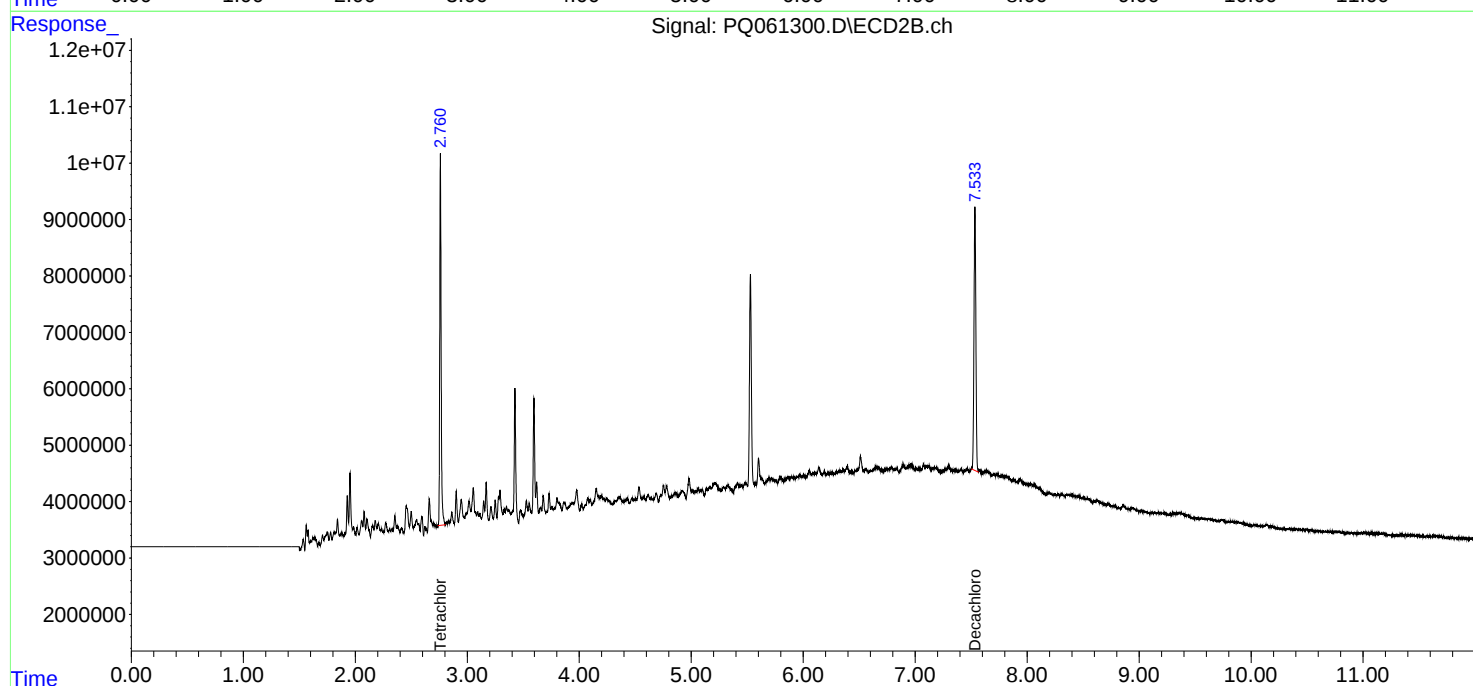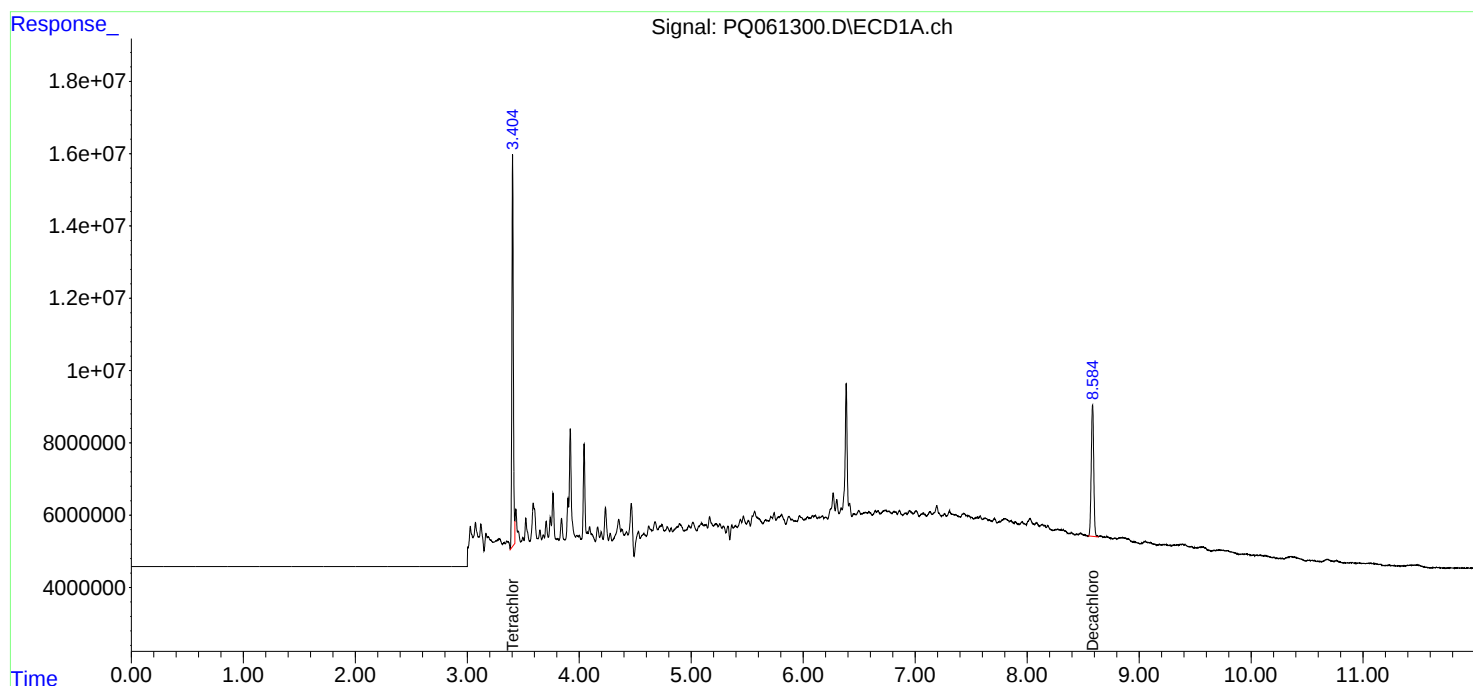

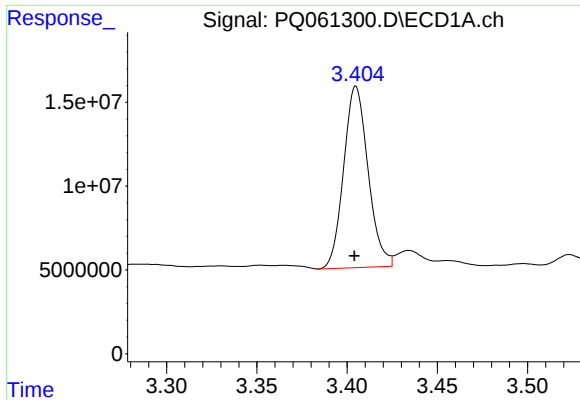


#1 Tetrachloro-m-xylene

R.T.: 3.404 min
Delta R.T.: 0.000 min
Response: 101874099
Conc: 20.33 ng/ml

Instrument :
ECD_Q
ClientSampleId :
TWP02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2023
Supervised By :Ankita Jodhani 05/30/2023

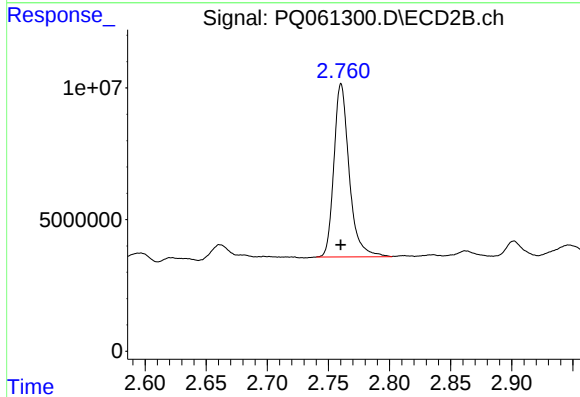


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 57394009
Conc: 19.87 ng/ml

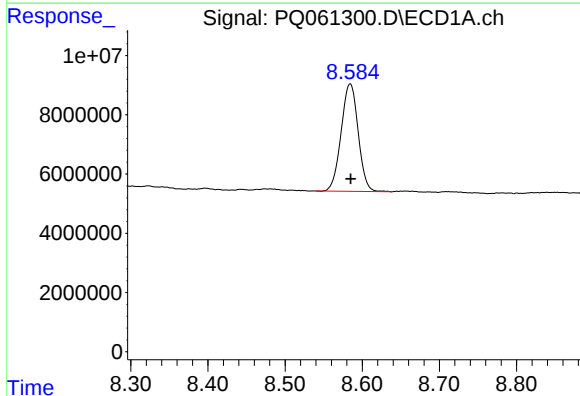

#2 Decachlorobiphenyl

R.T.: 8.584 min
Delta R.T.: 0.000 min
Response: 55595508
Conc: 14.37 ng/ml

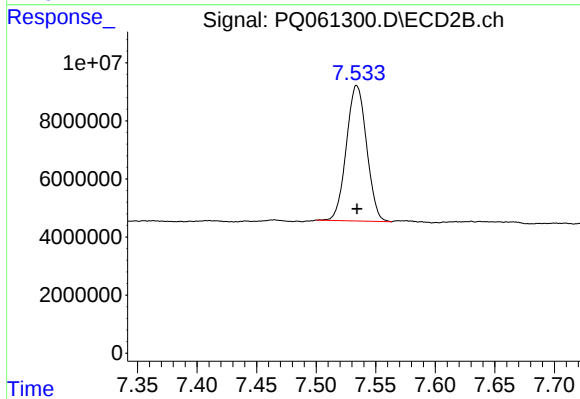

#2 Decachlorobiphenyl

R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 55237161
Conc: 15.17 ng/ml