

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ052623\
 Data File : PQ061303.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2023 21:27
 Operator : YP\AJ
 Sample : 02955-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 TWP05

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/30/2023
 Supervised By :Ankita Jodhani 05/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 05:26:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 25 13:25:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.405	2.760	78067382	50305327	15.580m	17.413
2) SA Decachlor...	8.583	7.533	58715267	56470187	15.179	15.508

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ052623\
Data File : PQ061303.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2023 21:27
Operator : YP\AJ
Sample : 02955-15
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
TWP05


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2023
Supervised By :Ankita Jodhani 05/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 05:26:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052523.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 25 13:25:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

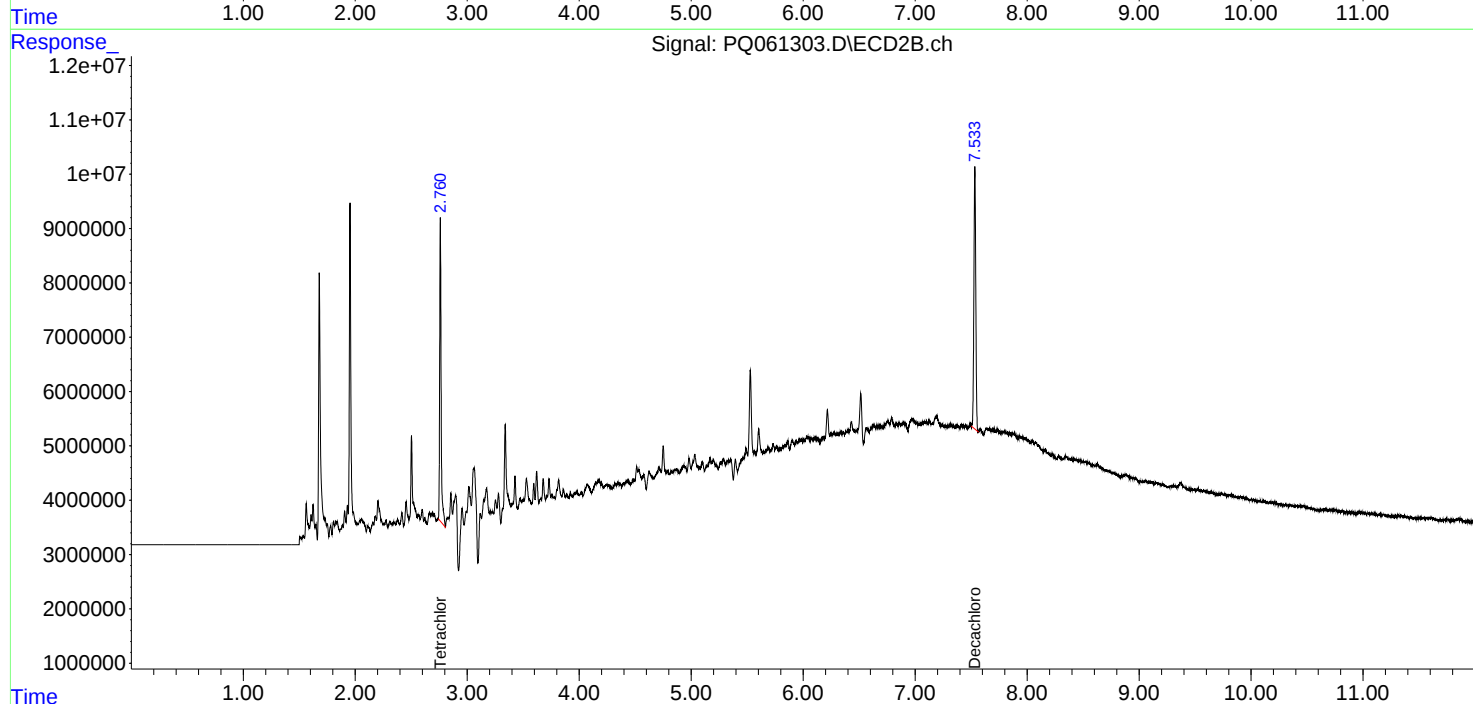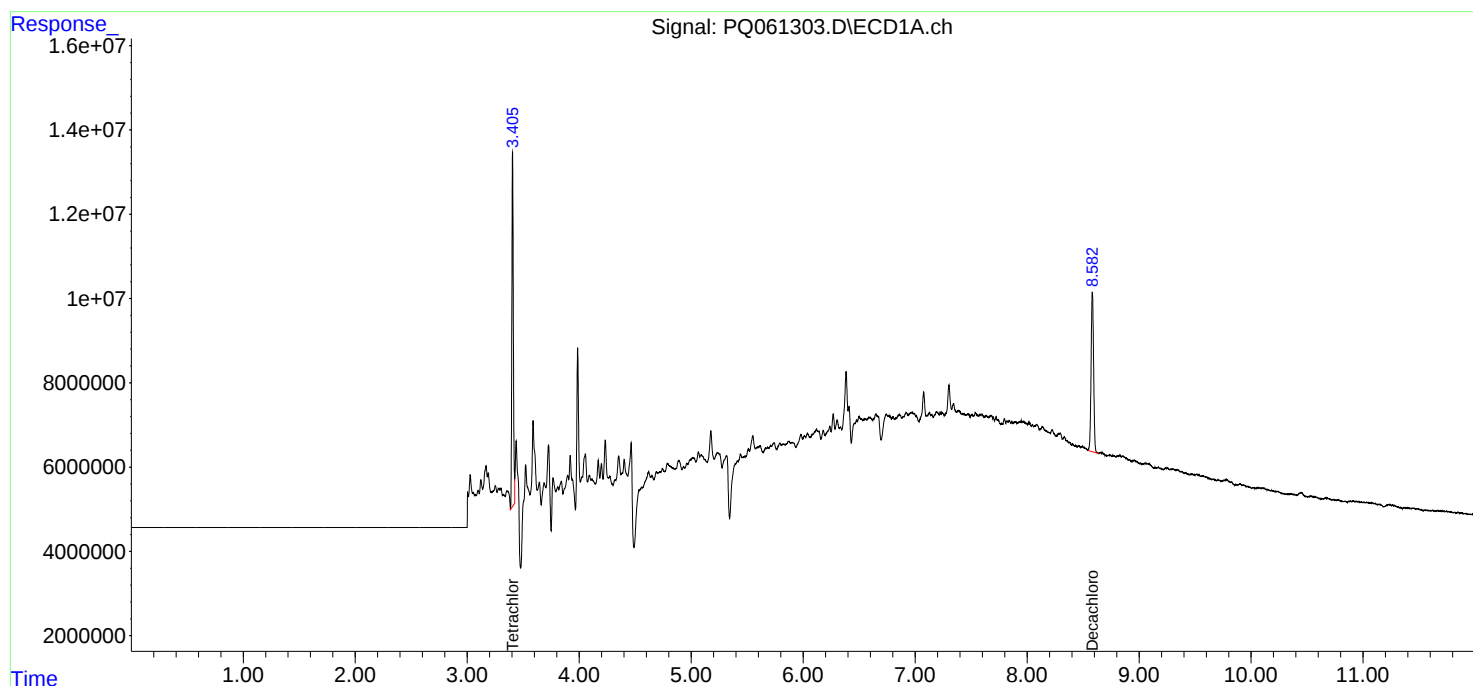

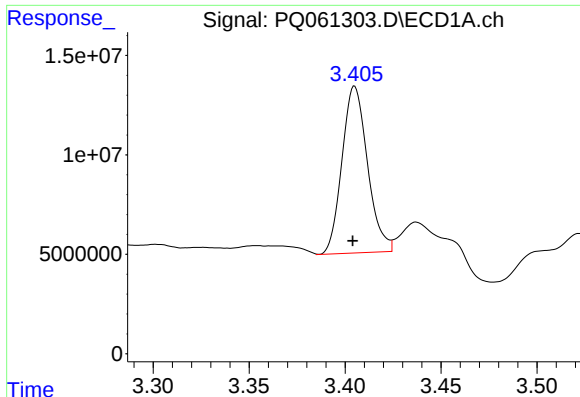


#1 Tetrachloro-m-xylene

R.T.: 3.405 min
Delta R.T.: 0.000 min
Response: 78067382
Conc: 15.58 ng/ml

Instrument :
ECD_Q
ClientSampleId :
TWP05


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2023
Supervised By :Ankita Jodhani 05/30/2023

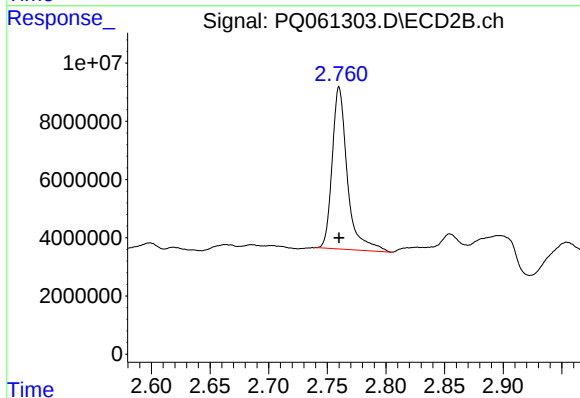


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 50305327
Conc: 17.41 ng/ml

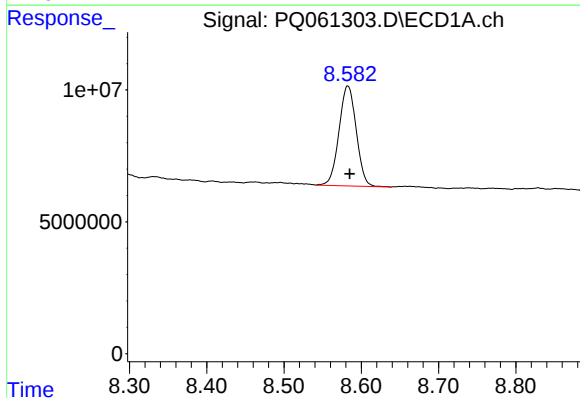

#2 Decachlorobiphenyl

R.T.: 8.583 min
Delta R.T.: -0.002 min
Response: 58715267
Conc: 15.18 ng/ml

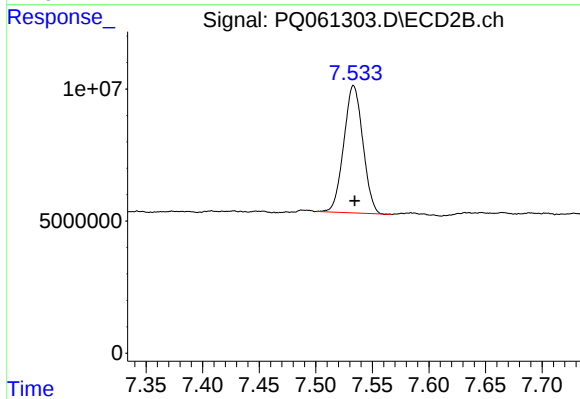

#2 Decachlorobiphenyl

R.T.: 7.533 min
Delta R.T.: 0.000 min
Response: 56470187
Conc: 15.51 ng/ml