

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060220\
 Data File : PQ047973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2020 14:54
 Operator : AJ\MA
 Sample : L2832-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 20200383-DI-WATER

Manual Integrations
 APPROVED

Sohil
 6/4/2020 8:35:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 15:28:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 27 17:33:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.317	4.296	188.9E6	93004366	26.442	27.871m
2) SA Decachlor...	11.610	9.673	188.9E6	99433256	26.452	27.495

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060220\
Data File : PQ047973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2020 14:54
Operator : AJ\MA
Sample : L2832-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
20200383-DI-WATER


Manual Integrations
APPROVED

Sohil
6/4/2020 8:35:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 15:28:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 27 17:33:08 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

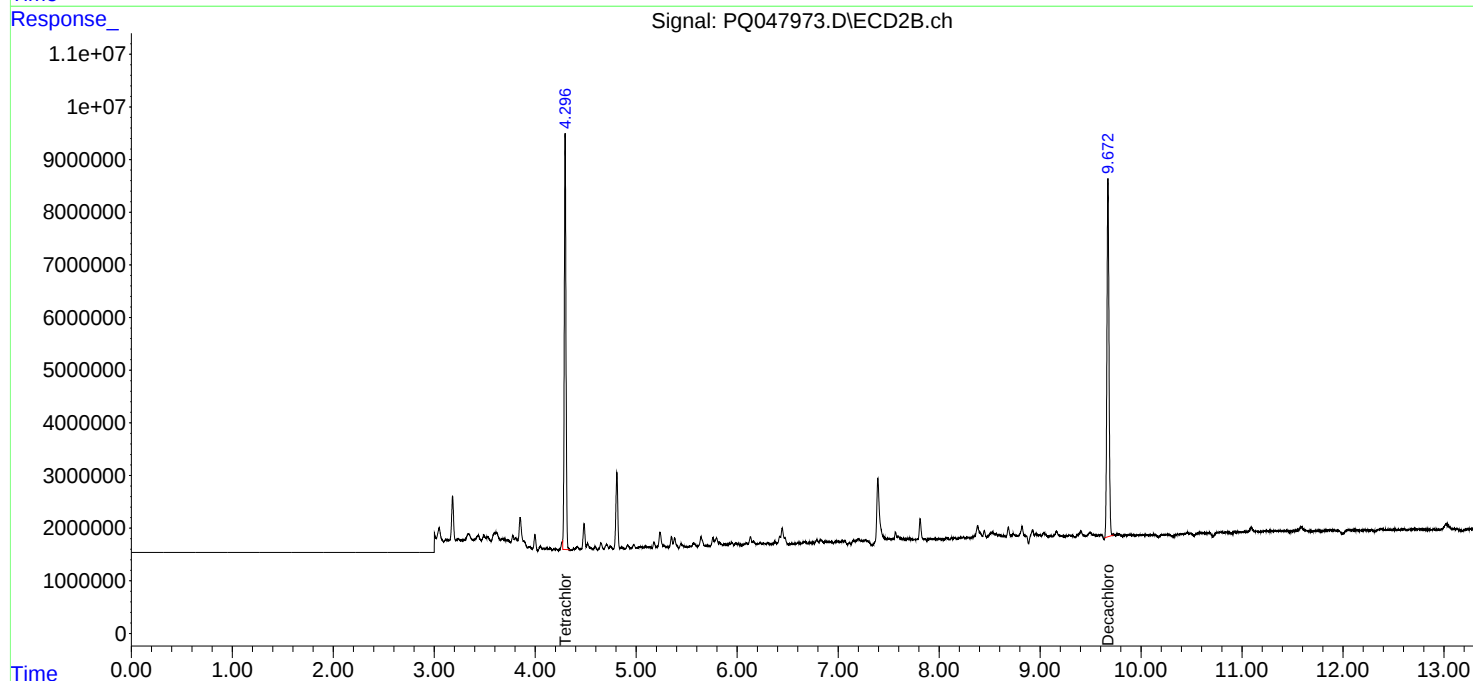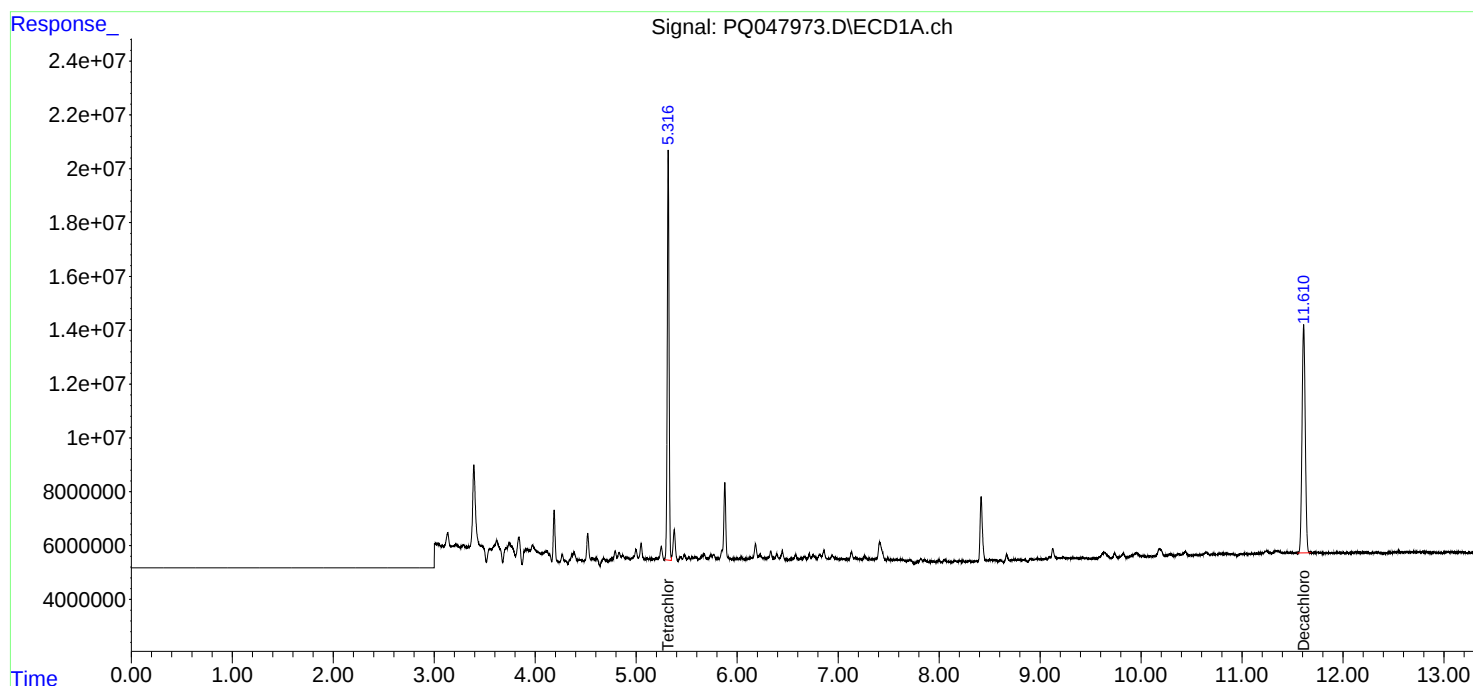

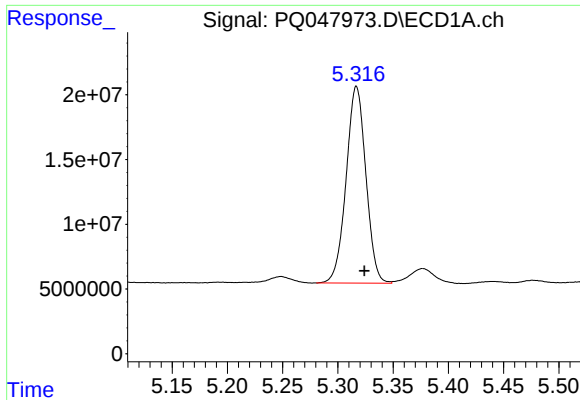


#1 Tetrachloro-m-xylene

R.T.: 5.317 min
Delta R.T.: -0.007 min
Response: 188934781
Conc: 26.44 ng/ml

Instrument :
ECD_Q
ClientSampleId :
20200383-DI-WATER


Manual Integrations
APPROVED

Sohil
6/4/2020 8:35:56 AM

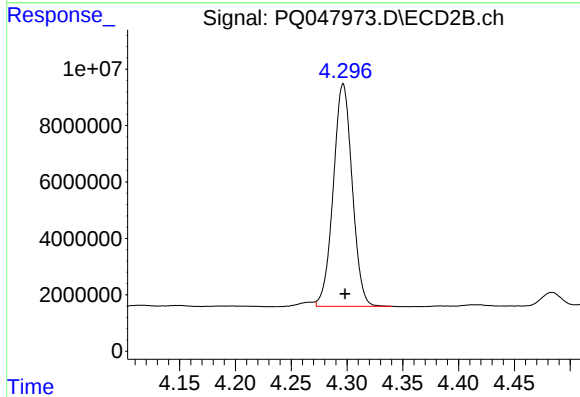


#1 Tetrachloro-m-xylene

R.T.: 4.296 min
Delta R.T.: -0.002 min
Response: 93004366
Conc: 27.87 ng/ml m

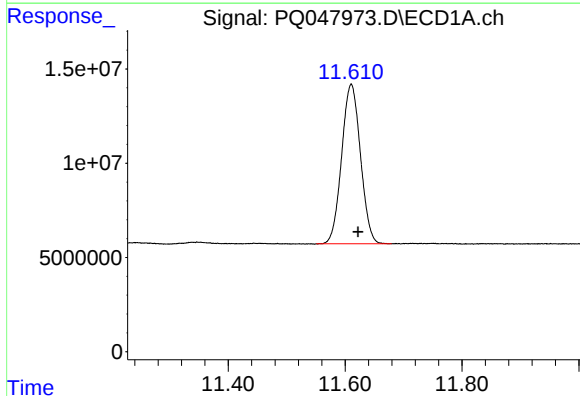

#2 Decachlorobiphenyl

R.T.: 11.610 min
Delta R.T.: -0.012 min
Response: 188922003
Conc: 26.45 ng/ml

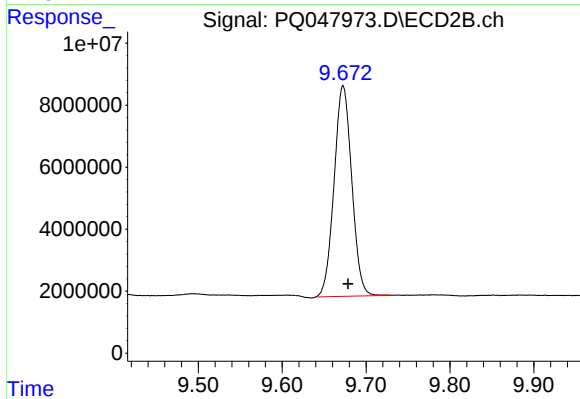

#2 Decachlorobiphenyl

R.T.: 9.673 min
Delta R.T.: -0.006 min
Response: 99433256
Conc: 27.49 ng/ml