

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060220\
 Data File : PQ047974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2020 15:10
 Operator : AJ\MA
 Sample : L2494-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 20200382-MANASQUAN-WATER

Manual Integrations
 APPROVED

Sohil
 6/4/2020 8:35:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 15:28:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 27 17:33:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.319	4.299	234.9E6	111.1E6	32.874m	33.279m
2) SA Decachlor...	11.611	9.674	170.4E6	88582927	23.853	24.495

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060220\
Data File : PQ047974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2020 15:10
Operator : AJ\MA
Sample : L2494-02
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
20200382-MANASQUAN-WATER


Manual Integrations
APPROVED

Sohil
6/4/2020 8:35:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 15:28:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 27 17:33:08 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

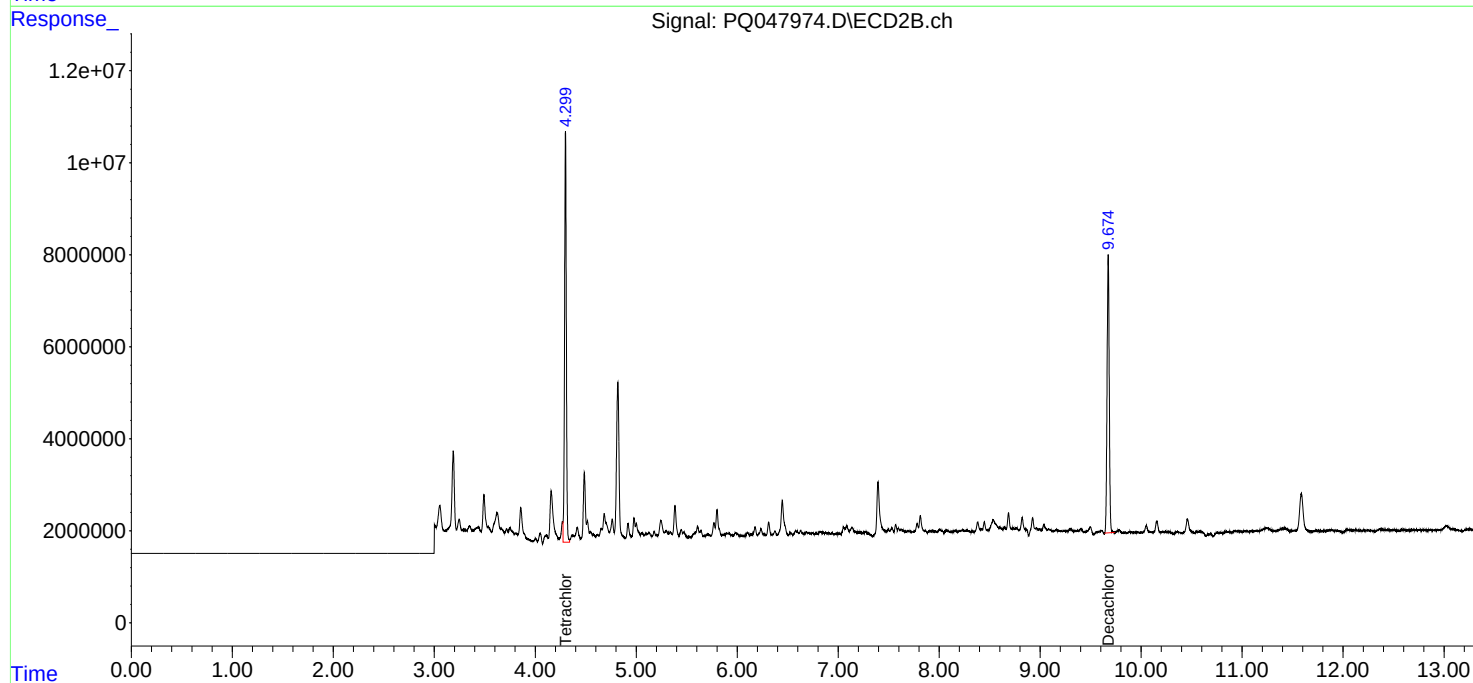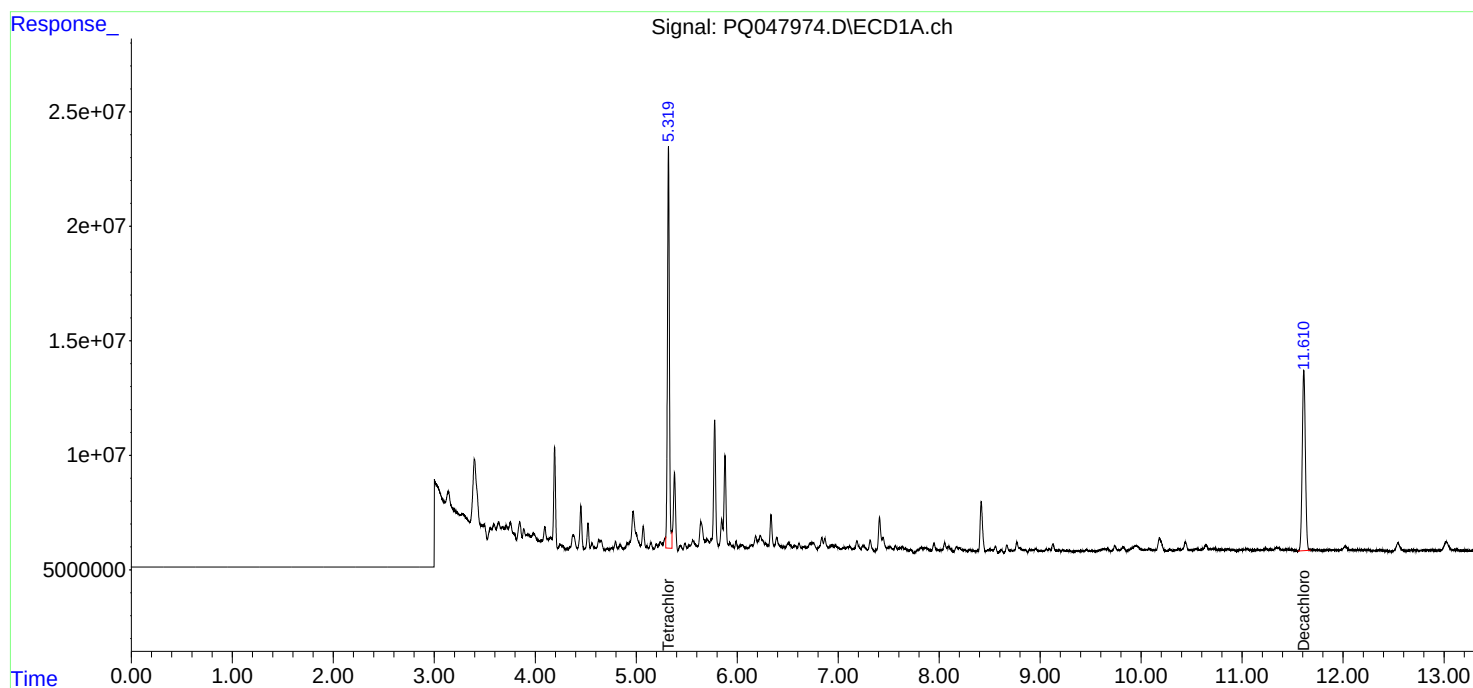

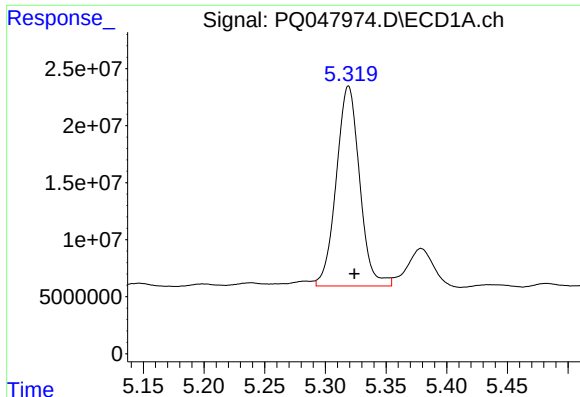


#1 Tetrachloro-m-xylene

R.T.: 5.319 min
Delta R.T.: -0.005 min
Response: 234897164
Conc: 32.87 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
20200382-MANASQUAN-WATER


Manual Integrations
APPROVED

Sohil
6/4/2020 8:35:57 AM

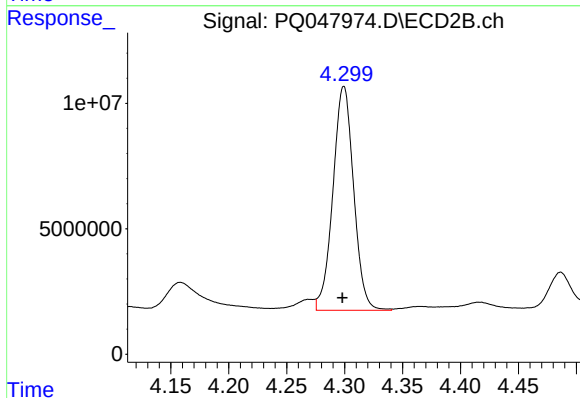


#1 Tetrachloro-m-xylene

R.T.: 4.299 min
Delta R.T.: 0.001 min
Response: 111052394
Conc: 33.28 ng/ml m

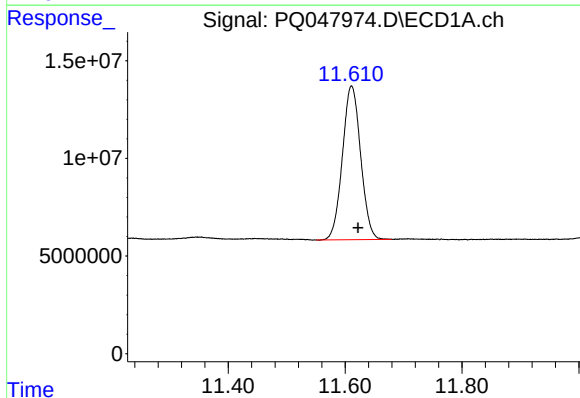

#2 Decachlorobiphenyl

R.T.: 11.611 min
Delta R.T.: -0.011 min
Response: 170359714
Conc: 23.85 ng/ml

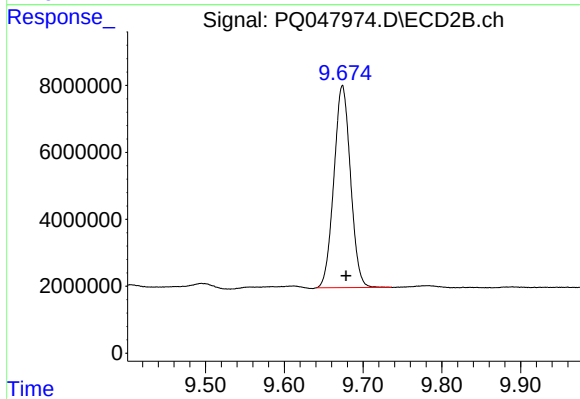

#2 Decachlorobiphenyl

R.T.: 9.674 min
Delta R.T.: -0.005 min
Response: 88582927
Conc: 24.49 ng/ml