

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061020\
 Data File : PQ048249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2020 08:57
 Operator : AJ\MA
 Sample : L2494-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 20200382-MANASQUAN-WATER

Manual Integrations
 APPROVED

Sohil
 6/11/2020 2:44:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 12:18:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 10 03:52:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.301	4.292	223.5E6	108.7E6	26.152m	26.323m
2) SA Decachlor...	11.579	9.663	200.5E6	93285047	21.621	20.842

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061020\
Data File : PQ048249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2020 08:57
Operator : AJ\MA
Sample : L2494-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
20200382-MANASQUAN-WATER


Manual Integrations
APPROVED

Sohil
6/11/2020 2:44:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 12:18:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 10 03:52:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

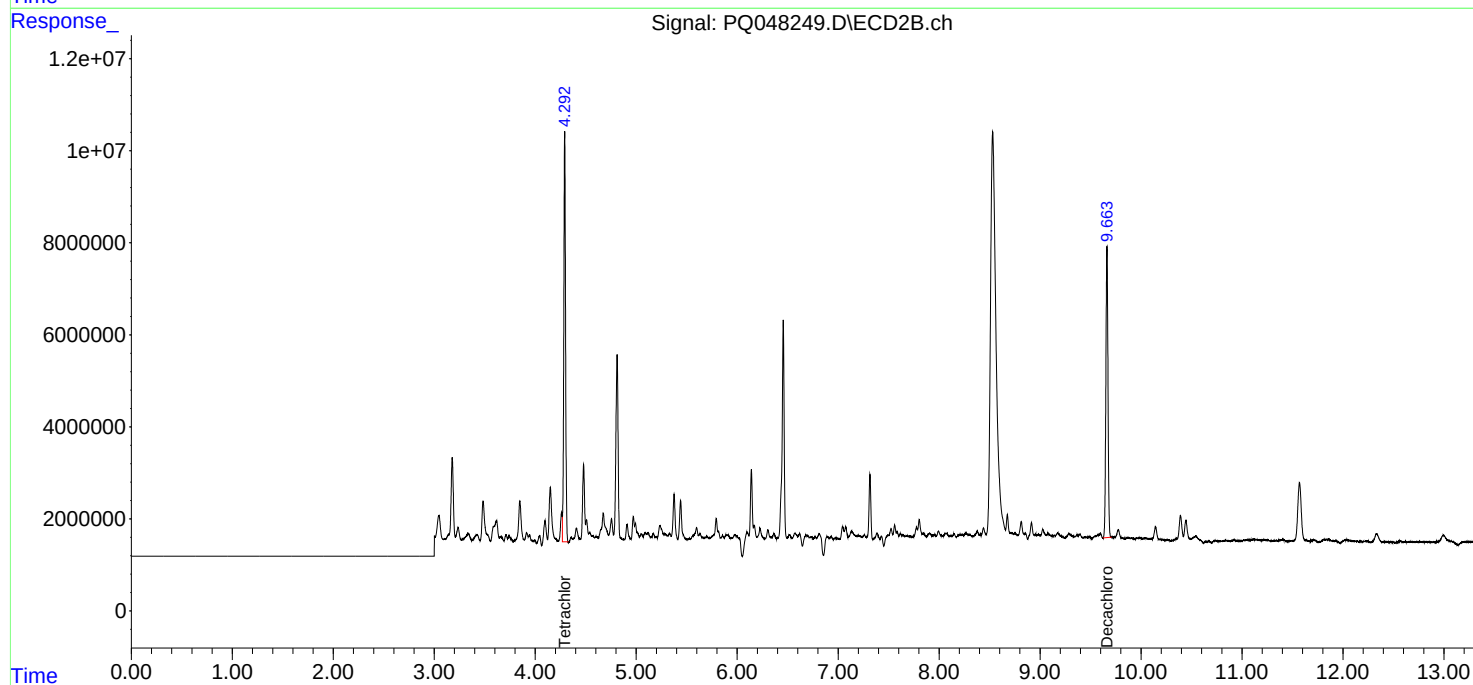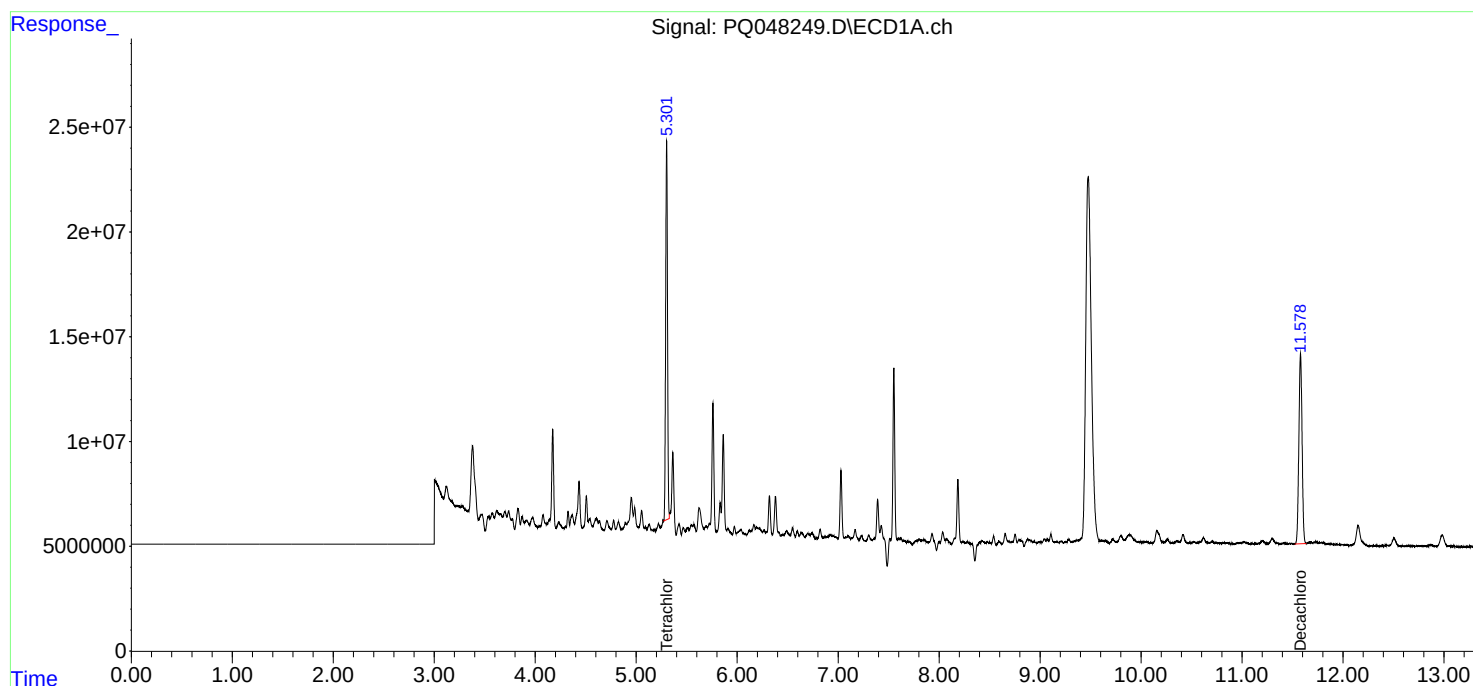

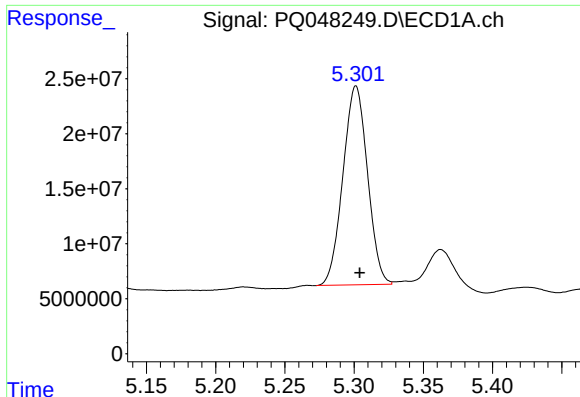


#1 Tetrachloro-m-xylene

R.T.: 5.301 min
Delta R.T.: -0.003 min
Response: 223470780
Conc: 26.15 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
20200382-MANASQUAN-WATER


Manual Integrations
APPROVED

Sohil
6/11/2020 2:44:26 PM

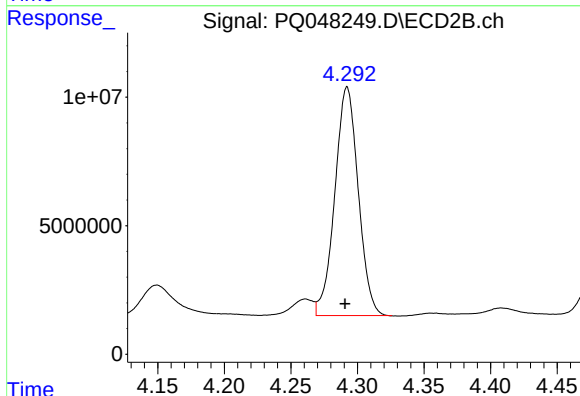


#1 Tetrachloro-m-xylene

R.T.: 4.292 min
Delta R.T.: 0.001 min
Response: 108723942
Conc: 26.32 ng/ml m

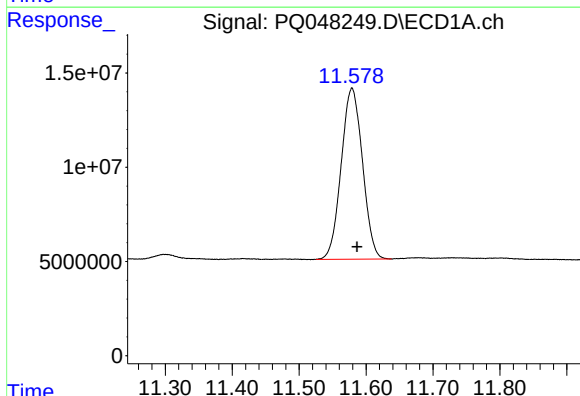

#2 Decachlorobiphenyl

R.T.: 11.579 min
Delta R.T.: -0.008 min
Response: 200485632
Conc: 21.62 ng/ml

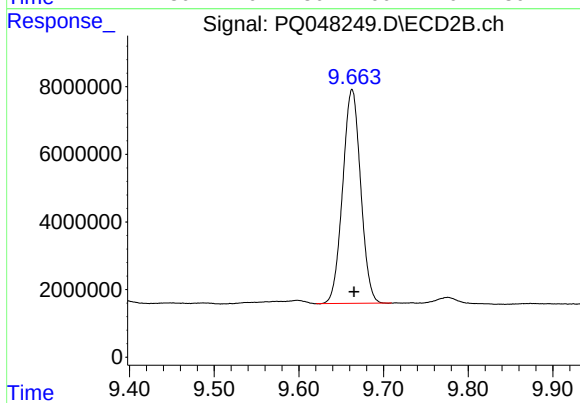

#2 Decachlorobiphenyl

R.T.: 9.663 min
Delta R.T.: -0.002 min
Response: 93285047
Conc: 20.84 ng/ml