

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061120\
 Data File : PQ048363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2020 21:30
 Operator : AJ\MA
 Sample : L2965-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SAFE-COMP

Manual Integrations
 APPROVED

Sohil
 6/15/2020 8:30:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 06:05:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060920.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 10 03:52:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.295	4.290	116.2E6	60178479	13.603	14.570
2) SA Decachlor...	11.566	9.656	118.6E6	70075492	12.787	15.656m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061120\
Data File : PQ048363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2020 21:30
Operator : AJ\MA
Sample : L2965-08
Misc :
ALS Vial : 27 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 06:05:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060920.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 10 03:52:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Instrument :
ECD_Q
ClientSampleId :
SAFE-COMP

Manual Integrations
APPROVED


Sohil
6/15/2020 8:30:20 AM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

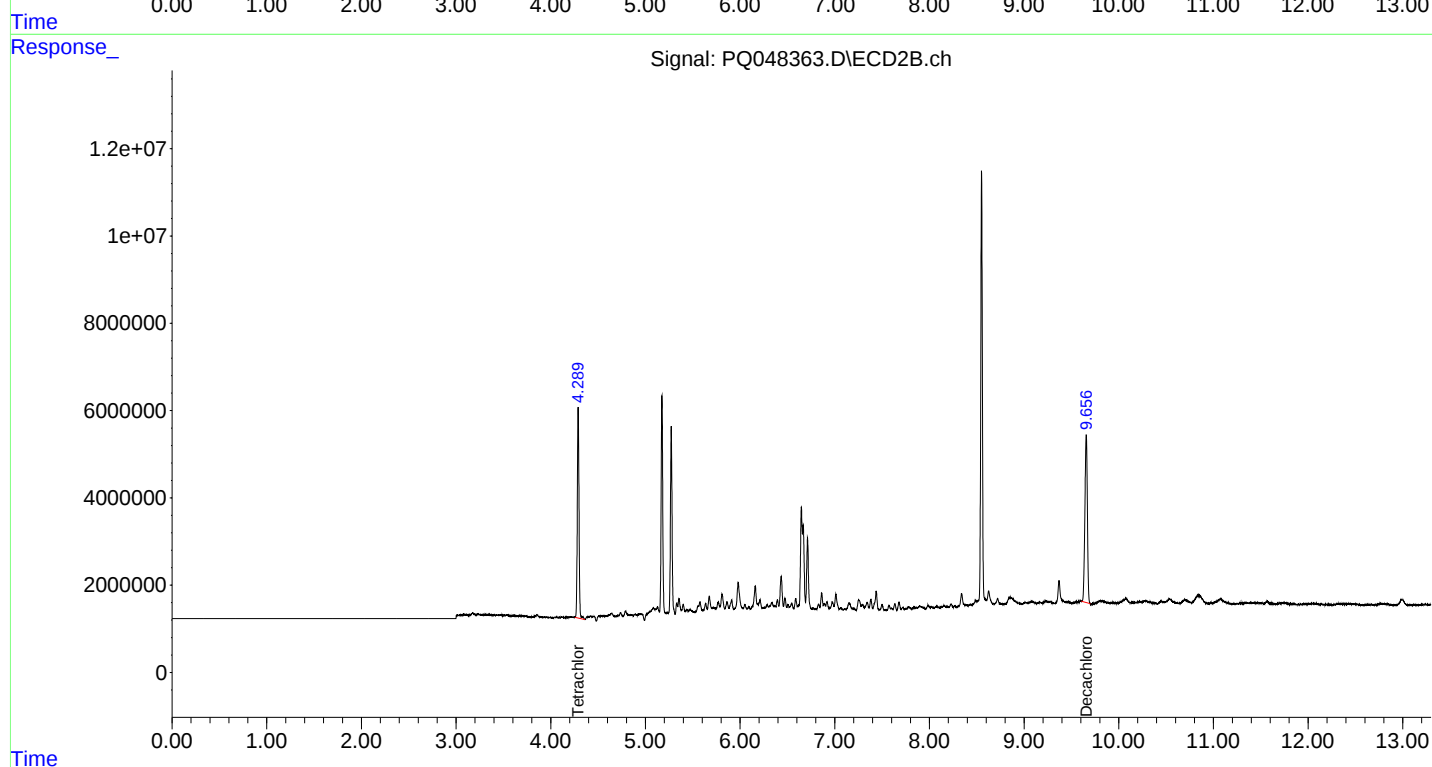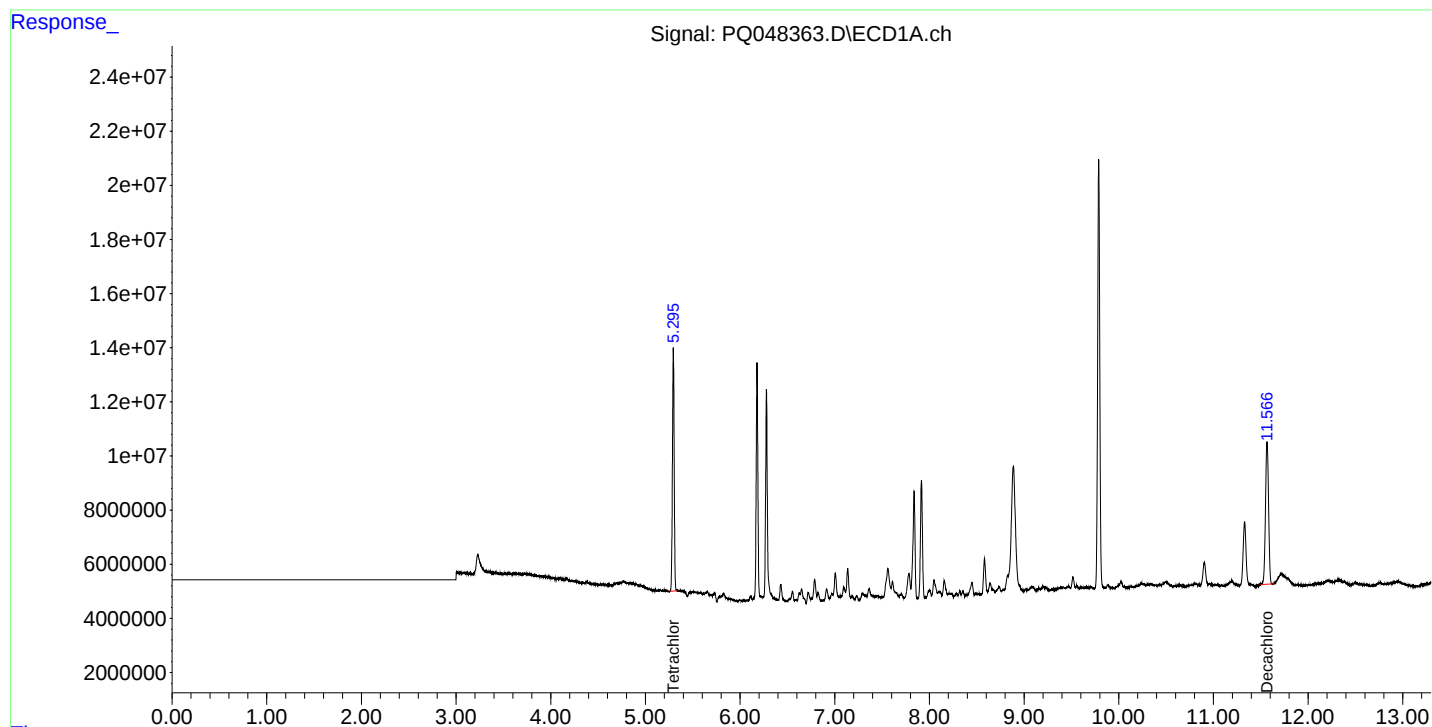

Response_

Signal: PQ048363.D\ECD1A.ch

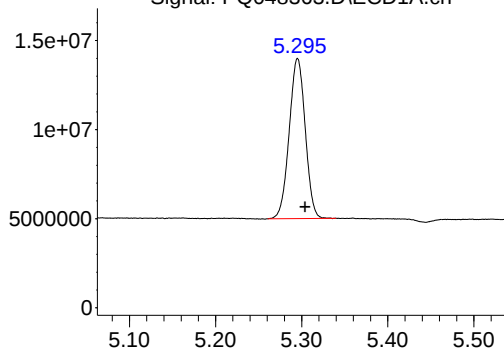

#1 Tetrachloro-m-xylene

R.T.: 5.295 min
Delta R.T.: -0.009 min
Response: 116239744
Conc: 13.60 ng/ml

Instrument :

ECD_Q


ClientSampleId :

SAFE-COMP

Time

Response_

Signal: PQ048363.D\ECD2B.ch

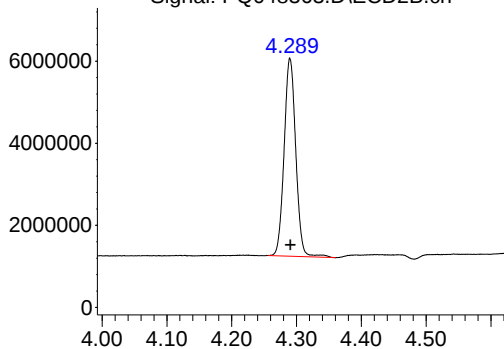

#1 Tetrachloro-m-xylene

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 60178479
Conc: 14.57 ng/ml

Manual Integrations
APPROVED

Sohil

6/15/2020 8:30:20 AM

Time