

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ101719\  
Data File : PQ044458.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 17 Oct 2019 07:19  
Operator : HP\AJ  
Sample : K5236-10  
Misc :  
ALS Vial : 35 Sample Multiplier: 1


Instrument :  
ECD\_Q  
ClientSampleId :  
BEPL9

Manual Integrations  
APPROVED

Ankita  
10/21/2019 10:18:28 AM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 17 09:00:09 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ100819CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Oct 10 02:55:10 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

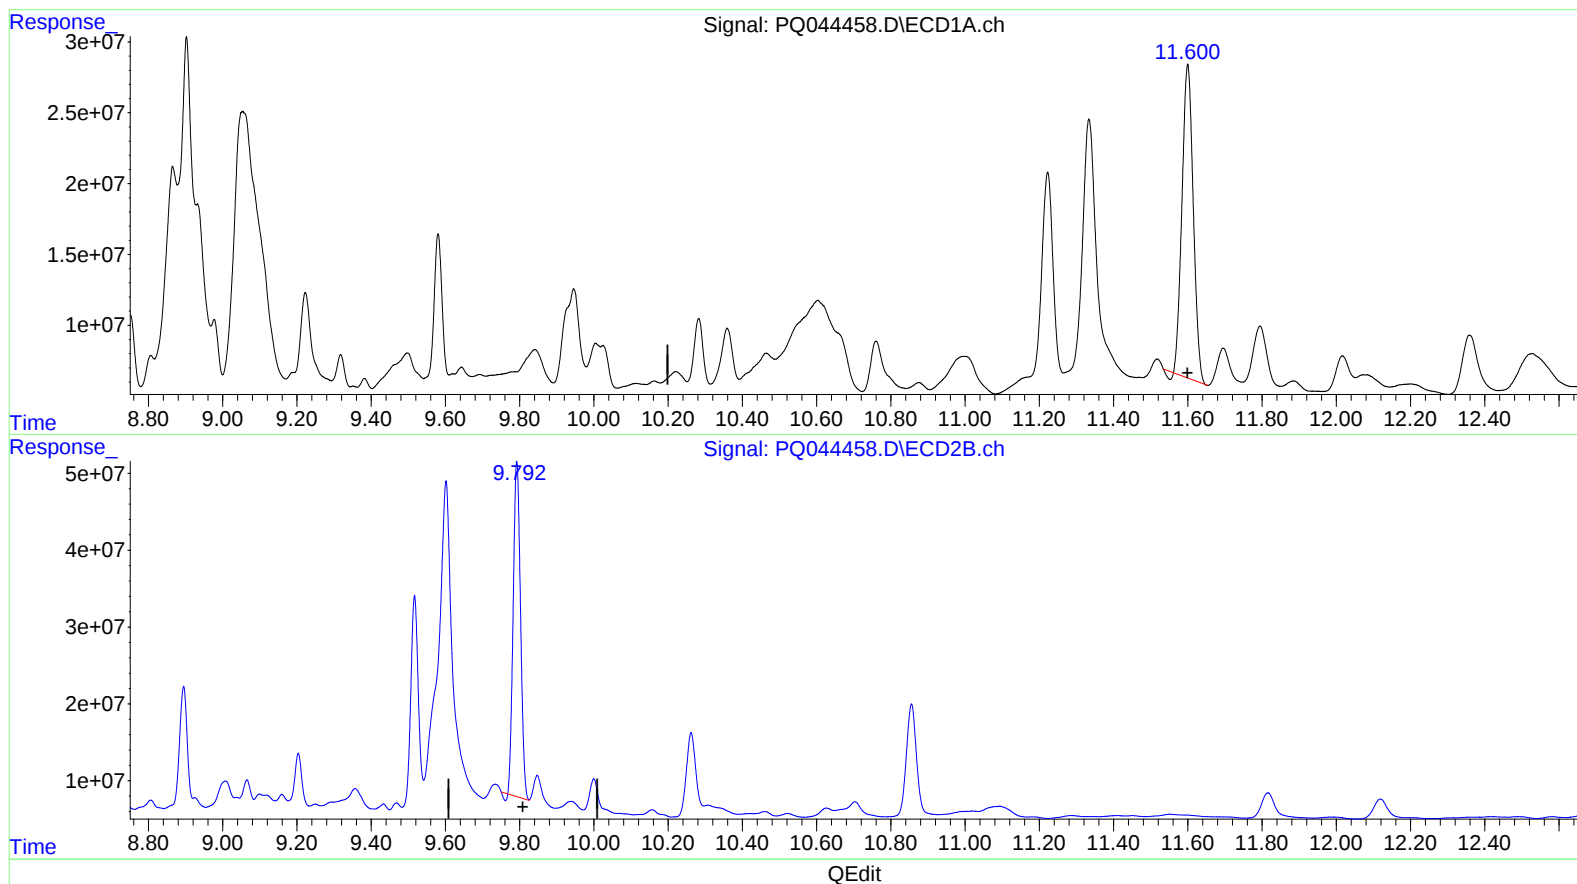

(2) Decachlorobiphenyl (SA)

11.600min 86.747 ng/ml

response 464750871

(2) Decachlorobiphenyl #2 (SA)

9.792min 99.079 ng/ml

response 592632392

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ101719\  
Data File : PQ044458.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 17 Oct 2019 07:19  
Operator : HP\AJ  
Sample : K5236-10  
Misc :  
ALS Vial : 35 Sample Multiplier: 1


Instrument :  
ECD\_Q  
ClientSampleId :  
BEPL9

Manual Integrations  
APPROVED

Ankita  
10/21/2019 10:18:28 AM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 17 09:00:09 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ100819CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Oct 10 02:55:10 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

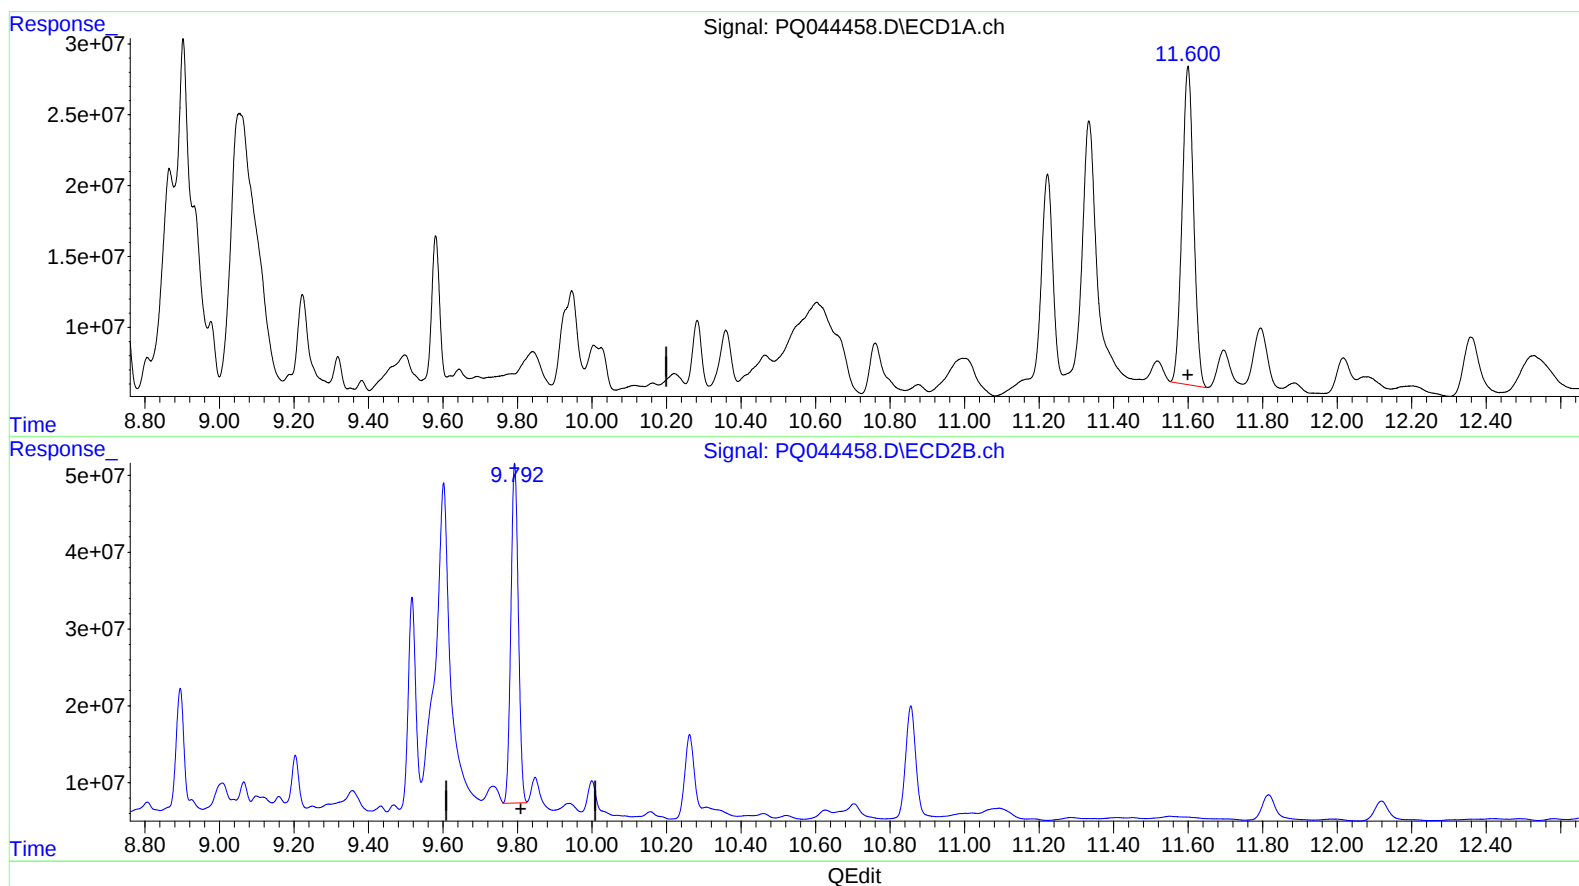

(2) Decachlorobiphenyl (SA)

11.600min 90.516 ng/ml m

response 484942277

(2) Decachlorobiphenyl #2 (SA)

9.792min 103.353 ng/ml m

response 618197238

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Data\PQ101719\  
 Data File : PQ044458.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 17 Oct 2019 07:19  
 Operator : HP\AJ  
 Sample : K5236-10  
 Misc :  
 ALS Vial : 35 Sample Multiplier: 1

Instrument :  
 ECD\_Q  
 ClientSampleId :  
 BEPL9

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 17 09:00:09 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_Q\Method\PQ100819CLP.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Oct 10 02:55:10 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Manual Integrations  
 APPROVED

Ankita  
 10/21/2019 10:18:28 AM

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml    | ng/ml     |
|-----------------------------|--------|-------|----------|----------|----------|-----------|
| -----                       |        |       |          |          |          |           |
| System Monitoring Compounds |        |       |          |          |          |           |
| 1) SA Tetrachlo...          | 5.317  | 4.350 | 68733647 | 80968362 | 17.680   | 18.139    |
| 2) SA Decachlor...          | 11.600 | 9.792 | 484.9E6  | 618.2E6  | 90.516m  | 103.353m  |
| Target Compounds            |        |       |          |          |          |           |
| 26) L6 AR-1254-1            | 7.556  | 6.515 | 116.3E6  | 200.4E6  | 864.116  | 687.121   |
| 27) L6 AR-1254-2            | 7.786  | 6.673 | 227.0E6  | 245.5E6  | 1062.723 | 940.400   |
| 28) L6 AR-1254-3            | 8.172  | 7.101 | 266.0E6  | 572.2E6  | 1081.290 | 1309.617  |
| 29) L6 AR-1254-4            | 8.468  | 7.341 | 132.0E6  | 246.3E6  | 657.939  | 916.767 # |
| 30) L6 AR-1254-5            | 8.903  | 7.775 | 715.4E6  | 360.7E6  | 2988.981 | 902.036 # |
| -----                       |        |       |          |          |          |           |

3 AJ  
 10/23/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.