

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102718\
Data File : PQ033695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2018 21:57
Operator : SM\SJ
Sample : J5673-07DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
C0BL1DL

Manual Integrations
APPROVED

sohil
10/30/2018 1:58:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:17:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ100918CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 10 08:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

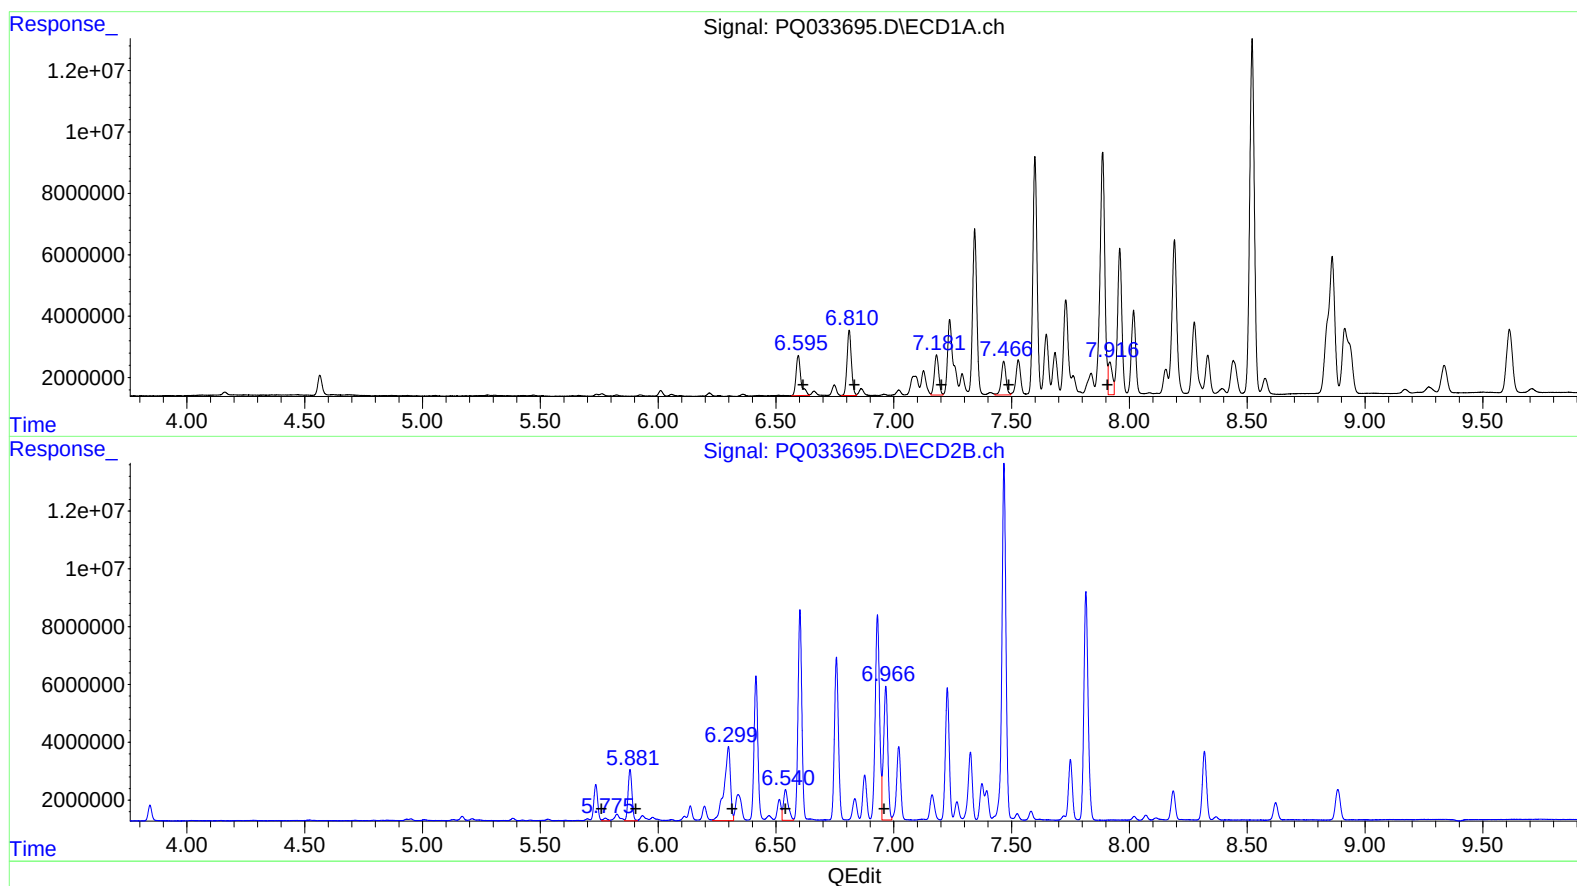

(26) AR-1254-1 (L6)
R.T. Response Conc
6.60 18958059 191.30
6.81 27255987 174.41
7.18 17211922 101.43
7.47 15239576 123.42
7.92 12902642 97.47

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
5.78 1116258 9.91
5.88 20281779 205.40
6.30 47809196 287.68
6.54 14970419 140.70
6.97 57586973 392.05

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102718\
Data File : PQ033695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2018 21:57
Operator : SM\SJ
Sample : J5673-07DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleID :
C0BL1DL

Manual Integrations
APPROVED

sohil
10/30/2018 1:58:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:17:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ100918CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 10 08:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

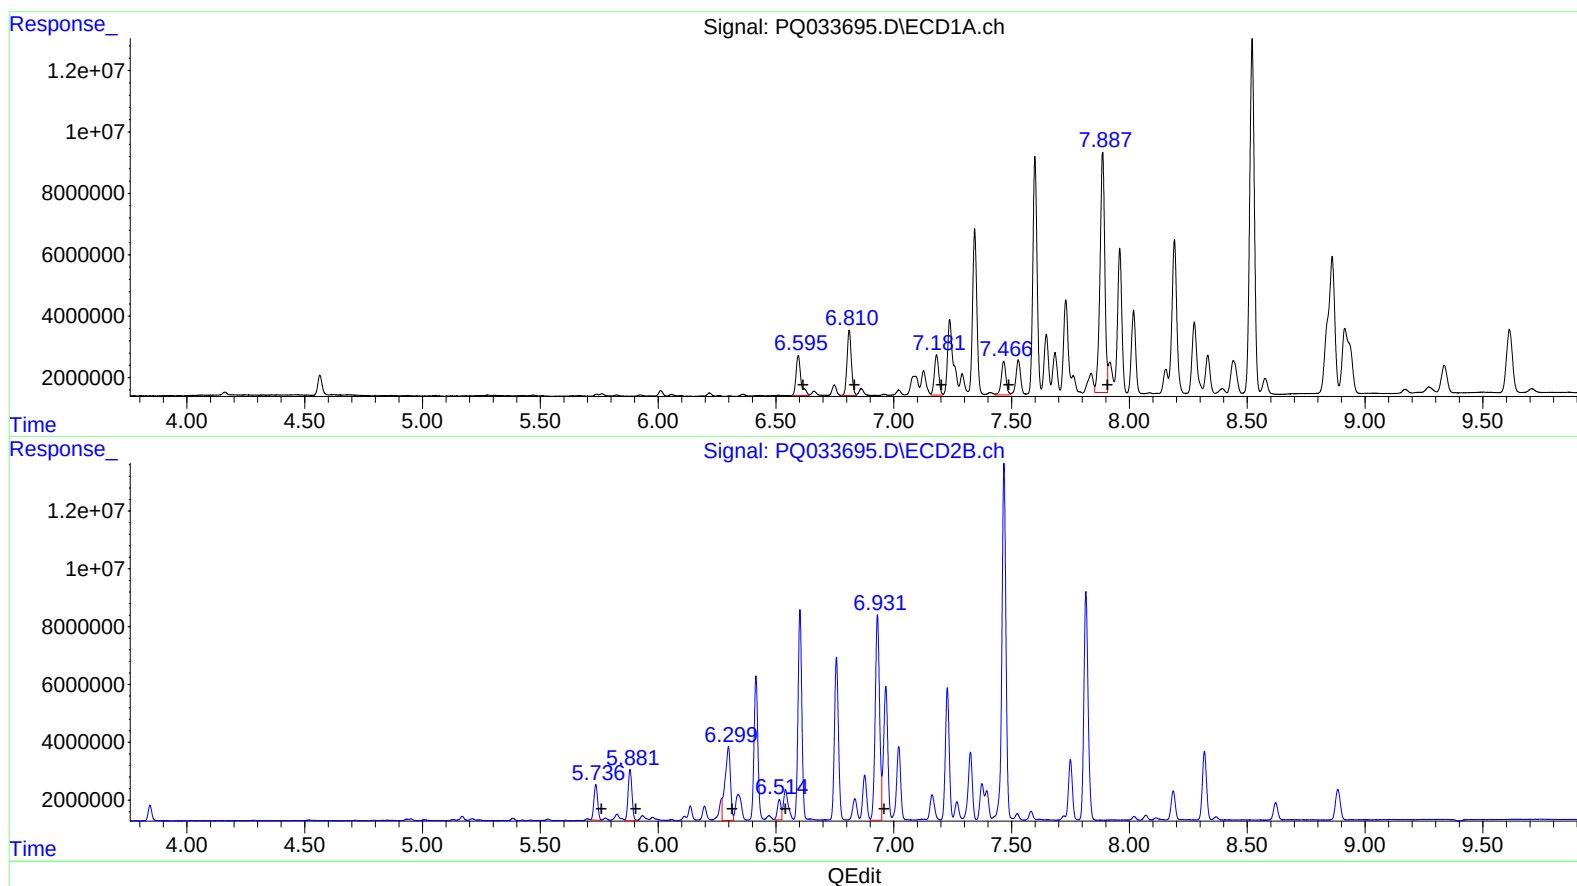

(26) AR-1254-1 (L6)
R.T. Response Conc
6.60 18958059 191.30
6.81 27255987 174.41
7.18 17211922 101.43
7.47 15239576 123.42
7.89 110499872 834.73

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
5.74 13618562 120.88
5.88 20281779 205.40
6.30 41016829 246.81
6.51 7581098 71.25
6.93 91544291 623.24

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102718\
Data File : PQ033695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2018 21:57
Operator : SM\SJ
Sample : J5673-07DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
C0BL1DL

Manual Integrations
APPROVED

sohil
10/30/2018 1:58:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:17:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ100918CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 10 08:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

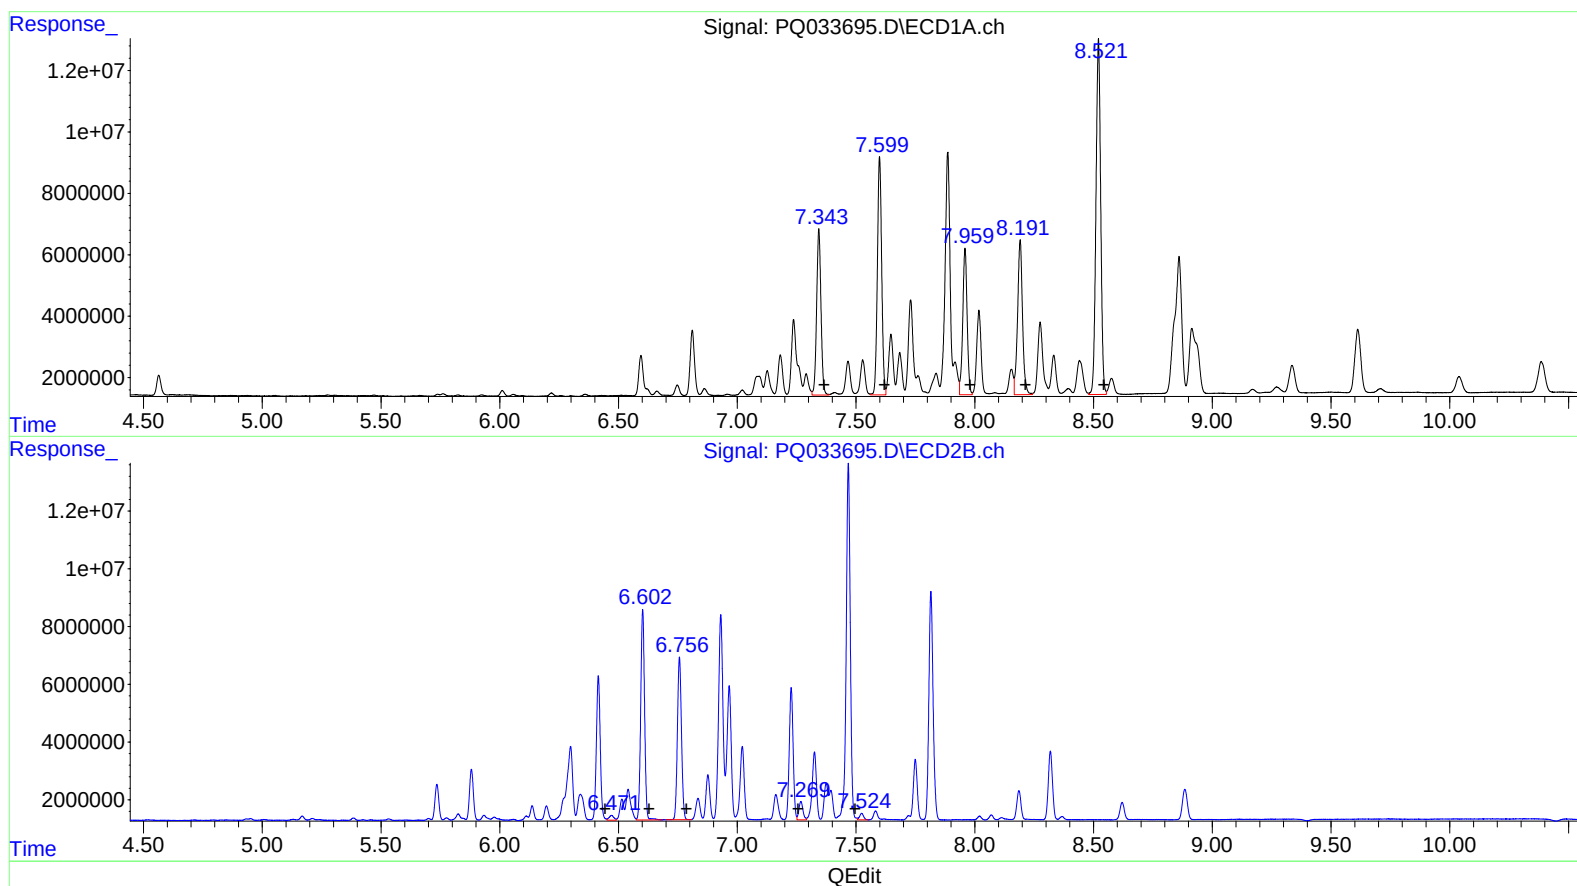

(31) AR-1260-1 (L7)
R.T. Response Conc
7.34 68560806 641.01
7.60 97060232 768.64
7.96 61352506 787.67
8.19 72897633 720.14
8.52 160496817 849.97

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.47 2276172 24.23
6.60 82693645 709.75
6.76 66387311 615.59
7.27 7535191 98.03
7.52 2677760 13.94

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102718\
Data File : PQ033695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2018 21:57
Operator : SM\SJ
Sample : J5673-07DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
C0BL1DL

Manual Integrations
APPROVED

sohil
10/30/2018 1:58:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:17:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ100918CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 10 08:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

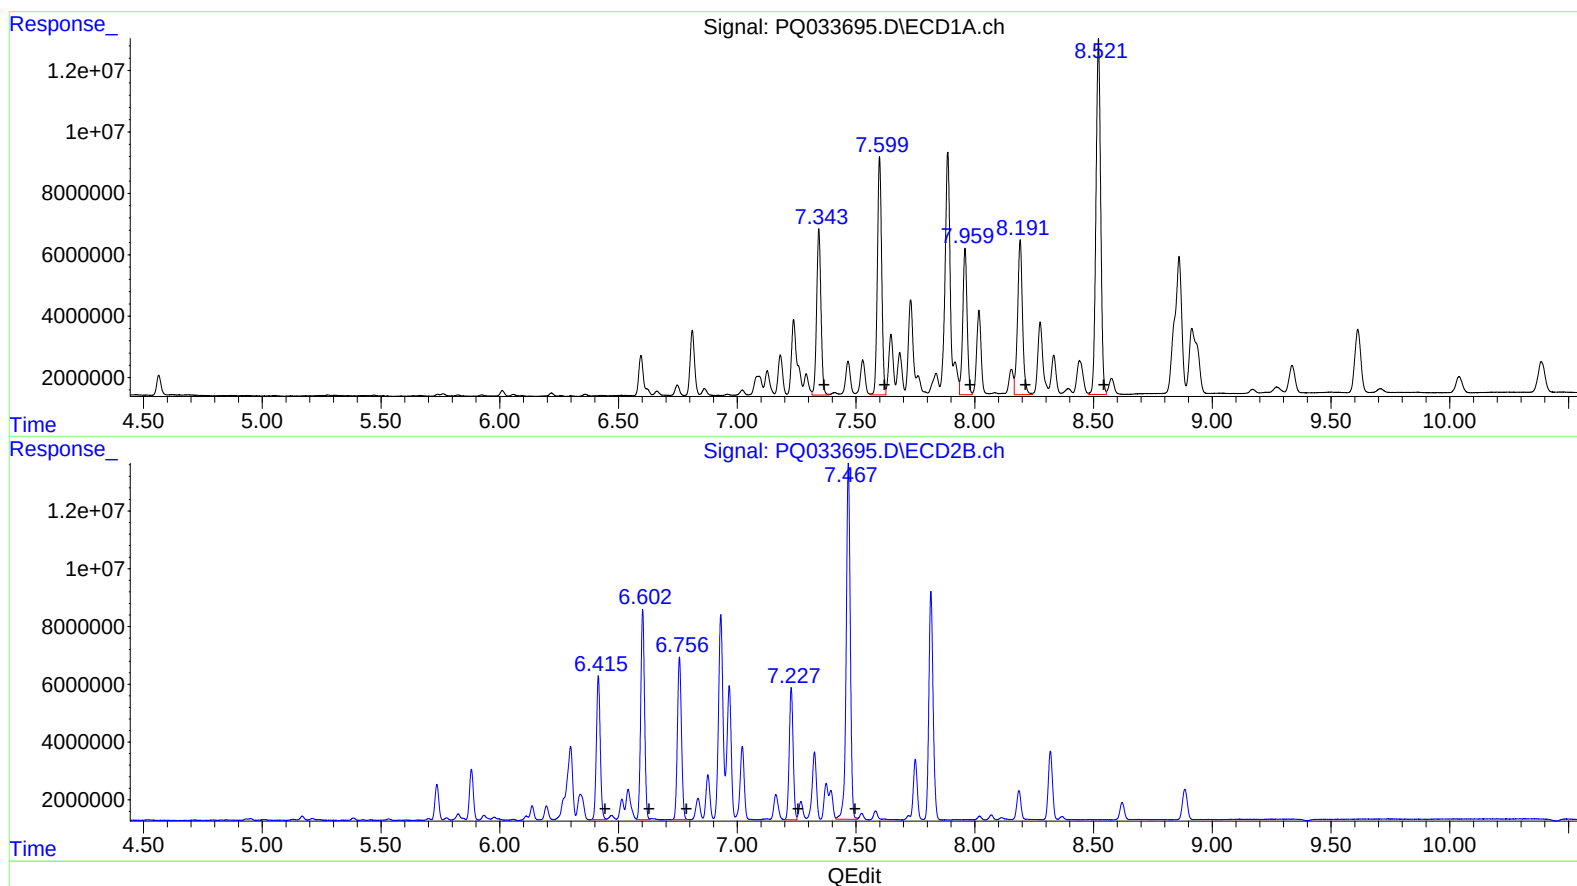

(31) AR-1260-1 (L7)
R.T. Response Conc
7.34 68560806 641.01
7.60 97060232 768.64
7.96 61352506 787.67
8.19 72897633 720.14
8.52 160496817 849.97

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.41 56543126 602.01
6.60 81502885 699.53
6.76 66341889 615.17
7.23 52227341 679.43
7.47 146844708 764.35

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ102718\
 Data File : PQ033695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2018 21:57
 Operator : SM\SJ
 Sample : J5673-07DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_Q
 Client Sampled :
 C0BL1DL

Manual Integrations
 APPROVED

sohil
 10/30/2018 1:58:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 04:17:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ100918CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 10 08:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.564	3.843	8131448	5836354	3.964	3.752
2) SA Decachlor...	10.385	8.885	20031094	15061280	10.597	9.369
Target Compounds						
26) L6 AR-1254-1	6.595	5.736	18958059	13618562	191.298	120.881m#)
27) L6 AR-1254-2	6.811	5.881	27255987	20281779	174.406	205.395
28) L6 AR-1254-3	7.181	6.299	17211922	41016829	101.435	246.806m#)
29) L6 AR-1254-4	7.466	6.514	15239576	7581098	123.423	71.253m#)
30) L6 AR-1254-5	7.887	6.931	110.5E6	91544291	834.725m)	623.237m#)
31) L7 AR-1260-1	7.343	6.415	68560806	56543126	641.014	602.008m)
32) L7 AR-1260-2	7.599	6.602	97060232	81502885	768.639	699.533m)
33) L7 AR-1260-3	7.959	6.756	61352506	66341889	787.665	615.173m)
34) L7 AR-1260-4	8.191	7.227	72897633	52227341	720.138	679.430m)
35) L7 AR-1260-5	8.521	7.467	160.5E6	146.8E6	849.965	764.347m)

5510/30/18

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.