

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ121819\
 Data File : PQ045885.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2019 22:19
 Operator : SM\AJ
 Sample : K6359-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 CH-WALLS

Manual Integrations
 APPROVED

Ankita
 12/19/2019 10:46:23 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 01:08:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ121719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 18 07:45:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.235	4.360	136.1E6	95070604	22.415	18.683
2)	SA Decachlor...	11.403	9.804	228.7E6	150.3E6	19.269	18.852
Target Compounds							
31)	L7 AR-1260-1	8.242	7.249	19845788	19052741	48.276	52.112
32)	L7 AR-1260-2	8.508	7.444	140.6E6	24439031	257.722m	54.101 #
33)	L7 AR-1260-3	8.875	7.605	21854338	17826706	45.050	41.856
34)	L7 AR-1260-4	9.112	8.093	39093758	12261581	80.742	32.157 #
35)	L7 AR-1260-5	9.458	8.337	44079444	39335310	38.594	41.690

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ121819\
Data File : PQ045885.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2019 22:19
Operator : SM\AJ
Sample : K6359-02
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampled :
CH-WALLS


Manual Integrations
APPROVED

Ankita
12/19/2019 10:46:23 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 01:08:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ121719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 18 07:45:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

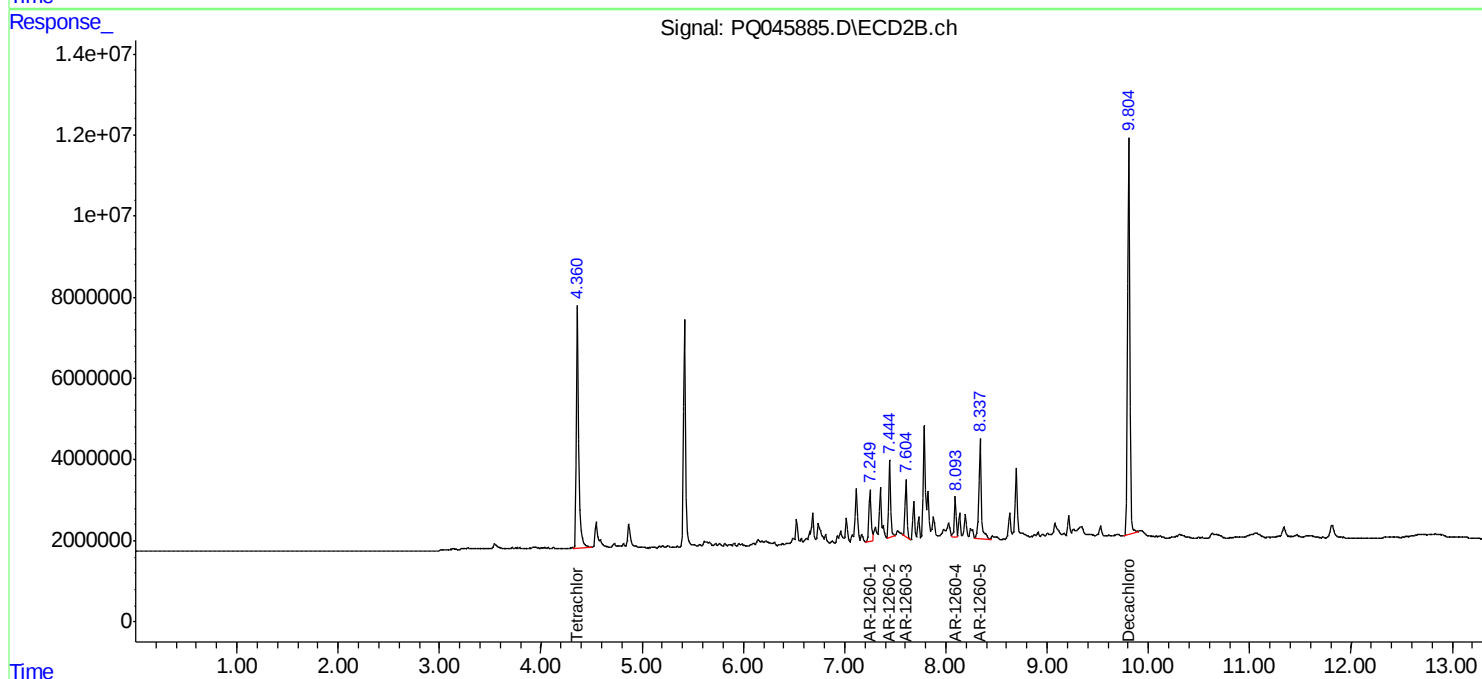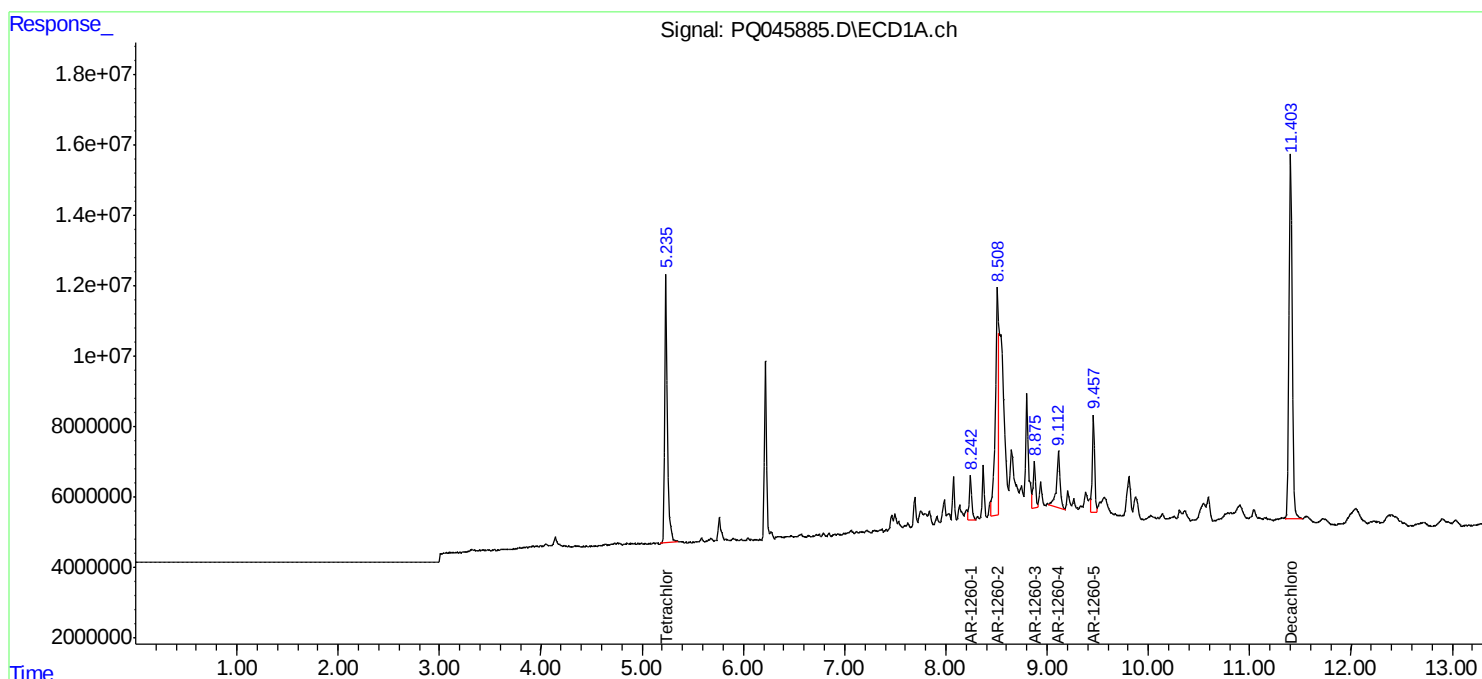

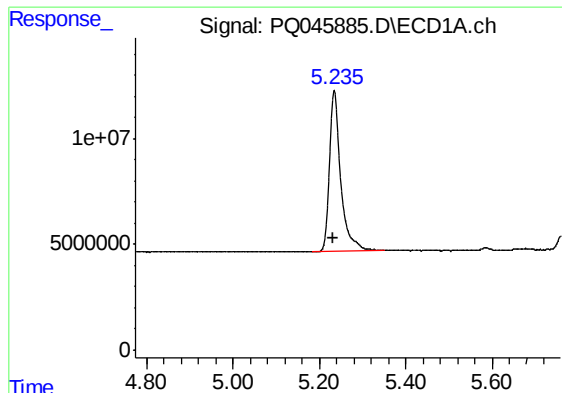


#1 Tetrachloro-m-xylene

R.T.: 5.235 min
Delta R.T.: 0.002 min
Response: 136071804
Conc: 22.41 ng/ml

Instrument :
ECD_Q
ClientSampleId :
CH-WALLS


Manual Integrations
APPROVED

Ankita
12/19/2019 10:46:23 AM

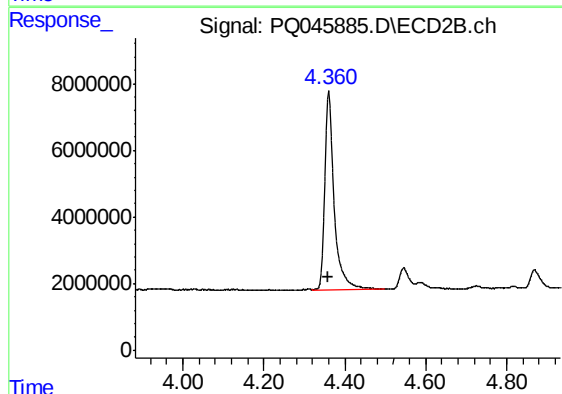


#1 Tetrachloro-m-xylene

R.T.: 4.360 min
Delta R.T.: 0.001 min
Response: 95070604
Conc: 18.68 ng/ml

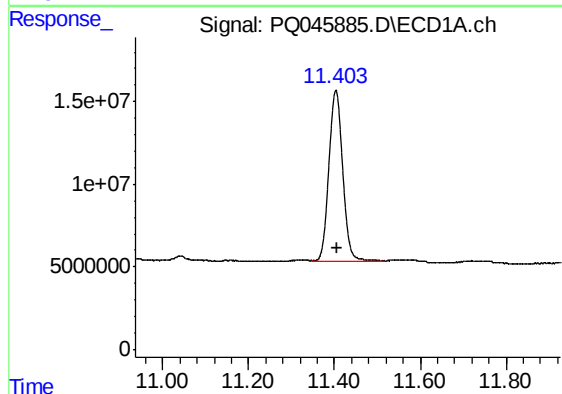


#2 Decachlorobiphenyl

R.T.: 11.403 min
Delta R.T.: -0.003 min
Response: 228749655
Conc: 19.27 ng/ml

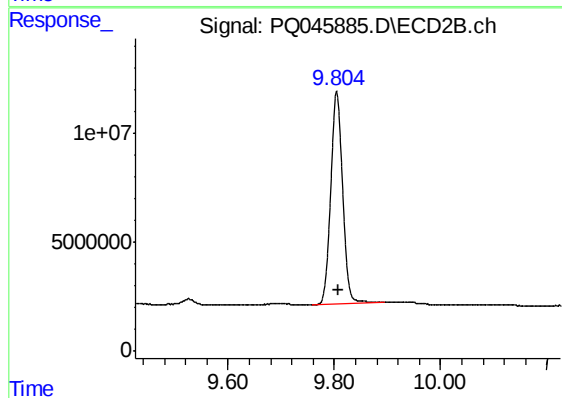

#2 Decachlorobiphenyl

R.T.: 9.804 min
Delta R.T.: -0.002 min
Response: 150301431
Conc: 18.85 ng/ml

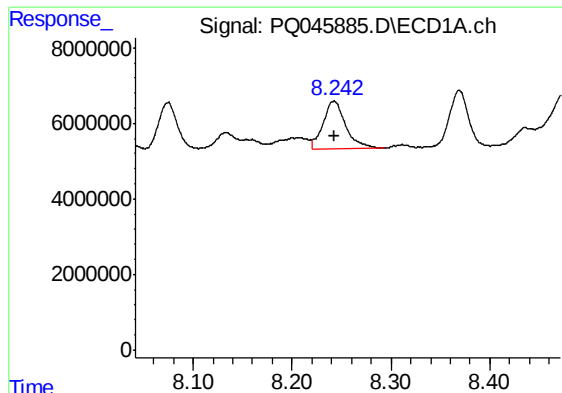


#31 AR-1260-1

R.T.: 8.242 min
Delta R.T.: 0.000 min
Response: 19845788
Conc: 48.28 ng/ml

Instrument :
ECD_Q
ClientSampleId :
CH-WALLS


Manual Integrations
APPROVED

Ankita
12/19/2019 10:46:23 AM

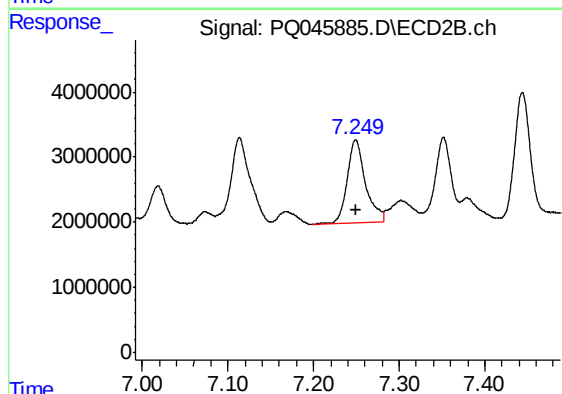


#31 AR-1260-1

R.T.: 7.249 min
Delta R.T.: 0.000 min
Response: 19052741
Conc: 52.11 ng/ml

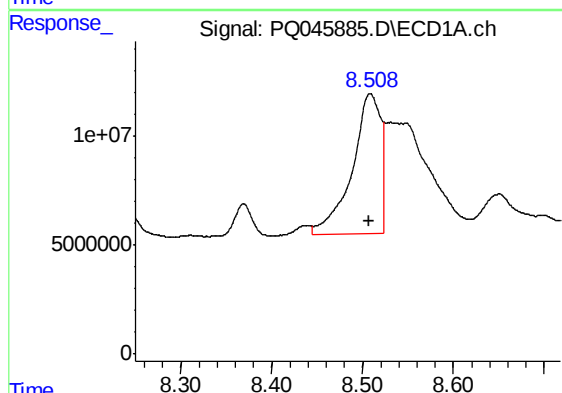


#32 AR-1260-2

R.T.: 8.508 min
Delta R.T.: 0.000 min
Response: 140592975
Conc: 257.72 ng/ml m

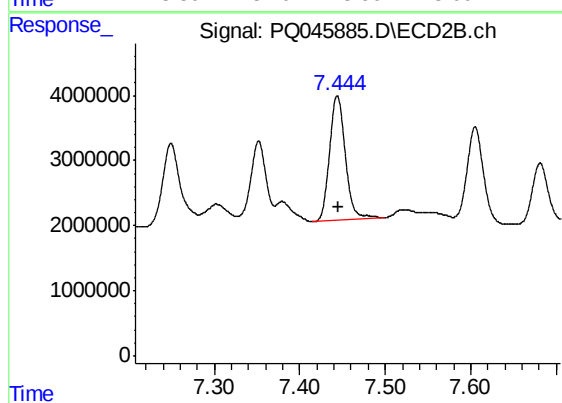

#32 AR-1260-2

R.T.: 7.444 min
Delta R.T.: 0.000 min
Response: 24439031
Conc: 54.10 ng/ml

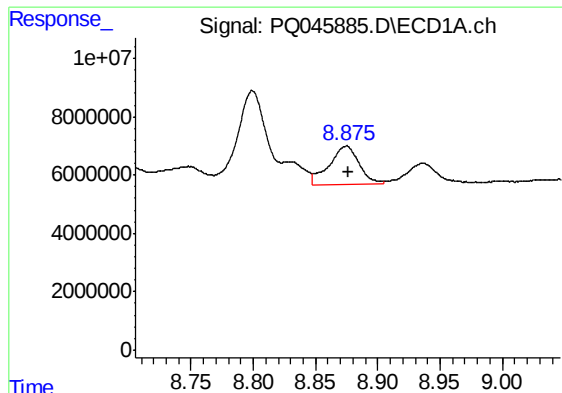


#33 AR-1260-3

R.T.: 8.875 min
Delta R.T.: -0.001 min
Response: 21854338
Conc: 45.05 ng/ml

Instrument :
ECD_Q
ClientSampleId :
CH-WALLS


Manual Integrations
APPROVED

Ankita
12/19/2019 10:46:23 AM

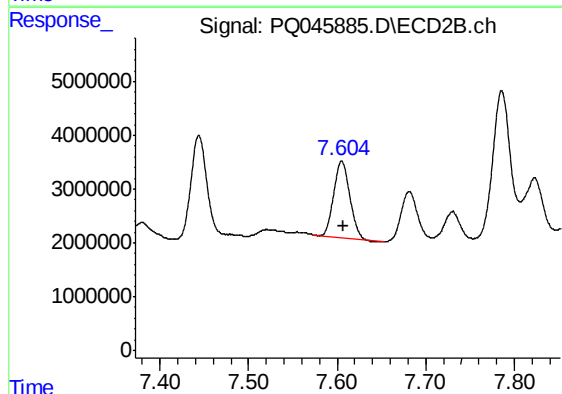


#33 AR-1260-3

R.T.: 7.605 min
Delta R.T.: -0.002 min
Response: 17826706
Conc: 41.86 ng/ml

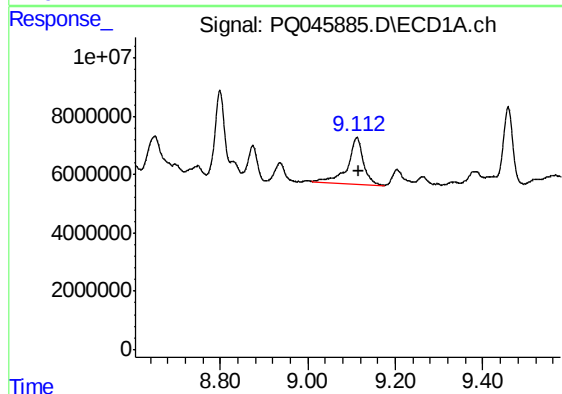


#34 AR-1260-4

R.T.: 9.112 min
Delta R.T.: -0.003 min
Response: 39093758
Conc: 80.74 ng/ml

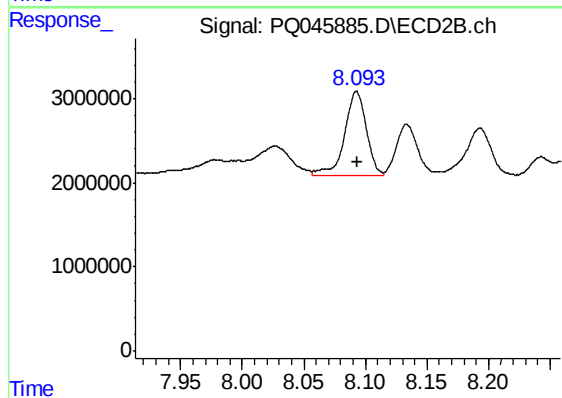

#34 AR-1260-4

R.T.: 8.093 min
Delta R.T.: -0.001 min
Response: 12261581
Conc: 32.16 ng/ml

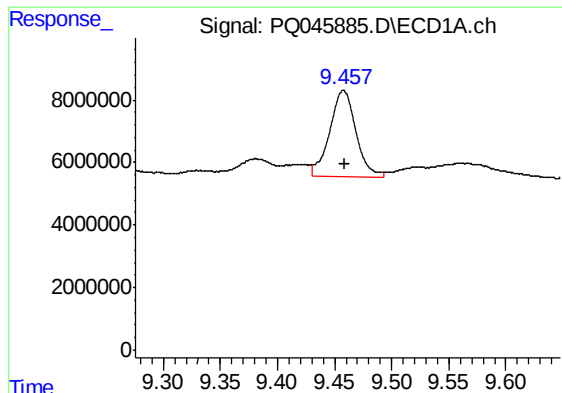


#35 AR-1260-5

R.T.: 9.458 min
Delta R.T.: 0.000 min
Response: 44079444
Conc: 38.59 ng/ml

Instrument :
ECD_Q
ClientSampleId :
CH-WALLS

Manual Integrations
APPROVED

Ankita
12/19/2019 10:46:23 AM

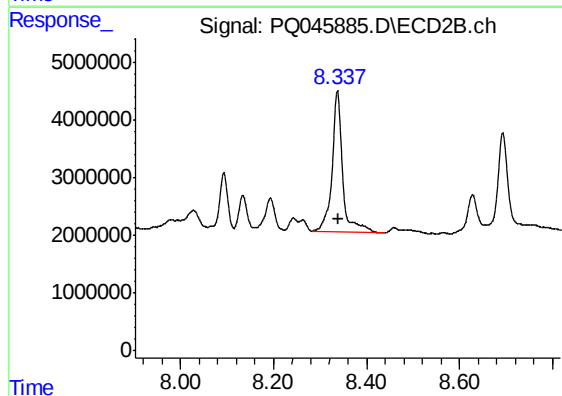

#35 AR-1260-5

R.T.: 8.337 min
Delta R.T.: -0.002 min
Response: 39335310
Conc: 41.69 ng/ml