

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR010623\
Data File : PR058847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2023 18:01
Operator : YP\AJ
Sample : AR1660CCC400
Misc :
ALS Vial : 3 Sample Multiplier: 1



Instrument :
ECD_R
LabSampleId :
AR1660CCC400

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 01/09/2023
Supervised By :Ankita Jodhani 01/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 21:34:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR121422CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 15 03:47:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

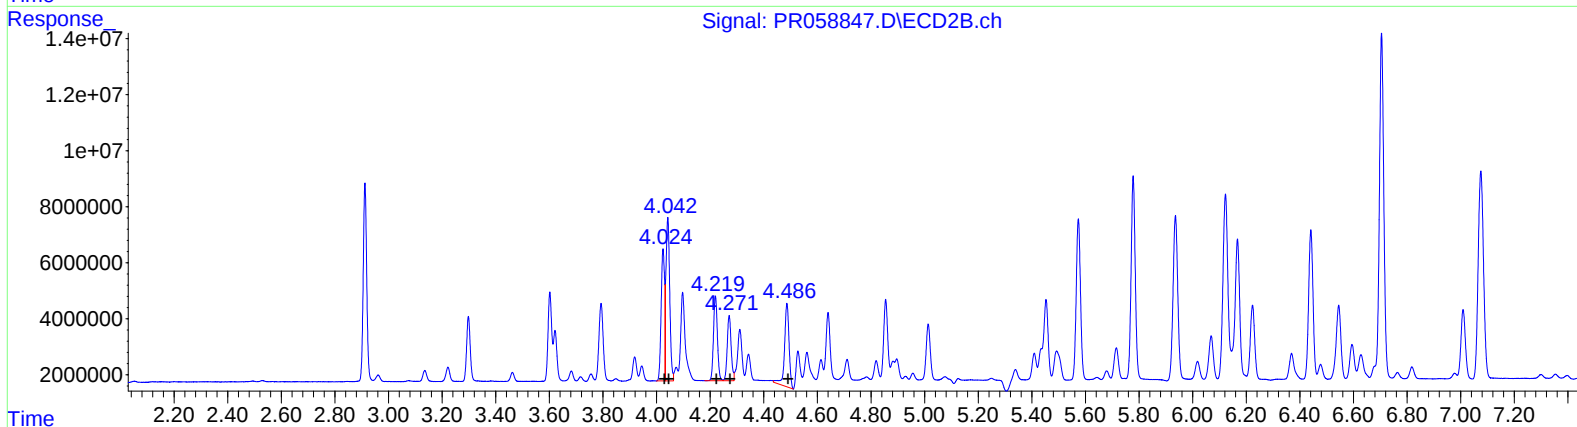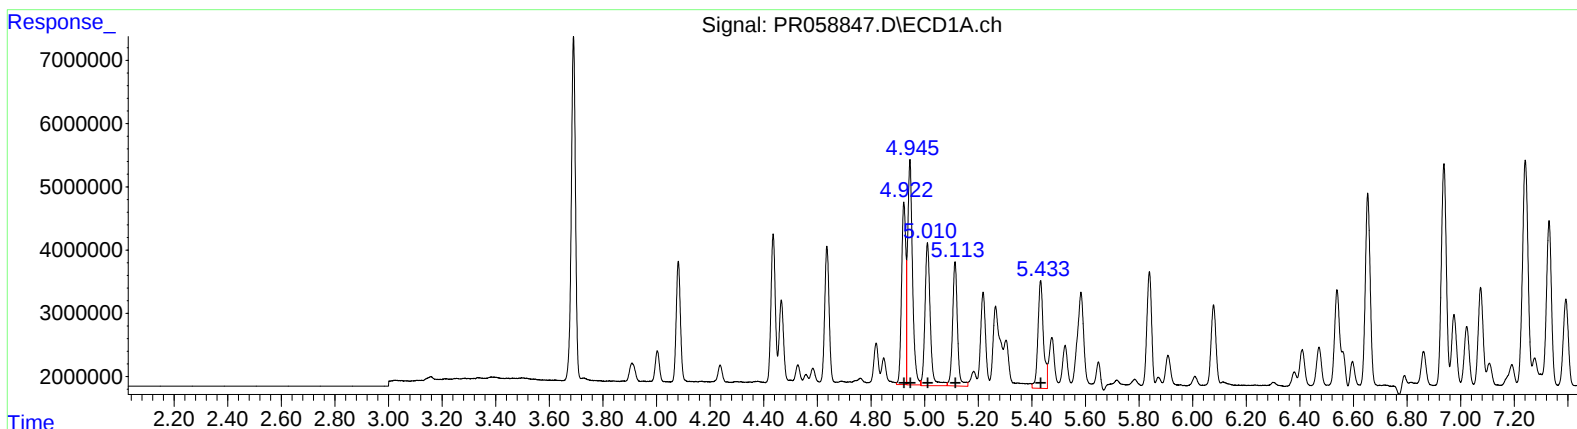

QEdit

(3) AR-1016-1 (L1)

R.T.	Response	Conc
4.92	31986198	380.51
4.95	44556648	389.44
5.01	30589442	411.23
5.11	24750051	409.83
5.43	24234064	414.99

(3) AR-1016-1 #2 (L1)

R.T.	Response	Conc
4.02	41694318	379.21
4.04	57708478	381.04
4.22	30606522	377.11
4.27	23624854	378.02
4.49	34823241	412.35

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR010623\
Data File : PR058847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2023 18:01
Operator : YP\AJ
Sample : AR1660CCC400
Misc :
ALS Vial : 3 Sample Multiplier: 1



Instrument :
ECD_R
LabSampleId :
AR1660CCC400

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 01/09/2023
Supervised By :Ankita Jodhani 01/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 21:34:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR121422CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 15 03:47:13 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

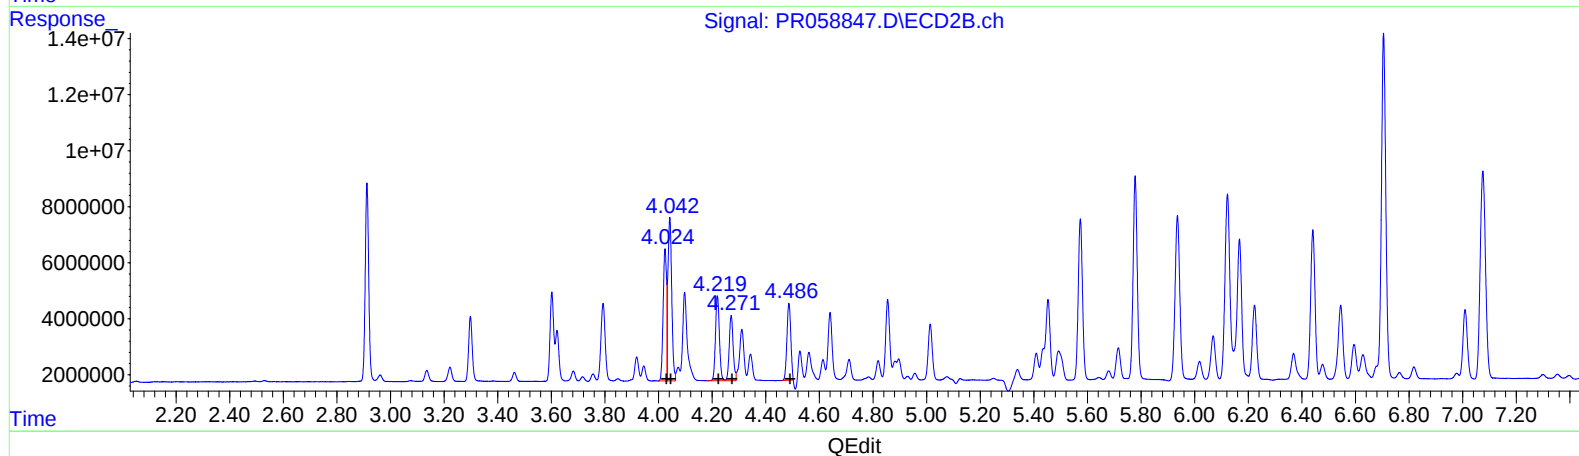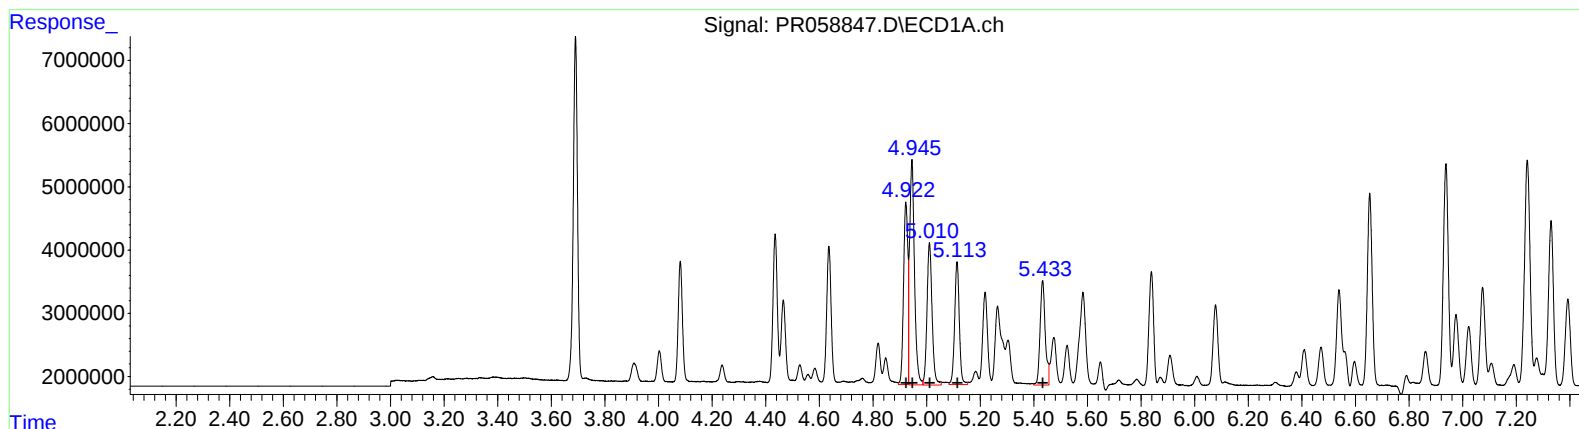

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
4.92 31986198 380.51
4.95 44556648 389.44
5.01 29576413 397.62
5.11 23565411 390.22
5.43 22134311 379.04

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
4.02 41694318 379.21
4.04 57708478 381.04
4.22 30606522 377.11
4.27 23624854 378.02
4.49 27299629 323.26

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR010623\
 Data File : PR058847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2023 18:01
 Operator : YP\AJ
 Sample : AR1660CCC400
 Misc :
 ALS Vial : 3 Sample Multiplier: 1


Instrument :
 ECD_R
 LabSampleId :
 AR1660CCC400

Manual IntegrationsAPPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 21:34:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR121422CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 15 03:47:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Reviewed By :Yogesh Patel 01/09/2023
 Supervised By :Ankita Jodhani 01/09/2023

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

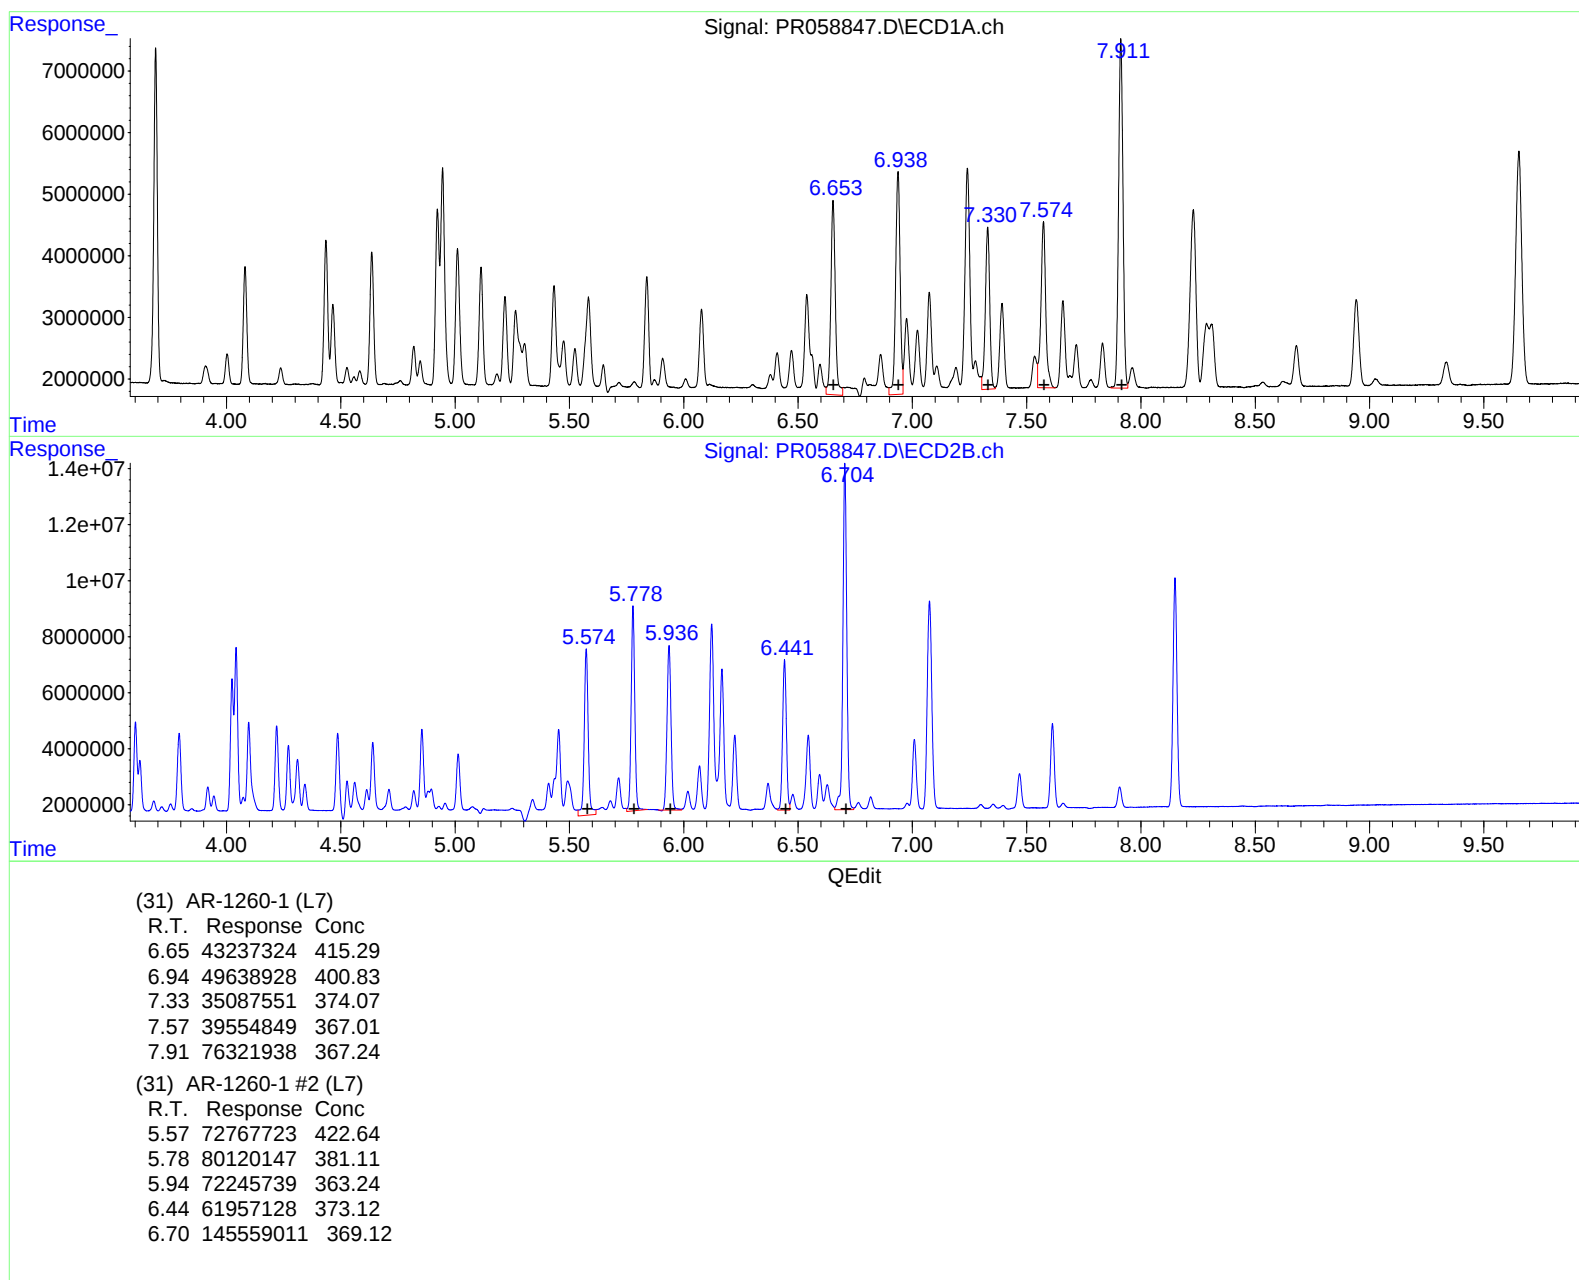

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR010623\
 Data File : PR058847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2023 18:01
 Operator : YP\AJ
 Sample : AR1660CCC400
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_R
 LabSampleId :
 AR1660CCC400

Manual IntegrationsAPPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 21:34:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR121422CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 15 03:47:13 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Reviewed By :Yogesh Patel 01/09/2023
 Supervised By :Ankita Jodhani 01/09/2023

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

