

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR010924\
 Data File : PR064877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jan 2024 14:15
 Operator : AJ\MA
 Sample : P1041-13
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PCB-GPC-BLANK-SPIKE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 21:47:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR121423CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 15 04:19:57 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.971f	0	339783	N.D.	0.063 #
2)	SA Decachlor...	0.000	8.315f	0	535107	N.D.	0.204 #
Target Compounds							
3)	L1 AR-1016-1	4.919	4.150	1002522	208861	5.538	1.126 #
4)	L1 AR-1016-2	4.919f	4.174	1002522	121579	3.779	0.479 #
5)	L1 AR-1016-3	0.000	4.349	0	186660	N.D.	1.353 #
6)	L1 AR-1016-4	0.000	4.414	0	58343	N.D.	0.548 #
7)	L1 AR-1016-5	0.000	4.624	0	94067	N.D.	0.671 #
8)	L2 AR-1221-1	3.952	3.257	513760	58562	7.499	0.967 #
9)	L2 AR-1221-2	3.952f	3.322	513760	22917	11.029	0.543 #
10)	L2 AR-1221-3	4.090	3.402	741895	506863	4.822	3.539 #
11)	L3 AR-1232-1	4.090	3.402	741895	506863	6.207	4.602 #
12)	L3 AR-1232-2	4.601f	4.174	404978	121579	6.075	1.136 #
13)	L3 AR-1232-3	4.919f	4.349	1002522	186660	8.749	3.295 #
14)	L3 AR-1232-4	0.000	4.433	0	47806	N.D.	0.964 #
15)	L3 AR-1232-5	0.000	4.624	0	94067	N.D.	1.738 #
16)	L4 AR-1242-1	4.919	4.150	1002522	208861	6.929	1.424 #
17)	L4 AR-1242-2	4.919f	4.174	1002522	121579	4.802	0.611 #
18)	L4 AR-1242-3	0.000	4.349	0	186660	N.D.	1.726 #
19)	L4 AR-1242-4	0.000	4.433	0	47806	N.D.	0.460 #
20)	L4 AR-1242-5	5.898	5.013	866226	98509	7.568	0.733 #
21)	L5 AR-1248-1	4.919	4.150	1002522	208861	9.159	1.881 #
22)	L5 AR-1248-2	0.000	4.414	0	58343	N.D.	0.388 #
23)	L5 AR-1248-3	0.000	4.433	0	47806	N.D.	0.304 #
24)	L5 AR-1248-4	5.898	4.624	866226	94067	4.429	0.496 #
25)	L5 AR-1248-5	5.898	5.049	866226	300200	4.431	1.554 #
26)	L6 AR-1254-1	5.898f	5.013	866226	98509	4.307	0.343 #
27)	L6 AR-1254-2	0.000	5.192	0	82536	N.D.	0.331 #
28)	L6 AR-1254-3	6.516	5.596	449554	1171960	1.444	2.945 #
29)	L6 AR-1254-4	0.000	5.852	0	264182	N.D.	1.058 #
30)	L6 AR-1254-5	0.000	6.306	0	65958	N.D.	0.185 #
31)	L7 AR-1260-1	0.000	5.745	0	207489	N.D.	0.718 #
32)	L7 AR-1260-2	0.000	5.969	0	166688	N.D.	0.480 #
33)	L7 AR-1260-3	0.000	6.126	0	1248030	N.D.	3.792 #
34)	L7 AR-1260-4	7.645f	6.638	332011	73423	1.444	0.272 #
35)	L7 AR-1260-5	0.000	6.918	0	641840	N.D.	1.027 #
36)	L8 AR-1262-1	0.000	6.380	0	182490	N.D.	0.500 #
37)	L8 AR-1262-2	0.000	6.918	0	641840	N.D.	0.973 #
38)	L8 AR-1262-3	0.000	7.178	0	281494	N.D.	1.123 #
39)	L8 AR-1262-4	0.000	7.303	0	658838	N.D.	1.380 #
40)	L8 AR-1262-5	9.041f	7.830	361692	41978	2.226	0.198 #
41)	L9 AR-1268-1	0.000	7.178	0	281494	N.D.	0.360 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR010924\
Data File : PR064877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jan 2024 14:15
Operator : AJ\MA
Sample : P1041-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 21:47:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR121423CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 15 04:19:57 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	0.000	7.303	0	658838	N.D.	0.918 #
43)	L9 AR-1268-3	0.000	7.543f	0	307556	N.D.	0.514 #
44)	L9 AR-1268-4	9.041f	7.830	361692	41978	1.946	0.168 #
45)	L9 AR-1268-5	0.000	8.129	0	69353	N.D.	0.039 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR010924\
Data File : PR064877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jan 2024 14:15
Operator : AJ\MA
Sample : P1041-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 21:47:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR121423CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 15 04:19:57 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

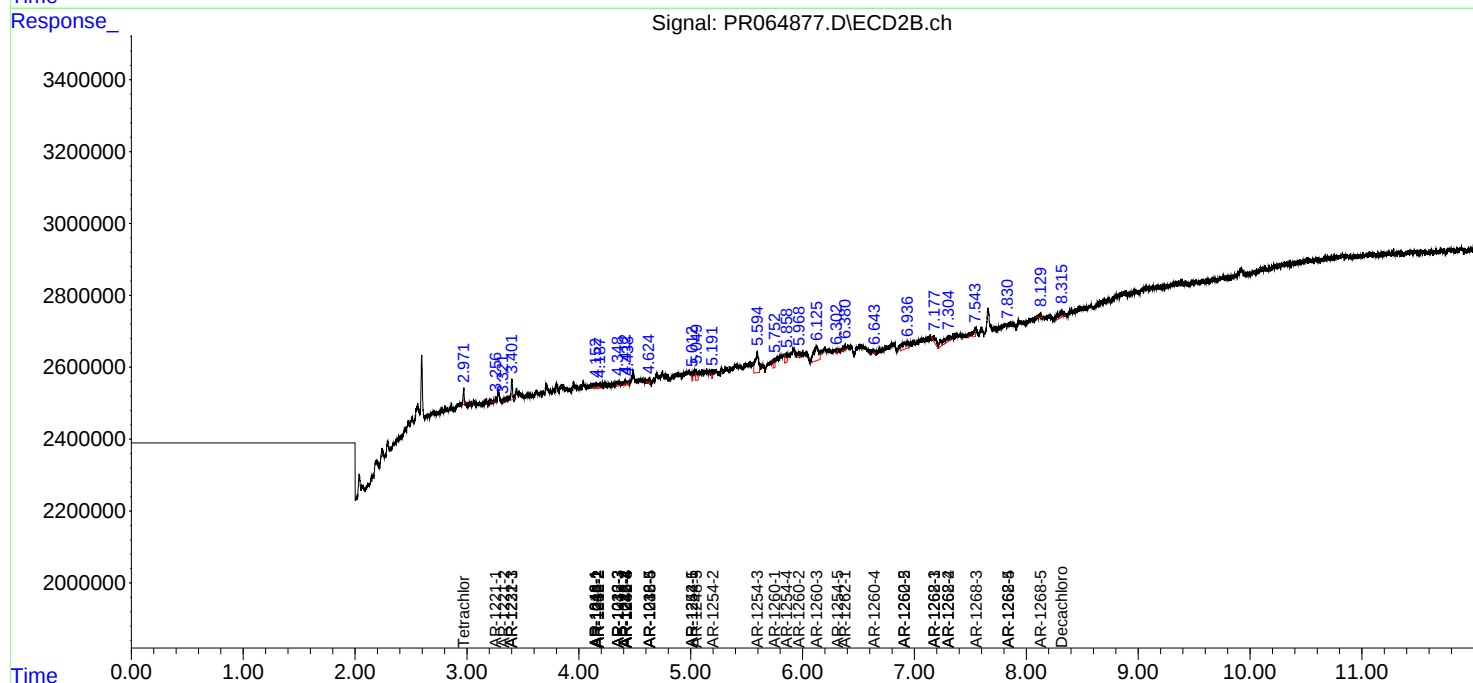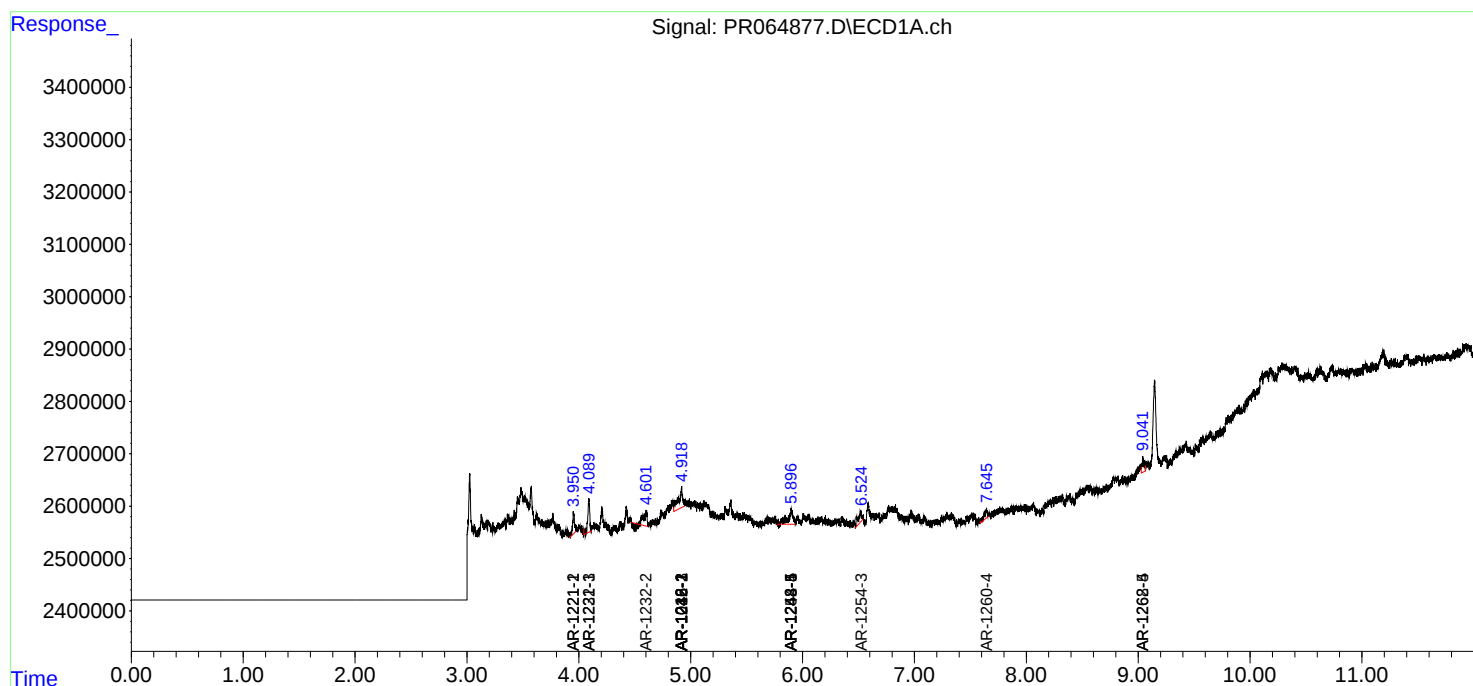


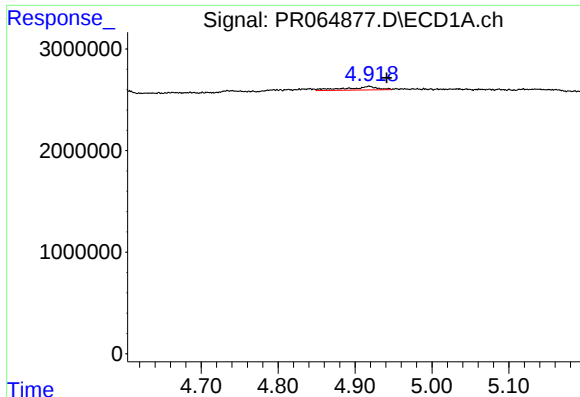

#3 AR-1016-1


R.T.: 4.919 min
Delta R.T.: -0.023 min
Response: 1002522
Conc: 5.54 ng/ml

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

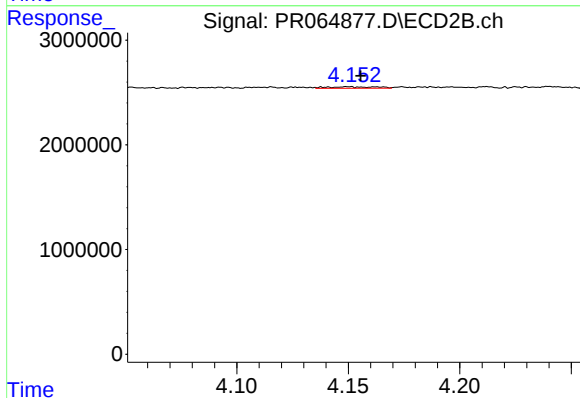


#3 AR-1016-1

R.T.: 4.150 min
Delta R.T.: -0.006 min
Response: 208861
Conc: 1.13 ng/ml

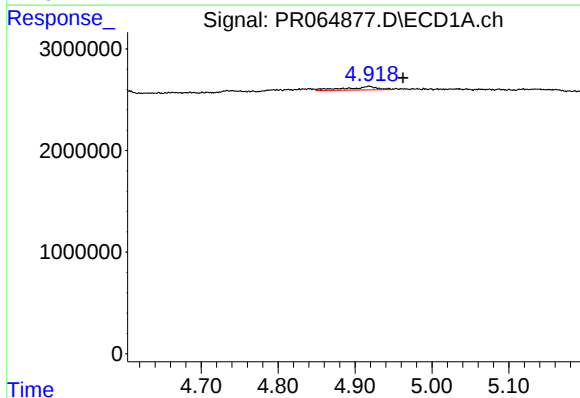


#4 AR-1016-2

R.T.: 4.919 min
Delta R.T.: -0.044 min
Response: 1002522
Conc: 3.78 ng/ml

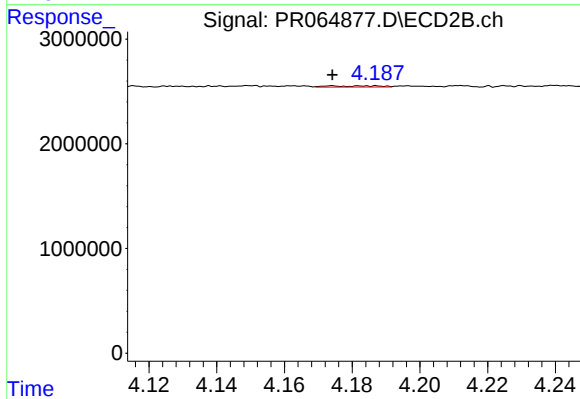

#4 AR-1016-2


R.T.: 4.174 min
Delta R.T.: 0.000 min
Response: 121579
Conc: 0.48 ng/ml

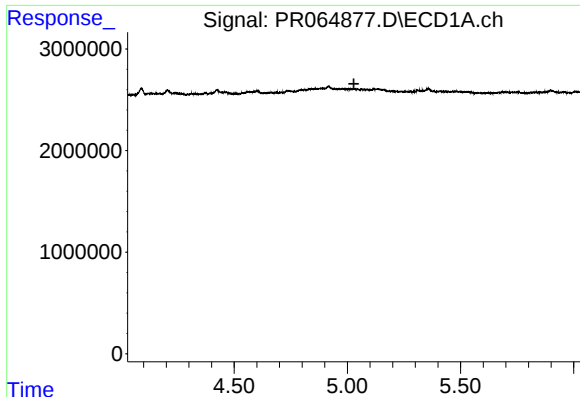

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

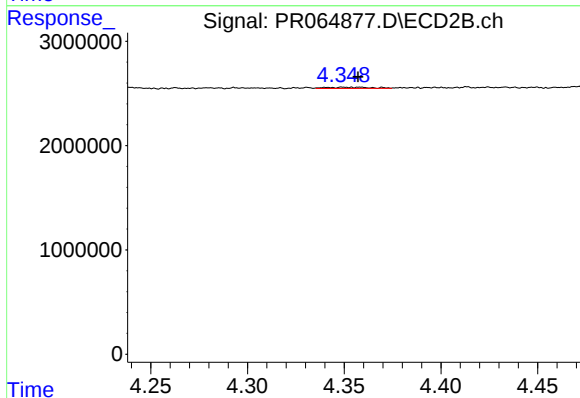


#5 AR-1016-3

R.T.: 4.349 min
Delta R.T.: -0.008 min
Response: 186660
Conc: 1.35 ng/ml

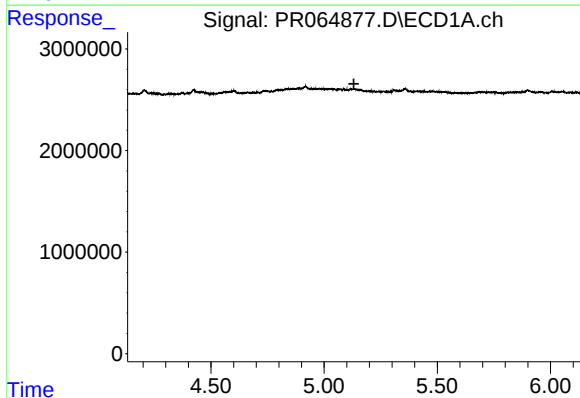


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.131 min
Response: 0
Conc: N.D.

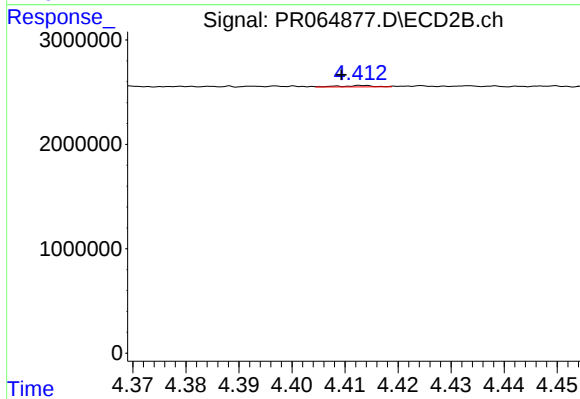

#6 AR-1016-4


R.T.: 4.414 min
Delta R.T.: 0.004 min
Response: 58343
Conc: 0.55 ng/ml

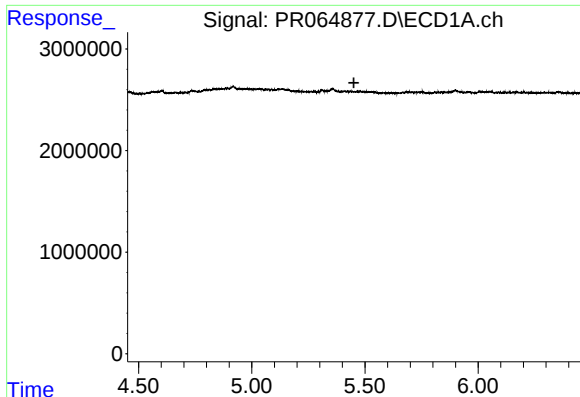

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

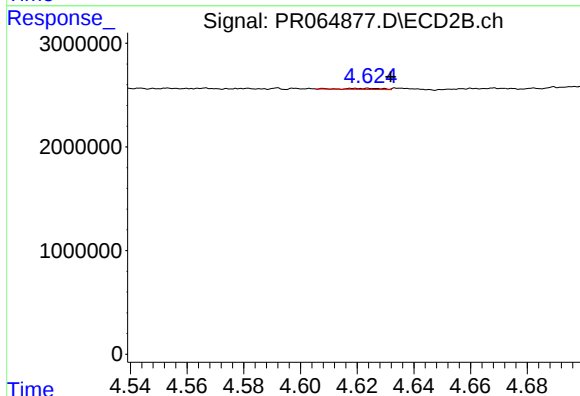


#7 AR-1016-5

R.T.: 4.624 min
Delta R.T.: -0.008 min
Response: 94067
Conc: 0.67 ng/ml

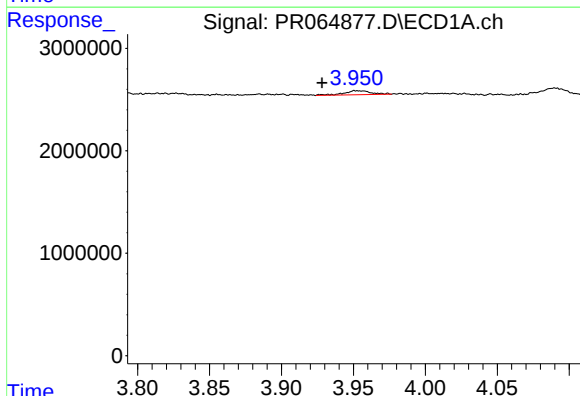


#8 AR-1221-1

R.T.: 3.952 min
Delta R.T.: 0.024 min
Response: 513760
Conc: 7.50 ng/ml

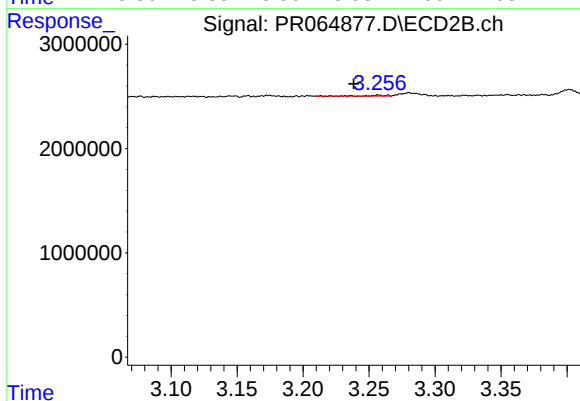

#8 AR-1221-1


R.T.: 3.257 min
Delta R.T.: 0.019 min
Response: 58562
Conc: 0.97 ng/ml

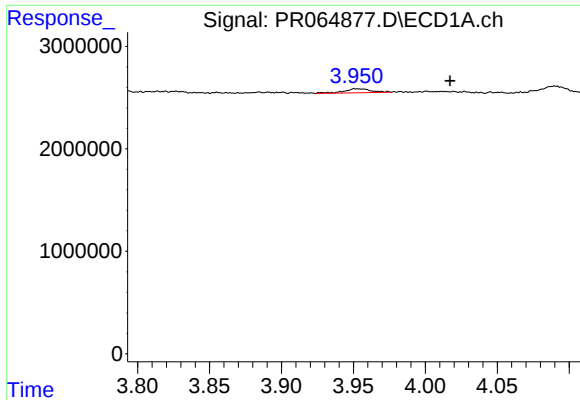

#9 AR-1221-2


R.T.: 3.952 min
Delta R.T.: -0.065 min
Response: 513760
Conc: 11.03 ng/ml

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

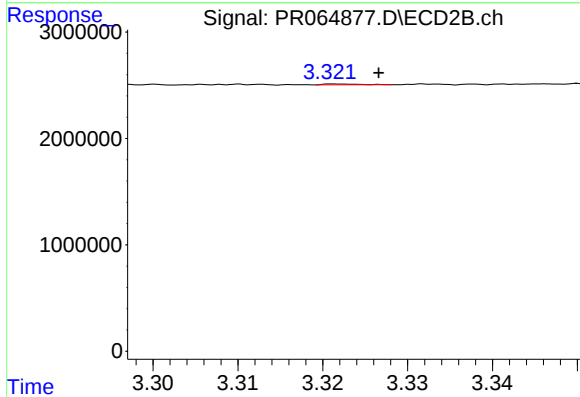


#9 AR-1221-2

R.T.: 3.322 min
Delta R.T.: -0.004 min
Response: 22917
Conc: 0.54 ng/ml

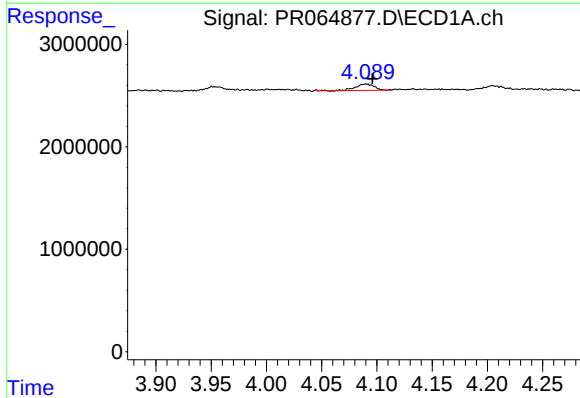


#10 AR-1221-3

R.T.: 4.090 min
Delta R.T.: -0.006 min
Response: 741895
Conc: 4.82 ng/ml

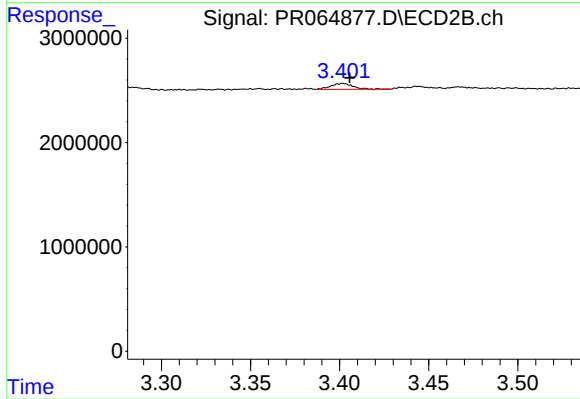

#10 AR-1221-3


R.T.: 3.402 min
Delta R.T.: -0.004 min
Response: 506863
Conc: 3.54 ng/ml

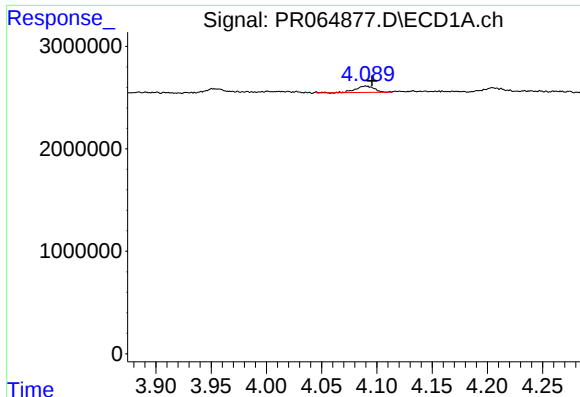

#11 AR-1232-1


R.T.: 4.090 min
Delta R.T.: -0.005 min
Response: 741895
Conc: 6.21 ng/ml

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

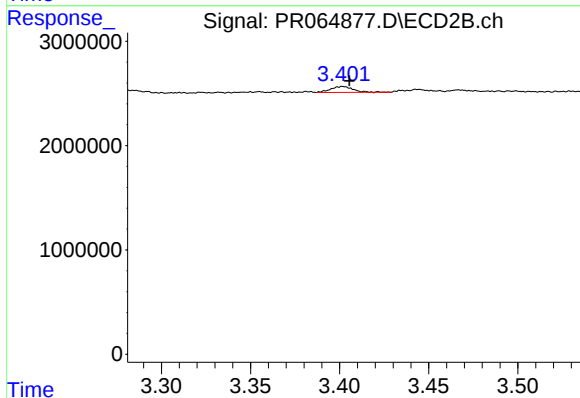


#11 AR-1232-1

R.T.: 3.402 min
Delta R.T.: -0.004 min
Response: 506863
Conc: 4.60 ng/ml

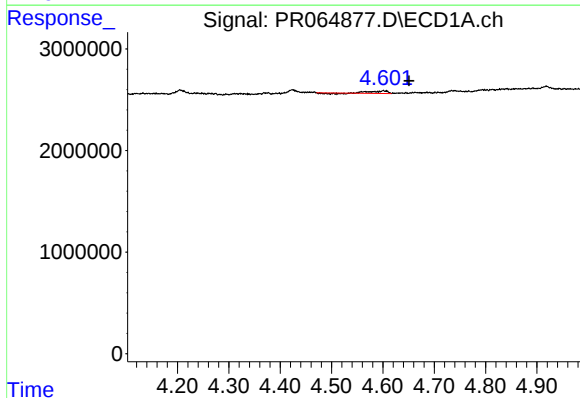


#12 AR-1232-2

R.T.: 4.601 min
Delta R.T.: -0.050 min
Response: 404978
Conc: 6.07 ng/ml

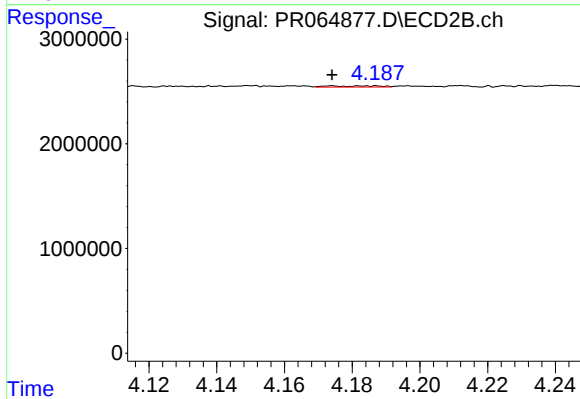

#12 AR-1232-2


R.T.: 4.174 min
Delta R.T.: 0.000 min
Response: 121579
Conc: 1.14 ng/ml

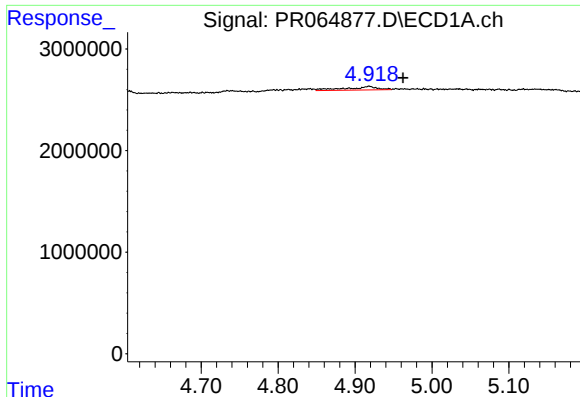

#13 AR-1232-3


R.T.: 4.919 min
Delta R.T.: -0.044 min
Response: 1002522
Conc: 8.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

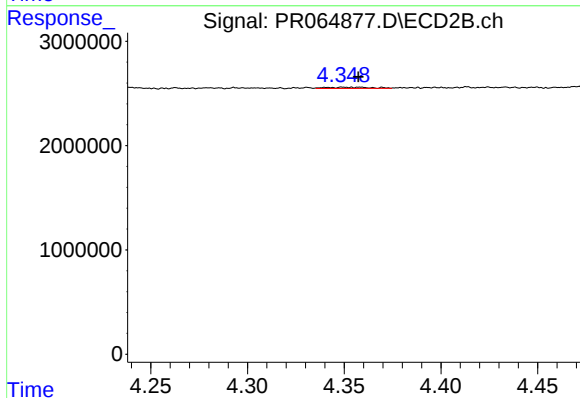


#13 AR-1232-3

R.T.: 4.349 min
Delta R.T.: -0.008 min
Response: 186660
Conc: 3.30 ng/ml

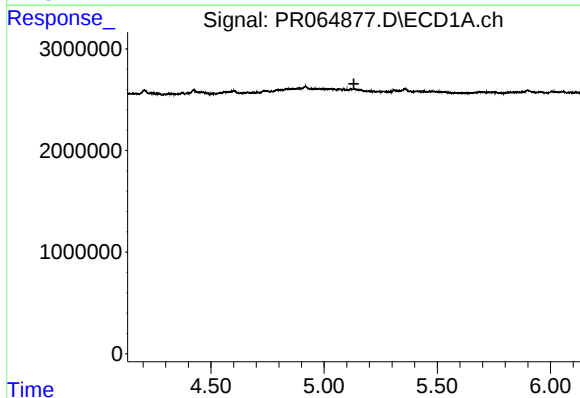


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.132 min
Response: 0
Conc: N.D.

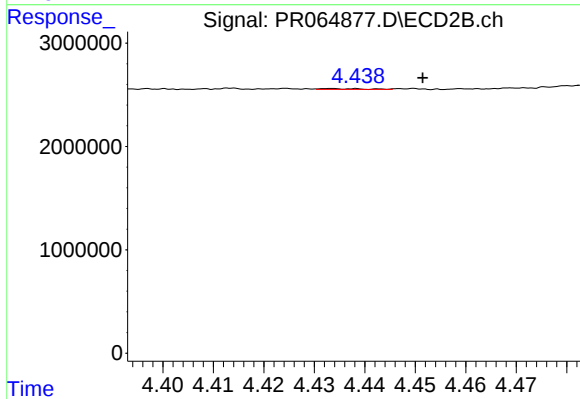

#14 AR-1232-4


R.T.: 4.433 min
Delta R.T.: -0.018 min
Response: 47806
Conc: 0.96 ng/ml

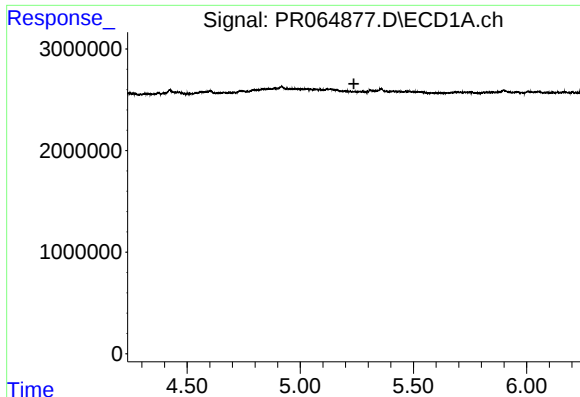

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.237 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

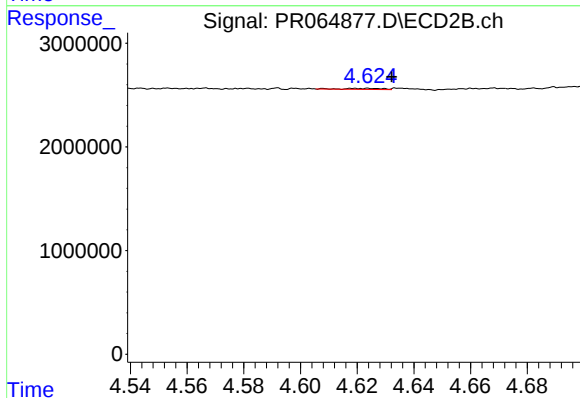


#15 AR-1232-5

R.T.: 4.624 min
Delta R.T.: -0.008 min
Response: 94067
Conc: 1.74 ng/ml

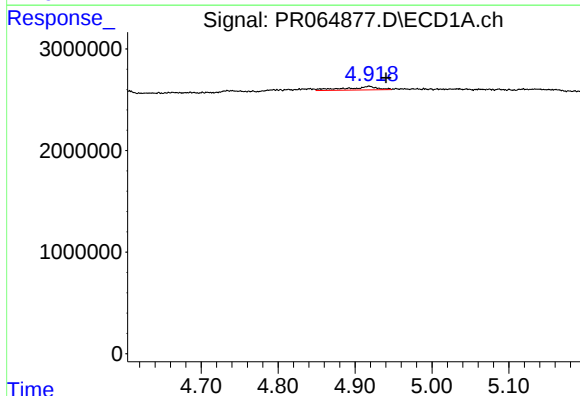


#16 AR-1242-1

R.T.: 4.919 min
Delta R.T.: -0.022 min
Response: 1002522
Conc: 6.93 ng/ml

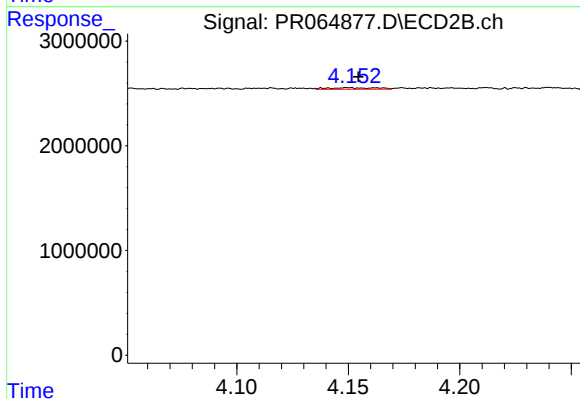

#16 AR-1242-1


R.T.: 4.150 min
Delta R.T.: -0.005 min
Response: 208861
Conc: 1.42 ng/ml

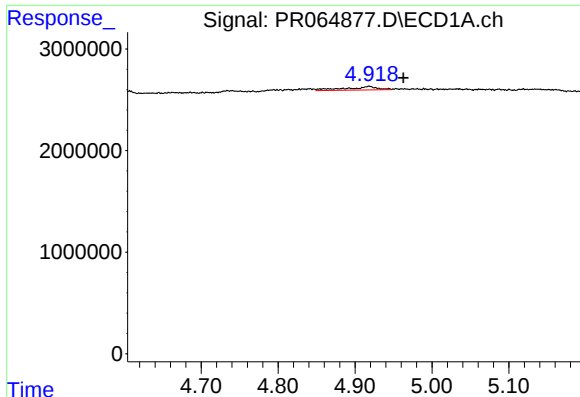

#17 AR-1242-2


R.T.: 4.919 min
Delta R.T.: -0.044 min
Response: 1002522
Conc: 4.80 ng/ml

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

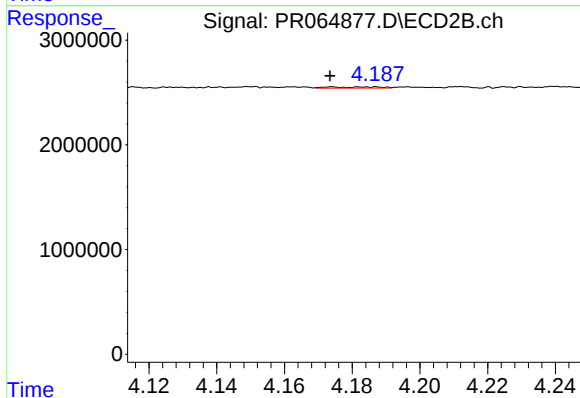


#17 AR-1242-2

R.T.: 4.174 min
Delta R.T.: 0.000 min
Response: 121579
Conc: 0.61 ng/ml

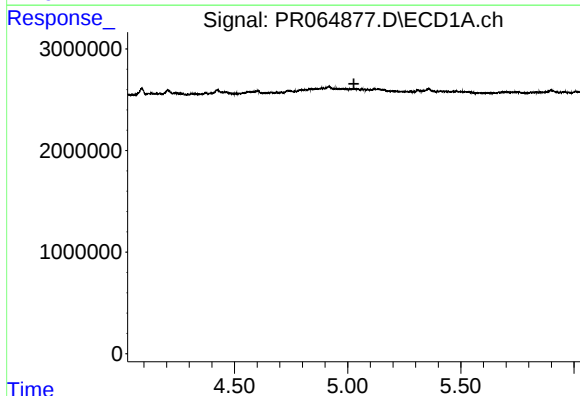


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T. : 5.028 min
Response: 0
Conc: N.D.

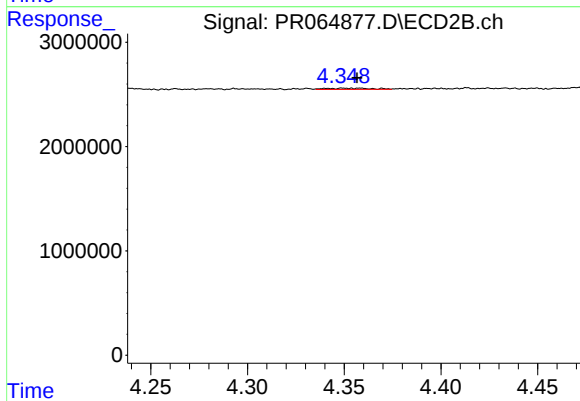

#18 AR-1242-3


R.T.: 4.349 min
Delta R.T.: -0.007 min
Response: 186660
Conc: 1.73 ng/ml

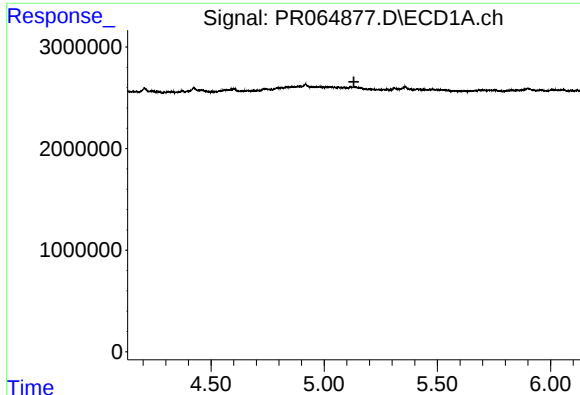

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.131 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

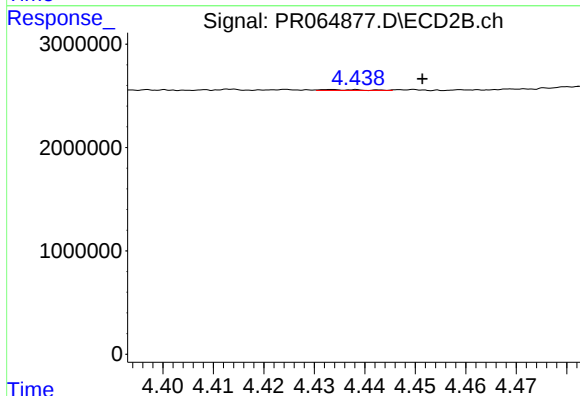


#19 AR-1242-4

R.T.: 4.433 min
Delta R.T.: -0.018 min
Response: 47806
Conc: 0.46 ng/ml

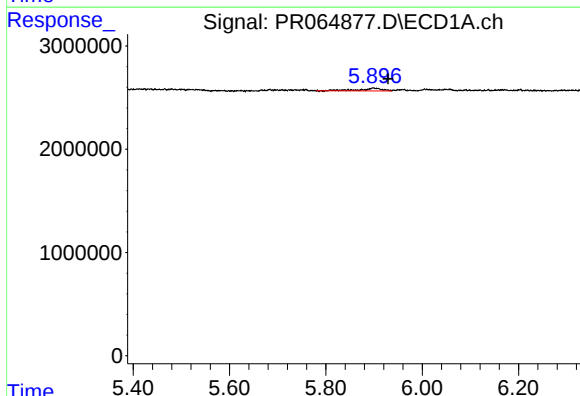


#20 AR-1242-5

R.T.: 5.898 min
Delta R.T.: -0.031 min
Response: 866226
Conc: 7.57 ng/ml

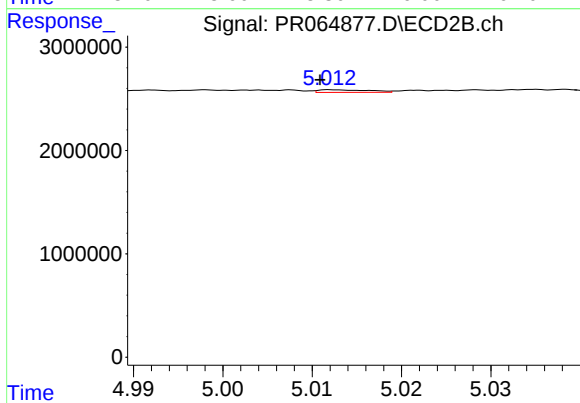

#20 AR-1242-5


R.T.: 5.013 min
Delta R.T.: 0.002 min
Response: 98509
Conc: 0.73 ng/ml

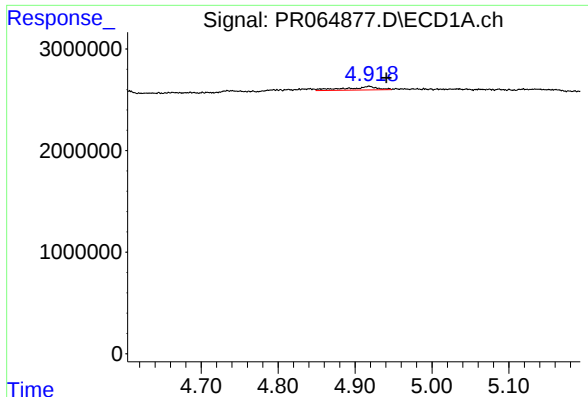

#21 AR-1248-1


R.T.: 4.919 min
Delta R.T.: -0.022 min
Response: 1002522
Conc: 9.16 ng/ml

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

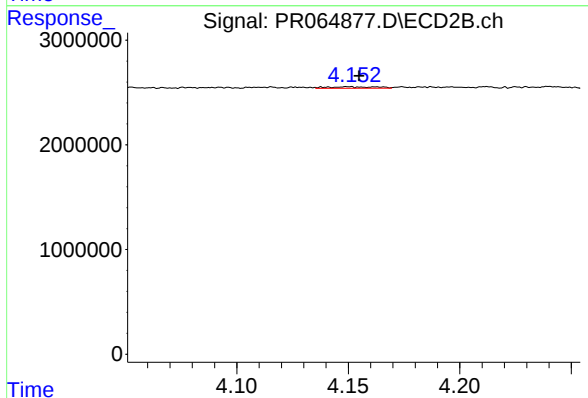


#21 AR-1248-1

R.T.: 4.150 min
Delta R.T.: -0.005 min
Response: 208861
Conc: 1.88 ng/ml

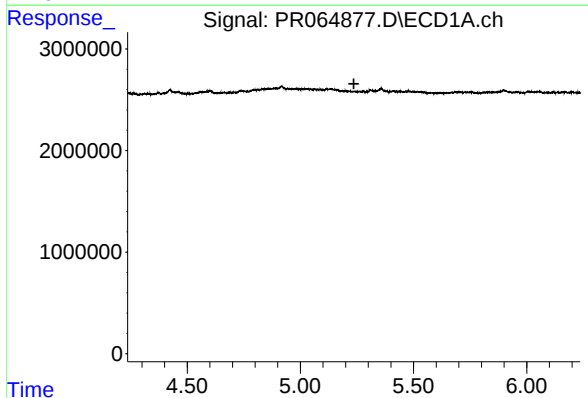


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.237 min
Response: 0
Conc: N.D.

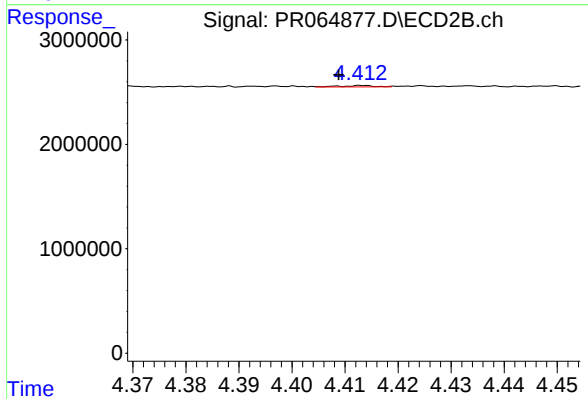

#22 AR-1248-2


R.T.: 4.414 min
Delta R.T.: 0.005 min
Response: 58343
Conc: 0.39 ng/ml

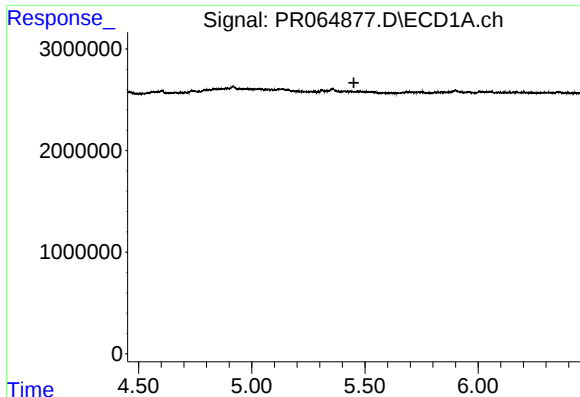

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

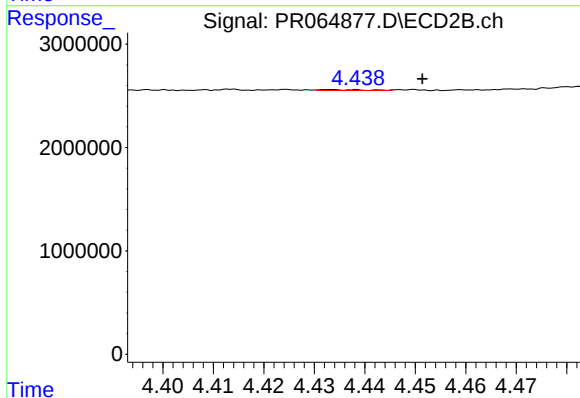


#23 AR-1248-3

R.T.: 4.433 min
Delta R.T.: -0.018 min
Response: 47806
Conc: 0.30 ng/ml

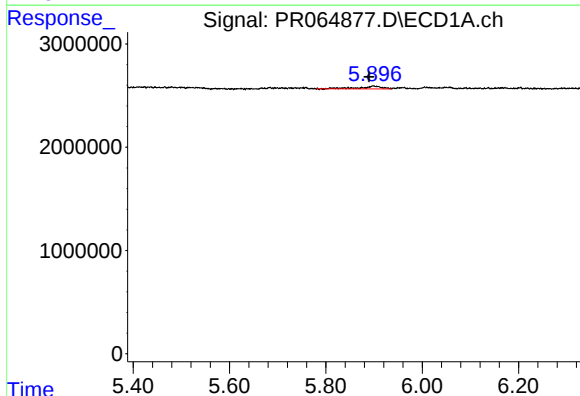


#24 AR-1248-4

R.T.: 5.898 min
Delta R.T.: 0.009 min
Response: 866226
Conc: 4.43 ng/ml

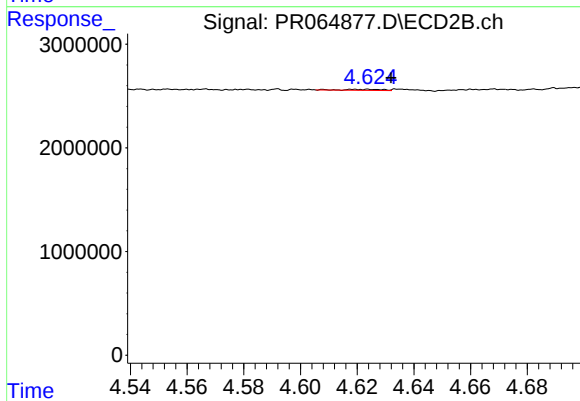

#24 AR-1248-4


R.T.: 4.624 min
Delta R.T.: -0.008 min
Response: 94067
Conc: 0.50 ng/ml

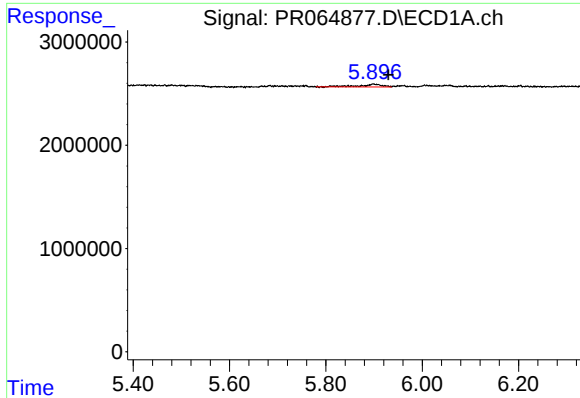

#25 AR-1248-5


R.T.: 5.898 min
Delta R.T.: -0.031 min
Response: 866226
Conc: 4.43 ng/ml

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

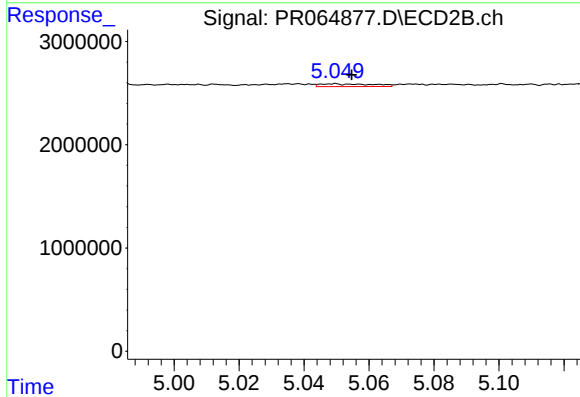


#25 AR-1248-5

R.T.: 5.049 min
Delta R.T.: -0.006 min
Response: 300200
Conc: 1.55 ng/ml

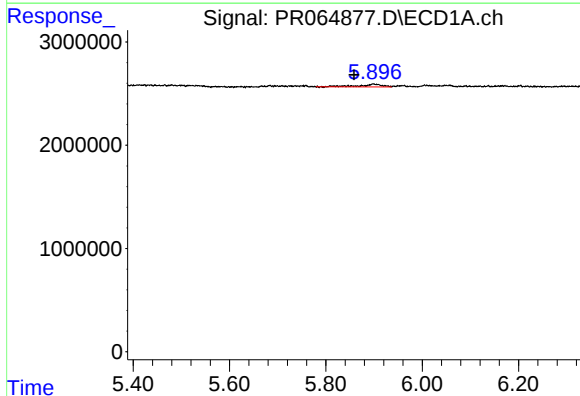


#26 AR-1254-1

R.T.: 5.898 min
Delta R.T.: 0.040 min
Response: 866226
Conc: 4.31 ng/ml

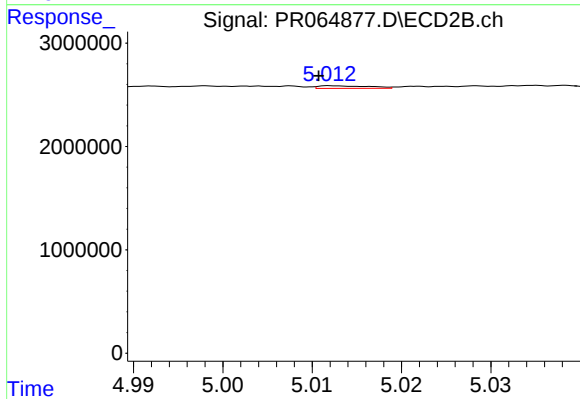

#26 AR-1254-1


R.T.: 5.013 min
Delta R.T.: 0.002 min
Response: 98509
Conc: 0.34 ng/ml

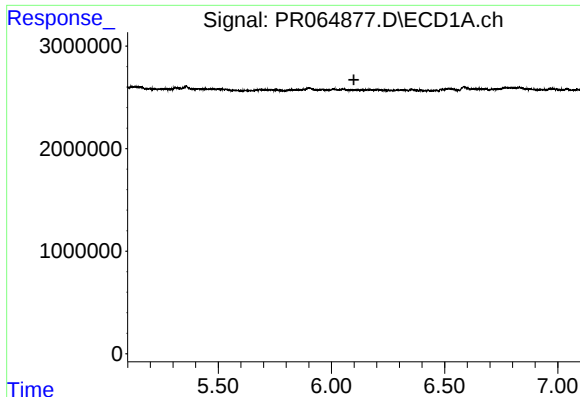

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 6.099 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

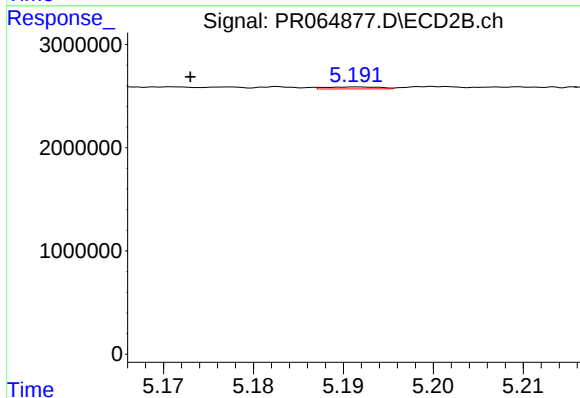


#27 AR-1254-2

R.T.: 5.192 min
Delta R.T.: 0.019 min
Response: 82536
Conc: 0.33 ng/ml

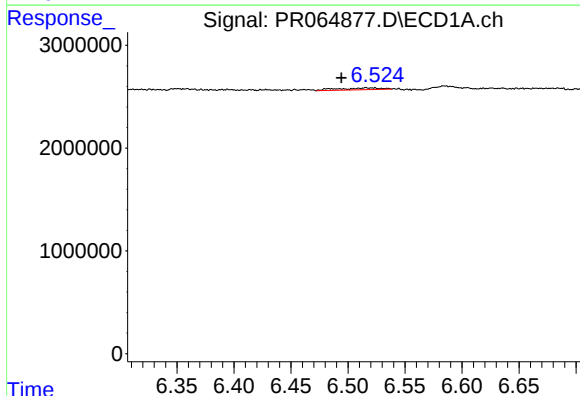


#28 AR-1254-3

R.T.: 6.516 min
Delta R.T.: 0.021 min
Response: 449554
Conc: 1.44 ng/ml

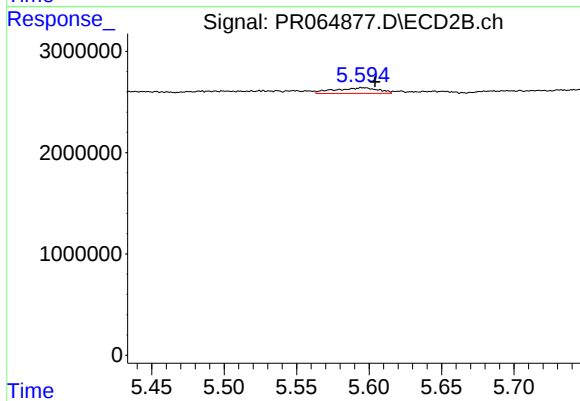

#28 AR-1254-3


R.T.: 5.596 min
Delta R.T.: -0.008 min
Response: 1171960
Conc: 2.95 ng/ml

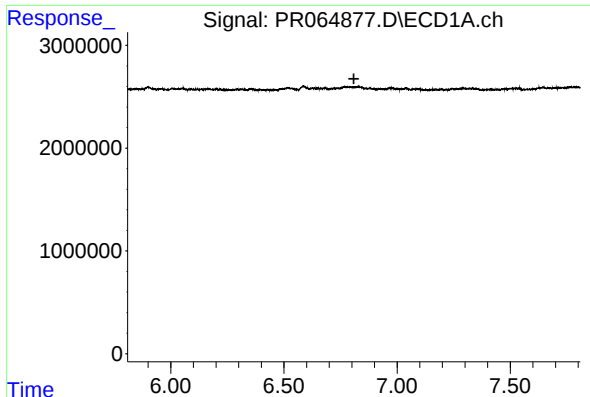

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 6.809 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

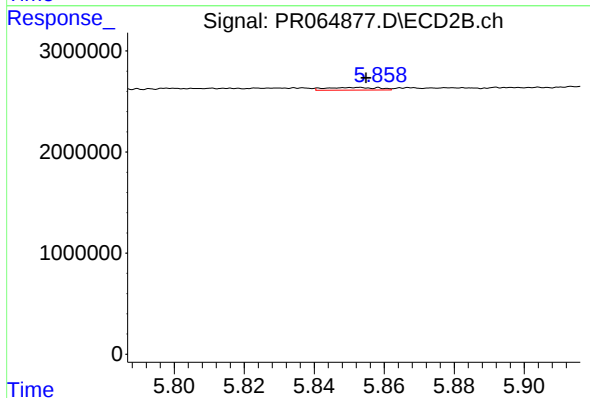


#29 AR-1254-4

R.T.: 5.852 min
Delta R.T.: -0.003 min
Response: 264182
Conc: 1.06 ng/ml

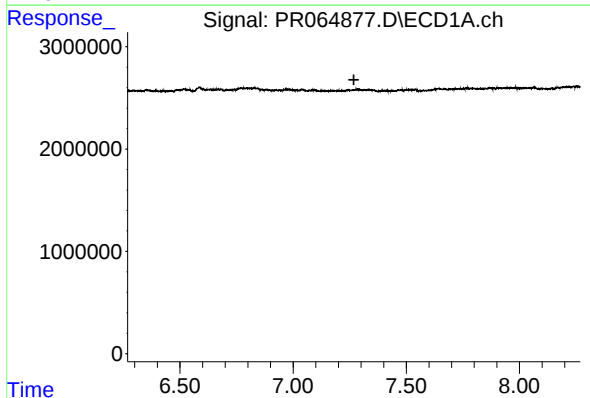


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

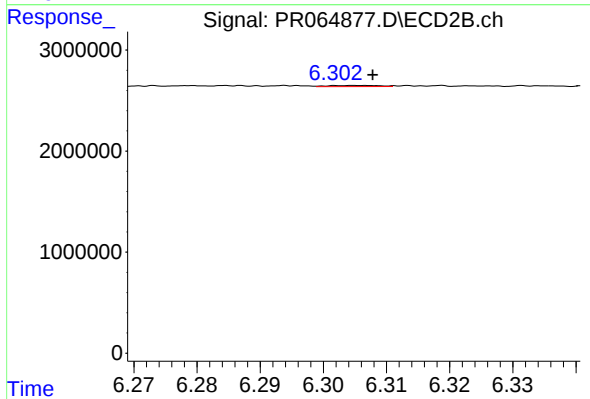

#30 AR-1254-5


R.T.: 6.306 min
Delta R.T.: -0.002 min
Response: 65958
Conc: 0.19 ng/ml

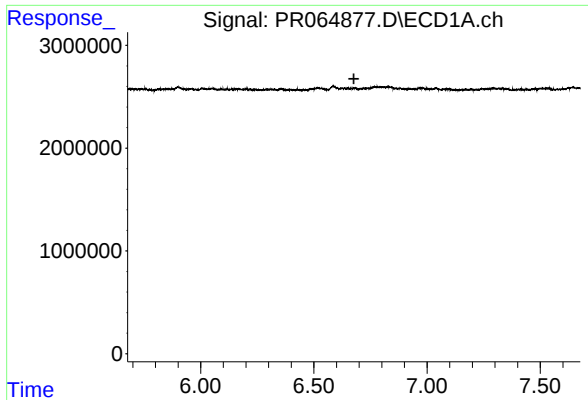

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 6.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

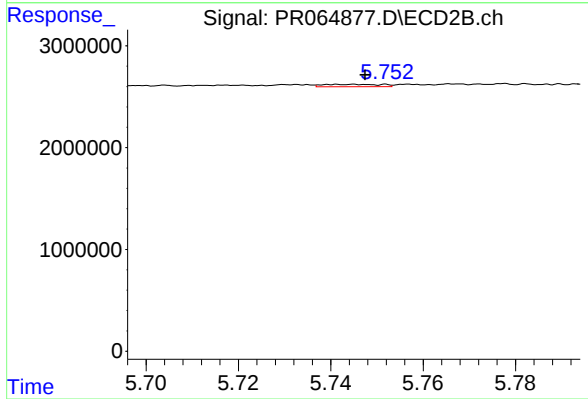


#31 AR-1260-1

R.T.: 5.745 min
Delta R.T.: -0.002 min
Response: 207489
Conc: 0.72 ng/ml

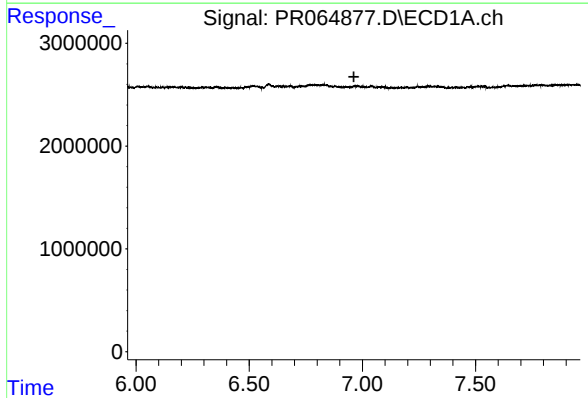


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 6.962 min
Response: 0
Conc: N.D.

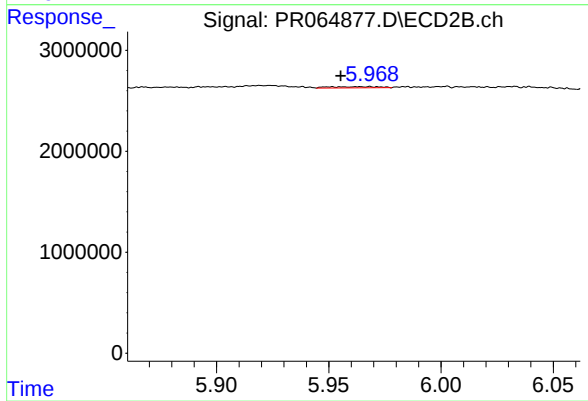

#32 AR-1260-2


R.T.: 5.969 min
Delta R.T.: 0.013 min
Response: 166688
Conc: 0.48 ng/ml

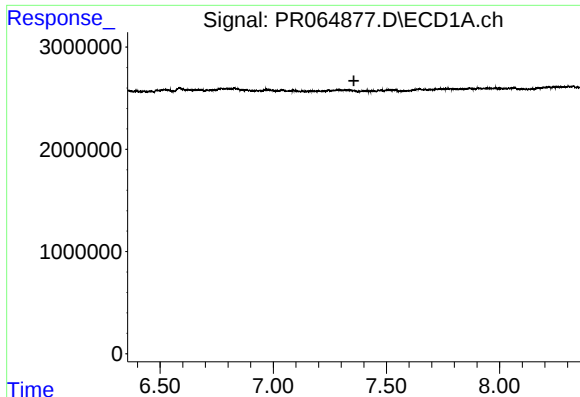

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.356 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

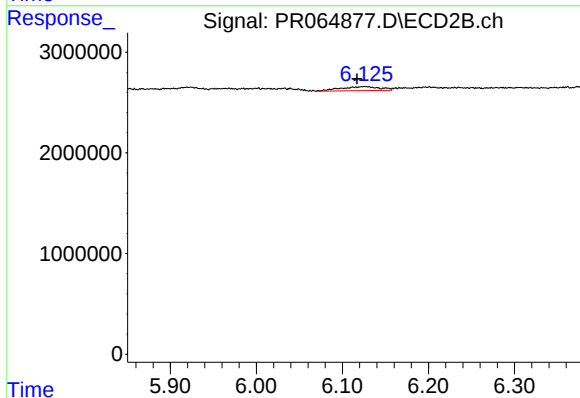


#33 AR-1260-3

R.T.: 6.126 min
Delta R.T.: 0.009 min
Response: 1248030
Conc: 3.79 ng/ml

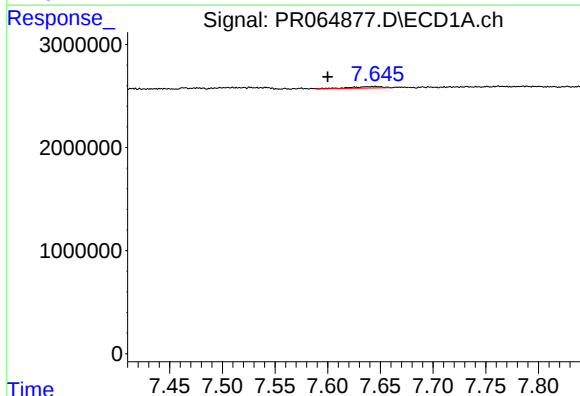


#34 AR-1260-4

R.T.: 7.645 min
Delta R.T.: 0.045 min
Response: 332011
Conc: 1.44 ng/ml

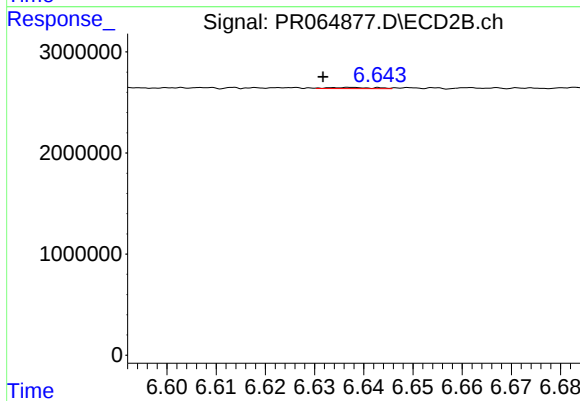

#34 AR-1260-4


R.T.: 6.638 min
Delta R.T.: 0.006 min
Response: 73423
Conc: 0.27 ng/ml

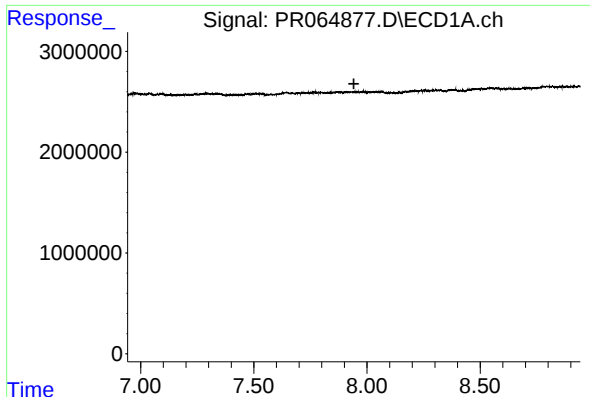

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

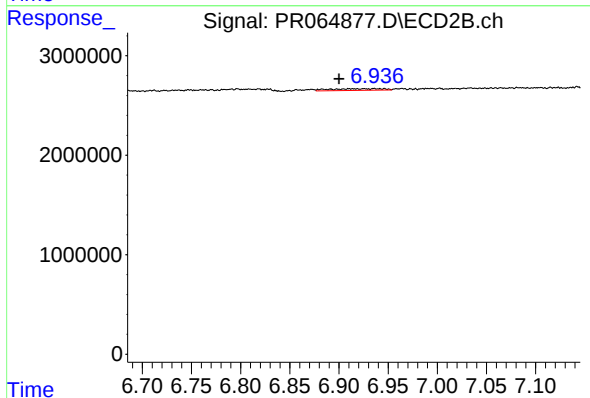


#35 AR-1260-5

R.T.: 6.918 min
Delta R.T.: 0.018 min
Response: 641840
Conc: 1.03 ng/ml

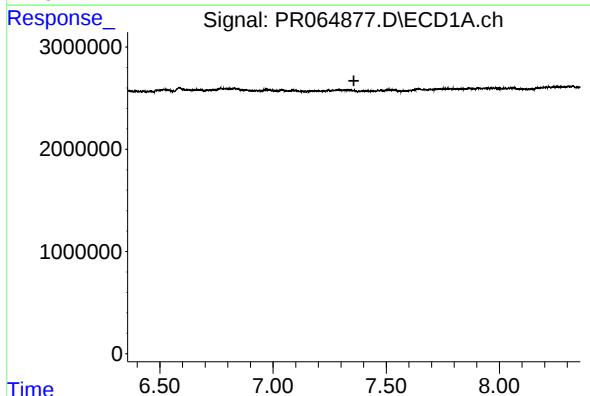


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.357 min
Response: 0
Conc: N.D.

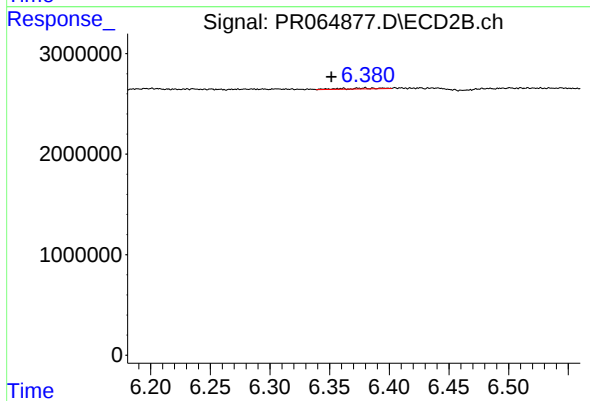

#36 AR-1262-1


R.T.: 6.380 min
Delta R.T.: 0.028 min
Response: 182490
Conc: 0.50 ng/ml

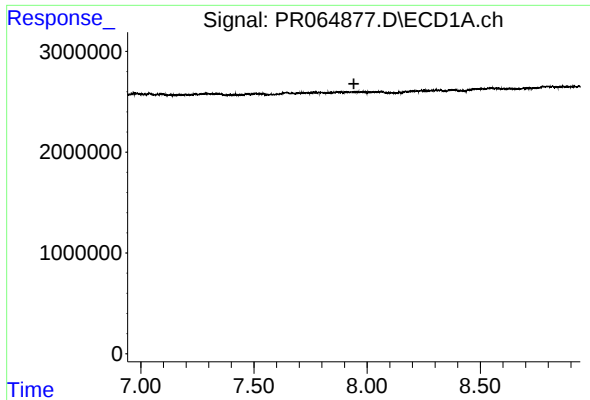

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 7.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

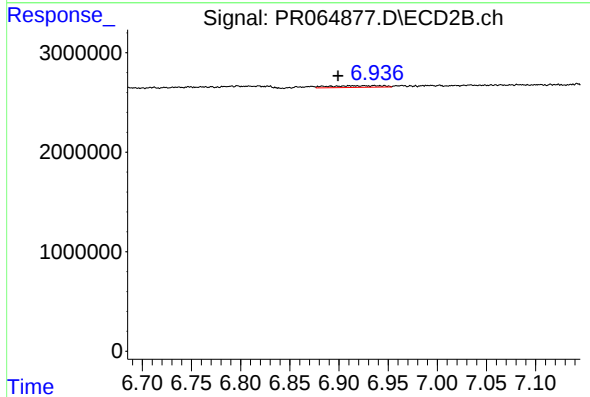


#37 AR-1262-2

R.T.: 6.918 min
Delta R.T.: 0.019 min
Response: 641840
Conc: 0.97 ng/ml

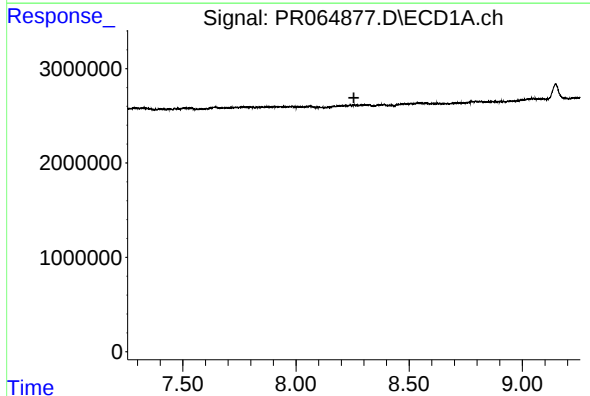


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.256 min
Response: 0
Conc: N.D.

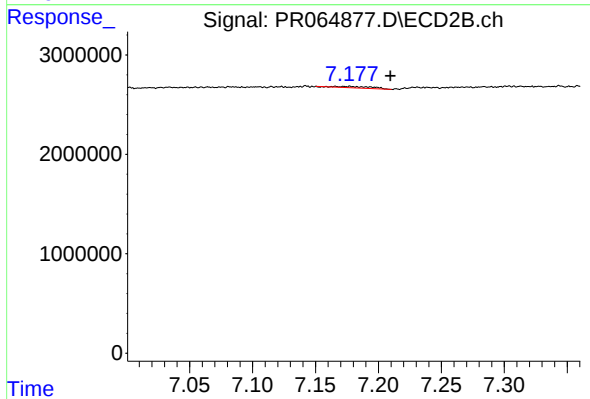

#38 AR-1262-3


R.T.: 7.178 min
Delta R.T.: -0.032 min
Response: 281494
Conc: 1.12 ng/ml

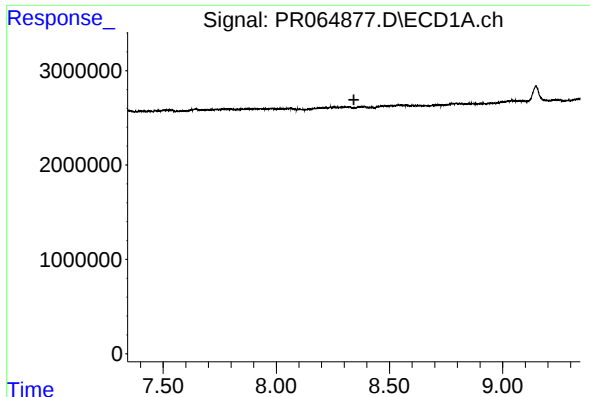

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

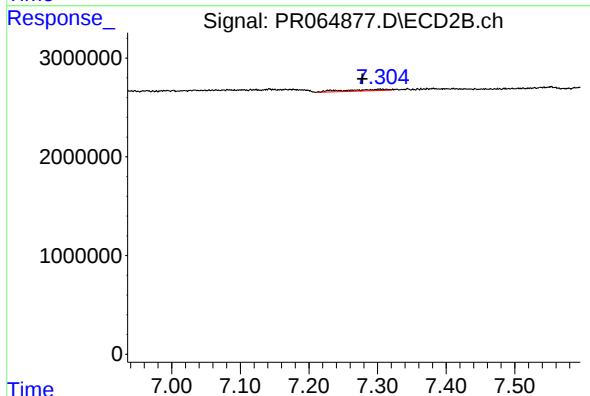


#39 AR-1262-4

R.T.: 7.303 min
Delta R.T.: 0.025 min
Response: 658838
Conc: 1.38 ng/ml

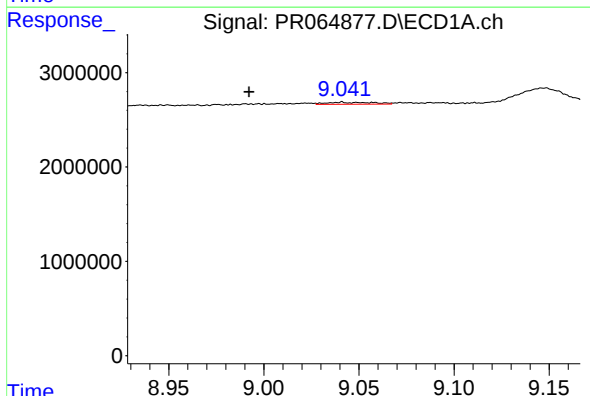


#40 AR-1262-5

R.T.: 9.041 min
Delta R.T.: 0.049 min
Response: 361692
Conc: 2.23 ng/ml

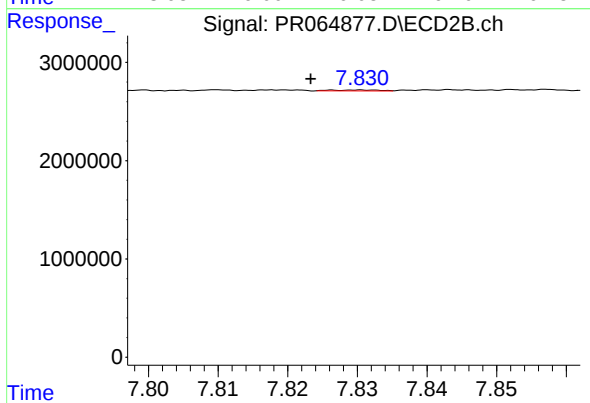

#40 AR-1262-5


R.T.: 7.830 min
Delta R.T.: 0.007 min
Response: 41978
Conc: 0.20 ng/ml

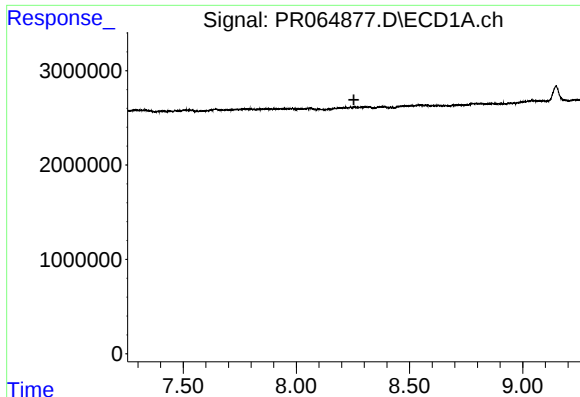

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.254 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

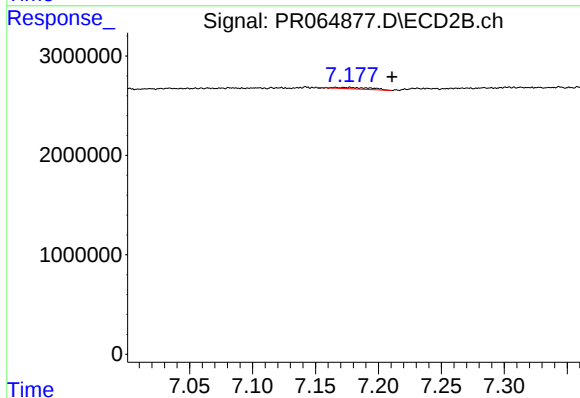


#41 AR-1268-1

R.T.: 7.178 min
Delta R.T.: -0.033 min
Response: 281494
Conc: 0.36 ng/ml

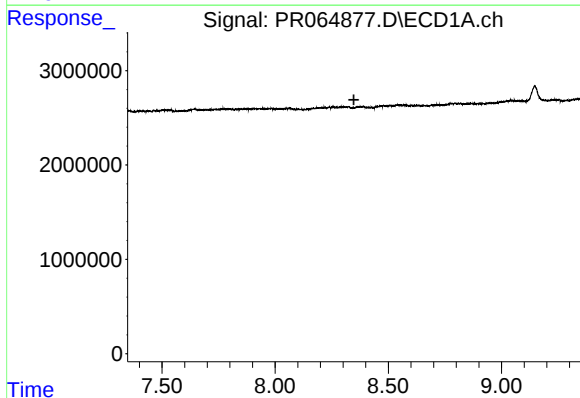


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.348 min
Response: 0
Conc: N.D.

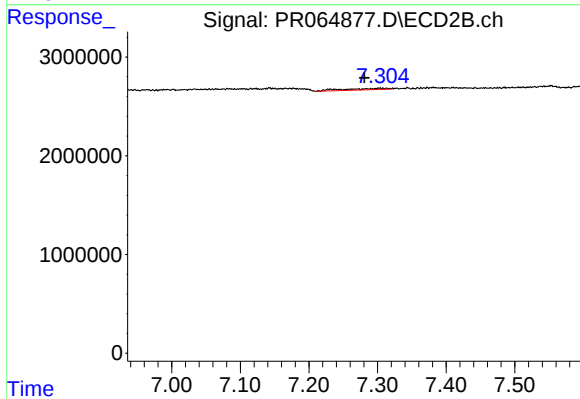

#42 AR-1268-2


R.T.: 7.303 min
Delta R.T.: 0.022 min
Response: 658838
Conc: 0.92 ng/ml

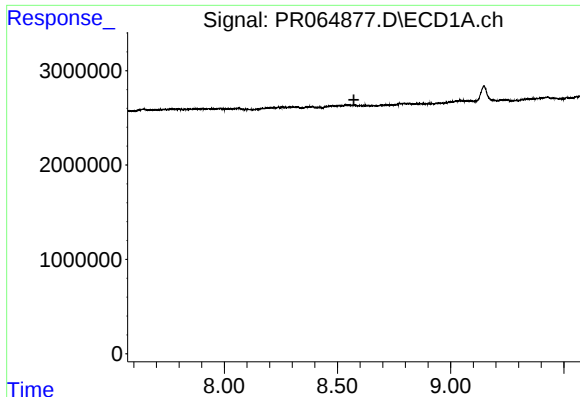

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

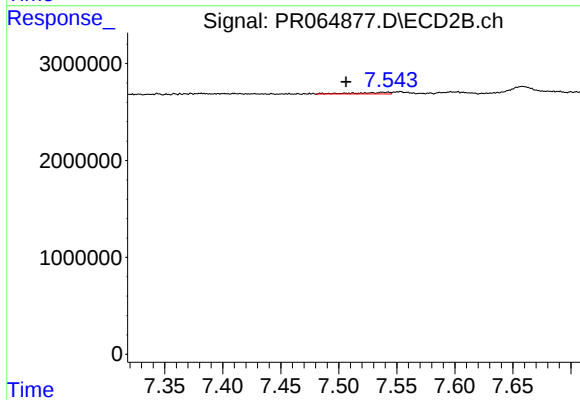


#43 AR-1268-3

R.T.: 7.543 min
Delta R.T.: 0.036 min
Response: 307556
Conc: 0.51 ng/ml

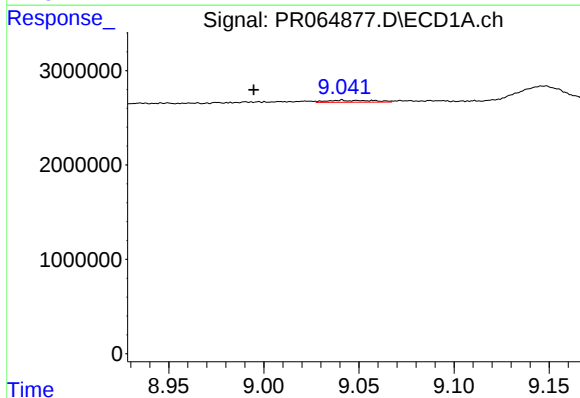


#44 AR-1268-4

R.T.: 9.041 min
Delta R.T.: 0.046 min
Response: 361692
Conc: 1.95 ng/ml

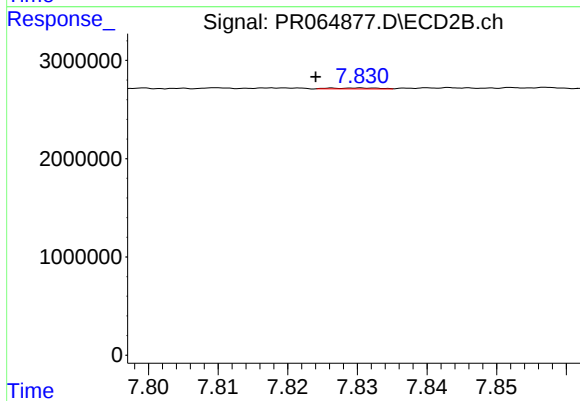

#44 AR-1268-4


R.T.: 7.830 min
Delta R.T.: 0.006 min
Response: 41978
Conc: 0.17 ng/ml

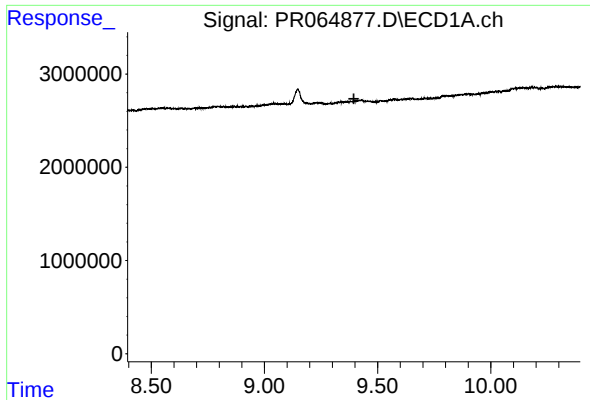

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
PCB-GPC-BLANK-SPIKE

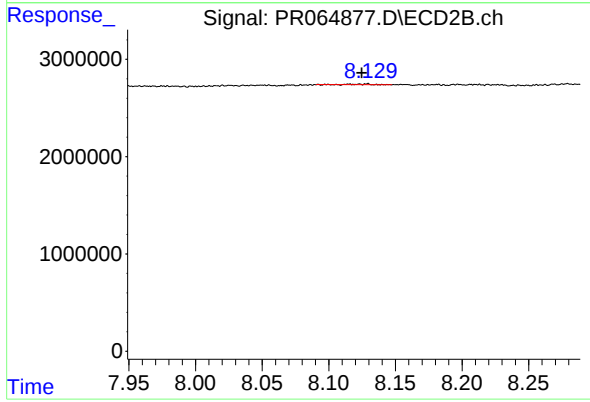

#45 AR-1268-5

R.T.: 8.129 min
Delta R.T.: 0.004 min
Response: 69353
Conc: 0.04 ng/ml