

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR011321\
 Data File : PR049299.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2021 15:45
 Operator : AJ\MA
 Sample : M1092-16
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 263K-6A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 9:47:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 09:52:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 13 16:16:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.669	3.855	46549759	65561588	19.594	24.248
2) SA Decachlor...	10.549	8.904	50147061	156.1E6	20.005	18.855
Target Compounds						
26) L6 AR-1254-1	6.698	5.742	37823578	17078189	392.640	171.766 #
27) L6 AR-1254-2	6.915	5.887	34891133	22448072	237.904	207.887
28) L6 AR-1254-3	7.286	6.292	65187740	108.6E6	434.047	514.236
29) L6 AR-1254-4	7.570	6.519	33658049	50457659	276.748	149.352 #
30) L6 AR-1254-5	7.997	6.935	133.1E6	2047.2E6	1090.975m	5105.977 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR011321\
Data File : PR049299.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2021 15:45
Operator : AJ\MA
Sample : M1092-16
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
263K-6A


Manual Integrations
APPROVED

Ankita
1/15/2021 9:47:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 09:52:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 13 16:16:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

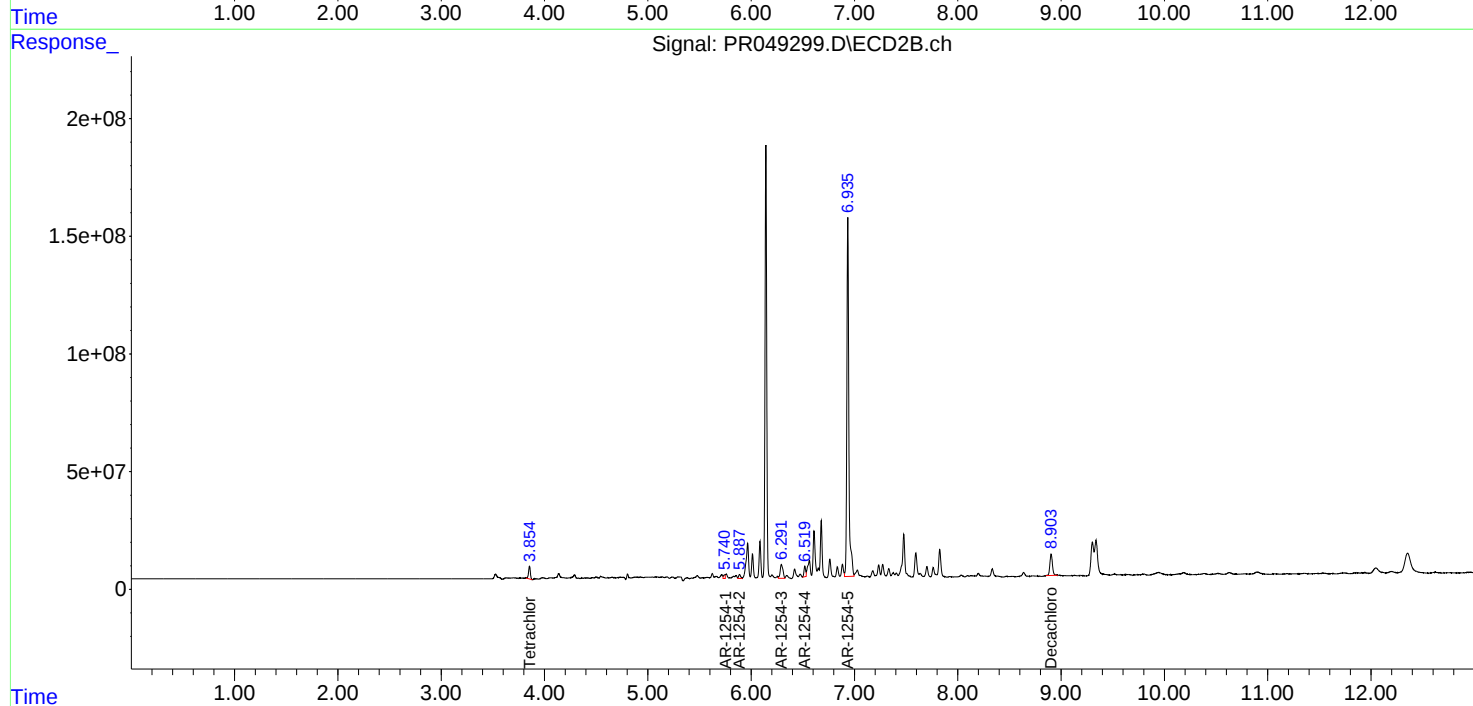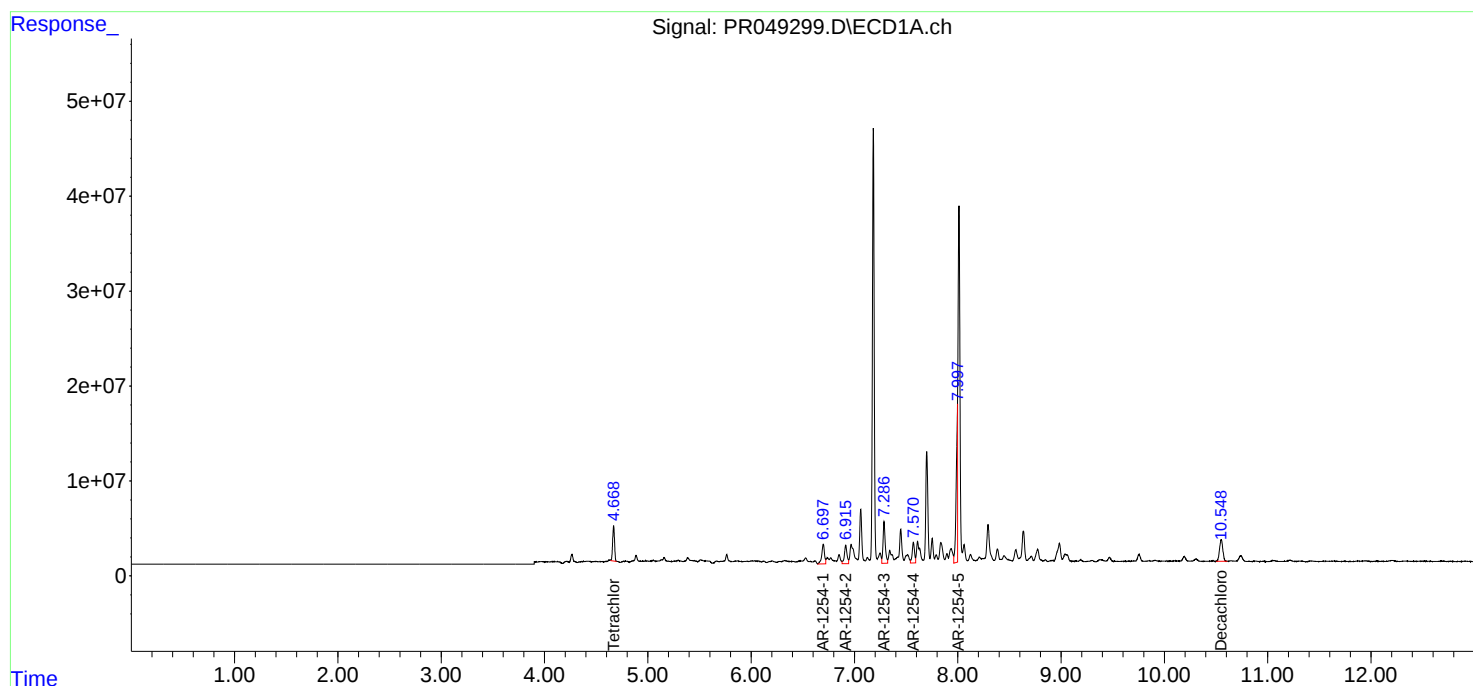

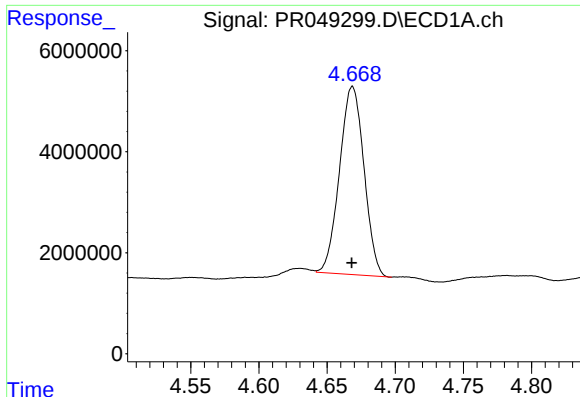


#1 Tetrachloro-m-xylene

R.T.: 4.669 min
Delta R.T.: 0.000 min
Response: 46549759
Conc: 19.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
263K-6A


Manual Integrations
APPROVED

Ankita
1/15/2021 9:47:44 AM

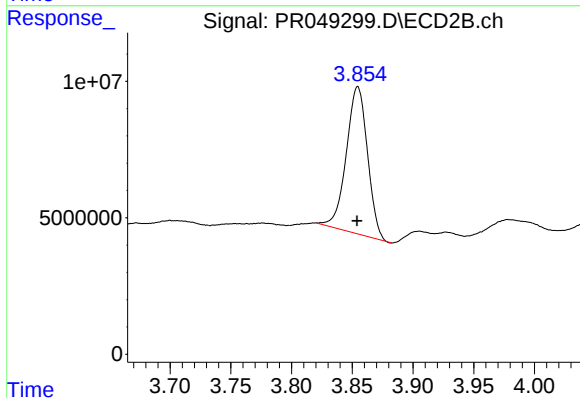


#1 Tetrachloro-m-xylene

R.T.: 3.855 min
Delta R.T.: 0.000 min
Response: 65561588
Conc: 24.25 ng/ml

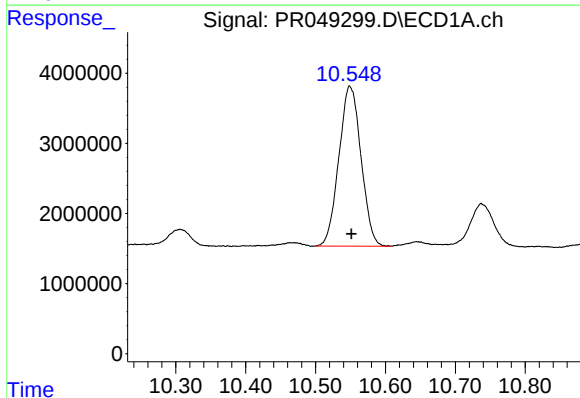


#2 Decachlorobiphenyl

R.T.: 10.549 min
Delta R.T.: -0.002 min
Response: 50147061
Conc: 20.00 ng/ml

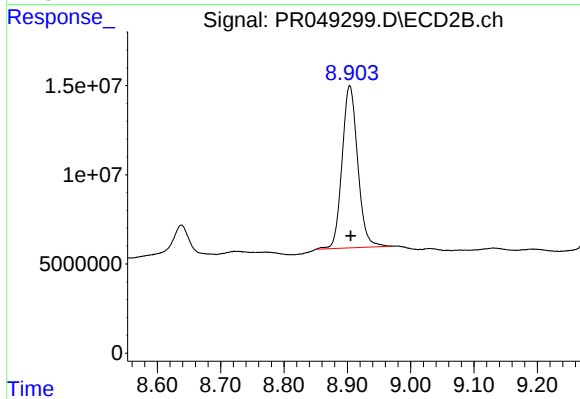

#2 Decachlorobiphenyl

R.T.: 8.904 min
Delta R.T.: -0.002 min
Response: 156129318
Conc: 18.85 ng/ml

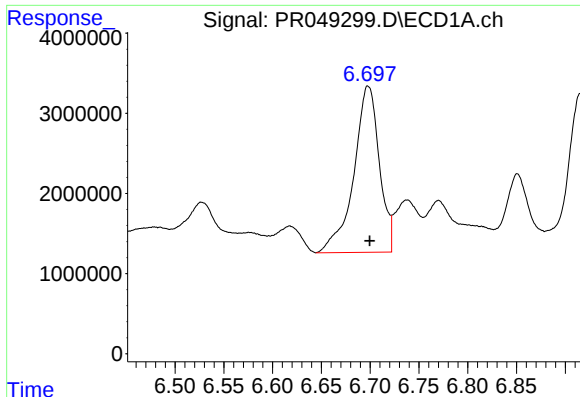


#26 AR-1254-1

R.T.: 6.698 min
Delta R.T.: -0.002 min
Response: 37823578
Conc: 392.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
263K-6A


Manual Integrations
APPROVED

Ankita
1/15/2021 9:47:44 AM

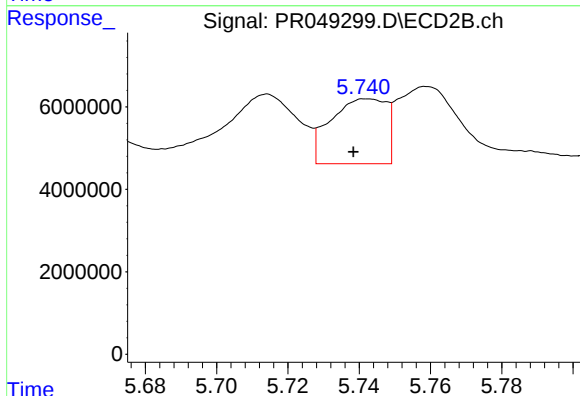


#26 AR-1254-1

R.T.: 5.742 min
Delta R.T.: 0.004 min
Response: 17078189
Conc: 171.77 ng/ml

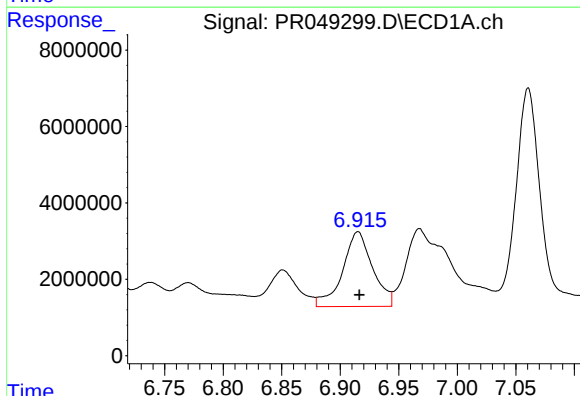


#27 AR-1254-2

R.T.: 6.915 min
Delta R.T.: -0.001 min
Response: 34891133
Conc: 237.90 ng/ml

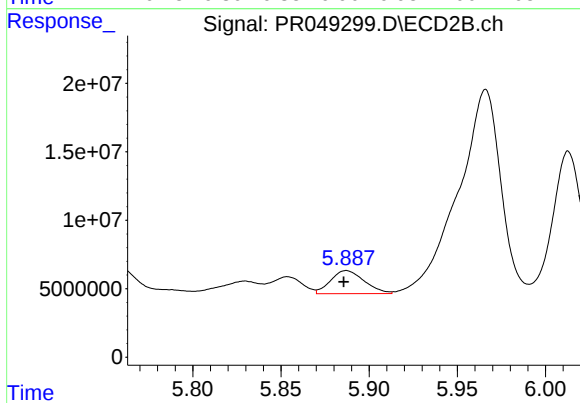

#27 AR-1254-2

R.T.: 5.887 min
Delta R.T.: 0.002 min
Response: 22448072
Conc: 207.89 ng/ml

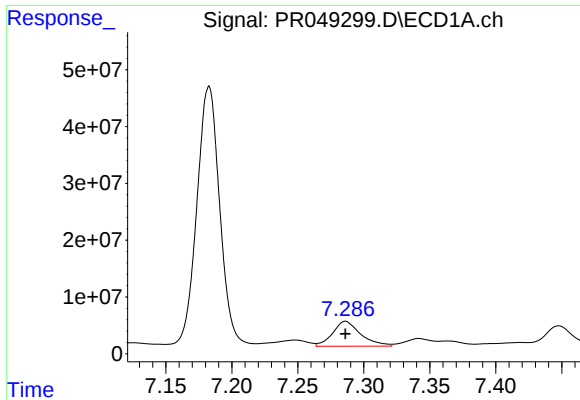


#28 AR-1254-3

R.T.: 7.286 min
Delta R.T.: 0.000 min
Response: 65187740
Conc: 434.05 ng/ml

Instrument :
ECD_R
ClientSampleId :
263K-6A


Manual Integrations
APPROVED

Ankita
1/15/2021 9:47:44 AM

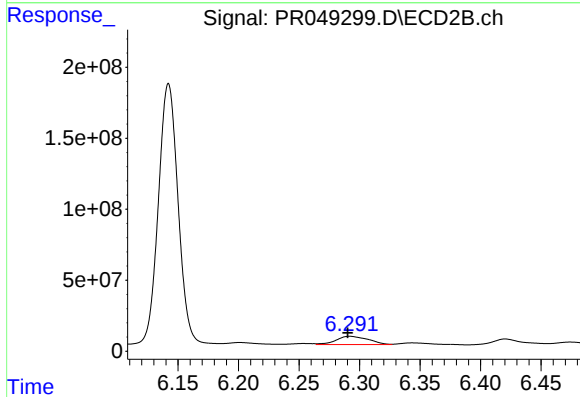


#28 AR-1254-3

R.T.: 6.292 min
Delta R.T.: 0.002 min
Response: 108626096
Conc: 514.24 ng/ml

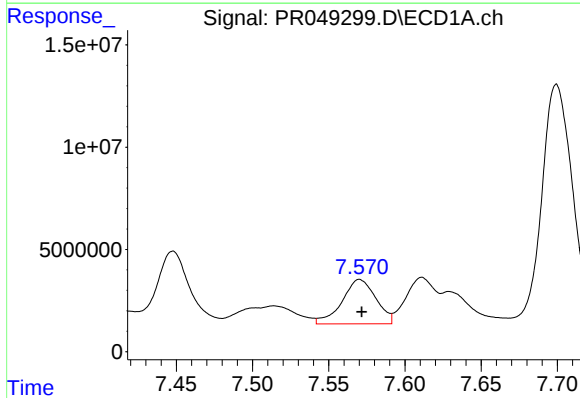


#29 AR-1254-4

R.T.: 7.570 min
Delta R.T.: -0.002 min
Response: 33658049
Conc: 276.75 ng/ml

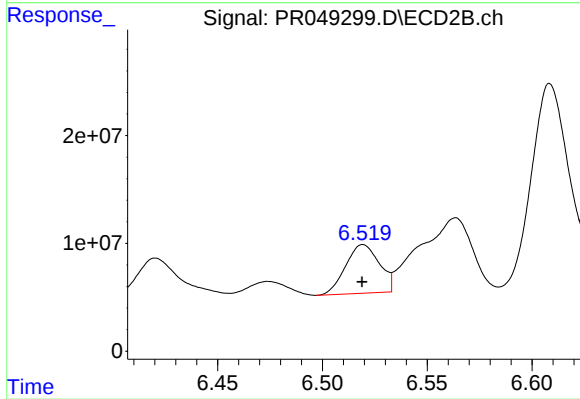

#29 AR-1254-4

R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 50457659
Conc: 149.35 ng/ml

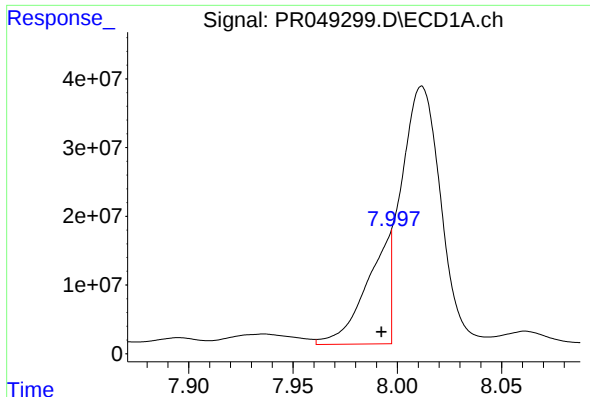


#30 AR-1254-5

R.T.: 7.997 min
Delta R.T.: 0.005 min
Response: 133105465
Conc: 1090.98 ng/ml m

Instrument :
ECD_R
ClientSampleId :
263K-6A

Manual Integrations
APPROVED

Ankita
1/15/2021 9:47:44 AM

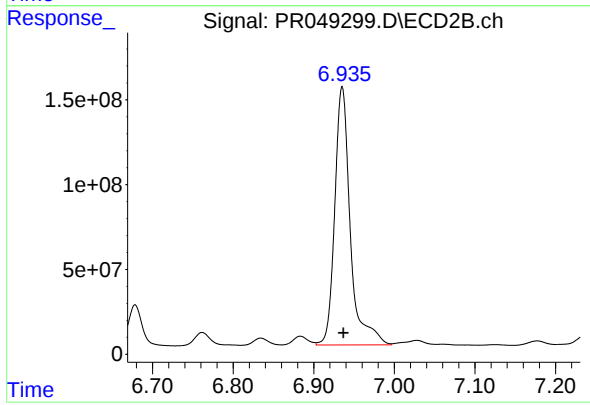

#30 AR-1254-5

R.T.: 6.935 min
Delta R.T.: -0.001 min
Response: 2047235616
Conc: 5105.98 ng/ml