

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR011321\
 Data File : PR049300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2021 16:00
 Operator : AJ\MA
 Sample : M1092-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 263K-7A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 9:47:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 09:53:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 13 16:16:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.668	3.854	44184562	66811577	18.599	24.710 #
2)	SA Decachlor...	10.550	8.906	51305992	148.5E6	20.467	17.934
Target Compounds							
26)	L6 AR-1254-1	6.698	5.741	28918088	31446593	300.194	316.278
27)	L6 AR-1254-2	6.916	5.888	36790108	25898409	250.852	239.840
28)	L6 AR-1254-3	7.287	6.292	72518264	136.6E6	482.857	646.735 #
29)	L6 AR-1254-4	7.571	6.519	31169896	49764386	256.289	147.300 #
30)	L6 AR-1254-5	7.992	6.936	112.2E6	3652.8E6	919.309m	9110.484 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR011321\
Data File : PR049300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2021 16:00
Operator : AJ\MA
Sample : M1092-19
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
263K-7A


Manual Integrations
APPROVED

Ankita
1/15/2021 9:47:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 09:53:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 13 16:16:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

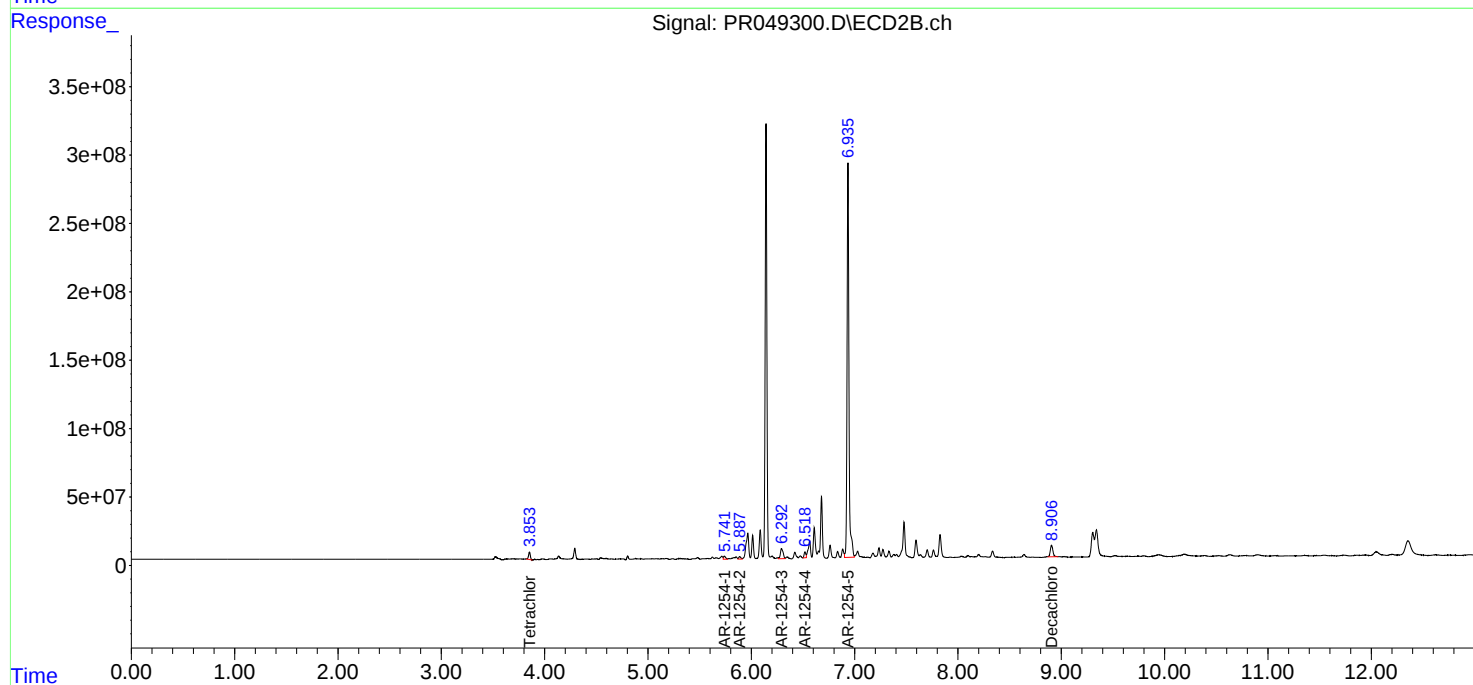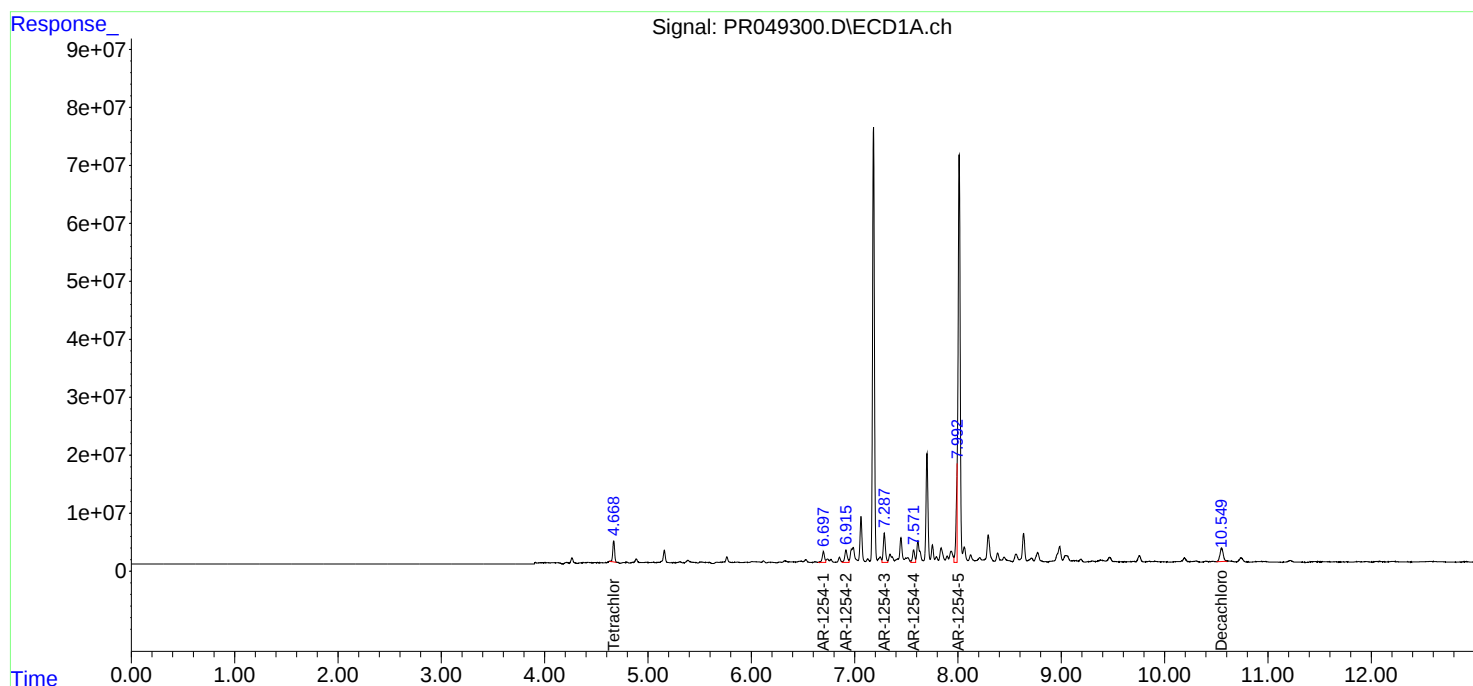

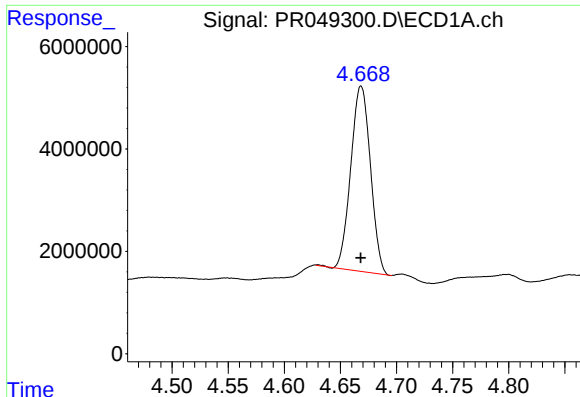


#1 Tetrachloro-m-xylene

R.T.: 4.668 min
Delta R.T.: 0.000 min
Response: 44184562
Conc: 18.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
263K-7A


Manual Integrations
APPROVED

Ankita
1/15/2021 9:47:46 AM

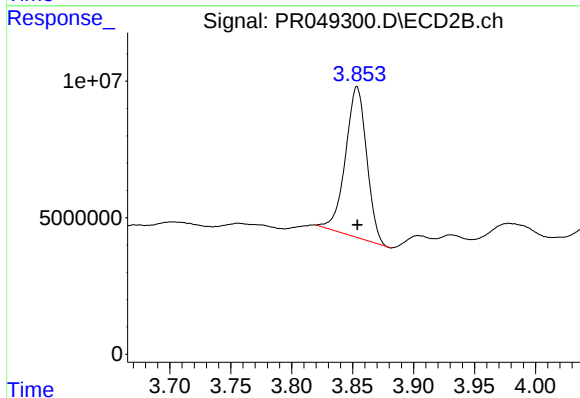


#1 Tetrachloro-m-xylene

R.T.: 3.854 min
Delta R.T.: 0.000 min
Response: 66811577
Conc: 24.71 ng/ml

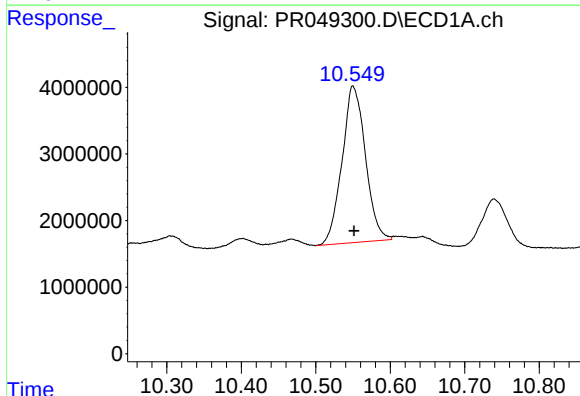


#2 Decachlorobiphenyl

R.T.: 10.550 min
Delta R.T.: -0.002 min
Response: 51305992
Conc: 20.47 ng/ml

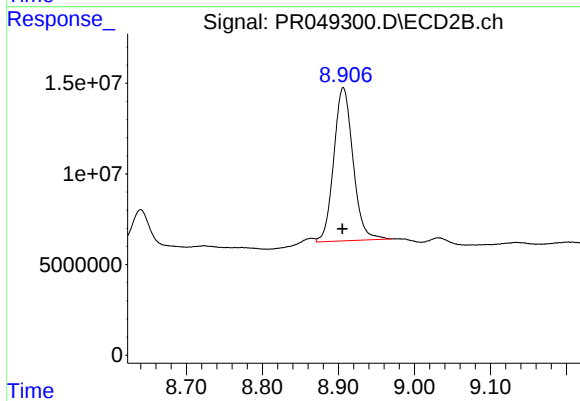

#2 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: 0.001 min
Response: 148510132
Conc: 17.93 ng/ml

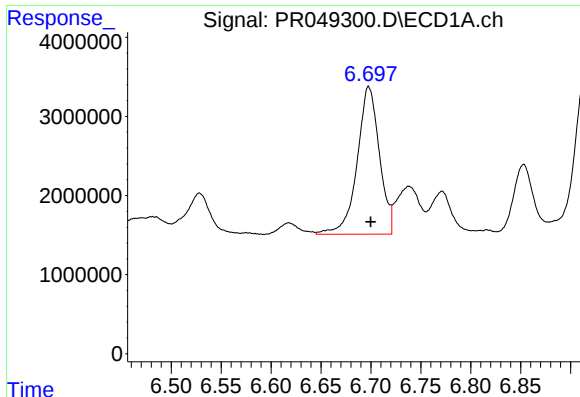


#26 AR-1254-1

R.T.: 6.698 min
Delta R.T.: -0.002 min
Response: 28918088
Conc: 300.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
263K-7A


Manual Integrations
APPROVED

Ankita
1/15/2021 9:47:46 AM

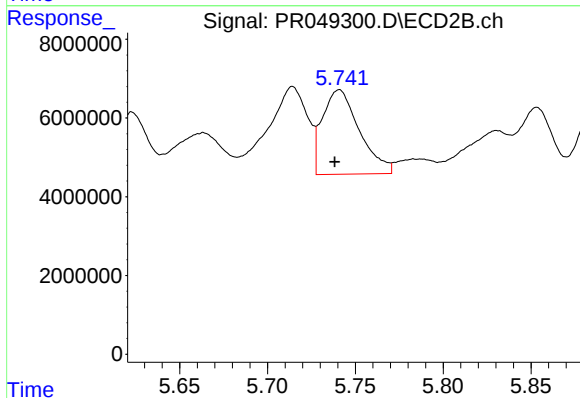


#26 AR-1254-1

R.T.: 5.741 min
Delta R.T.: 0.003 min
Response: 31446593
Conc: 316.28 ng/ml

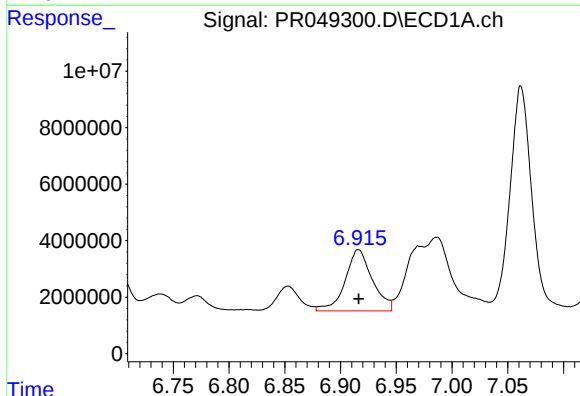


#27 AR-1254-2

R.T.: 6.916 min
Delta R.T.: 0.000 min
Response: 36790108
Conc: 250.85 ng/ml

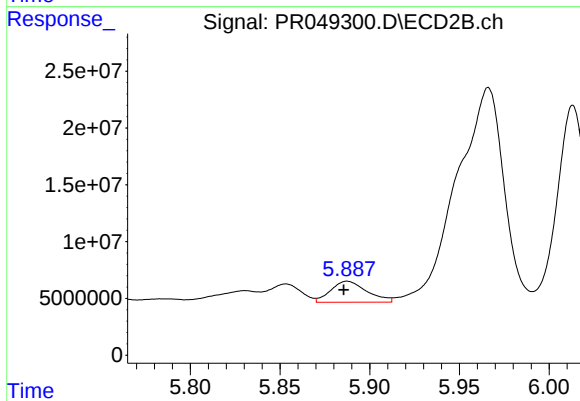

#27 AR-1254-2

R.T.: 5.888 min
Delta R.T.: 0.002 min
Response: 25898409
Conc: 239.84 ng/ml

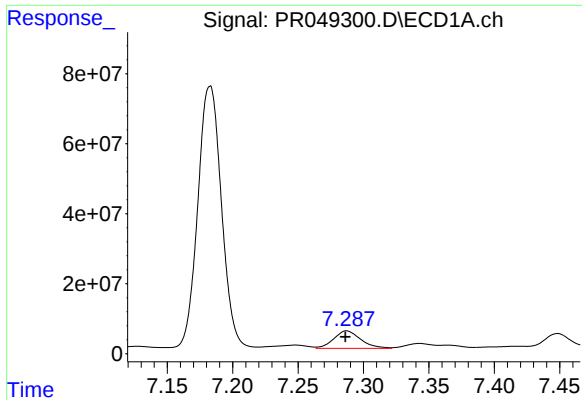


#28 AR-1254-3

R.T.: 7.287 min
Delta R.T.: 0.000 min
Response: 72518264
Conc: 482.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
263K-7A


Manual Integrations
APPROVED

Ankita
1/15/2021 9:47:46 AM

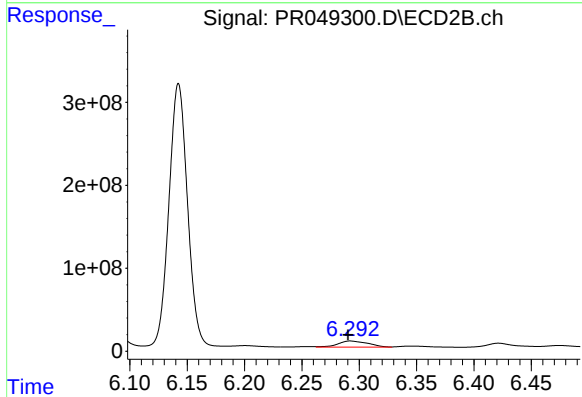


#28 AR-1254-3

R.T.: 6.292 min
Delta R.T.: 0.002 min
Response: 136614956
Conc: 646.73 ng/ml

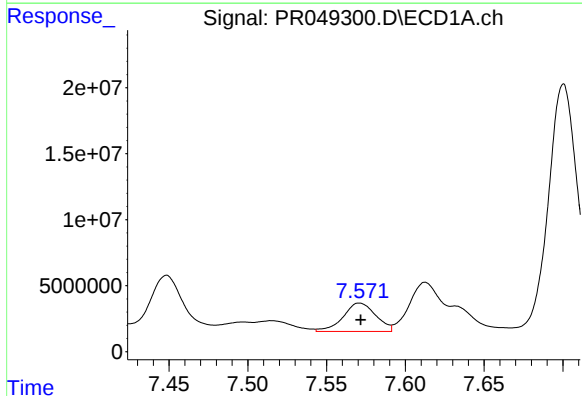


#29 AR-1254-4

R.T.: 7.571 min
Delta R.T.: 0.000 min
Response: 31169896
Conc: 256.29 ng/ml

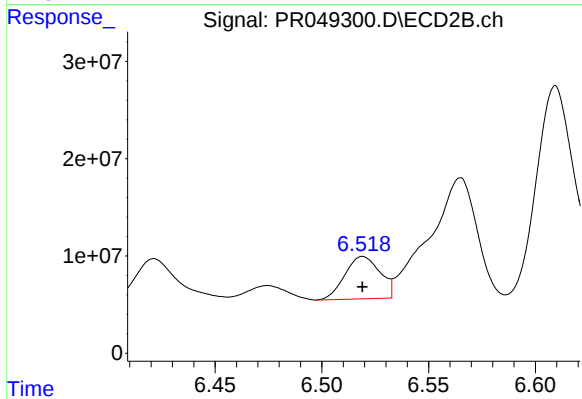

#29 AR-1254-4

R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 49764386
Conc: 147.30 ng/ml

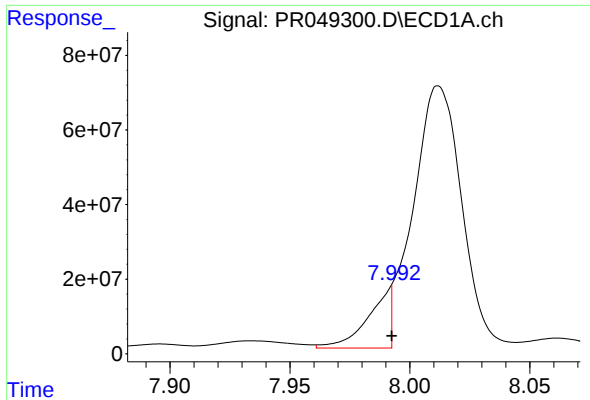


#30 AR-1254-5

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 112161145
Conc: 919.31 ng/ml m

Instrument :
ECD_R
ClientSampleId :
263K-7A

Manual Integrations
APPROVED

Ankita
1/15/2021 9:47:46 AM

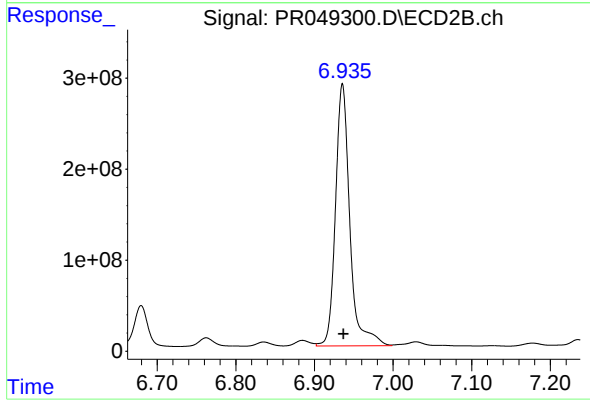

#30 AR-1254-5

R.T.: 6.936 min
Delta R.T.: -0.001 min
Response: 3652837547
Conc: 9110.48 ng/ml