

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR011421\
 Data File : PR049332.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2021 11:18
 Operator : AJ\MA
 Sample : M1092-16DL 2X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 263K-6ADL

Manual Integrations
 APPROVED

Ankita
 1/18/2021 10:18:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 01:09:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 13 16:16:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.668	3.853	23832441	38018761	10.032	14.061 #
2) SA Decachlor...	10.549	8.907	26818435	81527647	10.698	9.845
Target Compounds						
26) L6 AR-1254-1	6.698	5.739	13359085	12845944	138.678	129.200m
27) L6 AR-1254-2	6.915	5.887	15484556	17141215	105.581	158.741m#
28) L6 AR-1254-3	7.287	6.292	31056001	86729089	206.784	410.575 #
29) L6 AR-1254-4	7.572	6.519	17379745	39263746	142.902	116.218
30) L6 AR-1254-5	7.994	6.936	54043991	1129.0E6	442.962m	2815.736 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR011421\
Data File : PR049332.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2021 11:18
Operator : AJ\MA
Sample : M1092-16DL 2X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampled :
263K-6ADL


Manual Integrations
APPROVED

Ankita
1/18/2021 10:18:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 01:09:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 13 16:16:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

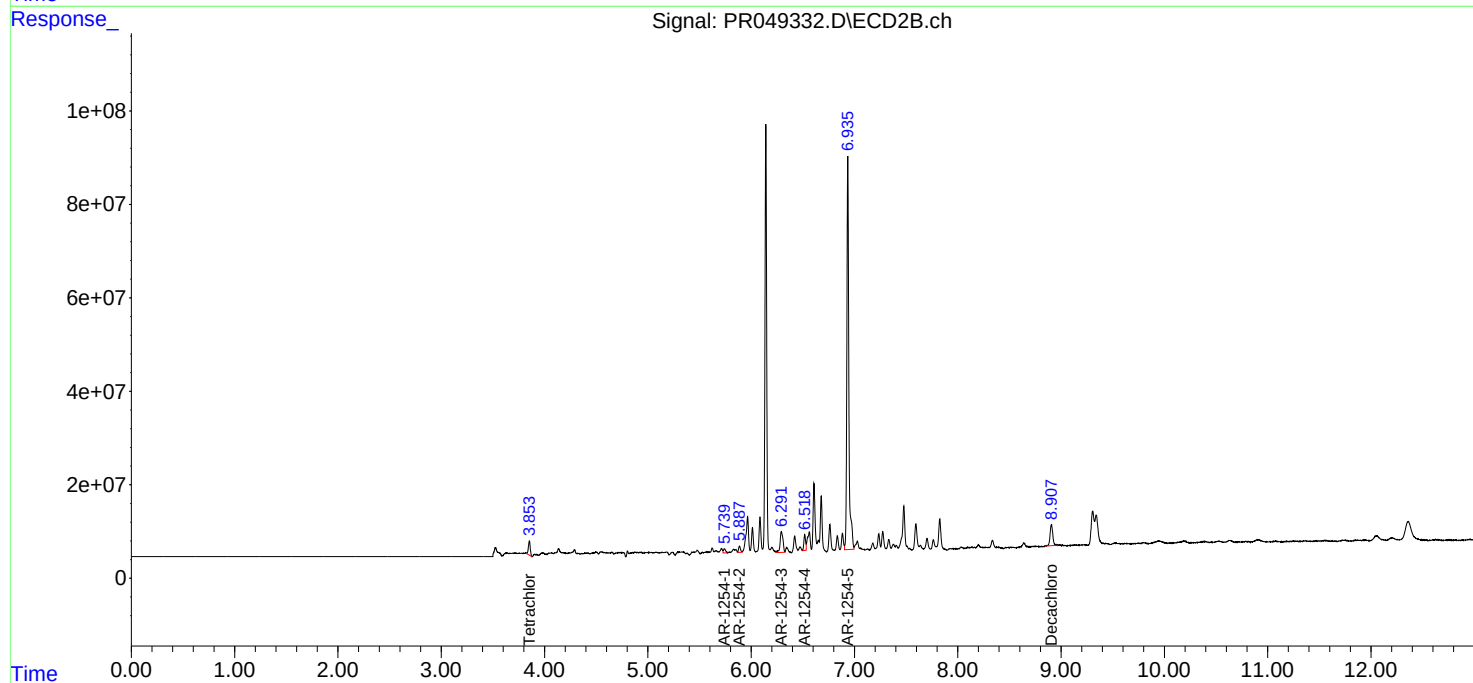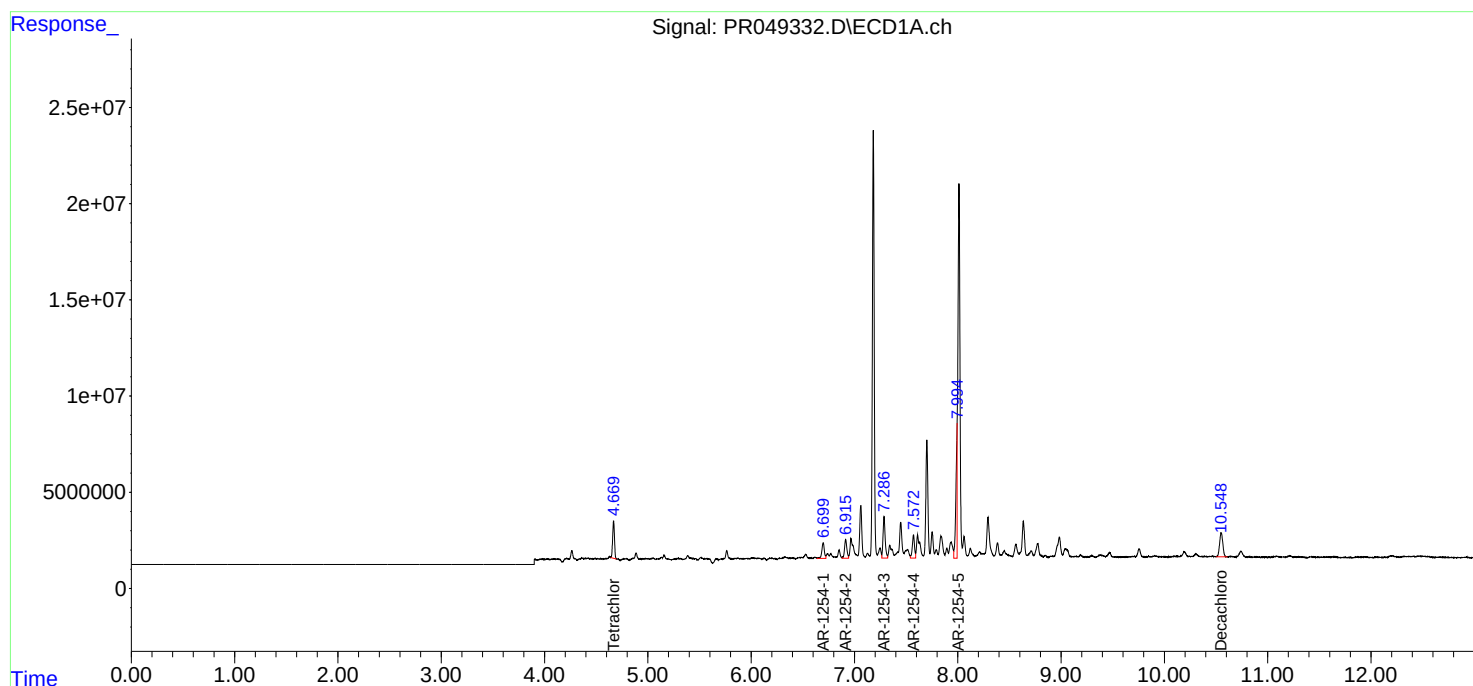

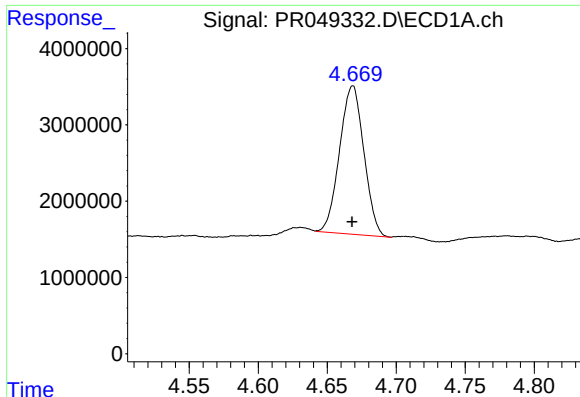


#1 Tetrachloro-m-xylene

R.T.: 4.668 min
Delta R.T.: 0.000 min
Response: 23832441
Conc: 10.03 ng/ml

Instrument :
ECD_R
ClientSampleId :
263K-6ADL


Manual Integrations
APPROVED

Ankita
1/18/2021 10:18:15 AM

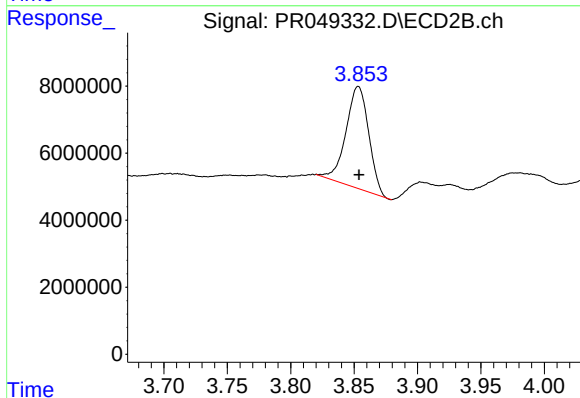


#1 Tetrachloro-m-xylene

R.T.: 3.853 min
Delta R.T.: 0.000 min
Response: 38018761
Conc: 14.06 ng/ml

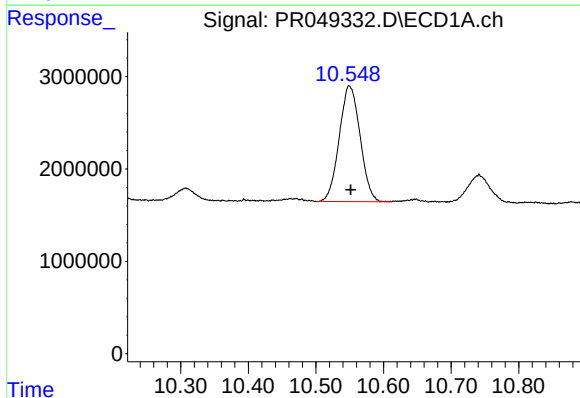


#2 Decachlorobiphenyl

R.T.: 10.549 min
Delta R.T.: -0.002 min
Response: 26818435
Conc: 10.70 ng/ml

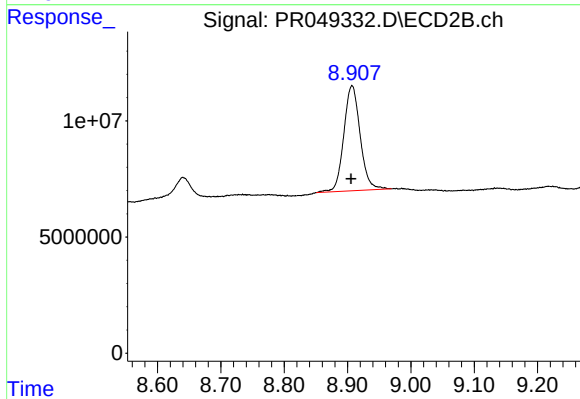

#2 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.002 min
Response: 81527647
Conc: 9.85 ng/ml

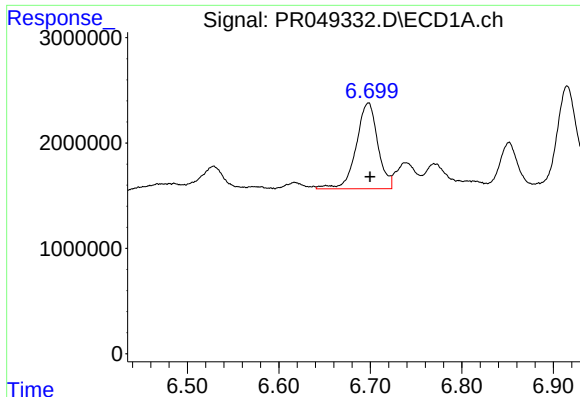


#26 AR-1254-1

R.T.: 6.698 min
Delta R.T.: -0.002 min
Response: 13359085
Conc: 138.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
263K-6ADL


Manual Integrations
APPROVED

Ankita
1/18/2021 10:18:15 AM

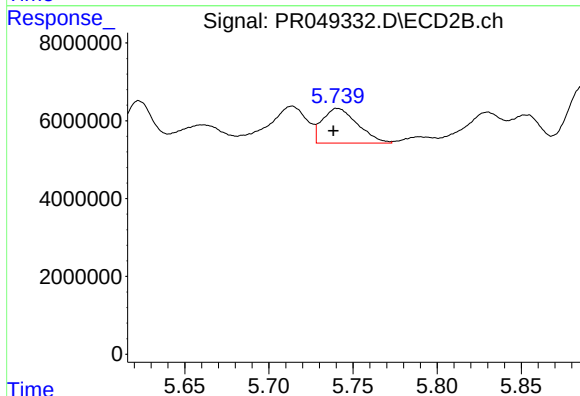


#26 AR-1254-1

R.T.: 5.739 min
Delta R.T.: 0.001 min
Response: 12845944
Conc: 129.20 ng/ml m

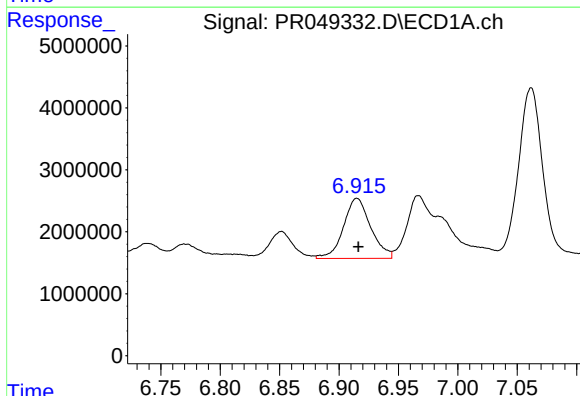


#27 AR-1254-2

R.T.: 6.915 min
Delta R.T.: -0.001 min
Response: 15484556
Conc: 105.58 ng/ml

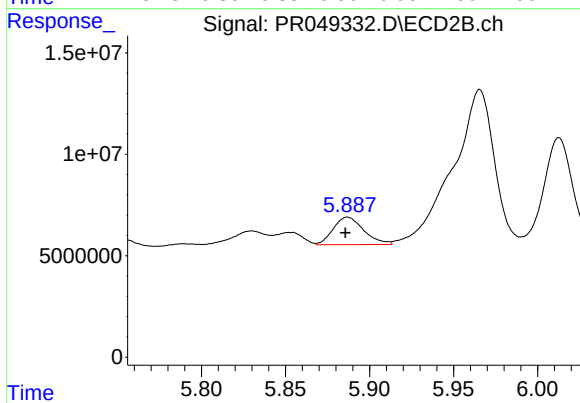

#27 AR-1254-2

R.T.: 5.887 min
Delta R.T.: 0.001 min
Response: 17141215
Conc: 158.74 ng/ml m

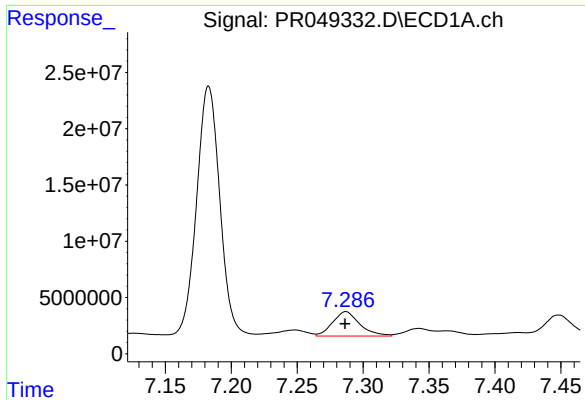


#28 AR-1254-3

R.T.: 7.287 min
Delta R.T.: 0.000 min
Response: 31056001
Conc: 206.78 ng/ml

Instrument :
ECD_R
ClientSampleId :
263K-6ADL


Manual Integrations
APPROVED

Ankita
1/18/2021 10:18:15 AM

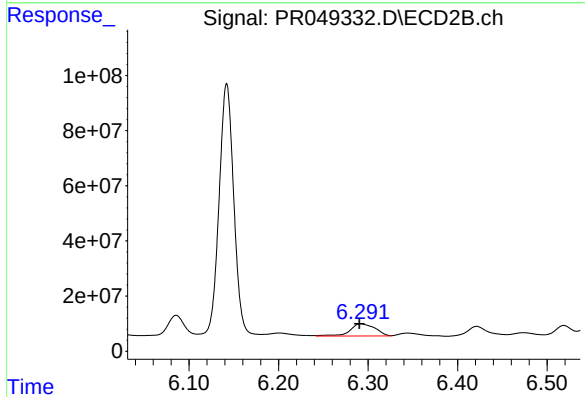


#28 AR-1254-3

R.T.: 6.292 min
Delta R.T.: 0.002 min
Response: 86729089
Conc: 410.58 ng/ml

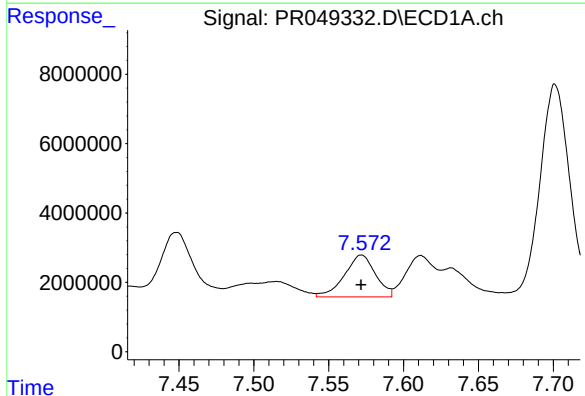


#29 AR-1254-4

R.T.: 7.572 min
Delta R.T.: 0.000 min
Response: 17379745
Conc: 142.90 ng/ml

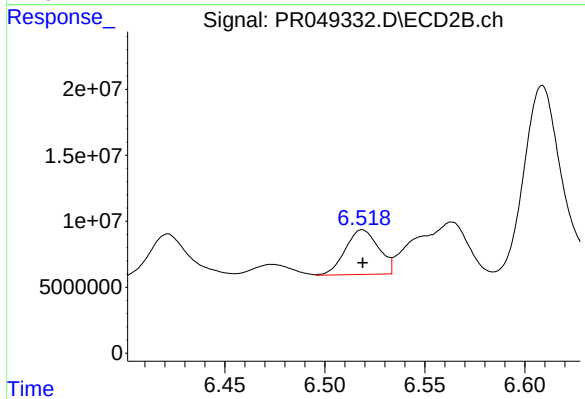

#29 AR-1254-4

R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 39263746
Conc: 116.22 ng/ml

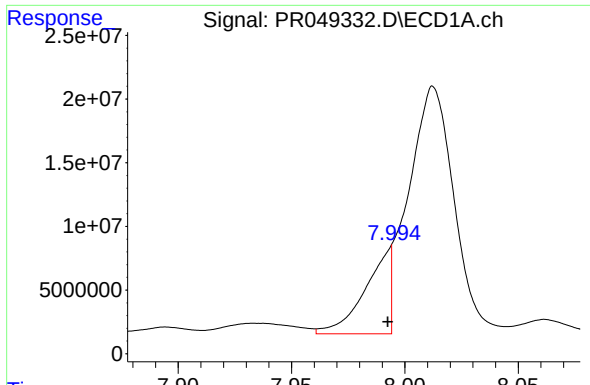


#30 AR-1254-5

R.T.: 7.994 min
Delta R.T.: 0.002 min
Response: 54043991
Conc: 442.96 ng/ml m

Instrument :
ECD_R
ClientSampleId :
263K-6ADL

Manual Integrations
APPROVED

Ankita
1/18/2021 10:18:15 AM

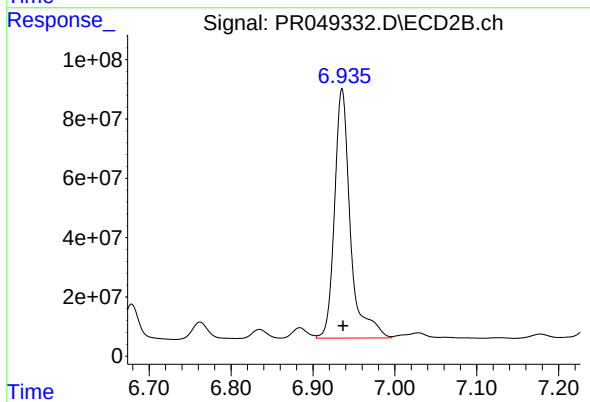

#30 AR-1254-5

R.T.: 6.936 min
Delta R.T.: -0.001 min
Response: 1128965998
Conc: 2815.74 ng/ml