

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR011421\
 Data File : PR049333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2021 11:33
 Operator : AJ\MA
 Sample : M1092-19DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 263K-7ADL

Manual Integrations
 APPROVED

Ankita
 1/18/2021 10:18:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 01:10:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 13 16:16:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.667	3.853	10212348	19048891	4.299m	7.045 #
2) SA Decachlor...	10.550	8.907	12731198	32841212	5.079	3.966
Target Compounds						
26) L6 AR-1254-1	6.699	5.741	7177597	13332743	74.509	134.096 #
27) L6 AR-1254-2	6.917	5.887	10891744	12324922	74.265	114.138 #
28) L6 AR-1254-3	7.287	6.292	16929637	43393029	112.725	205.423 #
29) L6 AR-1254-4	7.571	6.519	7960120	15773341	65.451	46.688 #
30) L6 AR-1254-5	7.993	6.936	25114662	695.8E6	205.848m	1735.421 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR011421\
Data File : PR049333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2021 11:33
Operator : AJ\MA
Sample : M1092-19DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
263K-7ADL


Manual Integrations
APPROVED

Ankita
1/18/2021 10:18:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 01:10:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 13 16:16:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

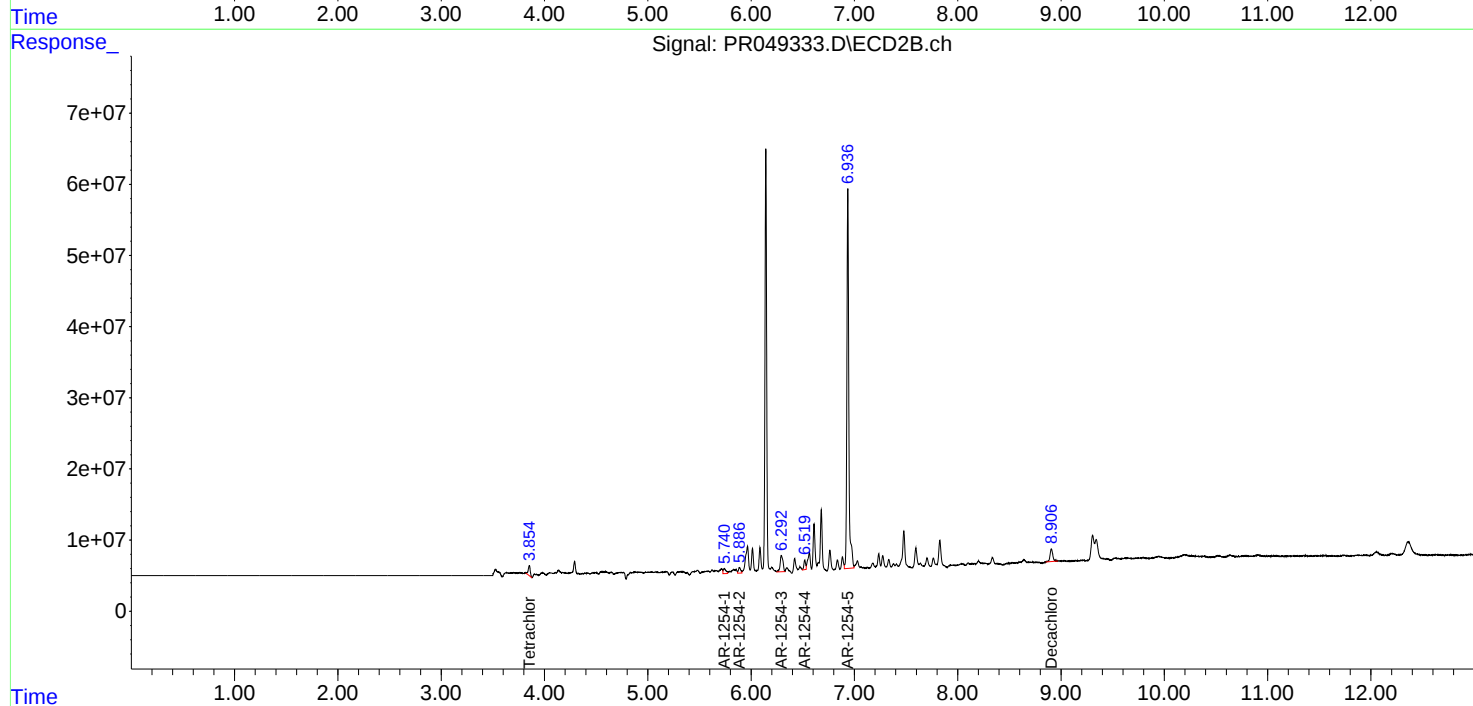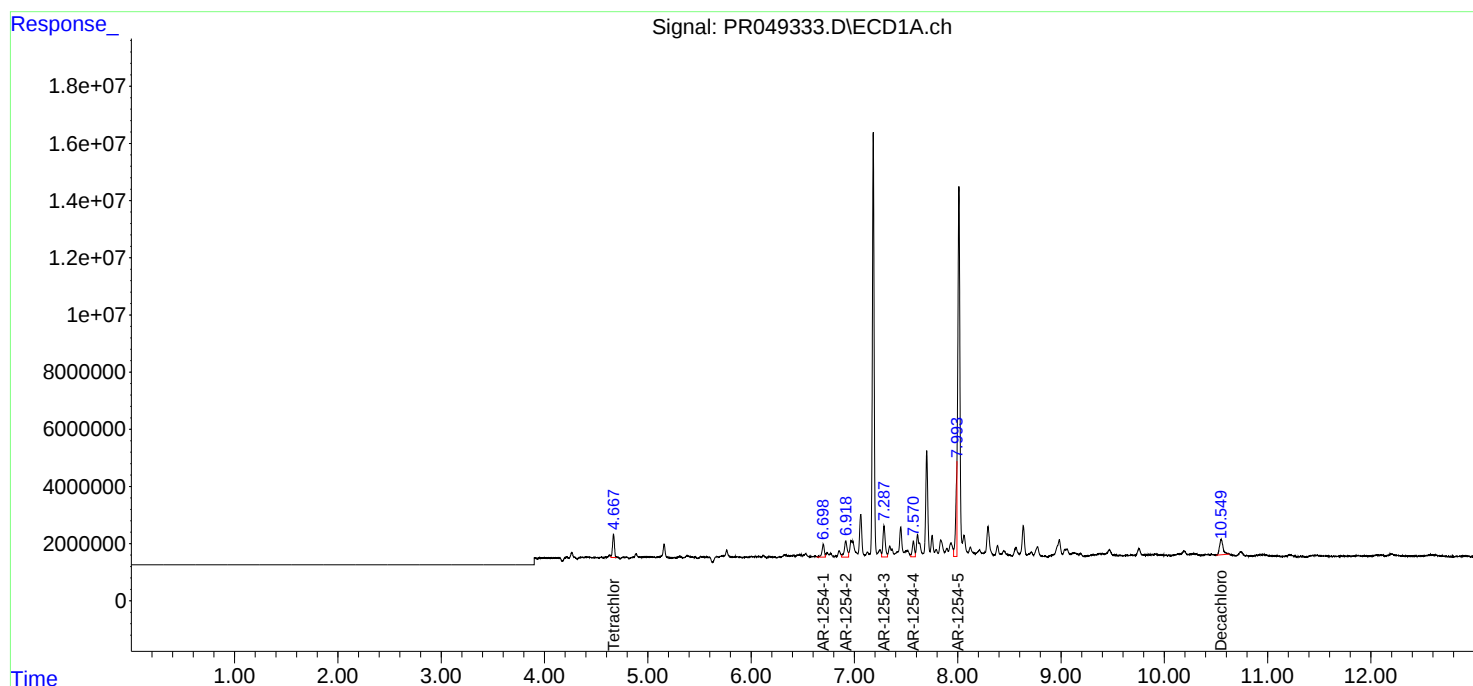

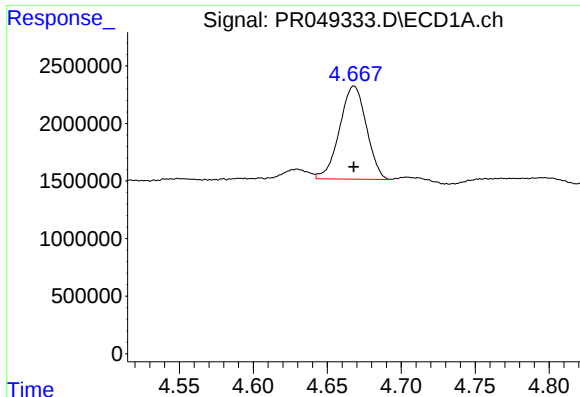


#1 Tetrachloro-m-xylene

R.T.: 4.667 min
Delta R.T.: 0.000 min
Response: 10212348
Conc: 4.30 ng/ml m

Instrument :
ECD_R
ClientSampleId :
263K-7ADL


Manual Integrations
APPROVED

Ankita
1/18/2021 10:18:17 AM

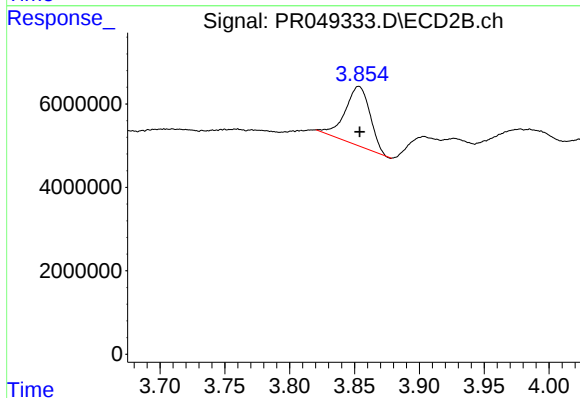


#1 Tetrachloro-m-xylene

R.T.: 3.853 min
Delta R.T.: 0.000 min
Response: 19048891
Conc: 7.05 ng/ml

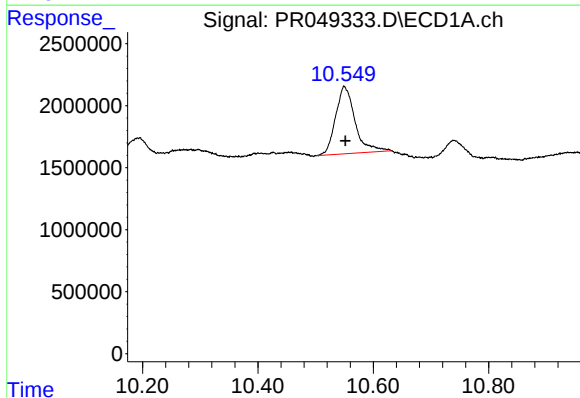


#2 Decachlorobiphenyl

R.T.: 10.550 min
Delta R.T.: -0.002 min
Response: 12731198
Conc: 5.08 ng/ml

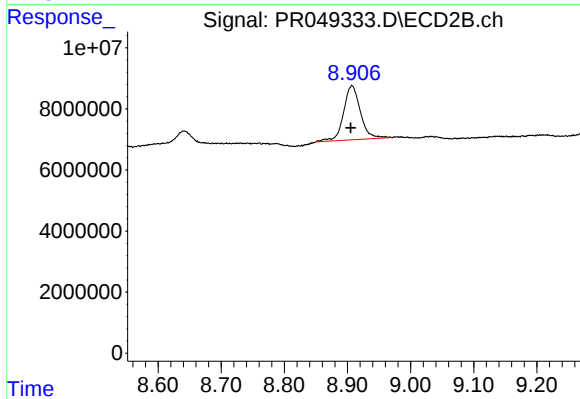

#2 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.002 min
Response: 32841212
Conc: 3.97 ng/ml

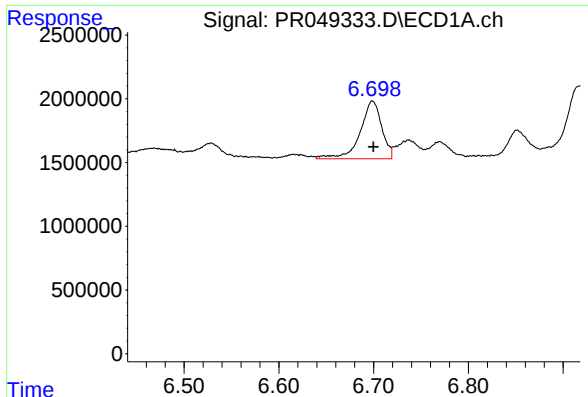


#26 AR-1254-1

R.T.: 6.699 min
Delta R.T.: 0.000 min
Response: 7177597
Conc: 74.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
263K-7ADL


Manual Integrations
APPROVED

Ankita
1/18/2021 10:18:17 AM

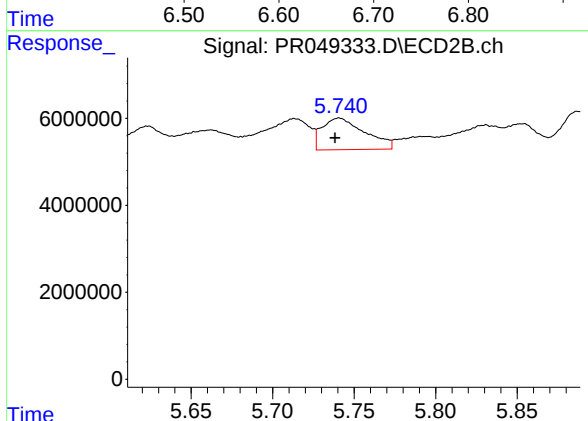


#26 AR-1254-1

R.T.: 5.741 min
Delta R.T.: 0.002 min
Response: 13332743
Conc: 134.10 ng/ml

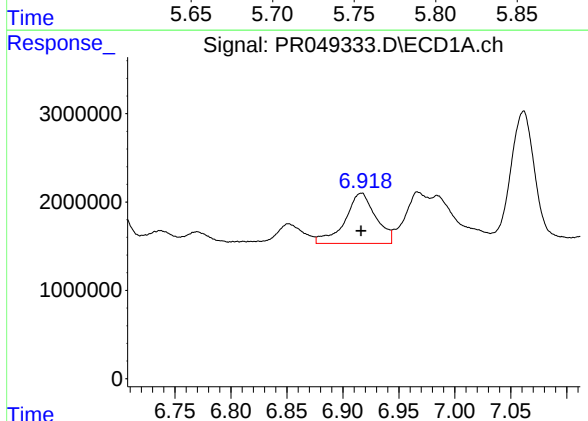


#27 AR-1254-2

R.T.: 6.917 min
Delta R.T.: 0.000 min
Response: 10891744
Conc: 74.26 ng/ml

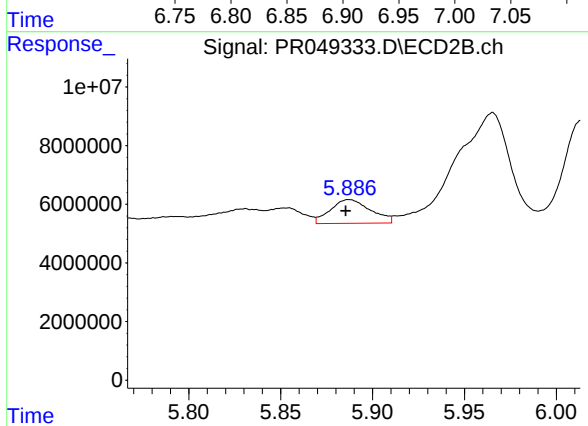

#27 AR-1254-2

R.T.: 5.887 min
Delta R.T.: 0.002 min
Response: 12324922
Conc: 114.14 ng/ml

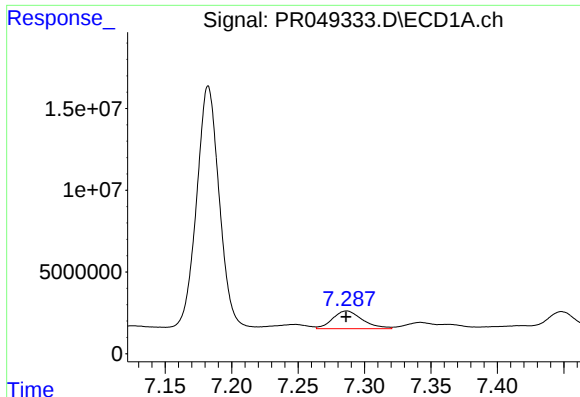


#28 AR-1254-3

R.T.: 7.287 min
Delta R.T.: 0.000 min
Response: 16929637
Conc: 112.72 ng/ml

Instrument :
ECD_R
ClientSampleId :
263K-7ADL


Manual Integrations
APPROVED

Ankita
1/18/2021 10:18:17 AM

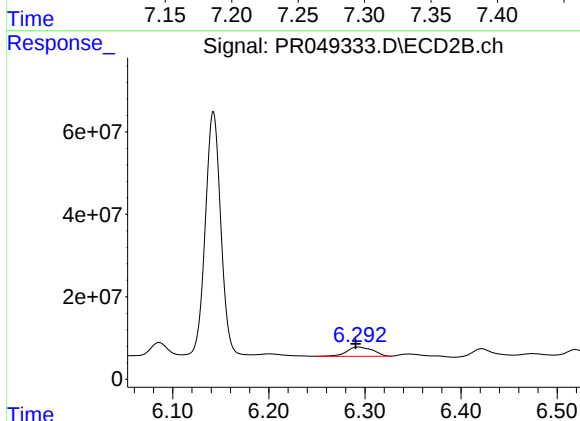


#28 AR-1254-3

R.T.: 6.292 min
Delta R.T.: 0.002 min
Response: 43393029
Conc: 205.42 ng/ml

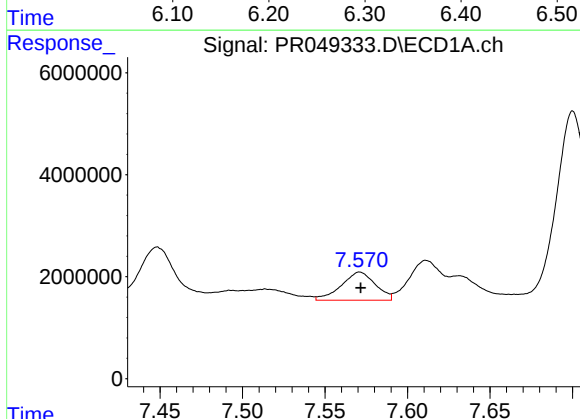


#29 AR-1254-4

R.T.: 7.571 min
Delta R.T.: 0.000 min
Response: 7960120
Conc: 65.45 ng/ml

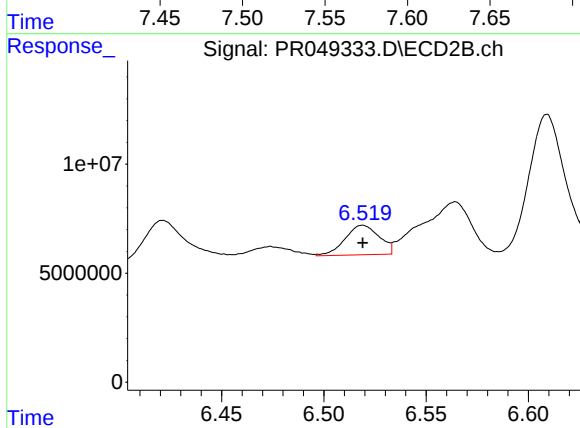

#29 AR-1254-4

R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 15773341
Conc: 46.69 ng/ml

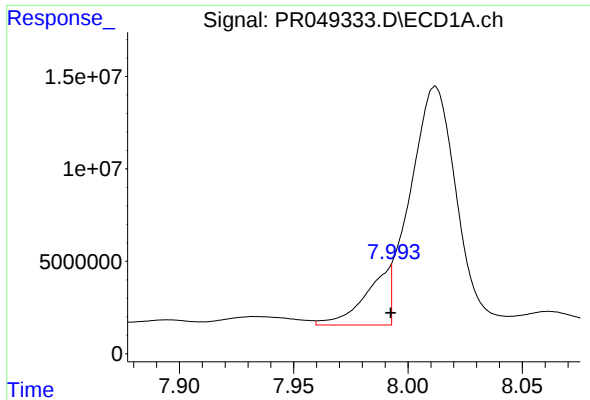


#30 AR-1254-5

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 25114662
Conc: 205.85 ng/ml m

Instrument :
ECD_R
ClientSampleId :
263K-7ADL

Manual Integrations
APPROVED

Ankita
1/18/2021 10:18:17 AM

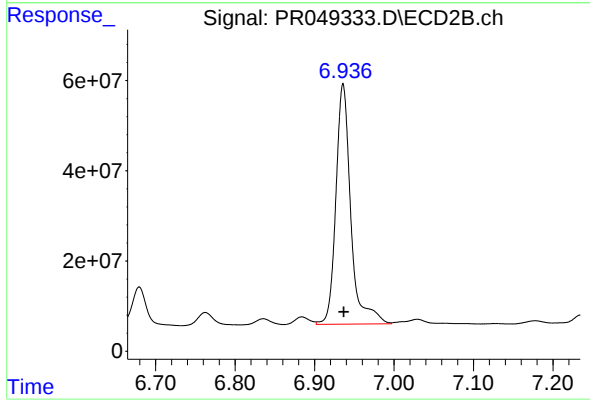

#30 AR-1254-5

R.T.: 6.936 min
Delta R.T.: 0.000 min
Response: 695814920
Conc: 1735.42 ng/ml