

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
 Data File : PR065276.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 18:36
 Operator : AJ\MA
 Sample : P1187-09
 Misc : AR1242 MDL 25 PPB
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:34:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.701	3.003	102.8E6	98985221	17.217	18.097
2) SA Decachlor...	9.740	8.373	73479219	88448356	18.372	18.689
Target Compounds						
3) L1 AR-1016-1	4.942	4.148	3220714	3403738	18.170	18.743
4) L1 AR-1016-2	4.964	4.167	4804720	4506936	18.430	18.229
5) L1 AR-1016-3	5.030	4.349	3410676	3975513	20.407	29.320 #
6) L1 AR-1016-4	5.134	4.402	2477399	2389073	18.476	22.813
7) L1 AR-1016-5	5.454	4.623	2746323	4573748	20.339	32.785 #
8) L2 AR-1221-1	3.919	3.221	941689	829616	13.120	13.397
9) L2 AR-1221-2	4.016	3.314	1911122	1579514	36.455	33.117
10) L2 AR-1221-3	4.095	3.401	2042065	2479088	13.291	17.947 #
11) L3 AR-1232-1	4.095	3.401	2042065	2479088	15.108	20.700 #
12) L3 AR-1232-2	4.652	4.167	3235097	4506936	41.993	36.890
13) L3 AR-1232-3	4.964	4.349	4804720	3975513	37.679	59.765 #
14) L3 AR-1232-4	5.134	4.444	2477399	3020868	37.796	52.757 #
15) L3 AR-1232-5	5.239	4.623	2252764	4573748	46.577	71.754 #
16) L4 AR-1242-1	4.942	4.148	3220714	3403738	22.530	23.291
17) L4 AR-1242-2	4.964	4.167	4804720	4506936	22.816	22.593
18) L4 AR-1242-3	5.030	4.349	3410676	3975513	25.184	36.307 #
19) L4 AR-1242-4	5.134	4.444	2477399	3020868	22.799	28.774 #
20) L4 AR-1242-5	5.934	5.005	2946038	4321333	26.044	32.005
21) L5 AR-1248-1	4.942	4.148	3220714	3403738	30.271	31.510
22) L5 AR-1248-2	5.239	4.402	2252764	2389073	14.498	16.496
23) L5 AR-1248-3	5.454	4.444	2746323	3020868	15.380	19.522 #
24) L5 AR-1248-4	5.892	4.623	2535682	4573748	13.375	24.423 #
25) L5 AR-1248-5	5.934	5.048	2946038	3907215	15.461	20.992 #
26) L6 AR-1254-1	5.865	5.005	2892531	4321333	14.123	14.830
27) L6 AR-1254-2	6.104	5.162	2406029	2149866	7.720	8.486
28) L6 AR-1254-3	6.500	5.600	1176976	1712929	3.679	4.187
29) L6 AR-1254-4	6.814	5.847	1065217	1051168	4.649	4.095
30) L6 AR-1254-5	7.272	6.300	651700	1190875	2.622	3.249
31) L7 AR-1260-1	0.000	5.741	0	1464780	N.D.	5.132 #
32) L7 AR-1260-2	6.971	5.950	261800	179099	0.911	0.516 #
33) L7 AR-1260-3	0.000	6.113	0	4430116	N.D.	13.636 #
34) L7 AR-1260-4	7.605	6.633	832690	293920	3.529	1.113 #
35) L7 AR-1260-5	7.961	6.912f	688332	100443	1.566	0.163 #
36) L8 AR-1262-1	0.000	6.402	0	334584	N.D.	1.865 #
37) L8 AR-1262-2	7.961	6.633	688332	293920	1.217	0.755 #
38) L8 AR-1262-3	8.277	7.219	188689	186422	0.496	0.658 #
39) L8 AR-1262-4	0.000	7.270	0	1711937	N.D.	2.973 #
40) L8 AR-1262-5	0.000	7.813	0	413009	N.D.	1.587 #
41) L9 AR-1268-1	8.277	7.219	188689	186422	0.311	0.235

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
 Data File : PR065276.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 18:36
 Operator : AJ\MA
 Sample : P1187-09
 Misc : AR1242 MDL 25 PPB
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:34:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.270	0	1711937	N.D.	2.300 #
43) L9	AR-1268-3	8.590	7.513	544172	1417713	1.147	2.238 #
44) L9	AR-1268-4	0.000	7.813	0	413009	N.D.	1.575 #
45) L9	AR-1268-5	9.414	8.120	493533	1820594	0.339	0.951 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
Data File : PR065276.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 18:36
Operator : AJ\MA
Sample : P1187-09
Misc : AR1242 MDL 25 PPB
ALS Vial : 67 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:34:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

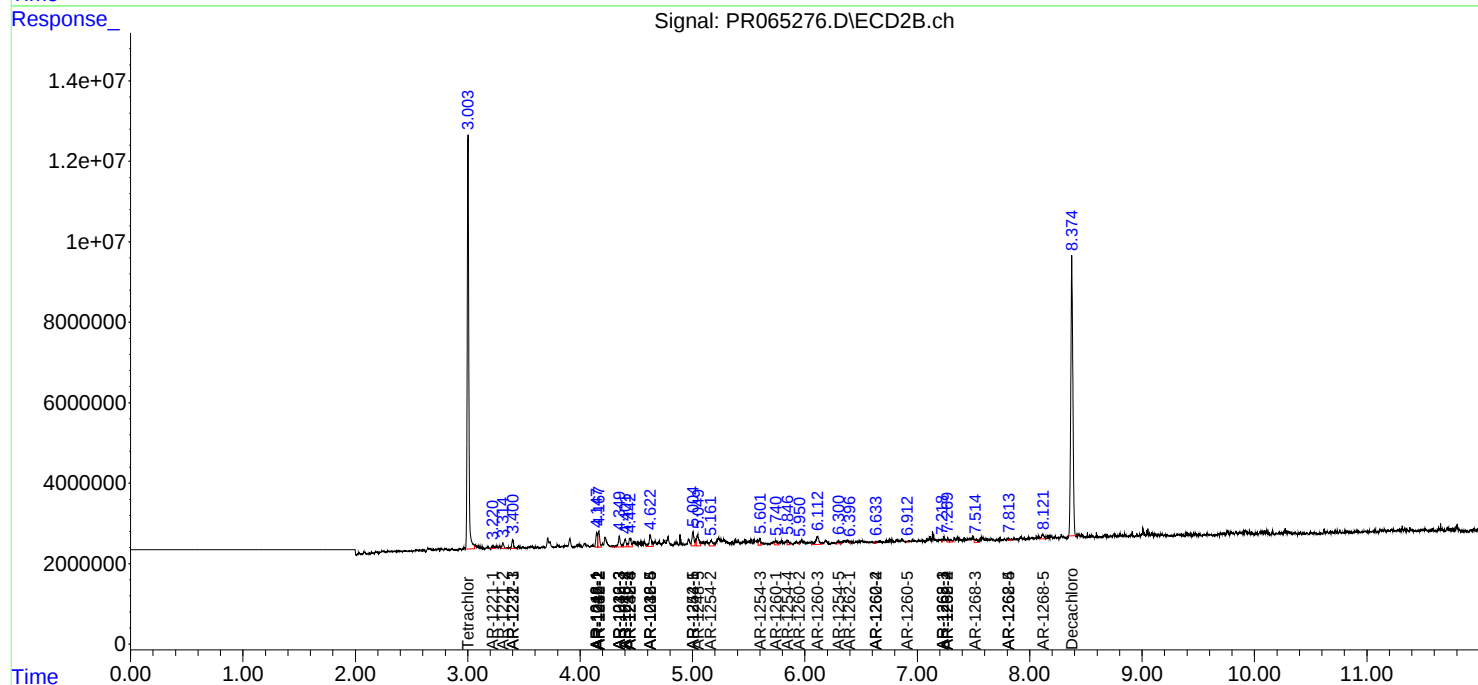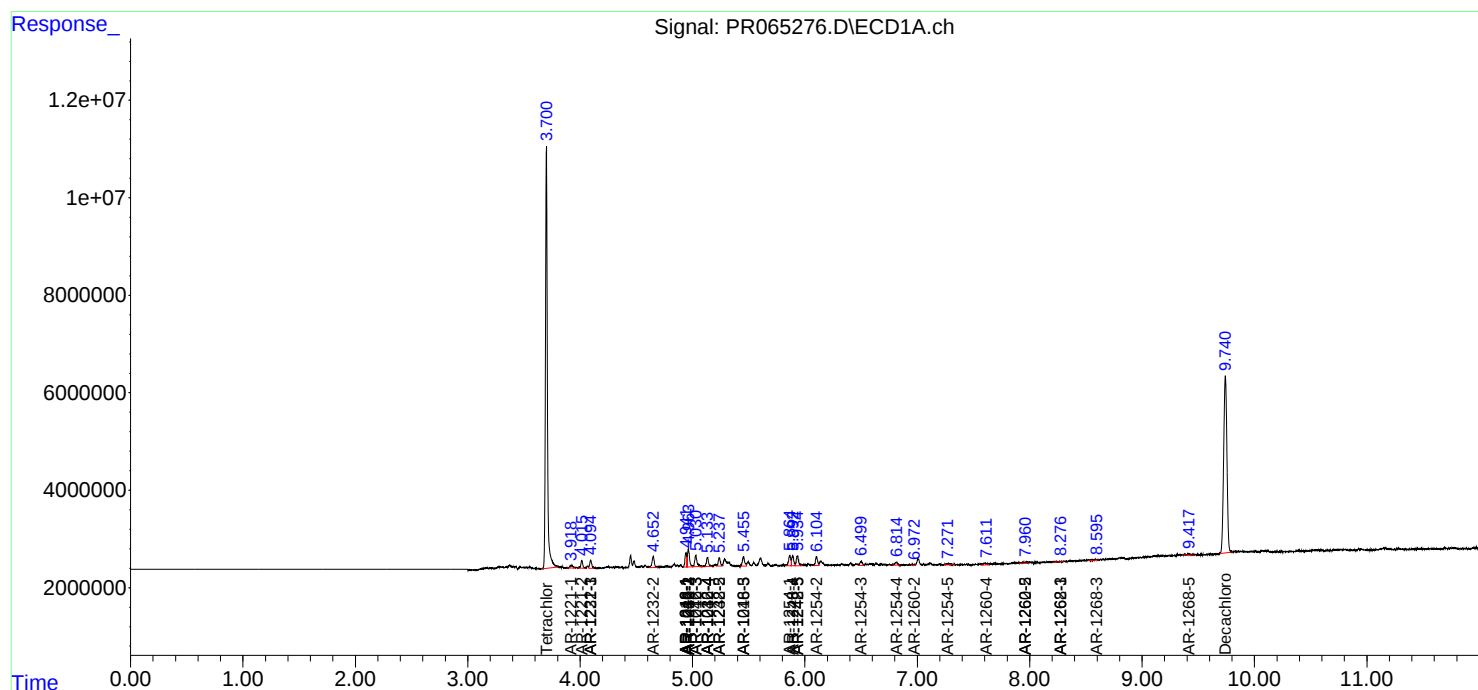


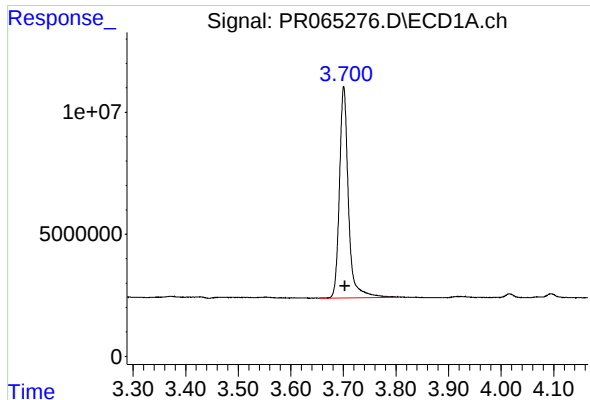

#1 Tetrachloro-m-xylene


R.T.: 3.701 min
Delta R.T.: -0.002 min
Response: 102771861
Conc: 17.22 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

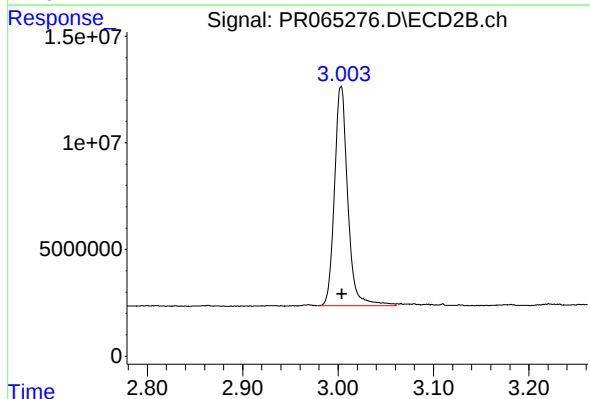


#1 Tetrachloro-m-xylene

R.T.: 3.003 min
Delta R.T.: -0.001 min
Response: 98985221
Conc: 18.10 ng/ml

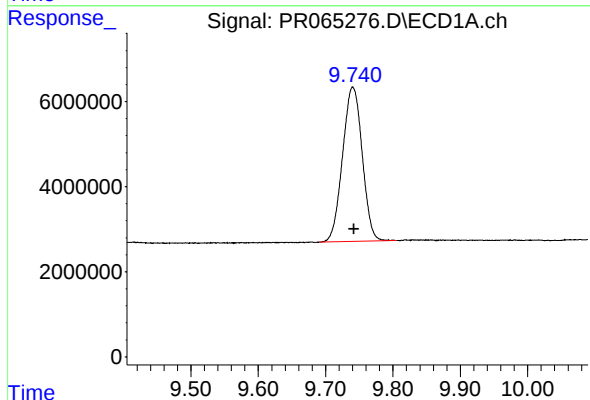


#2 Decachlorobiphenyl

R.T.: 9.740 min
Delta R.T.: -0.002 min
Response: 73479219
Conc: 18.37 ng/ml

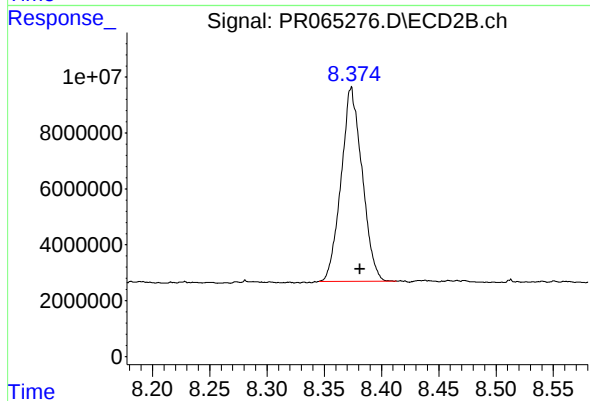

#2 Decachlorobiphenyl


R.T.: 8.373 min
Delta R.T.: -0.008 min
Response: 88448356
Conc: 18.69 ng/ml

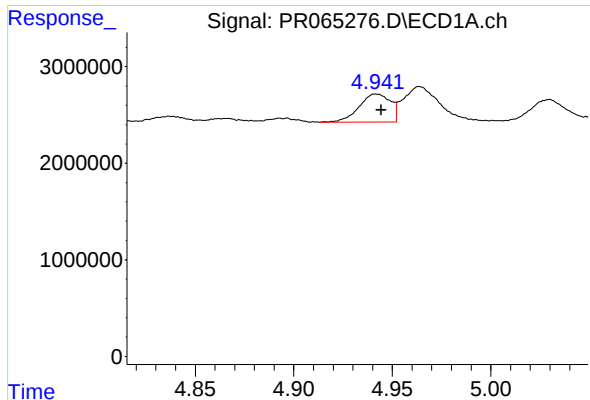

#3 AR-1016-1


R.T.: 4.942 min
Delta R.T.: -0.002 min
Response: 3220714
Conc: 18.17 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

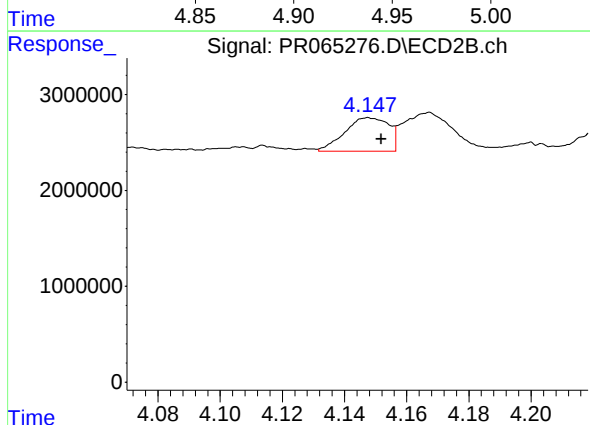


#3 AR-1016-1

R.T.: 4.148 min
Delta R.T.: -0.004 min
Response: 3403738
Conc: 18.74 ng/ml

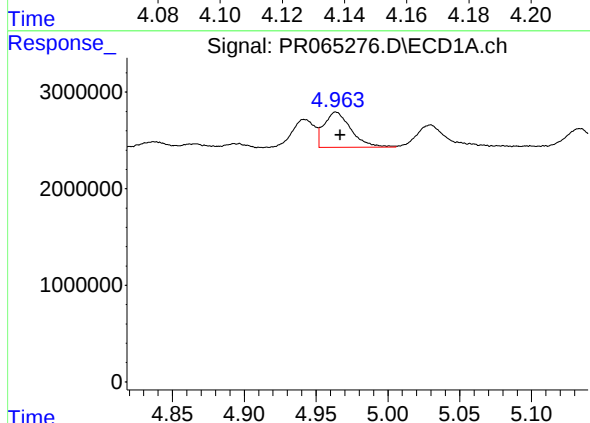


#4 AR-1016-2

R.T.: 4.964 min
Delta R.T.: -0.003 min
Response: 4804720
Conc: 18.43 ng/ml

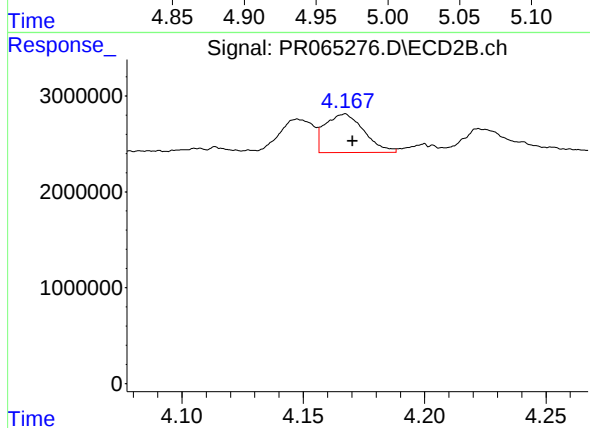

#4 AR-1016-2


R.T.: 4.167 min
Delta R.T.: -0.003 min
Response: 4506936
Conc: 18.23 ng/ml

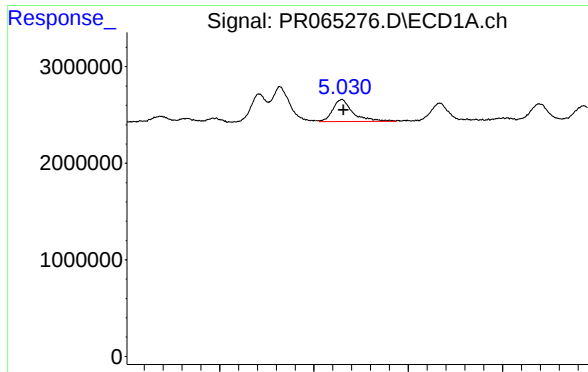

#5 AR-1016-3


R.T.: 5.030 min
Delta R.T.: -0.002 min
Response: 3410676
Conc: 20.41 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

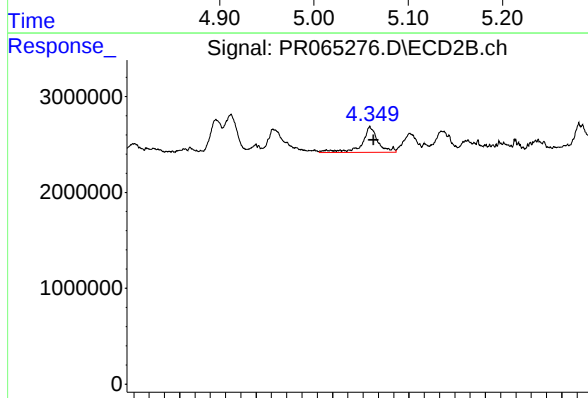


#5 AR-1016-3

R.T.: 4.349 min
Delta R.T.: -0.004 min
Response: 3975513
Conc: 29.32 ng/ml

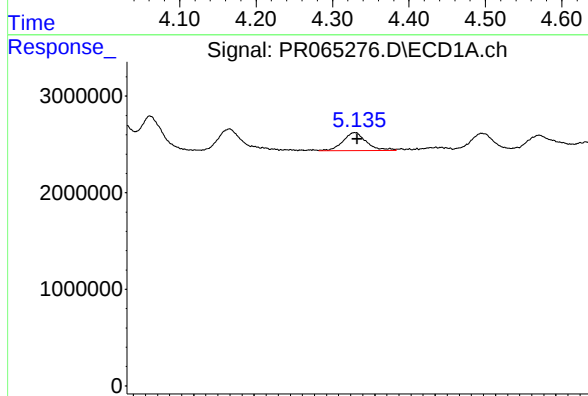


#6 AR-1016-4

R.T.: 5.134 min
Delta R.T.: -0.002 min
Response: 2477399
Conc: 18.48 ng/ml

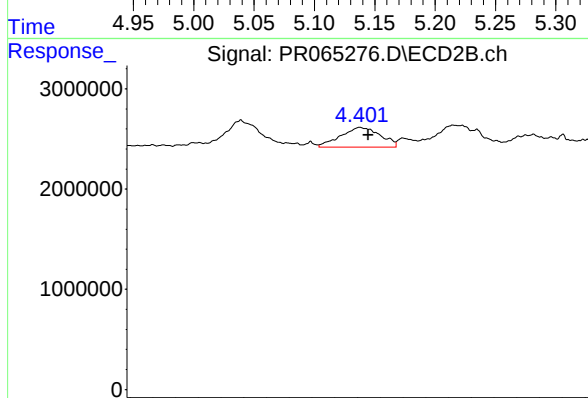

#6 AR-1016-4


R.T.: 4.402 min
Delta R.T.: -0.003 min
Response: 2389073
Conc: 22.81 ng/ml

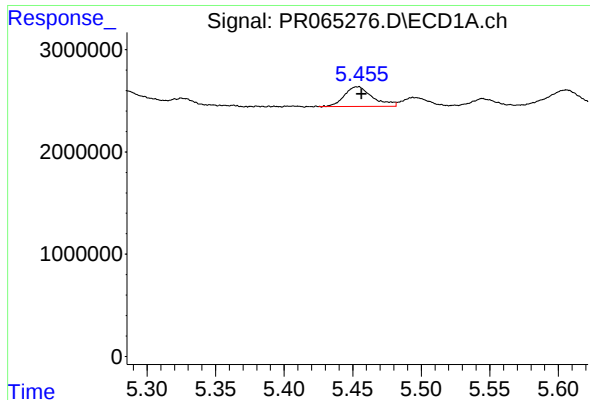

#7 AR-1016-5


R.T.: 5.454 min
Delta R.T.: -0.003 min
Response: 2746323
Conc: 20.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

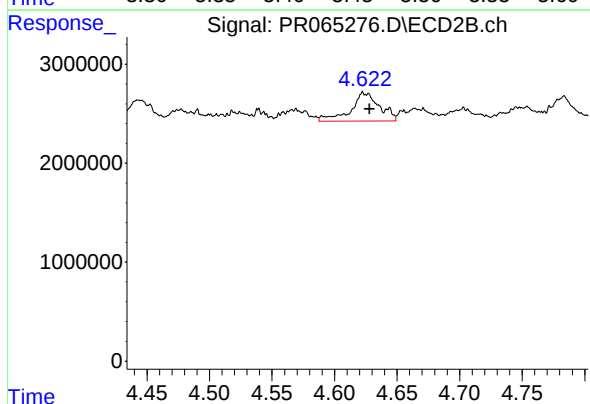


#7 AR-1016-5

R.T.: 4.623 min
Delta R.T.: -0.005 min
Response: 4573748
Conc: 32.78 ng/ml

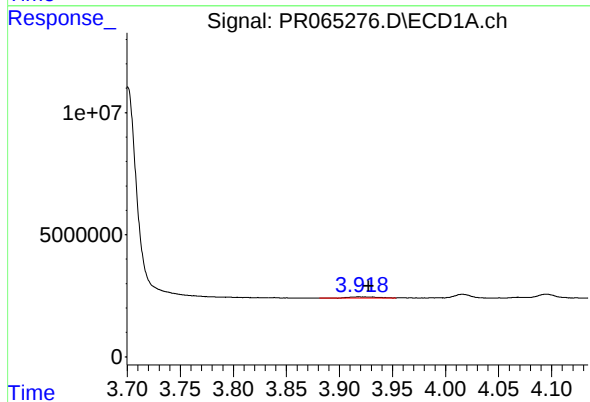


#8 AR-1221-1

R.T.: 3.919 min
Delta R.T.: -0.009 min
Response: 941689
Conc: 13.12 ng/ml

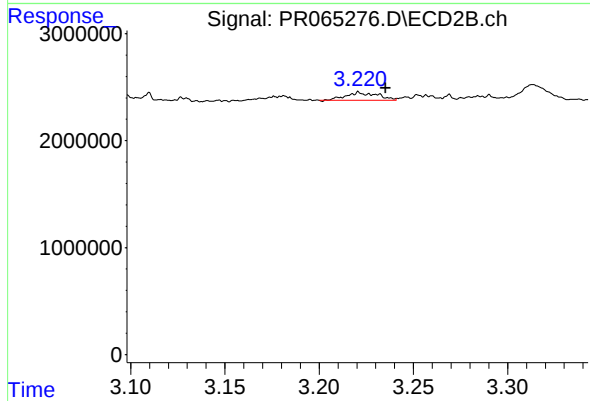

#8 AR-1221-1


R.T.: 3.221 min
Delta R.T.: -0.014 min
Response: 829616
Conc: 13.40 ng/ml

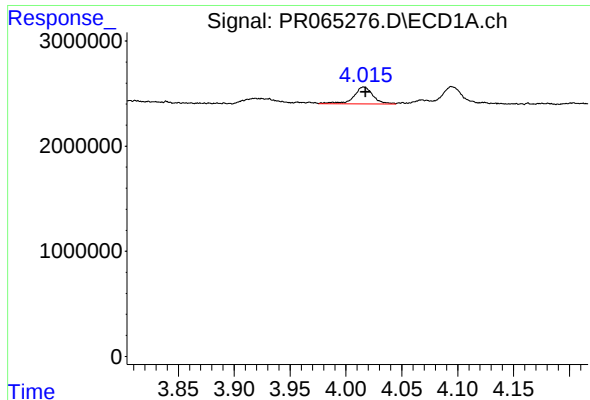

#9 AR-1221-2


R.T.: 4.016 min
Delta R.T.: -0.001 min
Response: 1911122
Conc: 36.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

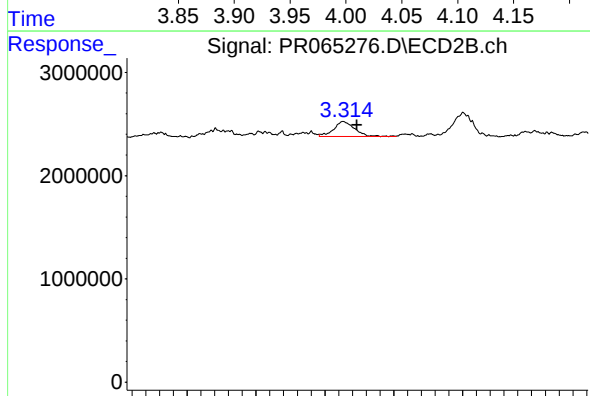


#9 AR-1221-2

R.T.: 3.314 min
Delta R.T.: -0.010 min
Response: 1579514
Conc: 33.12 ng/ml

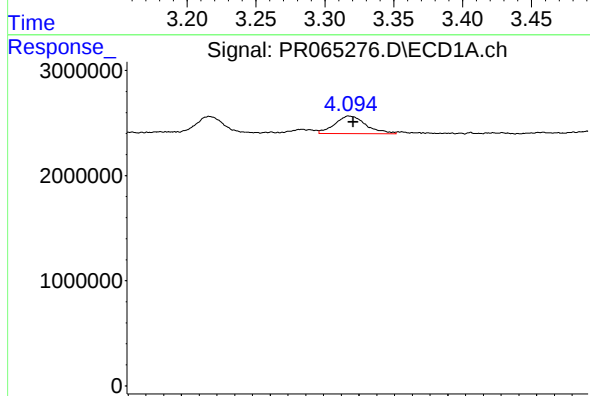


#10 AR-1221-3

R.T.: 4.095 min
Delta R.T.: -0.002 min
Response: 2042065
Conc: 13.29 ng/ml

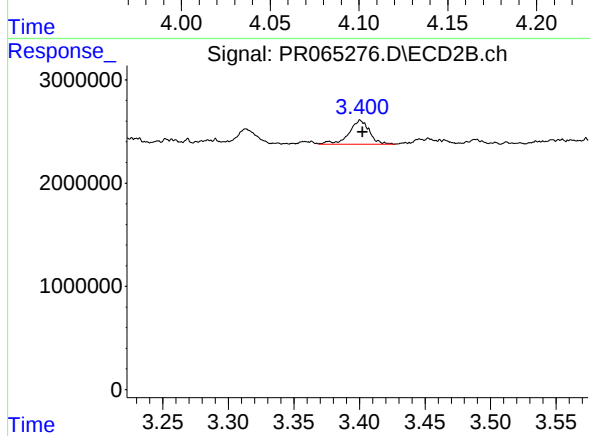

#10 AR-1221-3


R.T.: 3.401 min
Delta R.T.: -0.002 min
Response: 2479088
Conc: 17.95 ng/ml

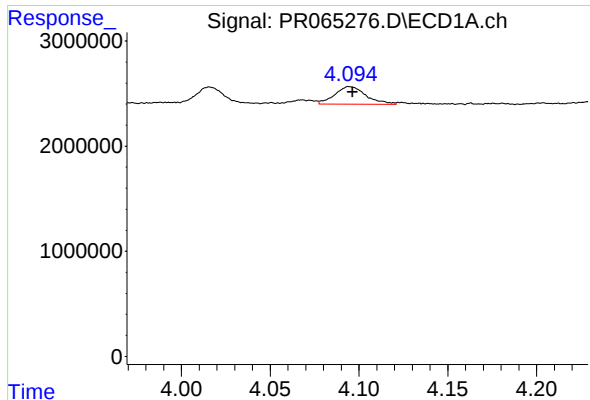

#11 AR-1232-1


R.T.: 4.095 min
Delta R.T.: -0.002 min
Response: 2042065
Conc: 15.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

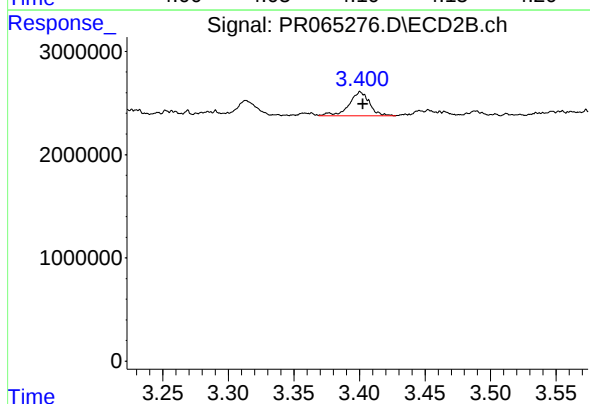


#11 AR-1232-1

R.T.: 3.401 min
Delta R.T.: -0.002 min
Response: 2479088
Conc: 20.70 ng/ml

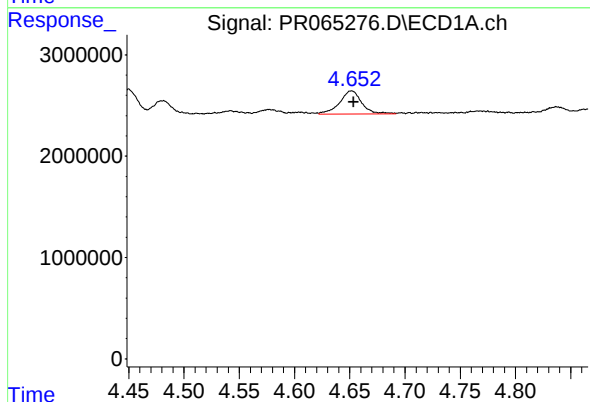


#12 AR-1232-2

R.T.: 4.652 min
Delta R.T.: -0.002 min
Response: 3235097
Conc: 41.99 ng/ml

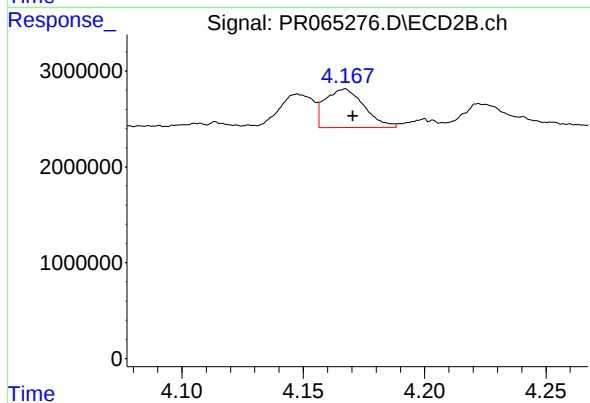

#12 AR-1232-2


R.T.: 4.167 min
Delta R.T.: -0.004 min
Response: 4506936
Conc: 36.89 ng/ml

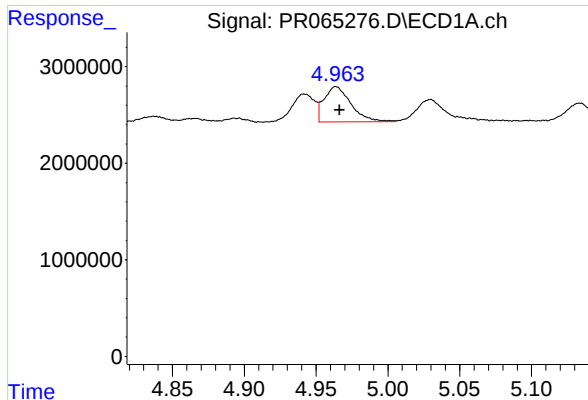

#13 AR-1232-3


R.T.: 4.964 min
Delta R.T.: -0.002 min
Response: 4804720
Conc: 37.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

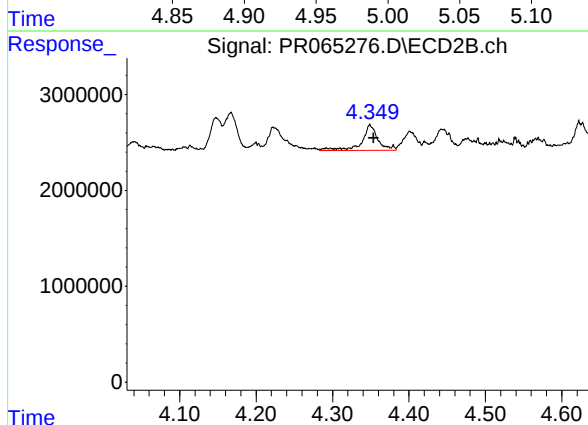


#13 AR-1232-3

R.T.: 4.349 min
Delta R.T.: -0.005 min
Response: 3975513
Conc: 59.77 ng/ml

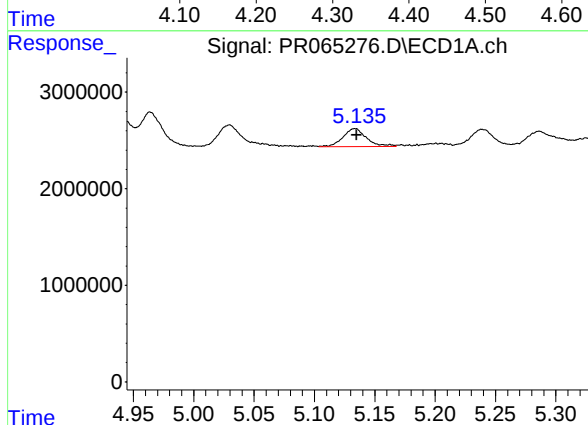


#14 AR-1232-4

R.T.: 5.134 min
Delta R.T.: -0.001 min
Response: 2477399
Conc: 37.80 ng/ml

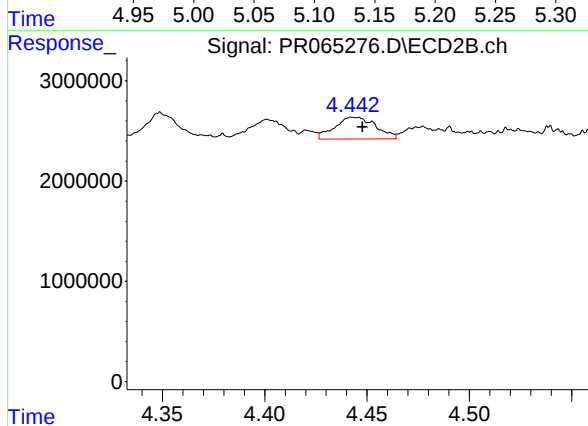

#14 AR-1232-4


R.T.: 4.444 min
Delta R.T.: -0.004 min
Response: 3020868
Conc: 52.76 ng/ml

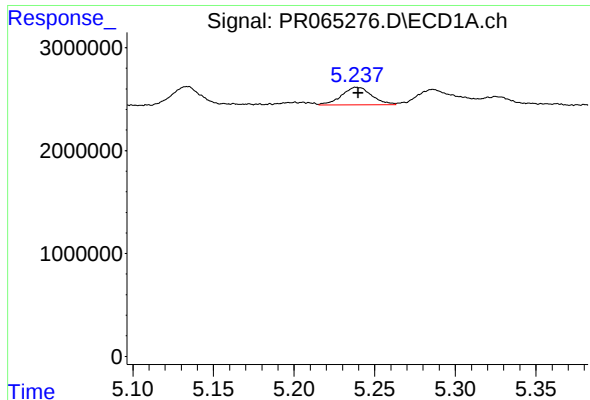

#15 AR-1232-5


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 2252764
Conc: 46.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

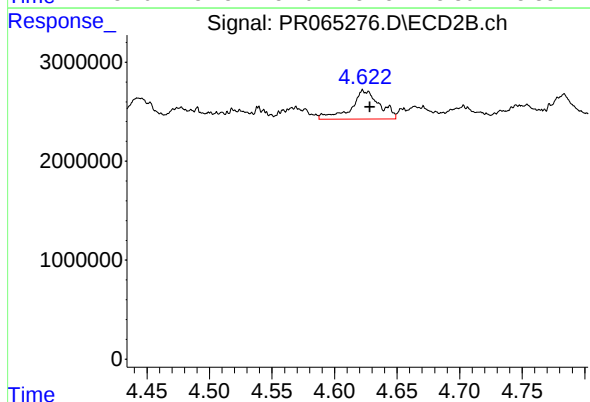


#15 AR-1232-5

R.T.: 4.623 min
Delta R.T.: -0.005 min
Response: 4573748
Conc: 71.75 ng/ml

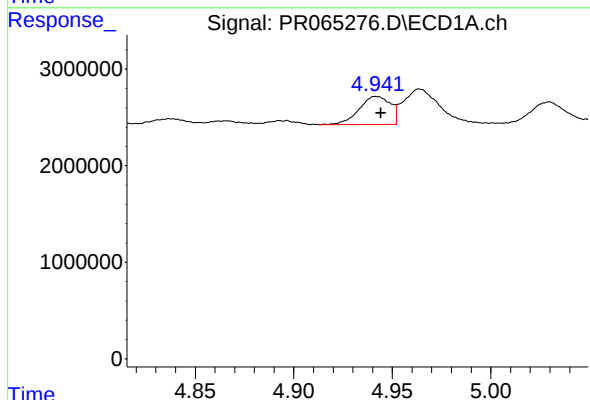


#16 AR-1242-1

R.T.: 4.942 min
Delta R.T.: -0.002 min
Response: 3220714
Conc: 22.53 ng/ml

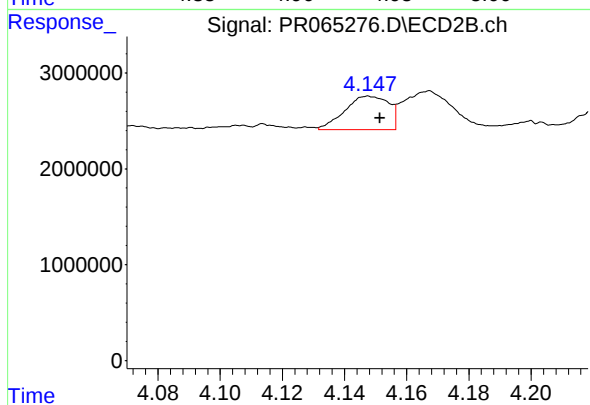

#16 AR-1242-1


R.T.: 4.148 min
Delta R.T.: -0.004 min
Response: 3403738
Conc: 23.29 ng/ml

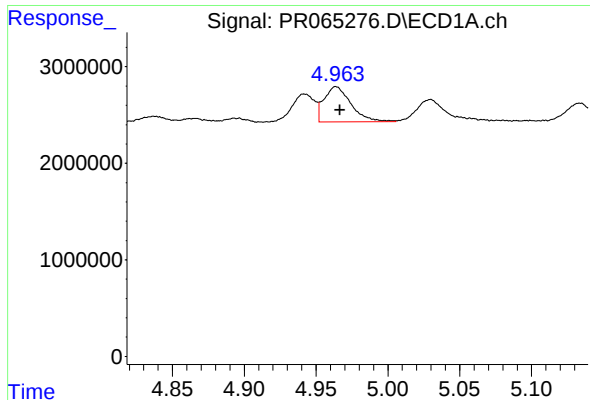

#17 AR-1242-2


R.T.: 4.964 min
Delta R.T.: -0.003 min
Response: 4804720
Conc: 22.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

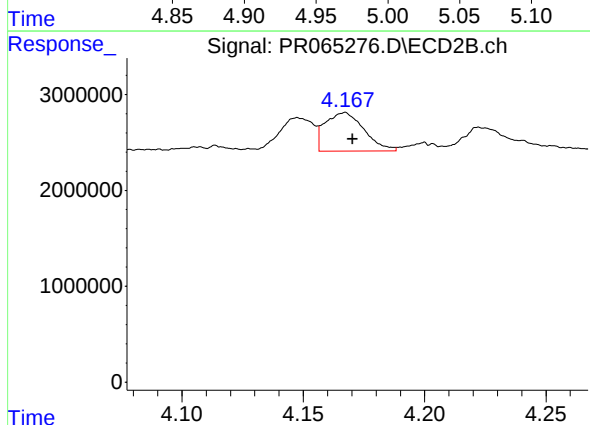


#17 AR-1242-2

R.T.: 4.167 min
Delta R.T.: -0.003 min
Response: 4506936
Conc: 22.59 ng/ml

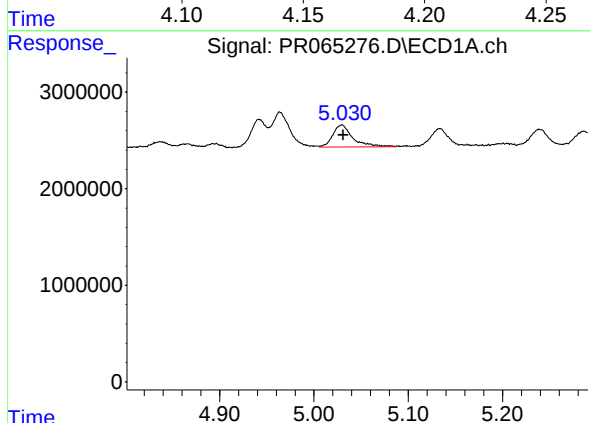


#18 AR-1242-3

R.T.: 5.030 min
Delta R.T.: -0.002 min
Response: 3410676
Conc: 25.18 ng/ml

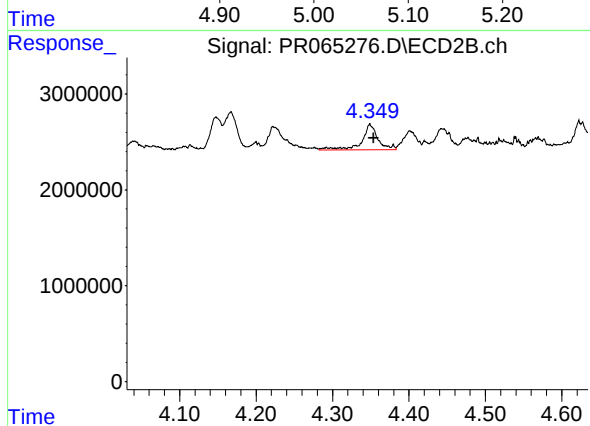

#18 AR-1242-3


R.T.: 4.349 min
Delta R.T.: -0.005 min
Response: 3975513
Conc: 36.31 ng/ml

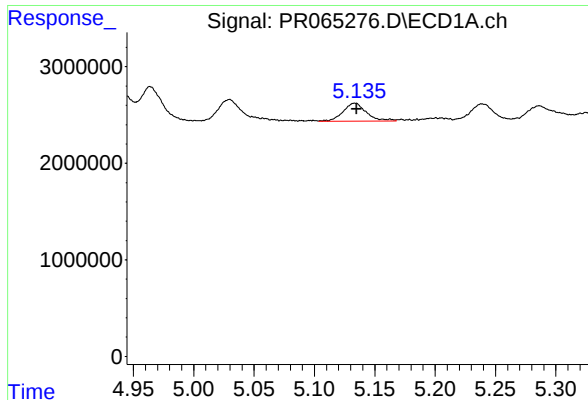

#19 AR-1242-4


R.T.: 5.134 min
Delta R.T.: -0.001 min
Response: 2477399
Conc: 22.80 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

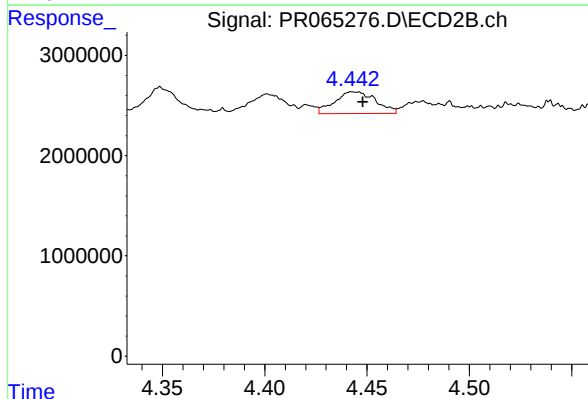


#19 AR-1242-4

R.T.: 4.444 min
Delta R.T.: -0.005 min
Response: 3020868
Conc: 28.77 ng/ml

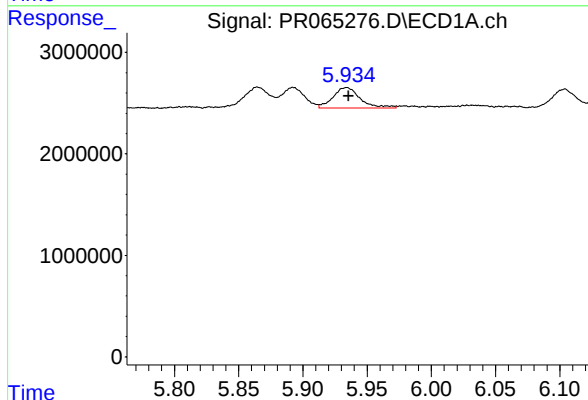


#20 AR-1242-5

R.T.: 5.934 min
Delta R.T.: -0.002 min
Response: 2946038
Conc: 26.04 ng/ml

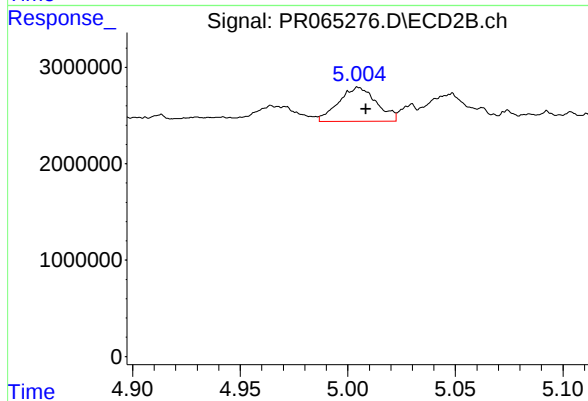

#20 AR-1242-5


R.T.: 5.005 min
Delta R.T.: -0.003 min
Response: 4321333
Conc: 32.00 ng/ml

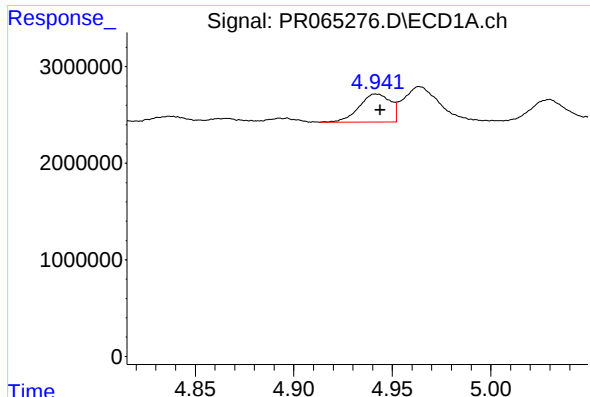

#21 AR-1248-1


R.T.: 4.942 min
Delta R.T.: -0.002 min
Response: 3220714
Conc: 30.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

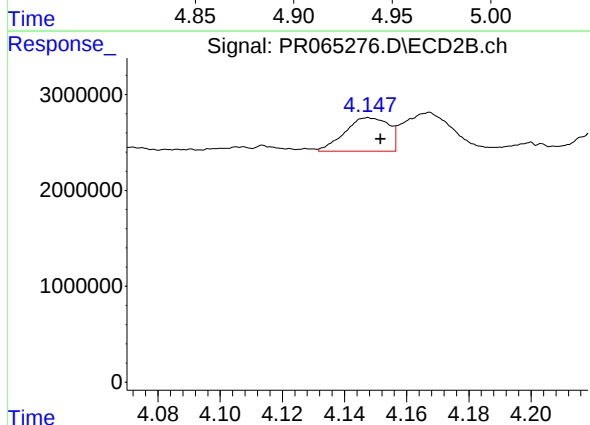


#21 AR-1248-1

R.T.: 4.148 min
Delta R.T.: -0.004 min
Response: 3403738
Conc: 31.51 ng/ml

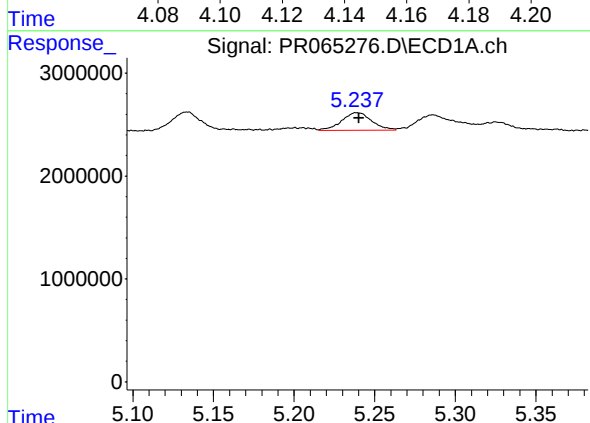


#22 AR-1248-2

R.T.: 5.239 min
Delta R.T.: -0.001 min
Response: 2252764
Conc: 14.50 ng/ml

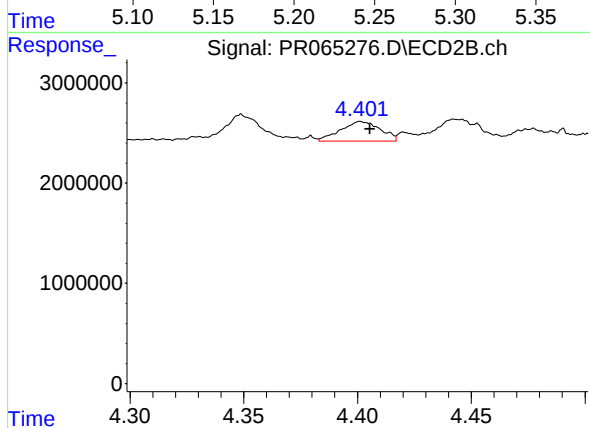

#22 AR-1248-2


R.T.: 4.402 min
Delta R.T.: -0.004 min
Response: 2389073
Conc: 16.50 ng/ml

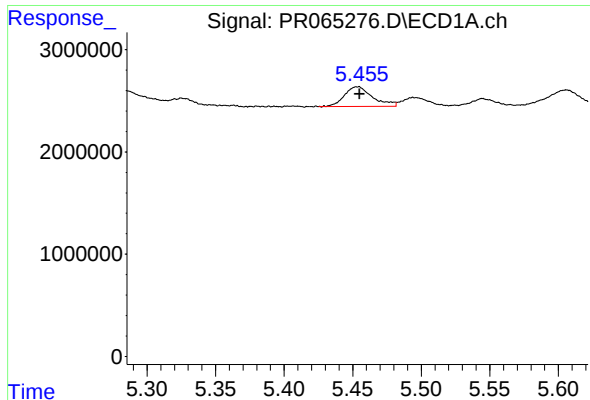

#23 AR-1248-3


R.T.: 5.454 min
Delta R.T.: -0.002 min
Response: 2746323
Conc: 15.38 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

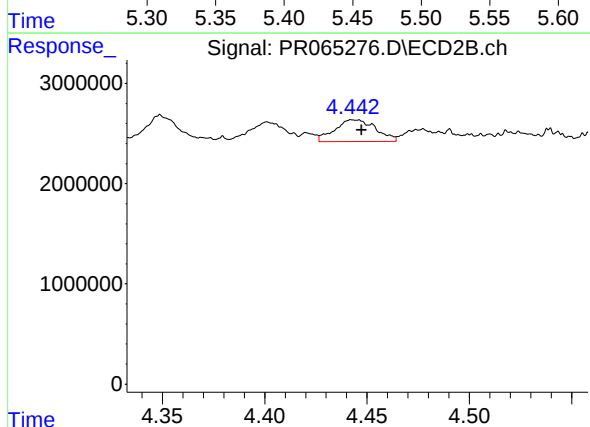


#23 AR-1248-3

R.T.: 4.444 min
Delta R.T.: -0.004 min
Response: 3020868
Conc: 19.52 ng/ml

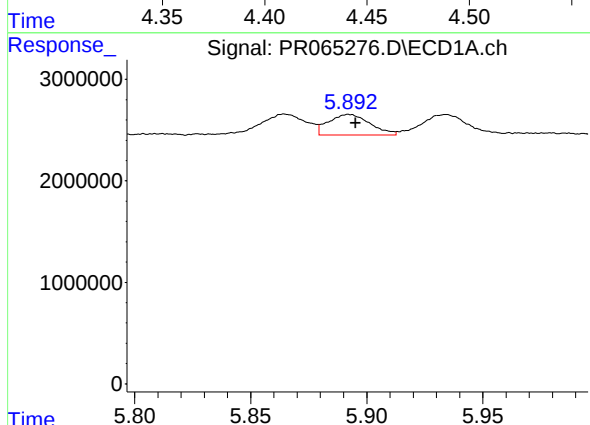


#24 AR-1248-4

R.T.: 5.892 min
Delta R.T.: -0.003 min
Response: 2535682
Conc: 13.37 ng/ml

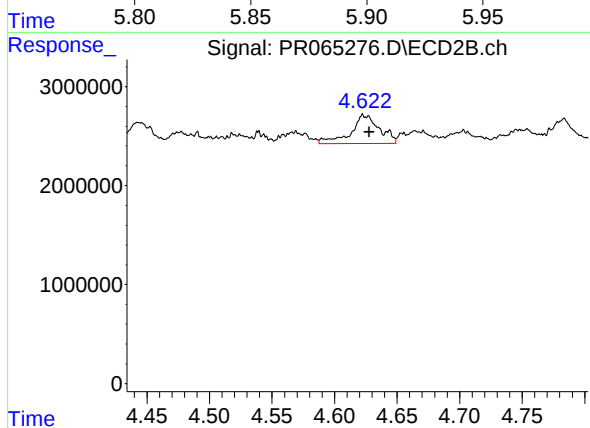

#24 AR-1248-4


R.T.: 4.623 min
Delta R.T.: -0.005 min
Response: 4573748
Conc: 24.42 ng/ml

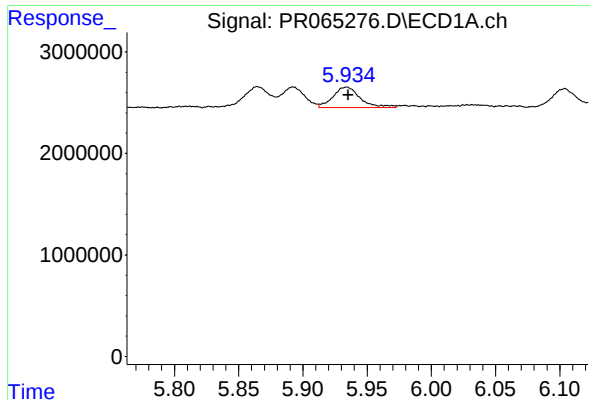

#25 AR-1248-5


R.T.: 5.934 min
Delta R.T.: -0.001 min
Response: 2946038
Conc: 15.46 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

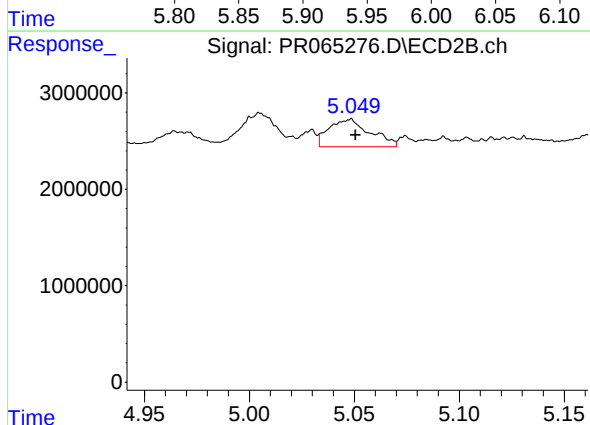


#25 AR-1248-5

R.T.: 5.048 min
Delta R.T.: -0.003 min
Response: 3907215
Conc: 20.99 ng/ml

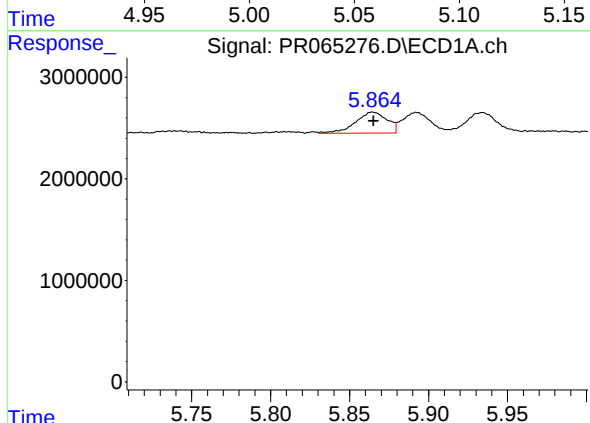


#26 AR-1254-1

R.T.: 5.865 min
Delta R.T.: 0.000 min
Response: 2892531
Conc: 14.12 ng/ml

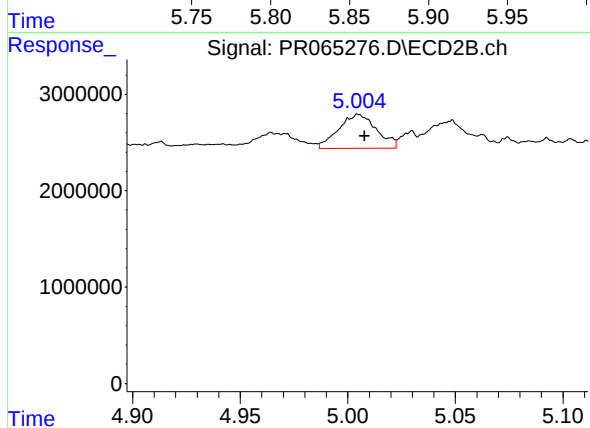

#26 AR-1254-1


R.T.: 5.005 min
Delta R.T.: -0.003 min
Response: 4321333
Conc: 14.83 ng/ml

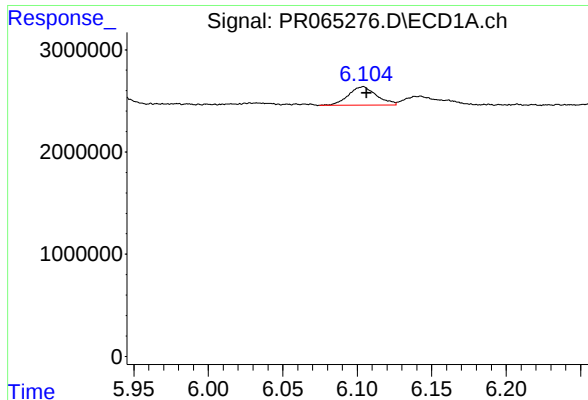

#27 AR-1254-2


R.T.: 6.104 min
Delta R.T.: -0.003 min
Response: 2406029
Conc: 7.72 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

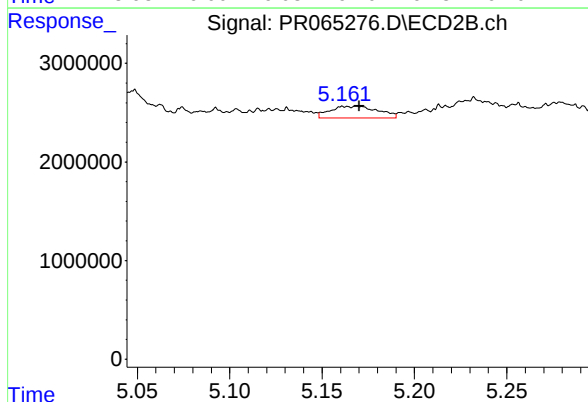


#27 AR-1254-2

R.T.: 5.162 min
Delta R.T.: -0.008 min
Response: 2149866
Conc: 8.49 ng/ml

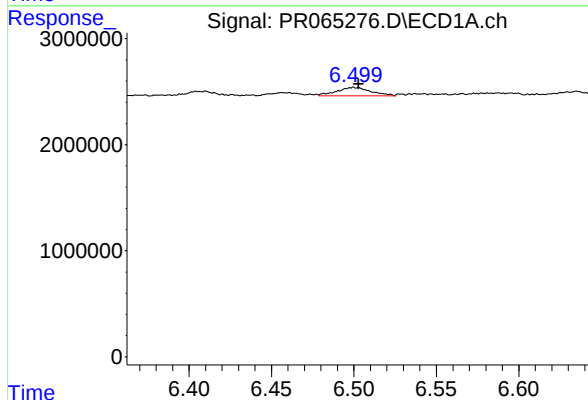


#28 AR-1254-3

R.T.: 6.500 min
Delta R.T.: -0.003 min
Response: 1176976
Conc: 3.68 ng/ml

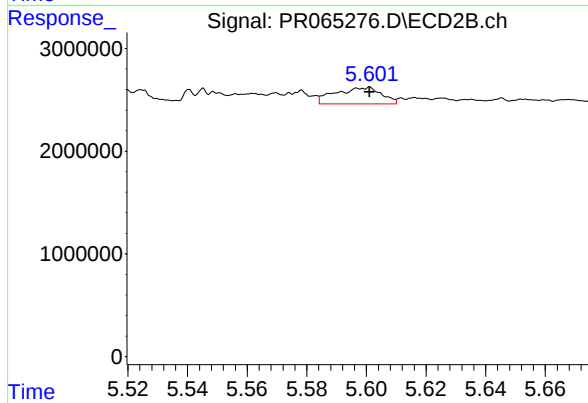

#28 AR-1254-3


R.T.: 5.600 min
Delta R.T.: 0.000 min
Response: 1712929
Conc: 4.19 ng/ml

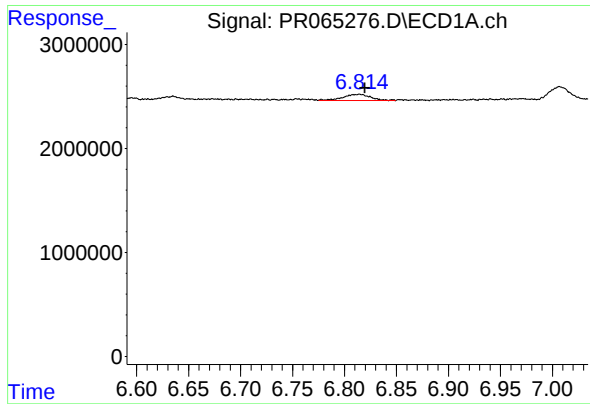

#29 AR-1254-4


R.T.: 6.814 min
Delta R.T.: -0.005 min
Response: 1065217
Conc: 4.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

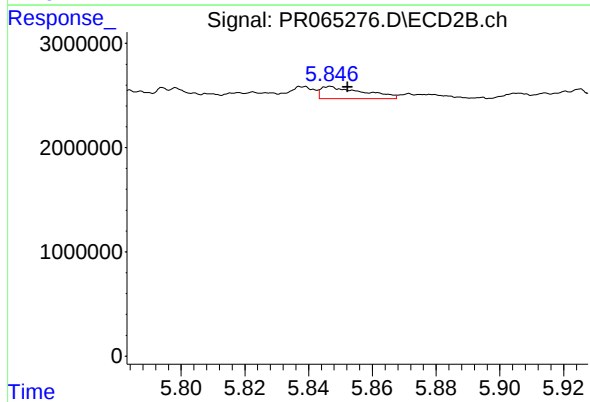


#29 AR-1254-4

R.T.: 5.847 min
Delta R.T.: -0.005 min
Response: 1051168
Conc: 4.09 ng/ml

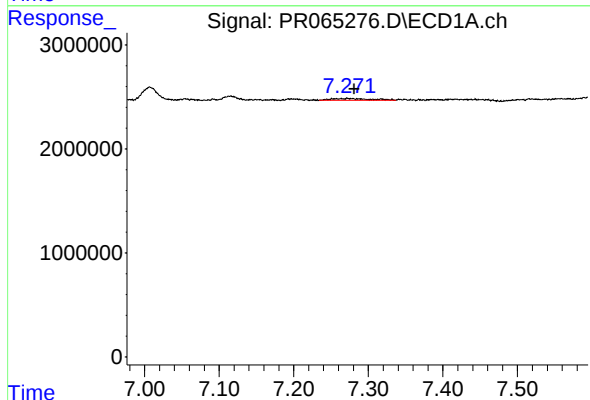


#30 AR-1254-5

R.T.: 7.272 min
Delta R.T.: -0.009 min
Response: 651700
Conc: 2.62 ng/ml

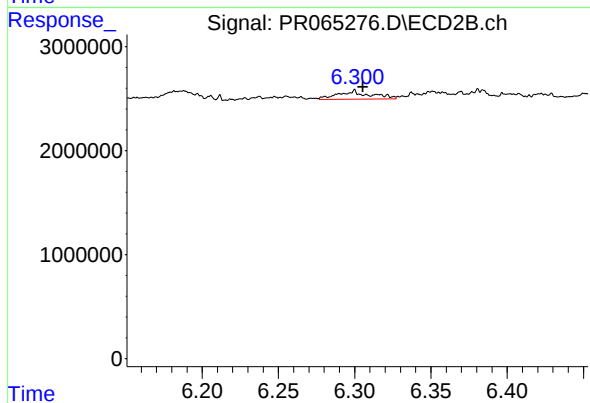

#30 AR-1254-5


R.T.: 6.300 min
Delta R.T.: -0.006 min
Response: 1190875
Conc: 3.25 ng/ml

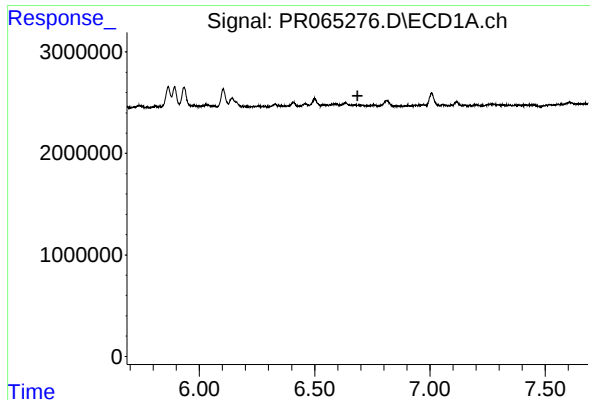

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 6.686 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

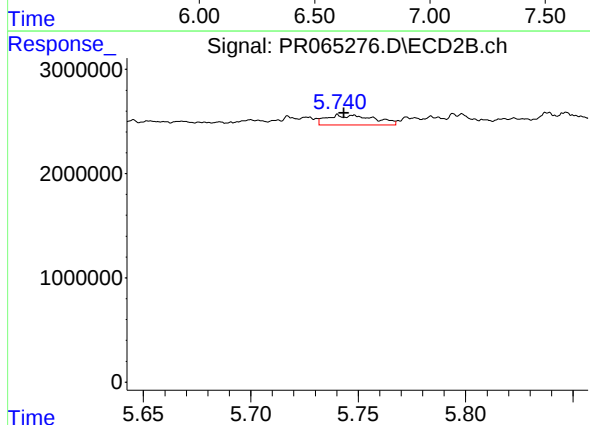


#31 AR-1260-1

R.T.: 5.741 min
Delta R.T.: -0.003 min
Response: 1464780
Conc: 5.13 ng/ml

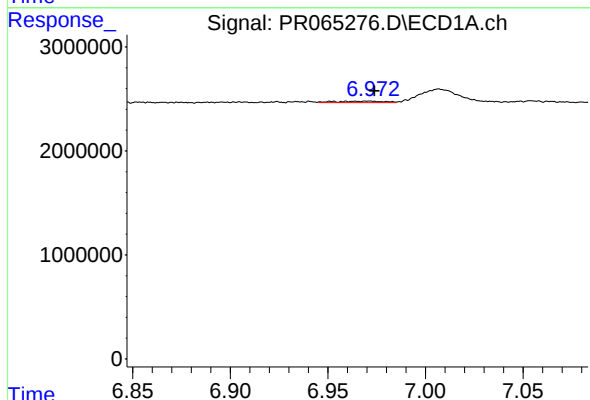


#32 AR-1260-2

R.T.: 6.971 min
Delta R.T.: -0.003 min
Response: 261800
Conc: 0.91 ng/ml

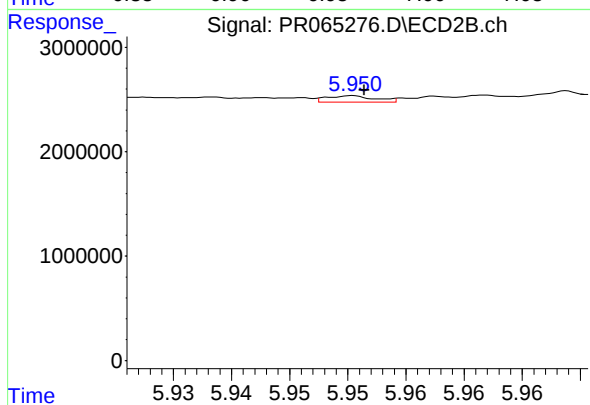

#32 AR-1260-2


R.T.: 5.950 min
Delta R.T.: -0.001 min
Response: 179099
Conc: 0.52 ng/ml

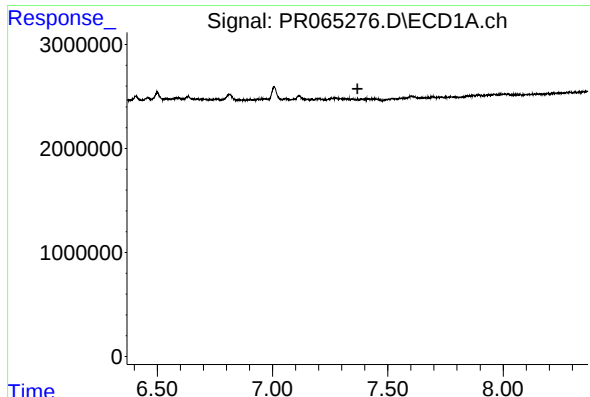

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

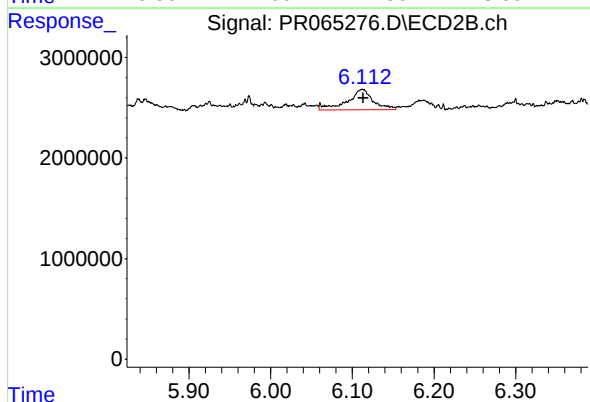


#33 AR-1260-3

R.T.: 6.113 min
Delta R.T.: 0.000 min
Response: 4430116
Conc: 13.64 ng/ml

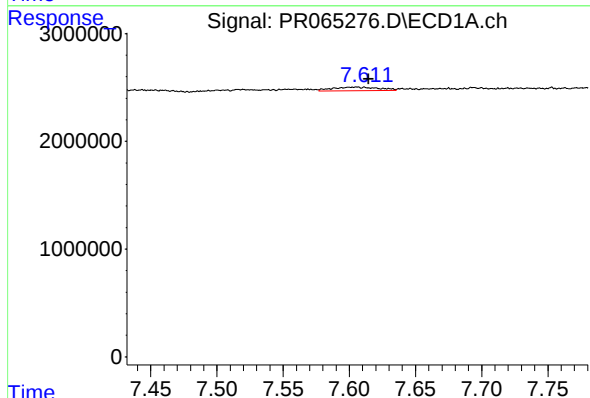


#34 AR-1260-4

R.T.: 7.605 min
Delta R.T.: -0.009 min
Response: 832690
Conc: 3.53 ng/ml

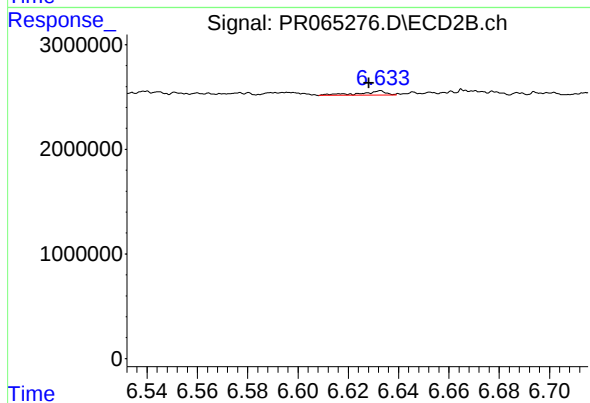

#34 AR-1260-4


R.T.: 6.633 min
Delta R.T.: 0.004 min
Response: 293920
Conc: 1.11 ng/ml

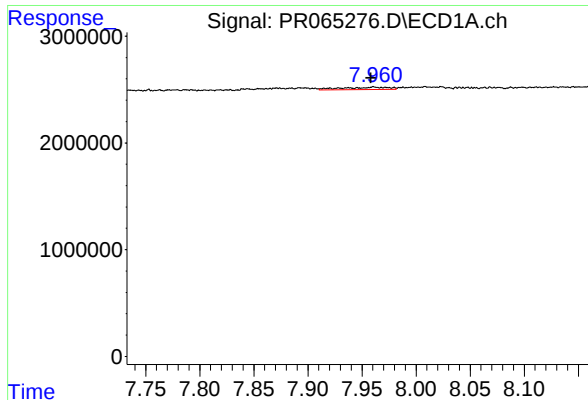

#35 AR-1260-5


R.T.: 7.961 min
Delta R.T.: 0.003 min
Response: 688332
Conc: 1.57 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

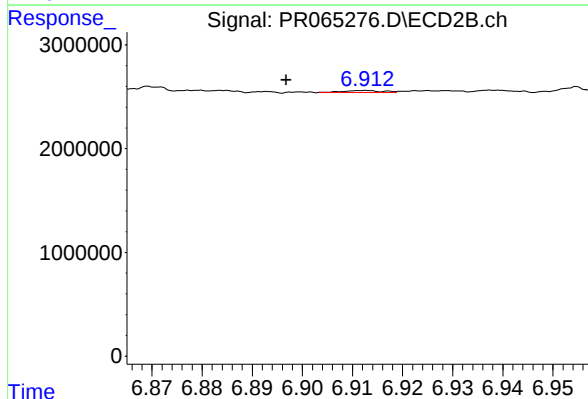


#35 AR-1260-5

R.T.: 6.912 min
Delta R.T.: 0.015 min
Response: 100443
Conc: 0.16 ng/ml

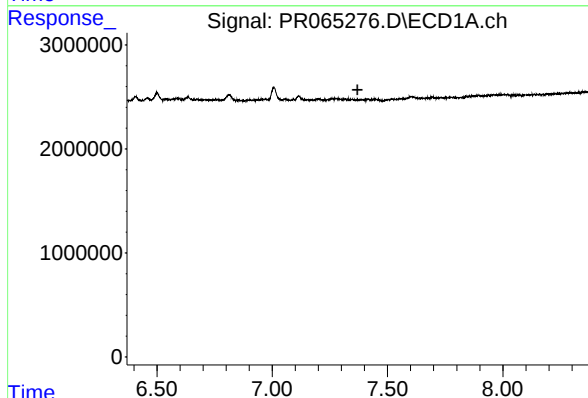


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

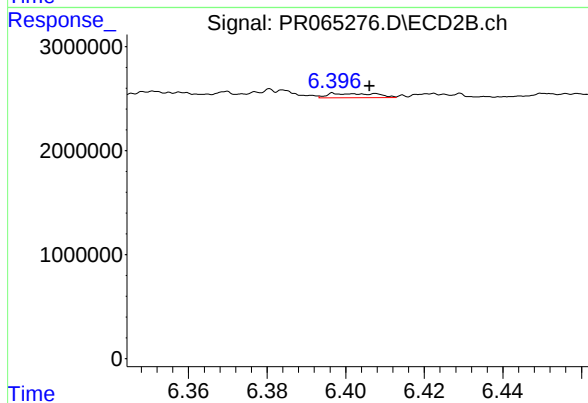

#36 AR-1262-1


R.T.: 6.402 min
Delta R.T.: -0.004 min
Response: 334584
Conc: 1.87 ng/ml

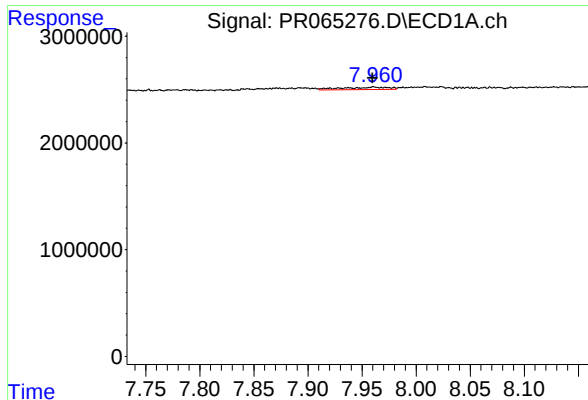

#37 AR-1262-2


R.T.: 7.961 min
Delta R.T.: 0.001 min
Response: 688332
Conc: 1.22 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

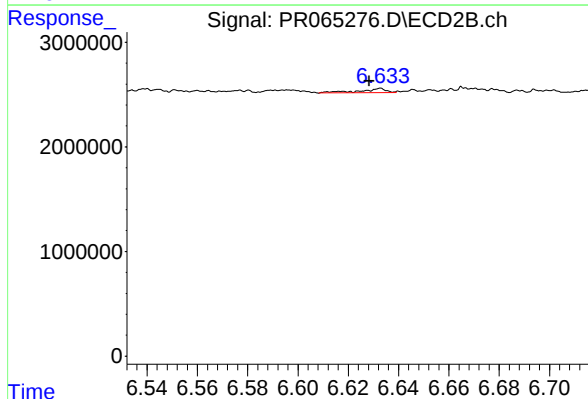


#37 AR-1262-2

R.T.: 6.633 min
Delta R.T.: 0.004 min
Response: 293920
Conc: 0.76 ng/ml

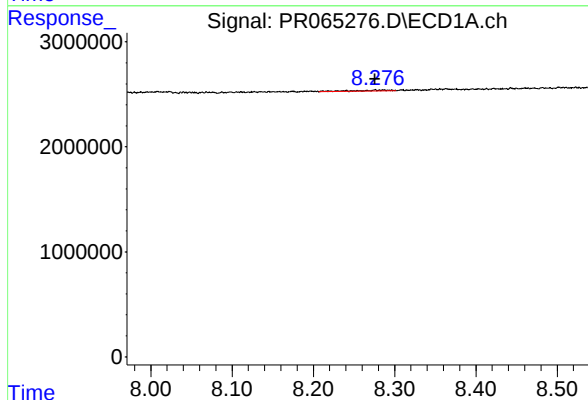


#38 AR-1262-3

R.T.: 8.277 min
Delta R.T.: 0.001 min
Response: 188689
Conc: 0.50 ng/ml

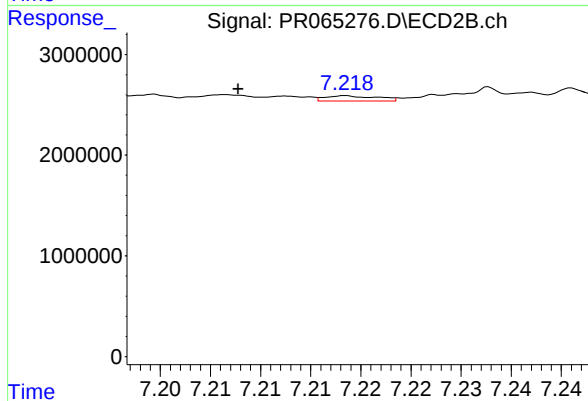

#38 AR-1262-3


R.T.: 7.219 min
Delta R.T.: 0.011 min
Response: 186422
Conc: 0.66 ng/ml

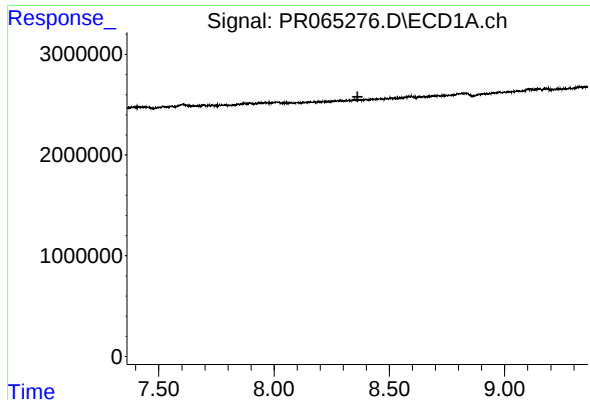

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

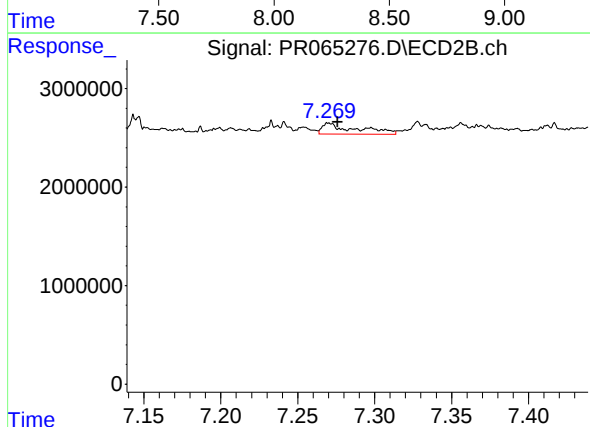


#39 AR-1262-4

R.T.: 7.270 min
Delta R.T.: -0.005 min
Response: 1711937
Conc: 2.97 ng/ml

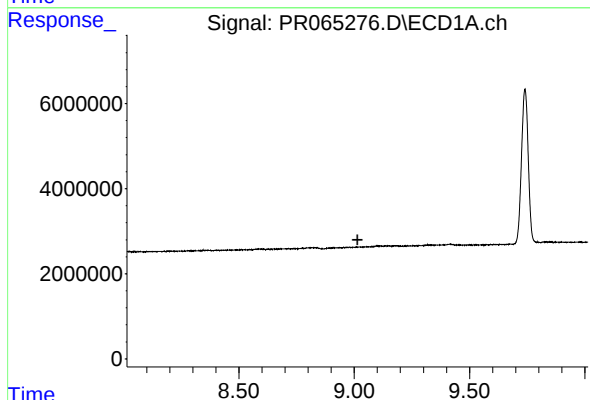


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.014 min
Response: 0
Conc: N.D.

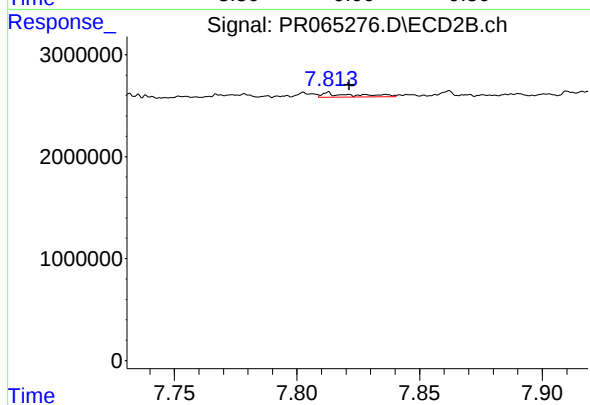

#40 AR-1262-5


R.T.: 7.813 min
Delta R.T.: -0.009 min
Response: 413009
Conc: 1.59 ng/ml

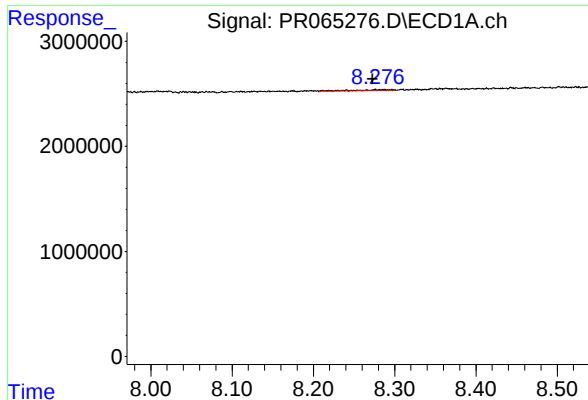

#41 AR-1268-1


R.T.: 8.277 min
Delta R.T.: 0.004 min
Response: 188689
Conc: 0.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

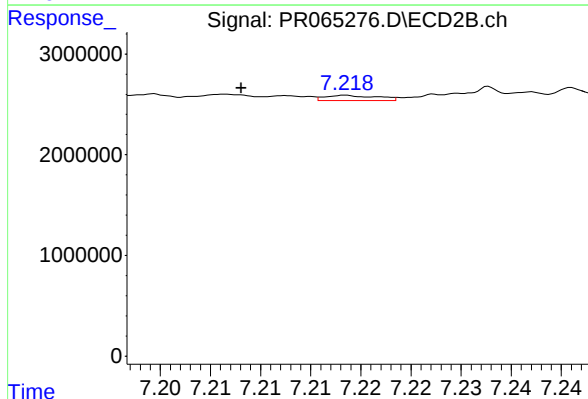


#41 AR-1268-1

R.T.: 7.219 min
Delta R.T.: 0.011 min
Response: 186422
Conc: 0.23 ng/ml

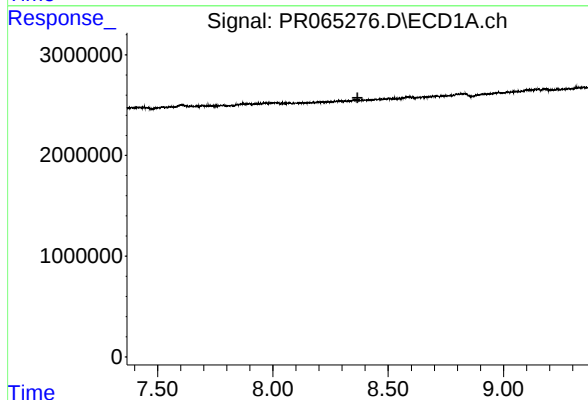


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.367 min
Response: 0
Conc: N.D.

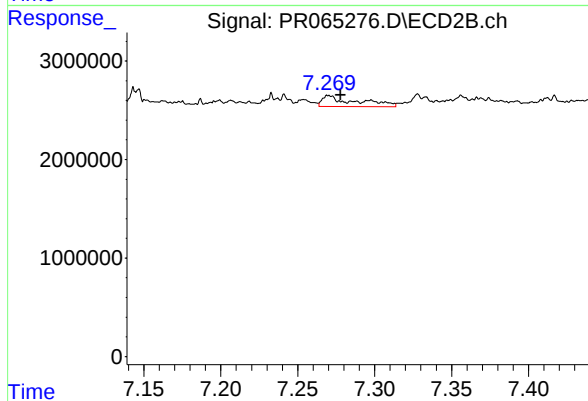

#42 AR-1268-2


R.T.: 7.270 min
Delta R.T.: -0.007 min
Response: 1711937
Conc: 2.30 ng/ml

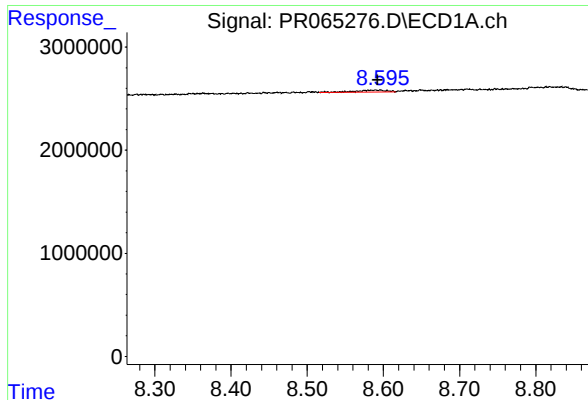

#43 AR-1268-3


R.T.: 8.590 min
Delta R.T.: -0.003 min
Response: 544172
Conc: 1.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

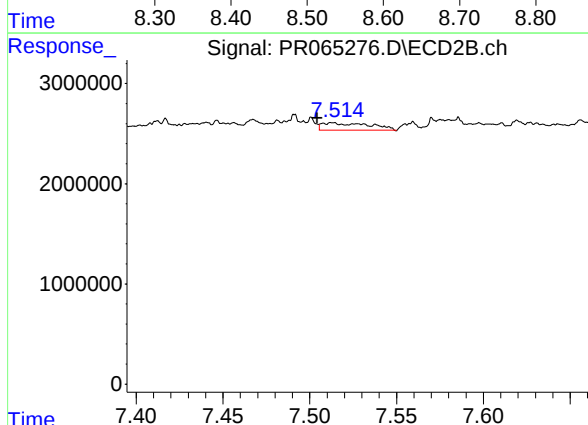


#43 AR-1268-3

R.T.: 7.513 min
Delta R.T.: 0.009 min
Response: 1417713
Conc: 2.24 ng/ml

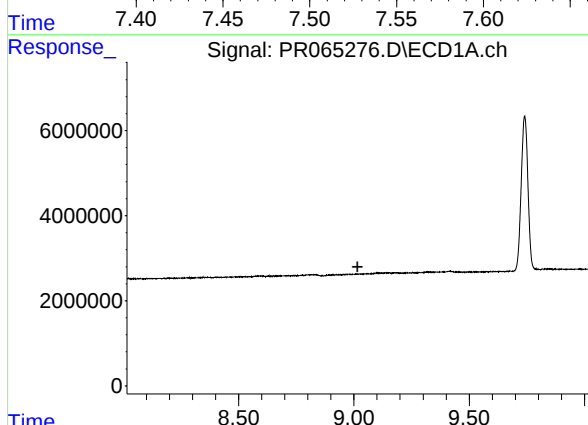


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.016 min
Response: 0
Conc: N.D.

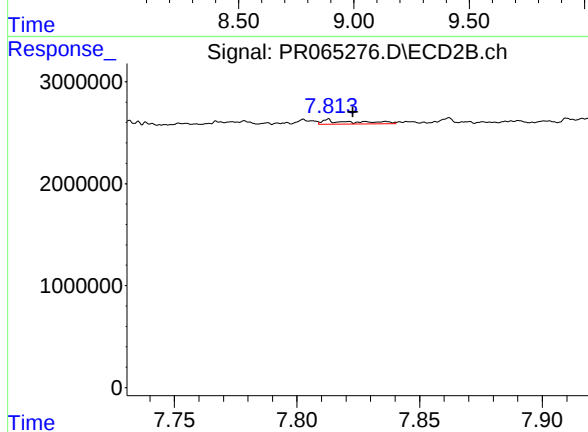

#44 AR-1268-4


R.T.: 7.813 min
Delta R.T.: -0.010 min
Response: 413009
Conc: 1.57 ng/ml

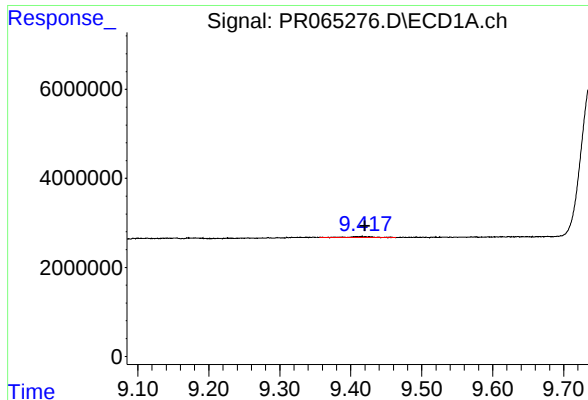

#45 AR-1268-5

R.T.: 9.414 min
Delta R.T.: -0.006 min
Response: 493533
Conc: 0.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

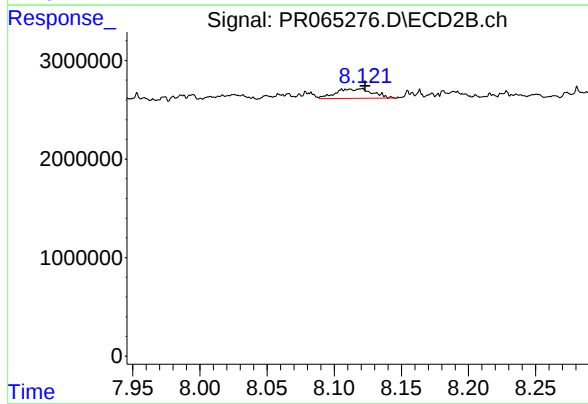

#45 AR-1268-5

R.T.: 8.120 min
Delta R.T.: -0.003 min
Response: 1820594
Conc: 0.95 ng/ml