

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
 Data File : PR065277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 18:51
 Operator : AJ\MA
 Sample : P1187-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:34:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.701	3.003	96378974	91772616	16.146	16.778
2) SA Decachlor...	9.739	8.374	71156838	79991323	17.791	16.902
Target Compounds						
3) L1 AR-1016-1	4.942	4.148	2412686	2412546	13.612	13.285
4) L1 AR-1016-2	4.965	4.166	3112841	2283044	11.940	9.234
5) L1 AR-1016-3	5.028	4.350	1812066	1803197	10.842	13.299
6) L1 AR-1016-4	5.132	4.402	1753215	3582683	13.075	34.210 #
7) L1 AR-1016-5	5.453	4.624	4110044	5322900	30.439	38.155 #
8) L2 AR-1221-1	3.912f	0.000	1488481	0	20.739	N.D. #
9) L2 AR-1221-2	4.016	3.313	2497725	2061990	47.645	43.233
10) L2 AR-1221-3	4.094	3.398	619658	813429	4.033	5.889 #
11) L3 AR-1232-1	4.094	3.398	619658	813429	4.584	6.792 #
12) L3 AR-1232-2	4.651	4.166	1570030	2283044	20.379	18.687
13) L3 AR-1232-3	4.965	4.350	3112841	1803197	24.411	27.108
14) L3 AR-1232-4	5.132	4.444	1753215	3430354	26.748	59.908 #
15) L3 AR-1232-5	5.239	4.624	3645936	5322900	75.381	83.507
16) L4 AR-1242-1	4.942	4.148	2412686	2412546	16.877	16.509
17) L4 AR-1242-2	4.965	4.166	3112841	2283044	14.782	11.445
18) L4 AR-1242-3	5.028	4.350	1812066	1803197	13.380	16.468
19) L4 AR-1242-4	5.132	4.444	1753215	3430354	16.135	32.675 #
20) L4 AR-1242-5	5.934	5.004	4352124	6377074	38.474	47.230
21) L5 AR-1248-1	4.942	4.148	2412686	2412546	22.676	22.334
22) L5 AR-1248-2	5.239	4.402	3645936	3582683	23.464	24.738
23) L5 AR-1248-3	5.453	4.444	4110044	3430354	23.018	22.168
24) L5 AR-1248-4	5.892	4.624	3882748	5322900	20.480	28.424 #
25) L5 AR-1248-5	5.934	5.047	4352124	5734307	22.840	30.808 #
26) L6 AR-1254-1	5.864	5.004	4281719	6377074	20.905	21.885
27) L6 AR-1254-2	6.103	5.165	4432777	3776076	14.222	14.906
28) L6 AR-1254-3	6.501	5.596	2721951	4105239	8.508	10.034
29) L6 AR-1254-4	6.815	5.846	1646370	4566305	7.185	17.787 #
30) L6 AR-1254-5	7.279	6.299	1033719	3057821	4.159	8.342 #
31) L7 AR-1260-1	6.684	5.750	233357	4107760	0.928	14.391 #
32) L7 AR-1260-2	6.972	5.946	487786	1492479	1.697	4.304 #
33) L7 AR-1260-3	0.000	6.110	0	5824801	N.D.	17.929 #
34) L7 AR-1260-4	7.603	0.000	1349879	0	5.720	N.D. #
35) L7 AR-1260-5	7.965	0.000	442674	0	1.007	N.D. #
36) L8 AR-1262-1	0.000	6.399	0	265615	N.D.	1.481 #
37) L8 AR-1262-2	7.965	0.000	442674	0	0.783	N.D. #
38) L8 AR-1262-3	8.281	7.181f	237315	1981621	0.624	6.991 #
39) L8 AR-1262-4	8.357	7.282	684572	3129856	2.337	5.435 #
40) L8 AR-1262-5	9.021	0.000	252519	0	1.260	N.D. #
41) L9 AR-1268-1	8.281	7.181f	237315	1981621	0.391	2.498 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
 Data File : PR065277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 18:51
 Operator : AJ\MA
 Sample : P1187-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:34:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm


	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.357	7.282	684572	3129856	1.251	4.204 #
43) L9	AR-1268-3	8.588	7.498	1282530	3963833	2.703	6.257 #
44) L9	AR-1268-4	9.021	0.000	252519	0	1.241	N.D. #
45) L9	AR-1268-5	9.412	8.114	444390	1507367	0.305	0.787 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

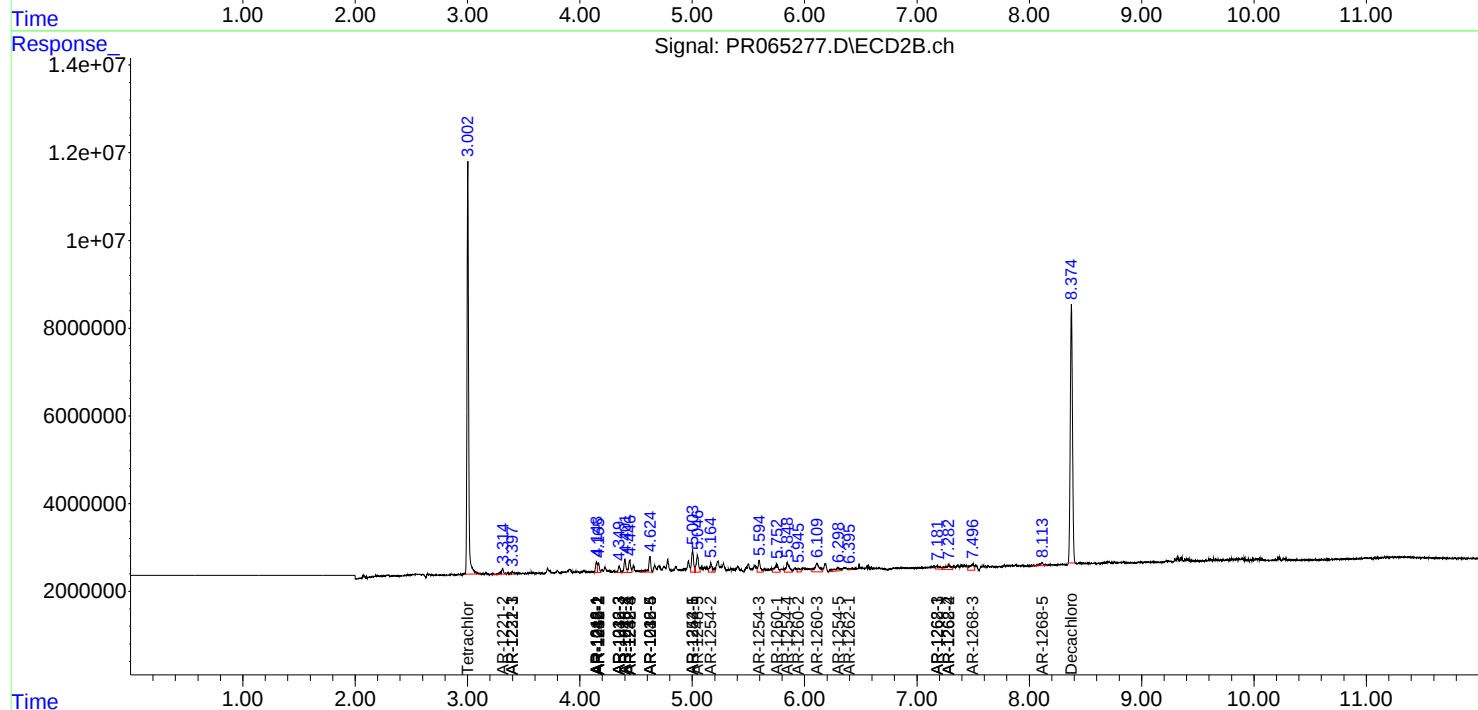


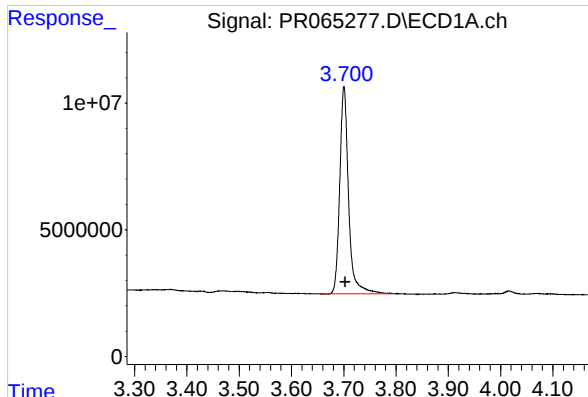

#1 Tetrachloro-m-xylene


R.T.: 3.701 min
Delta R.T.: -0.002 min
Response: 96378974
Conc: 16.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

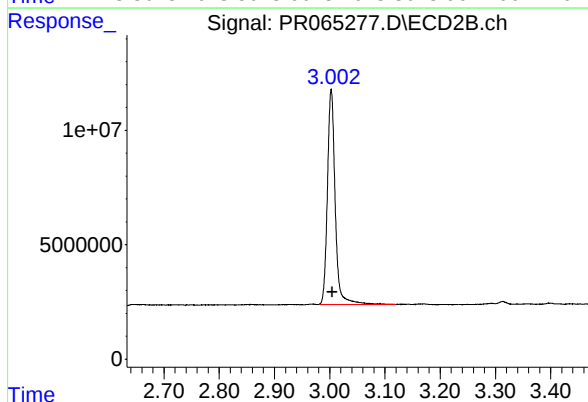


#1 Tetrachloro-m-xylene

R.T.: 3.003 min
Delta R.T.: -0.002 min
Response: 91772616
Conc: 16.78 ng/ml

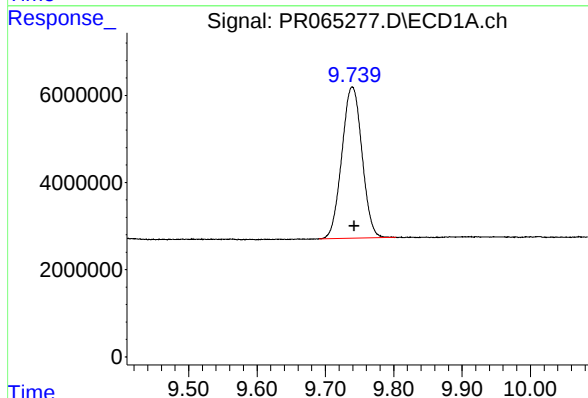


#2 Decachlorobiphenyl

R.T.: 9.739 min
Delta R.T.: -0.003 min
Response: 71156838
Conc: 17.79 ng/ml

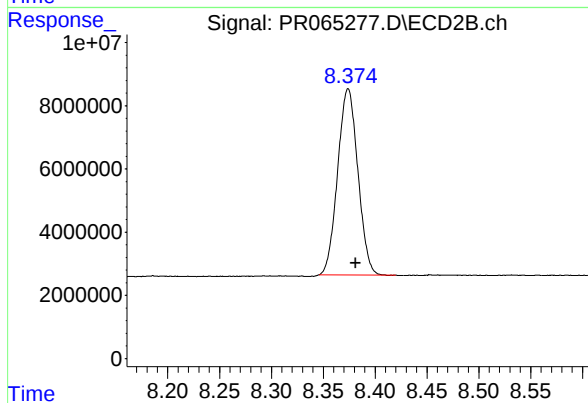

#2 Decachlorobiphenyl


R.T.: 8.374 min
Delta R.T.: -0.007 min
Response: 79991323
Conc: 16.90 ng/ml

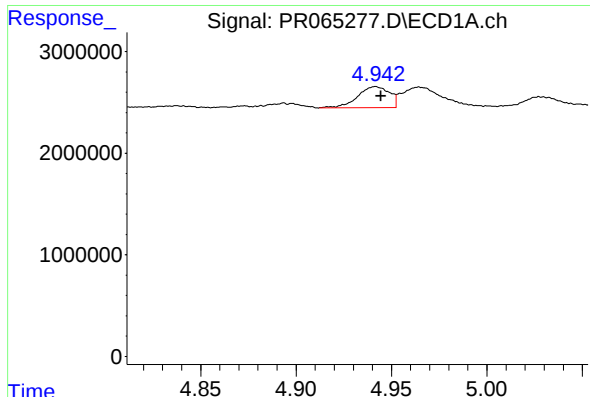

#3 AR-1016-1


R.T.: 4.942 min
Delta R.T.: -0.003 min
Response: 2412686
Conc: 13.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

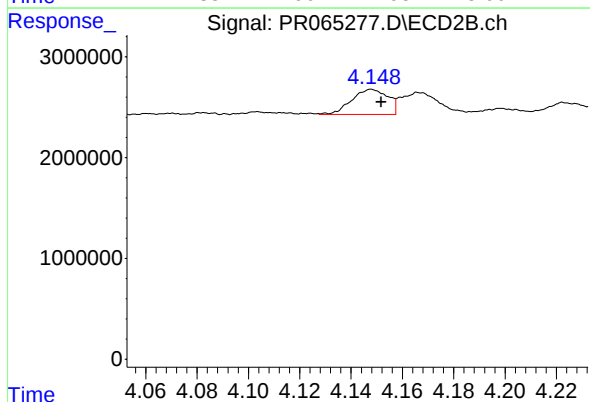


#3 AR-1016-1

R.T.: 4.148 min
Delta R.T.: -0.004 min
Response: 2412546
Conc: 13.28 ng/ml

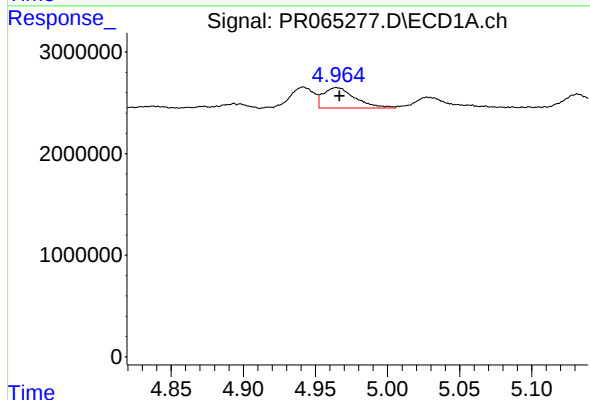


#4 AR-1016-2

R.T.: 4.965 min
Delta R.T.: -0.002 min
Response: 3112841
Conc: 11.94 ng/ml

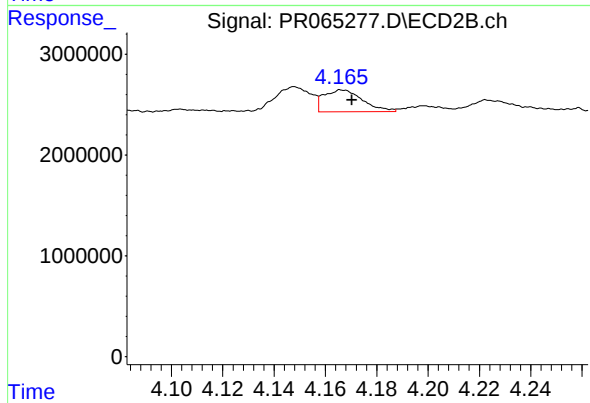

#4 AR-1016-2


R.T.: 4.166 min
Delta R.T.: -0.004 min
Response: 2283044
Conc: 9.23 ng/ml

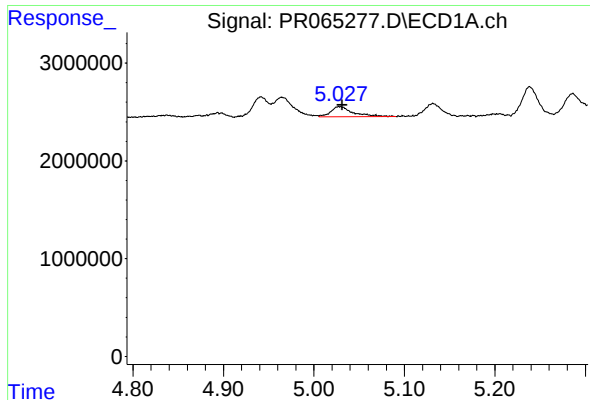

#5 AR-1016-3


R.T.: 5.028 min
Delta R.T.: -0.004 min
Response: 1812066
Conc: 10.84 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

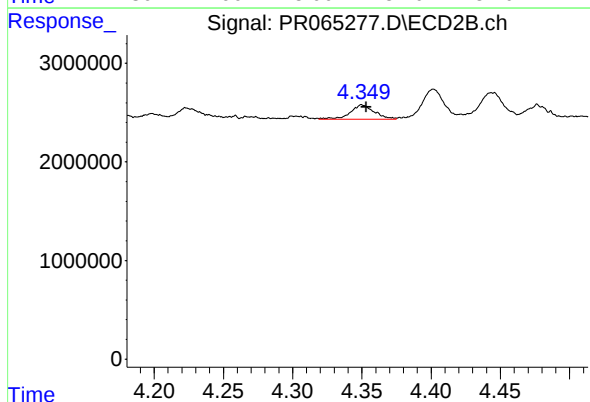


#5 AR-1016-3

R.T.: 4.350 min
Delta R.T.: -0.003 min
Response: 1803197
Conc: 13.30 ng/ml

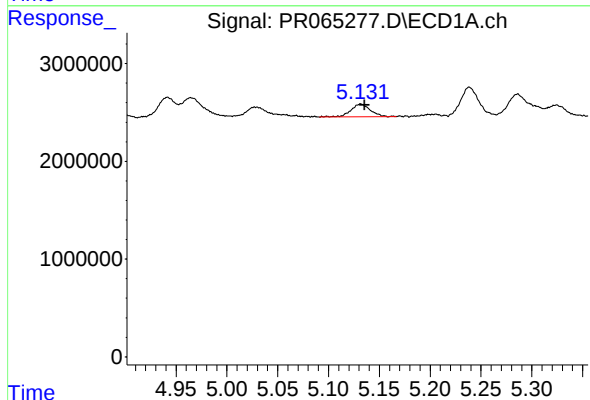


#6 AR-1016-4

R.T.: 5.132 min
Delta R.T.: -0.003 min
Response: 1753215
Conc: 13.07 ng/ml

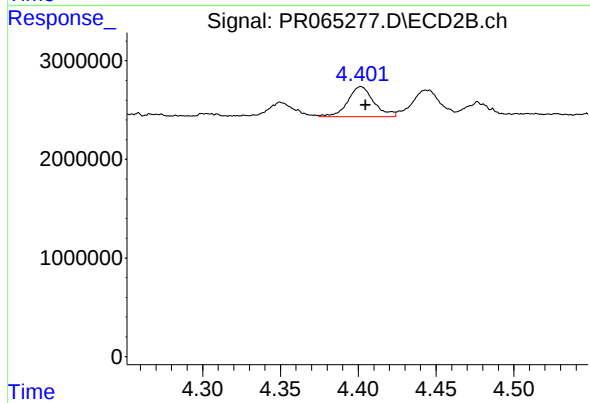

#6 AR-1016-4


R.T.: 4.402 min
Delta R.T.: -0.003 min
Response: 3582683
Conc: 34.21 ng/ml

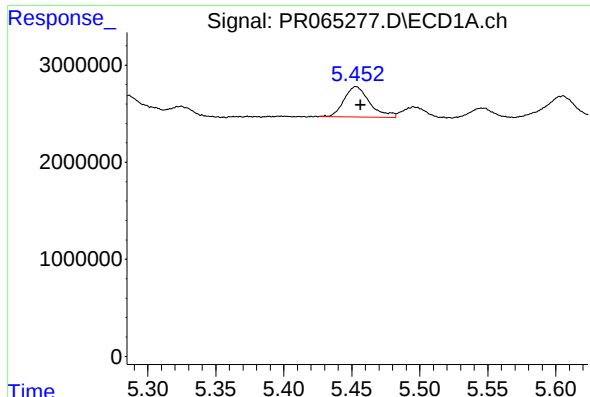

#7 AR-1016-5


R.T.: 5.453 min
Delta R.T.: -0.003 min
Response: 4110044
Conc: 30.44 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

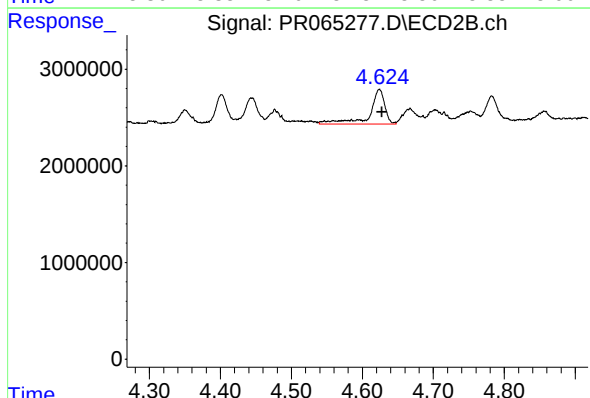


#7 AR-1016-5

R.T.: 4.624 min
Delta R.T.: -0.004 min
Response: 5322900
Conc: 38.15 ng/ml

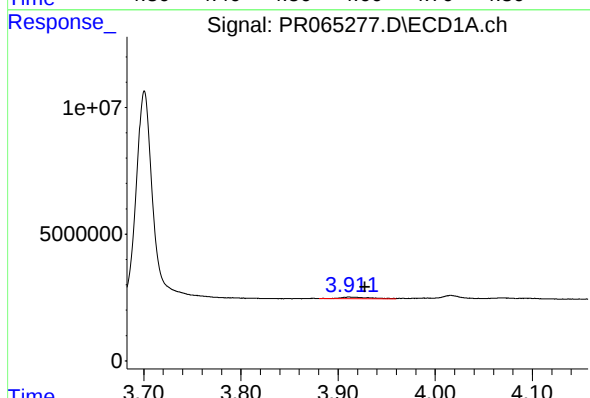


#8 AR-1221-1

R.T.: 3.912 min
Delta R.T.: -0.016 min
Response: 1488481
Conc: 20.74 ng/ml

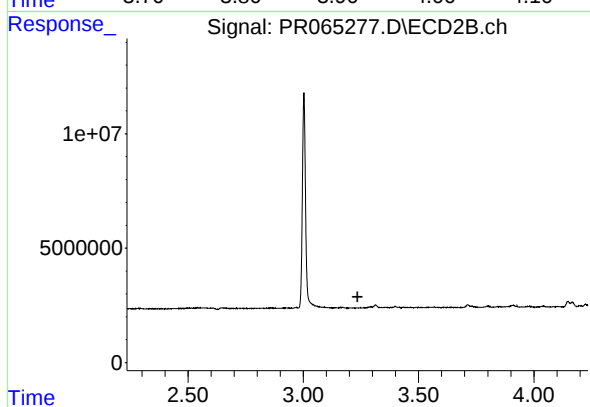

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.235 min
Response: 0
Conc: N.D.

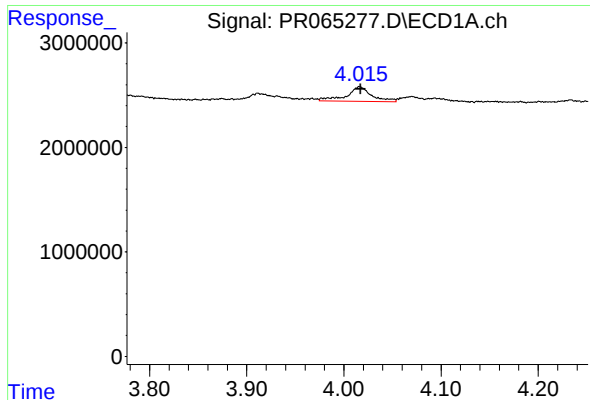

#9 AR-1221-2


R.T.: 4.016 min
Delta R.T.: -0.001 min
Response: 2497725
Conc: 47.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

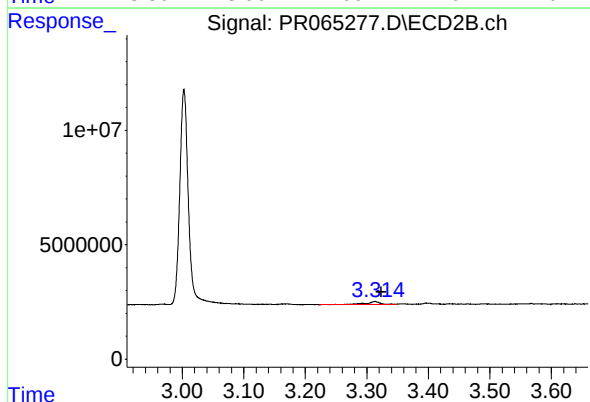


#9 AR-1221-2

R.T.: 3.313 min
Delta R.T.: -0.010 min
Response: 2061990
Conc: 43.23 ng/ml

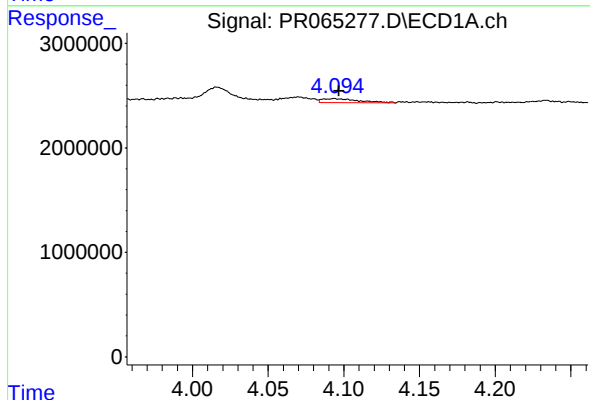


#10 AR-1221-3

R.T.: 4.094 min
Delta R.T.: -0.003 min
Response: 619658
Conc: 4.03 ng/ml

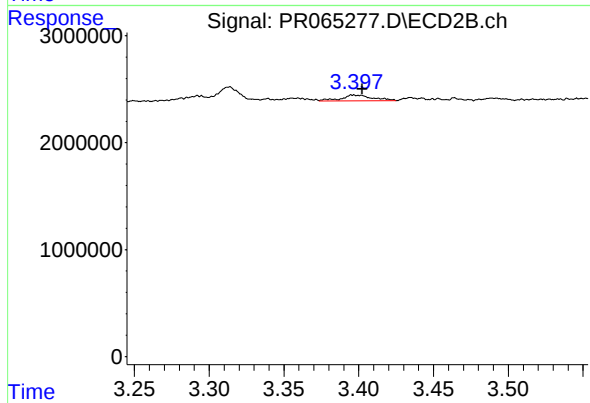

#10 AR-1221-3


R.T.: 3.398 min
Delta R.T.: -0.004 min
Response: 813429
Conc: 5.89 ng/ml

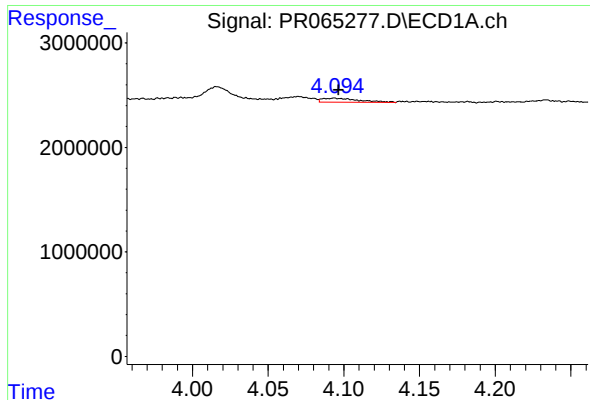

#11 AR-1232-1


R.T.: 4.094 min
Delta R.T.: -0.003 min
Response: 619658
Conc: 4.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

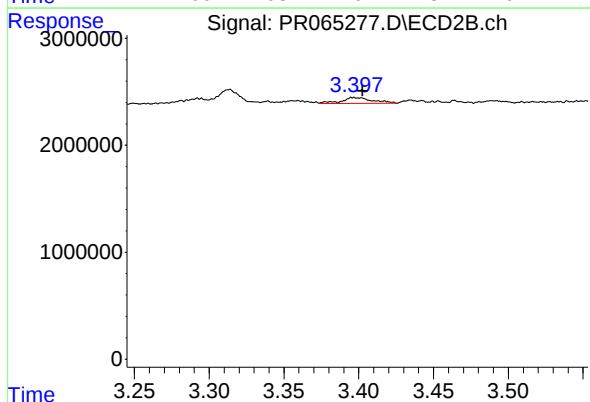


#11 AR-1232-1

R.T.: 3.398 min
Delta R.T.: -0.004 min
Response: 813429
Conc: 6.79 ng/ml

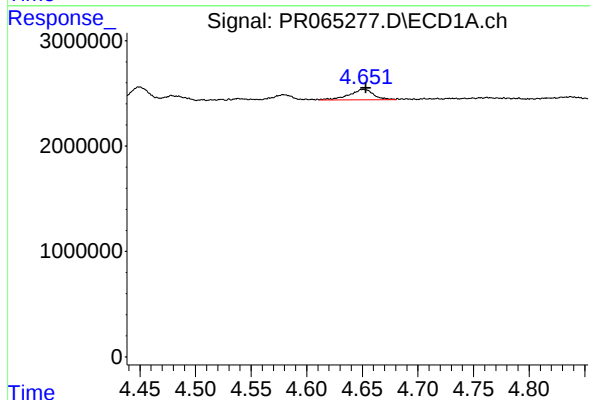


#12 AR-1232-2

R.T.: 4.651 min
Delta R.T.: -0.002 min
Response: 1570030
Conc: 20.38 ng/ml

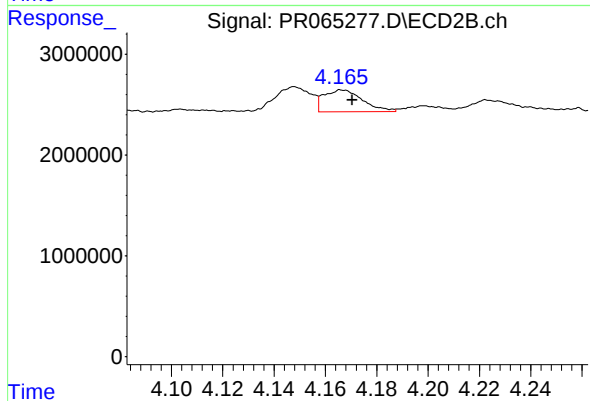

#12 AR-1232-2


R.T.: 4.166 min
Delta R.T.: -0.004 min
Response: 2283044
Conc: 18.69 ng/ml

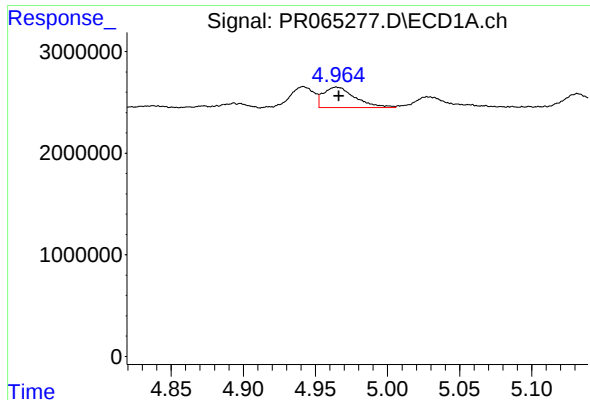

#13 AR-1232-3


R.T.: 4.965 min
Delta R.T.: -0.002 min
Response: 3112841
Conc: 24.41 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

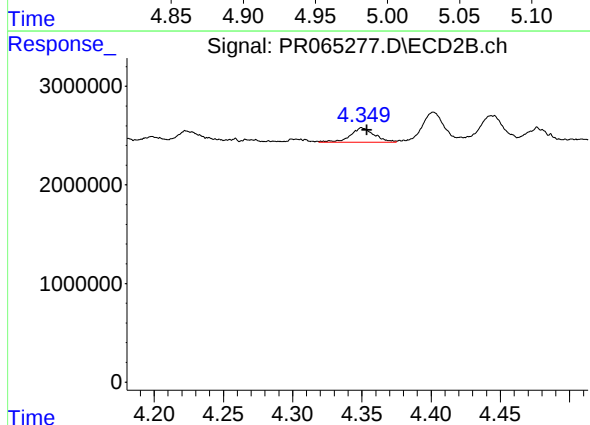


#13 AR-1232-3

R.T.: 4.350 min
Delta R.T.: -0.003 min
Response: 1803197
Conc: 27.11 ng/ml

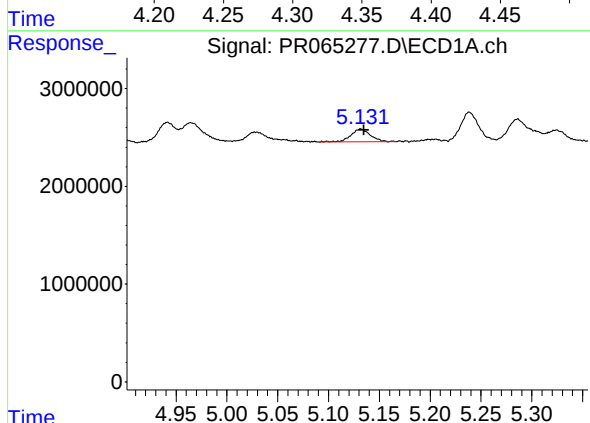


#14 AR-1232-4

R.T.: 5.132 min
Delta R.T.: -0.003 min
Response: 1753215
Conc: 26.75 ng/ml

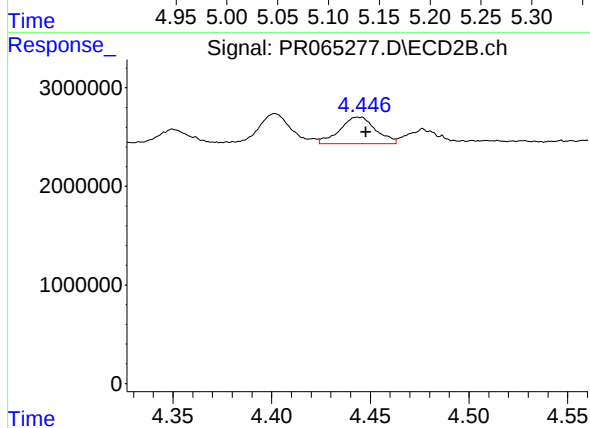

#14 AR-1232-4


R.T.: 4.444 min
Delta R.T.: -0.004 min
Response: 3430354
Conc: 59.91 ng/ml

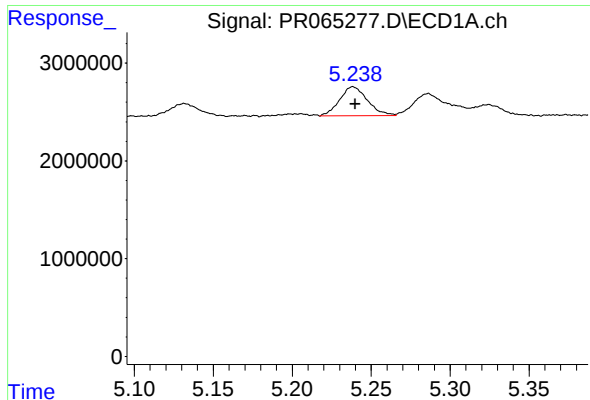

#15 AR-1232-5


R.T.: 5.239 min
Delta R.T.: -0.001 min
Response: 3645936
Conc: 75.38 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

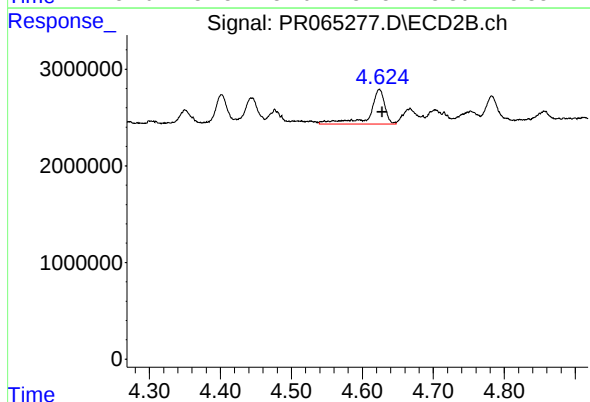


#15 AR-1232-5

R.T.: 4.624 min
Delta R.T.: -0.004 min
Response: 5322900
Conc: 83.51 ng/ml

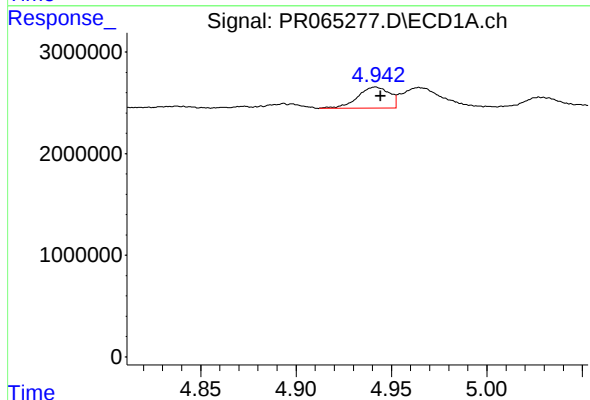


#16 AR-1242-1

R.T.: 4.942 min
Delta R.T.: -0.003 min
Response: 2412686
Conc: 16.88 ng/ml

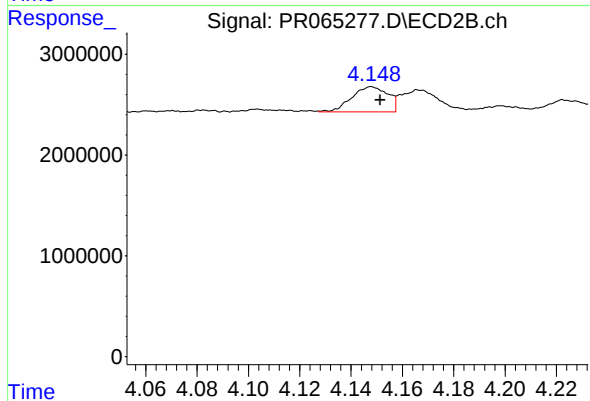

#16 AR-1242-1


R.T.: 4.148 min
Delta R.T.: -0.003 min
Response: 2412546
Conc: 16.51 ng/ml

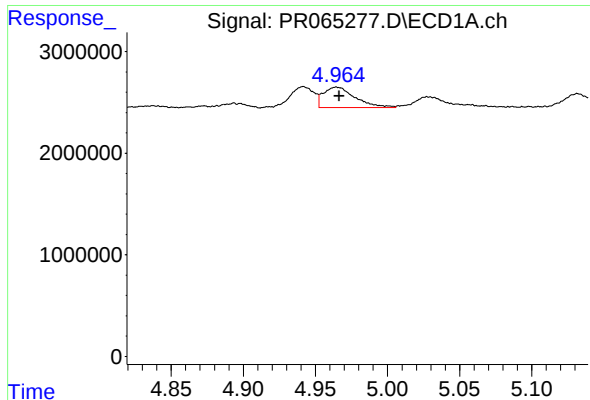

#17 AR-1242-2


R.T.: 4.965 min
Delta R.T.: -0.002 min
Response: 3112841
Conc: 14.78 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

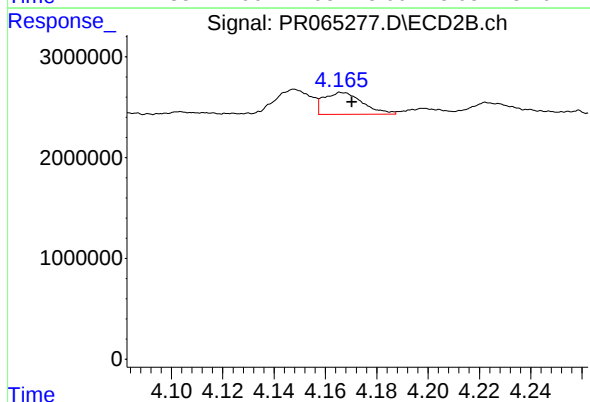


#17 AR-1242-2

R.T.: 4.166 min
Delta R.T.: -0.004 min
Response: 2283044
Conc: 11.44 ng/ml

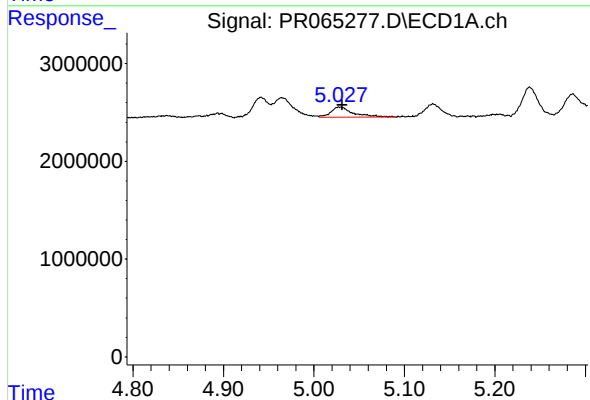


#18 AR-1242-3

R.T.: 5.028 min
Delta R.T.: -0.003 min
Response: 1812066
Conc: 13.38 ng/ml

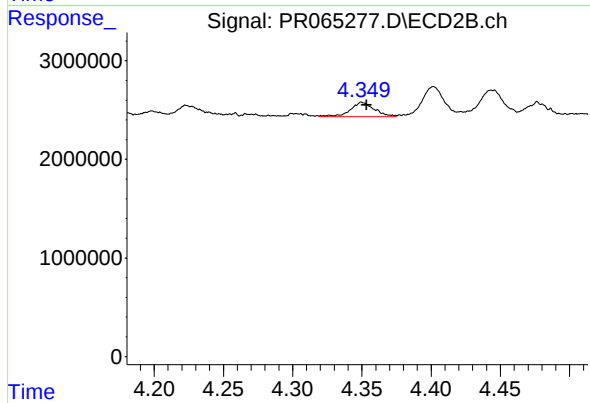

#18 AR-1242-3


R.T.: 4.350 min
Delta R.T.: -0.003 min
Response: 1803197
Conc: 16.47 ng/ml

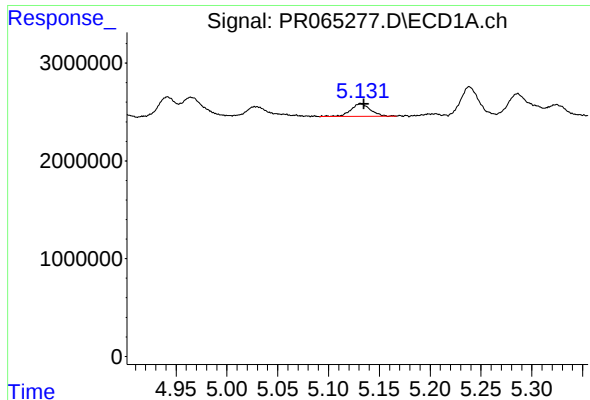

#19 AR-1242-4


R.T.: 5.132 min
Delta R.T.: -0.003 min
Response: 1753215
Conc: 16.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

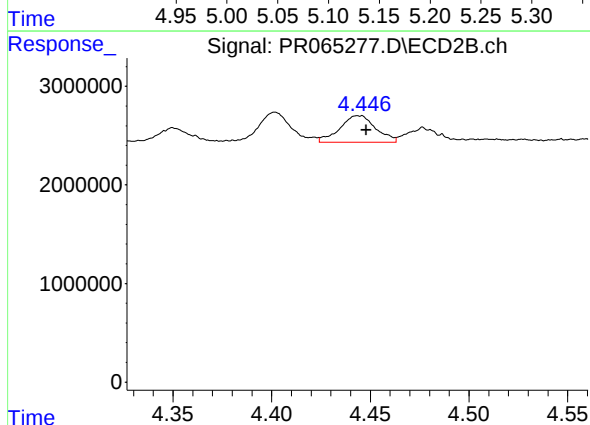


#19 AR-1242-4

R.T.: 4.444 min
Delta R.T.: -0.004 min
Response: 3430354
Conc: 32.67 ng/ml

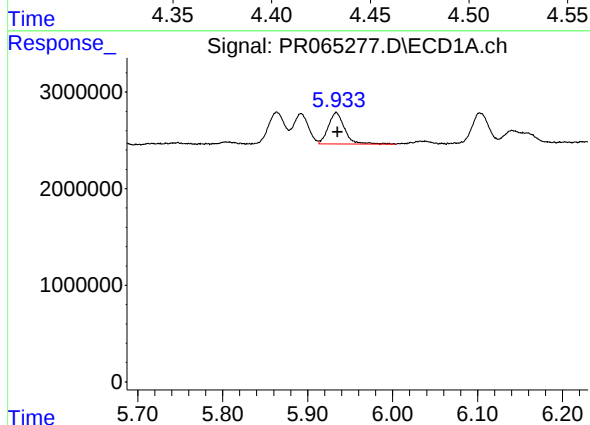


#20 AR-1242-5

R.T.: 5.934 min
Delta R.T.: -0.002 min
Response: 4352124
Conc: 38.47 ng/ml

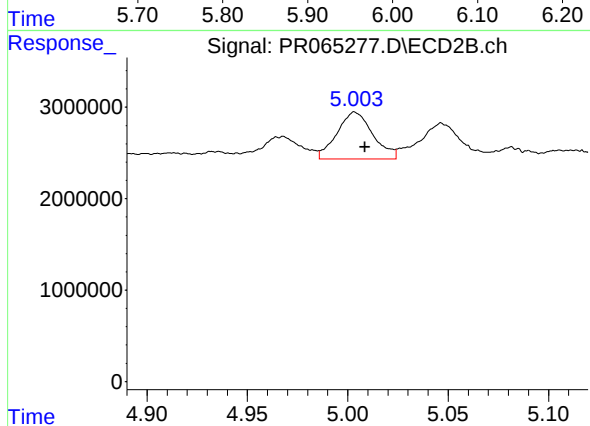

#20 AR-1242-5


R.T.: 5.004 min
Delta R.T.: -0.005 min
Response: 6377074
Conc: 47.23 ng/ml

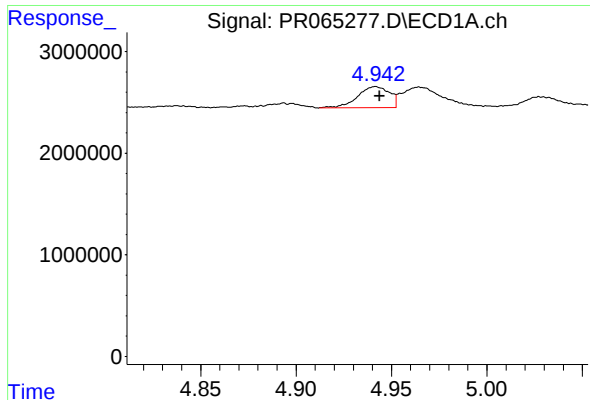

#21 AR-1248-1


R.T.: 4.942 min
Delta R.T.: -0.002 min
Response: 2412686
Conc: 22.68 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

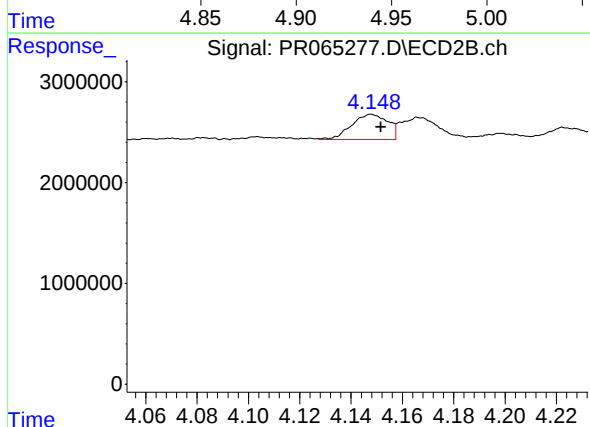


#21 AR-1248-1

R.T.: 4.148 min
Delta R.T.: -0.003 min
Response: 2412546
Conc: 22.33 ng/ml

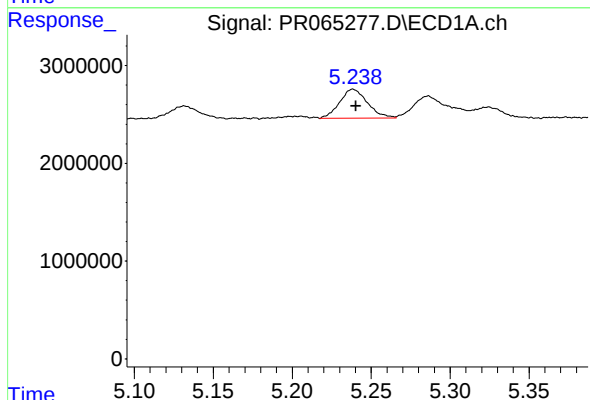


#22 AR-1248-2

R.T.: 5.239 min
Delta R.T.: -0.002 min
Response: 3645936
Conc: 23.46 ng/ml

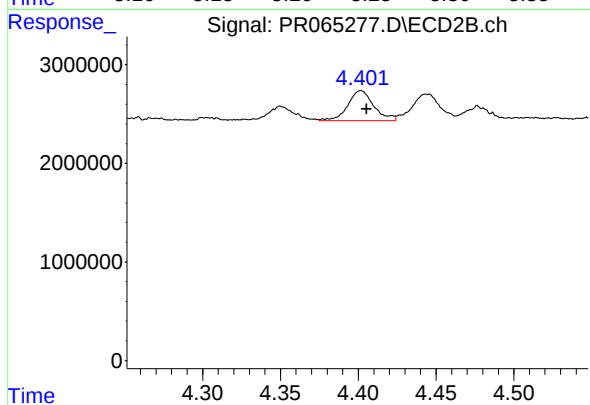

#22 AR-1248-2


R.T.: 4.402 min
Delta R.T.: -0.004 min
Response: 3582683
Conc: 24.74 ng/ml

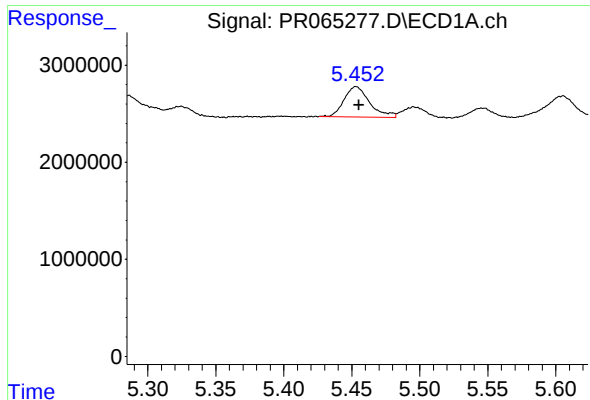

#23 AR-1248-3


R.T.: 5.453 min
Delta R.T.: -0.002 min
Response: 4110044
Conc: 23.02 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

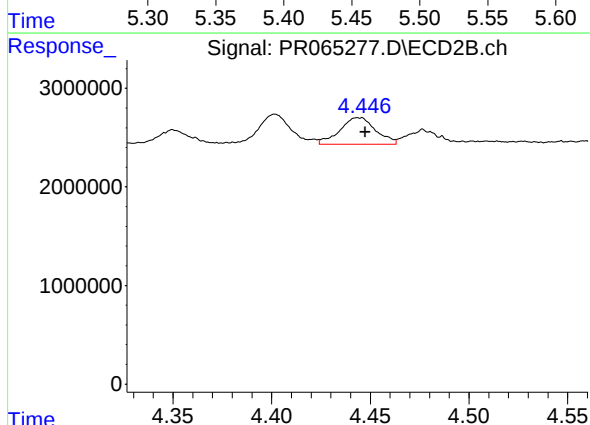


#23 AR-1248-3

R.T.: 4.444 min
Delta R.T.: -0.003 min
Response: 3430354
Conc: 22.17 ng/ml

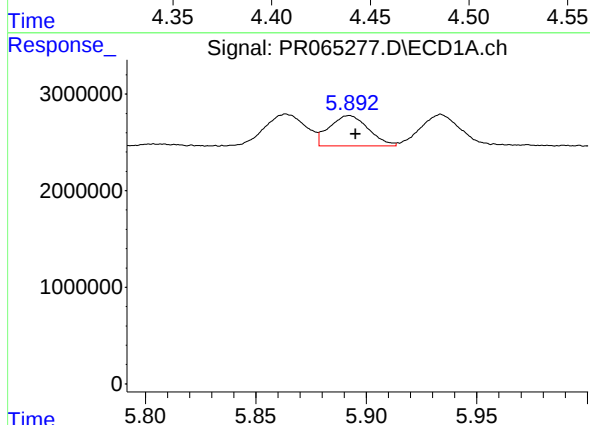


#24 AR-1248-4

R.T.: 5.892 min
Delta R.T.: -0.003 min
Response: 3882748
Conc: 20.48 ng/ml

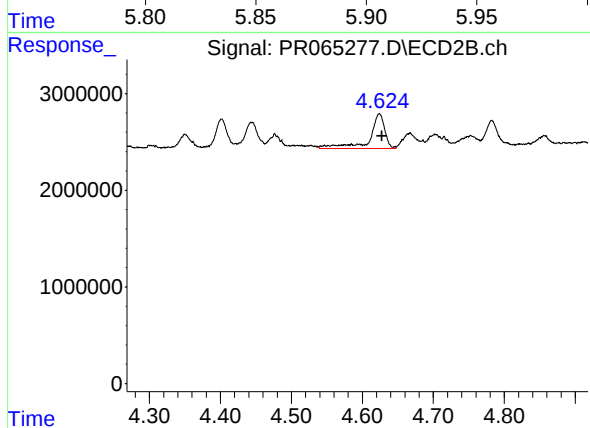

#24 AR-1248-4


R.T.: 4.624 min
Delta R.T.: -0.004 min
Response: 5322900
Conc: 28.42 ng/ml

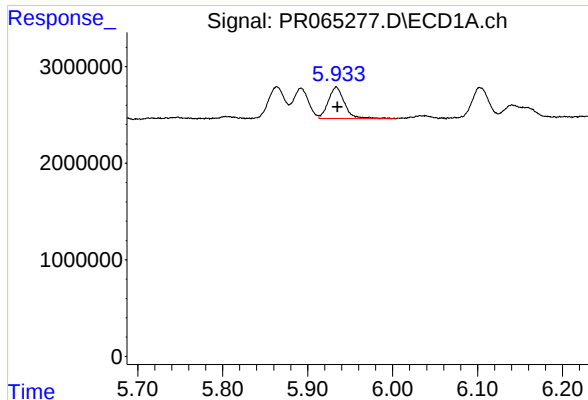

#25 AR-1248-5


R.T.: 5.934 min
Delta R.T.: -0.001 min
Response: 4352124
Conc: 22.84 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

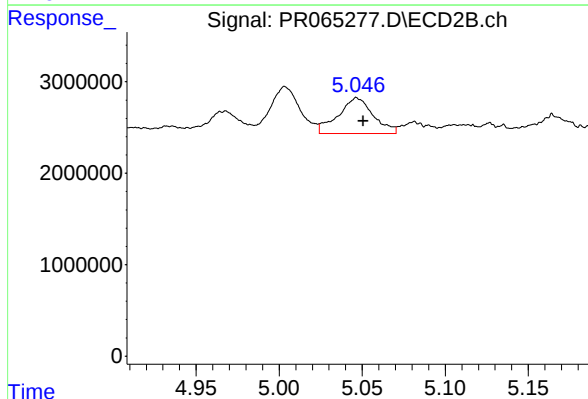


#25 AR-1248-5

R.T.: 5.047 min
Delta R.T.: -0.004 min
Response: 5734307
Conc: 30.81 ng/ml

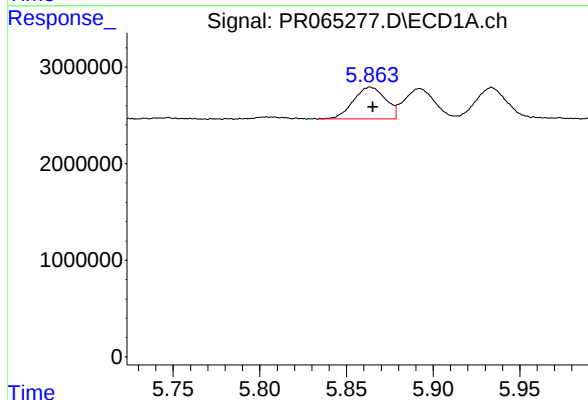


#26 AR-1254-1

R.T.: 5.864 min
Delta R.T.: -0.002 min
Response: 4281719
Conc: 20.91 ng/ml

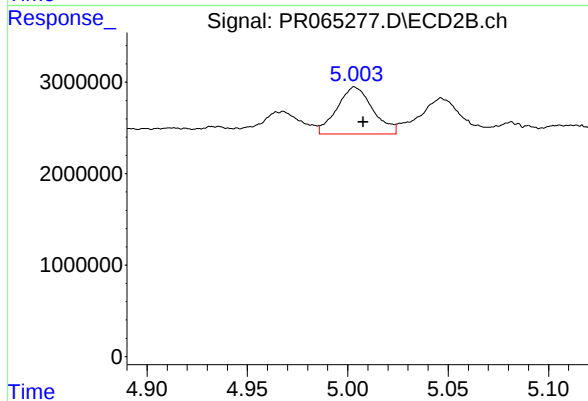

#26 AR-1254-1


R.T.: 5.004 min
Delta R.T.: -0.004 min
Response: 6377074
Conc: 21.89 ng/ml

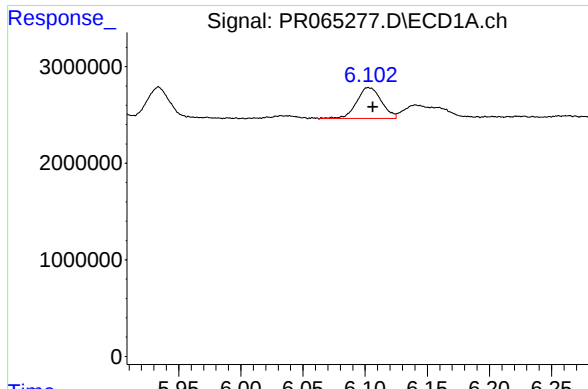

#27 AR-1254-2


R.T.: 6.103 min
Delta R.T.: -0.003 min
Response: 4432777
Conc: 14.22 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

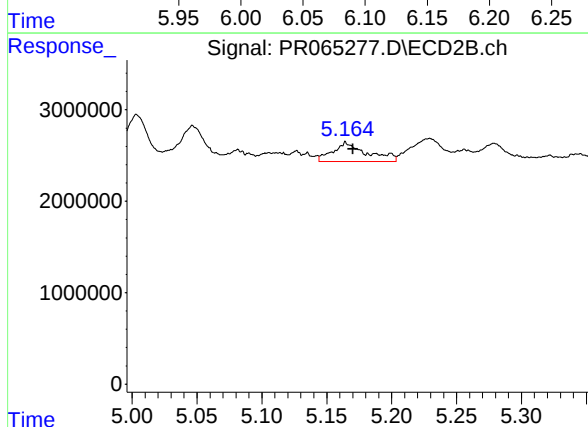


#27 AR-1254-2

R.T.: 5.165 min
Delta R.T.: -0.005 min
Response: 3776076
Conc: 14.91 ng/ml

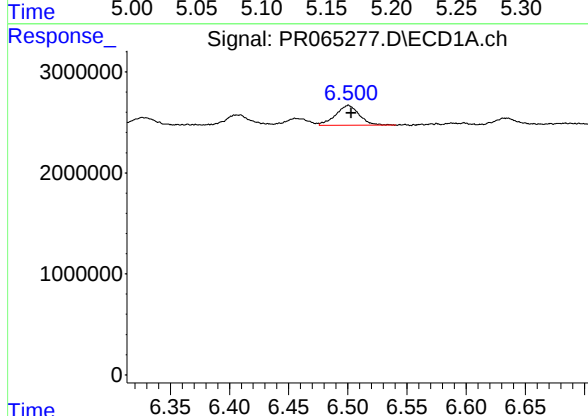


#28 AR-1254-3

R.T.: 6.501 min
Delta R.T.: -0.002 min
Response: 2721951
Conc: 8.51 ng/ml

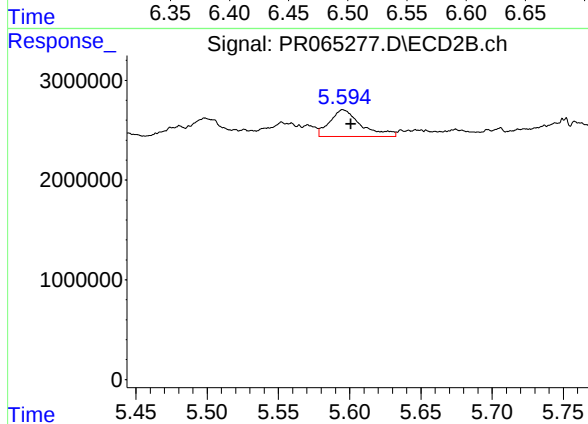

#28 AR-1254-3


R.T.: 5.596 min
Delta R.T.: -0.005 min
Response: 4105239
Conc: 10.03 ng/ml

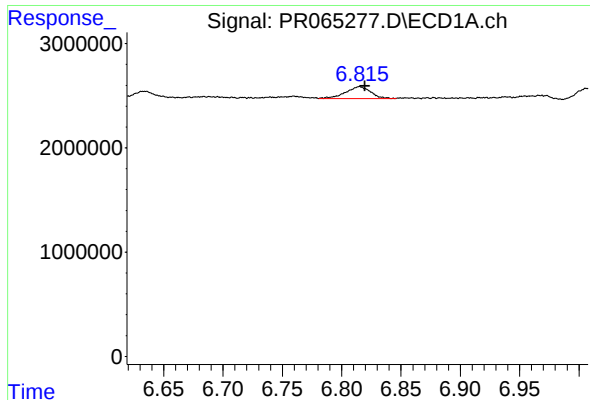

#29 AR-1254-4


R.T.: 6.815 min
Delta R.T.: -0.004 min
Response: 1646370
Conc: 7.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

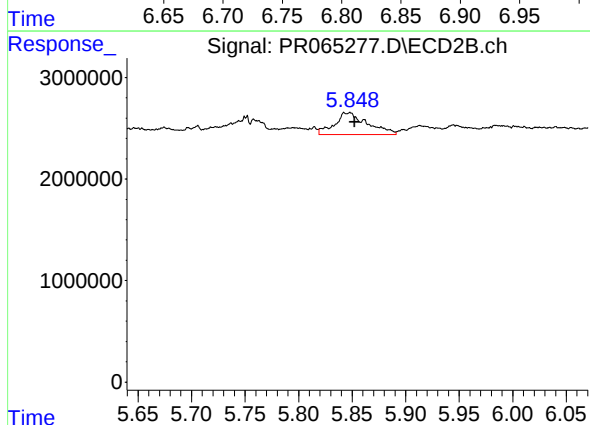


#29 AR-1254-4

R.T.: 5.846 min
Delta R.T.: -0.006 min
Response: 4566305
Conc: 17.79 ng/ml

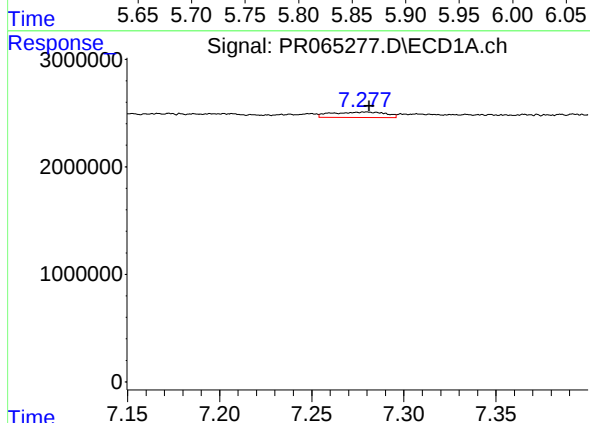


#30 AR-1254-5

R.T.: 7.279 min
Delta R.T.: -0.002 min
Response: 1033719
Conc: 4.16 ng/ml

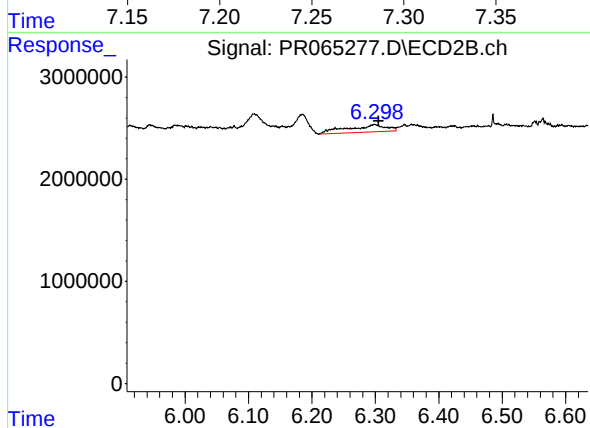

#30 AR-1254-5


R.T.: 6.299 min
Delta R.T.: -0.007 min
Response: 3057821
Conc: 8.34 ng/ml

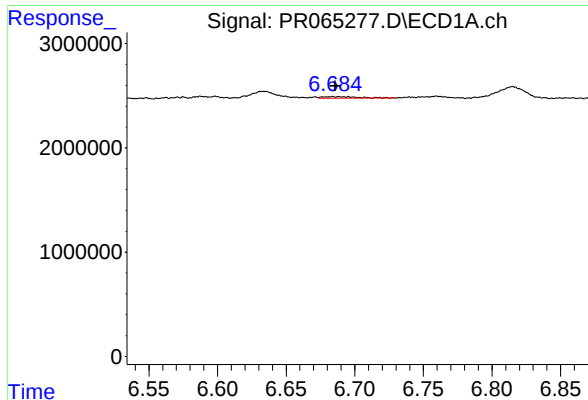

#31 AR-1260-1


R.T.: 6.684 min
Delta R.T.: -0.002 min
Response: 233357
Conc: 0.93 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

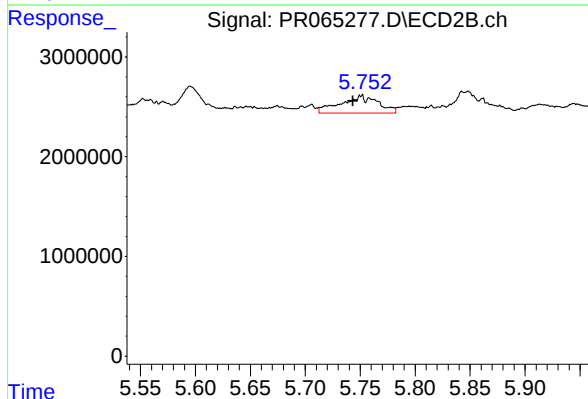


#31 AR-1260-1

R.T.: 5.750 min
Delta R.T.: 0.007 min
Response: 4107760
Conc: 14.39 ng/ml

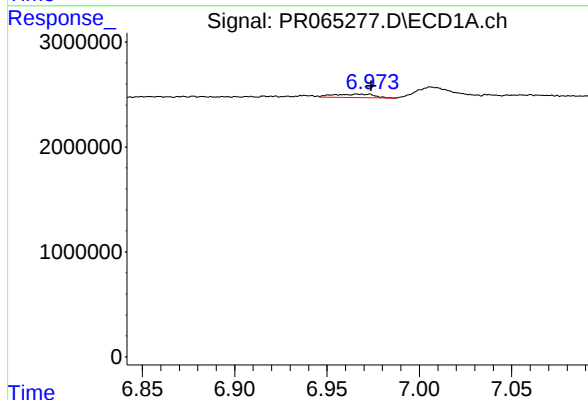


#32 AR-1260-2

R.T.: 6.972 min
Delta R.T.: -0.002 min
Response: 487786
Conc: 1.70 ng/ml

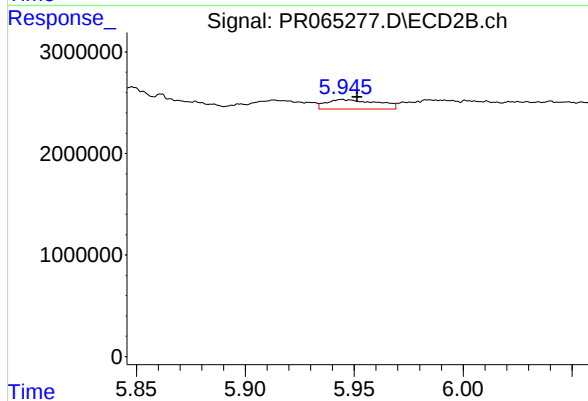

#32 AR-1260-2


R.T.: 5.946 min
Delta R.T.: -0.006 min
Response: 1492479
Conc: 4.30 ng/ml

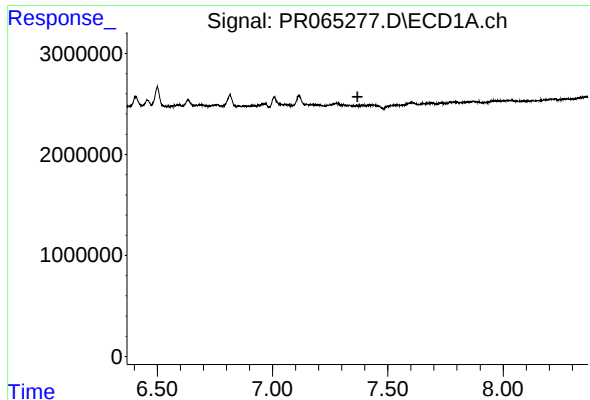

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

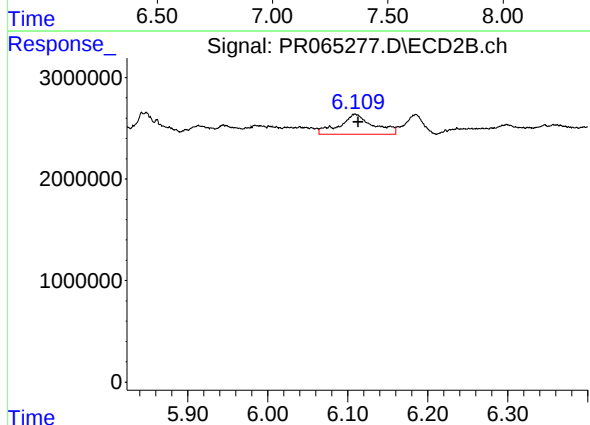


#33 AR-1260-3

R.T.: 6.110 min
Delta R.T.: -0.004 min
Response: 5824801
Conc: 17.93 ng/ml

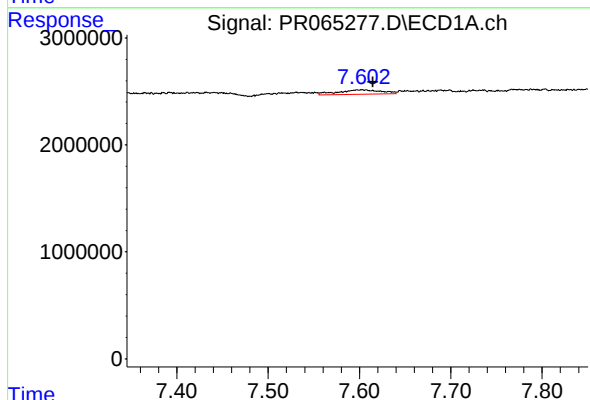


#34 AR-1260-4

R.T.: 7.603 min
Delta R.T.: -0.012 min
Response: 1349879
Conc: 5.72 ng/ml

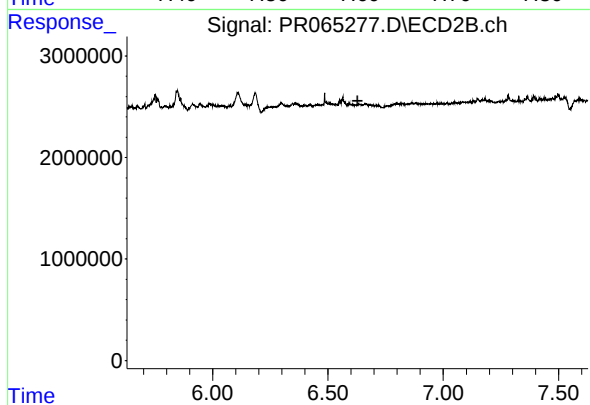

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 6.628 min
Response: 0
Conc: N.D.

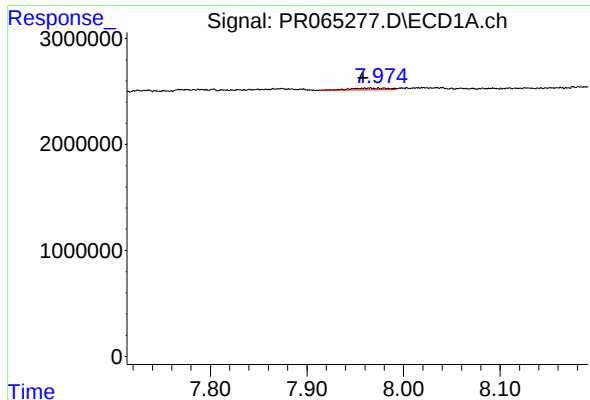

#35 AR-1260-5


R.T.: 7.965 min
Delta R.T.: 0.007 min
Response: 442674
Conc: 1.01 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

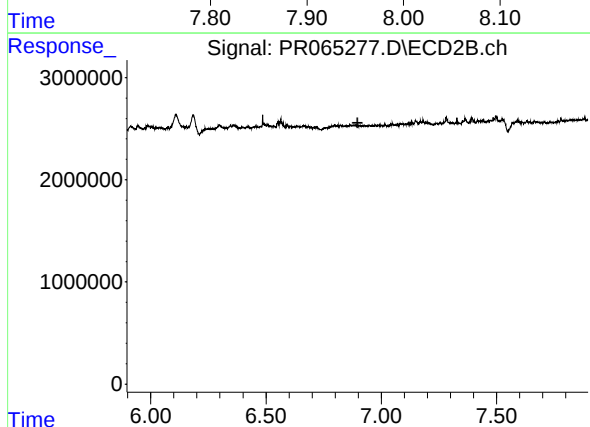


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 6.897 min
Response: 0
Conc: N.D.

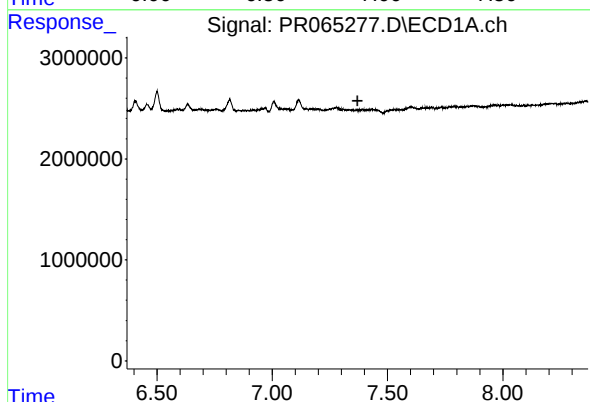


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.370 min
Response: 0
Conc: N.D.

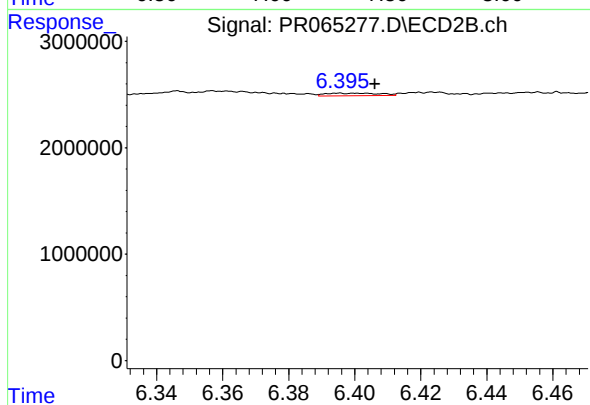

#36 AR-1262-1


R.T.: 6.399 min
Delta R.T.: -0.007 min
Response: 265615
Conc: 1.48 ng/ml

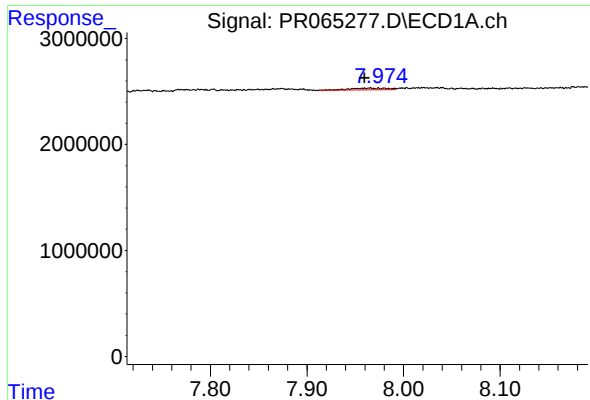

#37 AR-1262-2


R.T.: 7.965 min
Delta R.T.: 0.006 min
Response: 442674
Conc: 0.78 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

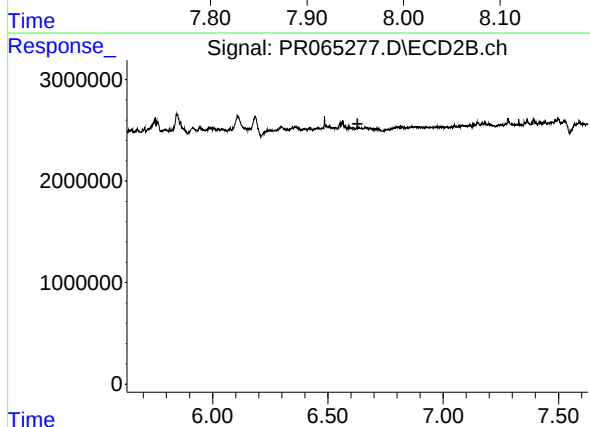


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 6.628 min
Response: 0
Conc: N.D.

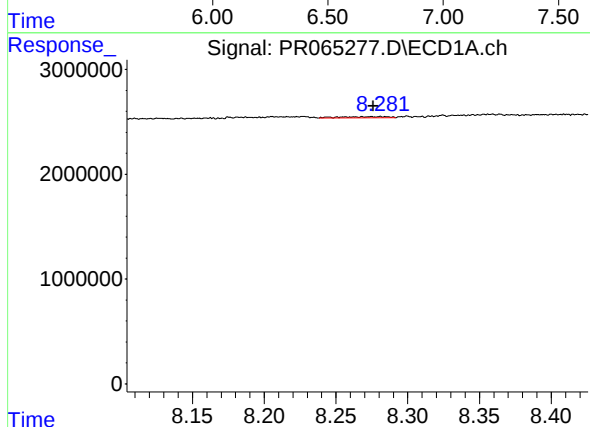


#38 AR-1262-3

R.T.: 8.281 min
Delta R.T.: 0.005 min
Response: 237315
Conc: 0.62 ng/ml

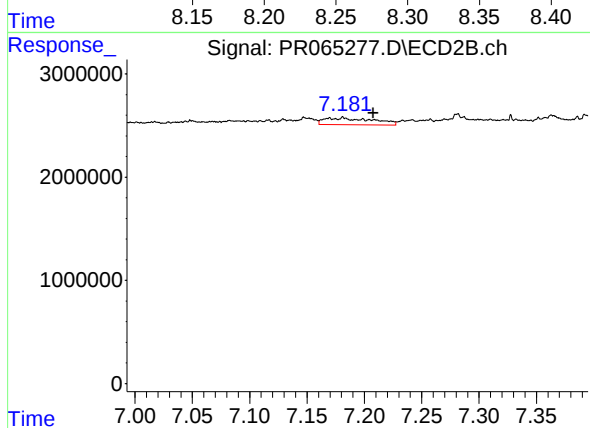

#38 AR-1262-3


R.T.: 7.181 min
Delta R.T.: -0.026 min
Response: 1981621
Conc: 6.99 ng/ml

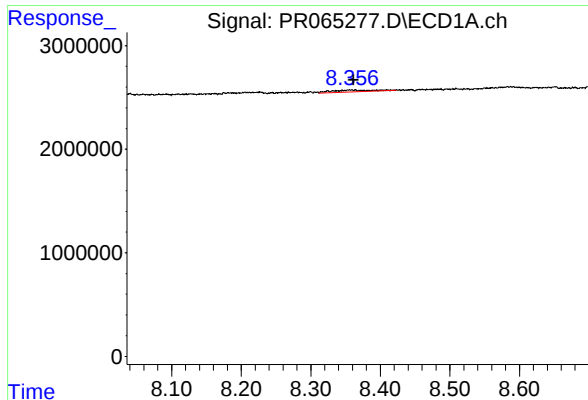

#39 AR-1262-4


R.T.: 8.357 min
Delta R.T.: -0.004 min
Response: 684572
Conc: 2.34 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

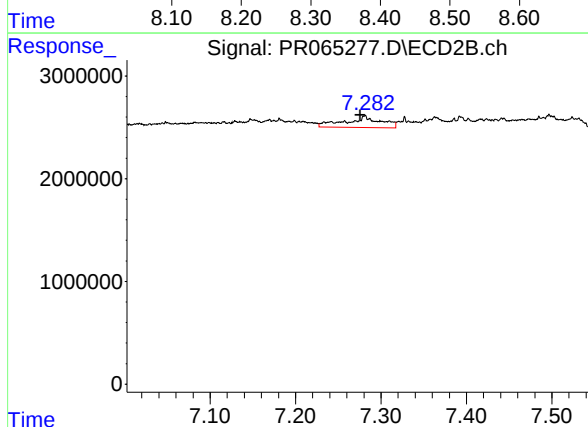


#39 AR-1262-4

R.T.: 7.282 min
Delta R.T.: 0.006 min
Response: 3129856
Conc: 5.43 ng/ml

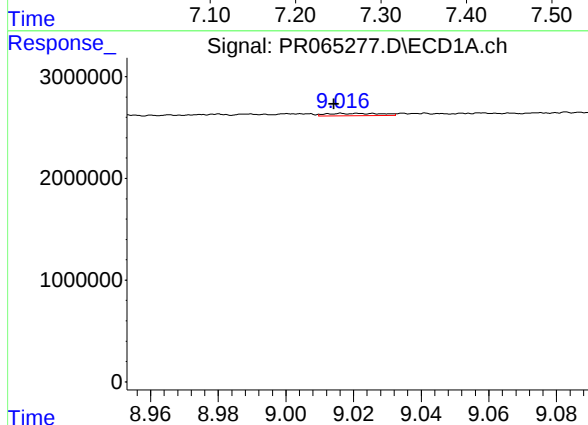


#40 AR-1262-5

R.T.: 9.021 min
Delta R.T.: 0.007 min
Response: 252519
Conc: 1.26 ng/ml

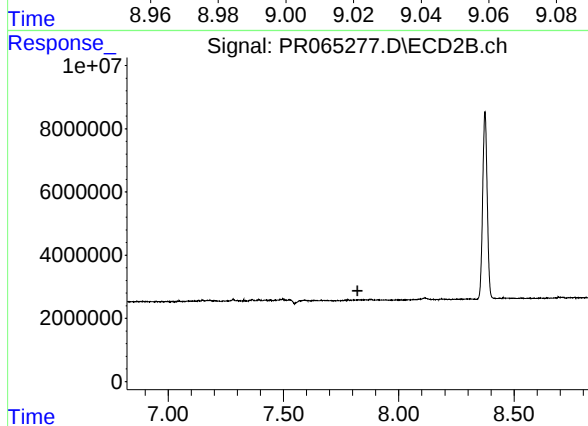

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 7.821 min
Response: 0
Conc: N.D.

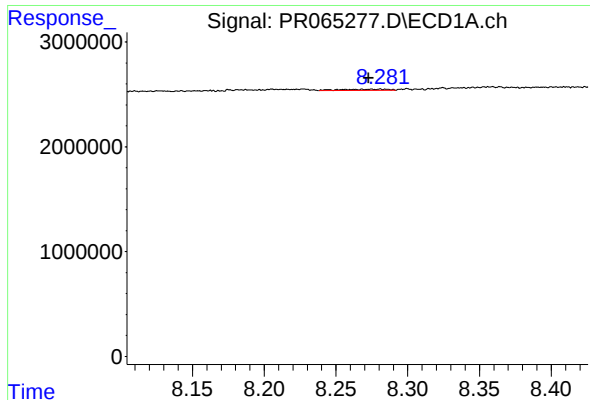

#41 AR-1268-1


R.T.: 8.281 min
Delta R.T.: 0.008 min
Response: 237315
Conc: 0.39 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

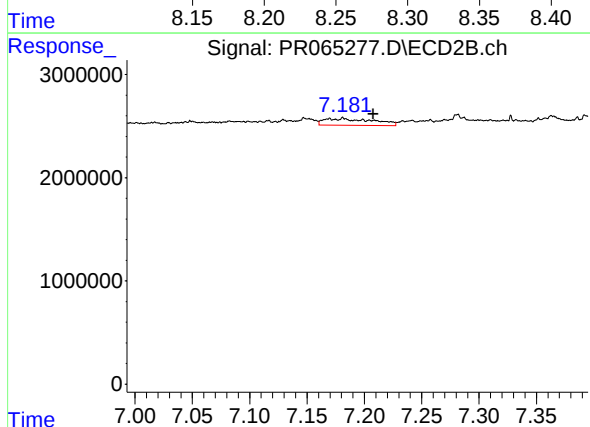


#41 AR-1268-1

R.T.: 7.181 min
Delta R.T.: -0.027 min
Response: 1981621
Conc: 2.50 ng/ml

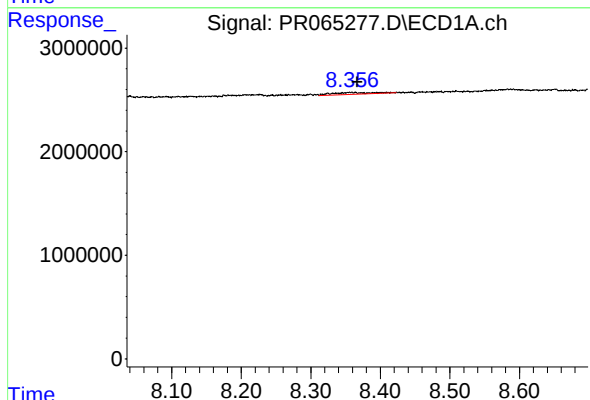


#42 AR-1268-2

R.T.: 8.357 min
Delta R.T.: -0.009 min
Response: 684572
Conc: 1.25 ng/ml

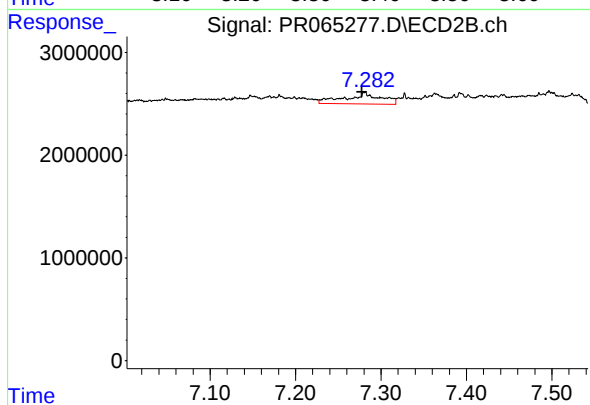

#42 AR-1268-2


R.T.: 7.282 min
Delta R.T.: 0.004 min
Response: 3129856
Conc: 4.20 ng/ml

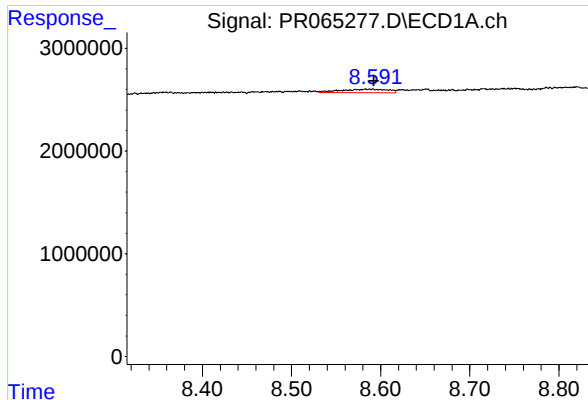

#43 AR-1268-3


R.T.: 8.588 min
Delta R.T.: -0.005 min
Response: 1282530
Conc: 2.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

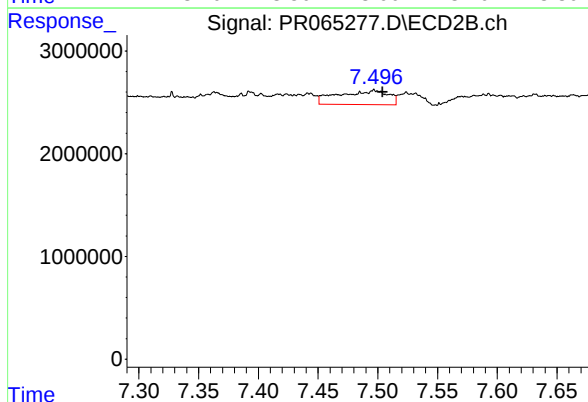


#43 AR-1268-3

R.T.: 7.498 min
Delta R.T.: -0.007 min
Response: 3963833
Conc: 6.26 ng/ml

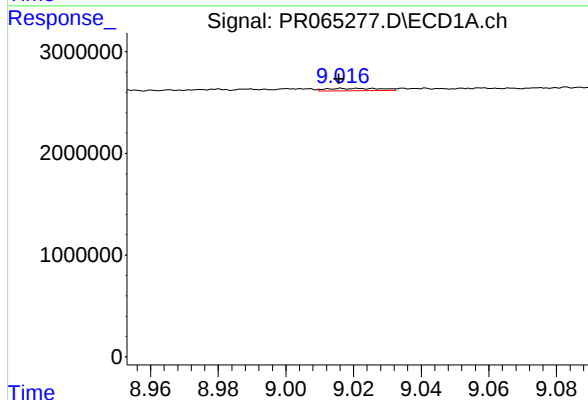


#44 AR-1268-4

R.T.: 9.021 min
Delta R.T.: 0.006 min
Response: 252519
Conc: 1.24 ng/ml

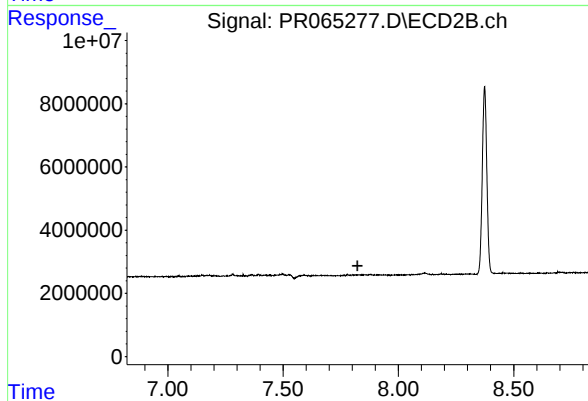

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 7.823 min
Response: 0
Conc: N.D.

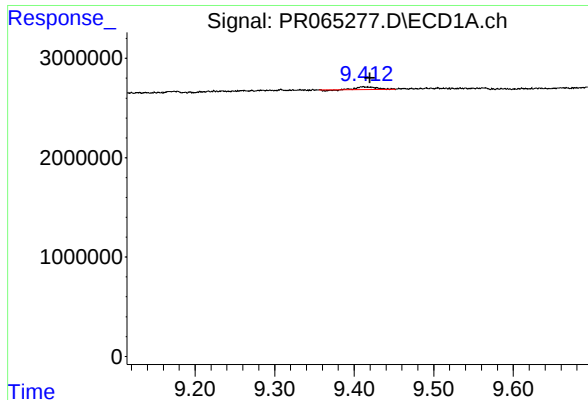

#45 AR-1268-5

R.T.: 9.412 min
Delta R.T.: -0.008 min
Response: 444390
Conc: 0.30 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

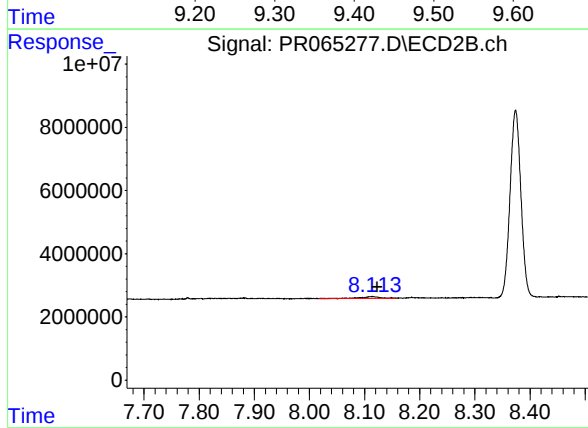

#45 AR-1268-5

R.T.: 8.114 min
Delta R.T.: -0.009 min
Response: 1507367
Conc: 0.79 ng/ml