

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
 Data File : PR065278.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 19:06
 Operator : AJ\MA
 Sample : P1187-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:34:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.701	3.003	116.9E6	112.0E6	19.592	20.483
2) SA Decachlor...	9.740	8.373	84454918	94758466	21.116	20.022
Target Compounds						
3) L1 AR-1016-1	4.945	4.147	438315	659955	2.473	3.634 #
4) L1 AR-1016-2	4.976	4.180	538542	79564	2.066	0.322 #
5) L1 AR-1016-3	5.058f	4.349	1408555	706957	8.428	5.214 #
6) L1 AR-1016-4	5.133	4.401	534834	3382169	3.989	32.295 #
7) L1 AR-1016-5	5.454	4.624	1542954	2023809	11.427	14.507 #
8) L2 AR-1221-1	3.914	0.000	999224	0	13.922	N.D. #
9) L2 AR-1221-2	4.016	3.313	1861609	1834413	35.511	38.461
10) L2 AR-1221-3	4.069f	3.400	1055346	614446	6.869	4.448 #
11) L3 AR-1232-1	4.069f	3.400	1055346	614446	7.808	5.131 #
12) L3 AR-1232-2	4.638f	4.180	794584	79564	10.314	0.651 #
13) L3 AR-1232-3	4.976	4.349	538542	706957	4.223	10.628 #
14) L3 AR-1232-4	5.133	4.444	534834	1156911	8.160	20.204 #
15) L3 AR-1232-5	5.238	4.624	3037021	2023809	62.792	31.750 #
16) L4 AR-1242-1	4.945	4.147	438315	659955	3.066	4.516 #
17) L4 AR-1242-2	4.976	4.180	538542	79564	2.557	0.399 #
18) L4 AR-1242-3	5.058f	4.349	1408555	706957	10.401	6.456 #
19) L4 AR-1242-4	5.133	4.444	534834	1156911	4.922	11.020 #
20) L4 AR-1242-5	5.935	5.003	1643308	7200952	14.527	53.332 #
21) L5 AR-1248-1	4.945	4.147	438315	659955	4.120	6.110 #
22) L5 AR-1248-2	5.238	4.401	3037021	3382169	19.546	23.354
23) L5 AR-1248-3	5.454	4.444	1542954	1156911	8.641	7.476
24) L5 AR-1248-4	5.892	4.624	2082186	2023809	10.983	10.807
25) L5 AR-1248-5	5.935	5.045	1643308	1884131	8.624	10.123
26) L6 AR-1254-1	5.864	5.003	6153041	7200952	30.042	24.713
27) L6 AR-1254-2	6.104	5.164	8501762	7436975	27.277	29.357
28) L6 AR-1254-3	6.500	5.595	8938562	9951014	27.941	24.321
29) L6 AR-1254-4	6.817	5.847	6506976	7563813	28.396	29.463
30) L6 AR-1254-5	7.280	6.300	6938562	10739760	27.918	29.298
31) L7 AR-1260-1	6.684	5.741	4423035	5930279	17.595	20.776
32) L7 AR-1260-2	6.972	5.948	4197044	4784374	14.604	13.797
33) L7 AR-1260-3	7.341f	6.107	963248	7635424	4.556	23.502 #
34) L7 AR-1260-4	7.593f	6.613f	3438834	615751	14.573	2.331 #
35) L7 AR-1260-5	7.956	6.891	954184	932807	2.170	1.513 #
36) L8 AR-1262-1	7.341f	6.415	963248	164815	2.846	0.919 #
37) L8 AR-1262-2	7.956	6.613f	954184	615751	1.687	1.583
38) L8 AR-1262-3	8.279	7.207	850740	416968	2.236	1.471 #
39) L8 AR-1262-4	8.363	7.265	358522	1905448	1.224	3.309 #
40) L8 AR-1262-5	9.014	7.839f	134002	757666	0.669	2.911 #
41) L9 AR-1268-1	8.279	7.207	850740	416968	1.403	0.526 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
 Data File : PR065278.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 19:06
 Operator : AJ\MA
 Sample : P1187-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:34:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.363	7.265	358522	1905448	0.655	2.559 #
43) L9	AR-1268-3	8.580	7.497	976243	4106507	2.057	6.482 #
44) L9	AR-1268-4	9.014	7.839f	134002	757666	0.659	2.888 #
45) L9	AR-1268-5	9.416	8.114	937974	1060113	0.643	0.554



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
Data File : PR065278.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 19:06
Operator : AJ\MA
Sample : P1187-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 69 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:34:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

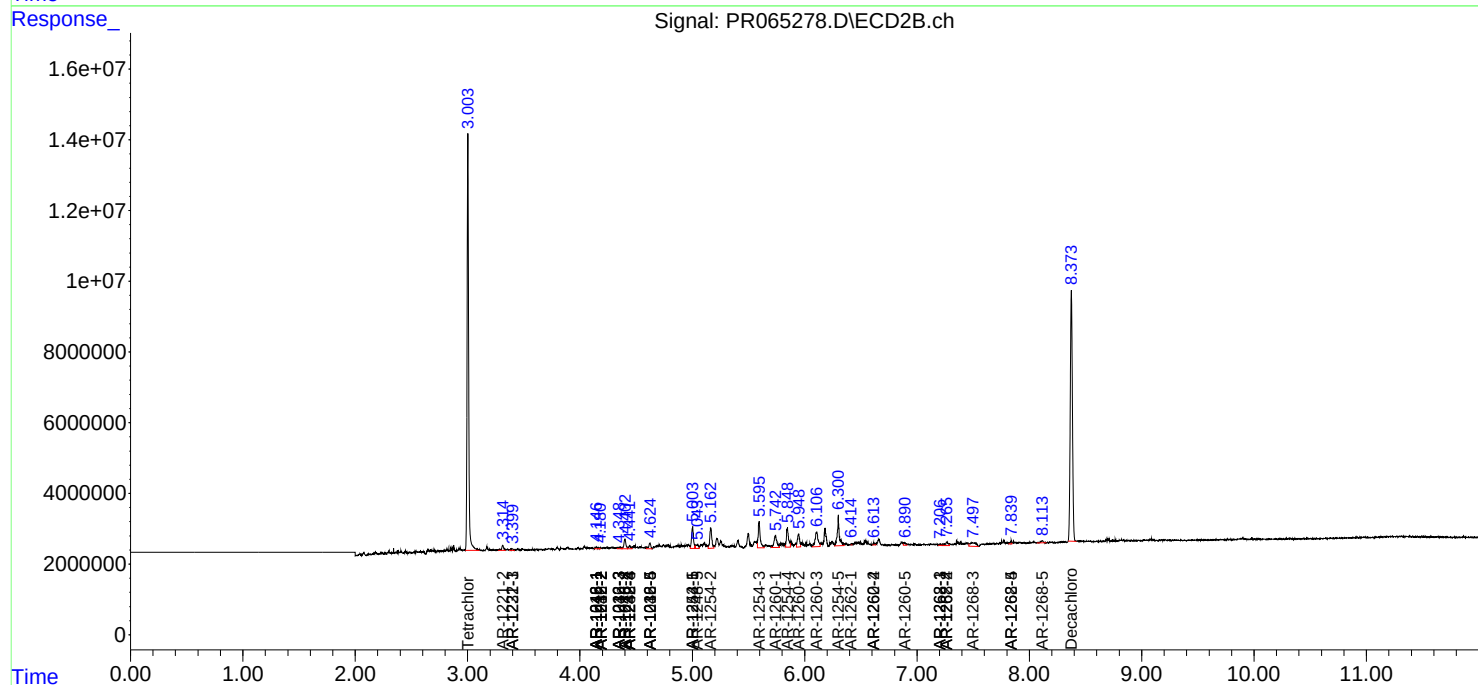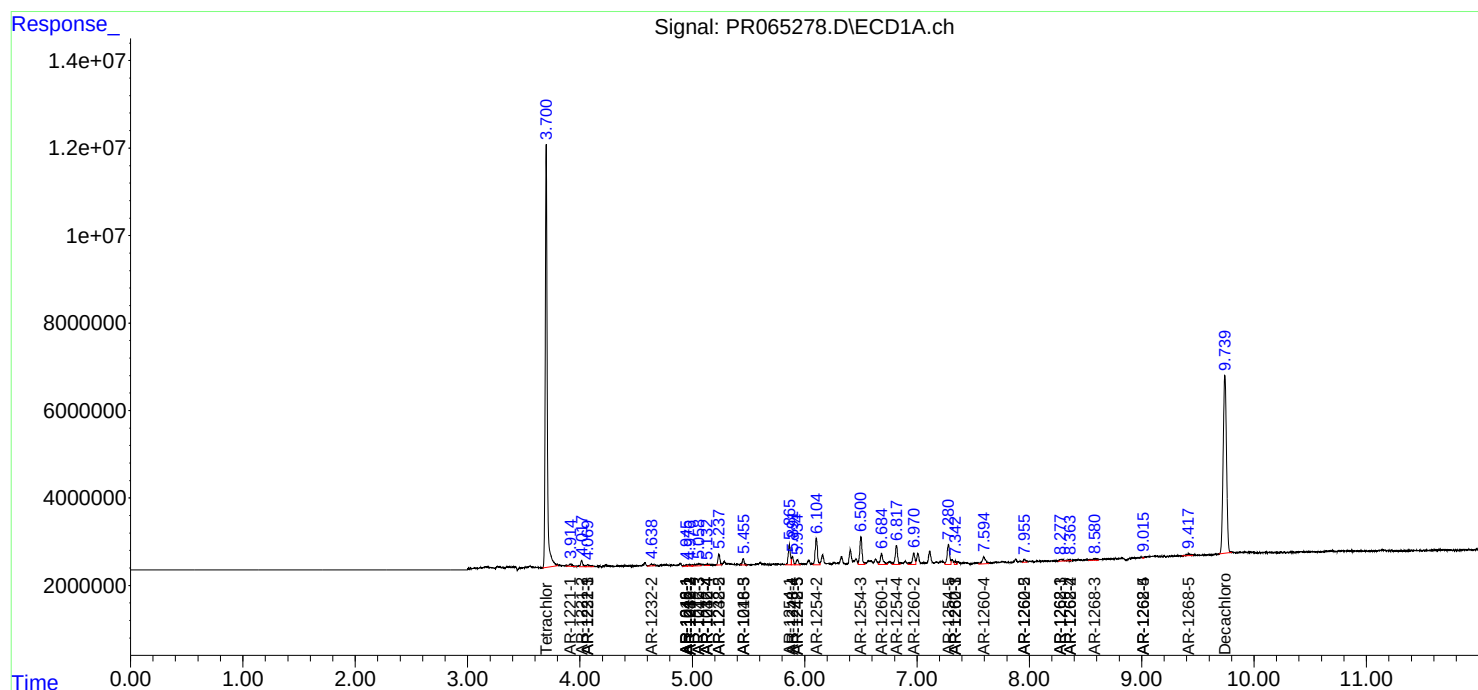


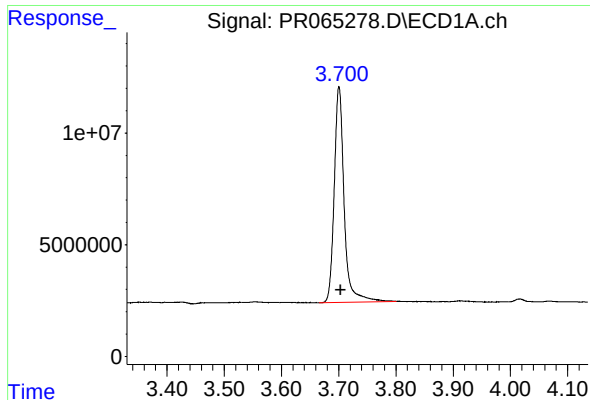

#1 Tetrachloro-m-xylene


R.T.: 3.701 min
Delta R.T.: -0.002 min
Response: 116946441
Conc: 19.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

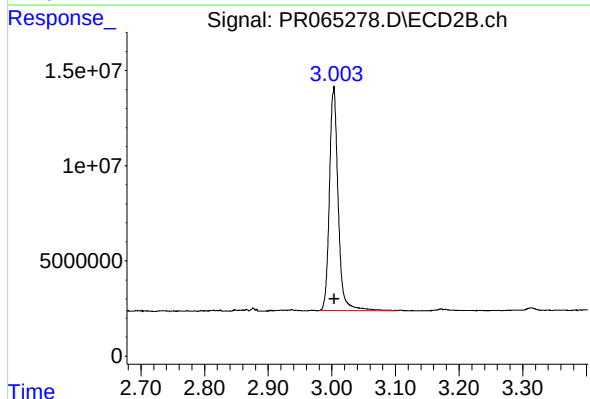


#1 Tetrachloro-m-xylene

R.T.: 3.003 min
Delta R.T.: -0.001 min
Response: 112038631
Conc: 20.48 ng/ml

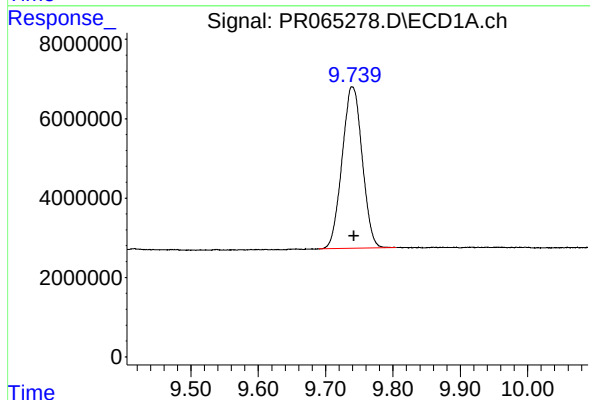


#2 Decachlorobiphenyl

R.T.: 9.740 min
Delta R.T.: -0.003 min
Response: 84454918
Conc: 21.12 ng/ml

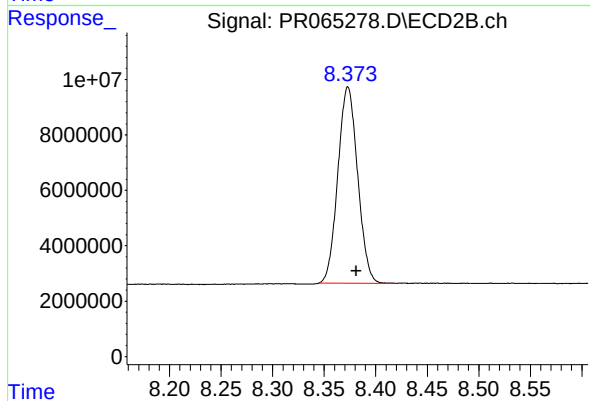

#2 Decachlorobiphenyl


R.T.: 8.373 min
Delta R.T.: -0.008 min
Response: 94758466
Conc: 20.02 ng/ml

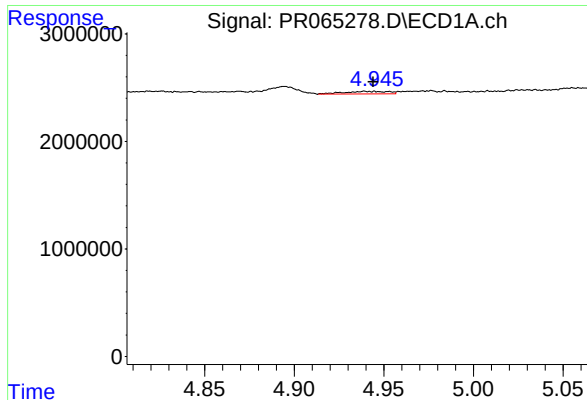

#3 AR-1016-1


R.T.: 4.945 min
Delta R.T.: 0.000 min
Response: 438315
Conc: 2.47 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

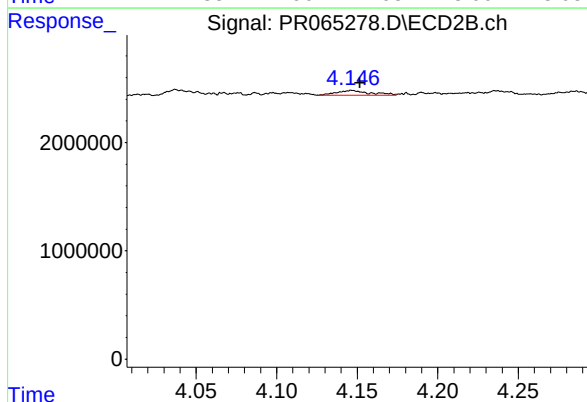


#3 AR-1016-1

R.T.: 4.147 min
Delta R.T.: -0.005 min
Response: 659955
Conc: 3.63 ng/ml

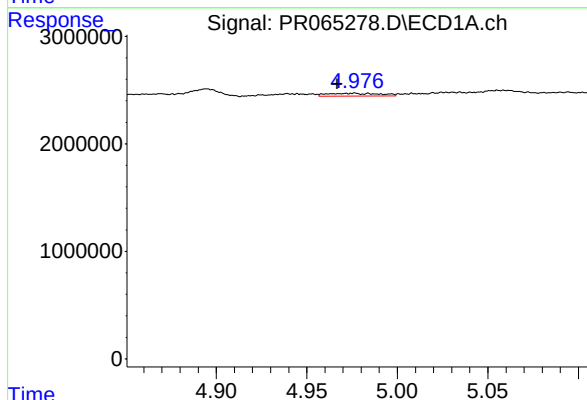


#4 AR-1016-2

R.T.: 4.976 min
Delta R.T.: 0.010 min
Response: 538542
Conc: 2.07 ng/ml

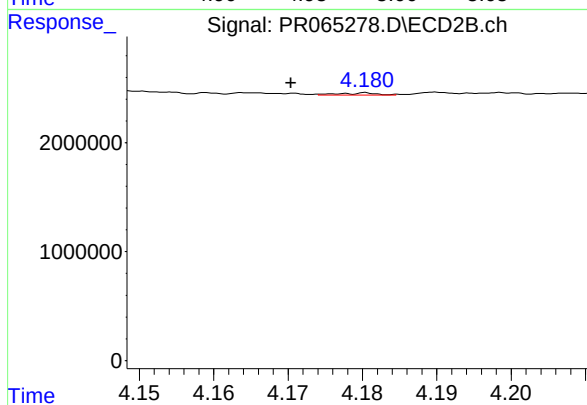

#4 AR-1016-2


R.T.: 4.180 min
Delta R.T.: 0.010 min
Response: 79564
Conc: 0.32 ng/ml

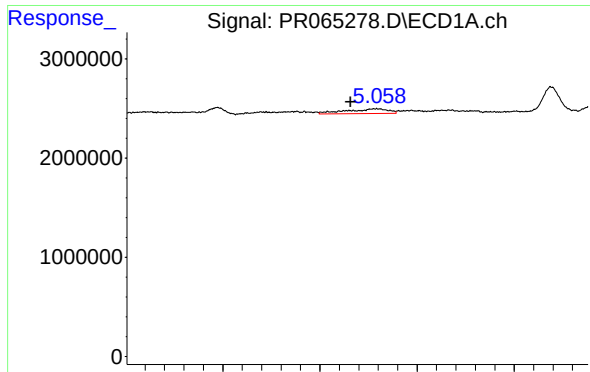

#5 AR-1016-3


R.T.: 5.058 min
Delta R.T.: 0.027 min
Response: 1408555
Conc: 8.43 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

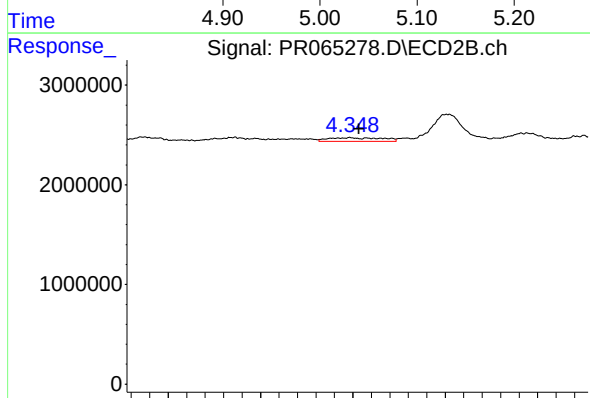


#5 AR-1016-3

R.T.: 4.349 min
Delta R.T.: -0.005 min
Response: 706957
Conc: 5.21 ng/ml

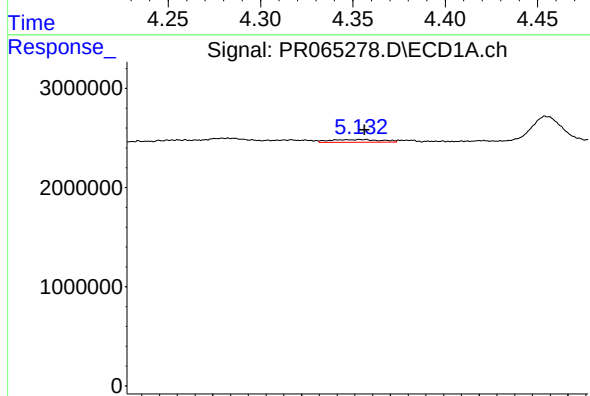


#6 AR-1016-4

R.T.: 5.133 min
Delta R.T.: -0.002 min
Response: 534834
Conc: 3.99 ng/ml

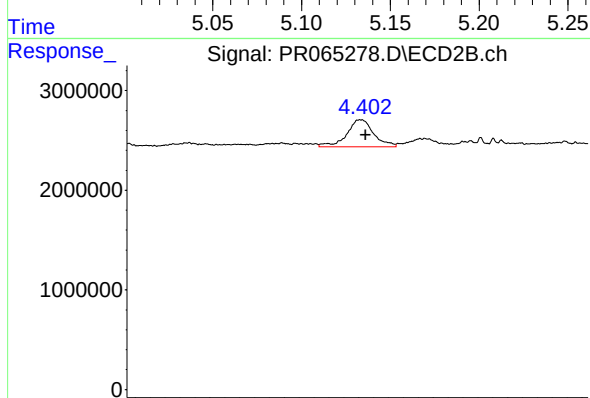

#6 AR-1016-4


R.T.: 4.401 min
Delta R.T.: -0.004 min
Response: 3382169
Conc: 32.30 ng/ml

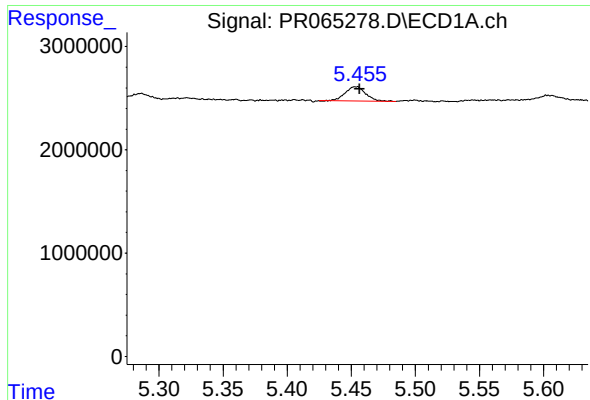

#7 AR-1016-5


R.T.: 5.454 min
Delta R.T.: -0.003 min
Response: 1542954
Conc: 11.43 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

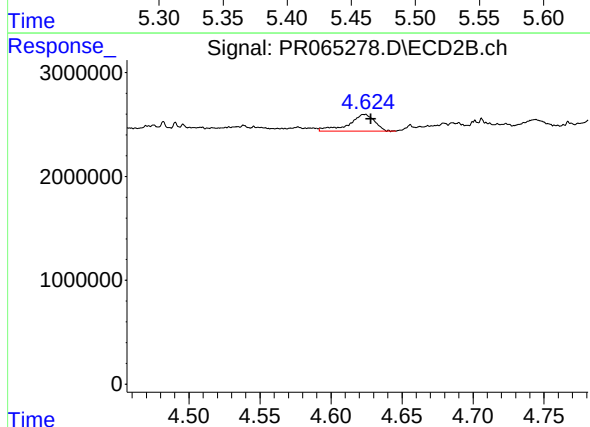


#7 AR-1016-5

R.T.: 4.624 min
Delta R.T.: -0.004 min
Response: 2023809
Conc: 14.51 ng/ml

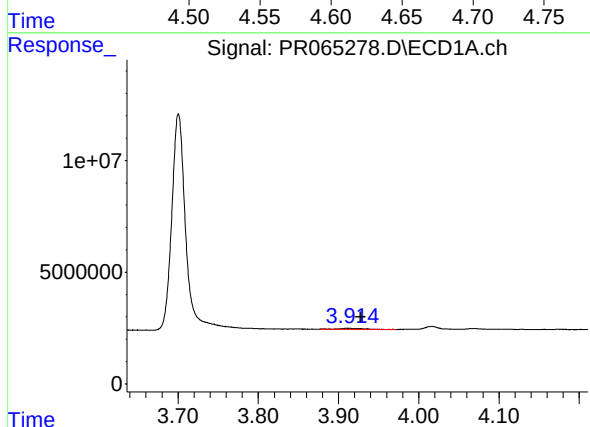


#8 AR-1221-1

R.T.: 3.914 min
Delta R.T.: -0.013 min
Response: 999224
Conc: 13.92 ng/ml

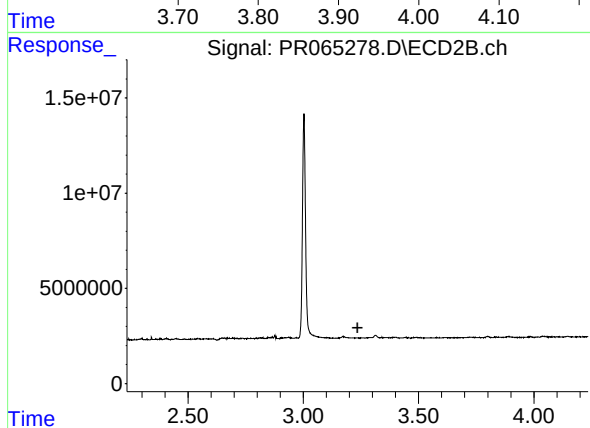

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 3.235 min
Response: 0
Conc: N.D.

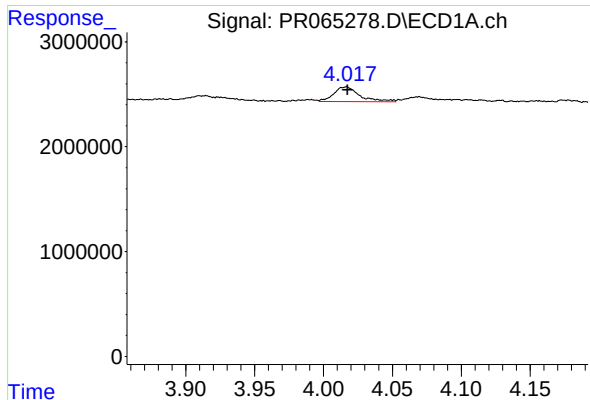

#9 AR-1221-2


R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 1861609
Conc: 35.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

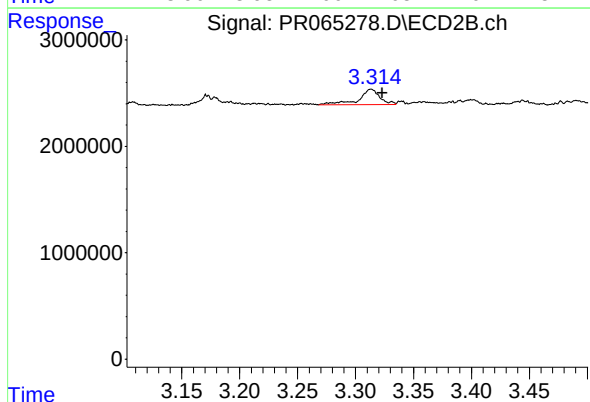


#9 AR-1221-2

R.T.: 3.313 min
Delta R.T.: -0.010 min
Response: 1834413
Conc: 38.46 ng/ml

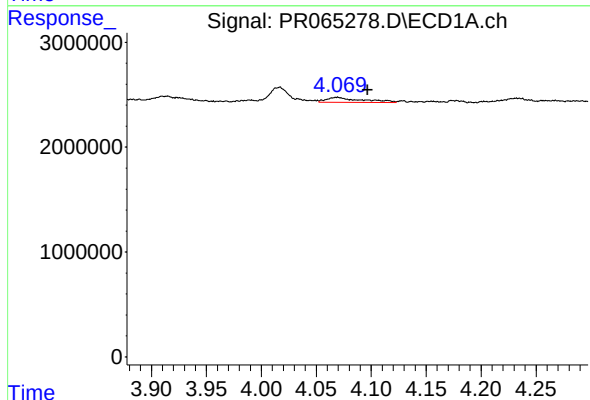


#10 AR-1221-3

R.T.: 4.069 min
Delta R.T.: -0.028 min
Response: 1055346
Conc: 6.87 ng/ml

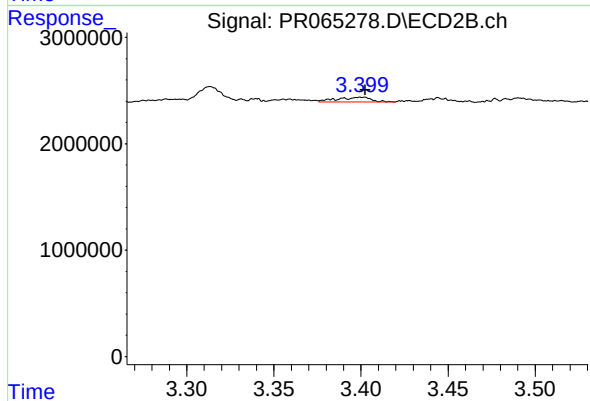

#10 AR-1221-3


R.T.: 3.400 min
Delta R.T.: -0.002 min
Response: 614446
Conc: 4.45 ng/ml

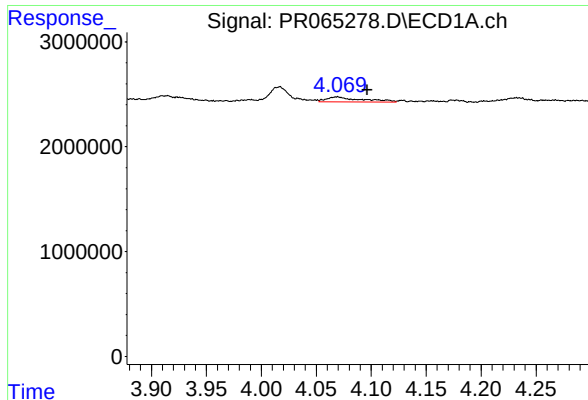

#11 AR-1232-1


R.T.: 4.069 min
Delta R.T.: -0.027 min
Response: 1055346
Conc: 7.81 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

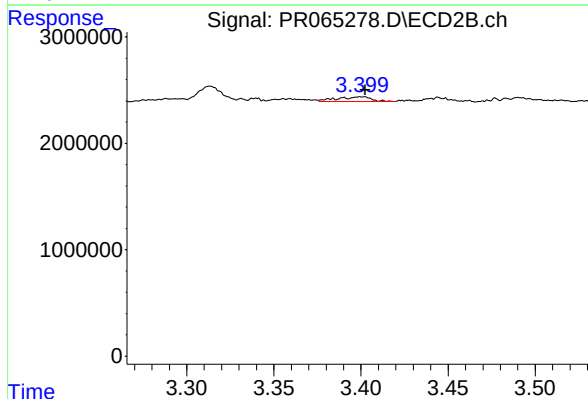


#11 AR-1232-1

R.T.: 3.400 min
Delta R.T.: -0.002 min
Response: 614446
Conc: 5.13 ng/ml

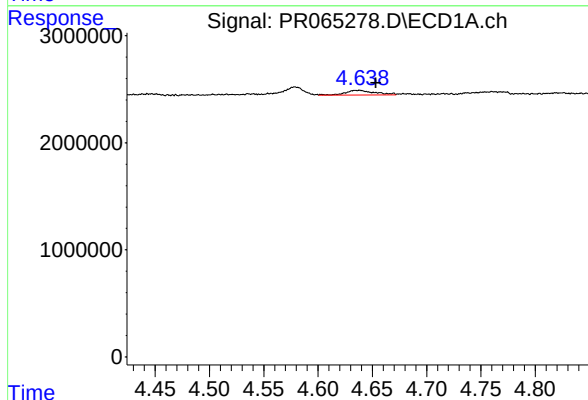


#12 AR-1232-2

R.T.: 4.638 min
Delta R.T.: -0.015 min
Response: 794584
Conc: 10.31 ng/ml

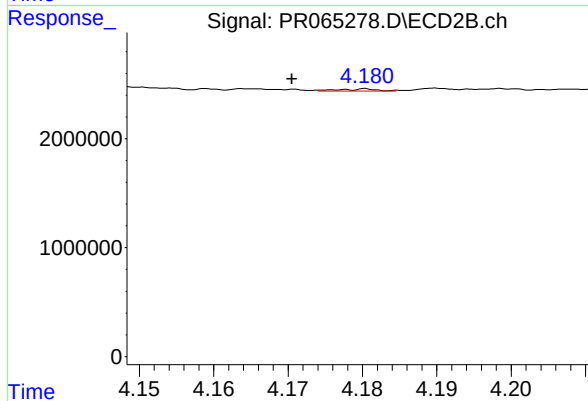

#12 AR-1232-2


R.T.: 4.180 min
Delta R.T.: 0.010 min
Response: 79564
Conc: 0.65 ng/ml

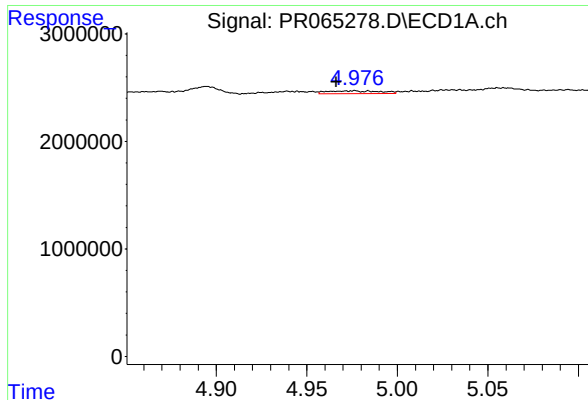

#13 AR-1232-3


R.T.: 4.976 min
Delta R.T.: 0.010 min
Response: 538542
Conc: 4.22 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

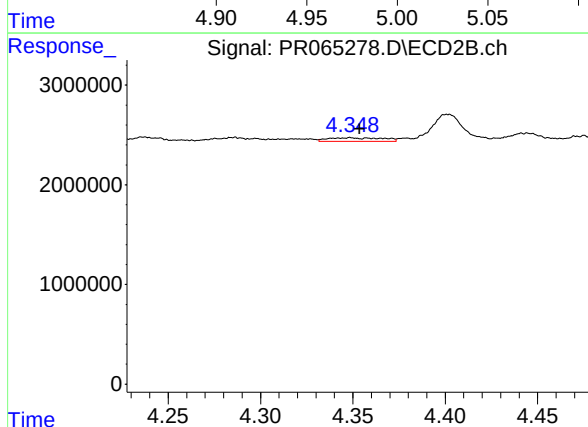


#13 AR-1232-3

R.T.: 4.349 min
Delta R.T.: -0.005 min
Response: 706957
Conc: 10.63 ng/ml

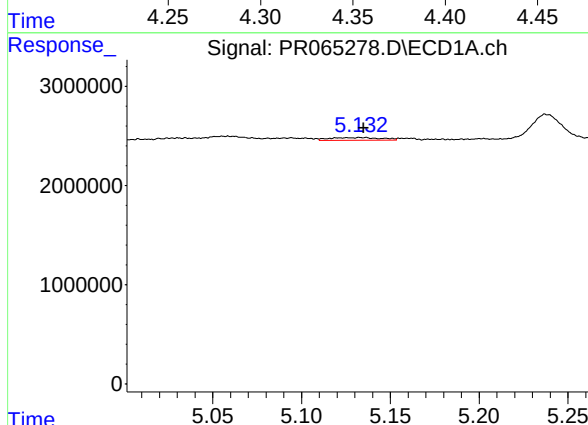


#14 AR-1232-4

R.T.: 5.133 min
Delta R.T.: -0.002 min
Response: 534834
Conc: 8.16 ng/ml

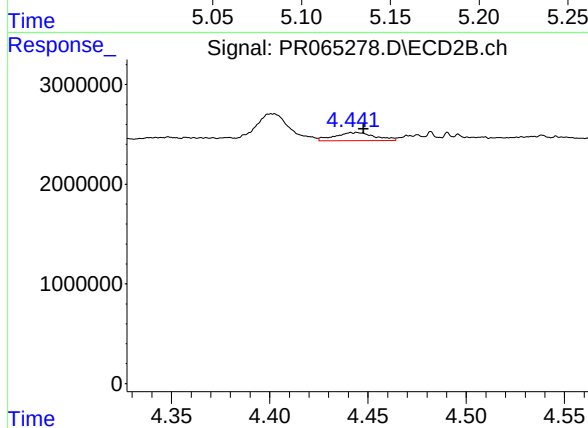

#14 AR-1232-4


R.T.: 4.444 min
Delta R.T.: -0.004 min
Response: 1156911
Conc: 20.20 ng/ml

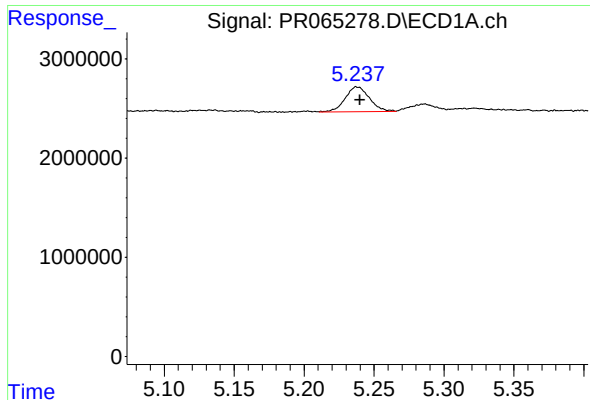

#15 AR-1232-5


R.T.: 5.238 min
Delta R.T.: -0.002 min
Response: 3037021
Conc: 62.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

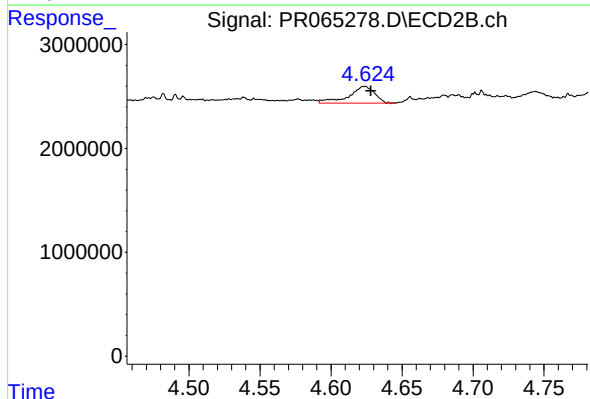


#15 AR-1232-5

R.T.: 4.624 min
Delta R.T.: -0.005 min
Response: 2023809
Conc: 31.75 ng/ml

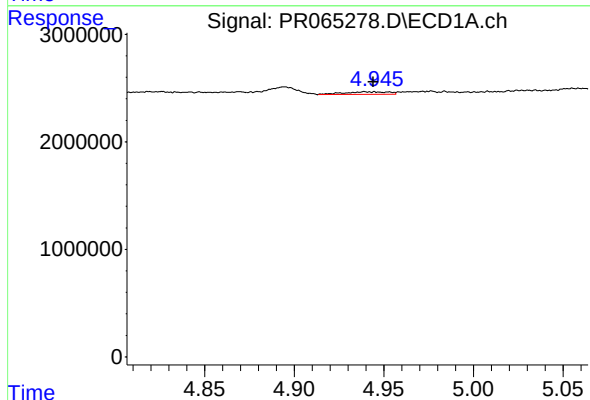


#16 AR-1242-1

R.T.: 4.945 min
Delta R.T.: 0.000 min
Response: 438315
Conc: 3.07 ng/ml

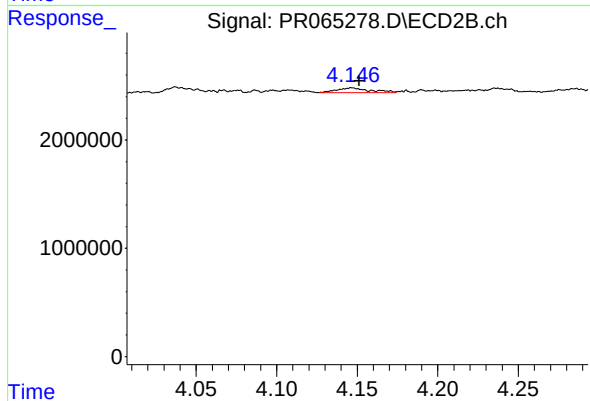

#16 AR-1242-1


R.T.: 4.147 min
Delta R.T.: -0.005 min
Response: 659955
Conc: 4.52 ng/ml

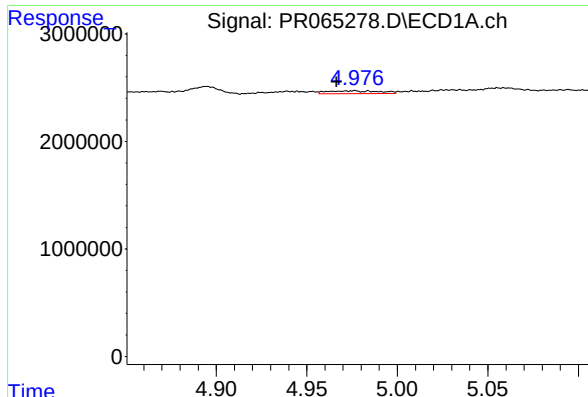

#17 AR-1242-2


R.T.: 4.976 min
Delta R.T.: 0.010 min
Response: 538542
Conc: 2.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

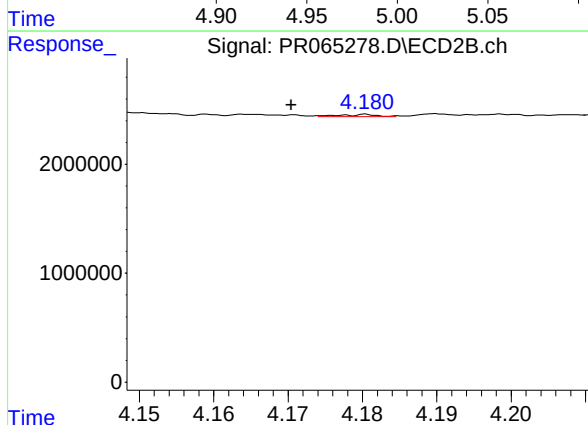


#17 AR-1242-2

R.T.: 4.180 min
Delta R.T.: 0.010 min
Response: 79564
Conc: 0.40 ng/ml

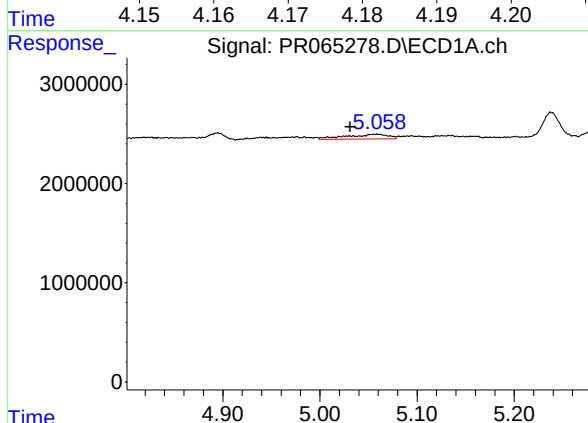


#18 AR-1242-3

R.T.: 5.058 min
Delta R.T.: 0.027 min
Response: 1408555
Conc: 10.40 ng/ml

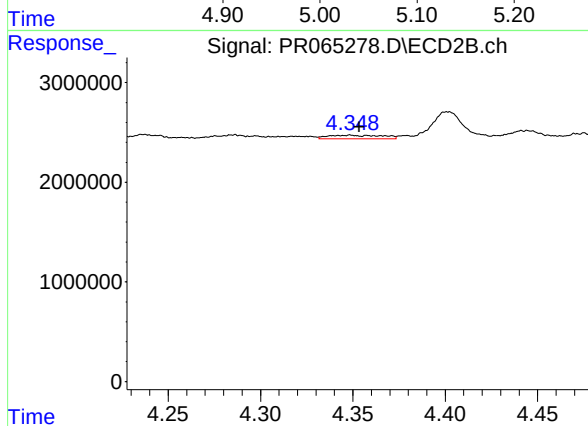

#18 AR-1242-3


R.T.: 4.349 min
Delta R.T.: -0.005 min
Response: 706957
Conc: 6.46 ng/ml

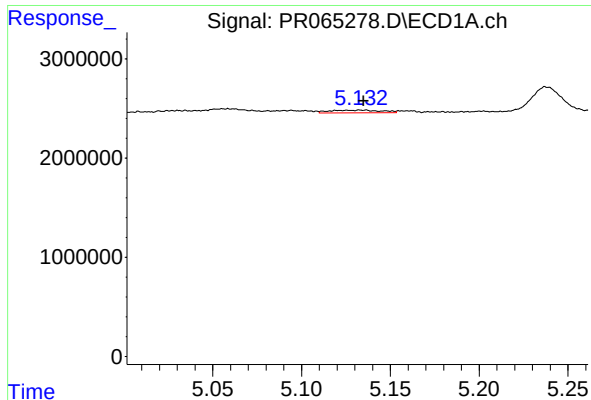

#19 AR-1242-4


R.T.: 5.133 min
Delta R.T.: -0.001 min
Response: 534834
Conc: 4.92 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

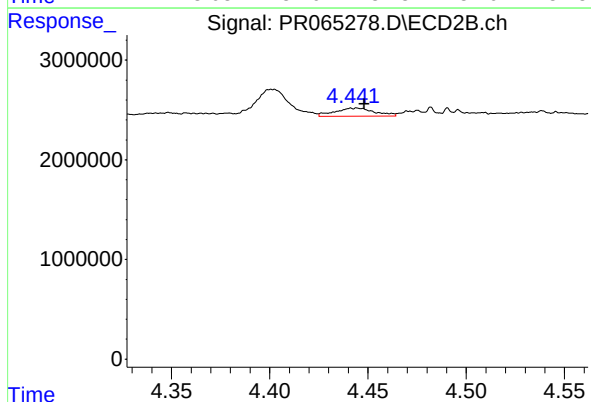


#19 AR-1242-4

R.T.: 4.444 min
Delta R.T.: -0.004 min
Response: 1156911
Conc: 11.02 ng/ml

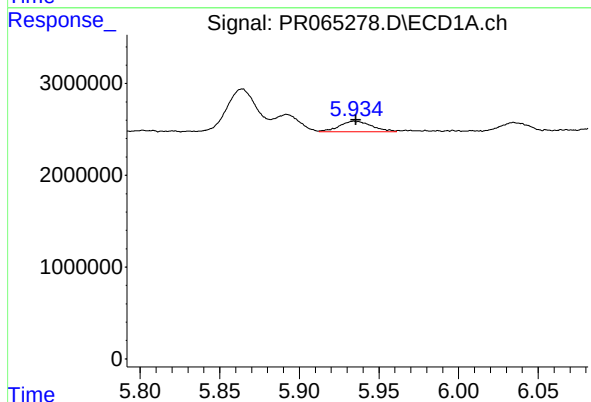


#20 AR-1242-5

R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 1643308
Conc: 14.53 ng/ml

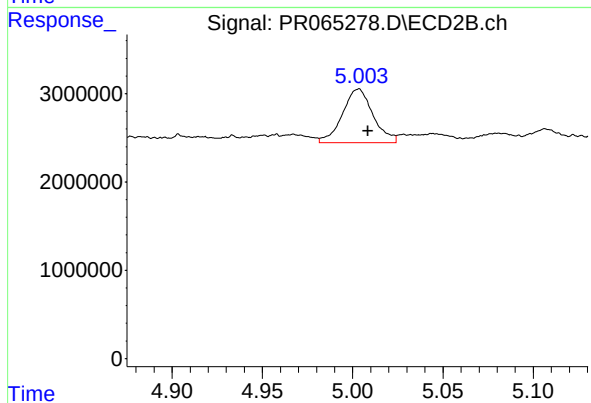

#20 AR-1242-5


R.T.: 5.003 min
Delta R.T.: -0.005 min
Response: 7200952
Conc: 53.33 ng/ml

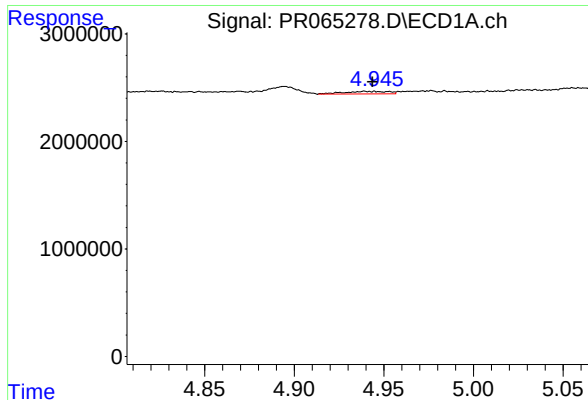

#21 AR-1248-1


R.T.: 4.945 min
Delta R.T.: 0.001 min
Response: 438315
Conc: 4.12 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

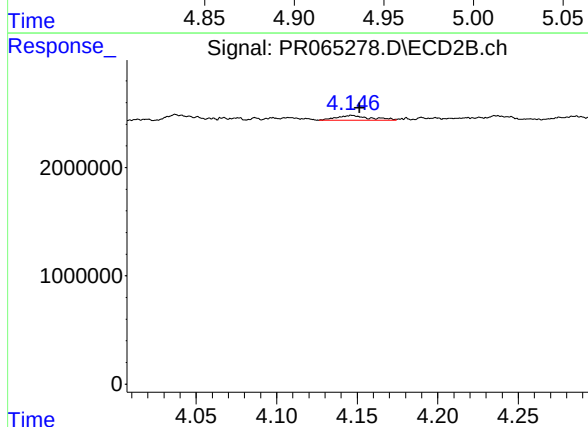


#21 AR-1248-1

R.T.: 4.147 min
Delta R.T.: -0.005 min
Response: 659955
Conc: 6.11 ng/ml

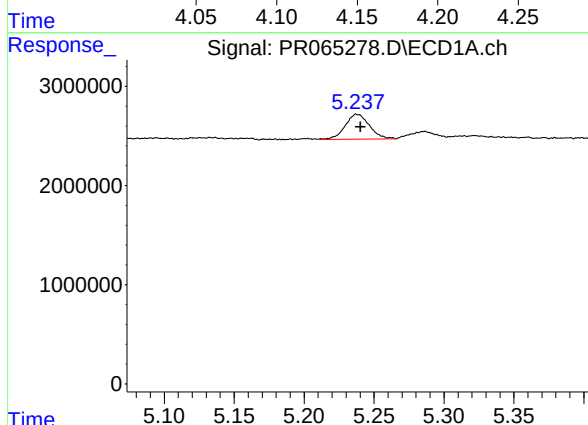


#22 AR-1248-2

R.T.: 5.238 min
Delta R.T.: -0.003 min
Response: 3037021
Conc: 19.55 ng/ml

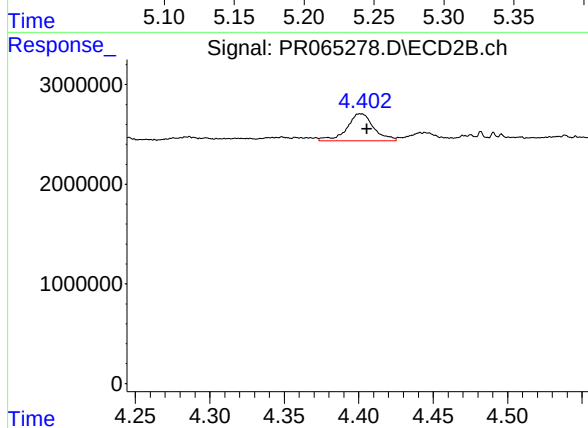

#22 AR-1248-2


R.T.: 4.401 min
Delta R.T.: -0.004 min
Response: 3382169
Conc: 23.35 ng/ml

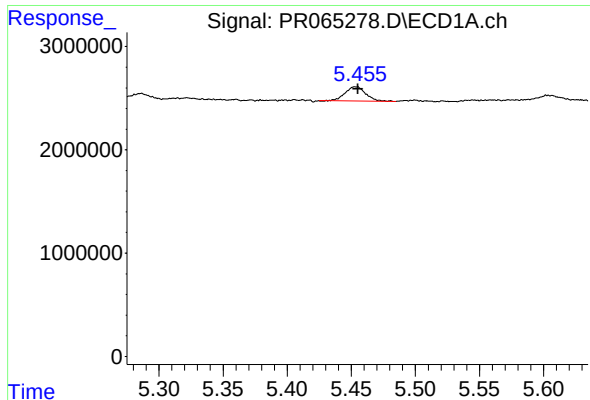

#23 AR-1248-3


R.T.: 5.454 min
Delta R.T.: -0.002 min
Response: 1542954
Conc: 8.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

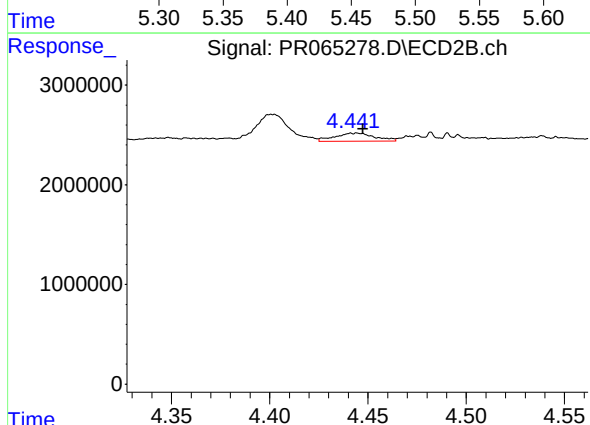


#23 AR-1248-3

R.T.: 4.444 min
Delta R.T.: -0.003 min
Response: 1156911
Conc: 7.48 ng/ml

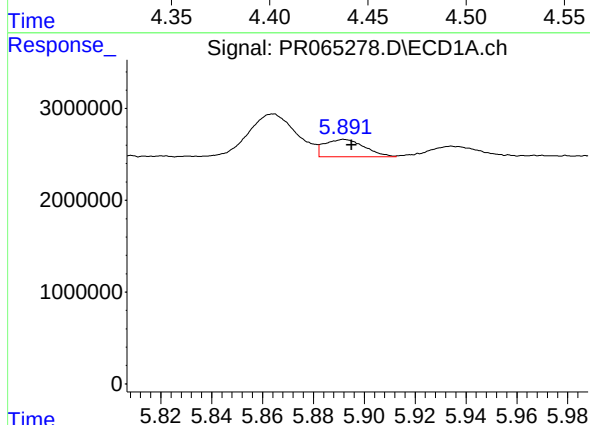


#24 AR-1248-4

R.T.: 5.892 min
Delta R.T.: -0.003 min
Response: 2082186
Conc: 10.98 ng/ml

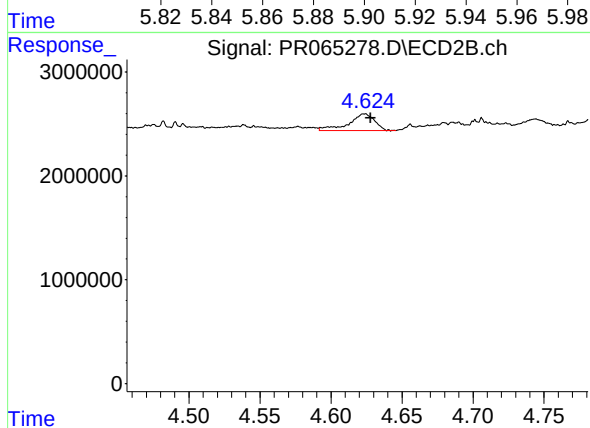

#24 AR-1248-4


R.T.: 4.624 min
Delta R.T.: -0.004 min
Response: 2023809
Conc: 10.81 ng/ml

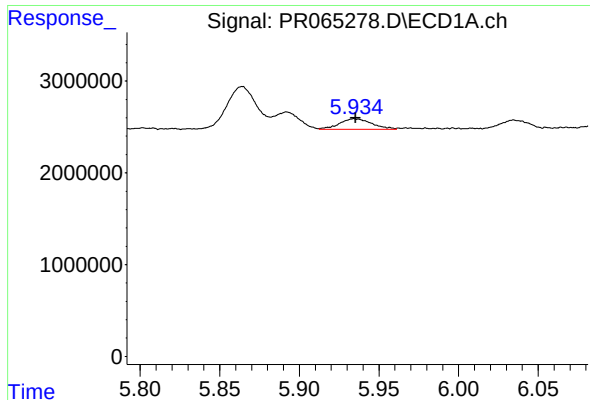

#25 AR-1248-5


R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 1643308
Conc: 8.62 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

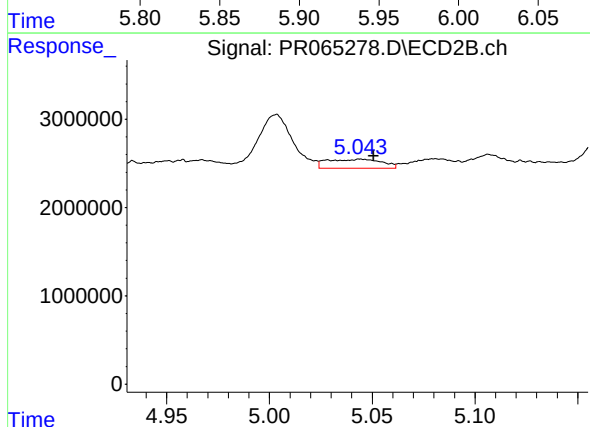


#25 AR-1248-5

R.T.: 5.045 min
Delta R.T.: -0.006 min
Response: 1884131
Conc: 10.12 ng/ml

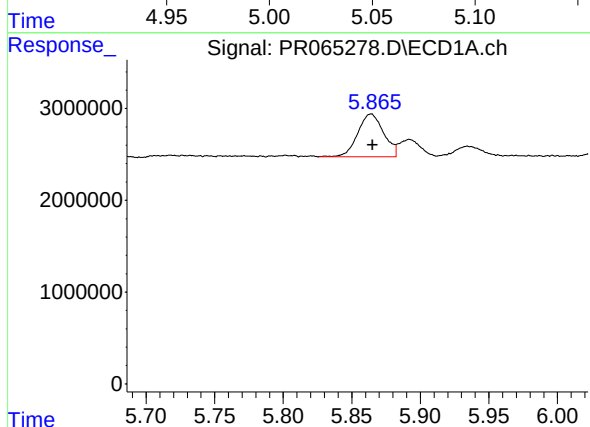


#26 AR-1254-1

R.T.: 5.864 min
Delta R.T.: -0.001 min
Response: 6153041
Conc: 30.04 ng/ml

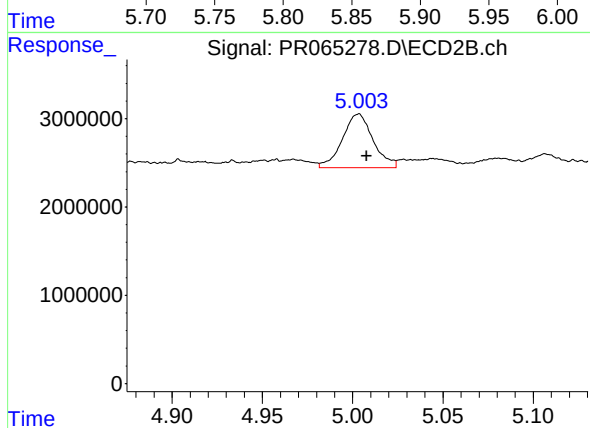

#26 AR-1254-1


R.T.: 5.003 min
Delta R.T.: -0.005 min
Response: 7200952
Conc: 24.71 ng/ml

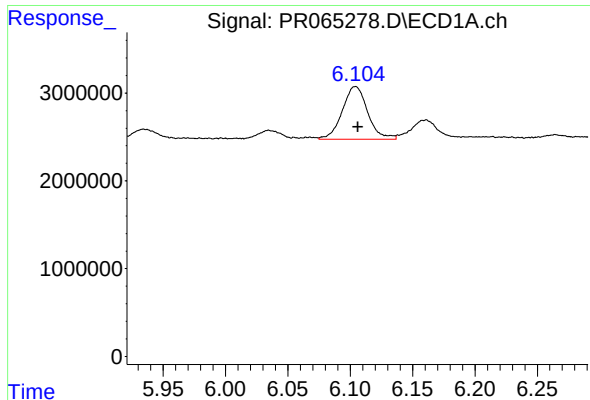

#27 AR-1254-2


R.T.: 6.104 min
Delta R.T.: -0.002 min
Response: 8501762
Conc: 27.28 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

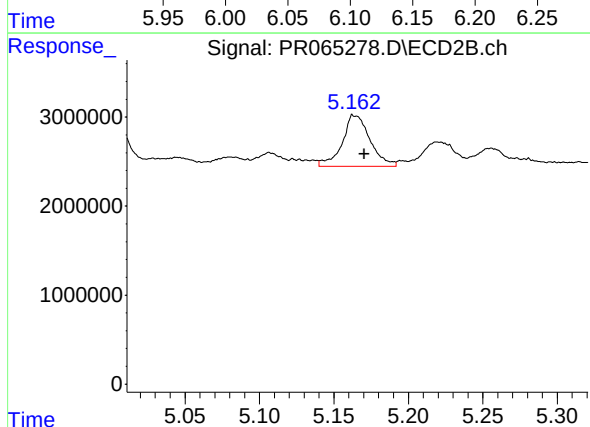


#27 AR-1254-2

R.T.: 5.164 min
Delta R.T.: -0.006 min
Response: 7436975
Conc: 29.36 ng/ml

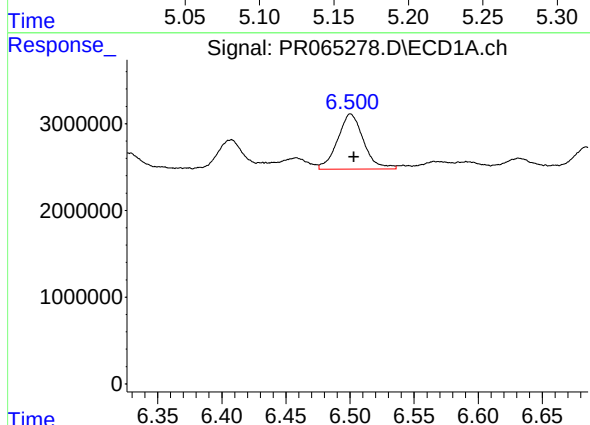


#28 AR-1254-3

R.T.: 6.500 min
Delta R.T.: -0.003 min
Response: 8938562
Conc: 27.94 ng/ml

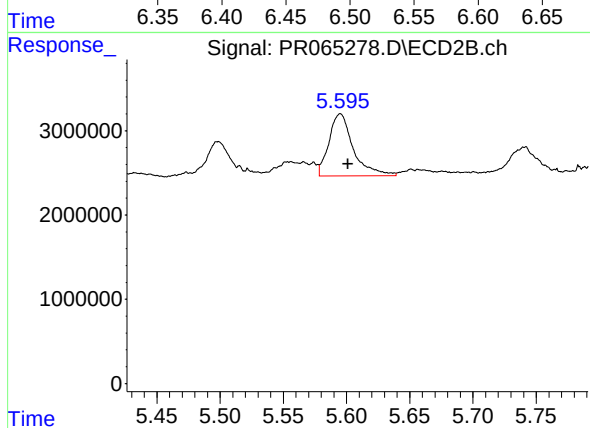

#28 AR-1254-3


R.T.: 5.595 min
Delta R.T.: -0.006 min
Response: 9951014
Conc: 24.32 ng/ml

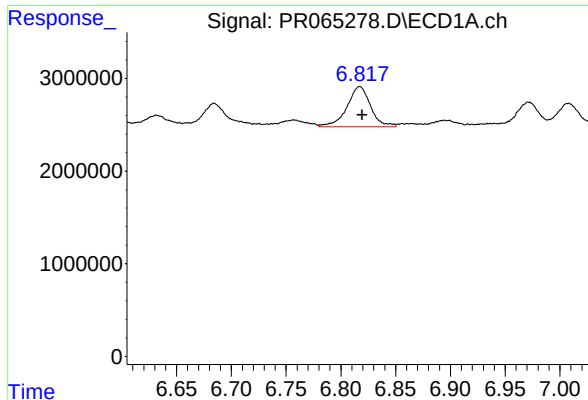

#29 AR-1254-4


R.T.: 6.817 min
Delta R.T.: -0.002 min
Response: 6506976
Conc: 28.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

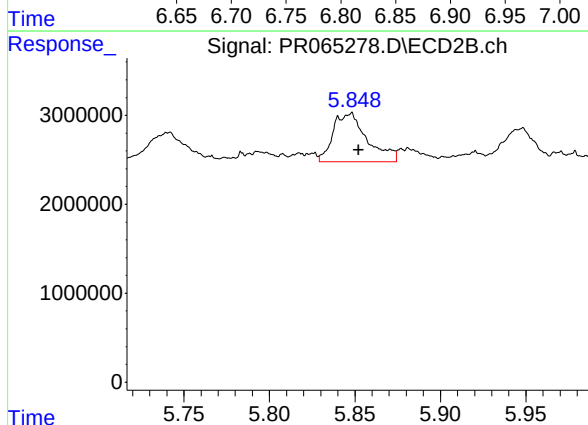


#29 AR-1254-4

R.T.: 5.847 min
Delta R.T.: -0.005 min
Response: 7563813
Conc: 29.46 ng/ml

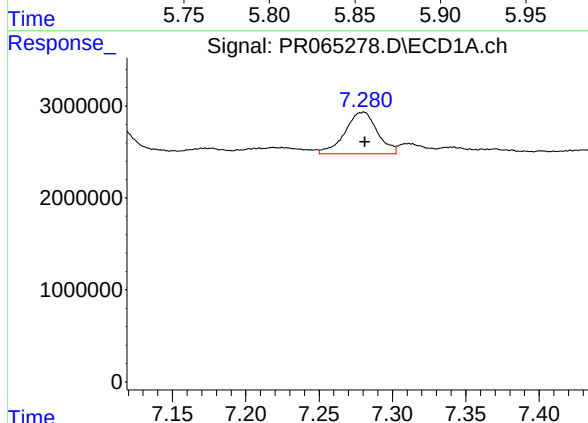


#30 AR-1254-5

R.T.: 7.280 min
Delta R.T.: -0.001 min
Response: 6938562
Conc: 27.92 ng/ml

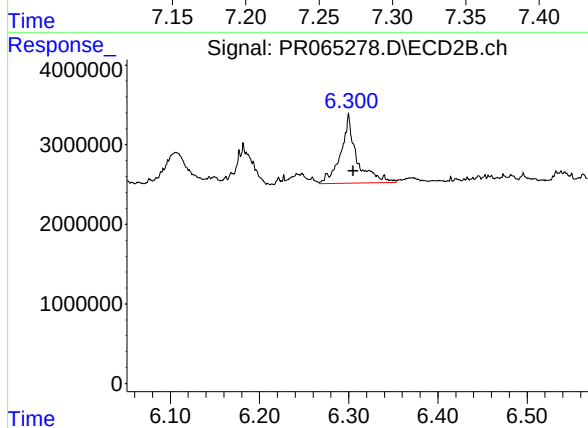

#30 AR-1254-5


R.T.: 6.300 min
Delta R.T.: -0.005 min
Response: 10739760
Conc: 29.30 ng/ml

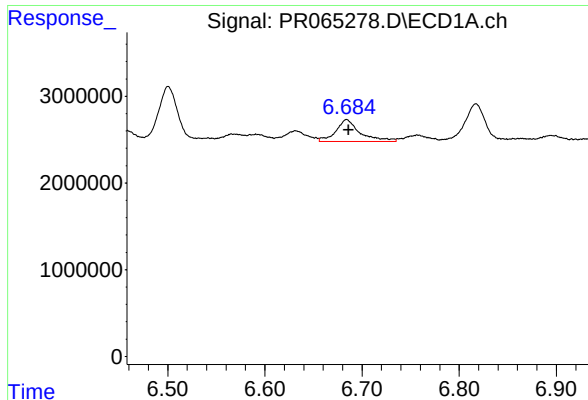

#31 AR-1260-1


R.T.: 6.684 min
Delta R.T.: -0.002 min
Response: 4423035
Conc: 17.60 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

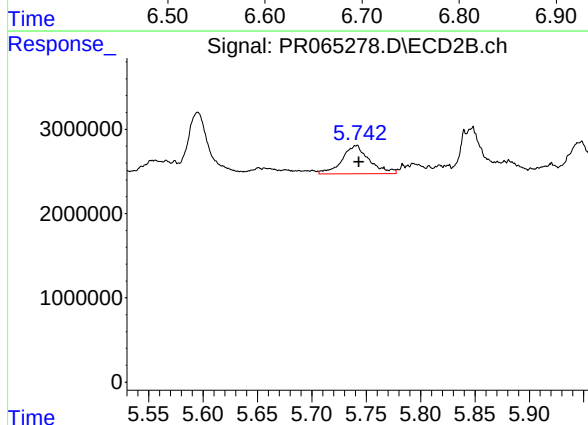


#31 AR-1260-1

R.T.: 5.741 min
Delta R.T.: -0.002 min
Response: 5930279
Conc: 20.78 ng/ml

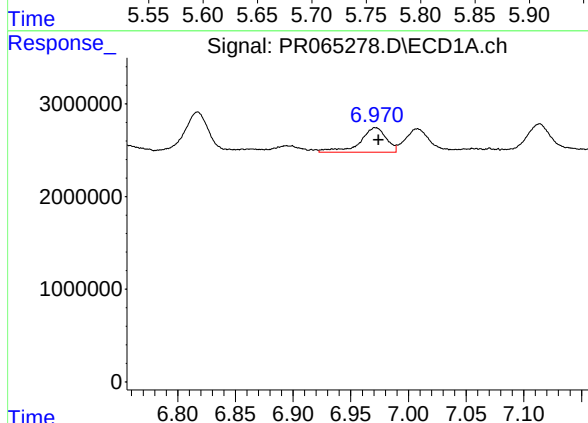


#32 AR-1260-2

R.T.: 6.972 min
Delta R.T.: -0.002 min
Response: 4197044
Conc: 14.60 ng/ml

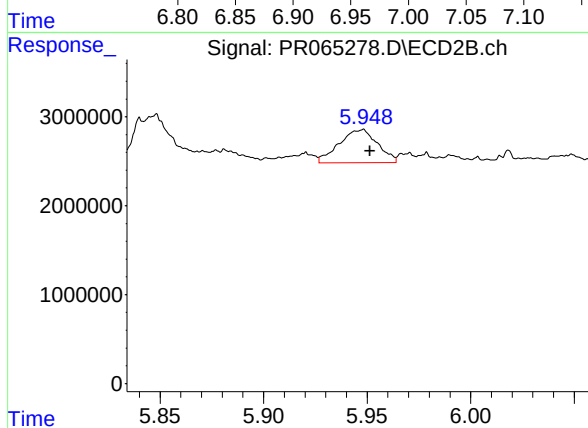

#32 AR-1260-2


R.T.: 5.948 min
Delta R.T.: -0.004 min
Response: 4784374
Conc: 13.80 ng/ml

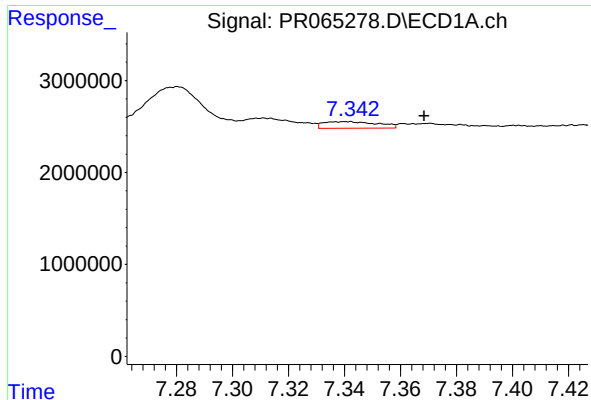

#33 AR-1260-3


R.T.: 7.341 min
Delta R.T.: -0.028 min
Response: 963248
Conc: 4.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

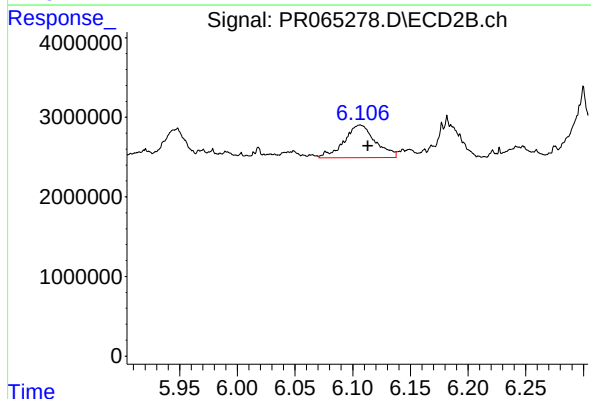


#33 AR-1260-3

R.T.: 6.107 min
Delta R.T.: -0.007 min
Response: 7635424
Conc: 23.50 ng/ml

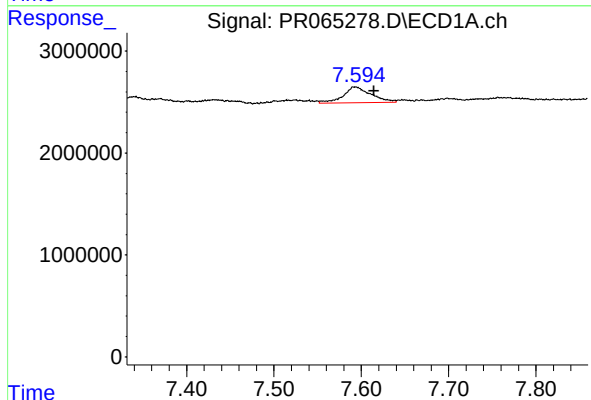


#34 AR-1260-4

R.T.: 7.593 min
Delta R.T.: -0.022 min
Response: 3438834
Conc: 14.57 ng/ml

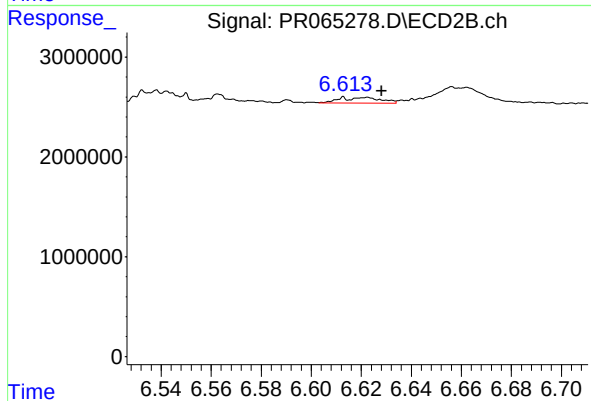

#34 AR-1260-4


R.T.: 6.613 min
Delta R.T.: -0.015 min
Response: 615751
Conc: 2.33 ng/ml

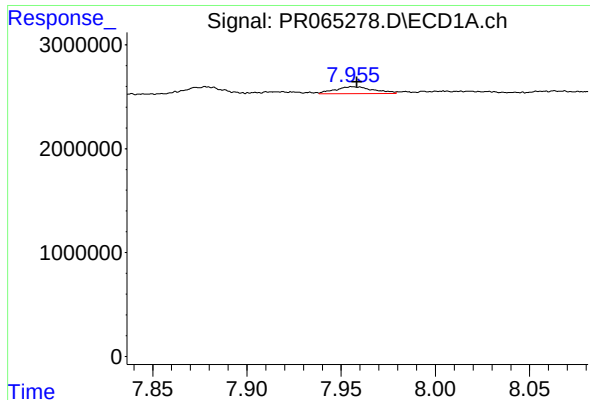

#35 AR-1260-5


R.T.: 7.956 min
Delta R.T.: -0.002 min
Response: 954184
Conc: 2.17 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

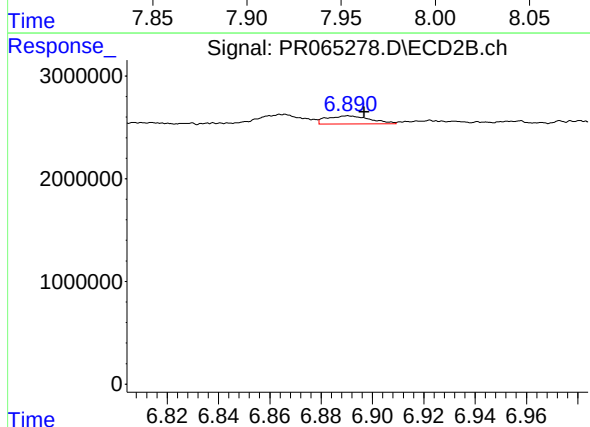


#35 AR-1260-5

R.T.: 6.891 min
Delta R.T.: -0.006 min
Response: 932807
Conc: 1.51 ng/ml

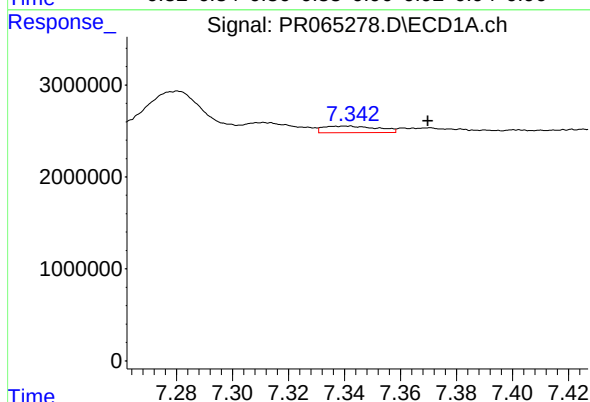


#36 AR-1262-1

R.T.: 7.341 min
Delta R.T.: -0.029 min
Response: 963248
Conc: 2.85 ng/ml

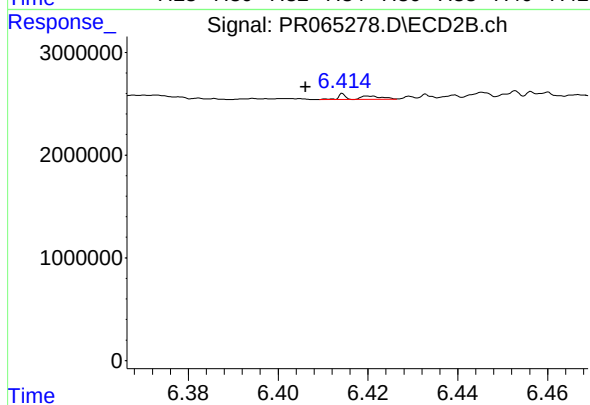

#36 AR-1262-1


R.T.: 6.415 min
Delta R.T.: 0.009 min
Response: 164815
Conc: 0.92 ng/ml

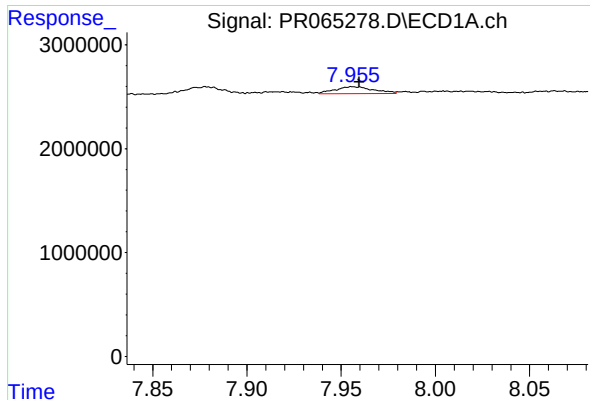

#37 AR-1262-2


R.T.: 7.956 min
Delta R.T.: -0.004 min
Response: 954184
Conc: 1.69 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

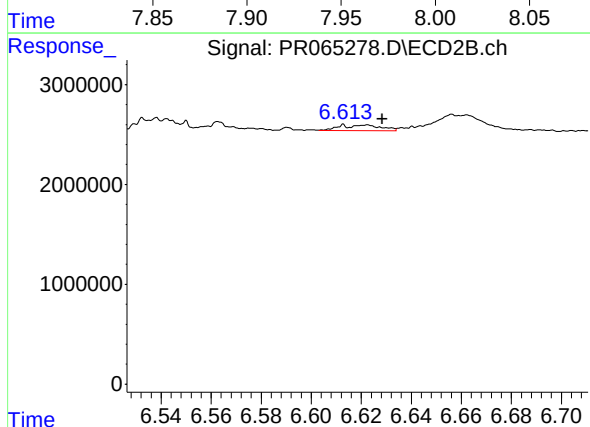


#37 AR-1262-2

R.T.: 6.613 min
Delta R.T.: -0.016 min
Response: 615751
Conc: 1.58 ng/ml

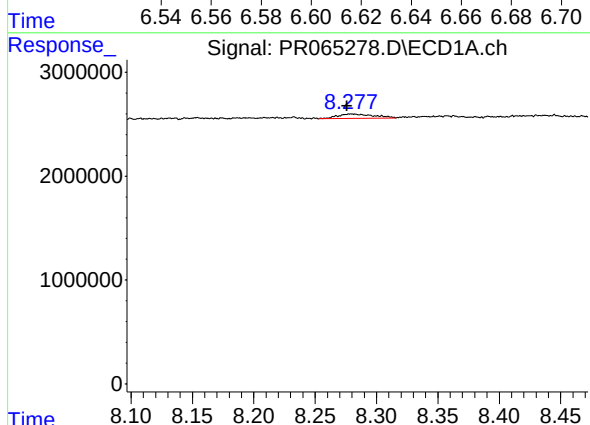


#38 AR-1262-3

R.T.: 8.279 min
Delta R.T.: 0.003 min
Response: 850740
Conc: 2.24 ng/ml

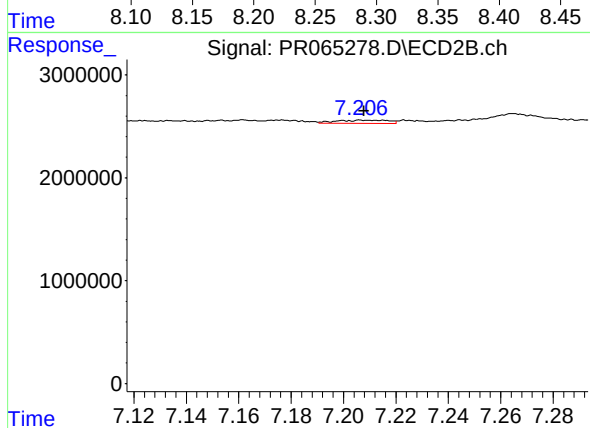

#38 AR-1262-3


R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 416968
Conc: 1.47 ng/ml

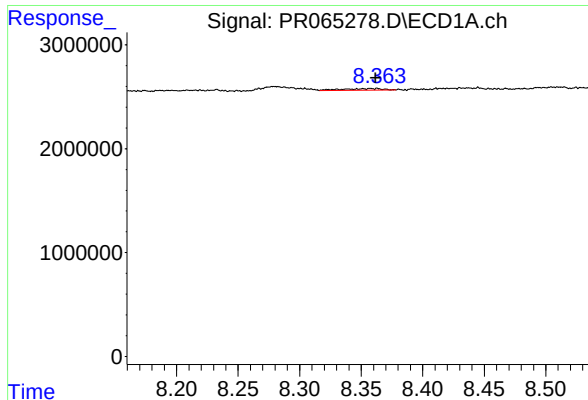

#39 AR-1262-4


R.T.: 8.363 min
Delta R.T.: 0.001 min
Response: 358522
Conc: 1.22 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

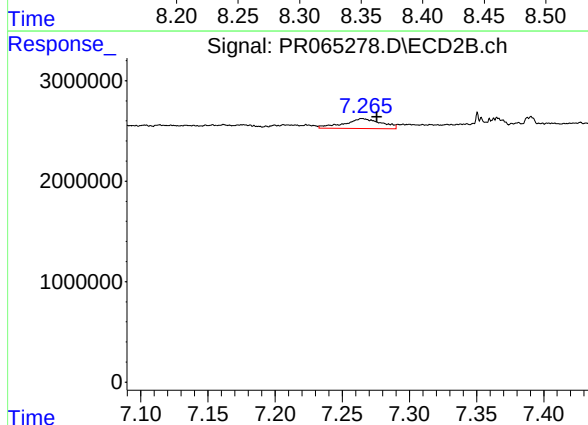


#39 AR-1262-4

R.T.: 7.265 min
Delta R.T.: -0.011 min
Response: 1905448
Conc: 3.31 ng/ml

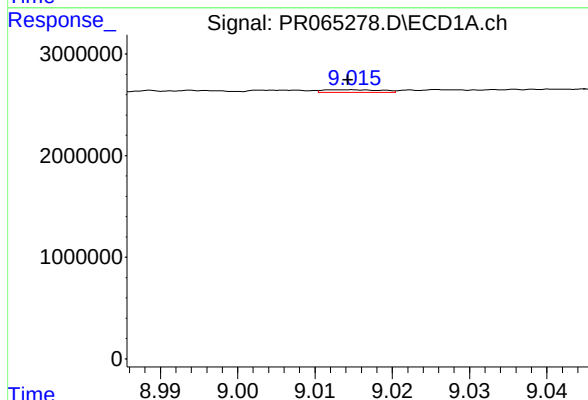


#40 AR-1262-5

R.T.: 9.014 min
Delta R.T.: 0.000 min
Response: 134002
Conc: 0.67 ng/ml

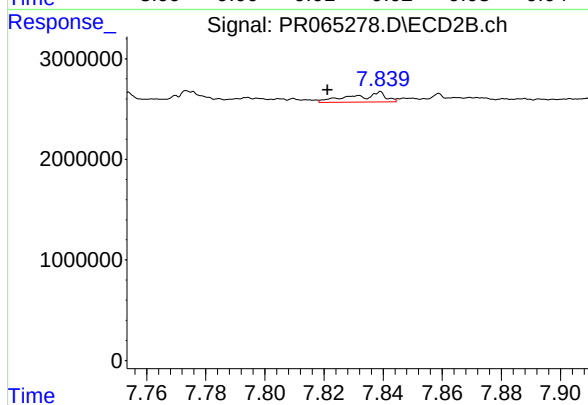

#40 AR-1262-5


R.T.: 7.839 min
Delta R.T.: 0.017 min
Response: 757666
Conc: 2.91 ng/ml

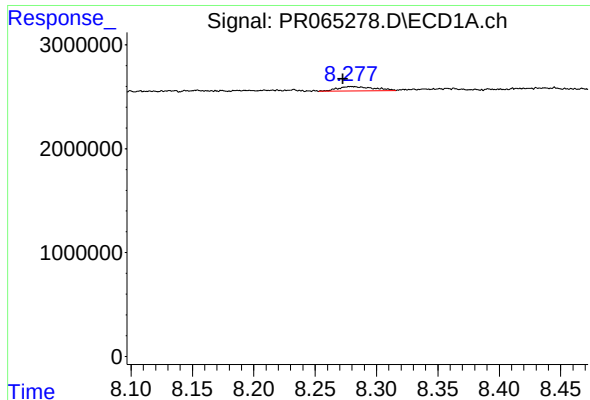

#41 AR-1268-1


R.T.: 8.279 min
Delta R.T.: 0.006 min
Response: 850740
Conc: 1.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

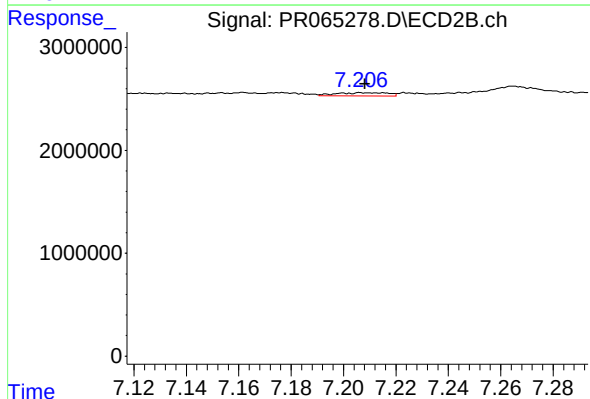


#41 AR-1268-1

R.T.: 7.207 min
Delta R.T.: -0.001 min
Response: 416968
Conc: 0.53 ng/ml

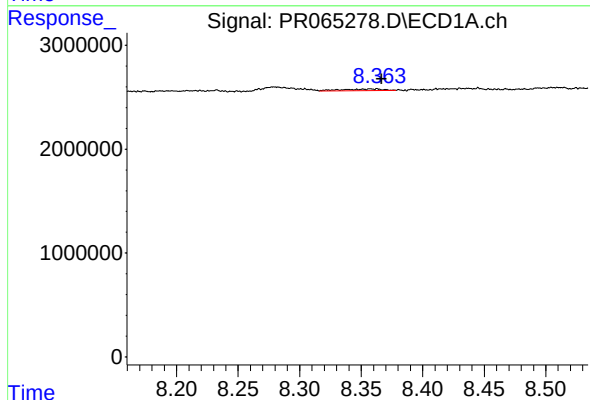


#42 AR-1268-2

R.T.: 8.363 min
Delta R.T.: -0.004 min
Response: 358522
Conc: 0.66 ng/ml

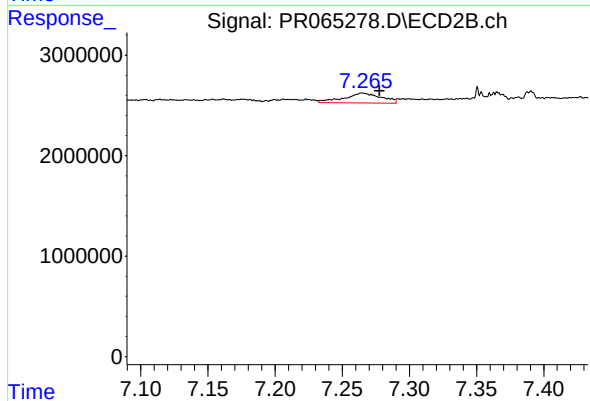

#42 AR-1268-2


R.T.: 7.265 min
Delta R.T.: -0.013 min
Response: 1905448
Conc: 2.56 ng/ml

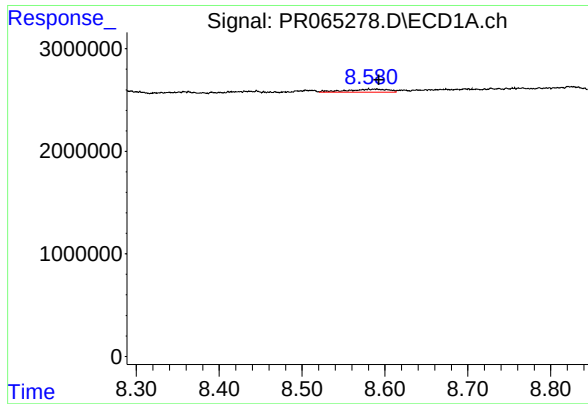

#43 AR-1268-3


R.T.: 8.580 min
Delta R.T.: -0.012 min
Response: 976243
Conc: 2.06 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

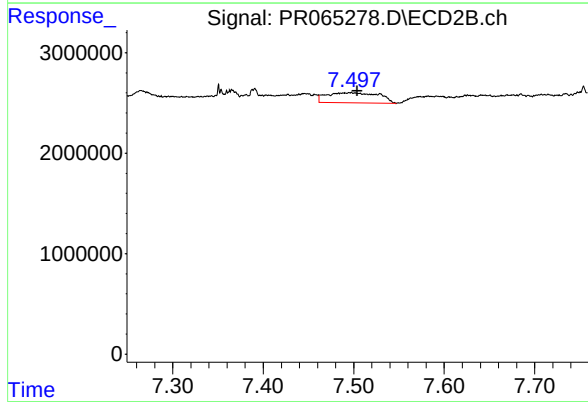


#43 AR-1268-3

R.T.: 7.497 min
Delta R.T.: -0.008 min
Response: 4106507
Conc: 6.48 ng/ml

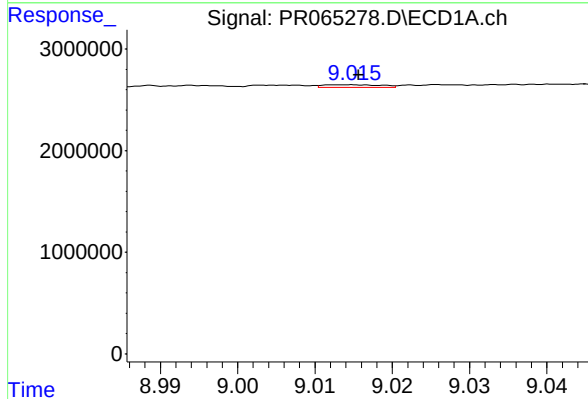


#44 AR-1268-4

R.T.: 9.014 min
Delta R.T.: -0.001 min
Response: 134002
Conc: 0.66 ng/ml

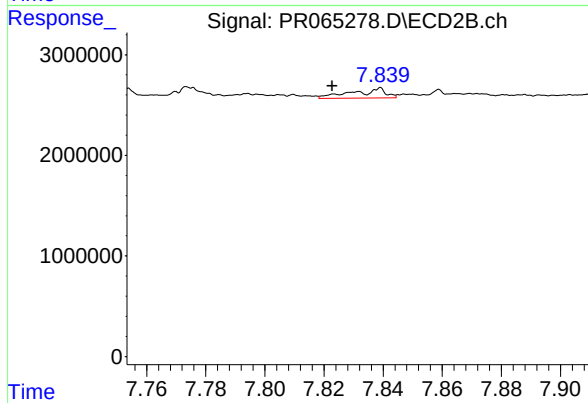

#44 AR-1268-4


R.T.: 7.839 min
Delta R.T.: 0.016 min
Response: 757666
Conc: 2.89 ng/ml

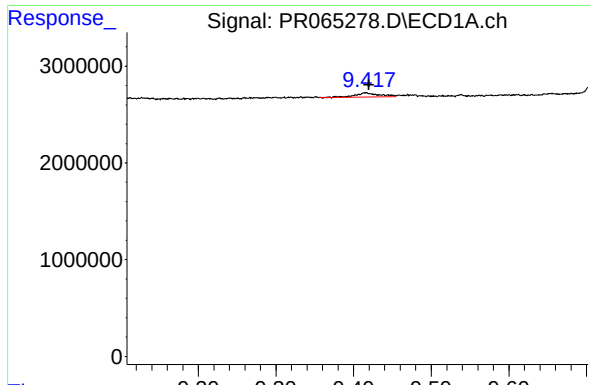

#45 AR-1268-5

R.T.: 9.416 min
Delta R.T.: -0.004 min
Response: 937974
Conc: 0.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

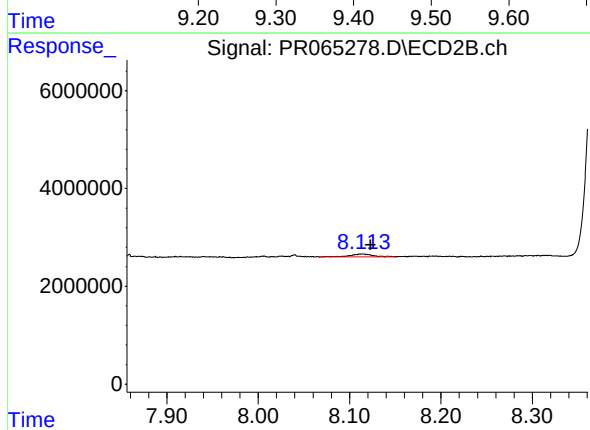

#45 AR-1268-5

R.T.: 8.114 min
Delta R.T.: -0.009 min
Response: 1060113
Conc: 0.55 ng/ml