

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
 Data File : PR065279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 19:20
 Operator : AJ\MA
 Sample : P1187-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:35:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.700	3.003	115.0E6	112.4E6	19.270	20.545
2) SA Decachlor...	9.738	8.374	83892783	98472910	20.976	20.807
Target Compounds						
3) L1 AR-1016-1	4.938	4.146	241257	324648	1.361	1.788 #
4) L1 AR-1016-2	4.971	4.182	188923	850844	0.725	3.441 #
5) L1 AR-1016-3	5.028	4.342	326401	600295	1.953	4.427 #
6) L1 AR-1016-4	5.127	4.406	141793	311030	1.057	2.970 #
7) L1 AR-1016-5	5.451	4.628	311743	386520	2.309	2.771
8) L2 AR-1221-1	3.912f	3.223	2929735	120924	40.819	1.953 #
9) L2 AR-1221-2	4.015	3.313	2004848	2391667	38.243	50.145 #
10) L2 AR-1221-3	0.000	3.394	0	776067	N.D.	5.618 #
11) L3 AR-1232-1	0.000	3.394	0	776067	N.D.	6.480 #
12) L3 AR-1232-2	4.668	4.182	191342	850844	2.484	6.964 #
13) L3 AR-1232-3	4.971	4.342	188923	600295	1.482	9.024 #
14) L3 AR-1232-4	5.127	4.447	141793	130856	2.163	2.285
15) L3 AR-1232-5	5.239	4.628	257219	386520	5.318	6.064
16) L4 AR-1242-1	4.938	4.146	241257	324648	1.688	2.221 #
17) L4 AR-1242-2	4.971	4.182	188923	850844	0.897	4.265 #
18) L4 AR-1242-3	5.028	4.342	326401	600295	2.410	5.482 #
19) L4 AR-1242-4	5.127	4.447	141793	130856	1.305	1.246
20) L4 AR-1242-5	5.940	5.004	675055	1390544	5.968	10.299 #
21) L5 AR-1248-1	4.938	4.146	241257	324648	2.268	3.005 #
22) L5 AR-1248-2	5.239	4.406	257219	311030	1.655	2.148 #
23) L5 AR-1248-3	5.451	4.447	311743	130856	1.746	0.846 #
24) L5 AR-1248-4	0.000	4.628	0	386520	N.D.	2.064 #
25) L5 AR-1248-5	5.940	5.051	675055	777298	3.543	4.176
26) L6 AR-1254-1	5.865	5.004	1598938	1390544	7.807	4.772 #
27) L6 AR-1254-2	6.105	5.165	1454895	1107380	4.668	4.371
28) L6 AR-1254-3	6.494	5.615	1493167	4031528	4.667	9.853 #
29) L6 AR-1254-4	6.812	5.848	356018	716401	1.554	2.791 #
30) L6 AR-1254-5	7.275	6.297	5177692	5067371	20.833	13.824 #
31) L7 AR-1260-1	6.684	5.738	5775390	6187431	22.975	21.676
32) L7 AR-1260-2	6.971	5.946	5867506	7154621	20.417	20.632
33) L7 AR-1260-3	7.367	6.110	8089189	8736203	38.261	26.890 #
34) L7 AR-1260-4	7.612	6.622	7463570	7515606	31.629	28.448
35) L7 AR-1260-5	7.957	6.891	12487322	14518958	28.401	23.542
36) L8 AR-1262-1	7.367	6.399	8089189	4321107	23.897	24.090
37) L8 AR-1262-2	7.957	6.622	12487322	7515606	22.077	19.316
38) L8 AR-1262-3	8.271	7.202	8457934	7522420	22.227	26.540
39) L8 AR-1262-4	8.359	7.270	6489172	11828738	22.153	20.540
40) L8 AR-1262-5	9.009	7.815	4453933	5399520	22.226	20.746
41) L9 AR-1268-1	8.271	7.202	8457934	7522420	13.951	9.482 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
Data File : PR065279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 19:20
Operator : AJ\MA
Sample : P1187-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 70 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:35:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.359	7.270	6489172	11828738	11.859	15.889 #
43)	L9 AR-1268-3	8.588	7.494	1226490	2055213	2.585	3.244 #
44)	L9 AR-1268-4	9.009	7.815	4453933	5399520	21.889	20.585
45)	L9 AR-1268-5	9.413	8.114	1837538	3639010	1.261	1.901 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
Data File : PR065279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 19:20
Operator : AJ\MA
Sample : P1187-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 70 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:35:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

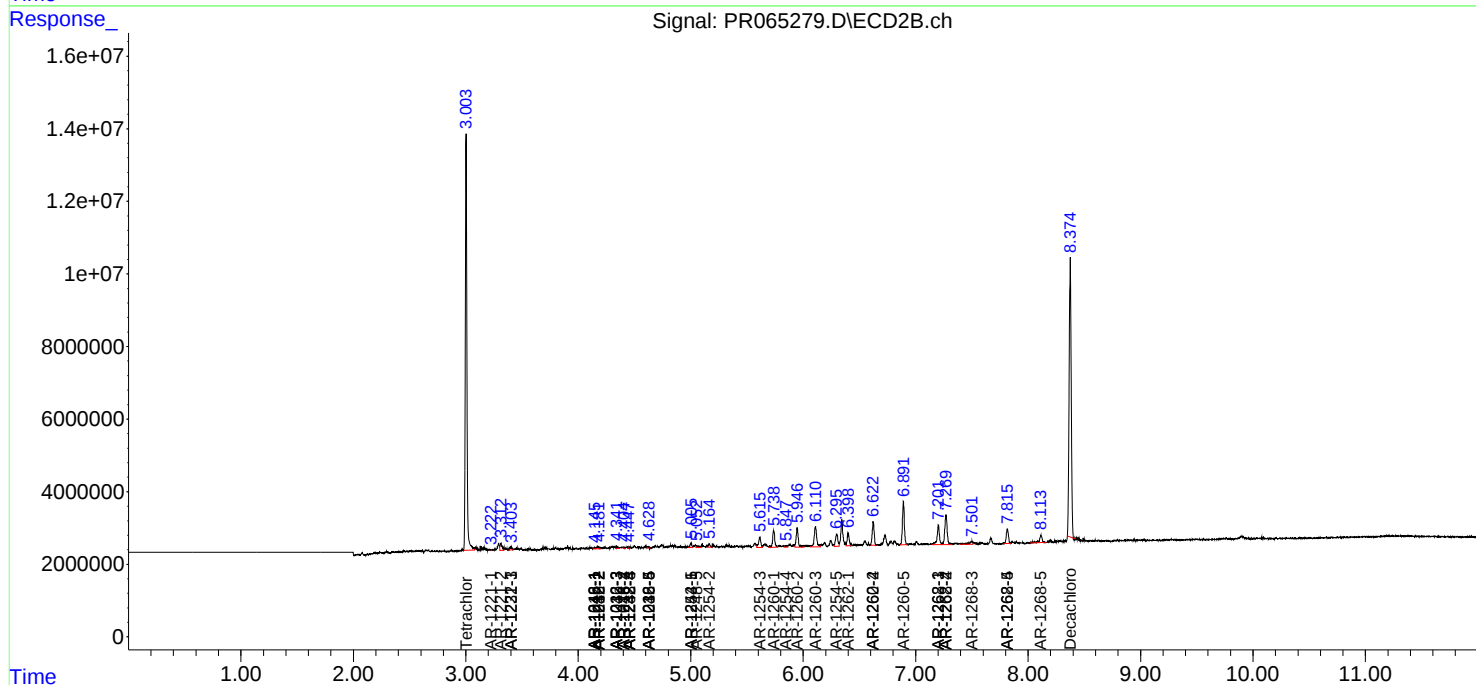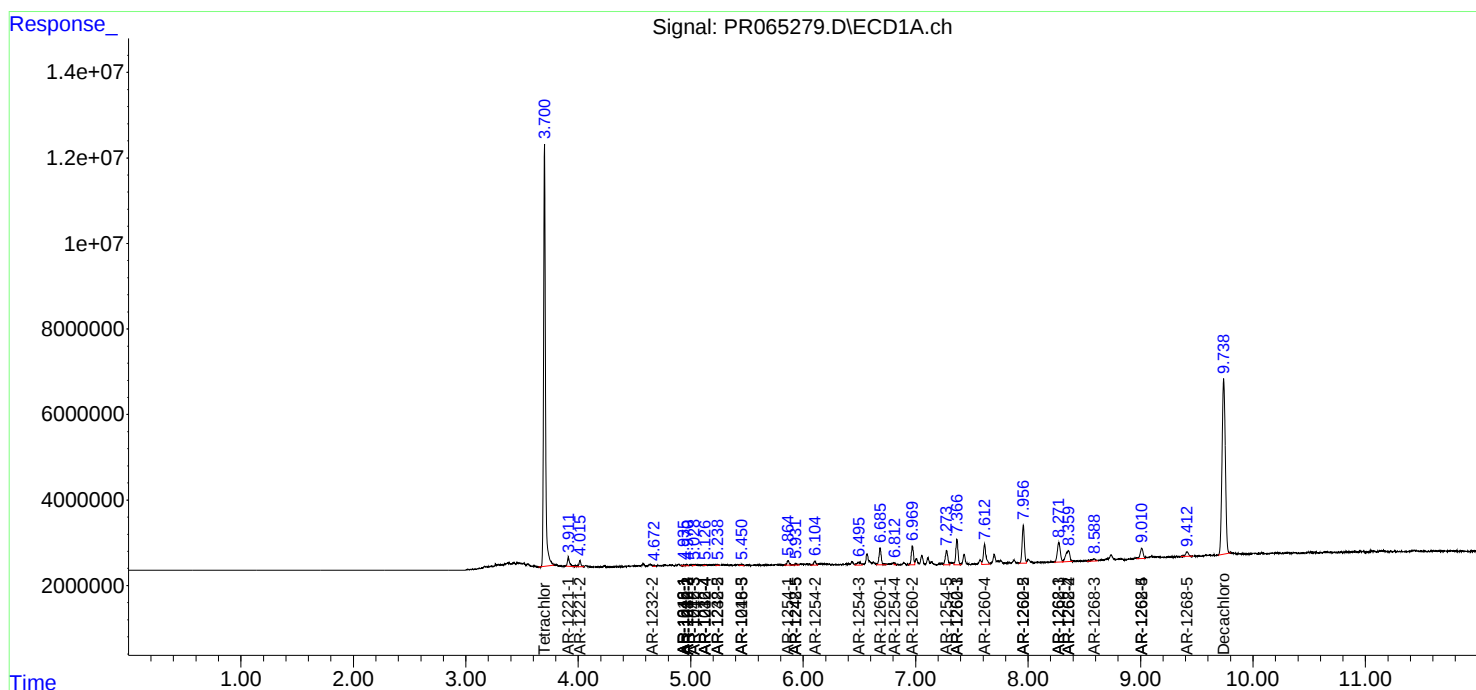


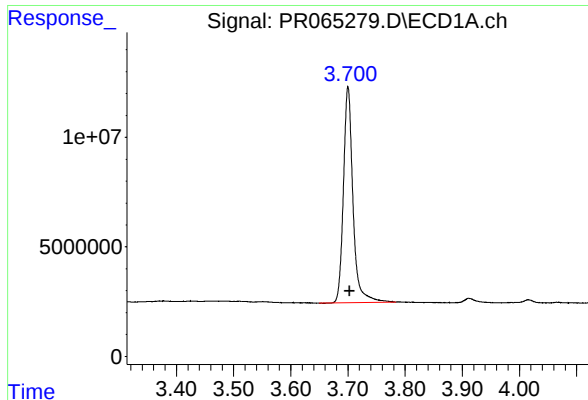

#1 Tetrachloro-m-xylene


R.T.: 3.700 min
Delta R.T.: -0.003 min
Response: 115028664
Conc: 19.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

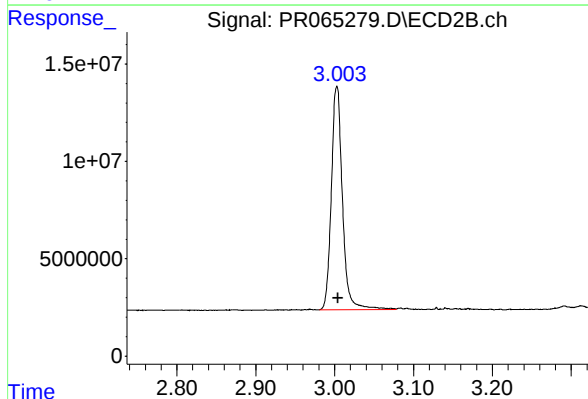


#1 Tetrachloro-m-xylene

R.T.: 3.003 min
Delta R.T.: -0.002 min
Response: 112377070
Conc: 20.54 ng/ml

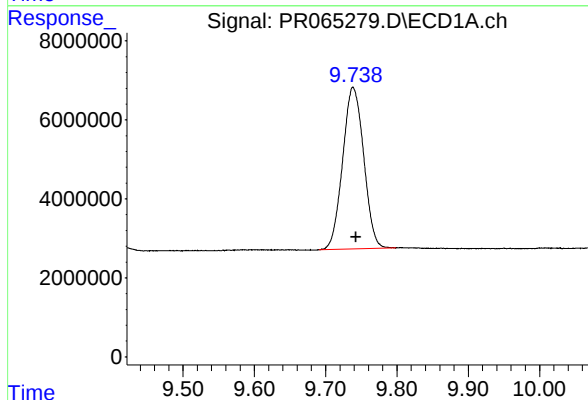


#2 Decachlorobiphenyl

R.T.: 9.738 min
Delta R.T.: -0.004 min
Response: 83892783
Conc: 20.98 ng/ml

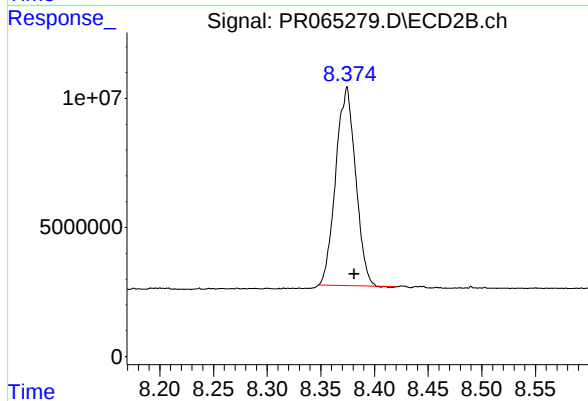

#2 Decachlorobiphenyl


R.T.: 8.374 min
Delta R.T.: -0.007 min
Response: 98472910
Conc: 20.81 ng/ml

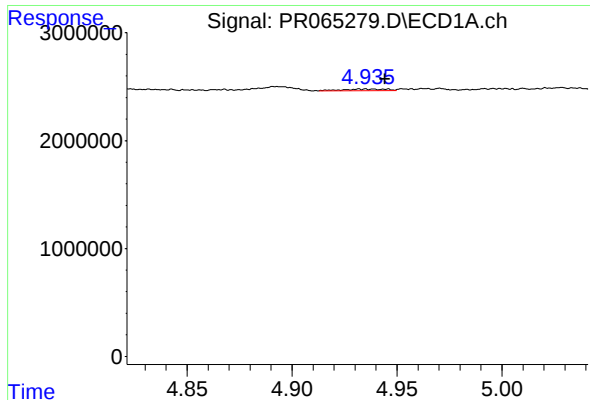

#3 AR-1016-1


R.T.: 4.938 min
Delta R.T.: -0.006 min
Response: 241257
Conc: 1.36 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

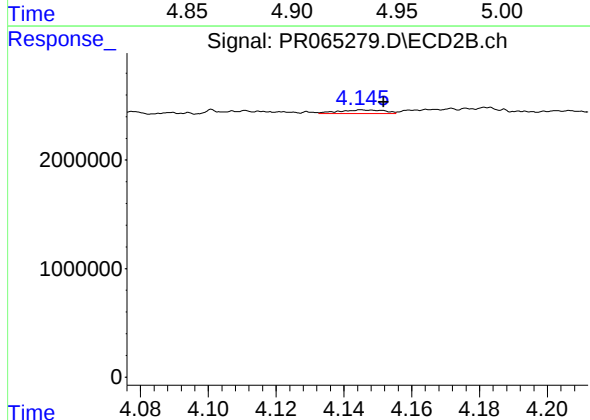


#3 AR-1016-1

R.T.: 4.146 min
Delta R.T.: -0.006 min
Response: 324648
Conc: 1.79 ng/ml

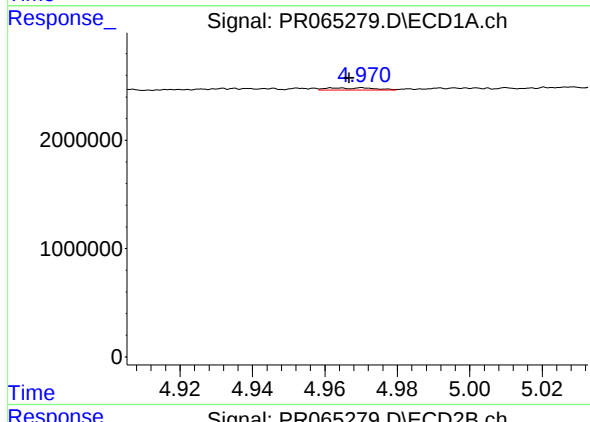


#4 AR-1016-2

R.T.: 4.971 min
Delta R.T.: 0.004 min
Response: 188923
Conc: 0.72 ng/ml

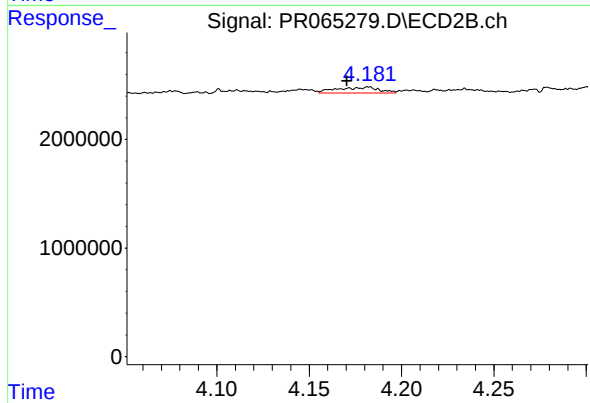

#4 AR-1016-2


R.T.: 4.182 min
Delta R.T.: 0.012 min
Response: 850844
Conc: 3.44 ng/ml

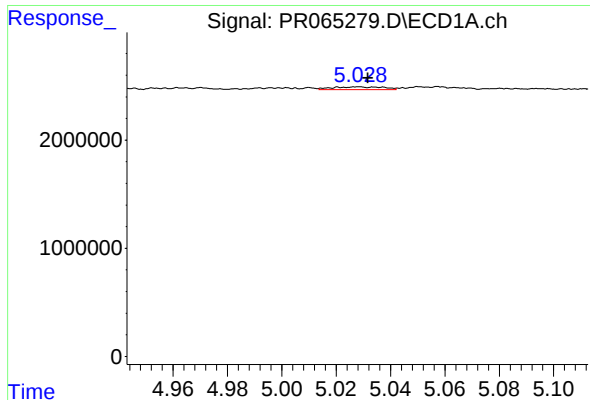

#5 AR-1016-3


R.T.: 5.028 min
Delta R.T.: -0.004 min
Response: 326401
Conc: 1.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

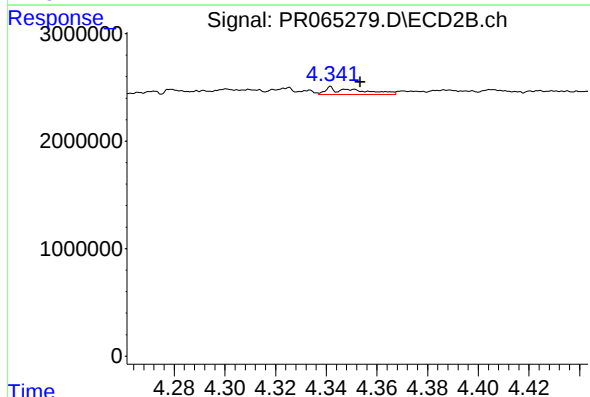


#5 AR-1016-3

R.T.: 4.342 min
Delta R.T.: -0.012 min
Response: 600295
Conc: 4.43 ng/ml

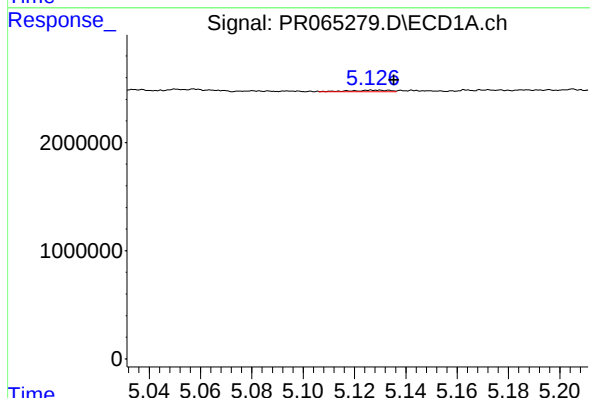


#6 AR-1016-4

R.T.: 5.127 min
Delta R.T.: -0.008 min
Response: 141793
Conc: 1.06 ng/ml

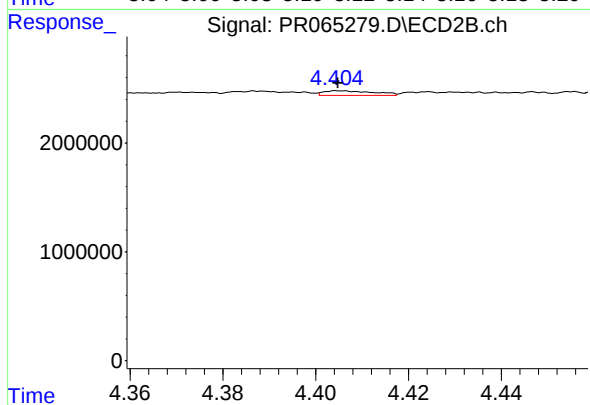

#6 AR-1016-4


R.T.: 4.406 min
Delta R.T.: 0.000 min
Response: 311030
Conc: 2.97 ng/ml

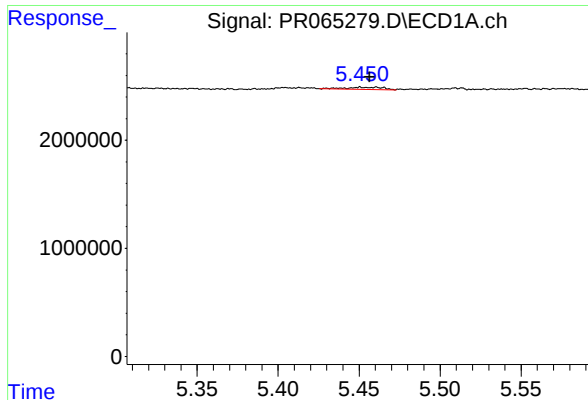

#7 AR-1016-5


R.T.: 5.451 min
Delta R.T.: -0.006 min
Response: 311743
Conc: 2.31 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

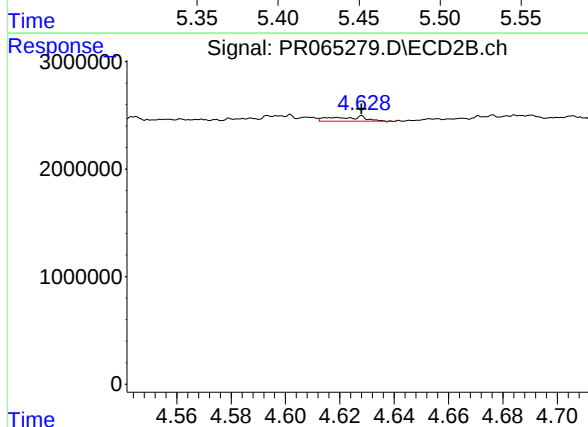


#7 AR-1016-5

R.T.: 4.628 min
Delta R.T.: 0.000 min
Response: 386520
Conc: 2.77 ng/ml

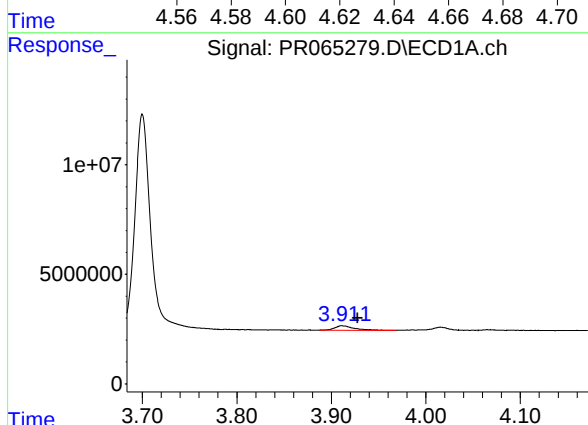


#8 AR-1221-1

R.T.: 3.912 min
Delta R.T.: -0.016 min
Response: 2929735
Conc: 40.82 ng/ml

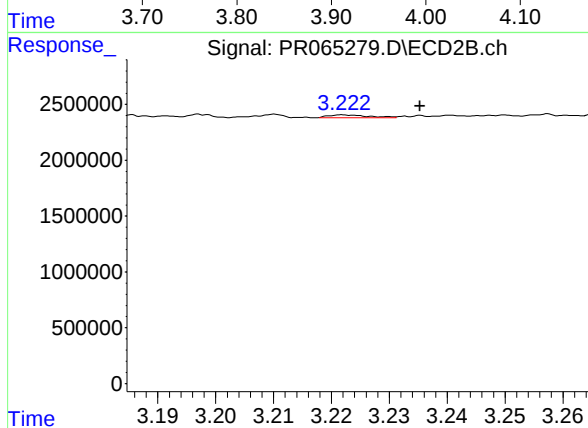

#8 AR-1221-1


R.T.: 3.223 min
Delta R.T.: -0.013 min
Response: 120924
Conc: 1.95 ng/ml

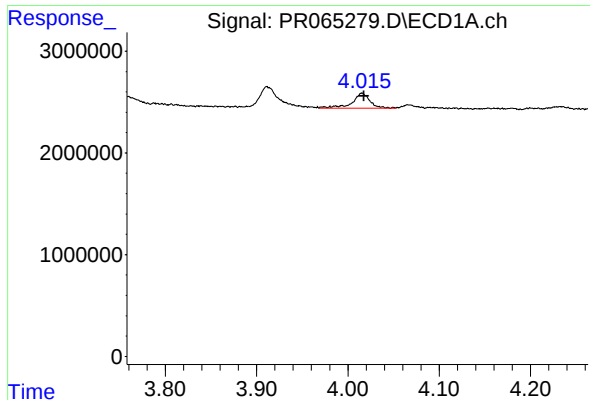

#9 AR-1221-2


R.T.: 4.015 min
Delta R.T.: -0.002 min
Response: 2004848
Conc: 38.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

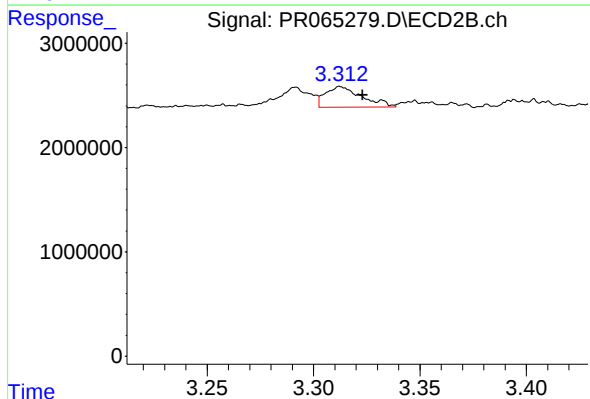


#9 AR-1221-2

R.T.: 3.313 min
Delta R.T.: -0.010 min
Response: 2391667
Conc: 50.14 ng/ml

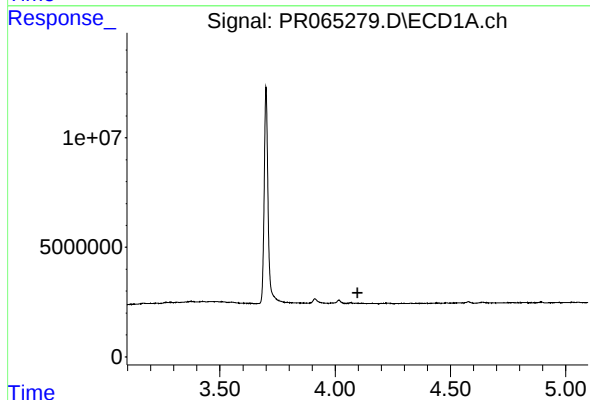


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T.: 4.097 min
Response: 0
Conc: N.D.

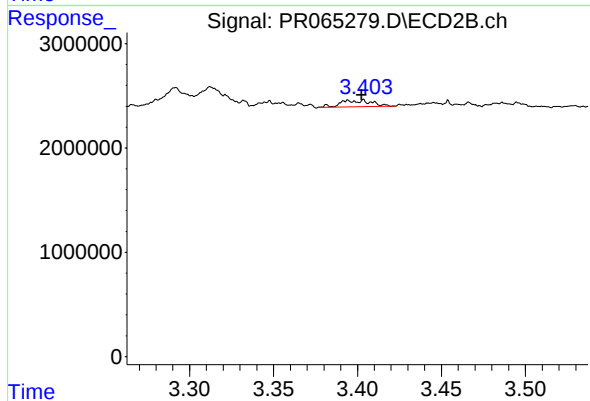

#10 AR-1221-3


R.T.: 3.394 min
Delta R.T.: -0.008 min
Response: 776067
Conc: 5.62 ng/ml

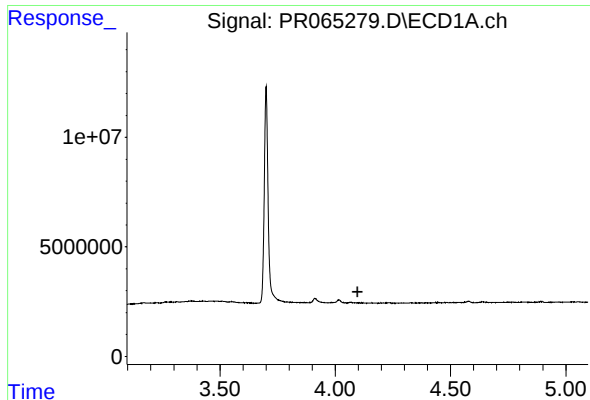

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

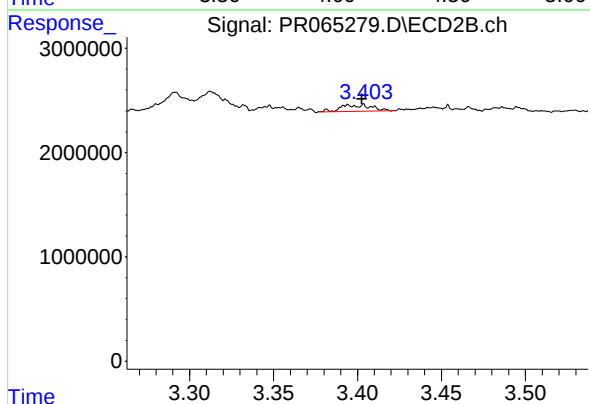


#11 AR-1232-1

R.T.: 3.394 min
Delta R.T.: -0.009 min
Response: 776067
Conc: 6.48 ng/ml

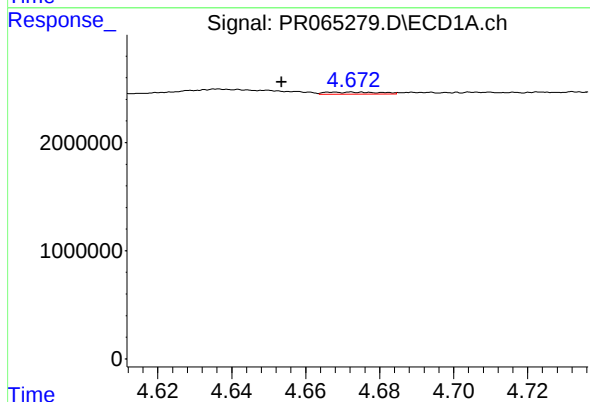


#12 AR-1232-2

R.T.: 4.668 min
Delta R.T.: 0.014 min
Response: 191342
Conc: 2.48 ng/ml

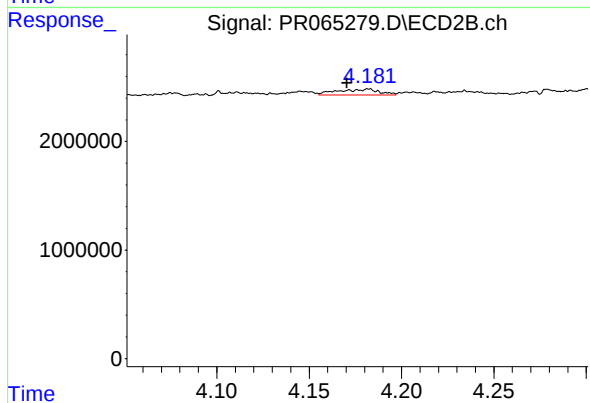

#12 AR-1232-2


R.T.: 4.182 min
Delta R.T.: 0.012 min
Response: 850844
Conc: 6.96 ng/ml

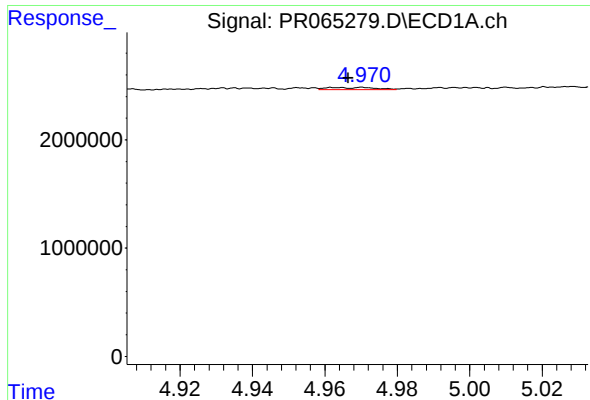

#13 AR-1232-3


R.T.: 4.971 min
Delta R.T.: 0.004 min
Response: 188923
Conc: 1.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

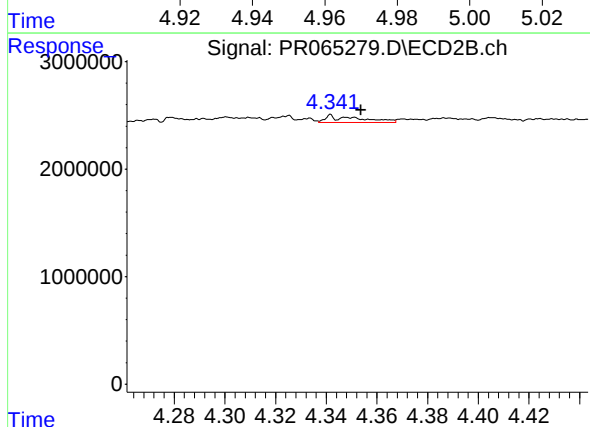


#13 AR-1232-3

R.T.: 4.342 min
Delta R.T.: -0.012 min
Response: 600295
Conc: 9.02 ng/ml

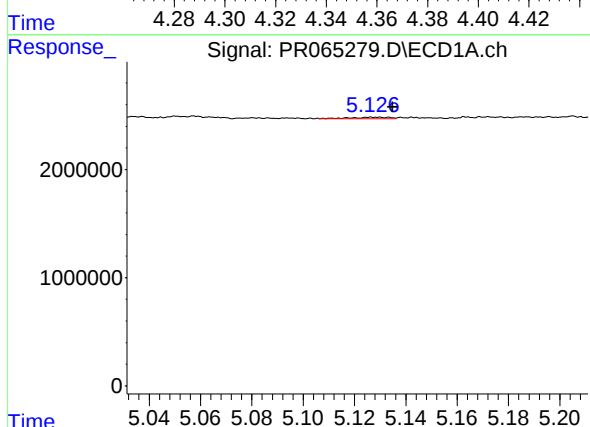


#14 AR-1232-4

R.T.: 5.127 min
Delta R.T.: -0.008 min
Response: 141793
Conc: 2.16 ng/ml

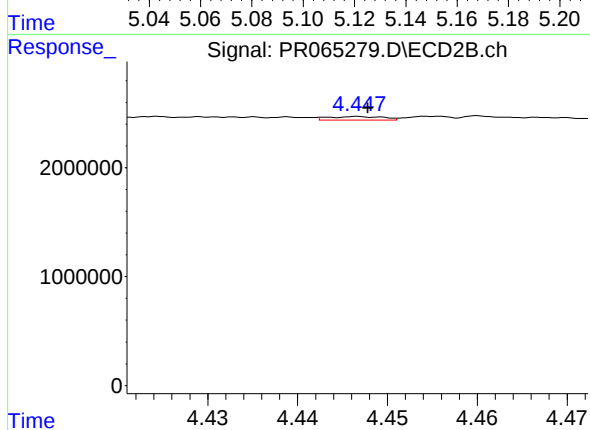

#14 AR-1232-4


R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 130856
Conc: 2.29 ng/ml

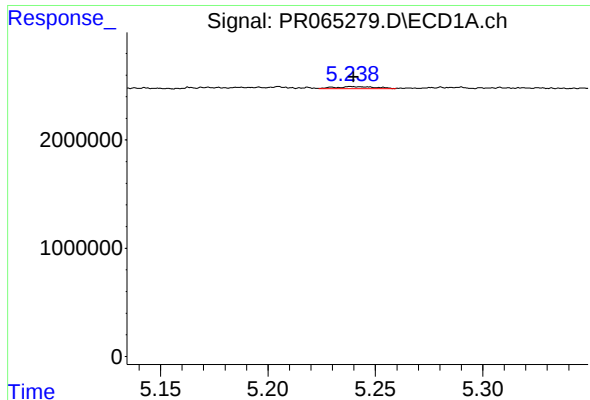

#15 AR-1232-5


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 257219
Conc: 5.32 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

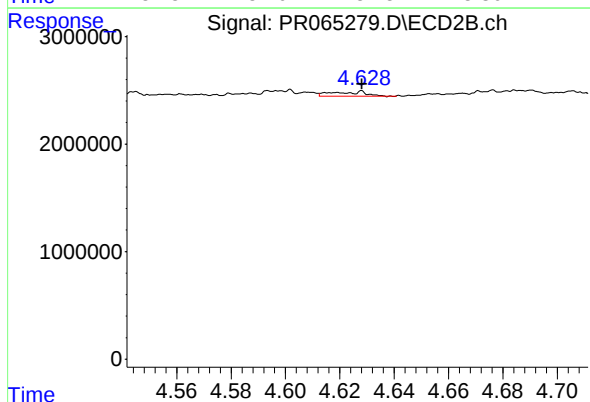


#15 AR-1232-5

R.T.: 4.628 min
Delta R.T.: 0.000 min
Response: 386520
Conc: 6.06 ng/ml

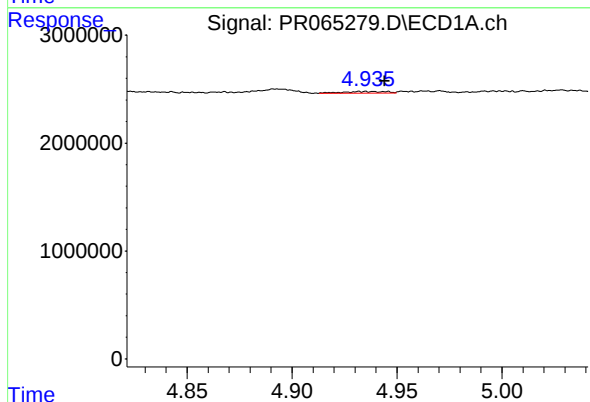


#16 AR-1242-1

R.T.: 4.938 min
Delta R.T.: -0.006 min
Response: 241257
Conc: 1.69 ng/ml

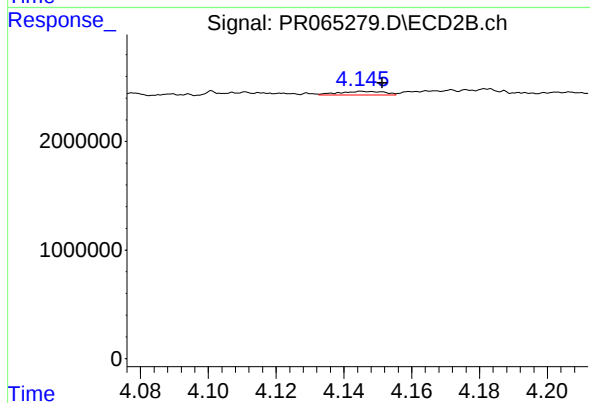

#16 AR-1242-1


R.T.: 4.146 min
Delta R.T.: -0.006 min
Response: 324648
Conc: 2.22 ng/ml

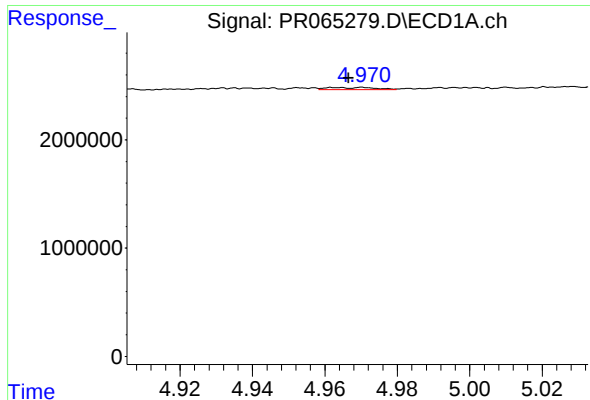

#17 AR-1242-2


R.T.: 4.971 min
Delta R.T.: 0.004 min
Response: 188923
Conc: 0.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

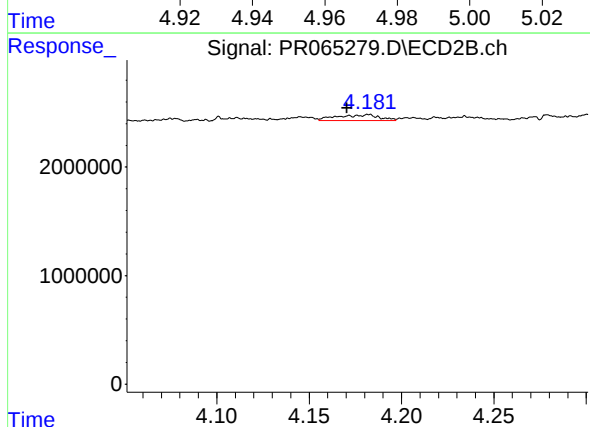


#17 AR-1242-2

R.T.: 4.182 min
Delta R.T.: 0.012 min
Response: 850844
Conc: 4.27 ng/ml

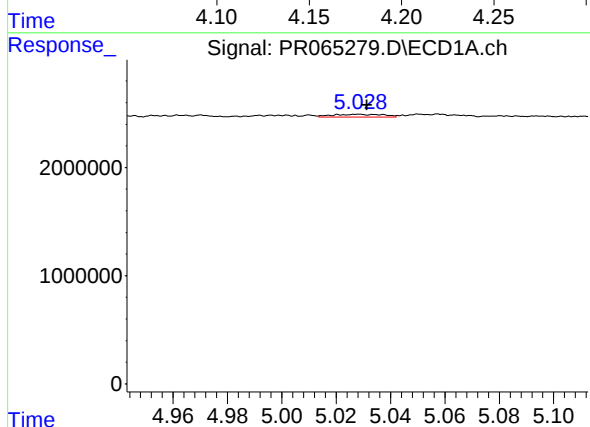


#18 AR-1242-3

R.T.: 5.028 min
Delta R.T.: -0.003 min
Response: 326401
Conc: 2.41 ng/ml

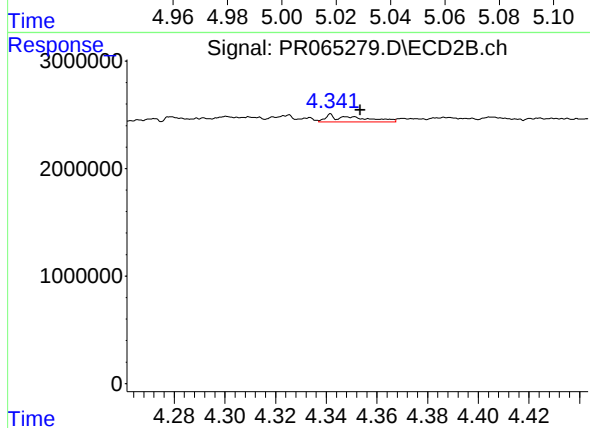

#18 AR-1242-3


R.T.: 4.342 min
Delta R.T.: -0.012 min
Response: 600295
Conc: 5.48 ng/ml

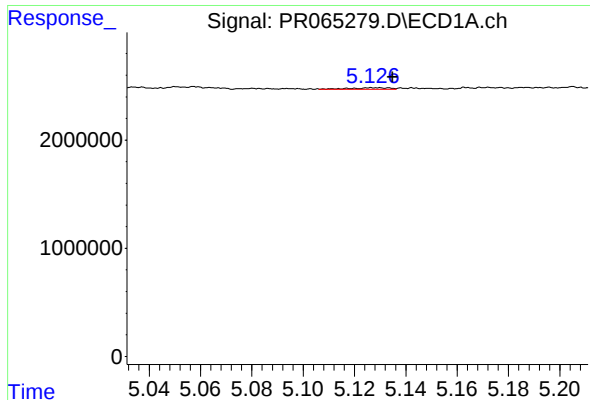

#19 AR-1242-4


R.T.: 5.127 min
Delta R.T.: -0.008 min
Response: 141793
Conc: 1.30 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

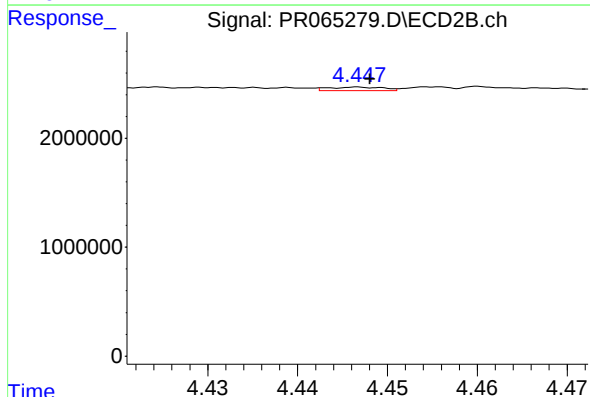


#19 AR-1242-4

R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 130856
Conc: 1.25 ng/ml

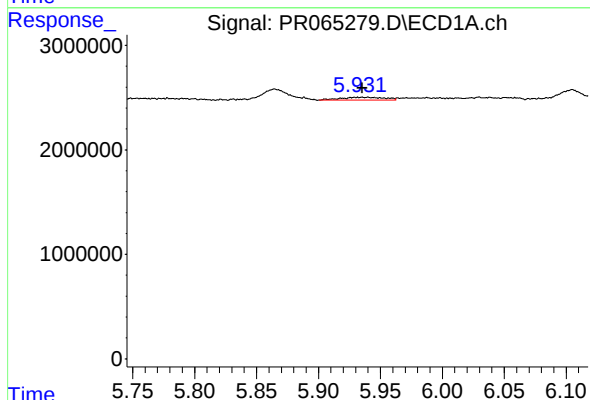


#20 AR-1242-5

R.T.: 5.940 min
Delta R.T.: 0.005 min
Response: 675055
Conc: 5.97 ng/ml

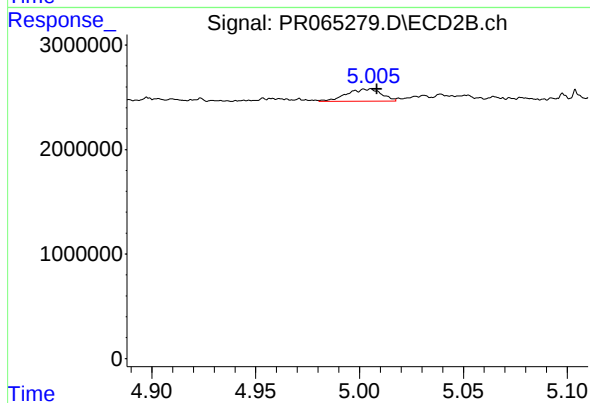

#20 AR-1242-5


R.T.: 5.004 min
Delta R.T.: -0.004 min
Response: 1390544
Conc: 10.30 ng/ml

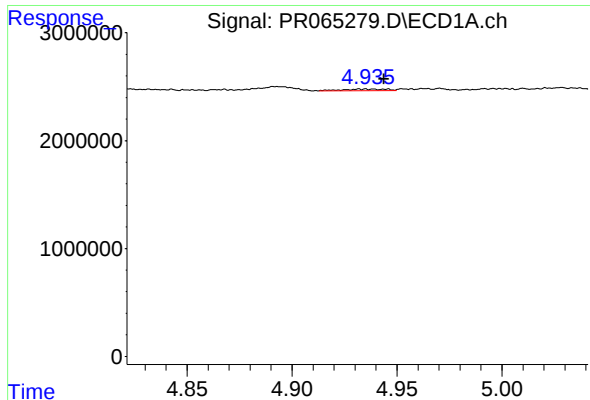

#21 AR-1248-1


R.T.: 4.938 min
Delta R.T.: -0.006 min
Response: 241257
Conc: 2.27 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

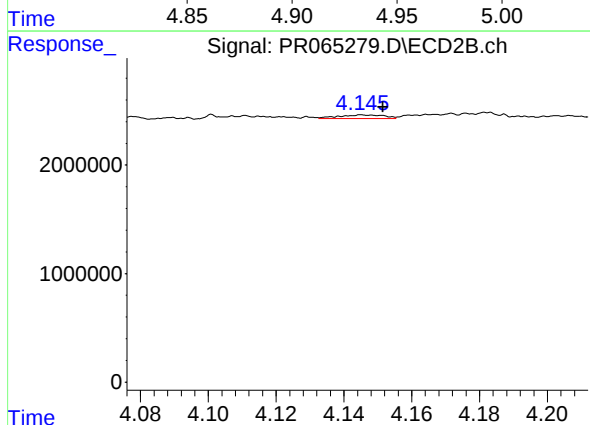


#21 AR-1248-1

R.T.: 4.146 min
Delta R.T.: -0.006 min
Response: 324648
Conc: 3.01 ng/ml

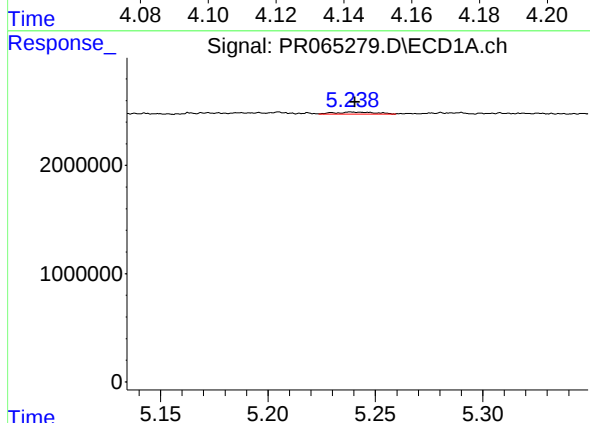


#22 AR-1248-2

R.T.: 5.239 min
Delta R.T.: -0.001 min
Response: 257219
Conc: 1.66 ng/ml

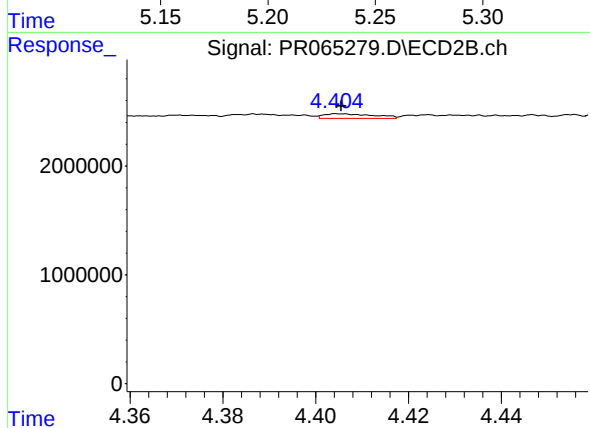

#22 AR-1248-2


R.T.: 4.406 min
Delta R.T.: 0.000 min
Response: 311030
Conc: 2.15 ng/ml

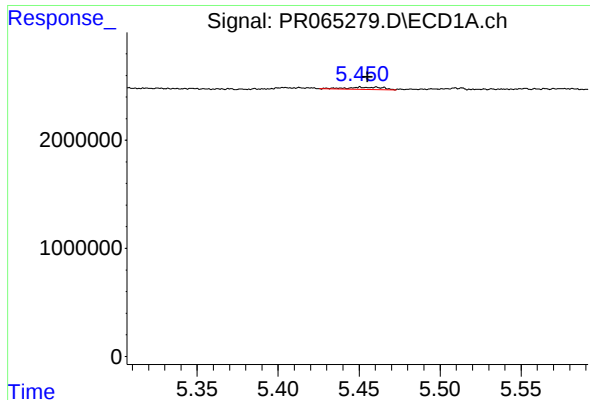

#23 AR-1248-3


R.T.: 5.451 min
Delta R.T.: -0.005 min
Response: 311743
Conc: 1.75 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

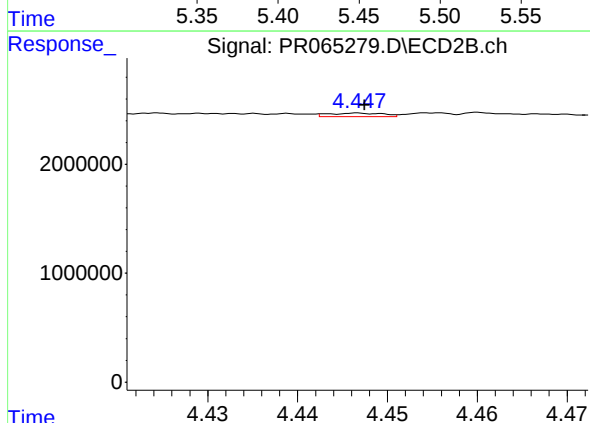


#23 AR-1248-3

R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 130856
Conc: 0.85 ng/ml

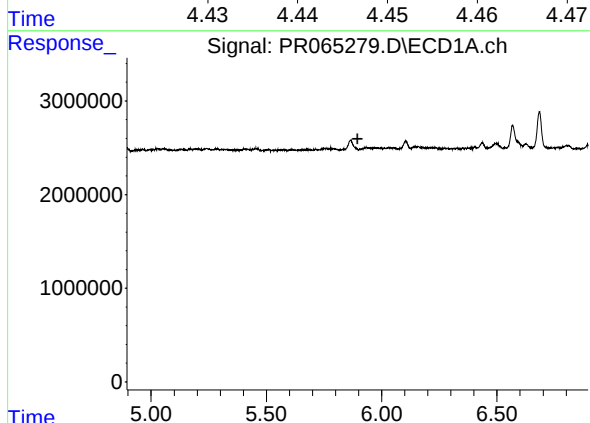


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 5.895 min
Response: 0
Conc: N.D.

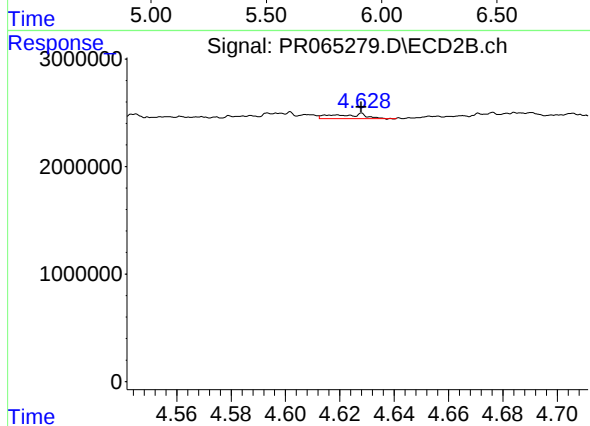

#24 AR-1248-4


R.T.: 4.628 min
Delta R.T.: 0.000 min
Response: 386520
Conc: 2.06 ng/ml

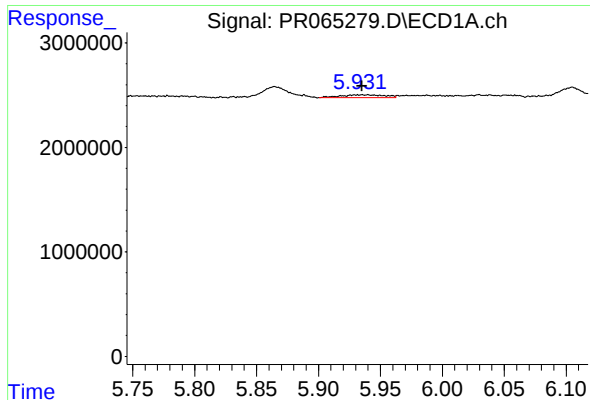

#25 AR-1248-5


R.T.: 5.940 min
Delta R.T.: 0.005 min
Response: 675055
Conc: 3.54 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

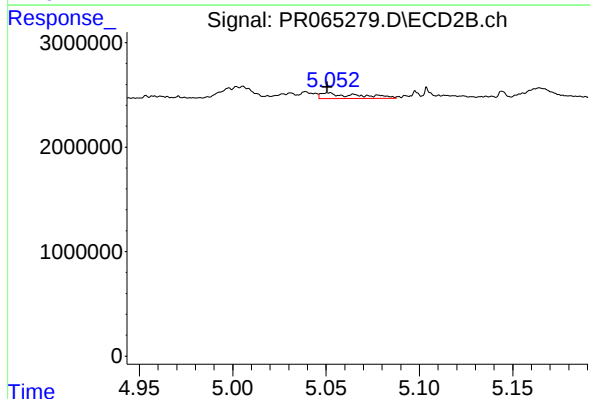


#25 AR-1248-5

R.T.: 5.051 min
Delta R.T.: 0.000 min
Response: 777298
Conc: 4.18 ng/ml

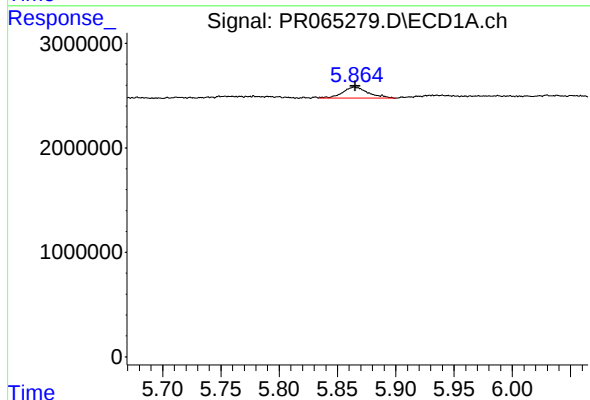


#26 AR-1254-1

R.T.: 5.865 min
Delta R.T.: 0.000 min
Response: 1598938
Conc: 7.81 ng/ml

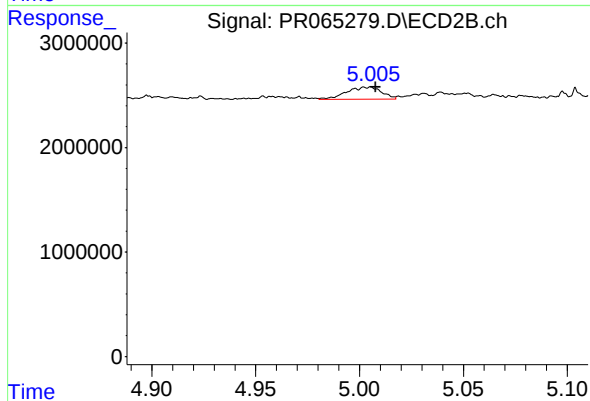

#26 AR-1254-1


R.T.: 5.004 min
Delta R.T.: -0.003 min
Response: 1390544
Conc: 4.77 ng/ml

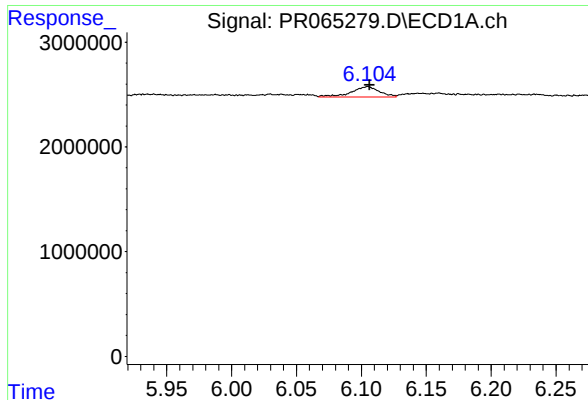

#27 AR-1254-2


R.T.: 6.105 min
Delta R.T.: -0.001 min
Response: 1454895
Conc: 4.67 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

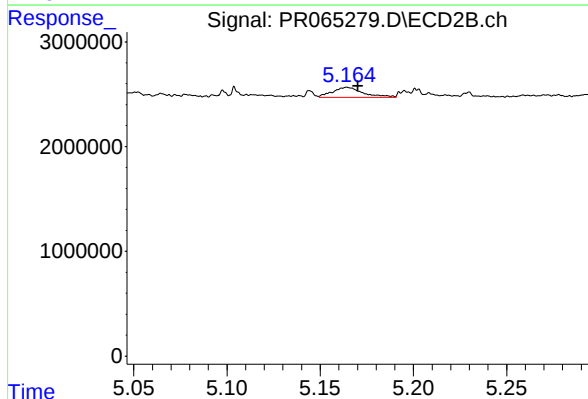


#27 AR-1254-2

R.T.: 5.165 min
Delta R.T.: -0.006 min
Response: 1107380
Conc: 4.37 ng/ml

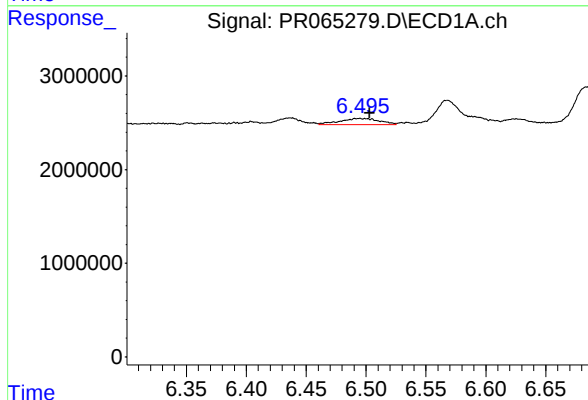


#28 AR-1254-3

R.T.: 6.494 min
Delta R.T.: -0.009 min
Response: 1493167
Conc: 4.67 ng/ml

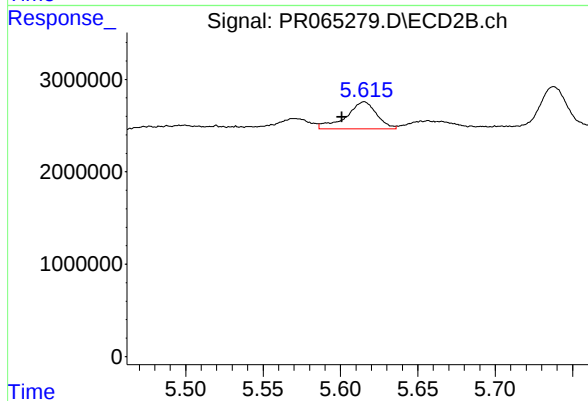

#28 AR-1254-3


R.T.: 5.615 min
Delta R.T.: 0.014 min
Response: 4031528
Conc: 9.85 ng/ml

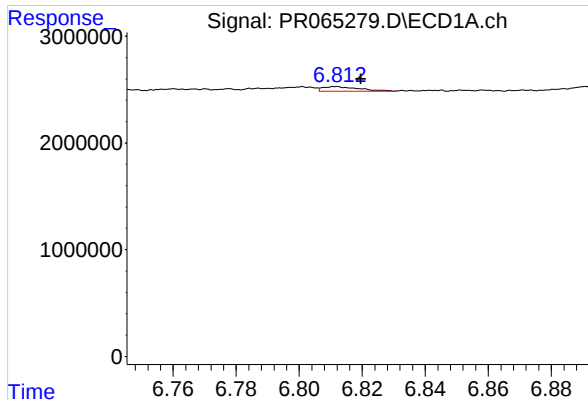

#29 AR-1254-4


R.T.: 6.812 min
Delta R.T.: -0.008 min
Response: 356018
Conc: 1.55 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

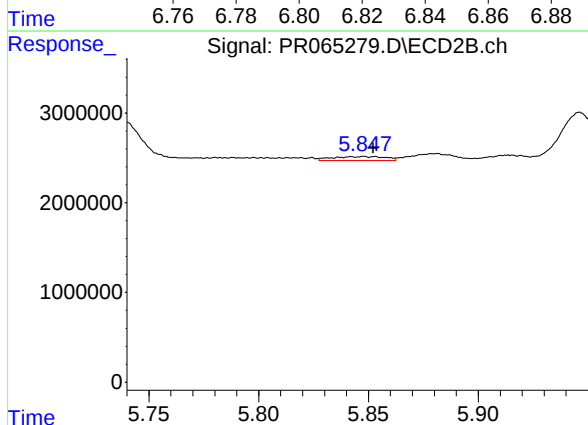


#29 AR-1254-4

R.T.: 5.848 min
Delta R.T.: -0.004 min
Response: 716401
Conc: 2.79 ng/ml

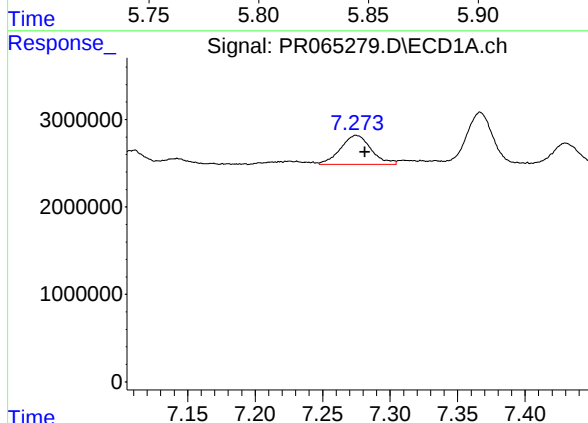


#30 AR-1254-5

R.T.: 7.275 min
Delta R.T.: -0.006 min
Response: 5177692
Conc: 20.83 ng/ml

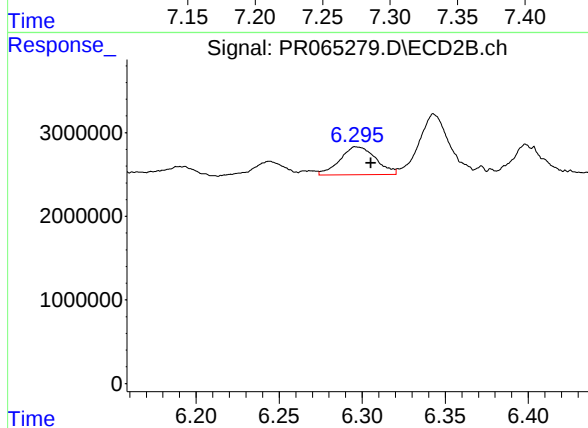

#30 AR-1254-5


R.T.: 6.297 min
Delta R.T.: -0.009 min
Response: 5067371
Conc: 13.82 ng/ml

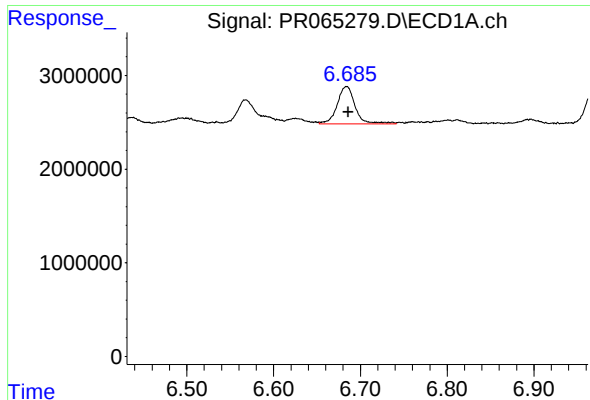

#31 AR-1260-1


R.T.: 6.684 min
Delta R.T.: -0.002 min
Response: 5775390
Conc: 22.97 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

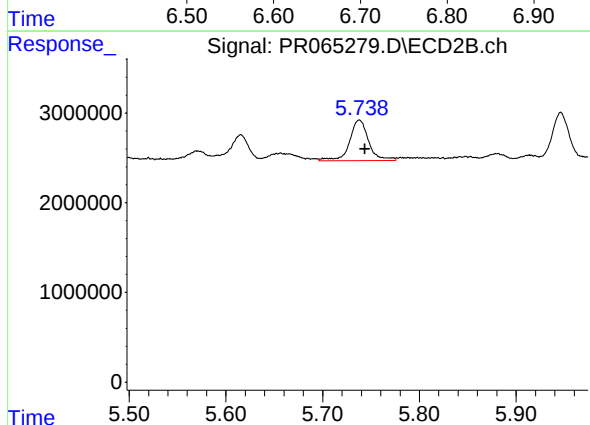


#31 AR-1260-1

R.T.: 5.738 min
Delta R.T.: -0.006 min
Response: 6187431
Conc: 21.68 ng/ml

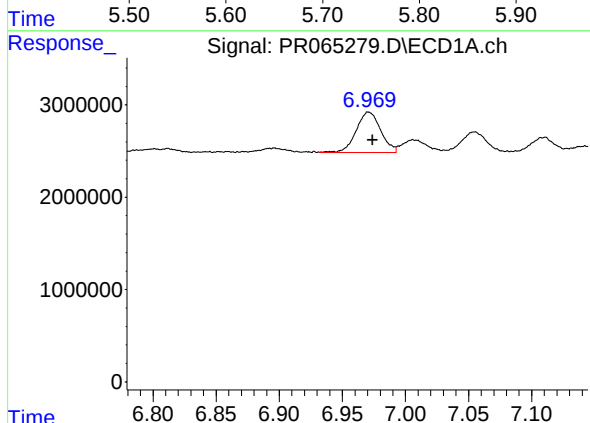


#32 AR-1260-2

R.T.: 6.971 min
Delta R.T.: -0.003 min
Response: 5867506
Conc: 20.42 ng/ml

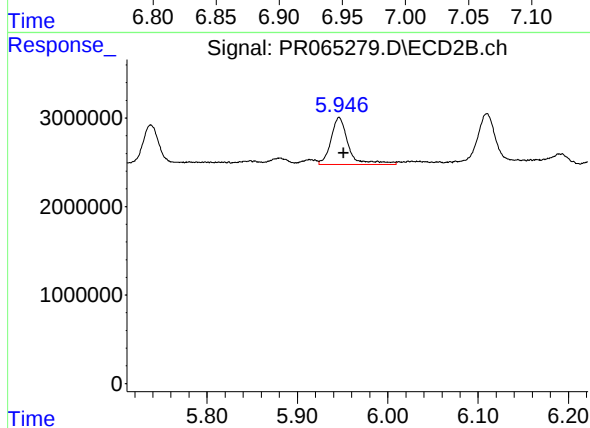

#32 AR-1260-2


R.T.: 5.946 min
Delta R.T.: -0.005 min
Response: 7154621
Conc: 20.63 ng/ml

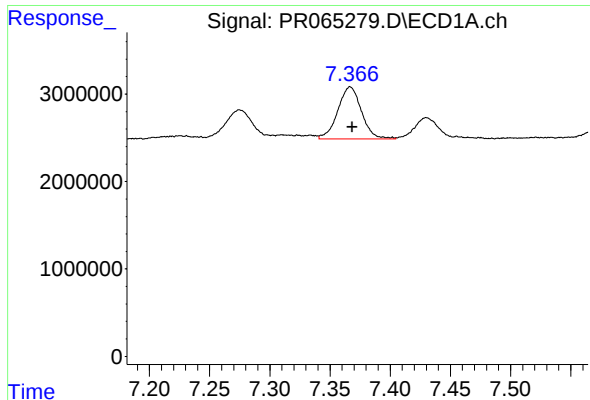

#33 AR-1260-3


R.T.: 7.367 min
Delta R.T.: -0.002 min
Response: 8089189
Conc: 38.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

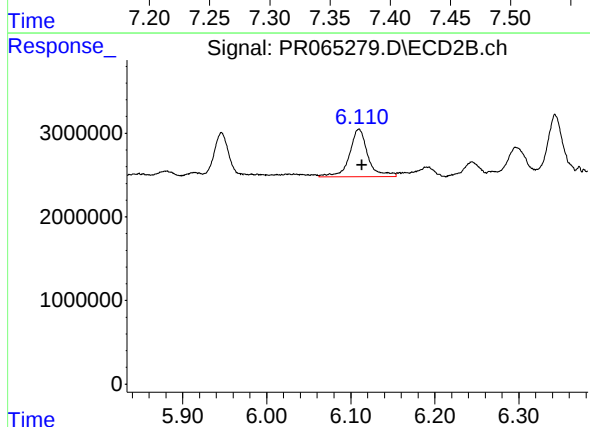


#33 AR-1260-3

R.T.: 6.110 min
Delta R.T.: -0.004 min
Response: 8736203
Conc: 26.89 ng/ml

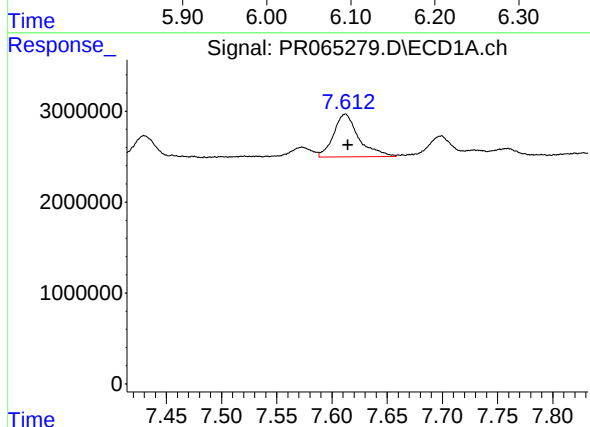


#34 AR-1260-4

R.T.: 7.612 min
Delta R.T.: -0.002 min
Response: 7463570
Conc: 31.63 ng/ml

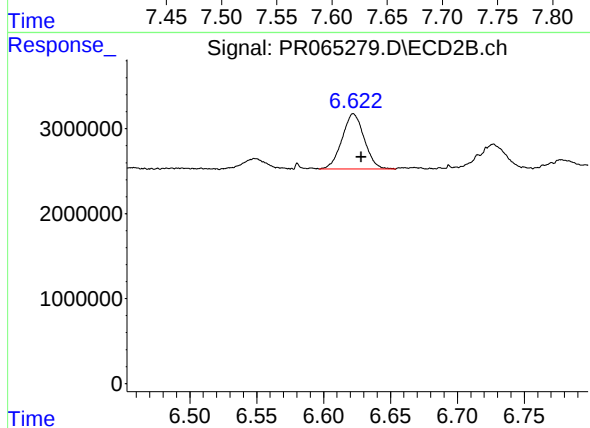

#34 AR-1260-4


R.T.: 6.622 min
Delta R.T.: -0.006 min
Response: 7515606
Conc: 28.45 ng/ml

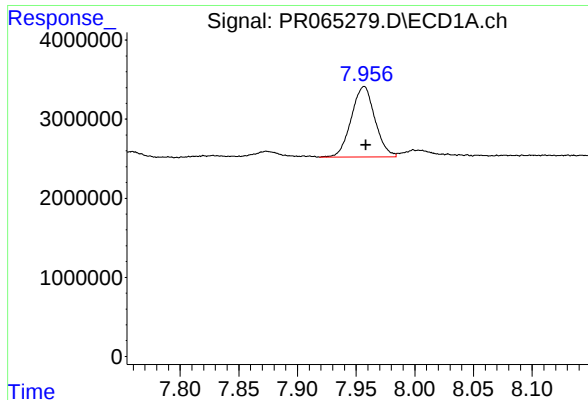

#35 AR-1260-5


R.T.: 7.957 min
Delta R.T.: -0.002 min
Response: 12487322
Conc: 28.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

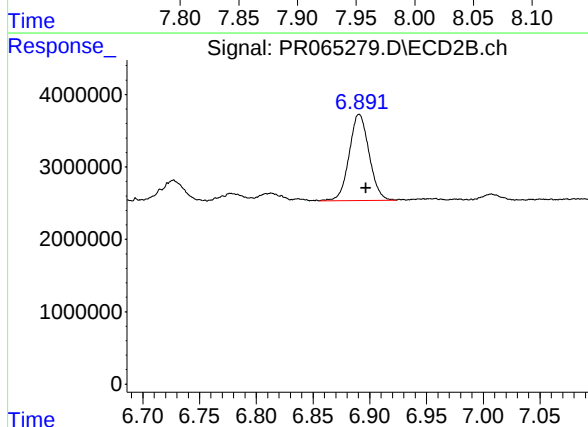


#35 AR-1260-5

R.T.: 6.891 min
Delta R.T.: -0.006 min
Response: 14518958
Conc: 23.54 ng/ml

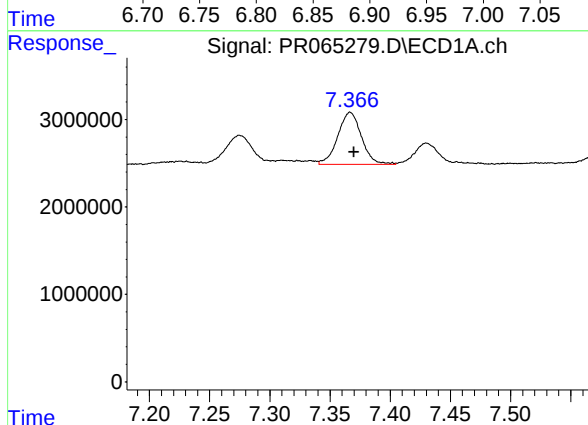


#36 AR-1262-1

R.T.: 7.367 min
Delta R.T.: -0.003 min
Response: 8089189
Conc: 23.90 ng/ml

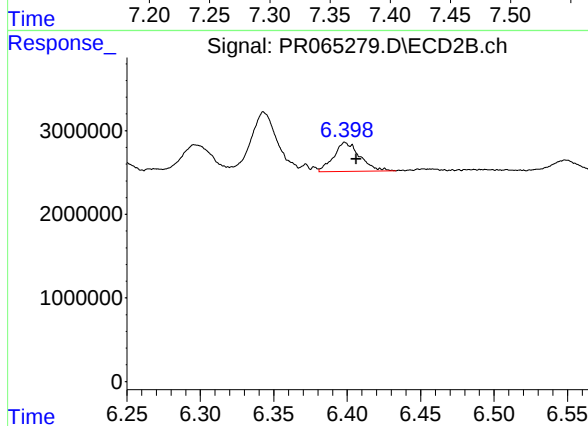

#36 AR-1262-1


R.T.: 6.399 min
Delta R.T.: -0.008 min
Response: 4321107
Conc: 24.09 ng/ml

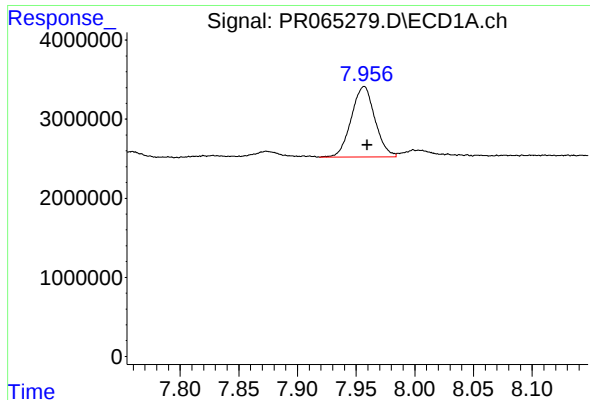

#37 AR-1262-2


R.T.: 7.957 min
Delta R.T.: -0.003 min
Response: 12487322
Conc: 22.08 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

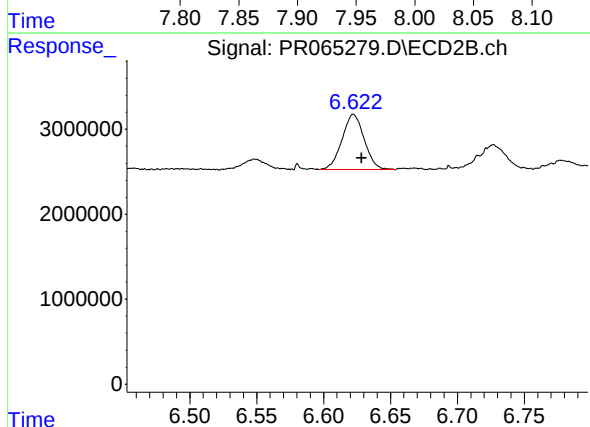


#37 AR-1262-2

R.T.: 6.622 min
Delta R.T.: -0.006 min
Response: 7515606
Conc: 19.32 ng/ml

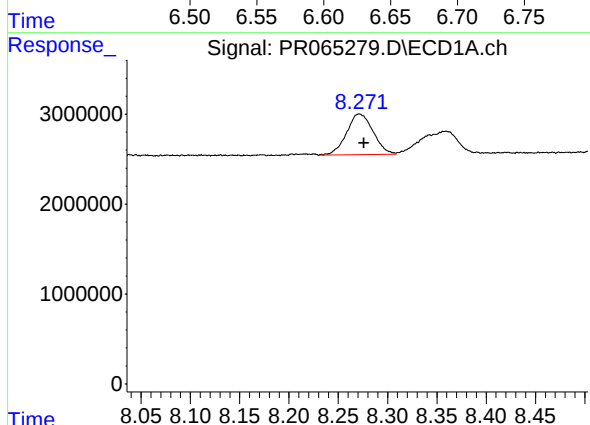


#38 AR-1262-3

R.T.: 8.271 min
Delta R.T.: -0.004 min
Response: 8457934
Conc: 22.23 ng/ml

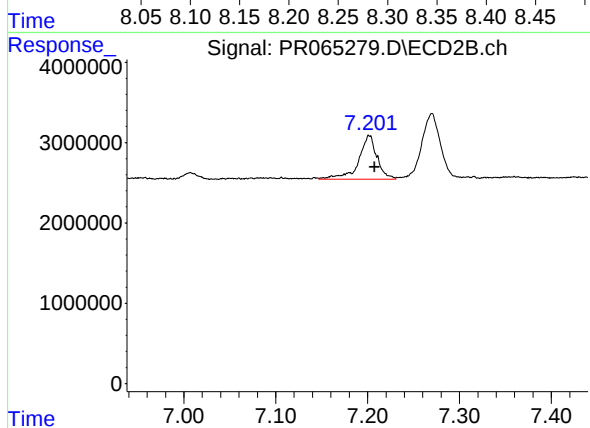

#38 AR-1262-3


R.T.: 7.202 min
Delta R.T.: -0.006 min
Response: 7522420
Conc: 26.54 ng/ml

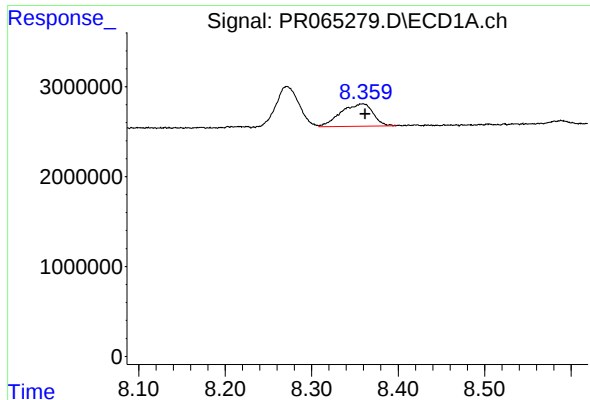

#39 AR-1262-4


R.T.: 8.359 min
Delta R.T.: -0.003 min
Response: 6489172
Conc: 22.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

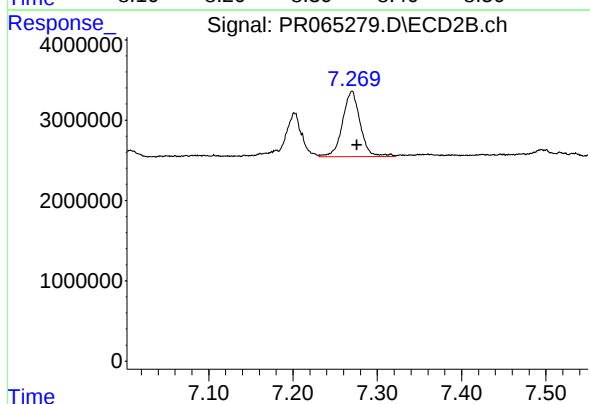


#39 AR-1262-4

R.T.: 7.270 min
Delta R.T.: -0.006 min
Response: 11828738
Conc: 20.54 ng/ml

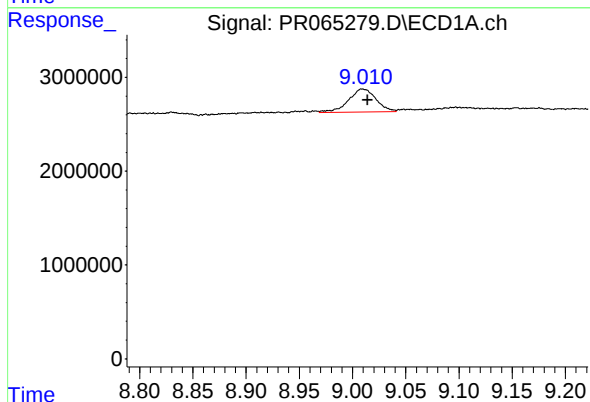


#40 AR-1262-5

R.T.: 9.009 min
Delta R.T.: -0.005 min
Response: 4453933
Conc: 22.23 ng/ml

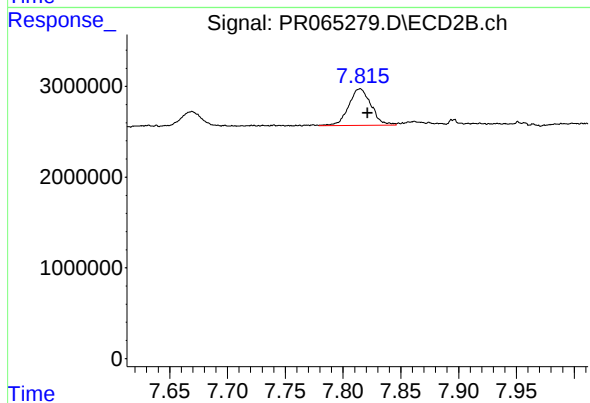

#40 AR-1262-5


R.T.: 7.815 min
Delta R.T.: -0.007 min
Response: 5399520
Conc: 20.75 ng/ml

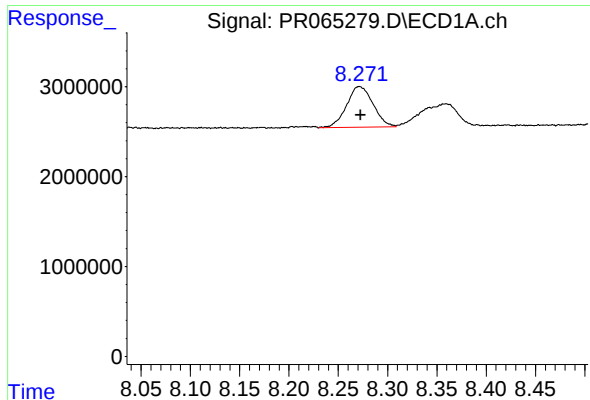

#41 AR-1268-1


R.T.: 8.271 min
Delta R.T.: -0.001 min
Response: 8457934
Conc: 13.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

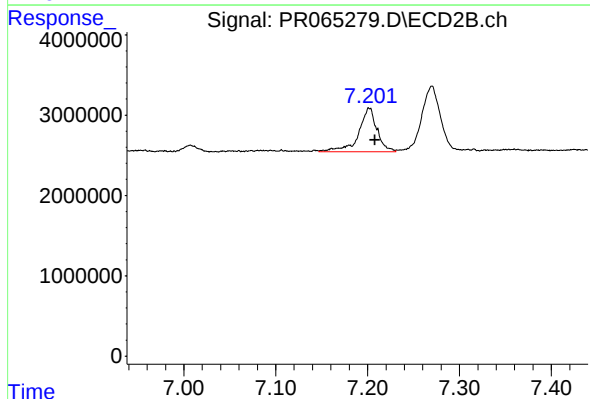


#41 AR-1268-1

R.T.: 7.202 min
Delta R.T.: -0.006 min
Response: 7522420
Conc: 9.48 ng/ml

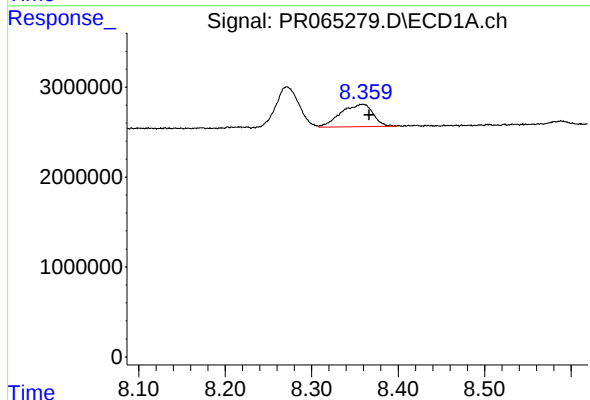


#42 AR-1268-2

R.T.: 8.359 min
Delta R.T.: -0.008 min
Response: 6489172
Conc: 11.86 ng/ml

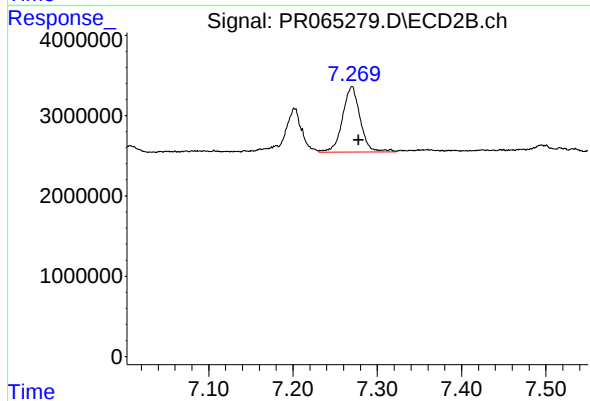

#42 AR-1268-2


R.T.: 7.270 min
Delta R.T.: -0.008 min
Response: 11828738
Conc: 15.89 ng/ml

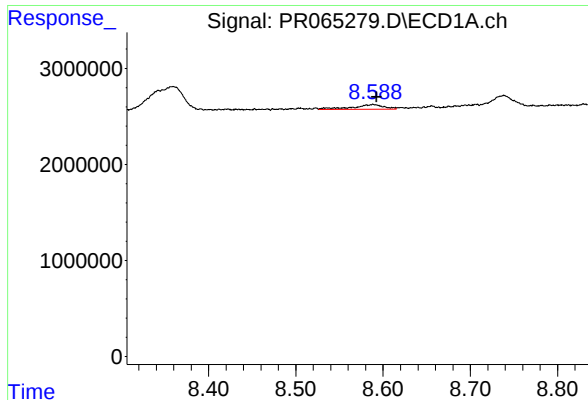

#43 AR-1268-3


R.T.: 8.588 min
Delta R.T.: -0.004 min
Response: 1226490
Conc: 2.58 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

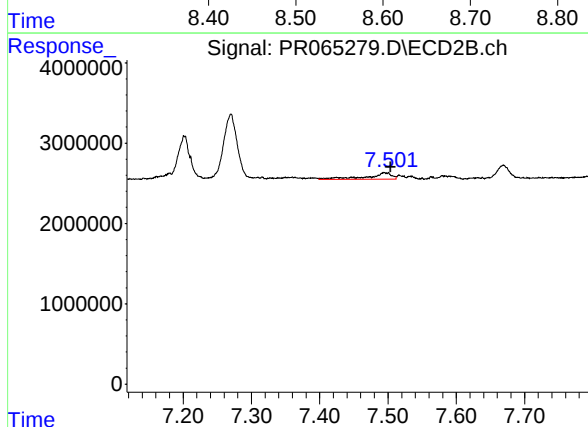


#43 AR-1268-3

R.T.: 7.494 min
Delta R.T.: -0.010 min
Response: 2055213
Conc: 3.24 ng/ml

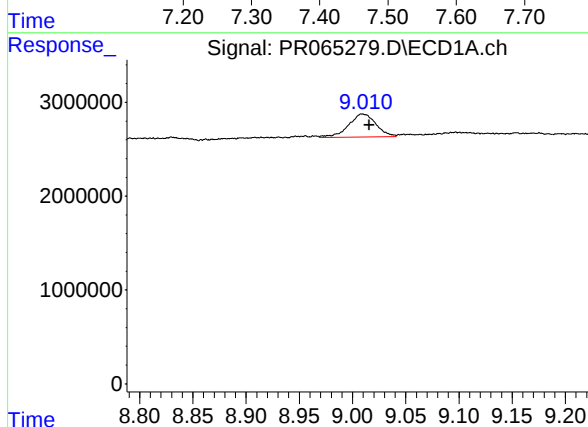


#44 AR-1268-4

R.T.: 9.009 min
Delta R.T.: -0.006 min
Response: 4453933
Conc: 21.89 ng/ml

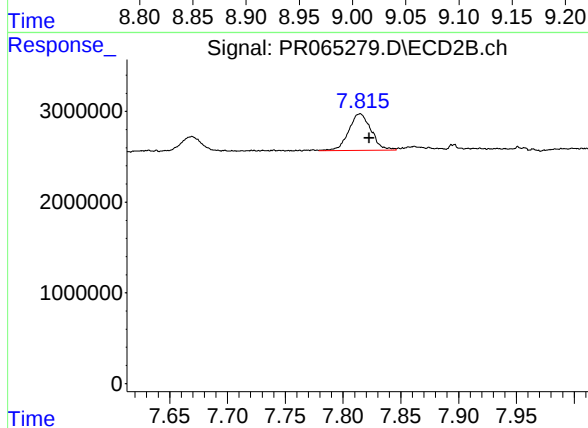

#44 AR-1268-4


R.T.: 7.815 min
Delta R.T.: -0.008 min
Response: 5399520
Conc: 20.58 ng/ml

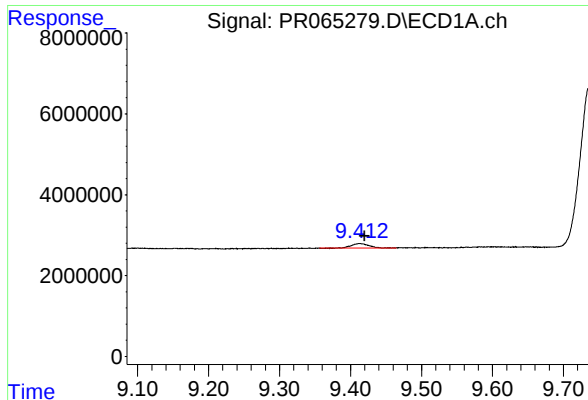

#45 AR-1268-5

R.T.: 9.413 min
Delta R.T.: -0.007 min
Response: 1837538
Conc: 1.26 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

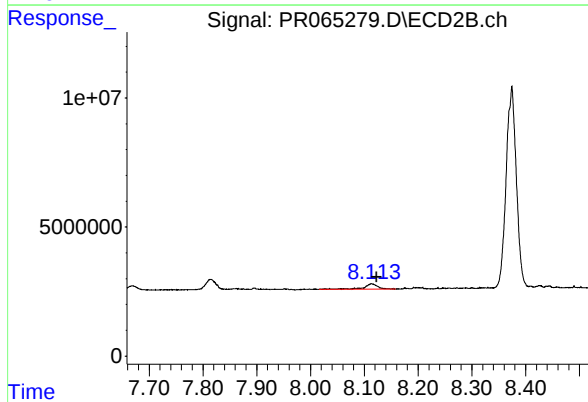

#45 AR-1268-5

R.T.: 8.114 min
Delta R.T.: -0.009 min
Response: 3639010
Conc: 1.90 ng/ml