

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
 Data File : PR065280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 19:35
 Operator : AJ\MA
 Sample : P1187-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:35:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.722f	3.003	100.5E6	102.2E6	16.844	18.690
2) SA Decachlor...	9.760f	8.373	77981935	91704989	19.498	19.377
Target Compounds						
3) L1 AR-1016-1	0.000	4.146	0	347782	N.D.	1.915 #
4) L1 AR-1016-2	0.000	4.164	0	863920	N.D.	3.494 #
5) L1 AR-1016-3	0.000	4.357	0	235620	N.D.	1.738 #
6) L1 AR-1016-4	0.000	4.402	0	565563	N.D.	5.400 #
7) L1 AR-1016-5	0.000	4.611f	0	479434	N.D.	3.437 #
8) L2 AR-1221-1	3.936	3.230	425195	130550	5.924	2.108 #
9) L2 AR-1221-2	4.038f	3.314	2146886	2026269	40.952	42.484
10) L2 AR-1221-3	4.088	3.402	684413	785089	4.455	5.684 #
11) L3 AR-1232-1	4.088	3.402	684413	785089	5.064	6.555 #
12) L3 AR-1232-2	4.660	4.164	658804	863920	8.551	7.071
13) L3 AR-1232-3	0.000	4.357	0	235620	N.D.	3.542 #
14) L3 AR-1232-4	0.000	4.439	0	240795	N.D.	4.205 #
15) L3 AR-1232-5	5.238	4.611f	265187	479434	5.483	7.521 #
16) L4 AR-1242-1	0.000	4.146	0	347782	N.D.	2.380 #
17) L4 AR-1242-2	0.000	4.164	0	863920	N.D.	4.331 #
18) L4 AR-1242-3	0.000	4.357	0	235620	N.D.	2.152 #
19) L4 AR-1242-4	0.000	4.439	0	240795	N.D.	2.294 #
20) L4 AR-1242-5	5.957f	5.003	424884	693918	3.756	5.139 #
21) L5 AR-1248-1	4.914f	4.146	332646	347782	3.126	3.220
22) L5 AR-1248-2	5.238	4.402	265187	565563	1.707	3.905 #
23) L5 AR-1248-3	0.000	4.439	0	240795	N.D.	1.556 #
24) L5 AR-1248-4	5.890	4.611f	952413	479434	5.024	2.560 #
25) L5 AR-1248-5	5.957f	5.060	424884	372517	2.230	2.001
26) L6 AR-1254-1	5.890f	5.003	952413	693918	4.650	2.381 #
27) L6 AR-1254-2	6.125f	5.183	595801	403772	1.912	1.594
28) L6 AR-1254-3	6.514	5.594	909516	688777	2.843	1.683 #
29) L6 AR-1254-4	6.827	5.835f	504522	258212	2.202	1.006 #
30) L6 AR-1254-5	7.286	6.290f	220235	242425	0.886	0.661 #
31) L7 AR-1260-1	6.696	5.733	207588	388620	0.826	1.361 #
32) L7 AR-1260-2	6.973	5.952	32957	205005	0.115	0.591 #
33) L7 AR-1260-3	7.388f	6.110	2644583	2923386	12.509	8.998 #
34) L7 AR-1260-4	0.000	6.621	0	3937828	N.D.	14.905 #
35) L7 AR-1260-5	7.977f	6.891	1295369	1911766	2.946	3.100
36) L8 AR-1262-1	7.388f	6.404	2644583	597665	7.813	3.332 #
37) L8 AR-1262-2	7.977f	6.621	1295369	3937828	2.290	10.120 #
38) L8 AR-1262-3	8.290	7.201	13178037	15998579	34.631	56.444 #
39) L8 AR-1262-4	8.383f	7.272	11607954	14331662	39.627	24.886 #
40) L8 AR-1262-5	9.031f	7.814	4956406	5386964	24.733	20.697
41) L9 AR-1268-1	8.290f	7.201	13178037	15998579	21.736	20.166

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
Data File : PR065280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 19:35
Operator : AJ\MA
Sample : P1187-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 71 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:35:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.383f	7.272	11607954	14331662	21.214	19.251
43)	L9 AR-1268-3	8.609f	7.496	10129147	13371488	21.348	21.107
44)	L9 AR-1268-4	9.031f	7.814	4956406	5386964	24.358	20.537
45)	L9 AR-1268-5	9.435f	8.115	29466034	36931649	20.214	19.290



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
Data File : PR065280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 19:35
Operator : AJ\MA
Sample : P1187-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 71 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:35:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

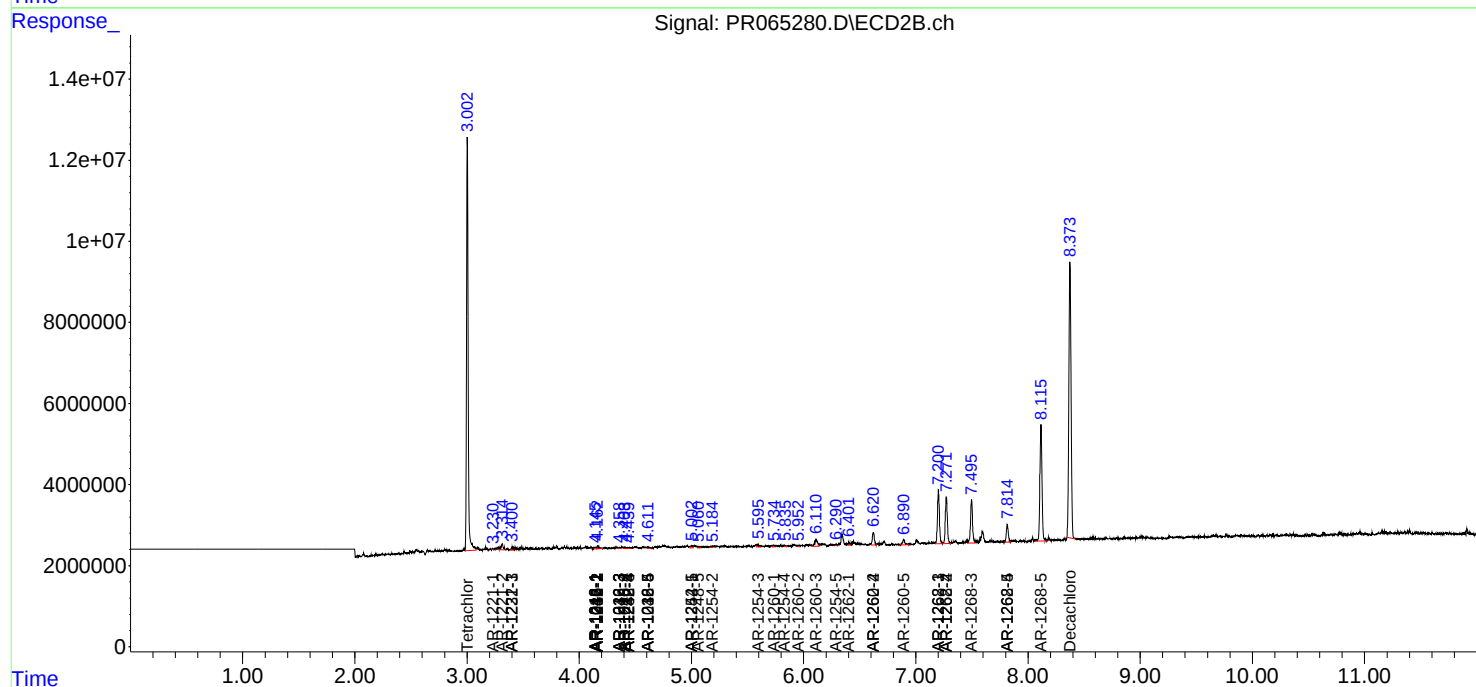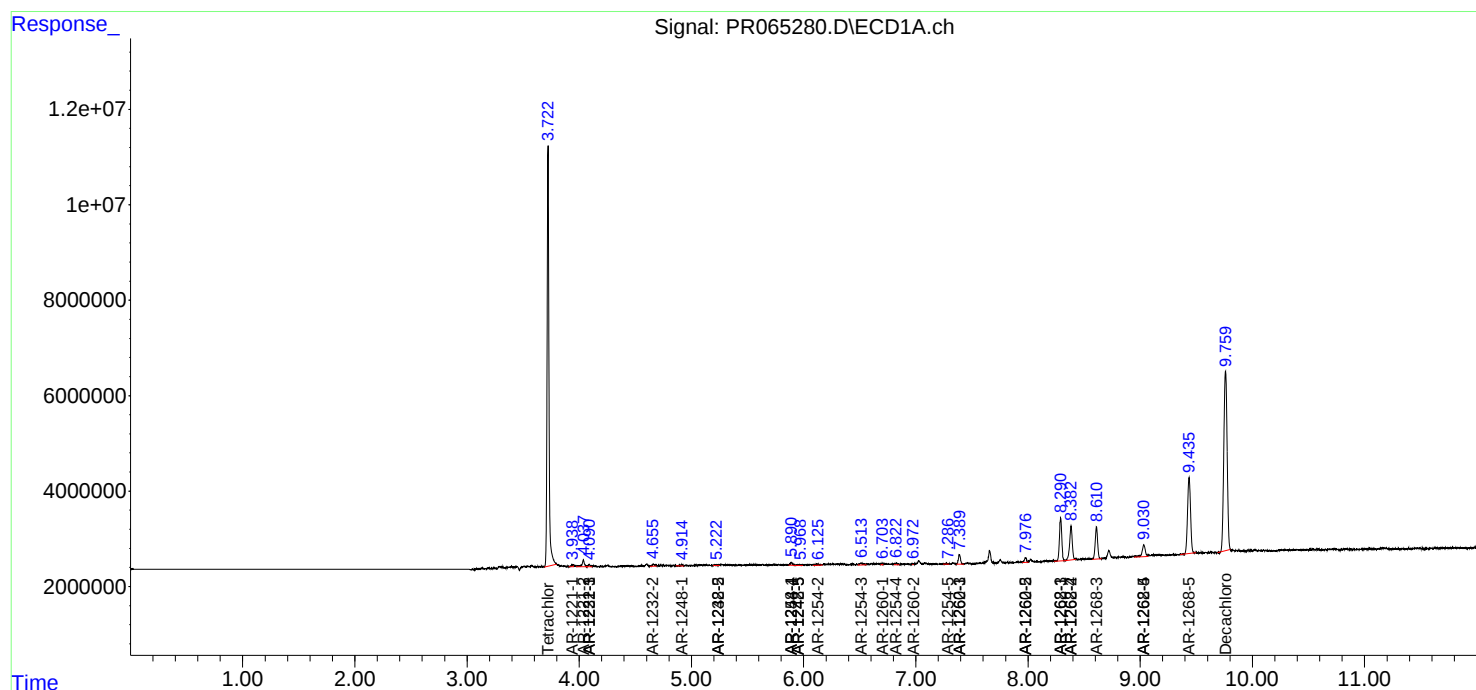


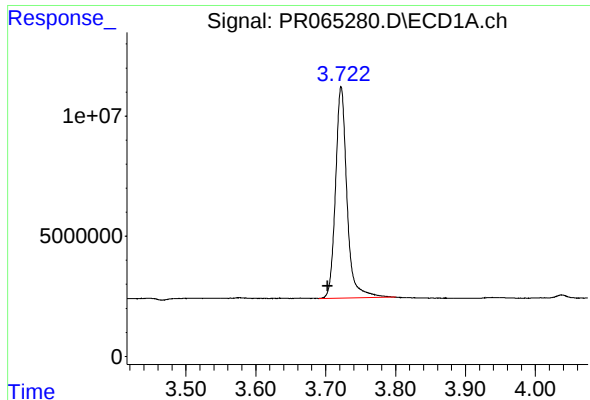

#1 Tetrachloro-m-xylene


R.T.: 3.722 min
Delta R.T.: 0.019 min
Response: 100544074
Conc: 16.84 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

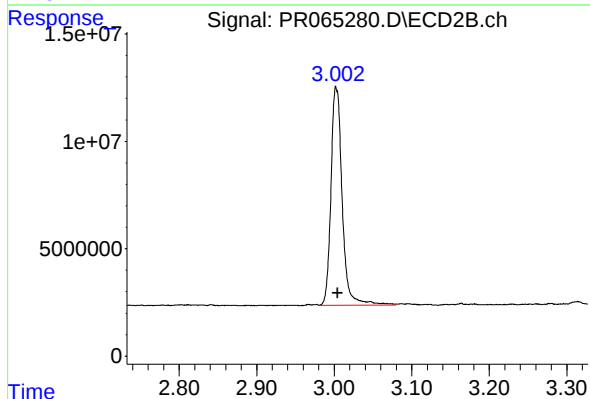


#1 Tetrachloro-m-xylene

R.T.: 3.003 min
Delta R.T.: -0.002 min
Response: 102232985
Conc: 18.69 ng/ml

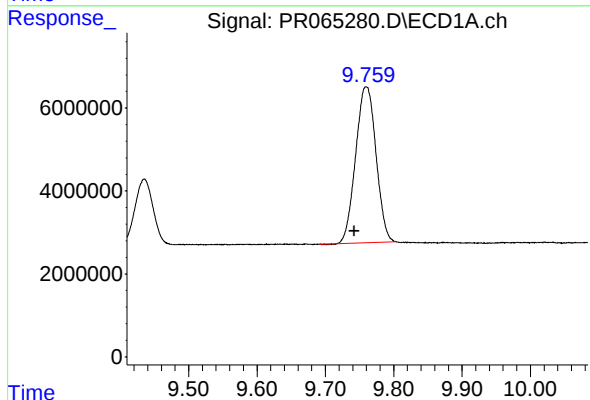


#2 Decachlorobiphenyl

R.T.: 9.760 min
Delta R.T.: 0.018 min
Response: 77981935
Conc: 19.50 ng/ml

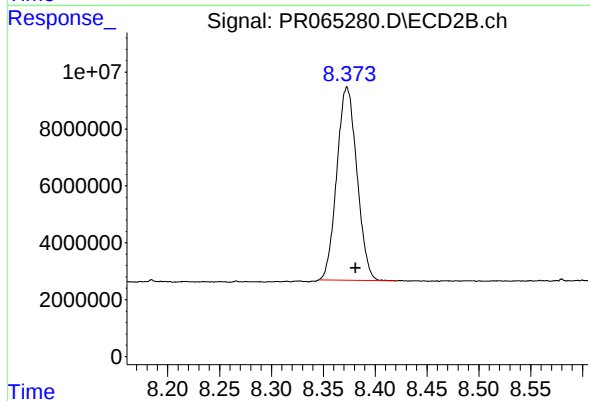

#2 Decachlorobiphenyl


R.T.: 8.373 min
Delta R.T.: -0.008 min
Response: 91704989
Conc: 19.38 ng/ml

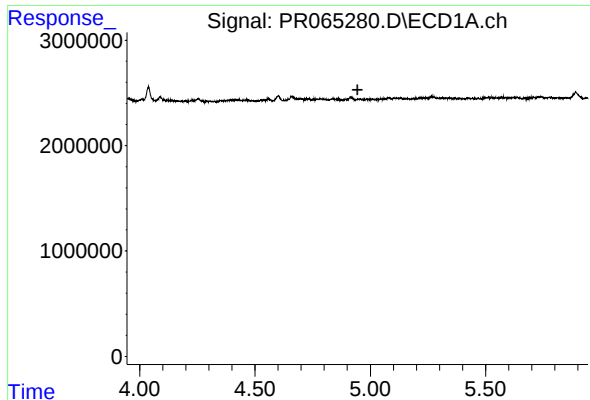

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 4.944 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

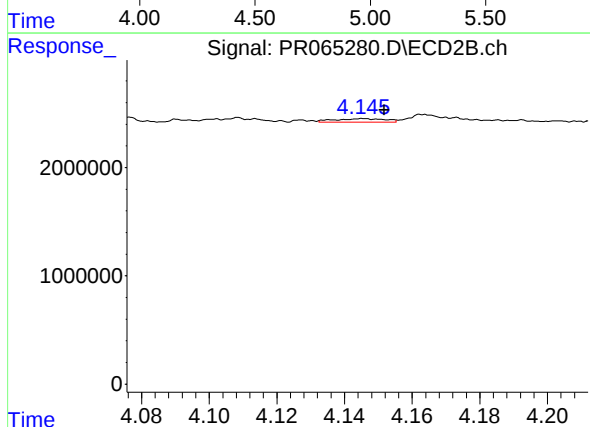


#3 AR-1016-1

R.T.: 4.146 min
Delta R.T.: -0.006 min
Response: 347782
Conc: 1.92 ng/ml

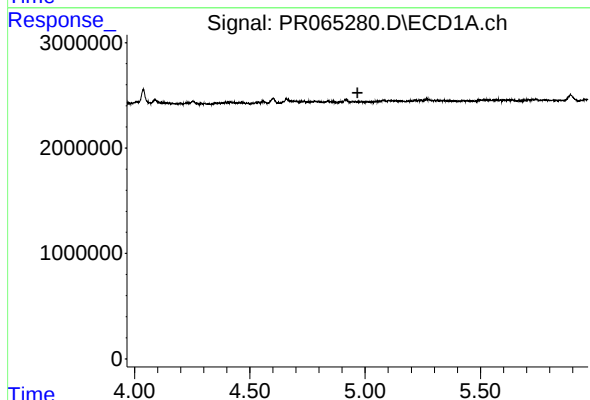


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 4.967 min
Response: 0
Conc: N.D.

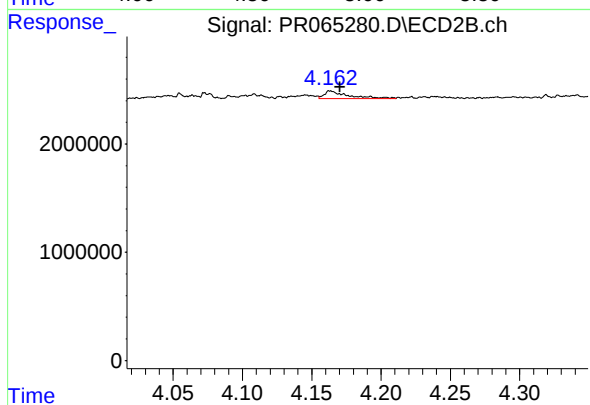

#4 AR-1016-2


R.T.: 4.164 min
Delta R.T.: -0.007 min
Response: 863920
Conc: 3.49 ng/ml

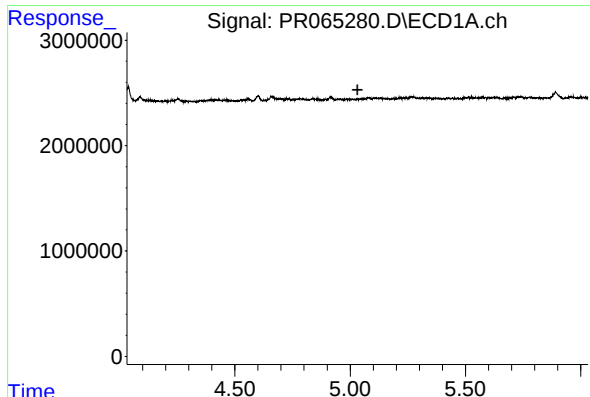

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.032 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

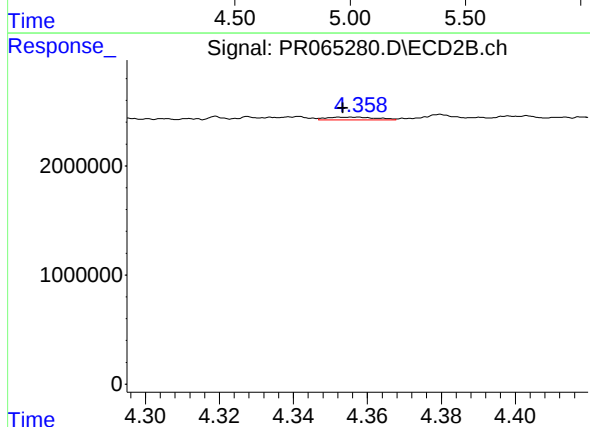


#5 AR-1016-3

R.T.: 4.357 min
Delta R.T.: 0.003 min
Response: 235620
Conc: 1.74 ng/ml

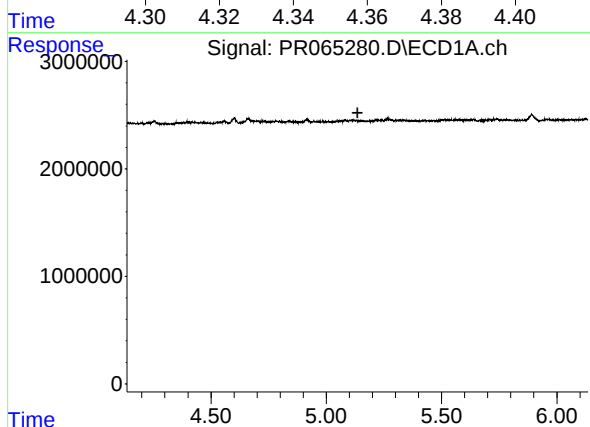


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.135 min
Response: 0
Conc: N.D.

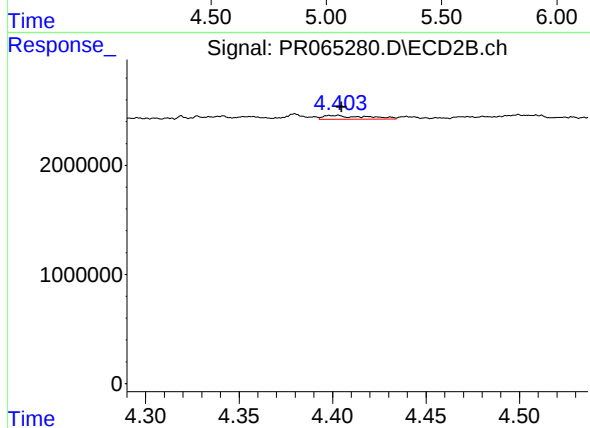

#6 AR-1016-4


R.T.: 4.402 min
Delta R.T.: -0.002 min
Response: 565563
Conc: 5.40 ng/ml

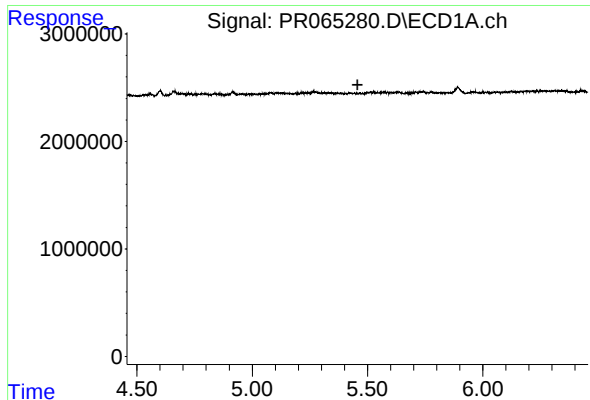

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

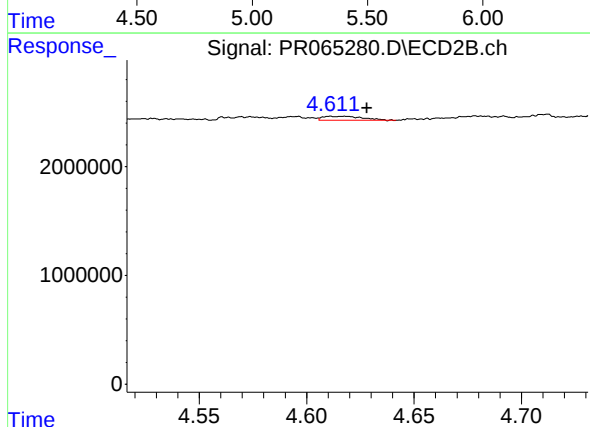


#7 AR-1016-5

R.T.: 4.611 min
Delta R.T.: -0.017 min
Response: 479434
Conc: 3.44 ng/ml

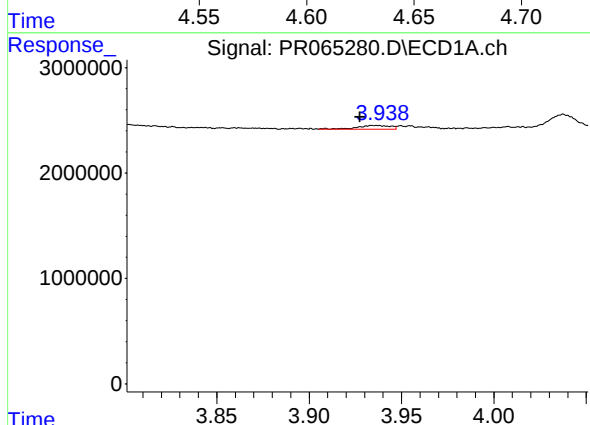


#8 AR-1221-1

R.T.: 3.936 min
Delta R.T.: 0.008 min
Response: 425195
Conc: 5.92 ng/ml

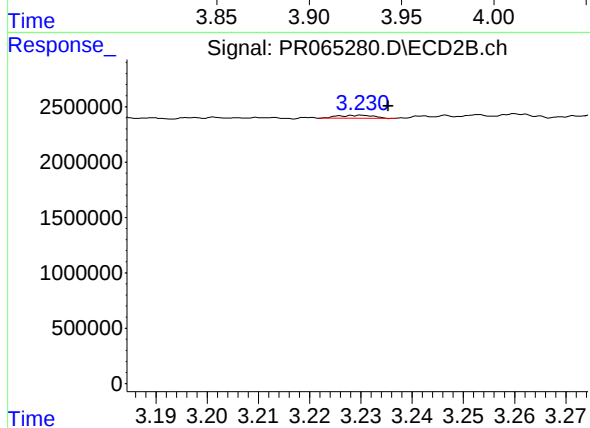

#8 AR-1221-1


R.T.: 3.230 min
Delta R.T.: -0.005 min
Response: 130550
Conc: 2.11 ng/ml

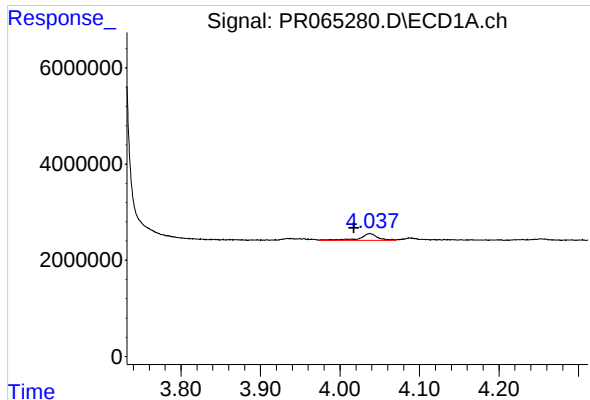

#9 AR-1221-2


R.T.: 4.038 min
Delta R.T.: 0.020 min
Response: 2146886
Conc: 40.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

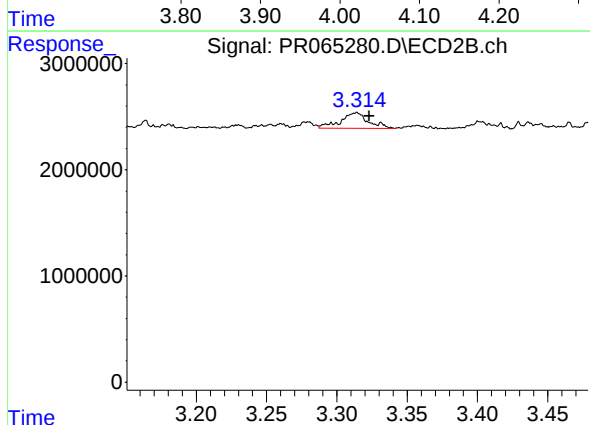


#9 AR-1221-2

R.T.: 3.314 min
Delta R.T.: -0.009 min
Response: 2026269
Conc: 42.48 ng/ml

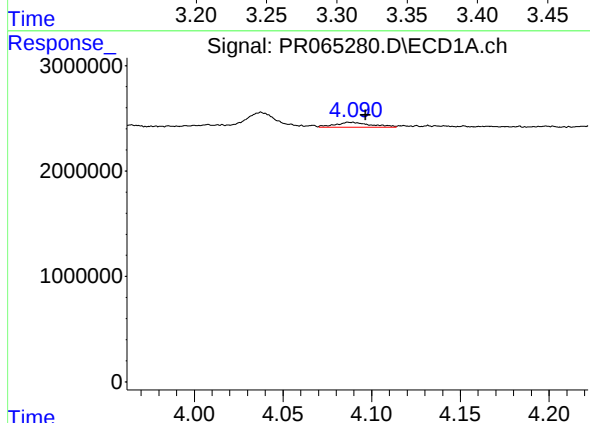


#10 AR-1221-3

R.T.: 4.088 min
Delta R.T.: -0.009 min
Response: 684413
Conc: 4.45 ng/ml

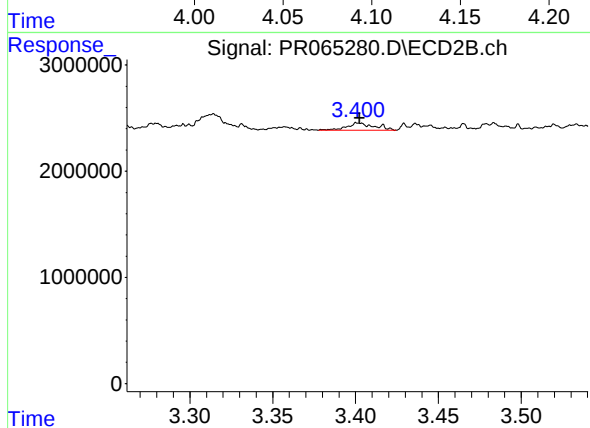

#10 AR-1221-3


R.T.: 3.402 min
Delta R.T.: 0.000 min
Response: 785089
Conc: 5.68 ng/ml

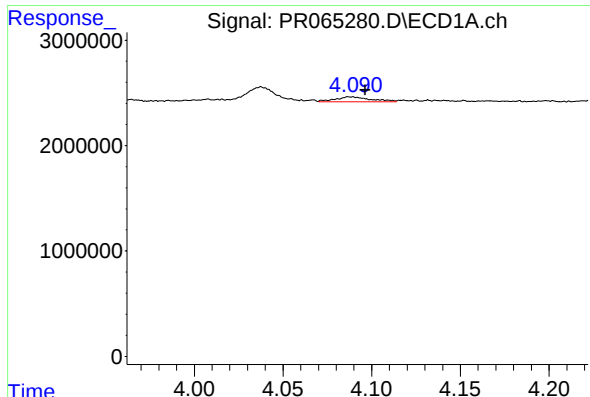

#11 AR-1232-1


R.T.: 4.088 min
Delta R.T.: -0.008 min
Response: 684413
Conc: 5.06 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

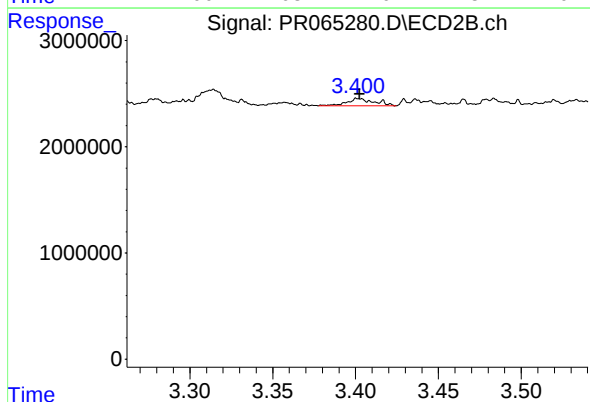


#11 AR-1232-1

R.T.: 3.402 min
Delta R.T.: 0.000 min
Response: 785089
Conc: 6.56 ng/ml

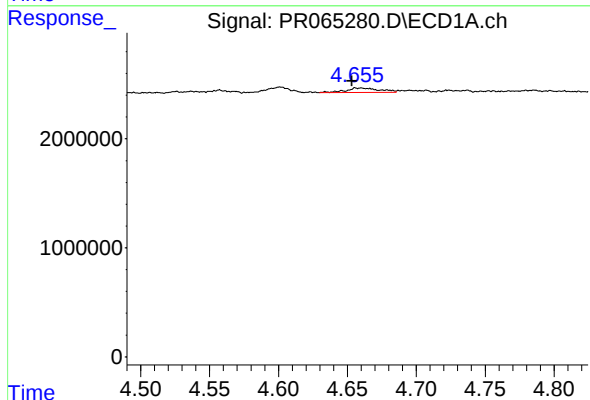


#12 AR-1232-2

R.T.: 4.660 min
Delta R.T.: 0.007 min
Response: 658804
Conc: 8.55 ng/ml

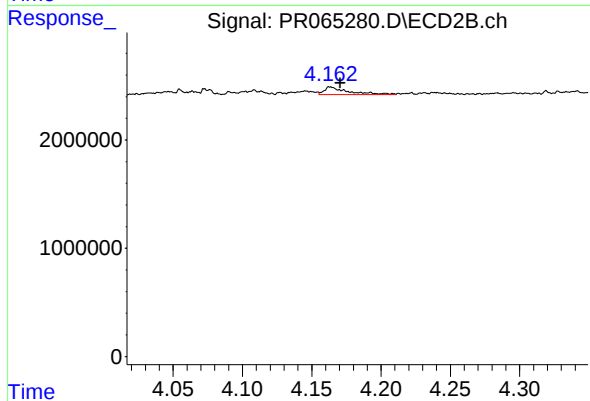

#12 AR-1232-2


R.T.: 4.164 min
Delta R.T.: -0.007 min
Response: 863920
Conc: 7.07 ng/ml

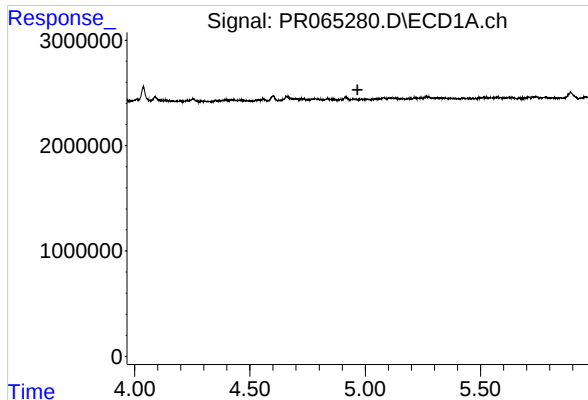

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 4.966 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

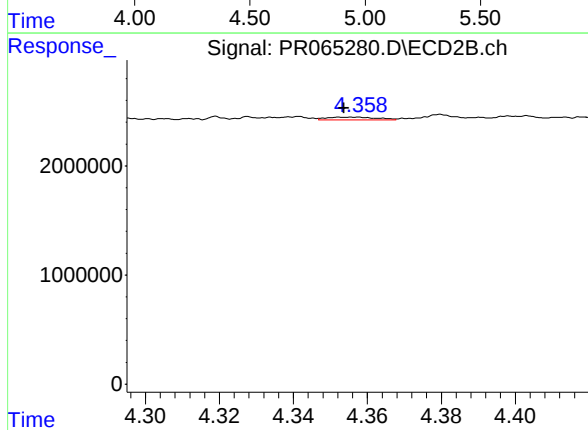


#13 AR-1232-3

R.T.: 4.357 min
Delta R.T.: 0.003 min
Response: 235620
Conc: 3.54 ng/ml

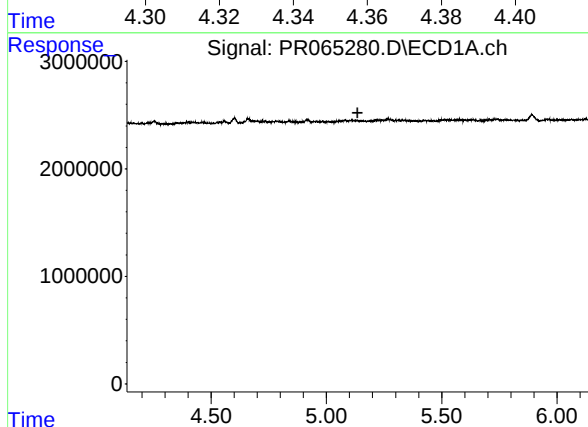


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.135 min
Response: 0
Conc: N.D.

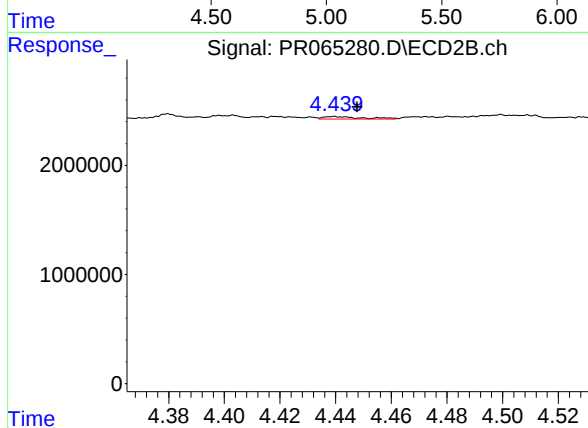

#14 AR-1232-4


R.T.: 4.439 min
Delta R.T.: -0.008 min
Response: 240795
Conc: 4.21 ng/ml

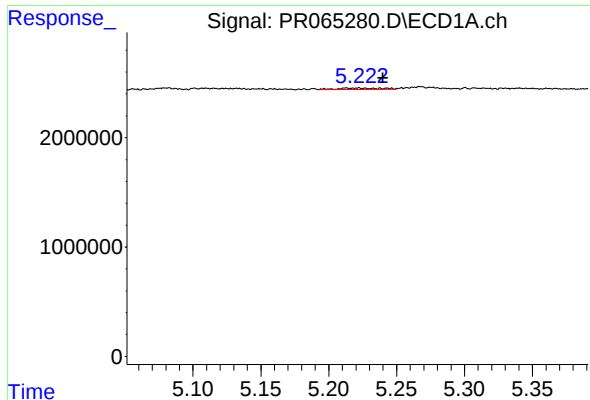

#15 AR-1232-5


R.T.: 5.238 min
Delta R.T.: -0.002 min
Response: 265187
Conc: 5.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

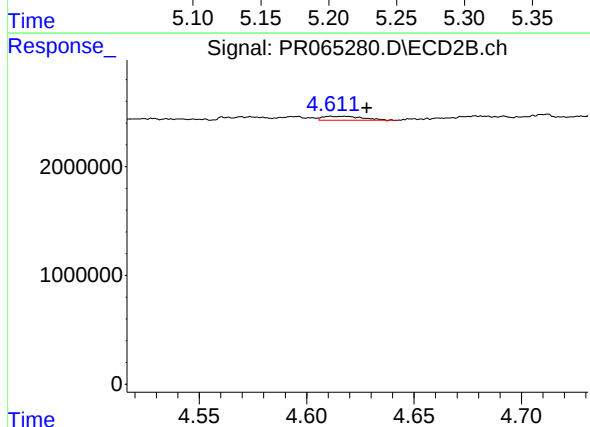


#15 AR-1232-5

R.T.: 4.611 min
Delta R.T.: -0.017 min
Response: 479434
Conc: 7.52 ng/ml

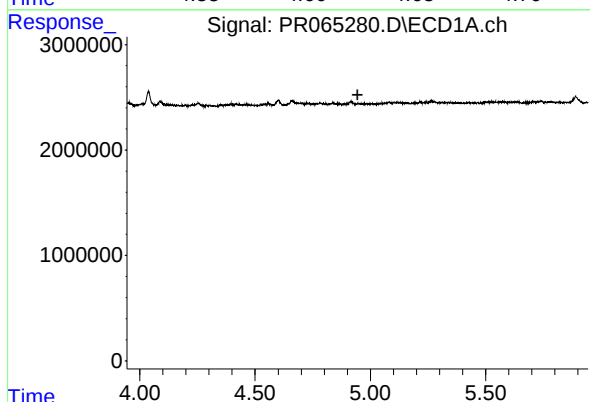


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 4.944 min
Response: 0
Conc: N.D.

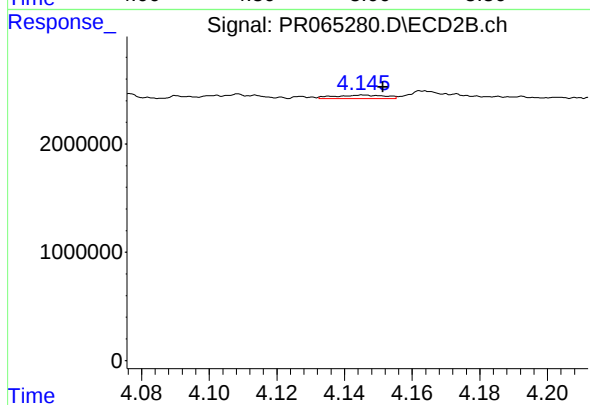

#16 AR-1242-1


R.T.: 4.146 min
Delta R.T.: -0.006 min
Response: 347782
Conc: 2.38 ng/ml

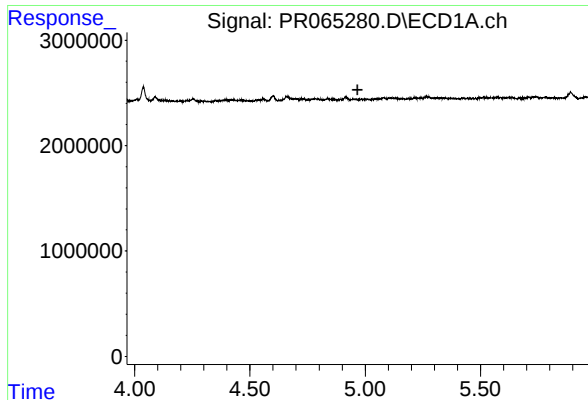

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 4.967 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

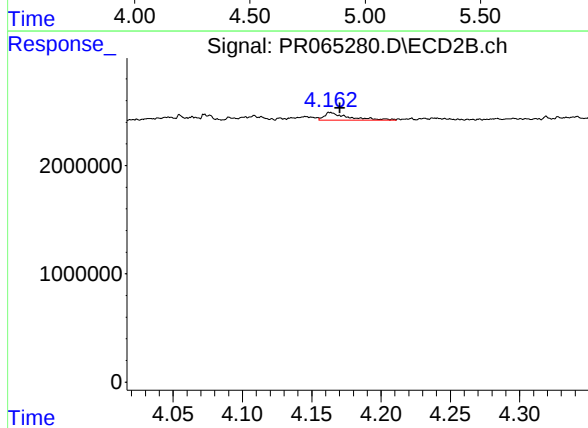


#17 AR-1242-2

R.T.: 4.164 min
Delta R.T.: -0.007 min
Response: 863920
Conc: 4.33 ng/ml

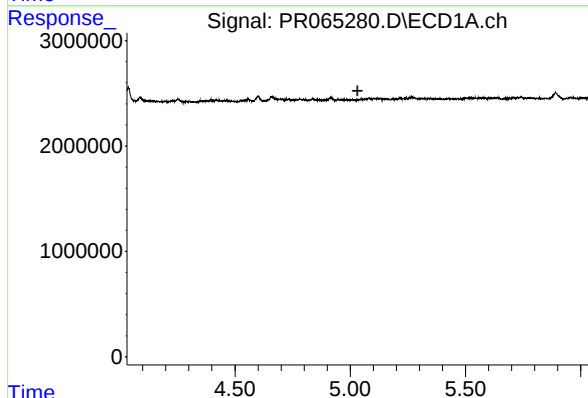


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 5.031 min
Response: 0
Conc: N.D.

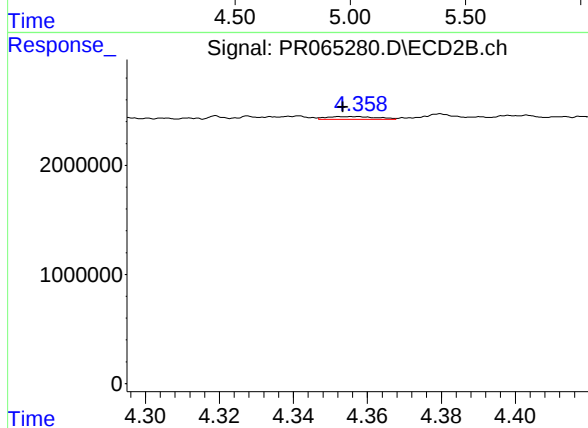

#18 AR-1242-3


R.T.: 4.357 min
Delta R.T.: 0.003 min
Response: 235620
Conc: 2.15 ng/ml

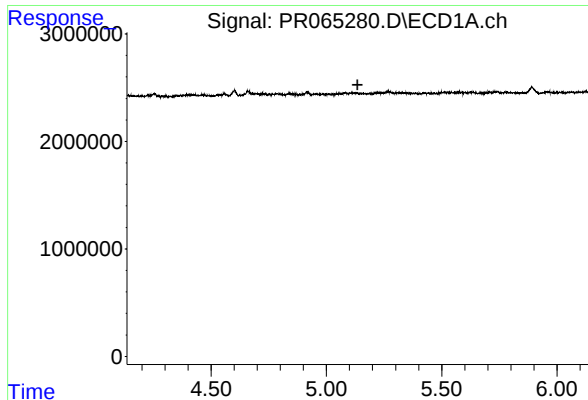

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

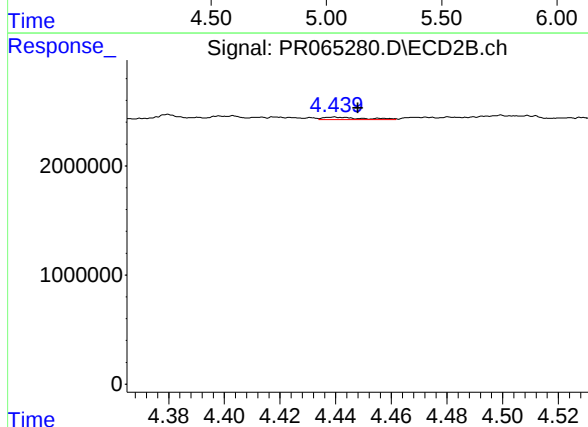


#19 AR-1242-4

R.T.: 4.439 min
Delta R.T.: -0.009 min
Response: 240795
Conc: 2.29 ng/ml

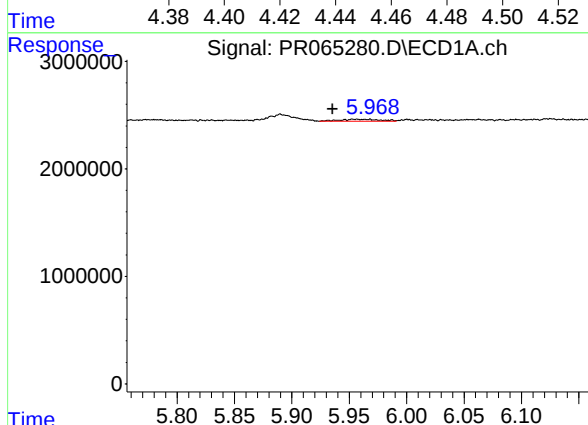


#20 AR-1242-5

R.T.: 5.957 min
Delta R.T.: 0.021 min
Response: 424884
Conc: 3.76 ng/ml

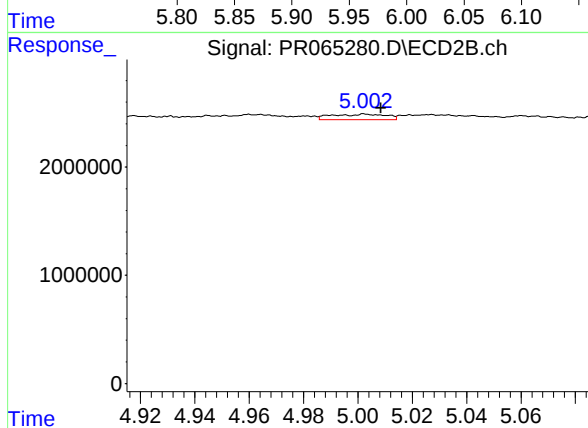

#20 AR-1242-5


R.T.: 5.003 min
Delta R.T.: -0.006 min
Response: 693918
Conc: 5.14 ng/ml

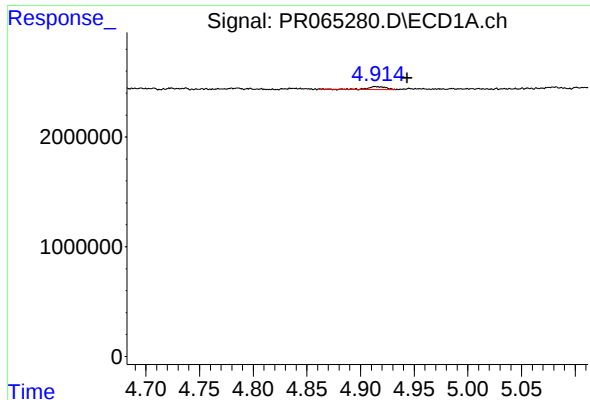

#21 AR-1248-1


R.T.: 4.914 min
Delta R.T.: -0.030 min
Response: 332646
Conc: 3.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

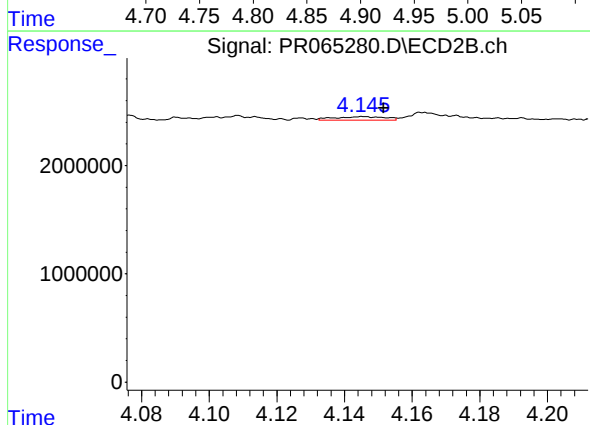


#21 AR-1248-1

R.T.: 4.146 min
Delta R.T.: -0.006 min
Response: 347782
Conc: 3.22 ng/ml

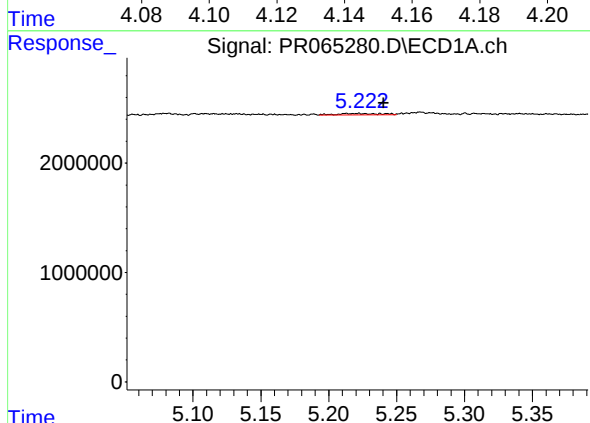


#22 AR-1248-2

R.T.: 5.238 min
Delta R.T.: -0.002 min
Response: 265187
Conc: 1.71 ng/ml

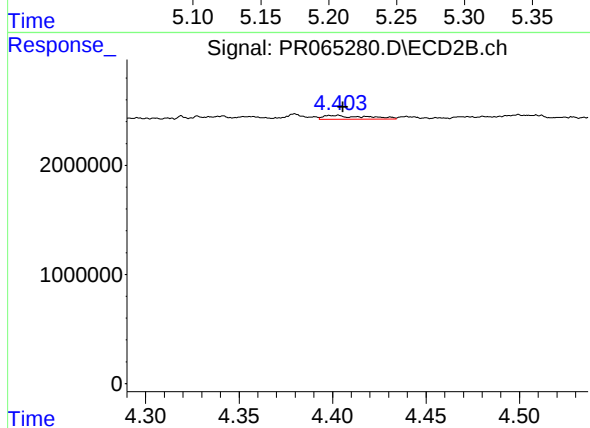

#22 AR-1248-2


R.T.: 4.402 min
Delta R.T.: -0.003 min
Response: 565563
Conc: 3.91 ng/ml

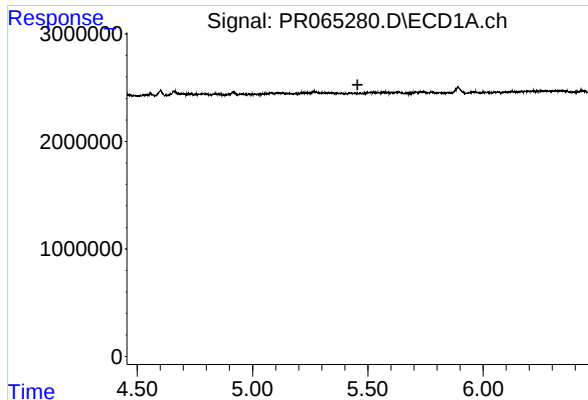

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

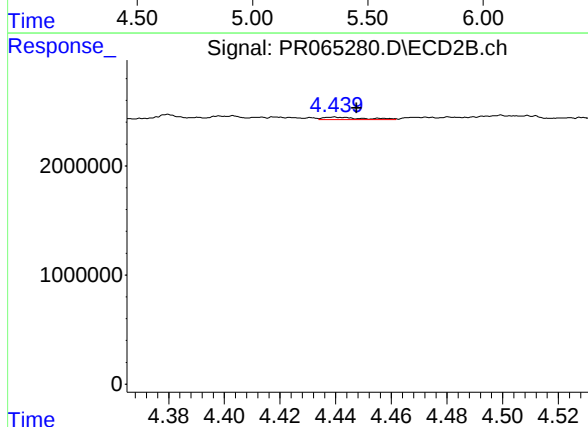


#23 AR-1248-3

R.T.: 4.439 min
Delta R.T.: -0.008 min
Response: 240795
Conc: 1.56 ng/ml

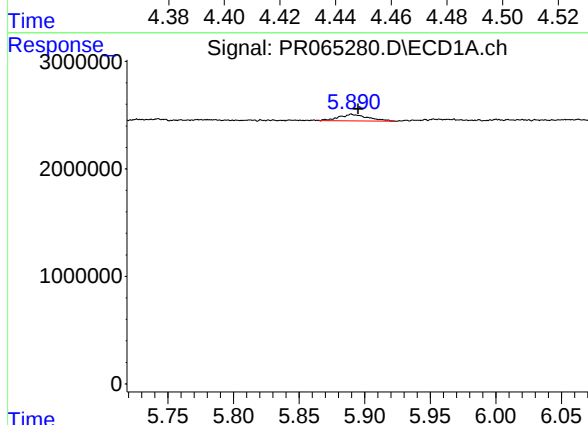


#24 AR-1248-4

R.T.: 5.890 min
Delta R.T.: -0.005 min
Response: 952413
Conc: 5.02 ng/ml

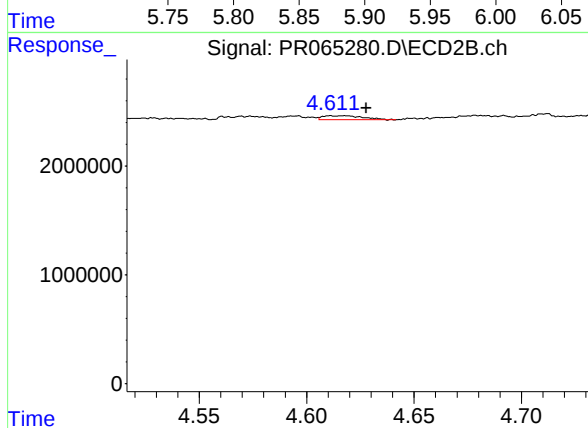

#24 AR-1248-4


R.T.: 4.611 min
Delta R.T.: -0.017 min
Response: 479434
Conc: 2.56 ng/ml

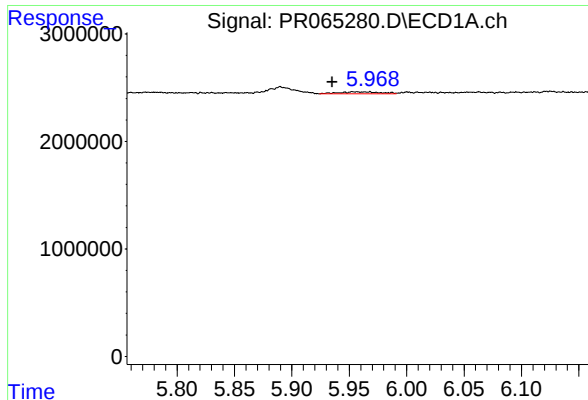

#25 AR-1248-5


R.T.: 5.957 min
Delta R.T.: 0.022 min
Response: 424884
Conc: 2.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

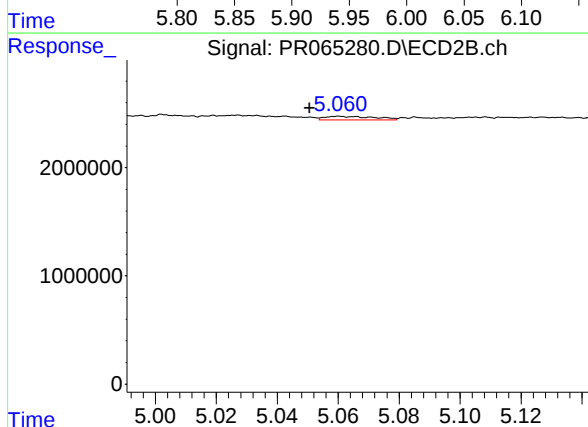


#25 AR-1248-5

R.T.: 5.060 min
Delta R.T.: 0.010 min
Response: 372517
Conc: 2.00 ng/ml

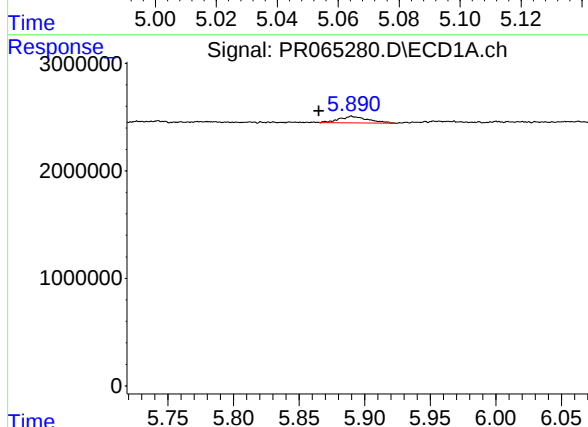


#26 AR-1254-1

R.T.: 5.890 min
Delta R.T.: 0.025 min
Response: 952413
Conc: 4.65 ng/ml

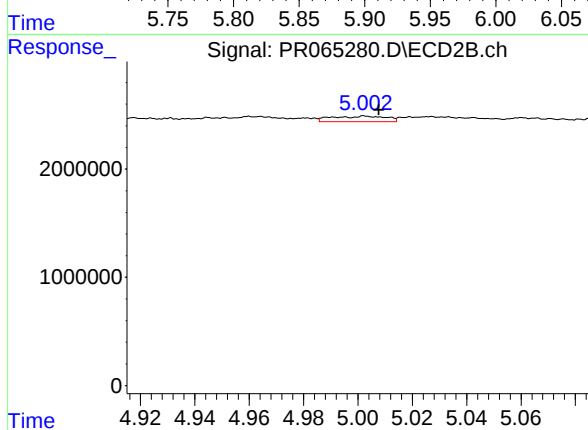

#26 AR-1254-1


R.T.: 5.003 min
Delta R.T.: -0.005 min
Response: 693918
Conc: 2.38 ng/ml

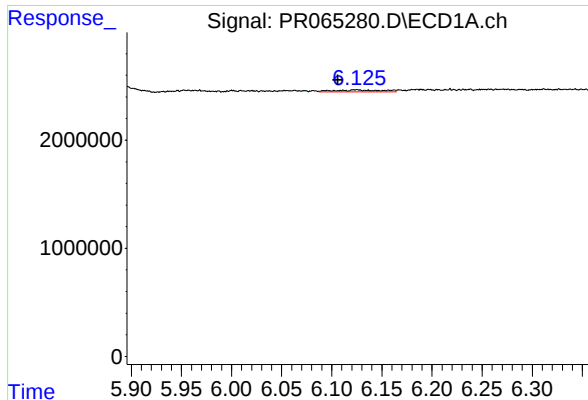

#27 AR-1254-2


R.T.: 6.125 min
Delta R.T.: 0.019 min
Response: 595801
Conc: 1.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

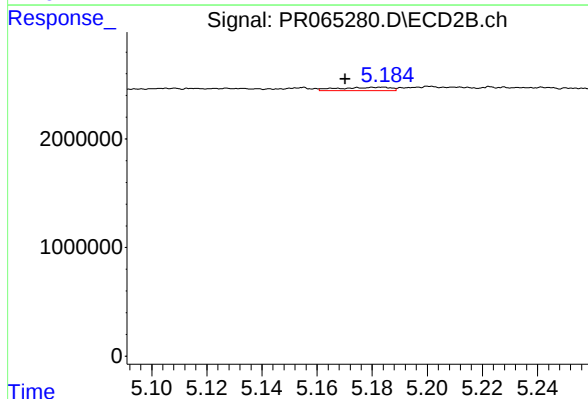


#27 AR-1254-2

R.T.: 5.183 min
Delta R.T.: 0.013 min
Response: 403772
Conc: 1.59 ng/ml

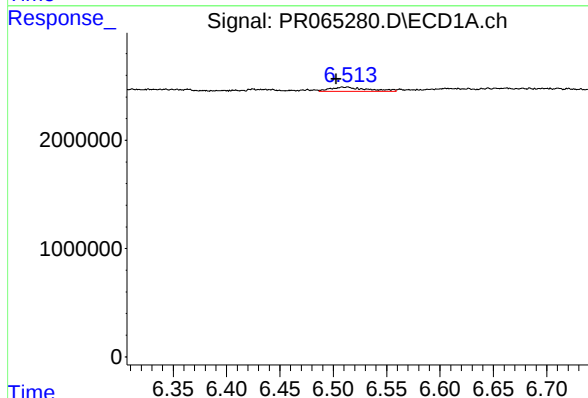


#28 AR-1254-3

R.T.: 6.514 min
Delta R.T.: 0.011 min
Response: 909516
Conc: 2.84 ng/ml

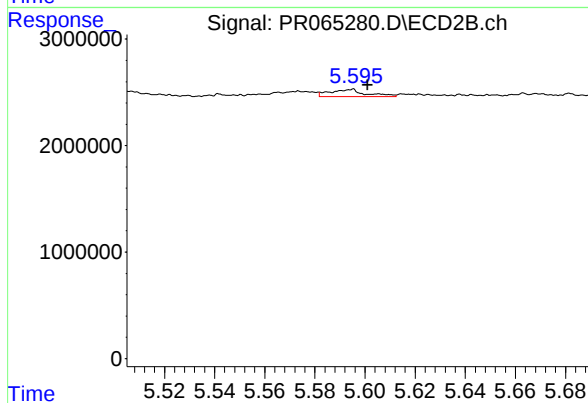

#28 AR-1254-3


R.T.: 5.594 min
Delta R.T.: -0.007 min
Response: 688777
Conc: 1.68 ng/ml

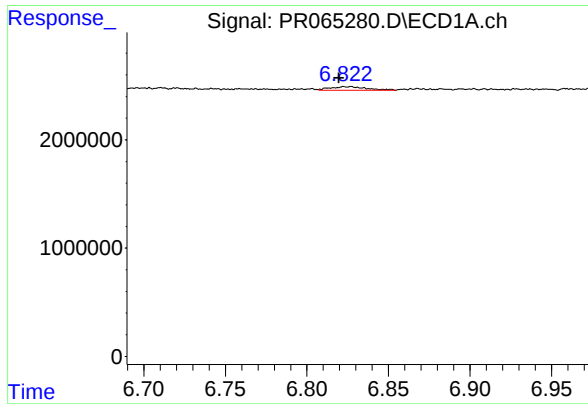

#29 AR-1254-4


R.T.: 6.827 min
Delta R.T.: 0.007 min
Response: 504522
Conc: 2.20 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

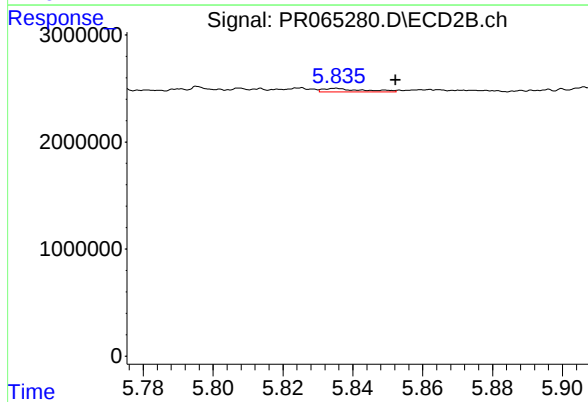


#29 AR-1254-4

R.T.: 5.835 min
Delta R.T.: -0.017 min
Response: 258212
Conc: 1.01 ng/ml

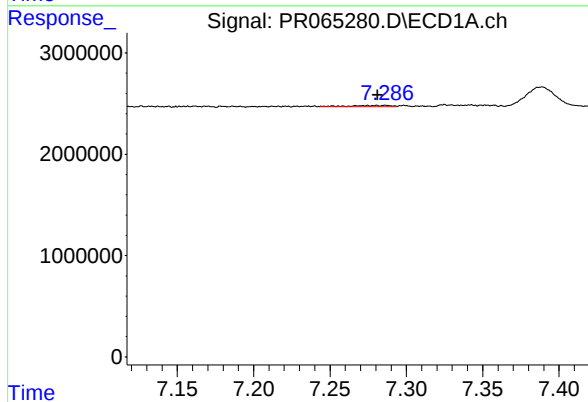


#30 AR-1254-5

R.T.: 7.286 min
Delta R.T.: 0.005 min
Response: 220235
Conc: 0.89 ng/ml

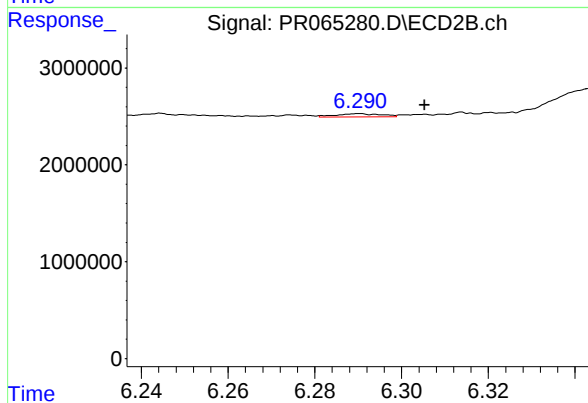

#30 AR-1254-5


R.T.: 6.290 min
Delta R.T.: -0.015 min
Response: 242425
Conc: 0.66 ng/ml

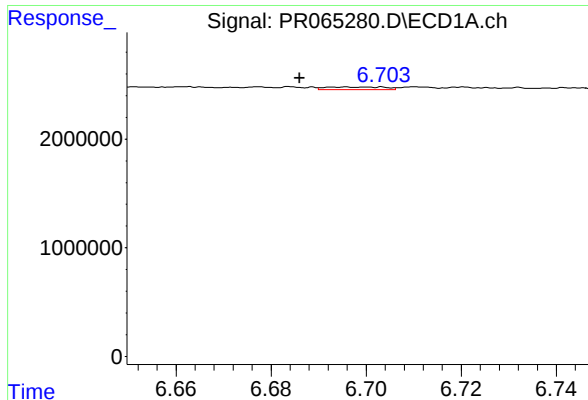

#31 AR-1260-1


R.T.: 6.696 min
Delta R.T.: 0.010 min
Response: 207588
Conc: 0.83 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

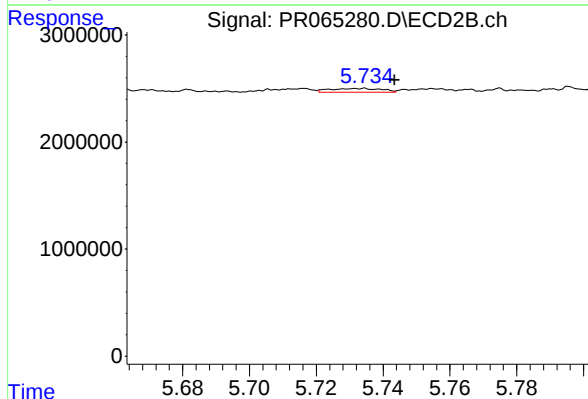


#31 AR-1260-1

R.T.: 5.733 min
Delta R.T.: -0.010 min
Response: 388620
Conc: 1.36 ng/ml

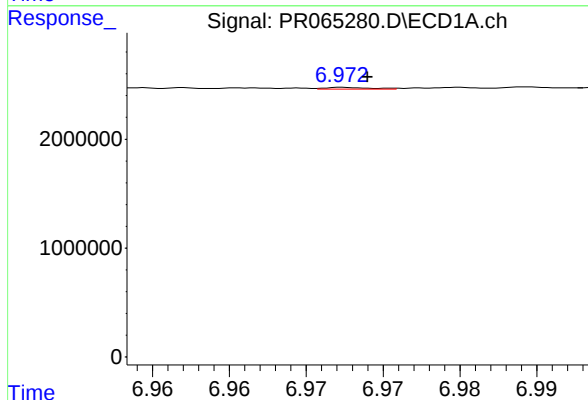


#32 AR-1260-2

R.T.: 6.973 min
Delta R.T.: -0.001 min
Response: 32957
Conc: 0.11 ng/ml

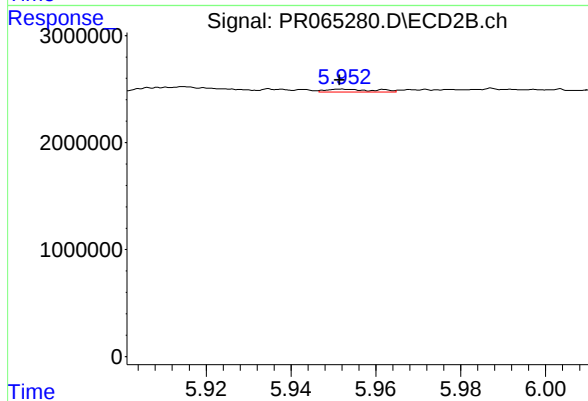

#32 AR-1260-2


R.T.: 5.952 min
Delta R.T.: 0.000 min
Response: 205005
Conc: 0.59 ng/ml

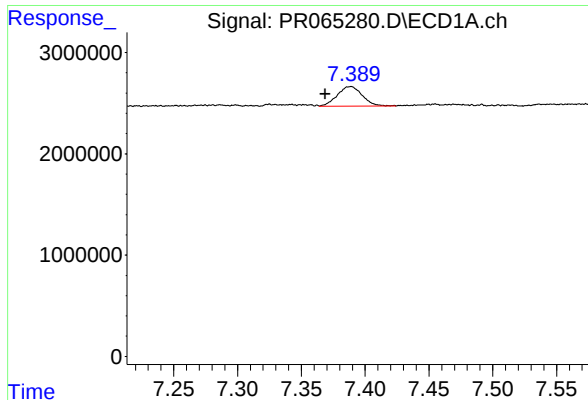

#33 AR-1260-3


R.T.: 7.388 min
Delta R.T.: 0.020 min
Response: 2644583
Conc: 12.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

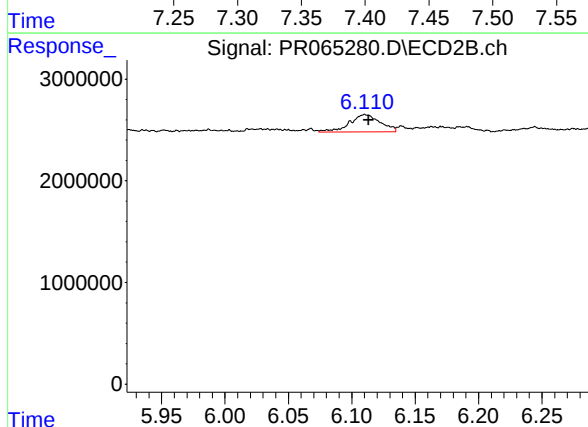


#33 AR-1260-3

R.T.: 6.110 min
Delta R.T.: -0.003 min
Response: 2923386
Conc: 9.00 ng/ml

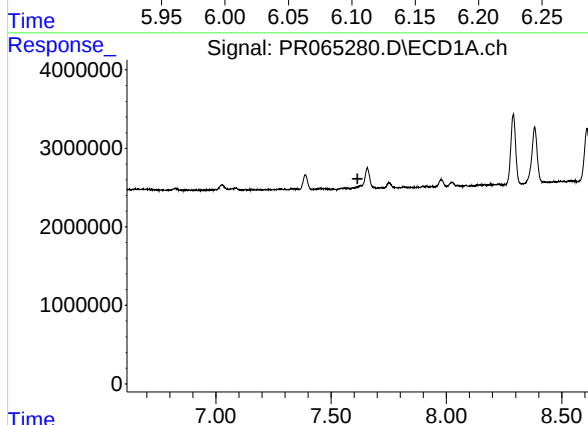


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.615 min
Response: 0
Conc: N.D.

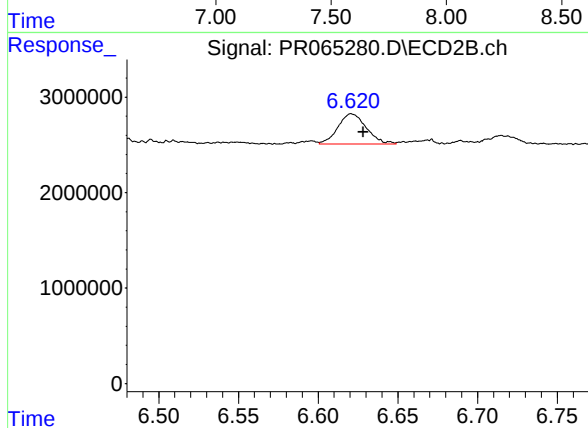

#34 AR-1260-4


R.T.: 6.621 min
Delta R.T.: -0.007 min
Response: 3937828
Conc: 14.91 ng/ml

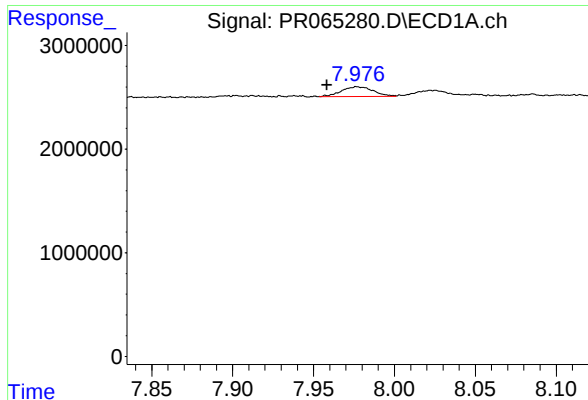

#35 AR-1260-5


R.T.: 7.977 min
Delta R.T.: 0.019 min
Response: 1295369
Conc: 2.95 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

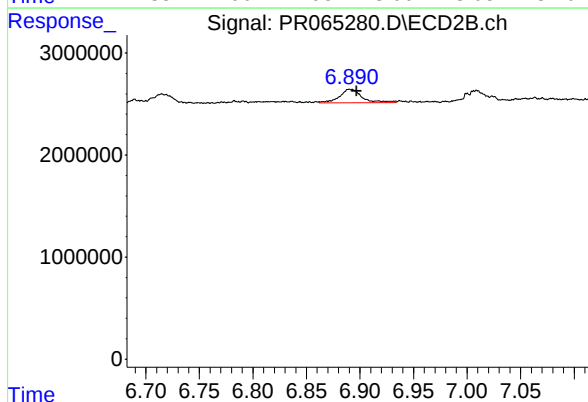


#35 AR-1260-5

R.T.: 6.891 min
Delta R.T.: -0.006 min
Response: 1911766
Conc: 3.10 ng/ml

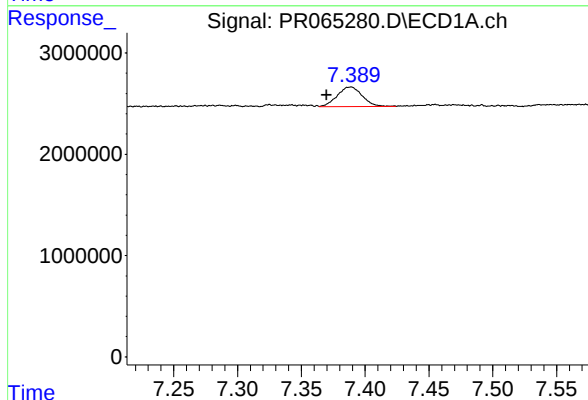


#36 AR-1262-1

R.T.: 7.388 min
Delta R.T.: 0.019 min
Response: 2644583
Conc: 7.81 ng/ml

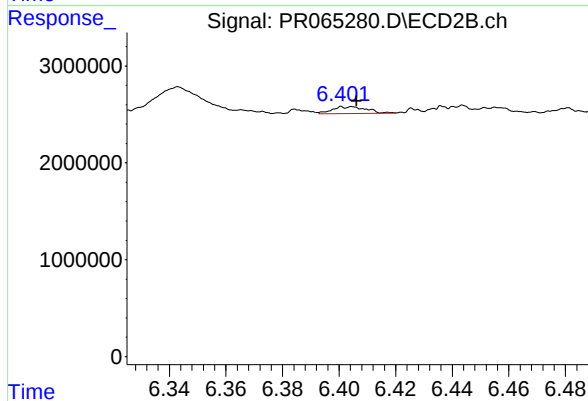

#36 AR-1262-1


R.T.: 6.404 min
Delta R.T.: -0.002 min
Response: 597665
Conc: 3.33 ng/ml

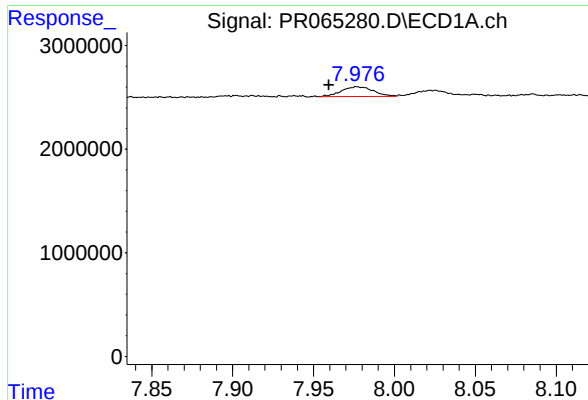

#37 AR-1262-2


R.T.: 7.977 min
Delta R.T.: 0.017 min
Response: 1295369
Conc: 2.29 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

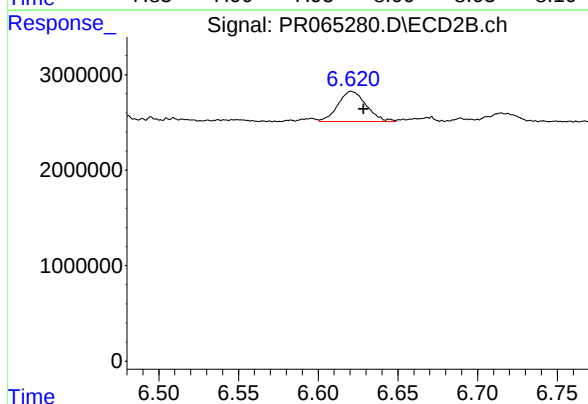


#37 AR-1262-2

R.T.: 6.621 min
Delta R.T.: -0.007 min
Response: 3937828
Conc: 10.12 ng/ml

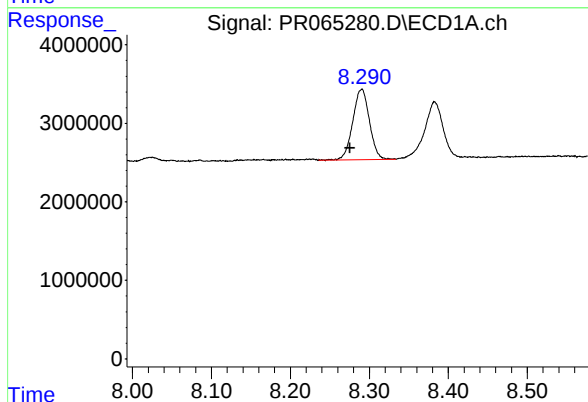


#38 AR-1262-3

R.T.: 8.290 min
Delta R.T.: 0.014 min
Response: 13178037
Conc: 34.63 ng/ml

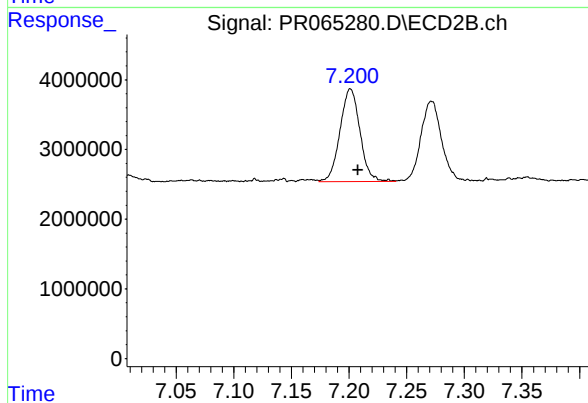

#38 AR-1262-3


R.T.: 7.201 min
Delta R.T.: -0.007 min
Response: 15998579
Conc: 56.44 ng/ml

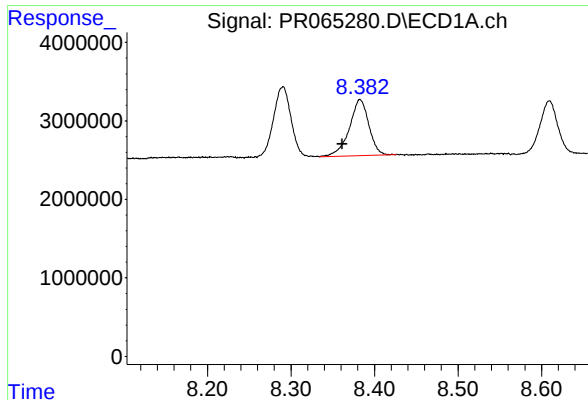

#39 AR-1262-4


R.T.: 8.383 min
Delta R.T.: 0.021 min
Response: 11607954
Conc: 39.63 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

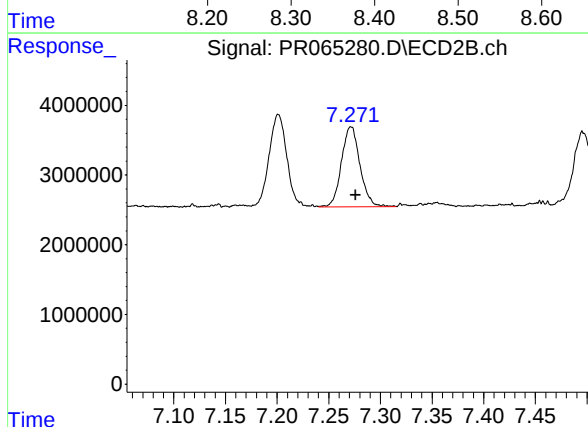


#39 AR-1262-4

R.T.: 7.272 min
Delta R.T.: -0.004 min
Response: 14331662
Conc: 24.89 ng/ml

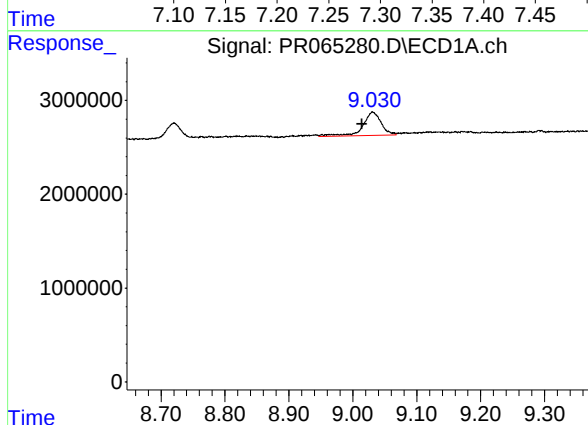


#40 AR-1262-5

R.T.: 9.031 min
Delta R.T.: 0.017 min
Response: 4956406
Conc: 24.73 ng/ml

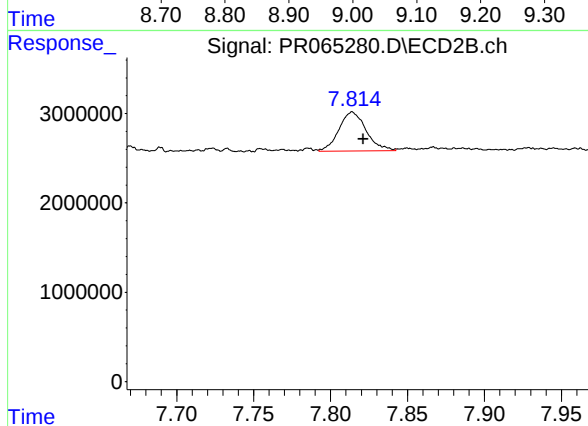

#40 AR-1262-5


R.T.: 7.814 min
Delta R.T.: -0.007 min
Response: 5386964
Conc: 20.70 ng/ml

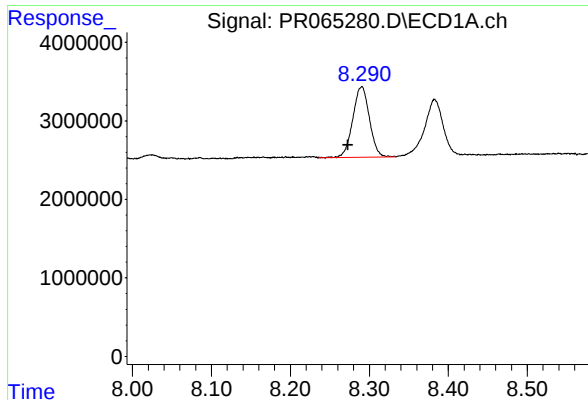

#41 AR-1268-1


R.T.: 8.290 min
Delta R.T.: 0.018 min
Response: 13178037
Conc: 21.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

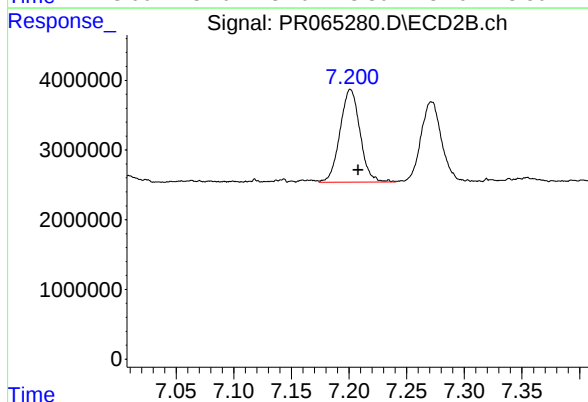


#41 AR-1268-1

R.T.: 7.201 min
Delta R.T.: -0.007 min
Response: 15998579
Conc: 20.17 ng/ml

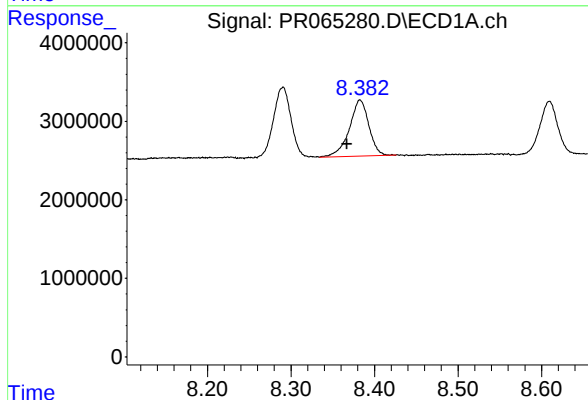


#42 AR-1268-2

R.T.: 8.383 min
Delta R.T.: 0.016 min
Response: 11607954
Conc: 21.21 ng/ml

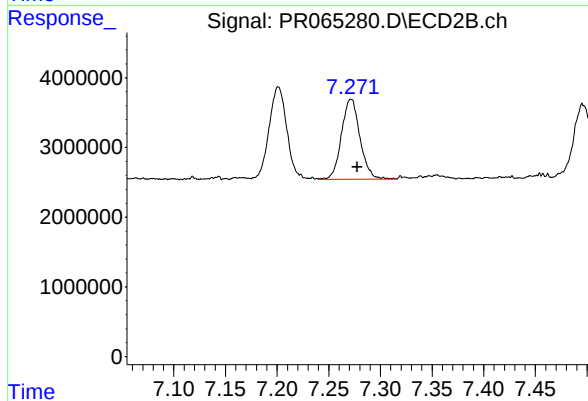

#42 AR-1268-2


R.T.: 7.272 min
Delta R.T.: -0.006 min
Response: 14331662
Conc: 19.25 ng/ml

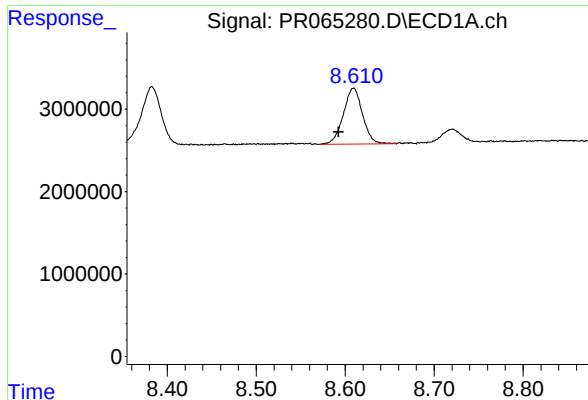

#43 AR-1268-3


R.T.: 8.609 min
Delta R.T.: 0.017 min
Response: 10129147
Conc: 21.35 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

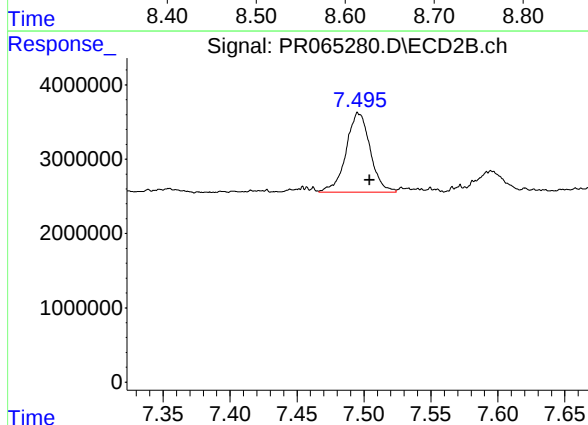


#43 AR-1268-3

R.T.: 7.496 min
Delta R.T.: -0.008 min
Response: 13371488
Conc: 21.11 ng/ml

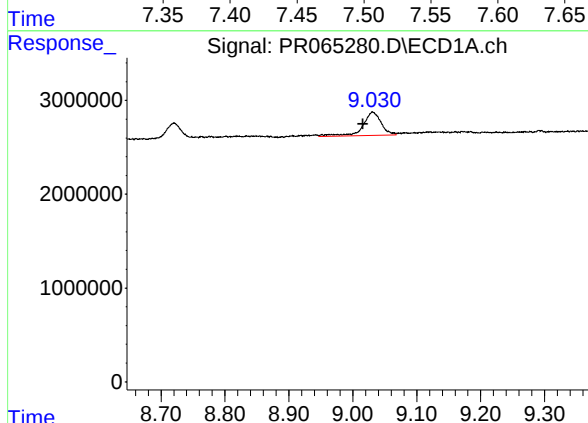


#44 AR-1268-4

R.T.: 9.031 min
Delta R.T.: 0.016 min
Response: 4956406
Conc: 24.36 ng/ml

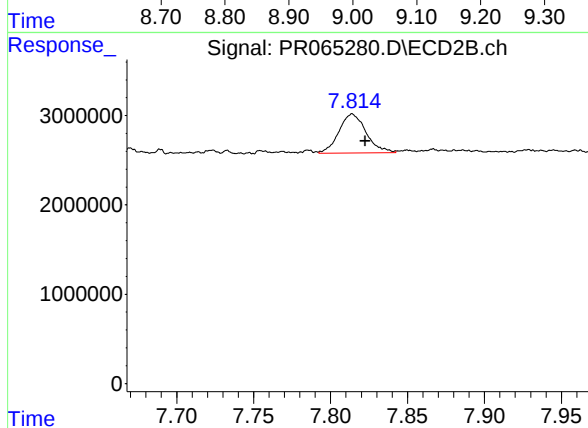

#44 AR-1268-4


R.T.: 7.814 min
Delta R.T.: -0.009 min
Response: 5386964
Conc: 20.54 ng/ml

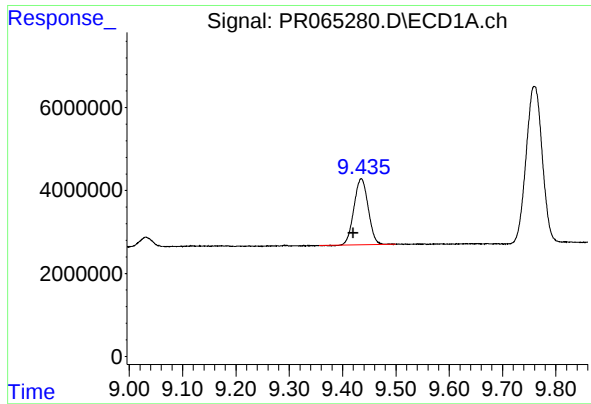

#45 AR-1268-5

R.T.: 9.435 min
Delta R.T.: 0.015 min
Response: 29466034
Conc: 20.21 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

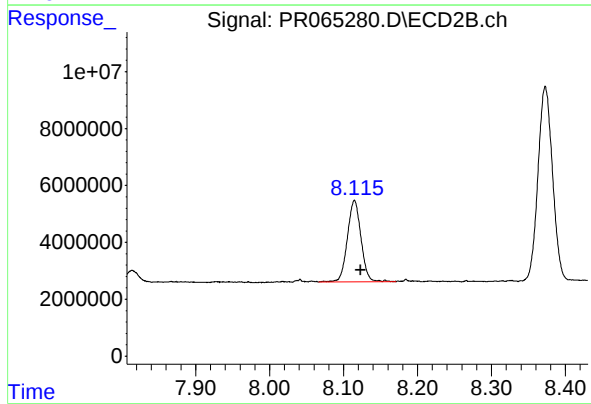

#45 AR-1268-5

R.T.: 8.115 min
Delta R.T.: -0.008 min
Response: 36931649
Conc: 19.29 ng/ml