

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
 Data File : PR065289.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 21:49
 Operator : AJ\MA
 Sample : P1187-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:38:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.700	3.003	129.5E6	122.2E6	21.697	22.345
2) SA Decachlor...	9.738	8.373	91885967	107.2E6	22.974	22.658
Target Compounds						
3) L1 AR-1016-1	4.943	4.146	412323	446421	2.326	2.458
4) L1 AR-1016-2	4.961	4.164	499502	558444	1.916	2.259
5) L1 AR-1016-3	5.034	4.355	358637	527675	2.146	3.892 #
6) L1 AR-1016-4	5.135	4.409	260395	669228	1.942	6.390 #
7) L1 AR-1016-5	5.454	4.624	174246	619938	1.290	4.444 #
8) L2 AR-1221-1	3.911f	3.239	2485105	188798	34.625	3.049 #
9) L2 AR-1221-2	4.016	3.314	1828074	1755832	34.871	36.814
10) L2 AR-1221-3	4.096	3.400	116076	708861	0.756	5.132 #
11) L3 AR-1232-1	4.096	3.400	116076	708861	0.859	5.919 #
12) L3 AR-1232-2	4.639	4.164	1527487	558444	19.827	4.571 #
13) L3 AR-1232-3	4.961	4.355	499502	527675	3.917	7.933 #
14) L3 AR-1232-4	5.135	4.433	260395	713501	3.973	12.461 #
15) L3 AR-1232-5	5.240	4.624	702958	619938	14.534	9.726 #
16) L4 AR-1242-1	4.943	4.146	412323	446421	2.884	3.055
17) L4 AR-1242-2	4.961	4.164	499502	558444	2.372	2.800
18) L4 AR-1242-3	5.034	4.355	358637	527675	2.648	4.819 #
19) L4 AR-1242-4	5.135	4.433f	260395	713501	2.396	6.796 #
20) L4 AR-1242-5	5.926	5.003	551810	2233652	4.878	16.543 #
21) L5 AR-1248-1	4.943	4.146	412323	446421	3.875	4.133
22) L5 AR-1248-2	5.240	4.409	702958	669228	4.524	4.621
23) L5 AR-1248-3	5.454	4.433	174246	713501	0.976	4.611 #
24) L5 AR-1248-4	5.865f	4.624	2851493	619938	15.041	3.310 #
25) L5 AR-1248-5	5.926	5.063	551810	301829	2.896	1.622 #
26) L6 AR-1254-1	5.865	5.003	2851493	2233652	13.922	7.666 #
27) L6 AR-1254-2	6.104	5.164	2340275	2993209	7.509	11.816 #
28) L6 AR-1254-3	6.501	5.615	1564824	7110768	4.891	17.379 #
29) L6 AR-1254-4	6.806	5.848	1297719	1386833	5.663	5.402
30) L6 AR-1254-5	7.275	6.298	9307734	8248196	37.451	22.501 #
31) L7 AR-1260-1	6.683	5.738	9849851	10165849	39.183	35.614
32) L7 AR-1260-2	6.971	5.946	10411611	11649861	36.228	33.595
33) L7 AR-1260-3	7.367	6.110	14347092	13372621	67.861	41.161 #
34) L7 AR-1260-4	7.611	6.622	13486781	14062299	57.154	53.228
35) L7 AR-1260-5	7.955	6.891	21630091	26720919	49.195	43.327
36) L8 AR-1262-1	7.367	6.400	14347092	6439839	42.385	35.902
37) L8 AR-1262-2	7.955	6.622	21630091	14062299	38.240	36.141
38) L8 AR-1262-3	8.271	7.201	14944284	10874318	39.273	38.365
39) L8 AR-1262-4	8.360	7.269	11338013	20282317	38.706	35.219
40) L8 AR-1262-5	9.009	7.814	8632578	10448812	43.078	40.146
41) L9 AR-1268-1	8.271	7.201	14944284	10874318	24.650	13.707 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
 Data File : PR065289.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 21:49
 Operator : AJ\MA
 Sample : P1187-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:38:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.360	7.269	11338013	20282317	20.721	27.244 #
43) L9	AR-1268-3	8.585	7.495	994074	2920884	2.095	4.611 #
44) L9	AR-1268-4	9.009	7.814	8632578	10448812	42.424	39.834
45) L9	AR-1268-5	9.411	8.114	3225477	4192120	2.213	2.190



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
Data File : PR065289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 21:49
Operator : AJ\MA
Sample : P1187-07
Misc : AR1262 LOD 40 PPB
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:38:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

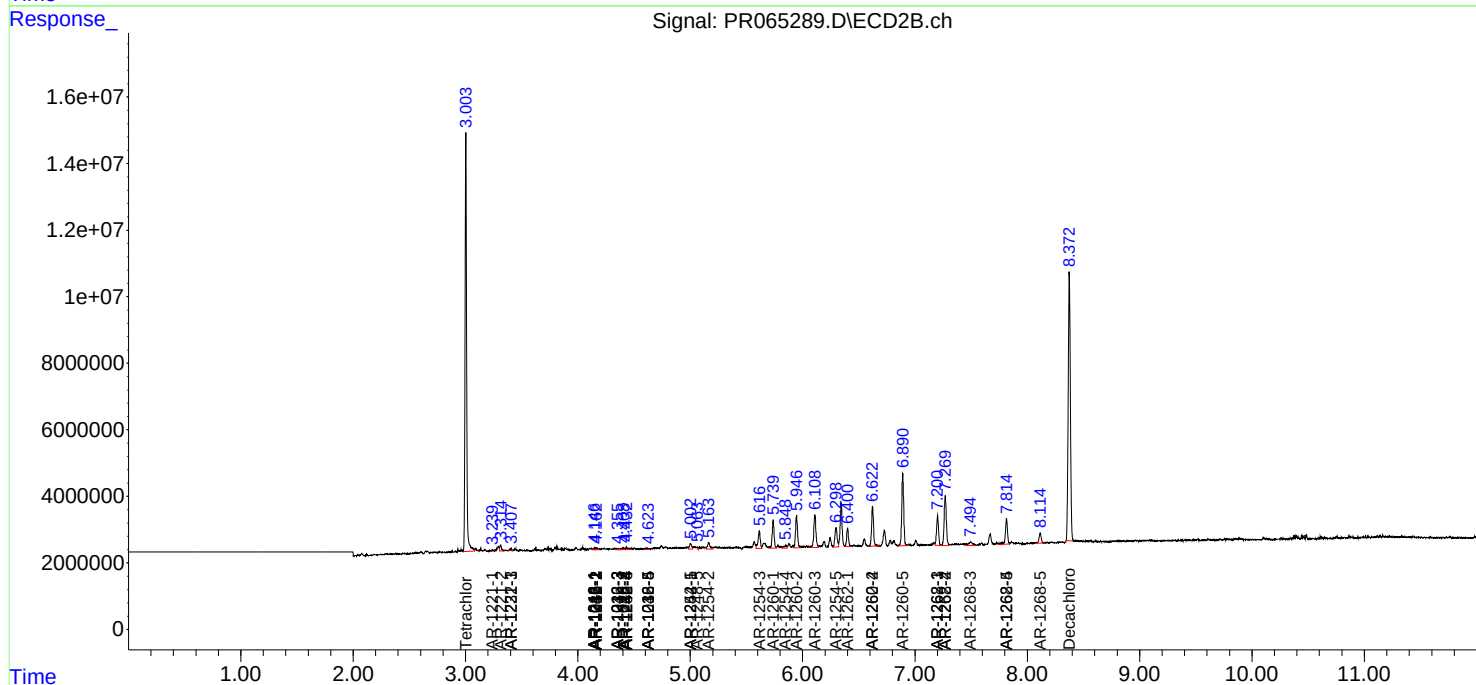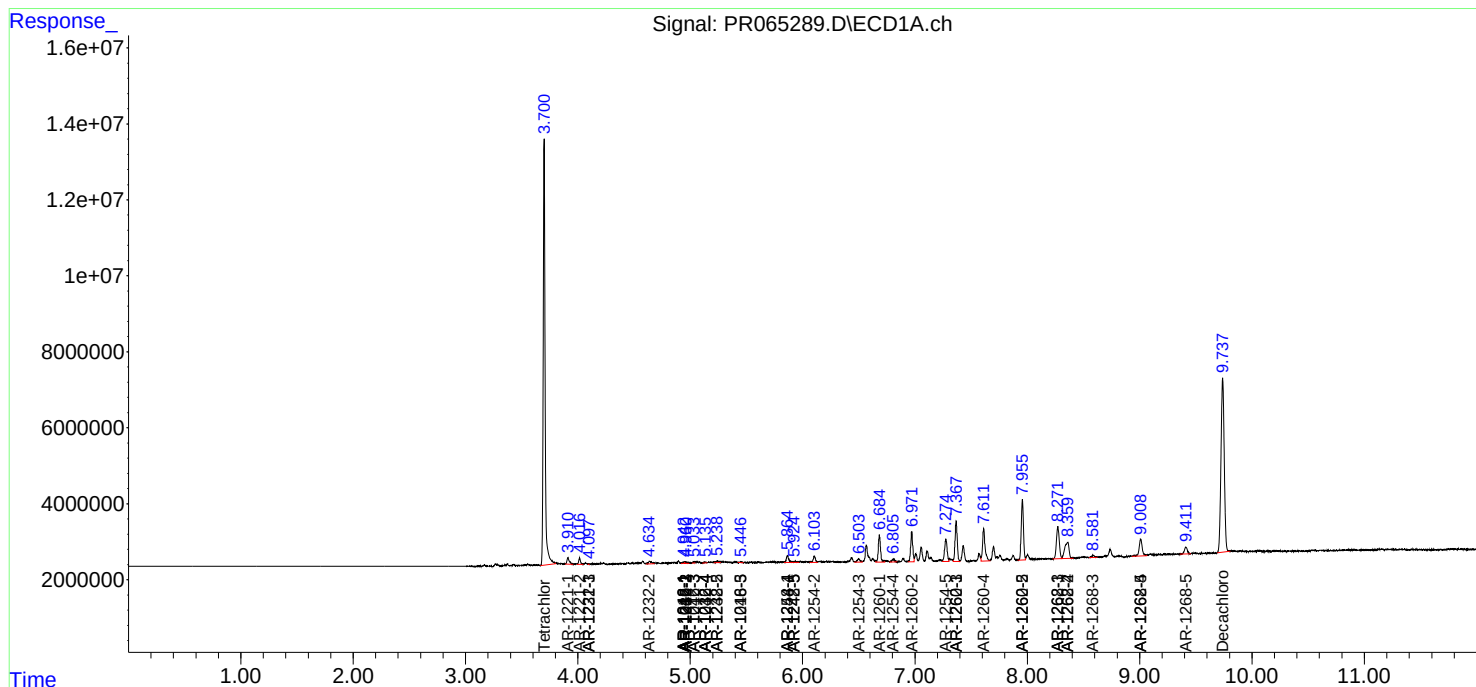


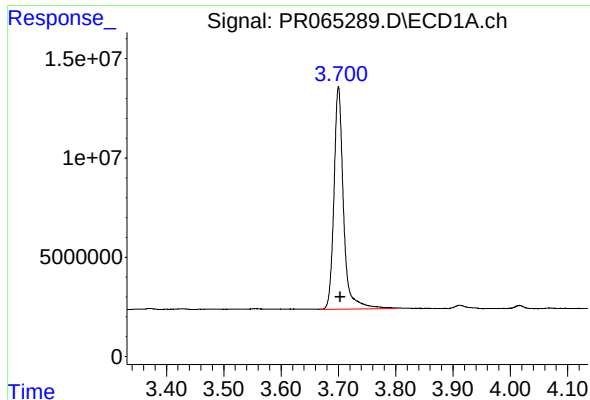

#1 Tetrachloro-m-xylene


R.T.: 3.700 min
Delta R.T.: -0.003 min
Response: 129514622
Conc: 21.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

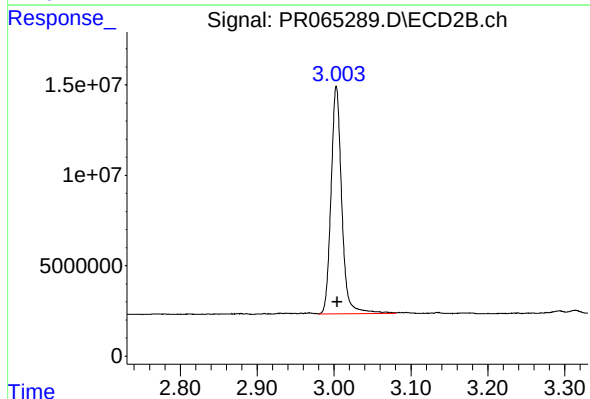


#1 Tetrachloro-m-xylene

R.T.: 3.003 min
Delta R.T.: -0.001 min
Response: 122223806
Conc: 22.35 ng/ml

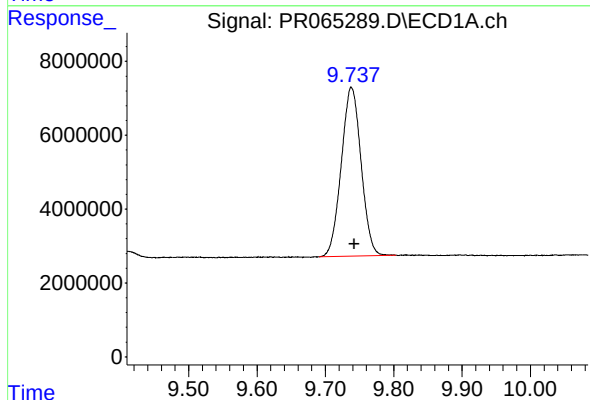


#2 Decachlorobiphenyl

R.T.: 9.738 min
Delta R.T.: -0.004 min
Response: 91885967
Conc: 22.97 ng/ml

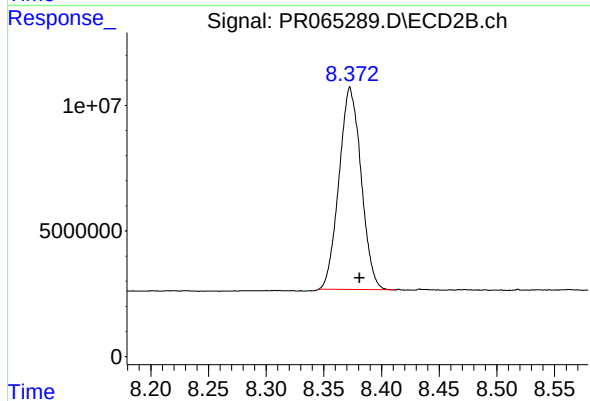

#2 Decachlorobiphenyl


R.T.: 8.373 min
Delta R.T.: -0.008 min
Response: 107232693
Conc: 22.66 ng/ml

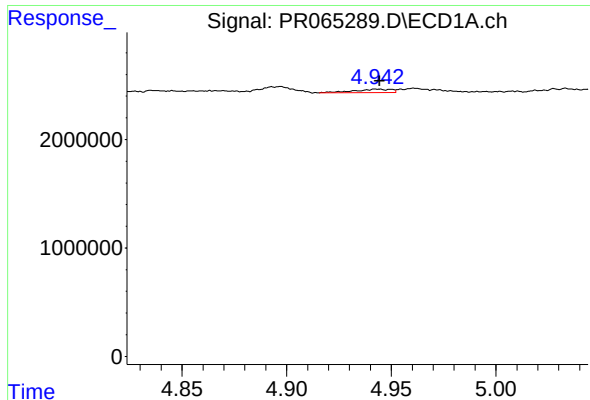

#3 AR-1016-1


R.T.: 4.943 min
Delta R.T.: -0.001 min
Response: 412323
Conc: 2.33 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

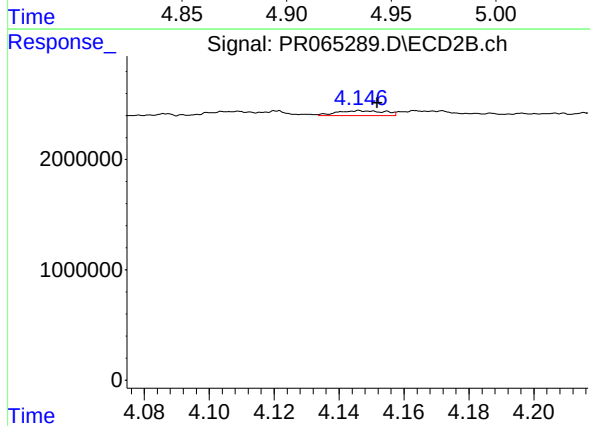


#3 AR-1016-1

R.T.: 4.146 min
Delta R.T.: -0.005 min
Response: 446421
Conc: 2.46 ng/ml

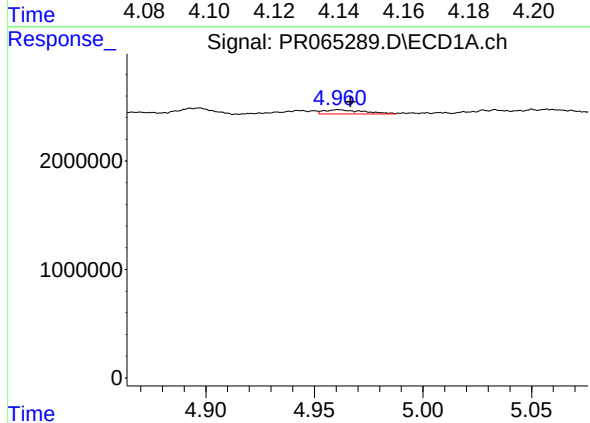


#4 AR-1016-2

R.T.: 4.961 min
Delta R.T.: -0.006 min
Response: 499502
Conc: 1.92 ng/ml

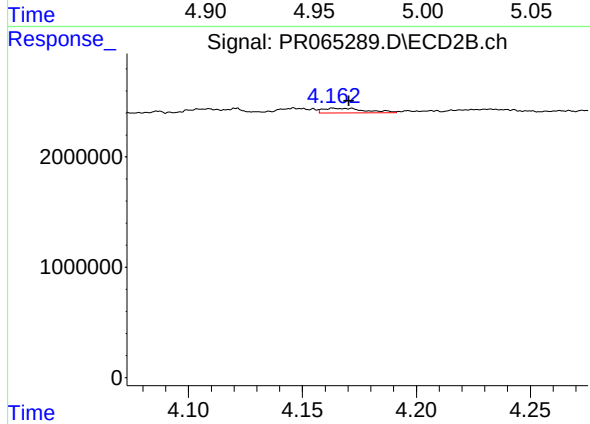

#4 AR-1016-2


R.T.: 4.164 min
Delta R.T.: -0.006 min
Response: 558444
Conc: 2.26 ng/ml

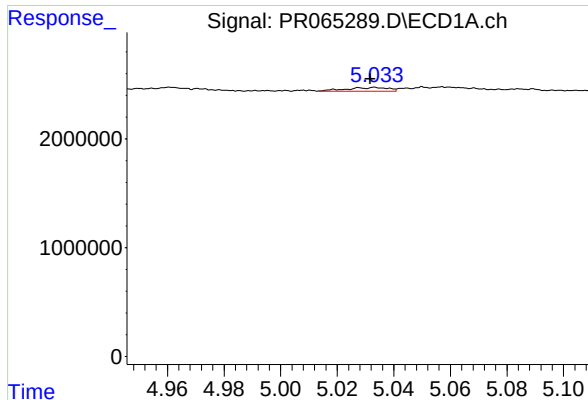

#5 AR-1016-3


R.T.: 5.034 min
Delta R.T.: 0.002 min
Response: 358637
Conc: 2.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

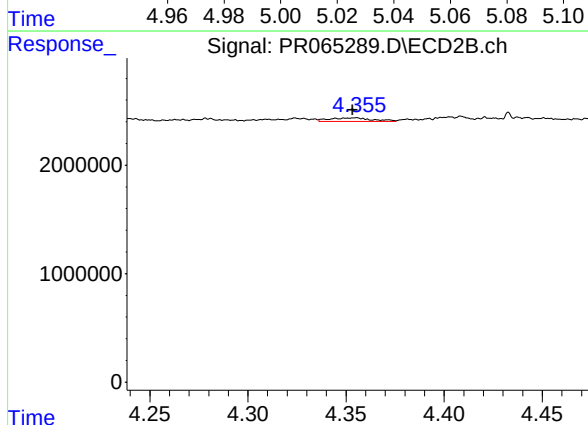


#5 AR-1016-3

R.T.: 4.355 min
Delta R.T.: 0.001 min
Response: 527675
Conc: 3.89 ng/ml

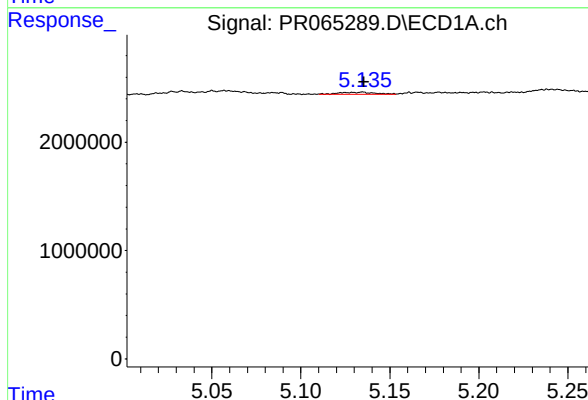


#6 AR-1016-4

R.T.: 5.135 min
Delta R.T.: 0.000 min
Response: 260395
Conc: 1.94 ng/ml

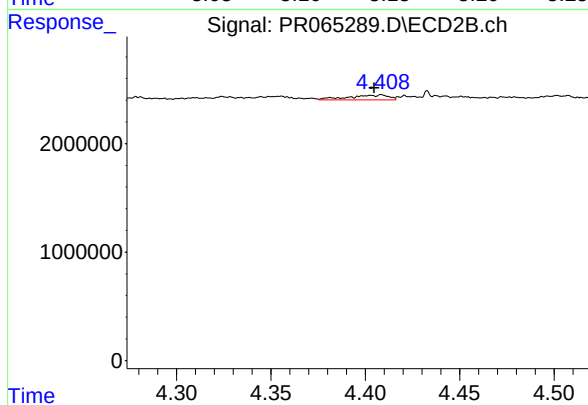

#6 AR-1016-4


R.T.: 4.409 min
Delta R.T.: 0.004 min
Response: 669228
Conc: 6.39 ng/ml

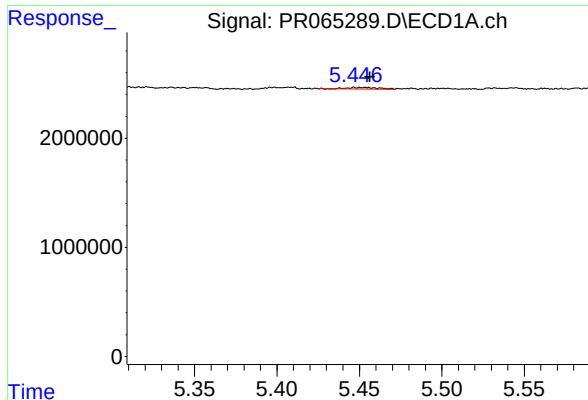

#7 AR-1016-5


R.T.: 5.454 min
Delta R.T.: -0.003 min
Response: 174246
Conc: 1.29 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

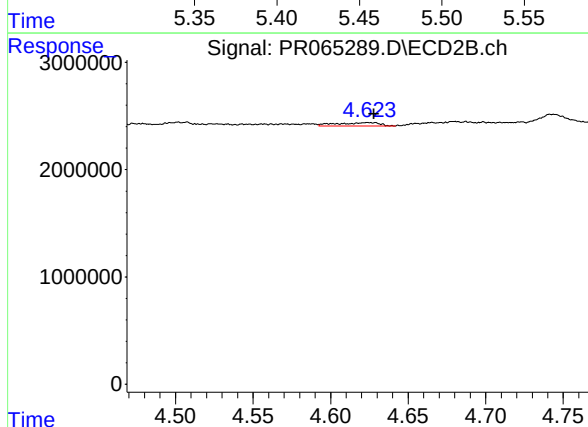


#7 AR-1016-5

R.T.: 4.624 min
Delta R.T.: -0.004 min
Response: 619938
Conc: 4.44 ng/ml

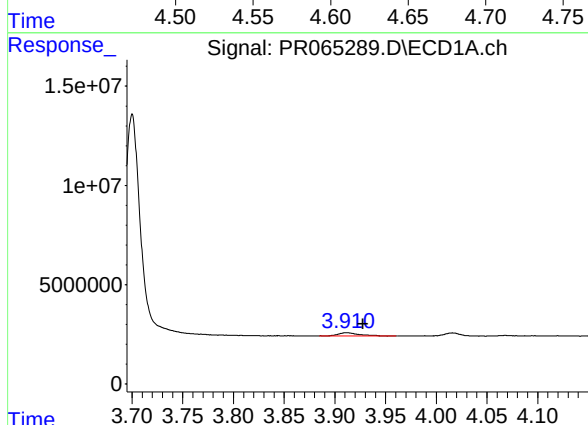


#8 AR-1221-1

R.T.: 3.911 min
Delta R.T.: -0.016 min
Response: 2485105
Conc: 34.62 ng/ml

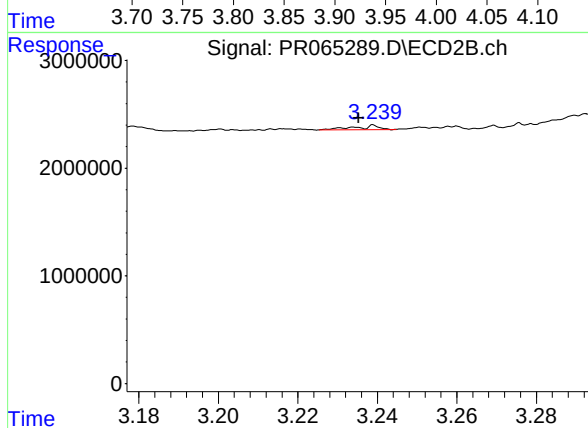

#8 AR-1221-1


R.T.: 3.239 min
Delta R.T.: 0.004 min
Response: 188798
Conc: 3.05 ng/ml

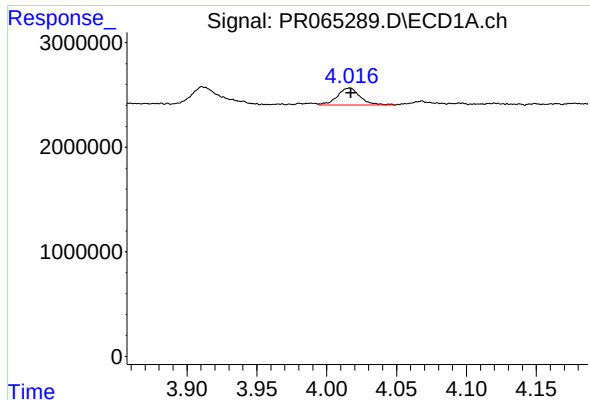

#9 AR-1221-2


R.T.: 4.016 min
Delta R.T.: -0.001 min
Response: 1828074
Conc: 34.87 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

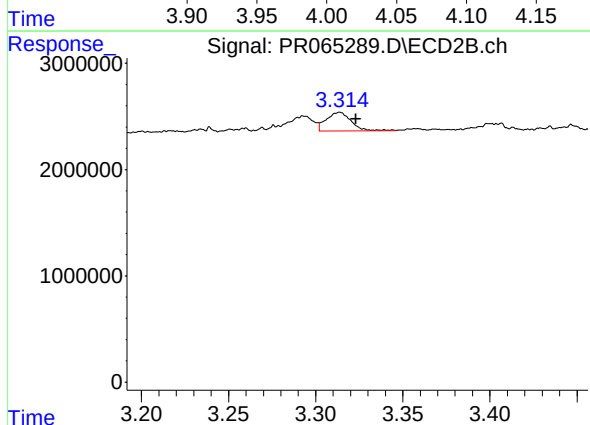


#9 AR-1221-2

R.T.: 3.314 min
Delta R.T.: -0.010 min
Response: 1755832
Conc: 36.81 ng/ml

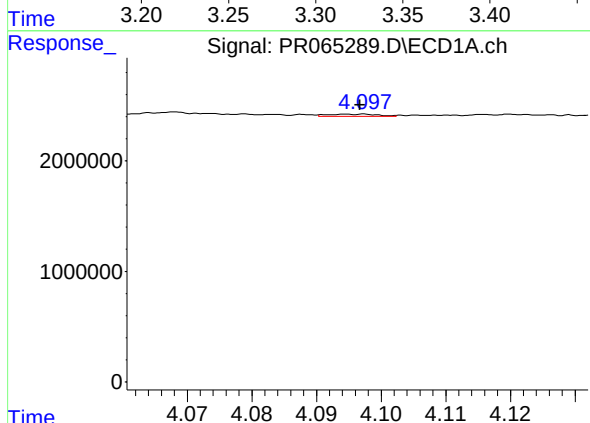


#10 AR-1221-3

R.T.: 4.096 min
Delta R.T.: -0.001 min
Response: 116076
Conc: 0.76 ng/ml

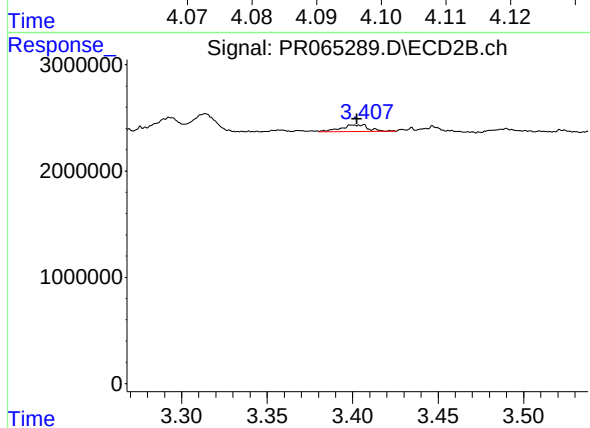

#10 AR-1221-3


R.T.: 3.400 min
Delta R.T.: -0.002 min
Response: 708861
Conc: 5.13 ng/ml

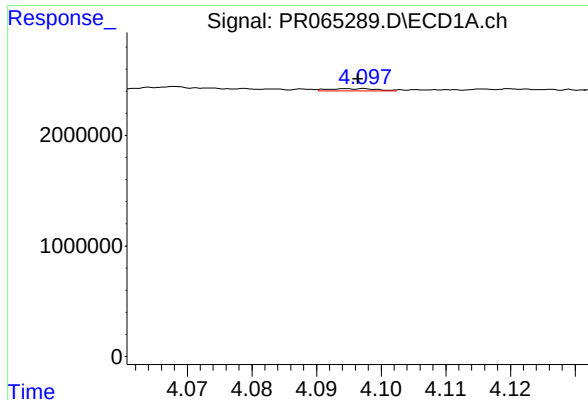

#11 AR-1232-1


R.T.: 4.096 min
Delta R.T.: 0.000 min
Response: 116076
Conc: 0.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

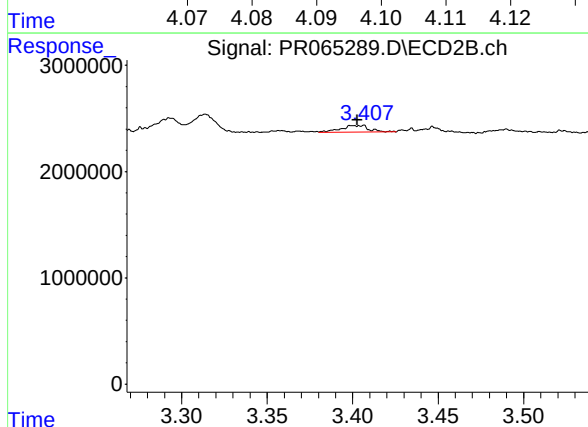


#11 AR-1232-1

R.T.: 3.400 min
Delta R.T.: -0.002 min
Response: 708861
Conc: 5.92 ng/ml

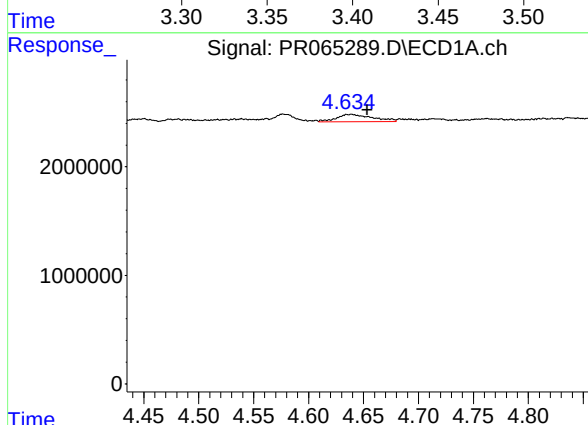


#12 AR-1232-2

R.T.: 4.639 min
Delta R.T.: -0.014 min
Response: 1527487
Conc: 19.83 ng/ml

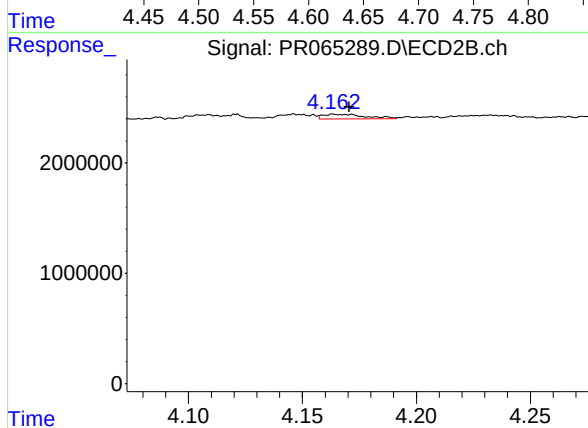

#12 AR-1232-2


R.T.: 4.164 min
Delta R.T.: -0.006 min
Response: 558444
Conc: 4.57 ng/ml

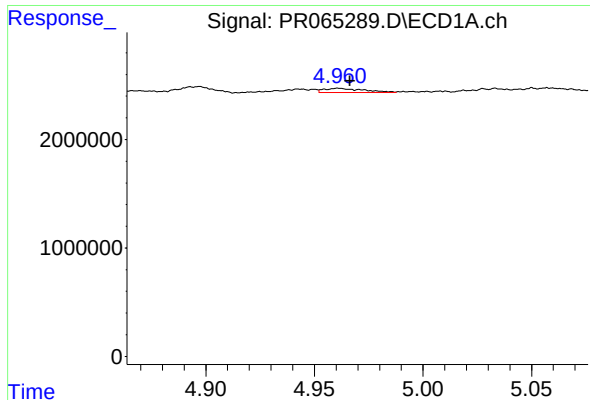

#13 AR-1232-3


R.T.: 4.961 min
Delta R.T.: -0.005 min
Response: 499502
Conc: 3.92 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

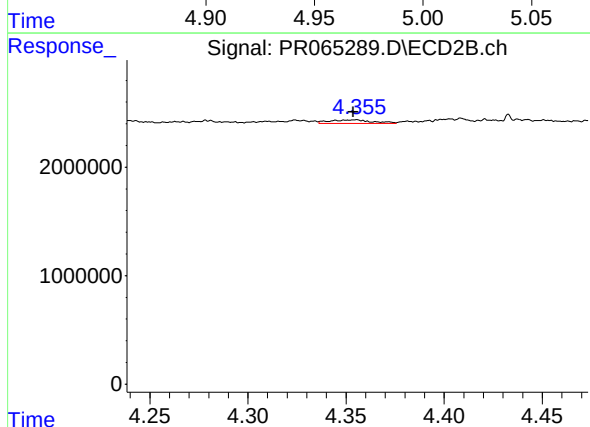


#13 AR-1232-3

R.T.: 4.355 min
Delta R.T.: 0.000 min
Response: 527675
Conc: 7.93 ng/ml

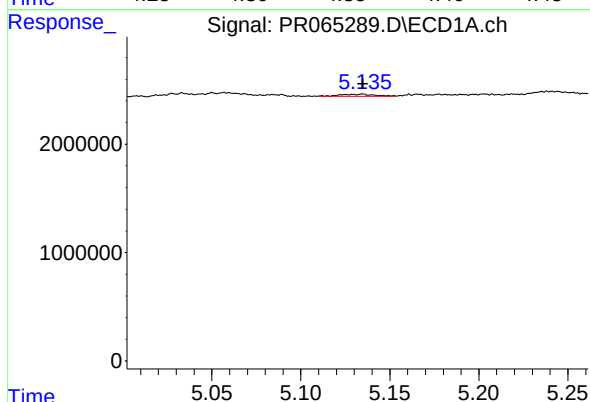


#14 AR-1232-4

R.T.: 5.135 min
Delta R.T.: 0.000 min
Response: 260395
Conc: 3.97 ng/ml

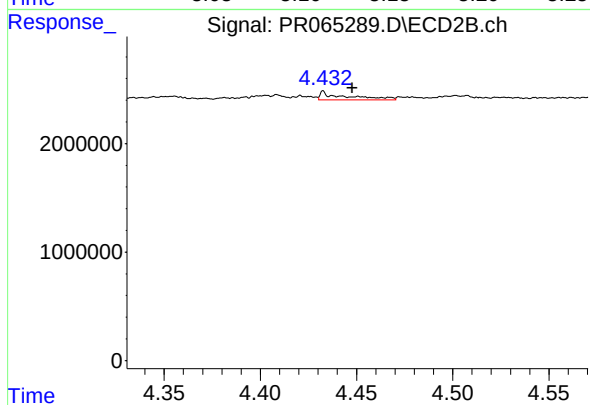

#14 AR-1232-4


R.T.: 4.433 min
Delta R.T.: -0.015 min
Response: 713501
Conc: 12.46 ng/ml

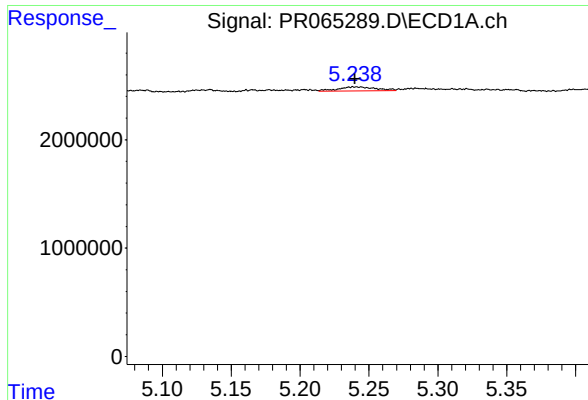

#15 AR-1232-5


R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 702958
Conc: 14.53 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

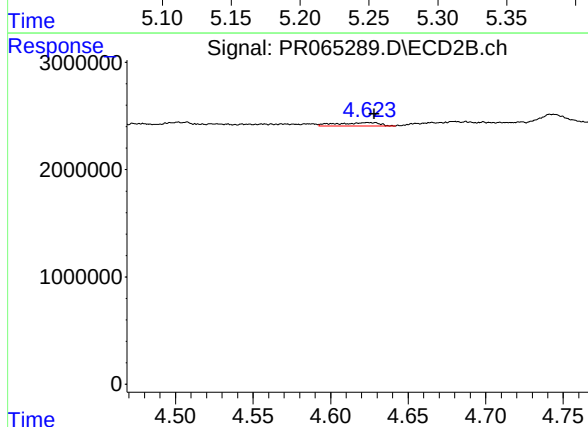


#15 AR-1232-5

R.T.: 4.624 min
Delta R.T.: -0.004 min
Response: 619938
Conc: 9.73 ng/ml

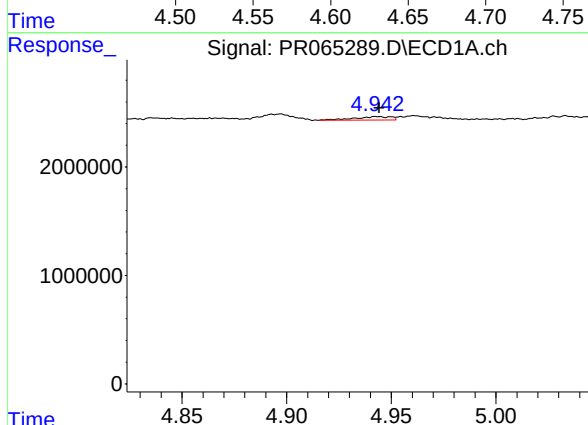


#16 AR-1242-1

R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 412323
Conc: 2.88 ng/ml

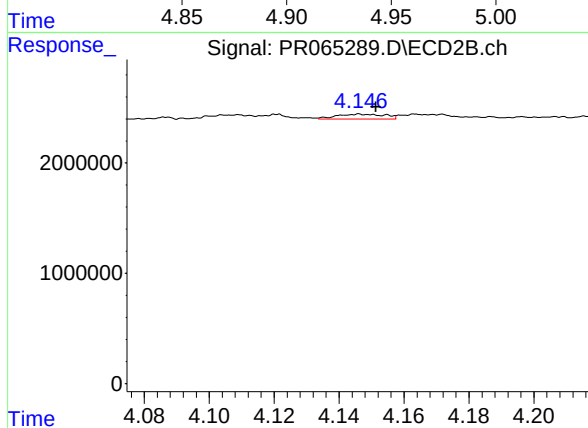

#16 AR-1242-1


R.T.: 4.146 min
Delta R.T.: -0.005 min
Response: 446421
Conc: 3.05 ng/ml

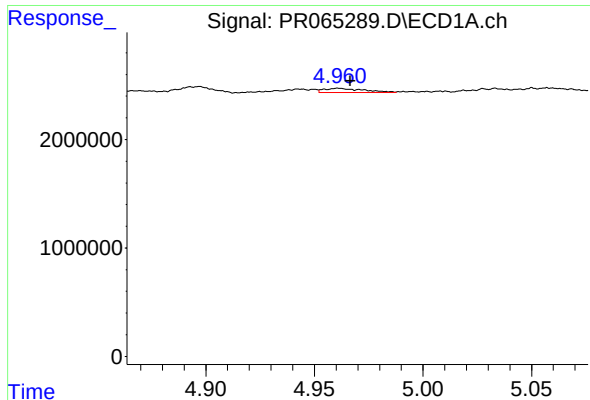

#17 AR-1242-2


R.T.: 4.961 min
Delta R.T.: -0.005 min
Response: 499502
Conc: 2.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

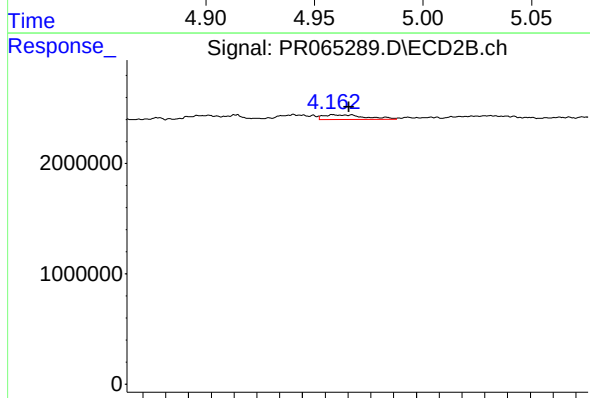


#17 AR-1242-2

R.T.: 4.164 min
Delta R.T.: -0.006 min
Response: 558444
Conc: 2.80 ng/ml

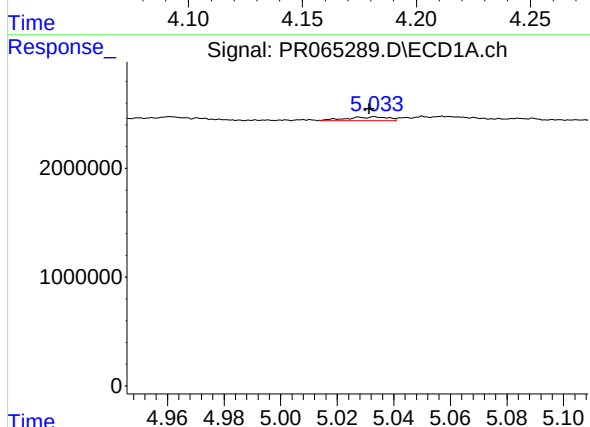


#18 AR-1242-3

R.T.: 5.034 min
Delta R.T.: 0.002 min
Response: 358637
Conc: 2.65 ng/ml

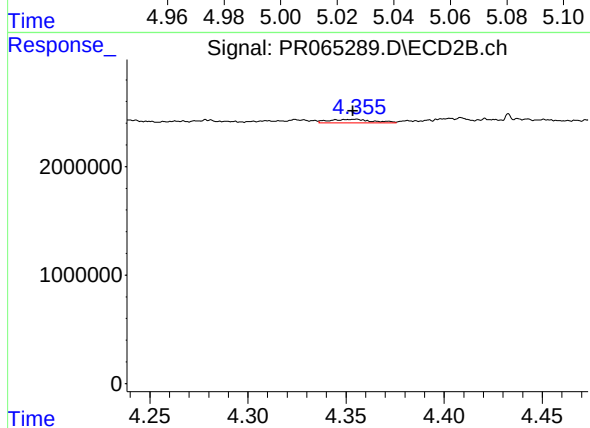

#18 AR-1242-3


R.T.: 4.355 min
Delta R.T.: 0.001 min
Response: 527675
Conc: 4.82 ng/ml

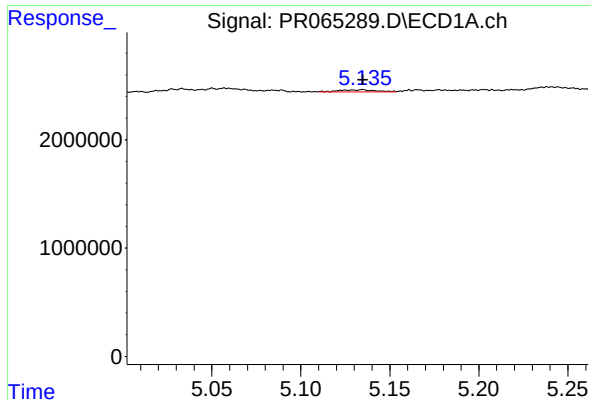

#19 AR-1242-4


R.T.: 5.135 min
Delta R.T.: 0.000 min
Response: 260395
Conc: 2.40 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

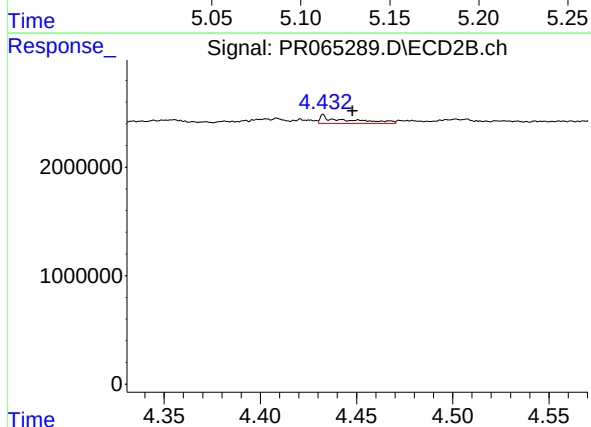


#19 AR-1242-4

R.T.: 4.433 min
Delta R.T.: -0.015 min
Response: 713501
Conc: 6.80 ng/ml

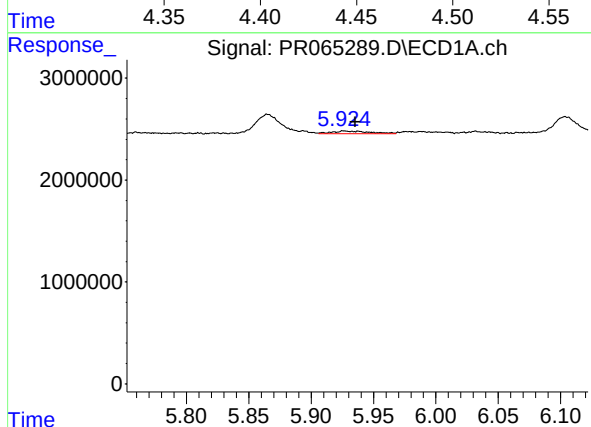


#20 AR-1242-5

R.T.: 5.926 min
Delta R.T.: -0.009 min
Response: 551810
Conc: 4.88 ng/ml

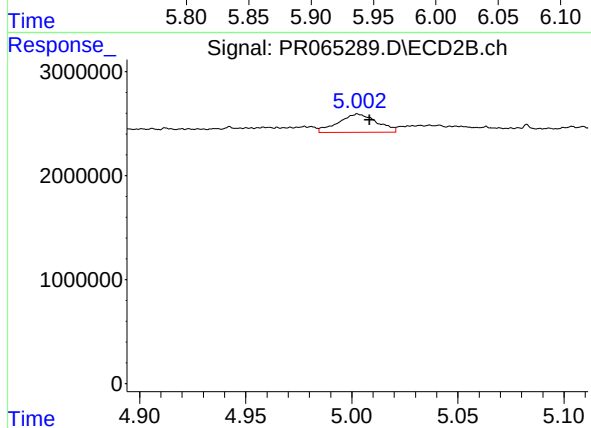

#20 AR-1242-5


R.T.: 5.003 min
Delta R.T.: -0.006 min
Response: 2233652
Conc: 16.54 ng/ml

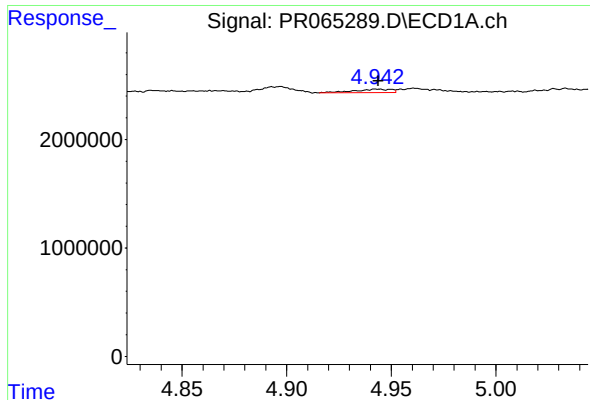

#21 AR-1248-1


R.T.: 4.943 min
Delta R.T.: 0.000 min
Response: 412323
Conc: 3.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

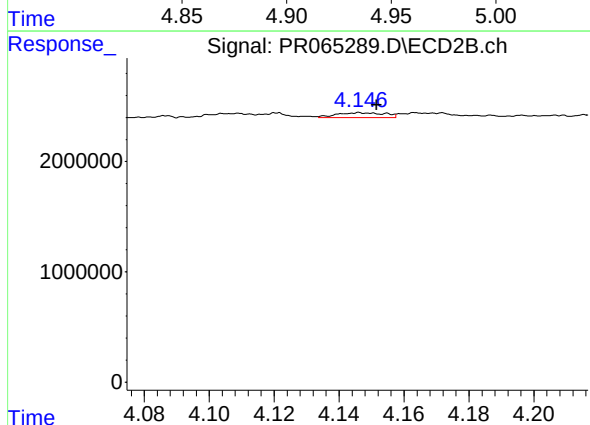


#21 AR-1248-1

R.T.: 4.146 min
Delta R.T.: -0.005 min
Response: 446421
Conc: 4.13 ng/ml

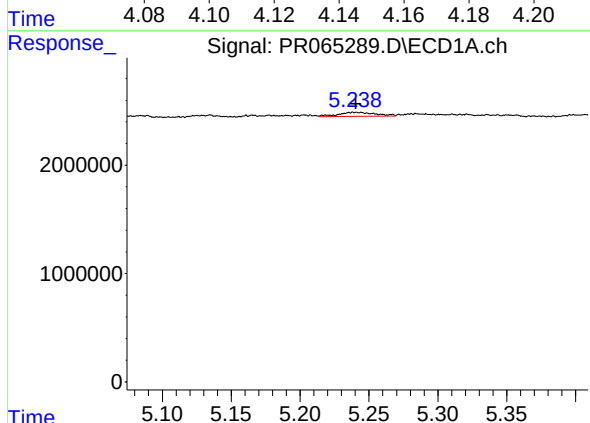


#22 AR-1248-2

R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 702958
Conc: 4.52 ng/ml

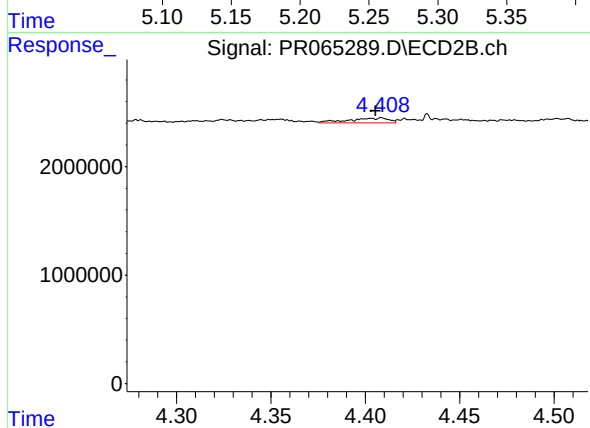

#22 AR-1248-2


R.T.: 4.409 min
Delta R.T.: 0.003 min
Response: 669228
Conc: 4.62 ng/ml

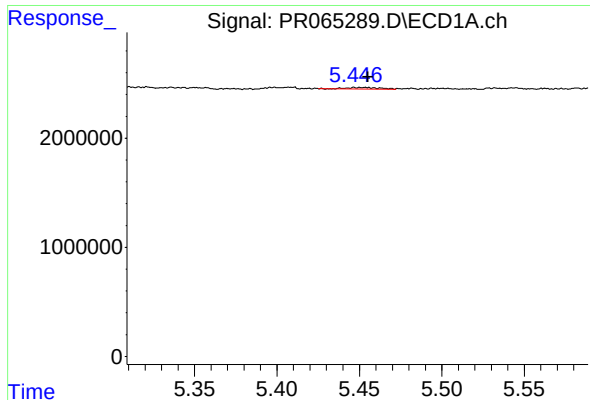

#23 AR-1248-3


R.T.: 5.454 min
Delta R.T.: -0.002 min
Response: 174246
Conc: 0.98 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

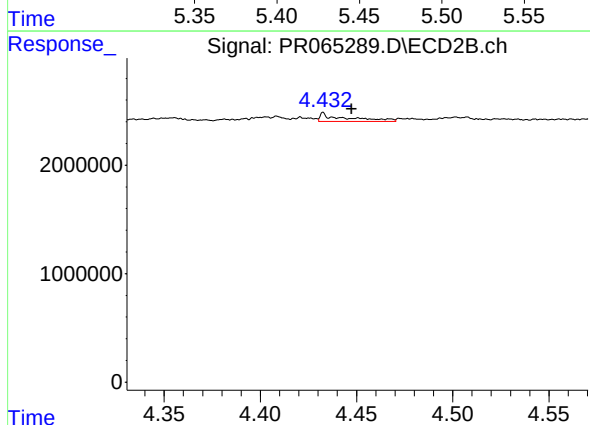


#23 AR-1248-3

R.T.: 4.433 min
Delta R.T.: -0.014 min
Response: 713501
Conc: 4.61 ng/ml

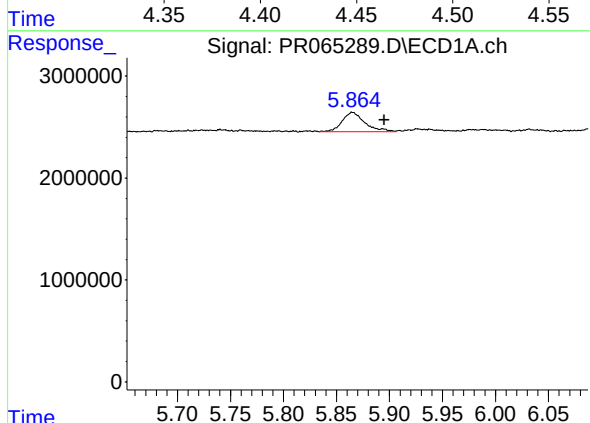


#24 AR-1248-4

R.T.: 5.865 min
Delta R.T.: -0.030 min
Response: 2851493
Conc: 15.04 ng/ml

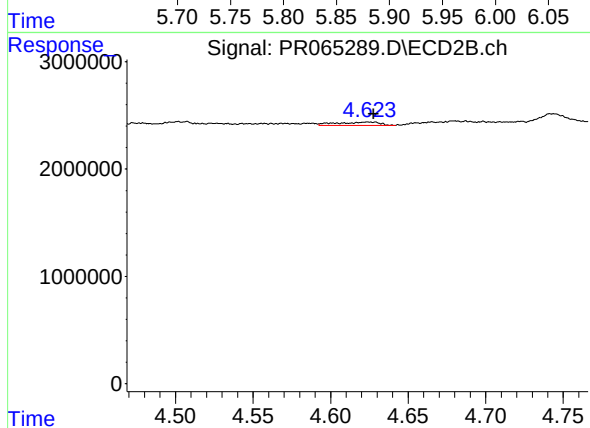

#24 AR-1248-4


R.T.: 4.624 min
Delta R.T.: -0.004 min
Response: 619938
Conc: 3.31 ng/ml

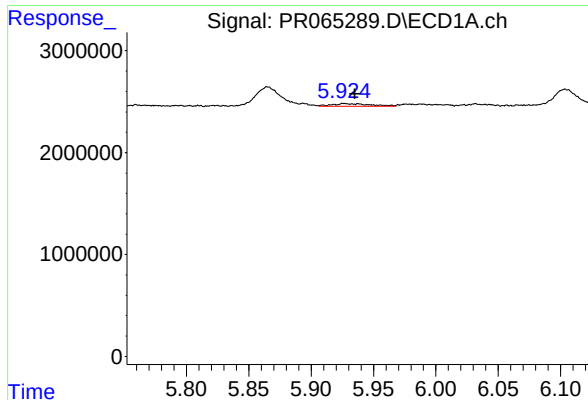

#25 AR-1248-5


R.T.: 5.926 min
Delta R.T.: -0.009 min
Response: 551810
Conc: 2.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

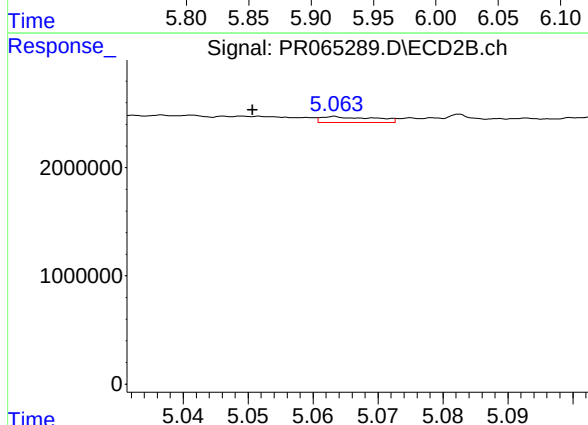


#25 AR-1248-5

R.T.: 5.063 min
Delta R.T.: 0.013 min
Response: 301829
Conc: 1.62 ng/ml

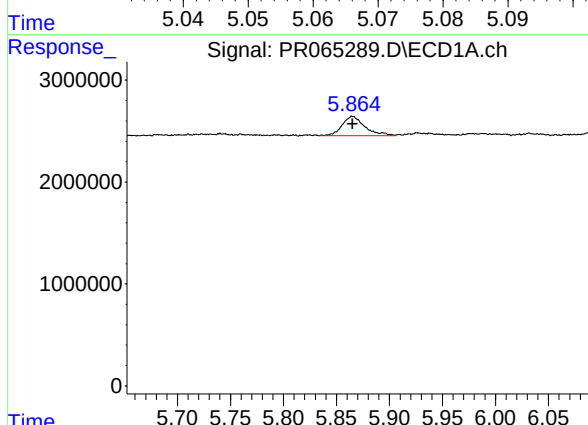


#26 AR-1254-1

R.T.: 5.865 min
Delta R.T.: 0.000 min
Response: 2851493
Conc: 13.92 ng/ml

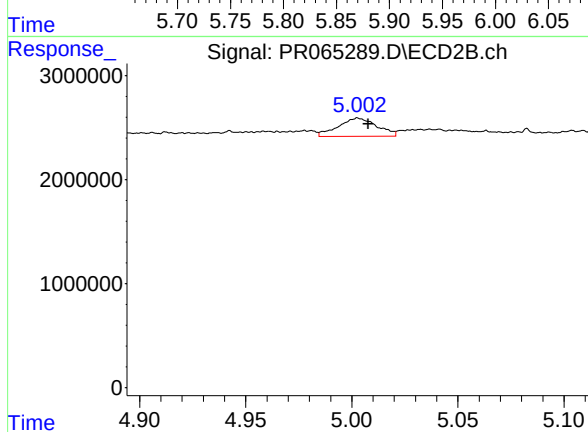

#26 AR-1254-1


R.T.: 5.003 min
Delta R.T.: -0.005 min
Response: 2233652
Conc: 7.67 ng/ml

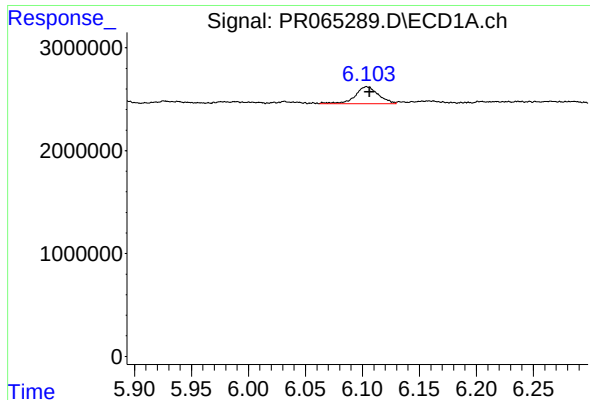

#27 AR-1254-2


R.T.: 6.104 min
Delta R.T.: -0.002 min
Response: 2340275
Conc: 7.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

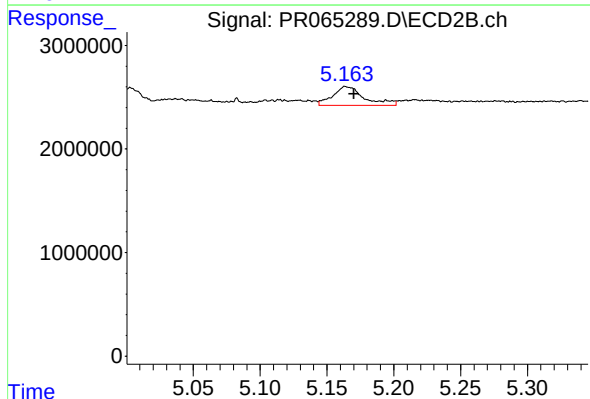


#27 AR-1254-2

R.T.: 5.164 min
Delta R.T.: -0.006 min
Response: 2993209
Conc: 11.82 ng/ml

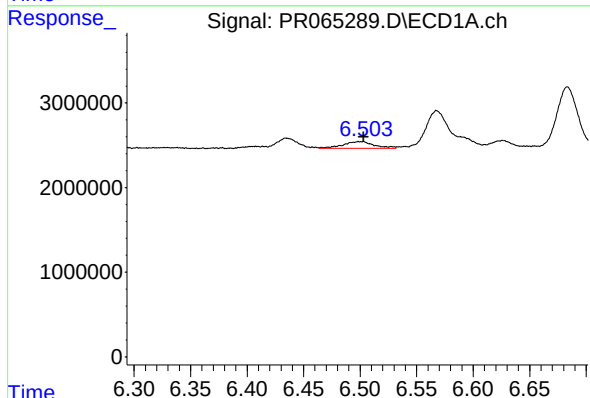


#28 AR-1254-3

R.T.: 6.501 min
Delta R.T.: -0.002 min
Response: 1564824
Conc: 4.89 ng/ml

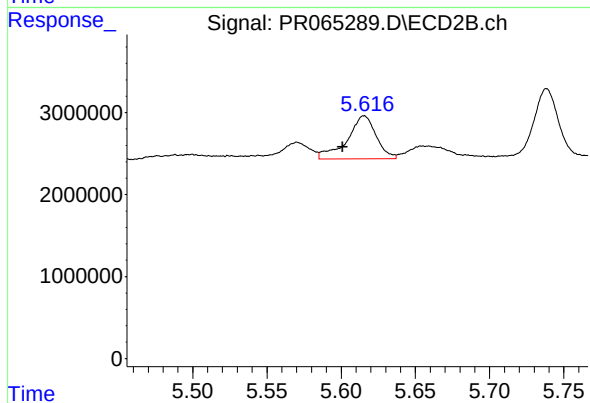

#28 AR-1254-3


R.T.: 5.615 min
Delta R.T.: 0.014 min
Response: 7110768
Conc: 17.38 ng/ml

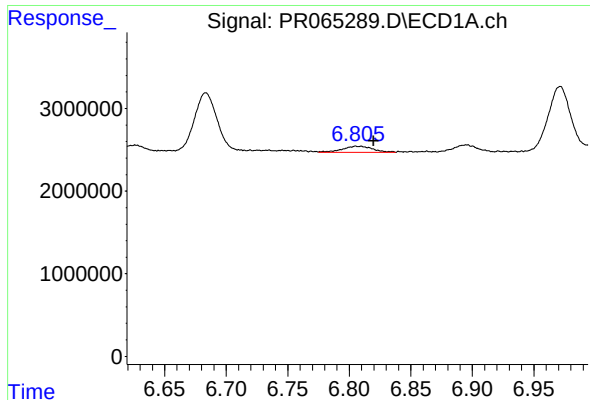

#29 AR-1254-4


R.T.: 6.806 min
Delta R.T.: -0.014 min
Response: 1297719
Conc: 5.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

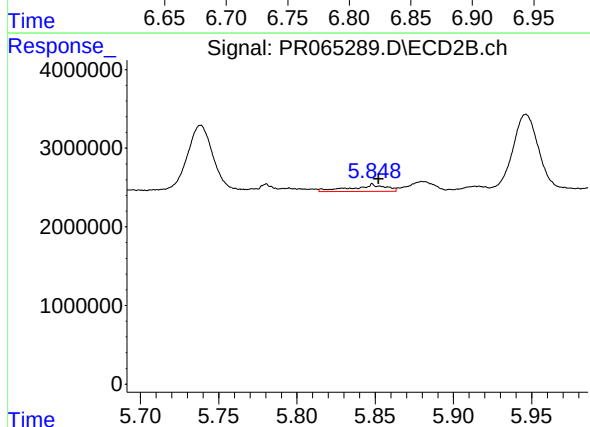


#29 AR-1254-4

R.T.: 5.848 min
Delta R.T.: -0.004 min
Response: 1386833
Conc: 5.40 ng/ml

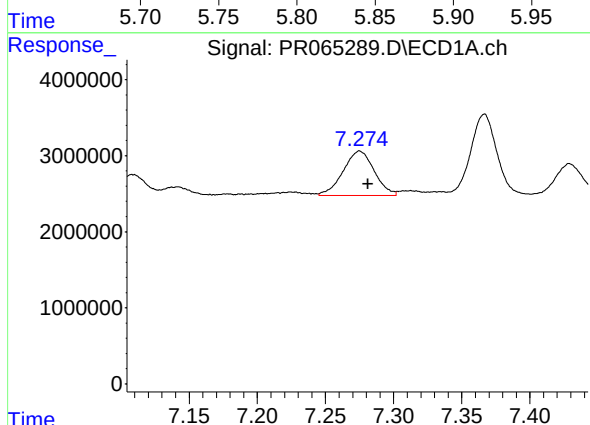


#30 AR-1254-5

R.T.: 7.275 min
Delta R.T.: -0.006 min
Response: 9307734
Conc: 37.45 ng/ml

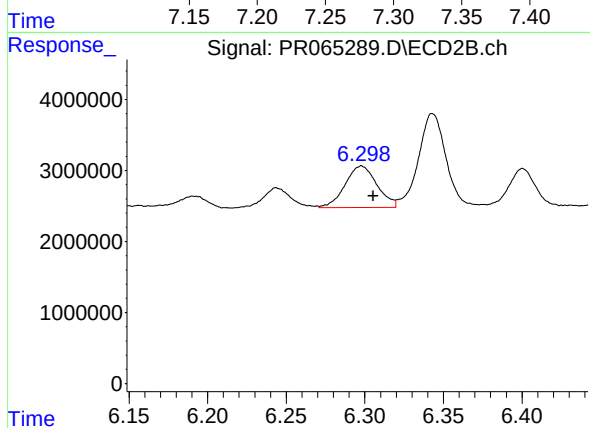

#30 AR-1254-5


R.T.: 6.298 min
Delta R.T.: -0.008 min
Response: 8248196
Conc: 22.50 ng/ml

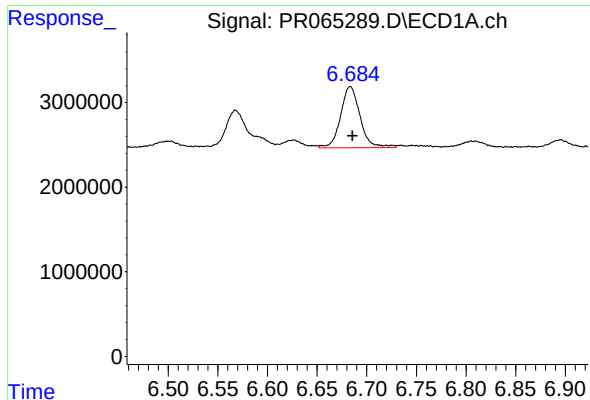

#31 AR-1260-1


R.T.: 6.683 min
Delta R.T.: -0.003 min
Response: 9849851
Conc: 39.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

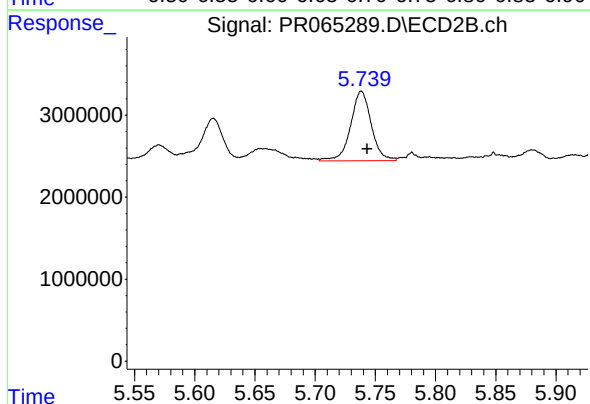


#31 AR-1260-1

R.T.: 5.738 min
Delta R.T.: -0.005 min
Response: 10165849
Conc: 35.61 ng/ml

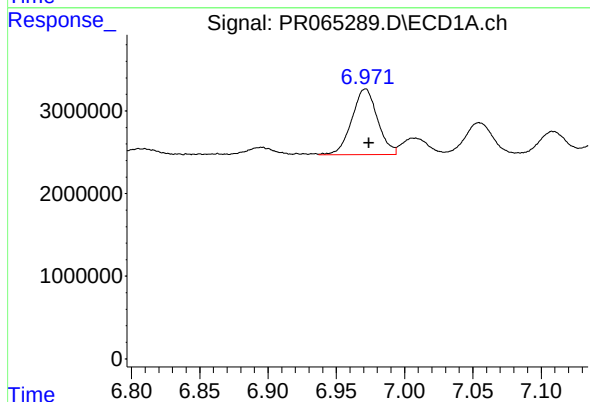


#32 AR-1260-2

R.T.: 6.971 min
Delta R.T.: -0.003 min
Response: 10411611
Conc: 36.23 ng/ml

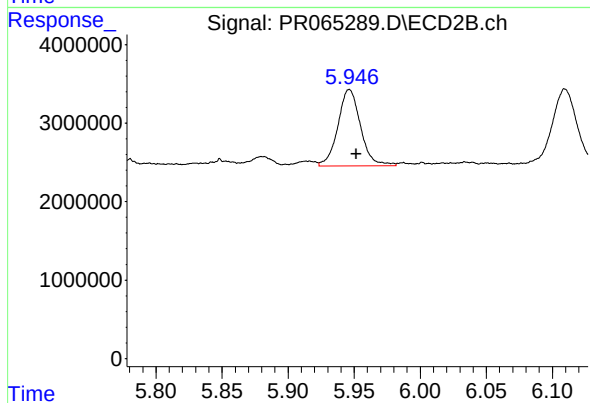

#32 AR-1260-2


R.T.: 5.946 min
Delta R.T.: -0.005 min
Response: 11649861
Conc: 33.59 ng/ml

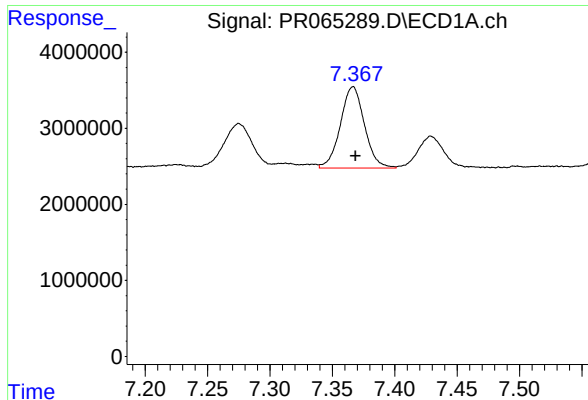

#33 AR-1260-3


R.T.: 7.367 min
Delta R.T.: -0.002 min
Response: 14347092
Conc: 67.86 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

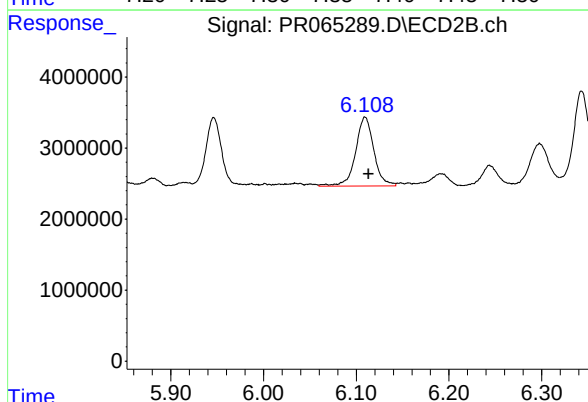


#33 AR-1260-3

R.T.: 6.110 min
Delta R.T.: -0.004 min
Response: 13372621
Conc: 41.16 ng/ml

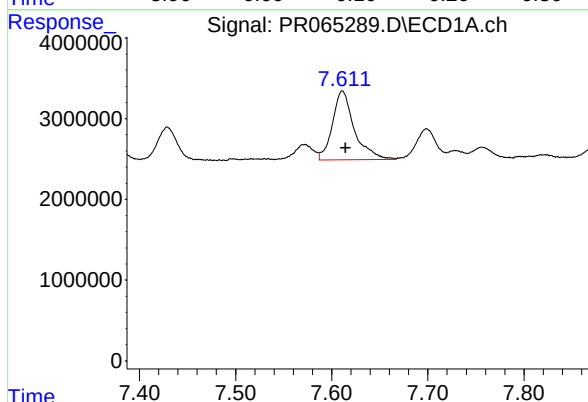


#34 AR-1260-4

R.T.: 7.611 min
Delta R.T.: -0.003 min
Response: 13486781
Conc: 57.15 ng/ml

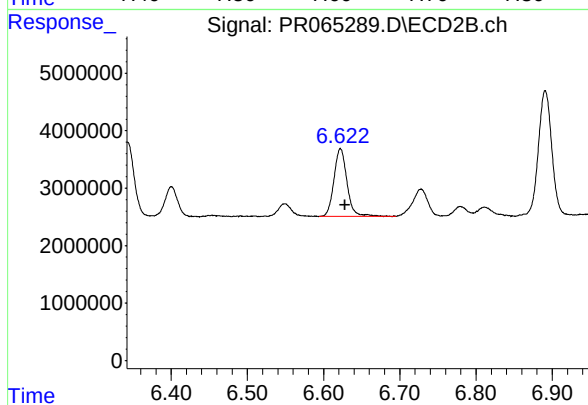

#34 AR-1260-4


R.T.: 6.622 min
Delta R.T.: -0.006 min
Response: 14062299
Conc: 53.23 ng/ml

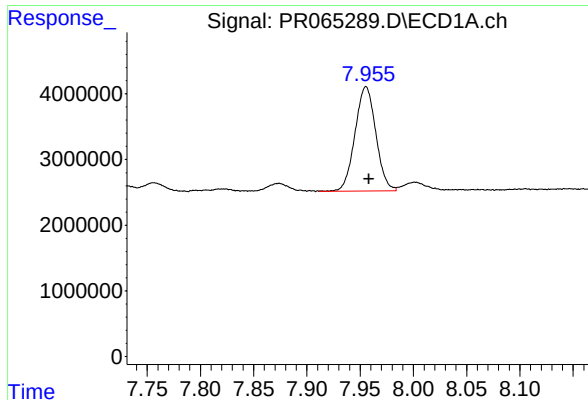

#35 AR-1260-5


R.T.: 7.955 min
Delta R.T.: -0.003 min
Response: 21630091
Conc: 49.20 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

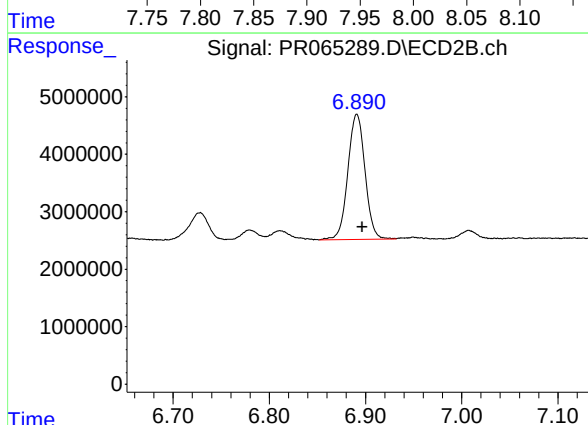


#35 AR-1260-5

R.T.: 6.891 min
Delta R.T.: -0.006 min
Response: 26720919
Conc: 43.33 ng/ml

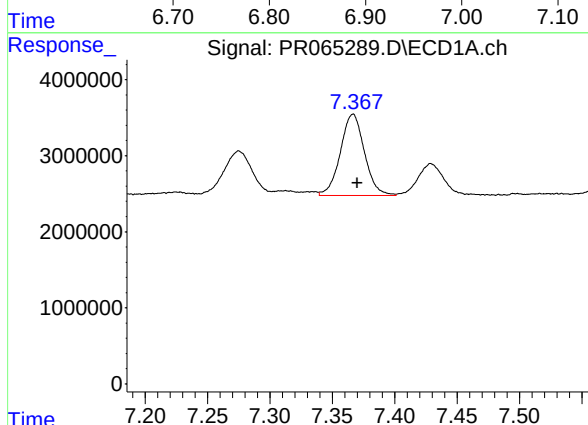


#36 AR-1262-1

R.T.: 7.367 min
Delta R.T.: -0.003 min
Response: 14347092
Conc: 42.38 ng/ml

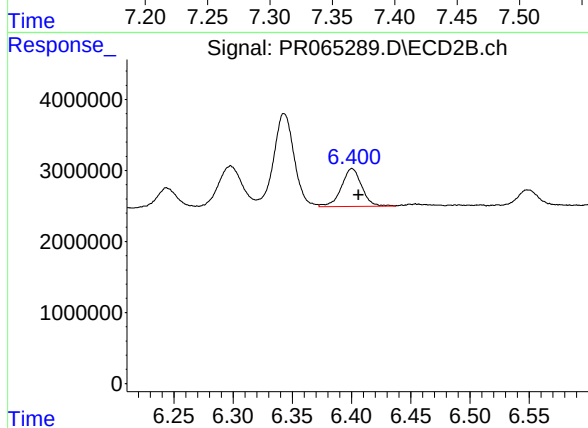

#36 AR-1262-1


R.T.: 6.400 min
Delta R.T.: -0.006 min
Response: 6439839
Conc: 35.90 ng/ml

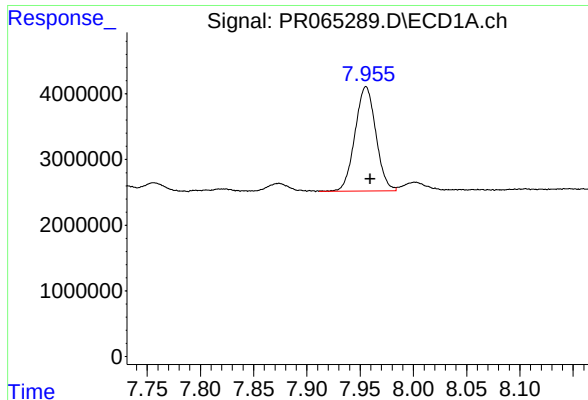

#37 AR-1262-2


R.T.: 7.955 min
Delta R.T.: -0.004 min
Response: 21630091
Conc: 38.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

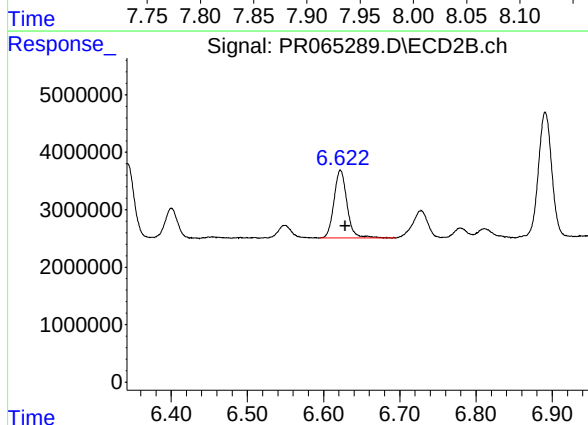


#37 AR-1262-2

R.T.: 6.622 min
Delta R.T.: -0.006 min
Response: 14062299
Conc: 36.14 ng/ml

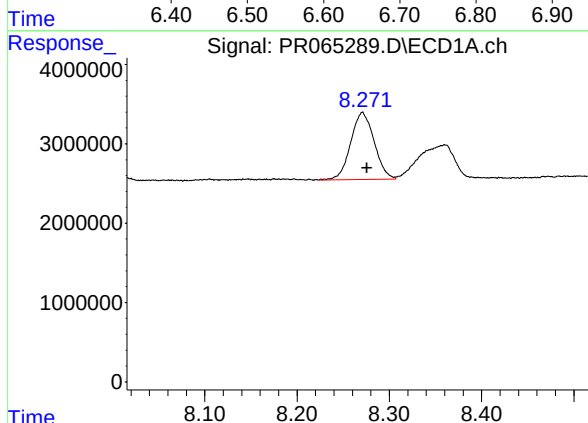


#38 AR-1262-3

R.T.: 8.271 min
Delta R.T.: -0.005 min
Response: 14944284
Conc: 39.27 ng/ml

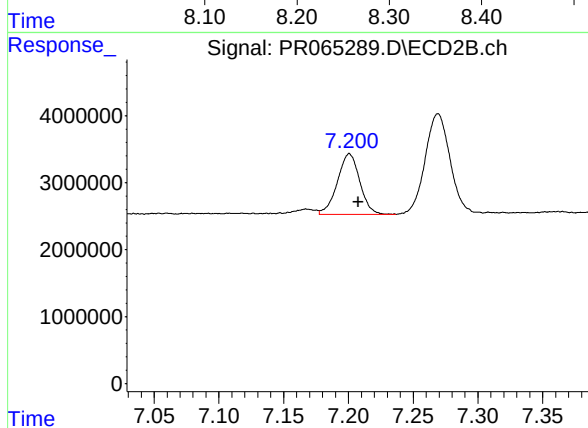

#38 AR-1262-3


R.T.: 7.201 min
Delta R.T.: -0.007 min
Response: 10874318
Conc: 38.37 ng/ml

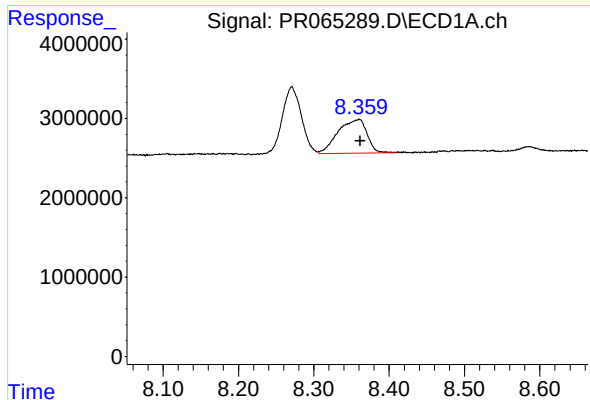

#39 AR-1262-4


R.T.: 8.360 min
Delta R.T.: -0.001 min
Response: 11338013
Conc: 38.71 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

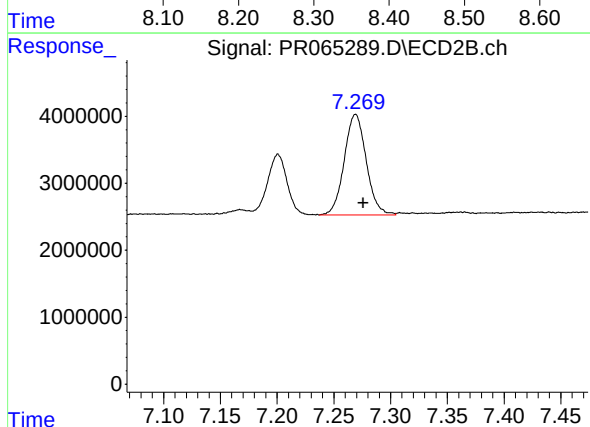


#39 AR-1262-4

R.T.: 7.269 min
Delta R.T.: -0.007 min
Response: 20282317
Conc: 35.22 ng/ml

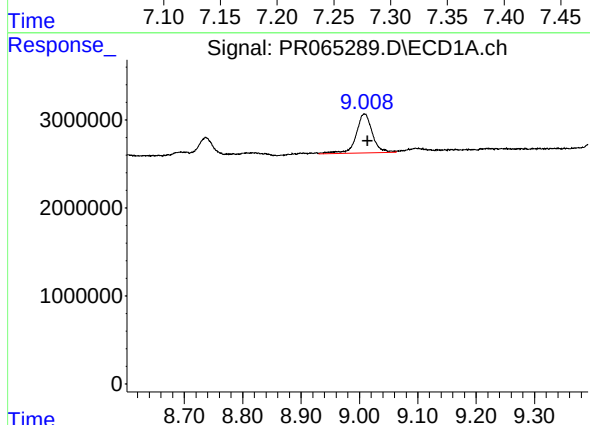


#40 AR-1262-5

R.T.: 9.009 min
Delta R.T.: -0.005 min
Response: 8632578
Conc: 43.08 ng/ml

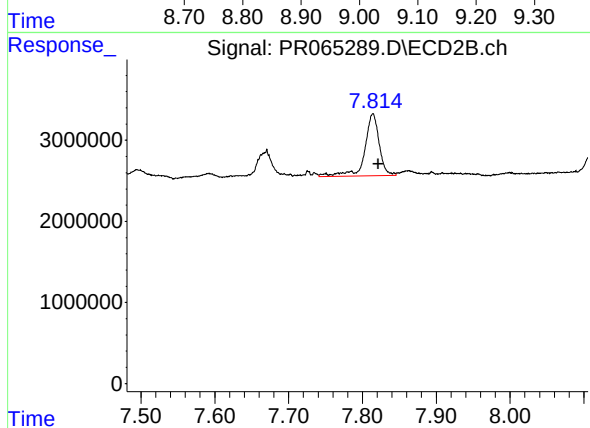

#40 AR-1262-5


R.T.: 7.814 min
Delta R.T.: -0.007 min
Response: 10448812
Conc: 40.15 ng/ml

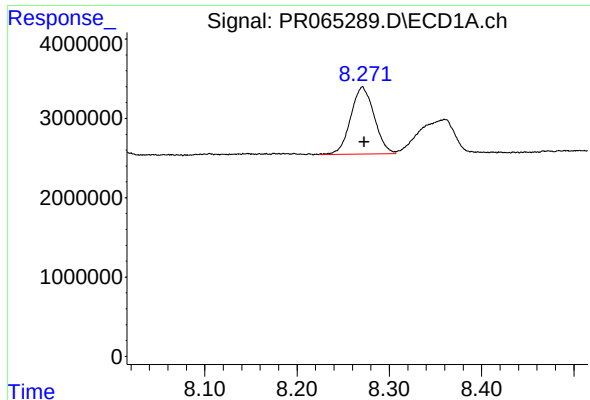

#41 AR-1268-1


R.T.: 8.271 min
Delta R.T.: -0.002 min
Response: 14944284
Conc: 24.65 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

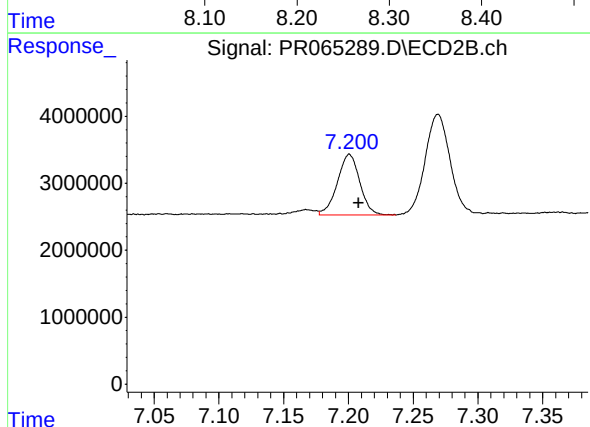


#41 AR-1268-1

R.T.: 7.201 min
Delta R.T.: -0.007 min
Response: 10874318
Conc: 13.71 ng/ml

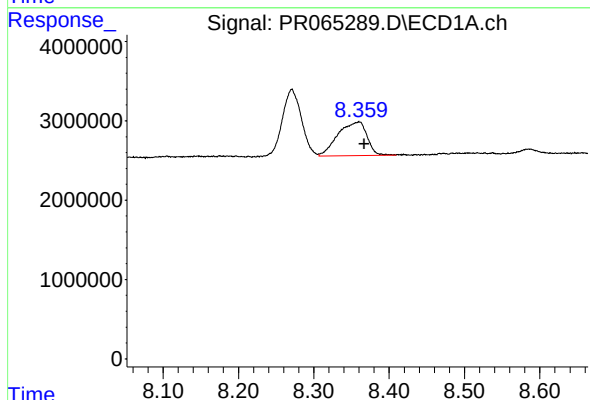


#42 AR-1268-2

R.T.: 8.360 min
Delta R.T.: -0.007 min
Response: 11338013
Conc: 20.72 ng/ml

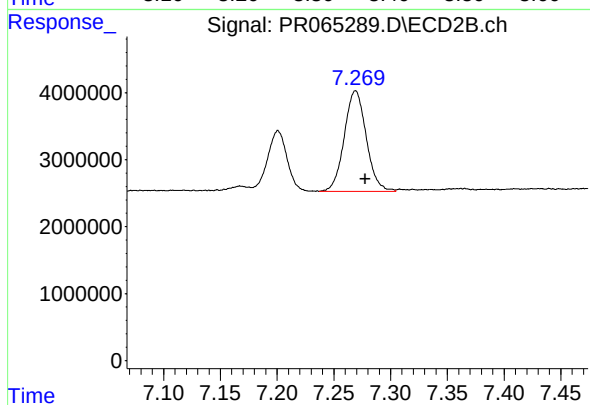

#42 AR-1268-2


R.T.: 7.269 min
Delta R.T.: -0.009 min
Response: 20282317
Conc: 27.24 ng/ml

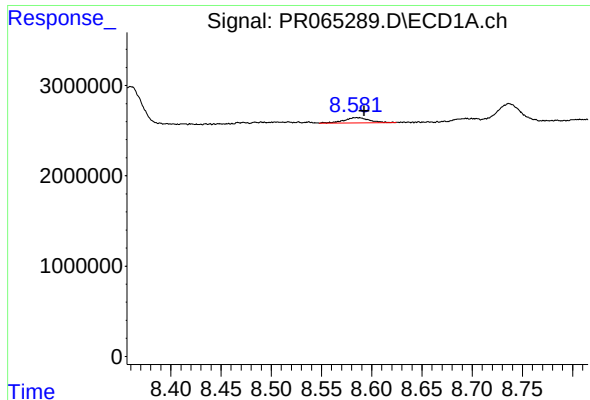

#43 AR-1268-3


R.T.: 8.585 min
Delta R.T.: -0.008 min
Response: 994074
Conc: 2.10 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

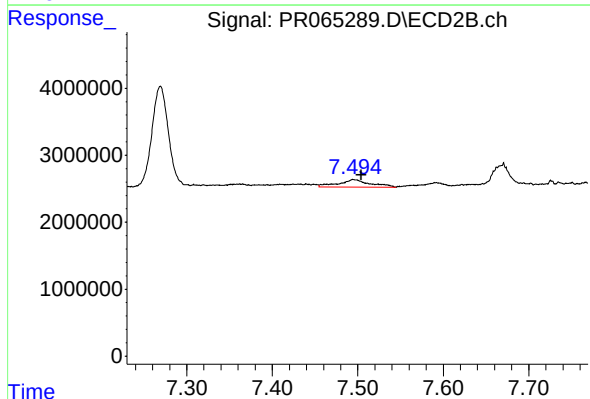


#43 AR-1268-3

R.T.: 7.495 min
Delta R.T.: -0.009 min
Response: 2920884
Conc: 4.61 ng/ml

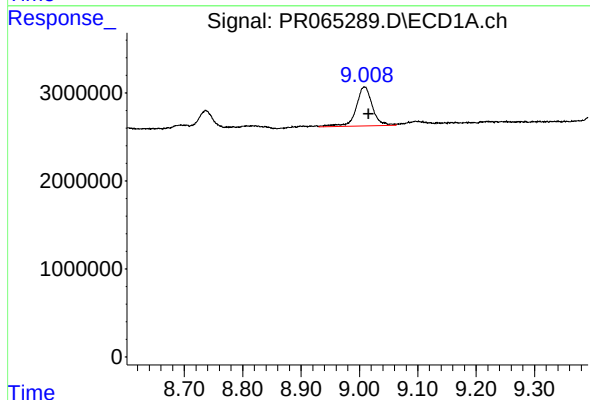


#44 AR-1268-4

R.T.: 9.009 min
Delta R.T.: -0.007 min
Response: 8632578
Conc: 42.42 ng/ml

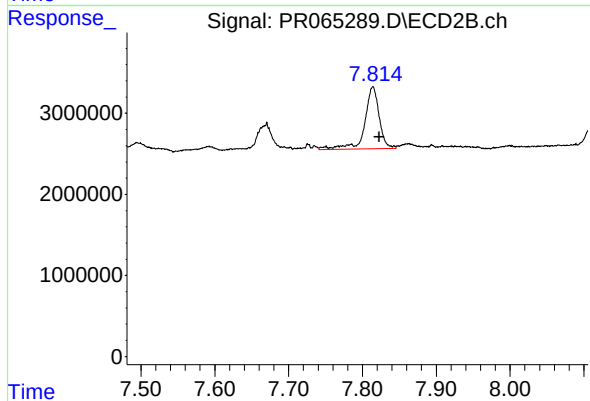

#44 AR-1268-4


R.T.: 7.814 min
Delta R.T.: -0.009 min
Response: 10448812
Conc: 39.83 ng/ml

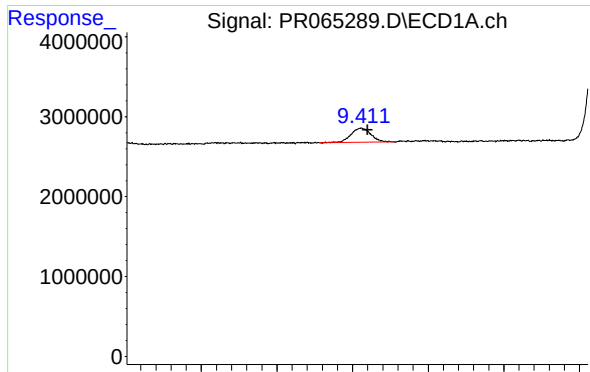

#45 AR-1268-5

R.T.: 9.411 min
Delta R.T.: -0.008 min
Response: 3225477
Conc: 2.21 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2024

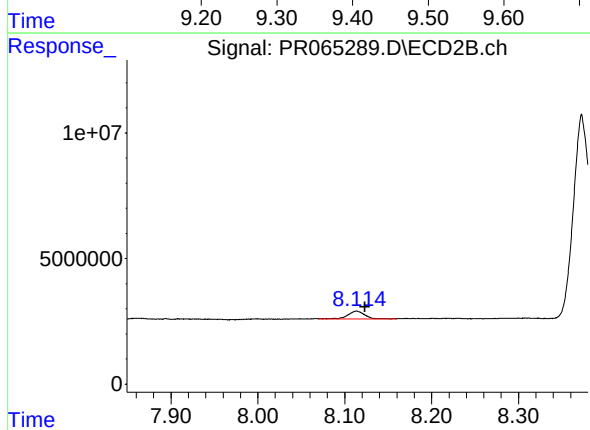

#45 AR-1268-5

R.T.: 8.114 min
Delta R.T.: -0.009 min
Response: 4192120
Conc: 2.19 ng/ml