

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
 Data File : PR065230.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 09:42
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/29/2024
 Supervised By :Sohil Jodhani 01/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:20:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.701	3.002	108.9E6	98705213	18.236	18.045
2) SA Decachlor...	9.740	8.370	81452736	86183334	20.366	18.210m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
Data File : PR065230.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 09:42
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/29/2024
Supervised By :Sohil Jodhani 01/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:20:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

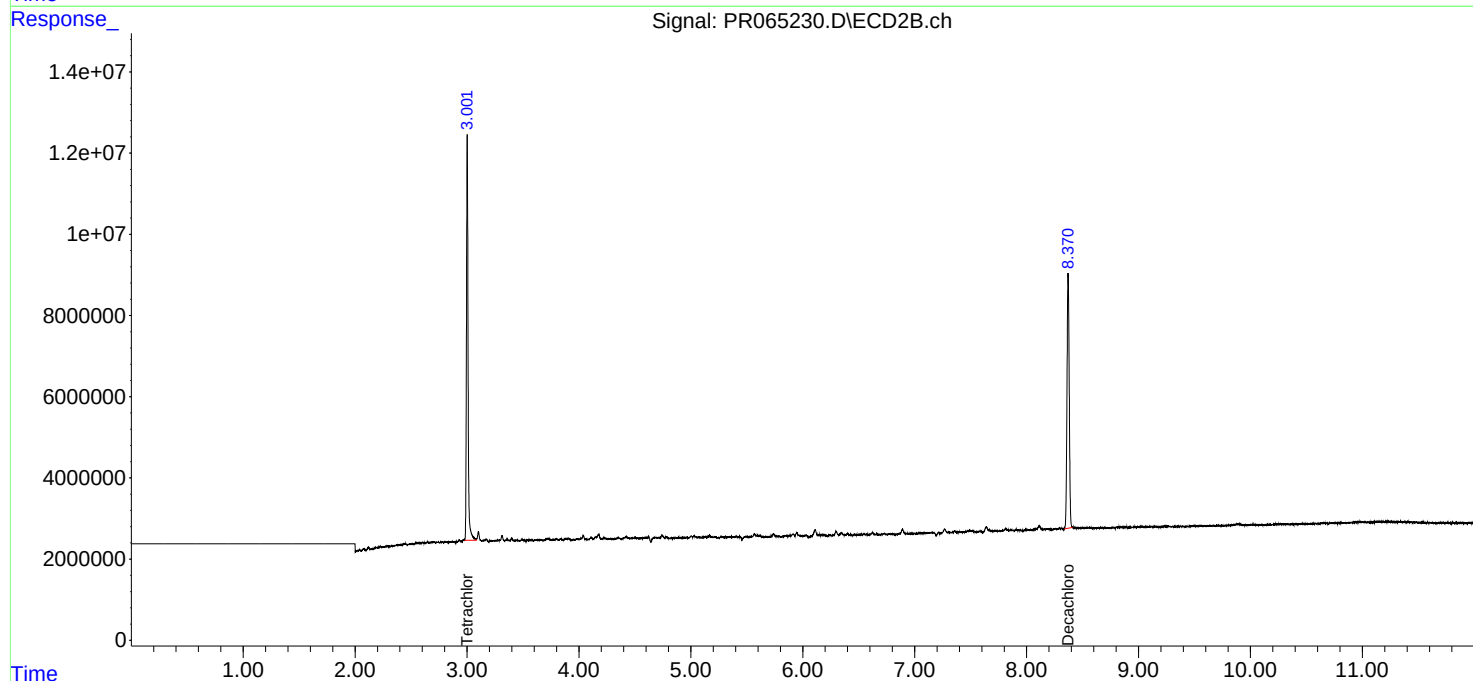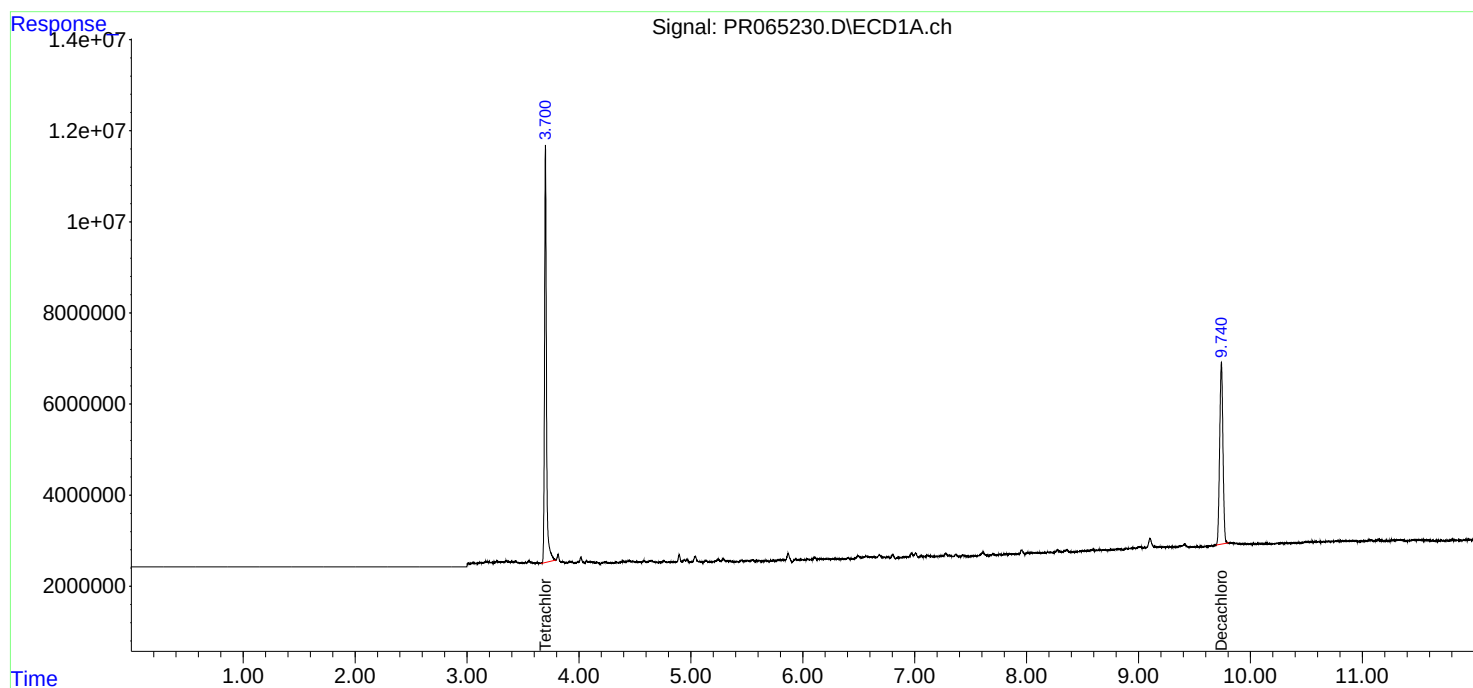

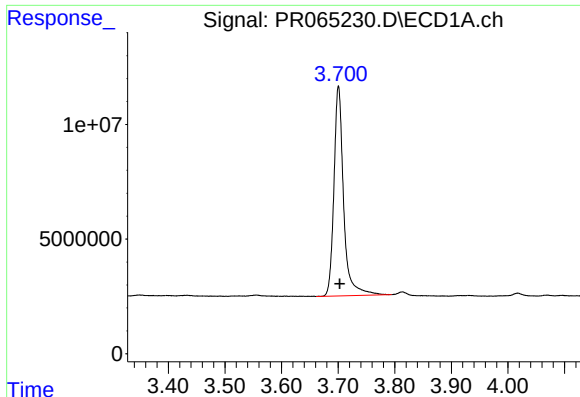

#1 Tetrachloro-m-xylene

R.T.: 3.701 min
Delta R.T.: -0.002 min
Response: 108852563
Conc: 18.24 ng/ml

Instrument :

ECD_R

ClientSampleId :


I.BLK

Manual Integrations

APPROVED


Reviewed By :Ankita Jodhani 01/29/2024

Supervised By :Sohil Jodhani 01/29/2024

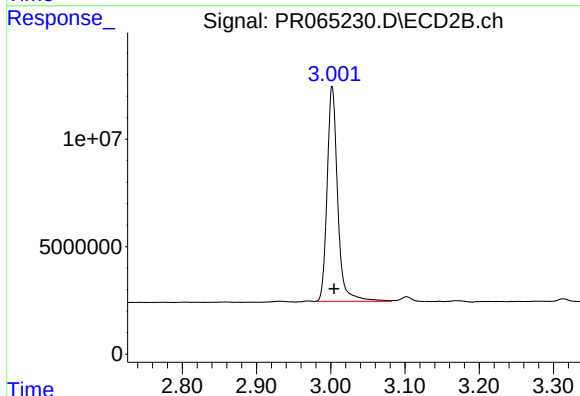


#1 Tetrachloro-m-xylene

R.T.: 3.002 min
Delta R.T.: -0.002 min
Response: 98705213
Conc: 18.05 ng/ml

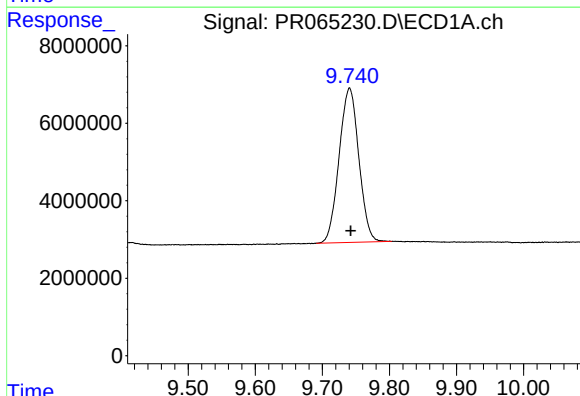

#2 Decachlorobiphenyl

R.T.: 9.740 min
Delta R.T.: -0.002 min
Response: 81452736
Conc: 20.37 ng/ml

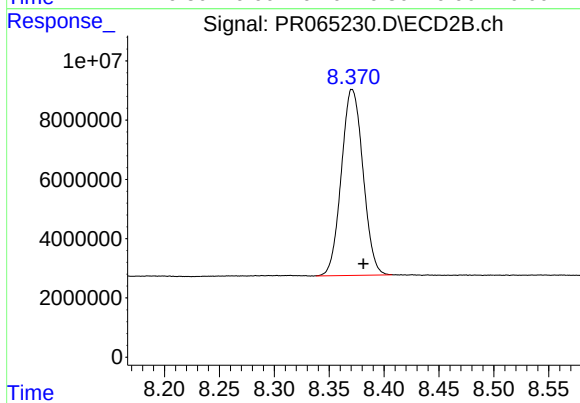

#2 Decachlorobiphenyl

R.T.: 8.370 min
Delta R.T.: -0.012 min
Response: 86183334
Conc: 18.21 ng/ml m