

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
 Data File : PR065241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2024 09:57
 Operator : AJ\MA
 Sample : PB158601BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 PB158601BL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/29/2024
 Supervised By :Sohil Jodhani 01/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:20:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.701	3.003	138.1E6	126.4E6	23.139	23.106
2) SA Decachlor...	9.737	8.370	101.2E6	109.5E6	25.292	23.147m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR012724\
Data File : PR065241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2024 09:57
Operator : AJ\MA
Sample : PB158601BL
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
PB158601BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/29/2024
Supervised By :Sohil Jodhani 01/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:20:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

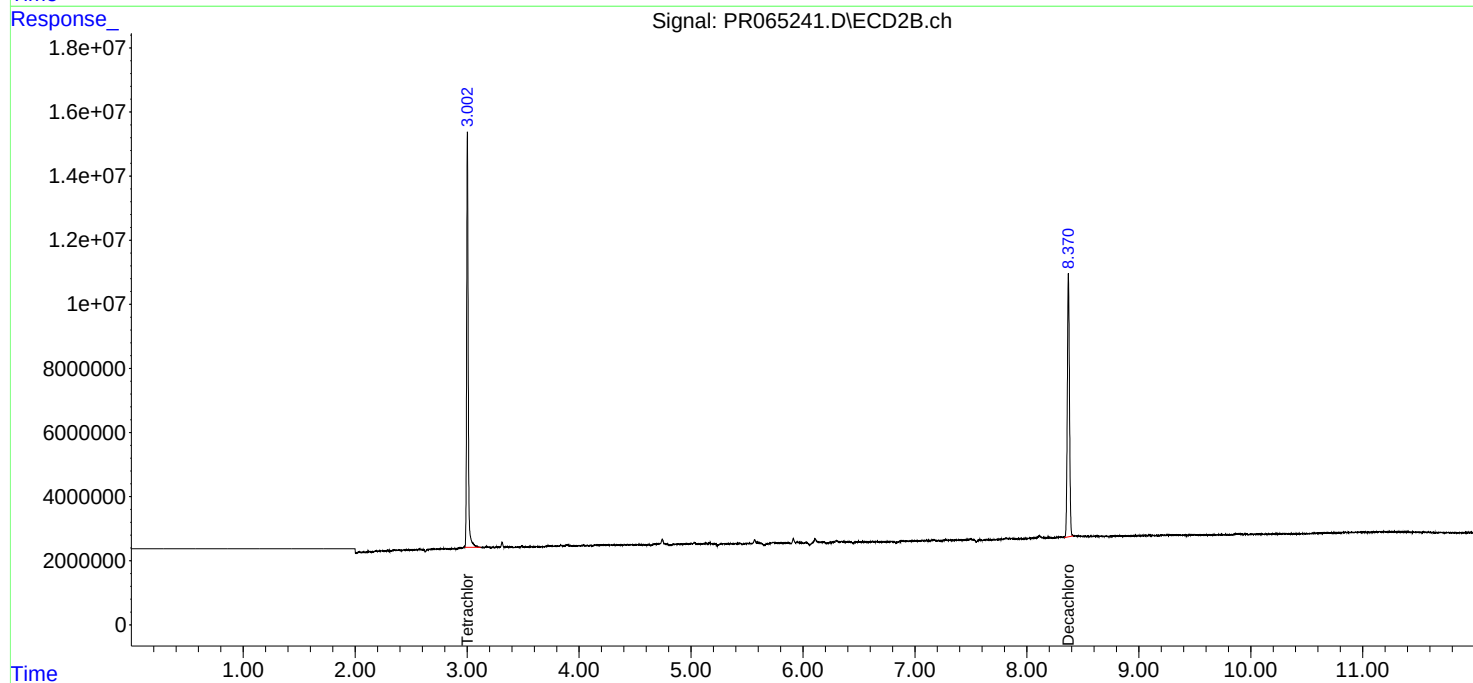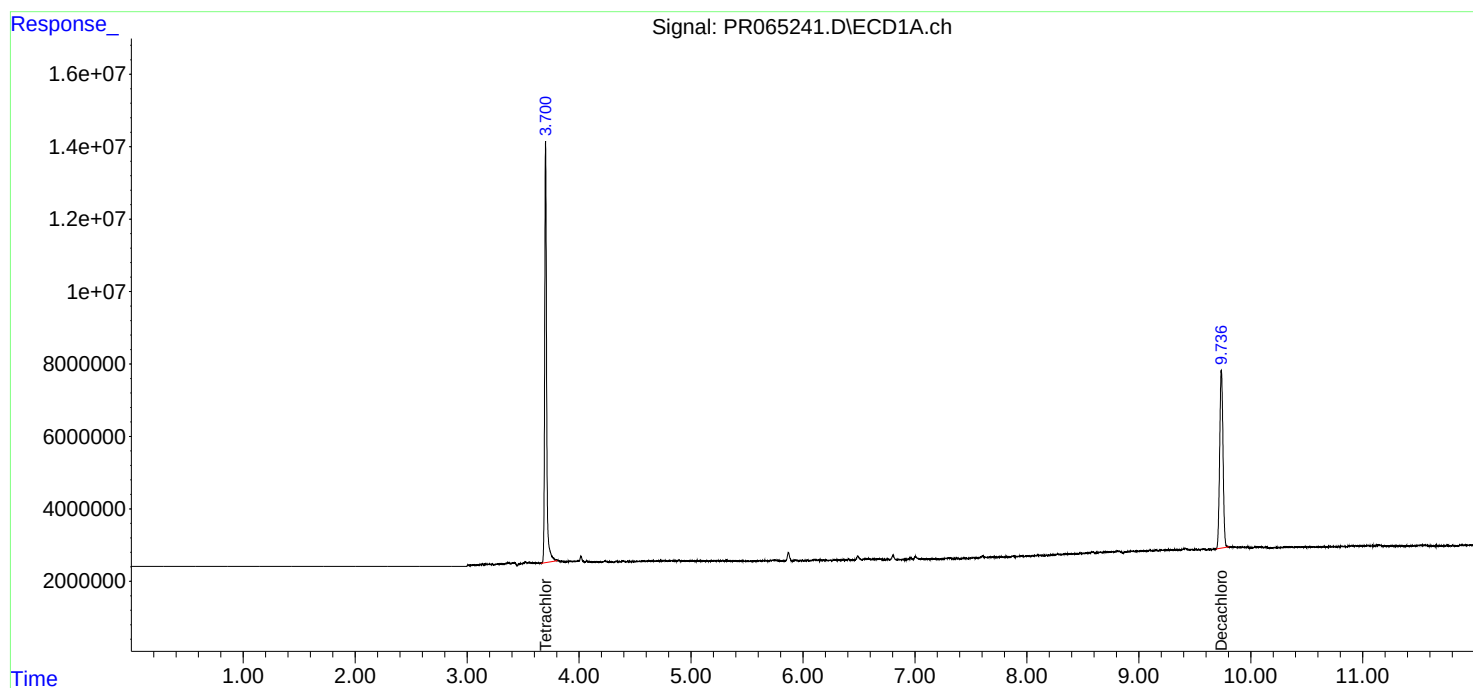

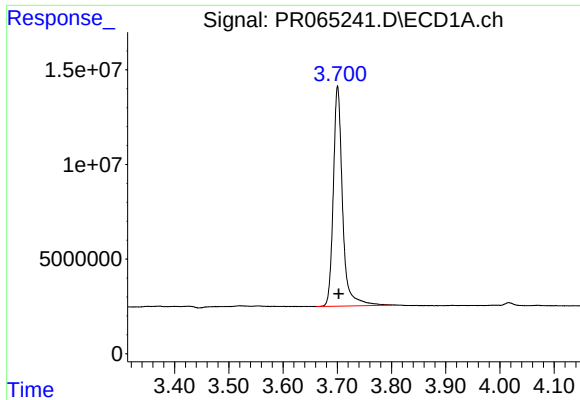


#1 Tetrachloro-m-xylene

R.T.: 3.701 min
Delta R.T.: -0.002 min
Response: 138123763
Conc: 23.14 ng/ml

Instrument :
ECD_R
ClientSampleId :
PB158601BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/29/2024
Supervised By :Sohil Jodhani 01/29/2024

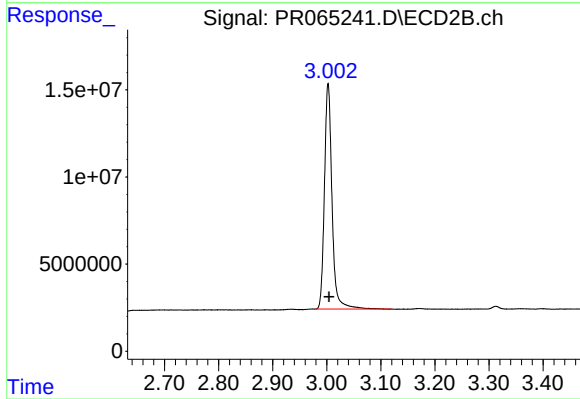


#1 Tetrachloro-m-xylene

R.T.: 3.003 min
Delta R.T.: -0.002 min
Response: 126383114
Conc: 23.11 ng/ml

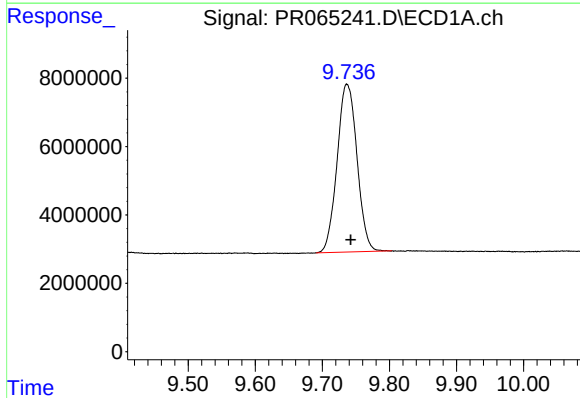

#2 Decachlorobiphenyl

R.T.: 9.737 min
Delta R.T.: -0.005 min
Response: 101156810
Conc: 25.29 ng/ml

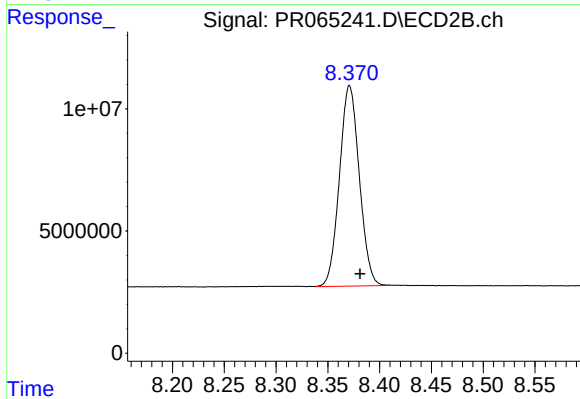

#2 Decachlorobiphenyl

R.T.: 8.370 min
Delta R.T.: -0.011 min
Response: 109548032
Conc: 23.15 ng/ml m