

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR013124\
 Data File : PR065339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2024 10:12
 Operator : AJ\MA
 Sample : P1187-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 19:11:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.701	3.001	132.5E6	121.6E6	22.192	22.239
2)	SA Decachlor...	9.742	8.374	103.1E6	116.7E6	25.783	24.663
Target Compounds							
3)	L1 AR-1016-1	4.949	4.151	500494	634663	2.824	3.495
4)	L1 AR-1016-2	4.967	4.151f	571105	634663	2.191	2.567
5)	L1 AR-1016-3	5.035	4.347	388316	226353	2.323	1.669 #
6)	L1 AR-1016-4	5.132	4.403	256603	279559	1.914	2.669 #
7)	L1 AR-1016-5	5.450	4.623	253368	284745	1.876	2.041
8)	L2 AR-1221-1	3.934	0.000	454509	0	6.333	N.D. #
9)	L2 AR-1221-2	4.017	3.311	2190732	1904275	41.789	39.926
10)	L2 AR-1221-3	4.070f	3.397	725346	612152	4.721	4.432
11)	L3 AR-1232-1	4.070f	3.397	725346	612152	5.366	5.111
12)	L3 AR-1232-2	4.639	4.151f	876769	634663	11.381	5.195 #
13)	L3 AR-1232-3	4.967	4.347	571105	226353	4.479	3.403
14)	L3 AR-1232-4	5.132	4.444	256603	234295	3.915	4.092
15)	L3 AR-1232-5	5.246	4.623	365461	284745	7.556	4.467 #
16)	L4 AR-1242-1	4.949	4.151	500494	634663	3.501	4.343
17)	L4 AR-1242-2	4.967	4.151f	571105	634663	2.712	3.182
18)	L4 AR-1242-3	5.035	4.347	388316	226353	2.867	2.067 #
19)	L4 AR-1242-4	5.132	4.444	256603	234295	2.361	2.232
20)	L4 AR-1242-5	5.938	5.002	352655	335092	3.118	2.482
21)	L5 AR-1248-1	4.949	4.151	500494	634663	4.704	5.875
22)	L5 AR-1248-2	5.246	4.403	365461	279559	2.352	1.930
23)	L5 AR-1248-3	5.450	4.444	253368	234295	1.419	1.514
24)	L5 AR-1248-4	5.873f	4.623	3014767	284745	15.902	1.521 #
25)	L5 AR-1248-5	5.938	5.049	352655	149904	1.851	0.805 #
26)	L6 AR-1254-1	5.873	5.002	3014767	335092	14.720	1.150 #
27)	L6 AR-1254-2	6.106	5.165	183725	279289	0.589	1.102 #
28)	L6 AR-1254-3	6.494	5.599	944852	638008	2.953	1.559 #
29)	L6 AR-1254-4	6.809	5.843	1946439	442552	8.494	1.724 #
30)	L6 AR-1254-5	7.278	6.298	559520	626812	2.251	1.710
31)	L7 AR-1260-1	6.684	5.739	747283	622576	2.973	2.181 #
32)	L7 AR-1260-2	6.970	5.946	504506	739331	1.755	2.132
33)	L7 AR-1260-3	7.369	6.112	3430669	1666951	16.227	5.131 #
34)	L7 AR-1260-4	7.638f	6.621	5366923	4844498	22.744	18.337
35)	L7 AR-1260-5	7.959	6.890	2391648	2632914	5.440	4.269
36)	L8 AR-1262-1	7.369	6.399	3430669	406054	10.135	2.264 #
37)	L8 AR-1262-2	7.959	6.621	2391648	4844498	4.228	12.451 #
38)	L8 AR-1262-3	8.272	7.201	17044500	20002814	44.792	70.572 #
39)	L8 AR-1262-4	8.365	7.271	15335126	17961208	52.351	31.188 #
40)	L8 AR-1262-5	9.014	7.816	5567895	6576264	27.785	25.267
41)	L9 AR-1268-1	8.272	7.201	17044500	20002814	28.114	25.214

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR013124\
Data File : PR065339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2024 10:12
Operator : AJ\MA
Sample : P1187-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 4 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 19:11:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.365	7.271	15335126	17961208	28.026	24.126
43)	L9 AR-1268-3	8.591	7.497	13145963	15970350	27.706	25.210
44)	L9 AR-1268-4	9.014	7.816	5567895	6576264	27.363	25.071
45)	L9 AR-1268-5	9.417	8.116	38788236	45655738	26.609	23.847


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

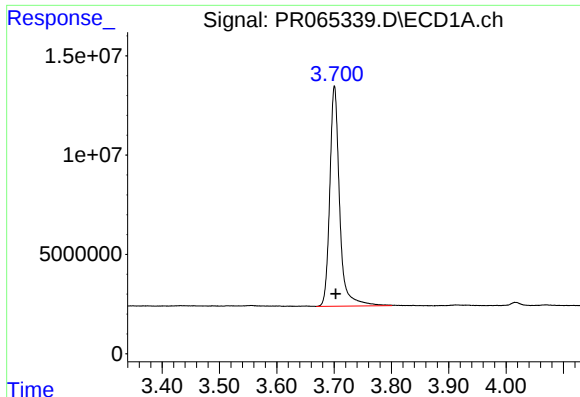

#1 Tetrachloro-m-xylene


R.T.: 3.701 min
Delta R.T.: -0.002 min
Response: 132471631
Conc: 22.19 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

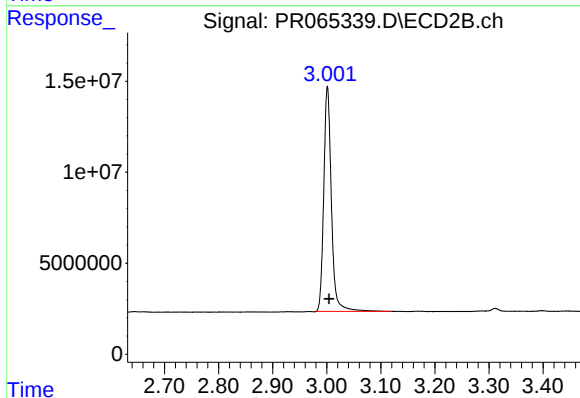


#1 Tetrachloro-m-xylene

R.T.: 3.001 min
Delta R.T.: -0.003 min
Response: 121645213
Conc: 22.24 ng/ml

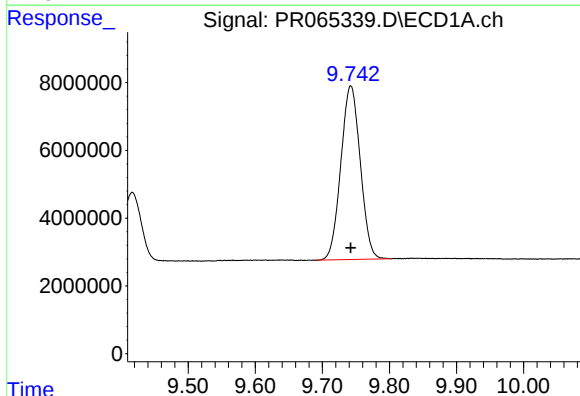


#2 Decachlorobiphenyl

R.T.: 9.742 min
Delta R.T.: 0.000 min
Response: 103118158
Conc: 25.78 ng/ml

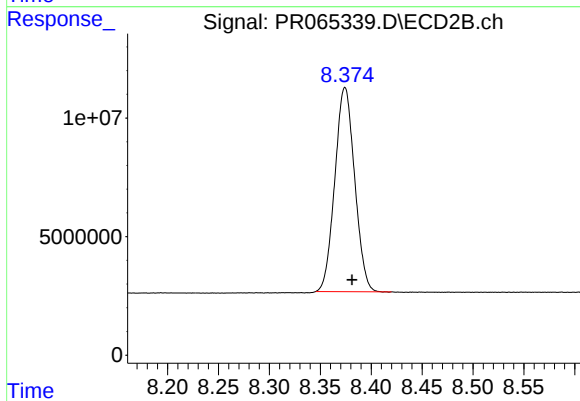

#2 Decachlorobiphenyl


R.T.: 8.374 min
Delta R.T.: -0.007 min
Response: 116721907
Conc: 24.66 ng/ml

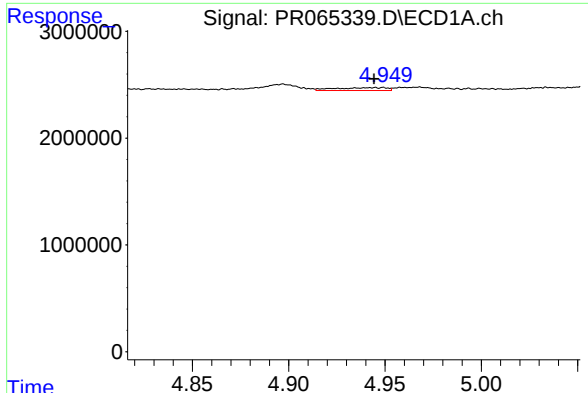

#3 AR-1016-1


R.T.: 4.949 min
Delta R.T.: 0.004 min
Response: 500494
Conc: 2.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

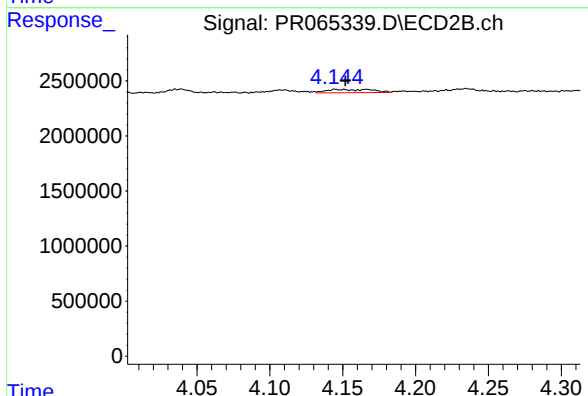


#3 AR-1016-1

R.T.: 4.151 min
Delta R.T.: 0.000 min
Response: 634663
Conc: 3.49 ng/ml

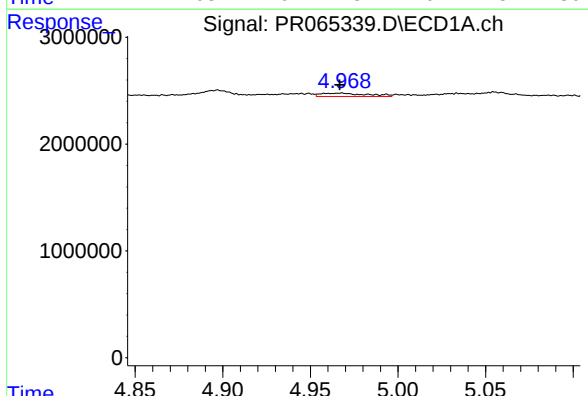


#4 AR-1016-2

R.T.: 4.967 min
Delta R.T.: 0.000 min
Response: 571105
Conc: 2.19 ng/ml

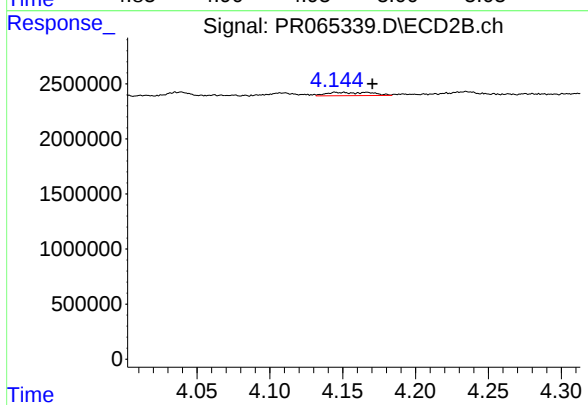

#4 AR-1016-2


R.T.: 4.151 min
Delta R.T.: -0.020 min
Response: 634663
Conc: 2.57 ng/ml

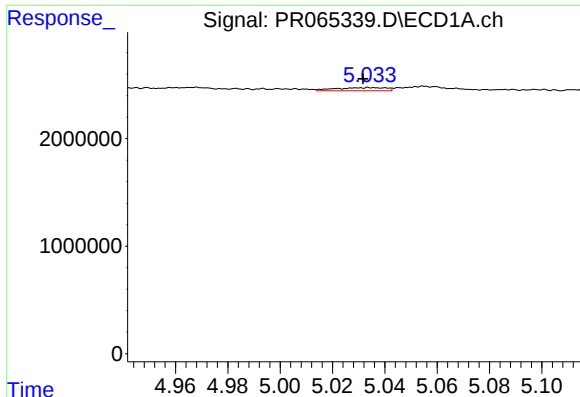

#5 AR-1016-3


R.T.: 5.035 min
Delta R.T.: 0.003 min
Response: 388316
Conc: 2.32 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

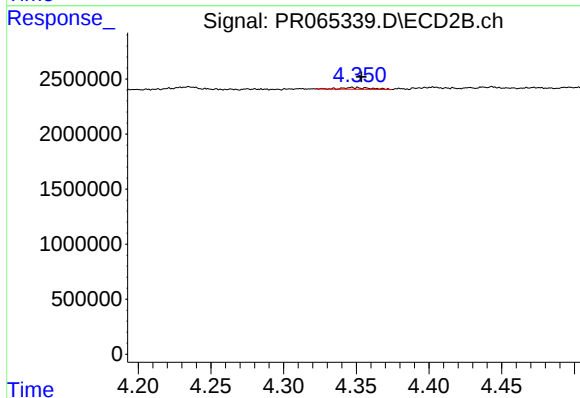


#5 AR-1016-3

R.T.: 4.347 min
Delta R.T.: -0.006 min
Response: 226353
Conc: 1.67 ng/ml

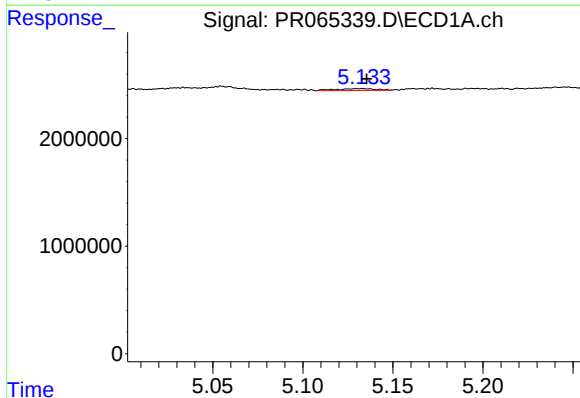


#6 AR-1016-4

R.T.: 5.132 min
Delta R.T.: -0.003 min
Response: 256603
Conc: 1.91 ng/ml

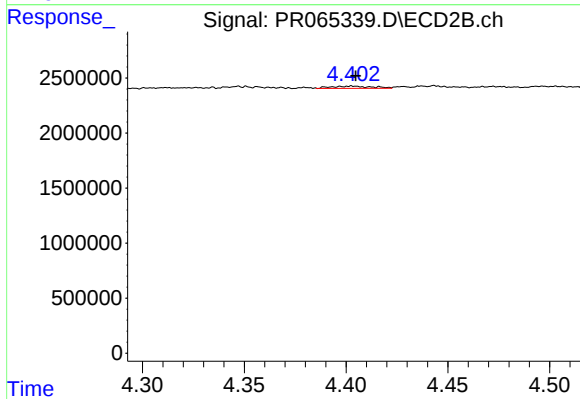

#6 AR-1016-4


R.T.: 4.403 min
Delta R.T.: -0.002 min
Response: 279559
Conc: 2.67 ng/ml

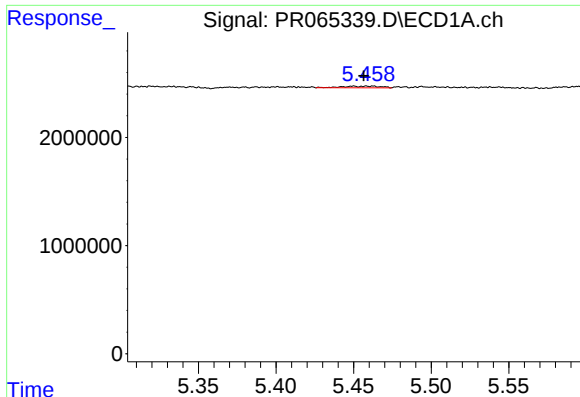

#7 AR-1016-5


R.T.: 5.450 min
Delta R.T.: -0.006 min
Response: 253368
Conc: 1.88 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

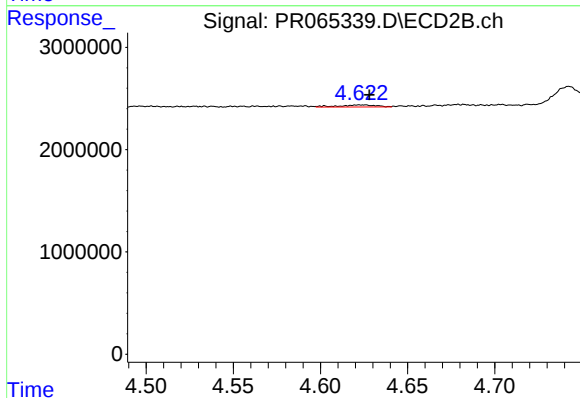


#7 AR-1016-5

R.T.: 4.623 min
Delta R.T.: -0.005 min
Response: 284745
Conc: 2.04 ng/ml

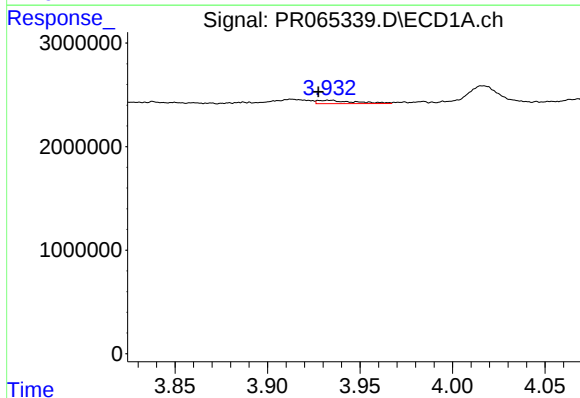


#8 AR-1221-1

R.T.: 3.934 min
Delta R.T.: 0.006 min
Response: 454509
Conc: 6.33 ng/ml

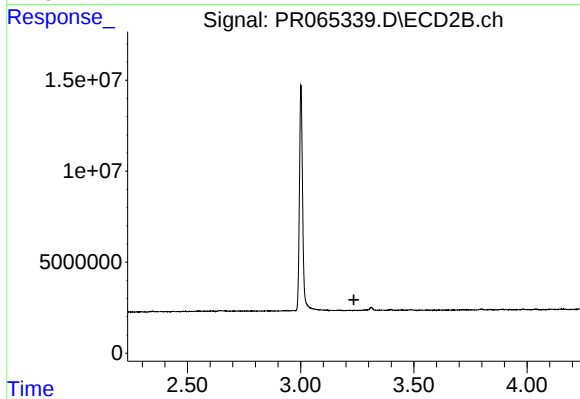

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.235 min
Response: 0
Conc: N.D.

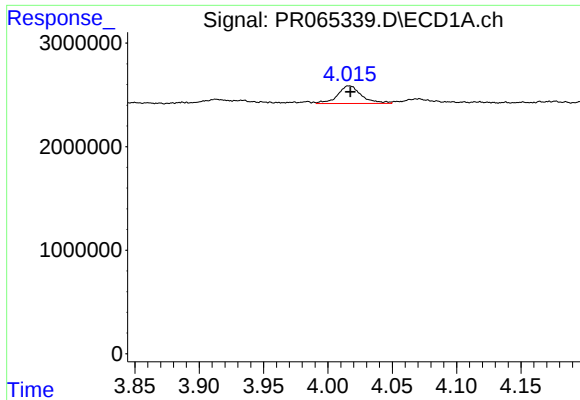

#9 AR-1221-2


R.T.: 4.017 min
Delta R.T.: 0.000 min
Response: 2190732
Conc: 41.79 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

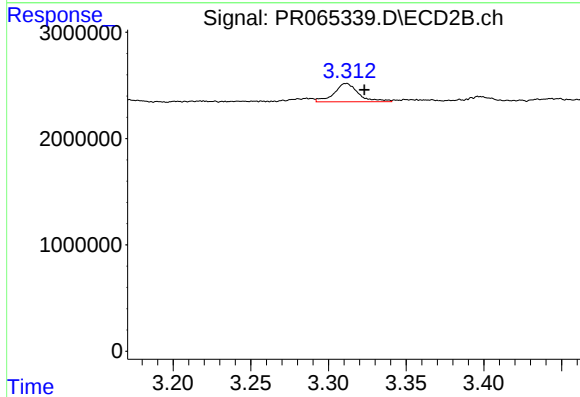


#9 AR-1221-2

R.T.: 3.311 min
Delta R.T.: -0.012 min
Response: 1904275
Conc: 39.93 ng/ml

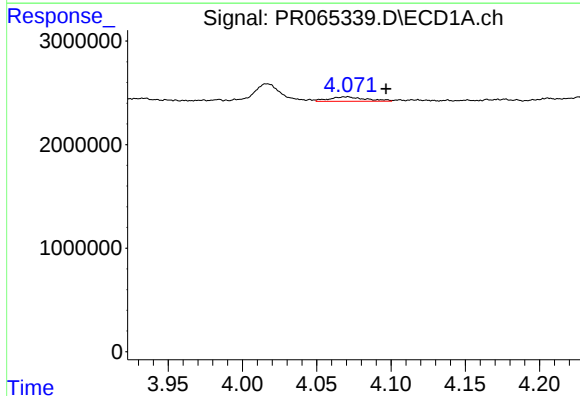


#10 AR-1221-3

R.T.: 4.070 min
Delta R.T.: -0.026 min
Response: 725346
Conc: 4.72 ng/ml

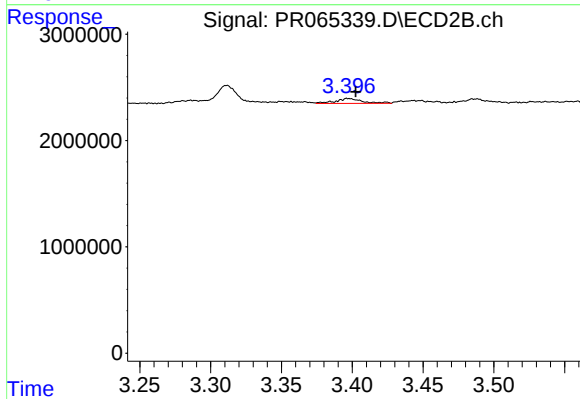

#10 AR-1221-3


R.T.: 3.397 min
Delta R.T.: -0.005 min
Response: 612152
Conc: 4.43 ng/ml

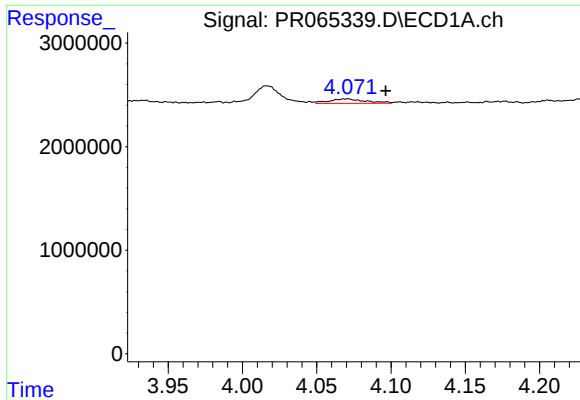

#11 AR-1232-1


R.T.: 4.070 min
Delta R.T.: -0.026 min
Response: 725346
Conc: 5.37 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

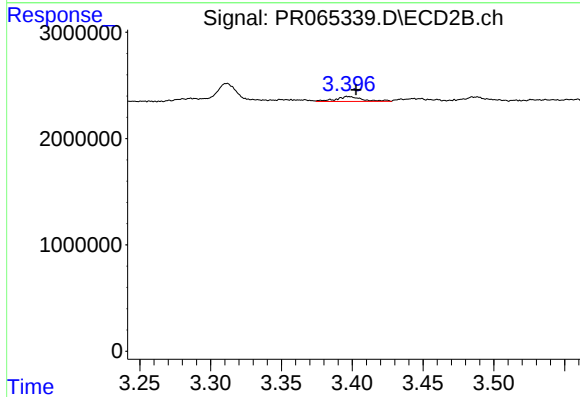


#11 AR-1232-1

R.T.: 3.397 min
Delta R.T.: -0.005 min
Response: 612152
Conc: 5.11 ng/ml

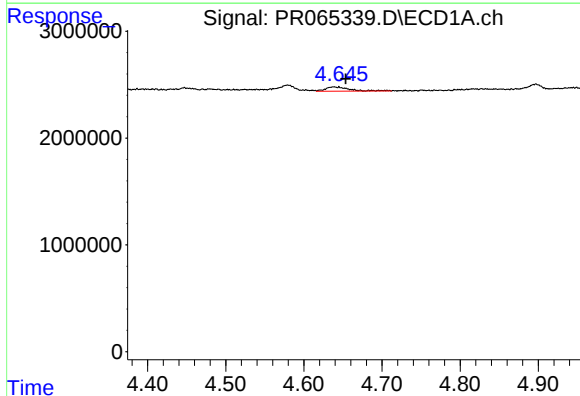


#12 AR-1232-2

R.T.: 4.639 min
Delta R.T.: -0.015 min
Response: 876769
Conc: 11.38 ng/ml

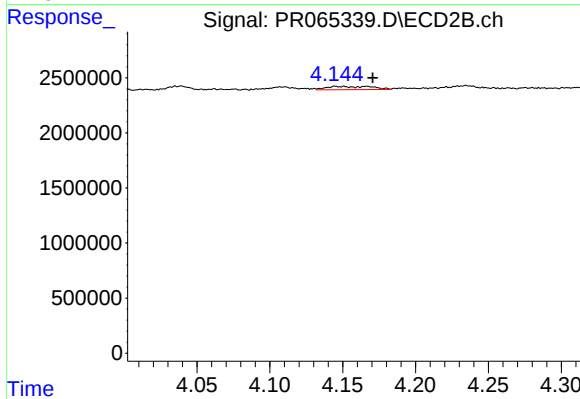

#12 AR-1232-2


R.T.: 4.151 min
Delta R.T.: -0.020 min
Response: 634663
Conc: 5.19 ng/ml

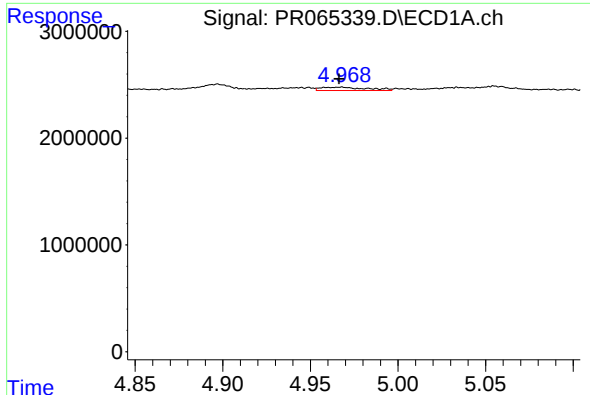

#13 AR-1232-3


R.T.: 4.967 min
Delta R.T.: 0.001 min
Response: 571105
Conc: 4.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

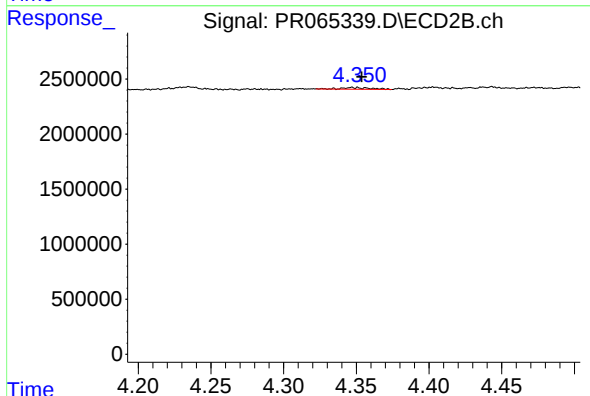


#13 AR-1232-3

R.T.: 4.347 min
Delta R.T.: -0.007 min
Response: 226353
Conc: 3.40 ng/ml

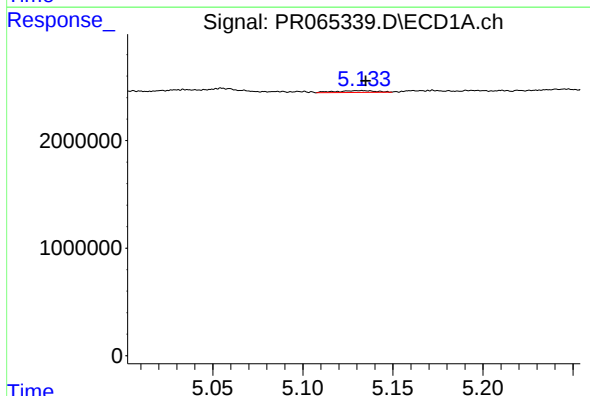


#14 AR-1232-4

R.T.: 5.132 min
Delta R.T.: -0.003 min
Response: 256603
Conc: 3.91 ng/ml

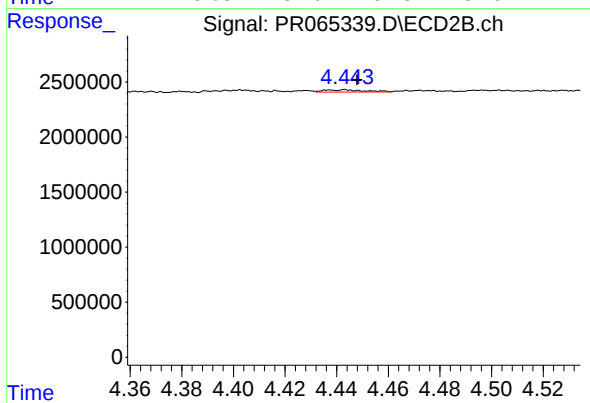

#14 AR-1232-4


R.T.: 4.444 min
Delta R.T.: -0.004 min
Response: 234295
Conc: 4.09 ng/ml

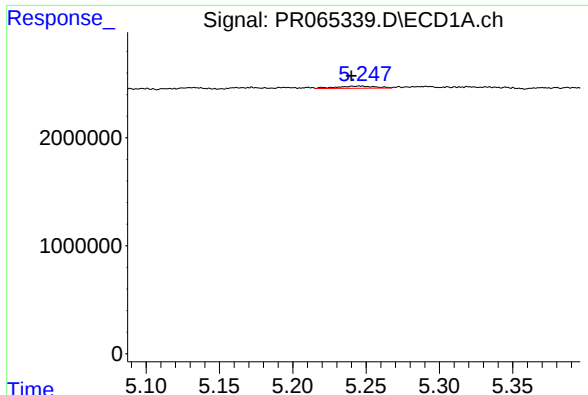

#15 AR-1232-5


R.T.: 5.246 min
Delta R.T.: 0.006 min
Response: 365461
Conc: 7.56 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

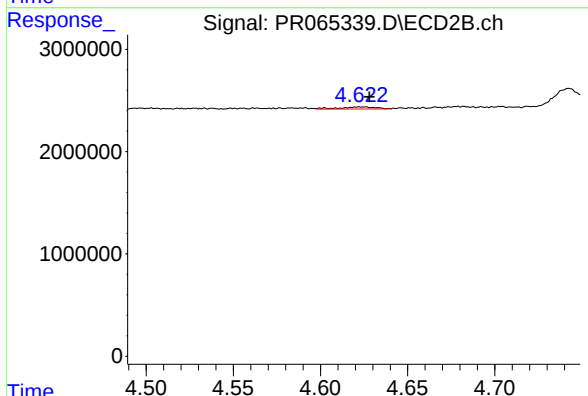


#15 AR-1232-5

R.T.: 4.623 min
Delta R.T.: -0.005 min
Response: 284745
Conc: 4.47 ng/ml

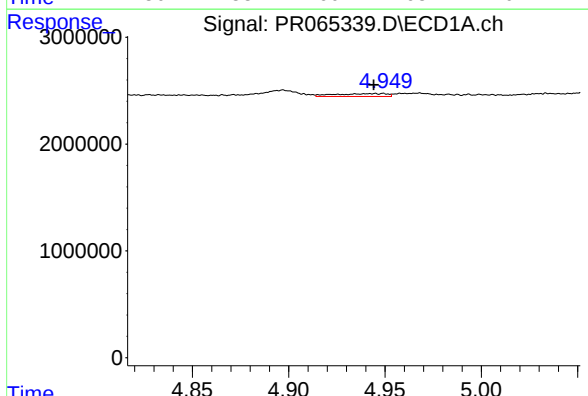


#16 AR-1242-1

R.T.: 4.949 min
Delta R.T.: 0.005 min
Response: 500494
Conc: 3.50 ng/ml

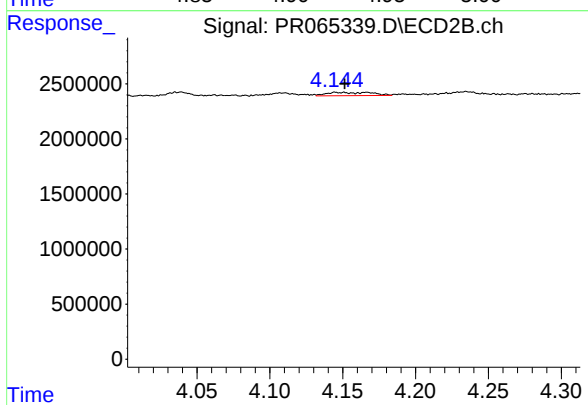

#16 AR-1242-1


R.T.: 4.151 min
Delta R.T.: 0.000 min
Response: 634663
Conc: 4.34 ng/ml

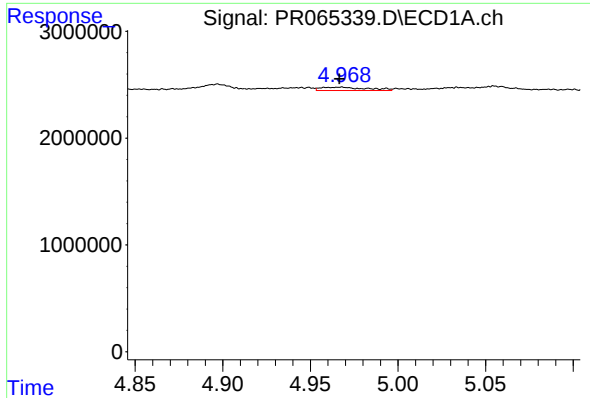

#17 AR-1242-2


R.T.: 4.967 min
Delta R.T.: 0.000 min
Response: 571105
Conc: 2.71 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

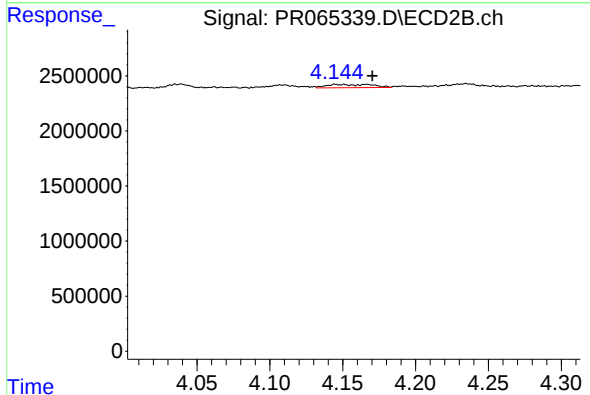


#17 AR-1242-2

R.T.: 4.151 min
Delta R.T.: -0.020 min
Response: 634663
Conc: 3.18 ng/ml

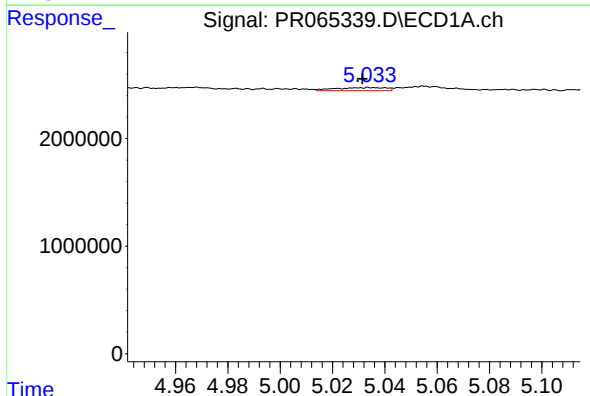


#18 AR-1242-3

R.T.: 5.035 min
Delta R.T.: 0.003 min
Response: 388316
Conc: 2.87 ng/ml

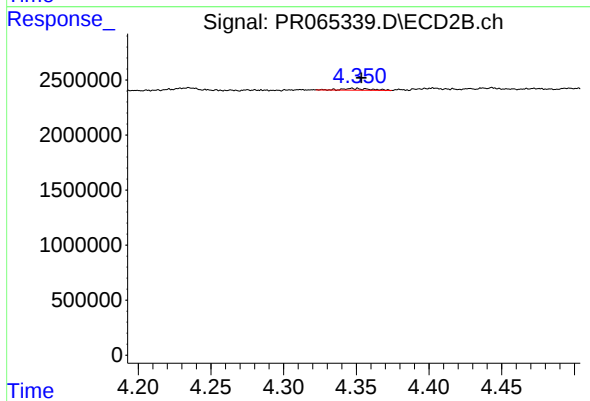

#18 AR-1242-3


R.T.: 4.347 min
Delta R.T.: -0.006 min
Response: 226353
Conc: 2.07 ng/ml

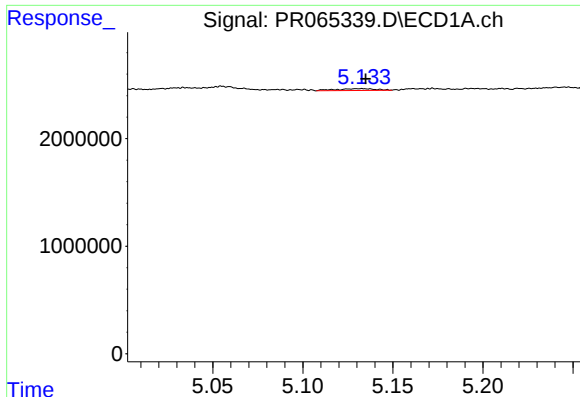

#19 AR-1242-4


R.T.: 5.132 min
Delta R.T.: -0.003 min
Response: 256603
Conc: 2.36 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

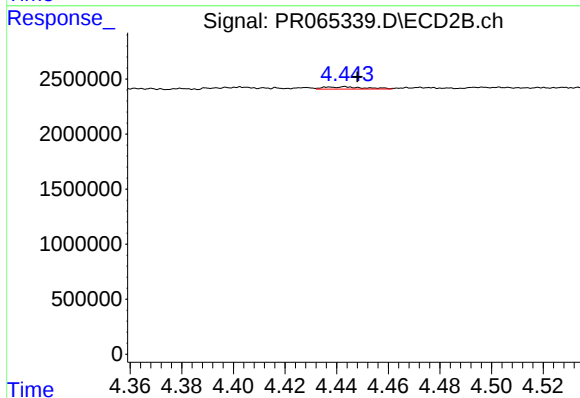


#19 AR-1242-4

R.T.: 4.444 min
Delta R.T.: -0.005 min
Response: 234295
Conc: 2.23 ng/ml

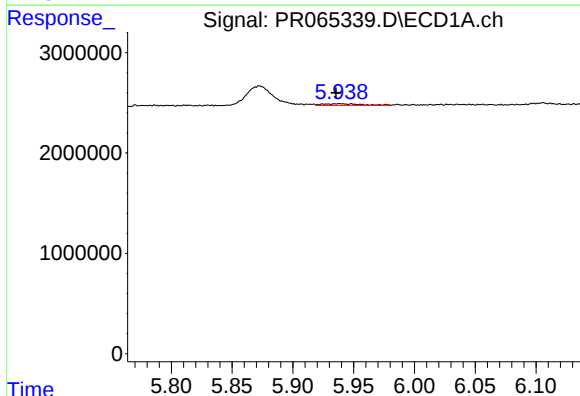


#20 AR-1242-5

R.T.: 5.938 min
Delta R.T.: 0.003 min
Response: 352655
Conc: 3.12 ng/ml

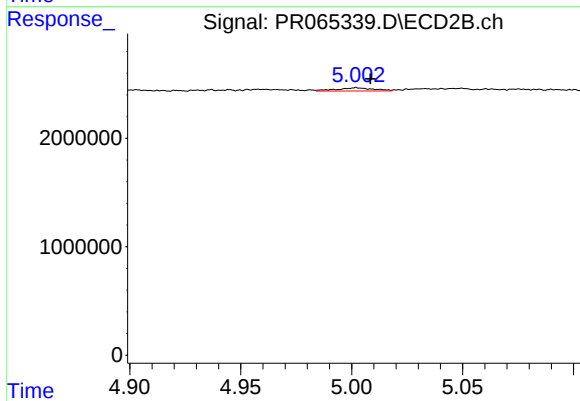

#20 AR-1242-5


R.T.: 5.002 min
Delta R.T.: -0.006 min
Response: 335092
Conc: 2.48 ng/ml

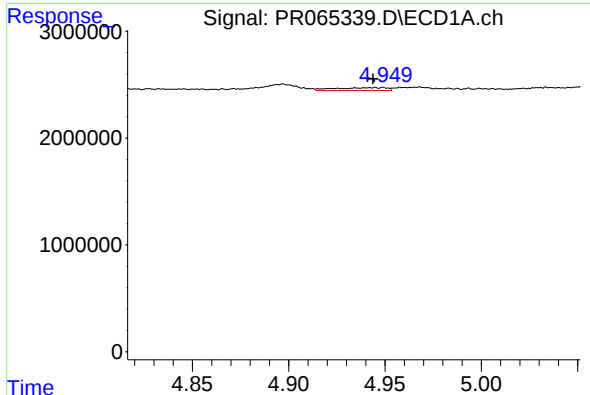

#21 AR-1248-1


R.T.: 4.949 min
Delta R.T.: 0.005 min
Response: 500494
Conc: 4.70 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

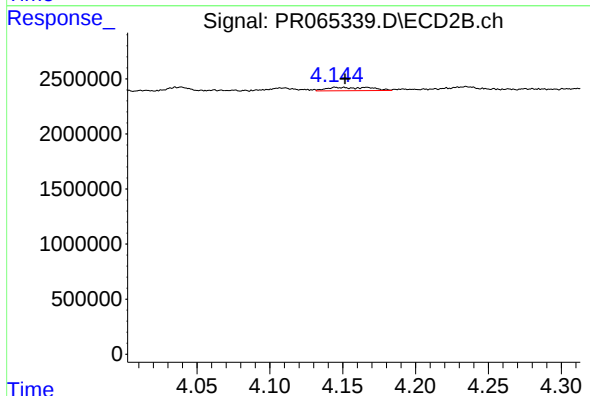


#21 AR-1248-1

R.T.: 4.151 min
Delta R.T.: 0.000 min
Response: 634663
Conc: 5.88 ng/ml

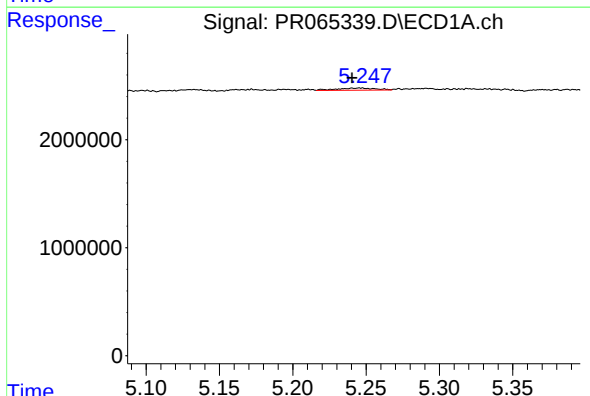


#22 AR-1248-2

R.T.: 5.246 min
Delta R.T.: 0.006 min
Response: 365461
Conc: 2.35 ng/ml

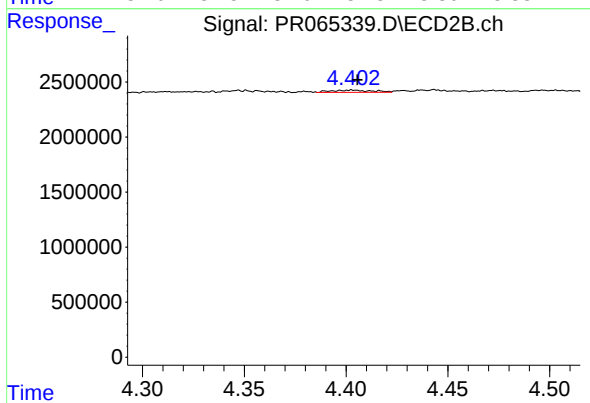

#22 AR-1248-2


R.T.: 4.403 min
Delta R.T.: -0.003 min
Response: 279559
Conc: 1.93 ng/ml

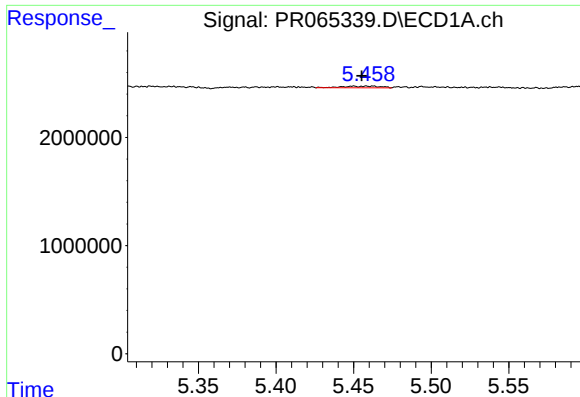

#23 AR-1248-3


R.T.: 5.450 min
Delta R.T.: -0.005 min
Response: 253368
Conc: 1.42 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

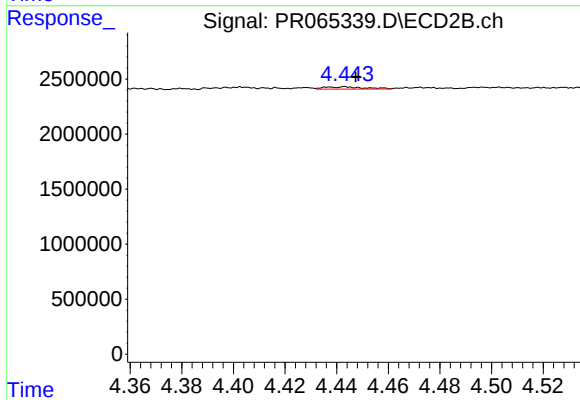


#23 AR-1248-3

R.T.: 4.444 min
Delta R.T.: -0.004 min
Response: 234295
Conc: 1.51 ng/ml

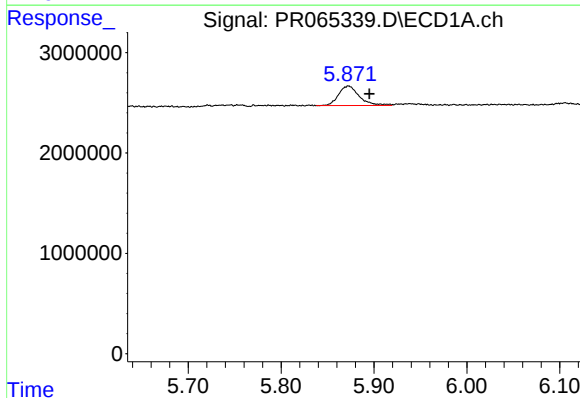


#24 AR-1248-4

R.T.: 5.873 min
Delta R.T.: -0.022 min
Response: 3014767
Conc: 15.90 ng/ml

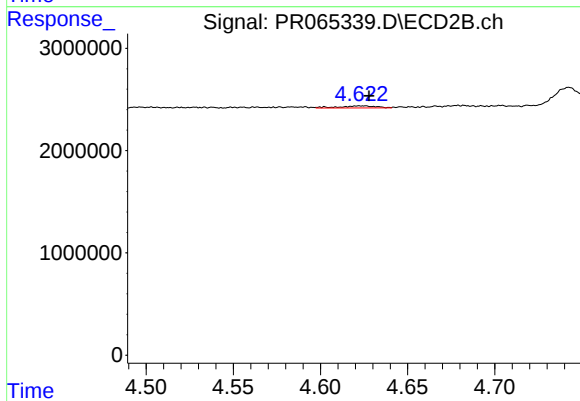

#24 AR-1248-4


R.T.: 4.623 min
Delta R.T.: -0.005 min
Response: 284745
Conc: 1.52 ng/ml

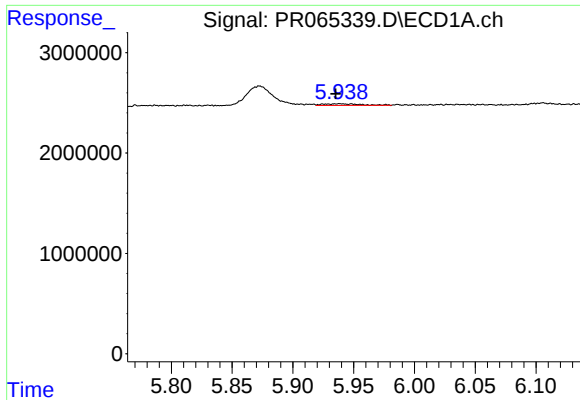

#25 AR-1248-5


R.T.: 5.938 min
Delta R.T.: 0.003 min
Response: 352655
Conc: 1.85 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

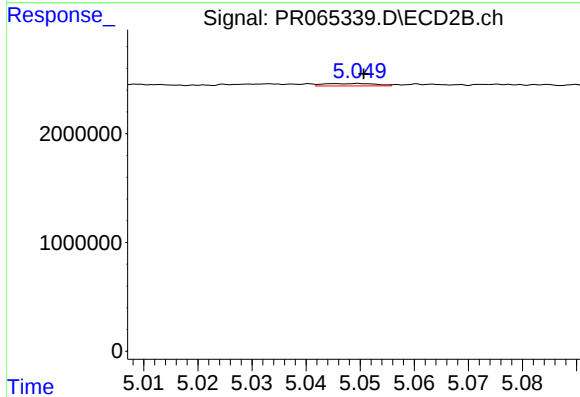


#25 AR-1248-5

R.T.: 5.049 min
Delta R.T.: -0.001 min
Response: 149904
Conc: 0.81 ng/ml

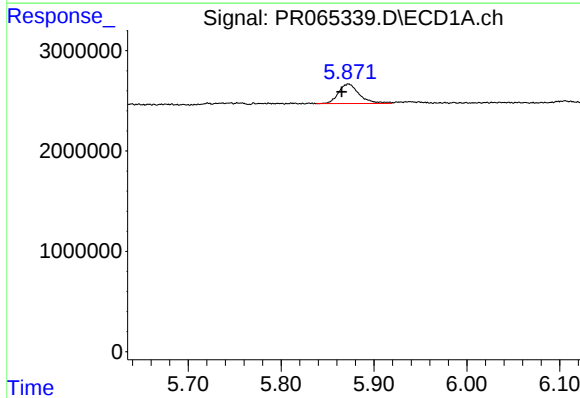


#26 AR-1254-1

R.T.: 5.873 min
Delta R.T.: 0.007 min
Response: 3014767
Conc: 14.72 ng/ml

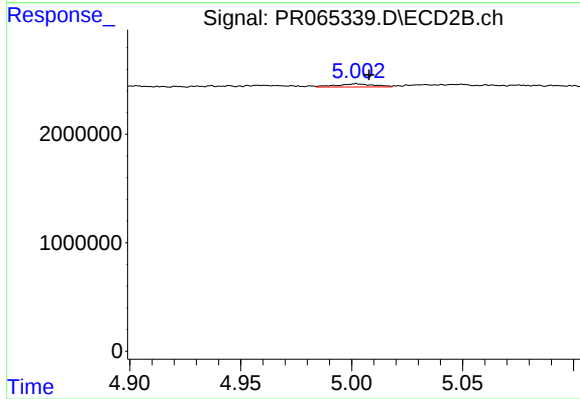

#26 AR-1254-1


R.T.: 5.002 min
Delta R.T.: -0.005 min
Response: 335092
Conc: 1.15 ng/ml

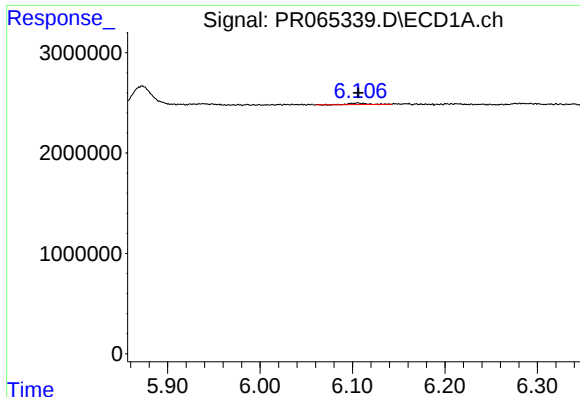

#27 AR-1254-2


R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 183725
Conc: 0.59 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

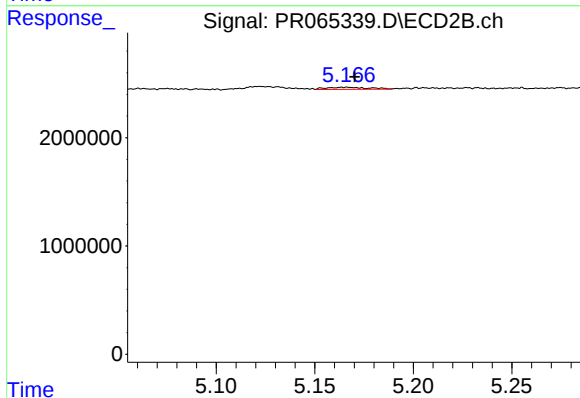


#27 AR-1254-2

R.T.: 5.165 min
Delta R.T.: -0.005 min
Response: 279289
Conc: 1.10 ng/ml

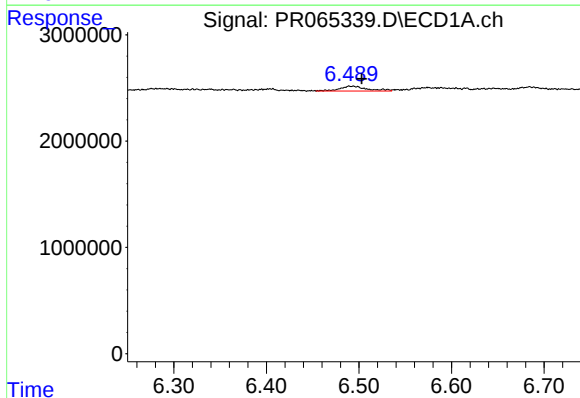


#28 AR-1254-3

R.T.: 6.494 min
Delta R.T.: -0.009 min
Response: 944852
Conc: 2.95 ng/ml

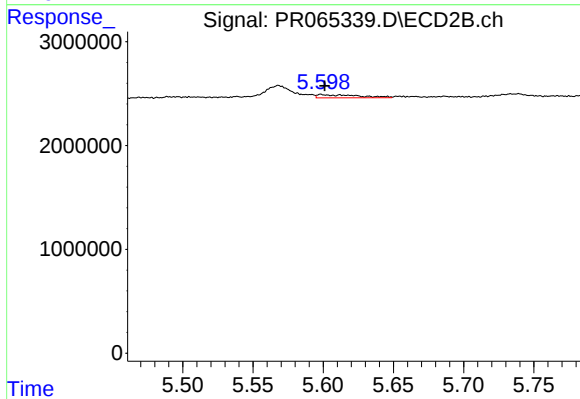

#28 AR-1254-3


R.T.: 5.599 min
Delta R.T.: -0.002 min
Response: 638008
Conc: 1.56 ng/ml

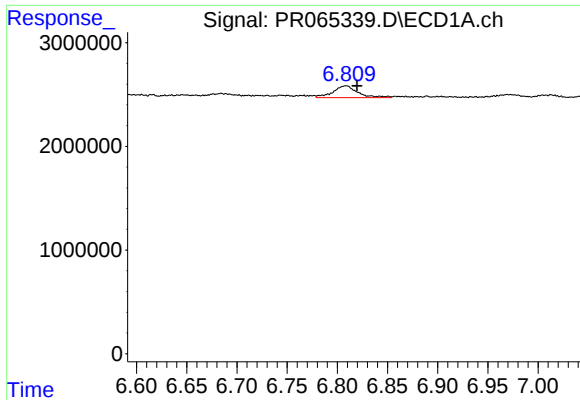

#29 AR-1254-4


R.T.: 6.809 min
Delta R.T.: -0.011 min
Response: 1946439
Conc: 8.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

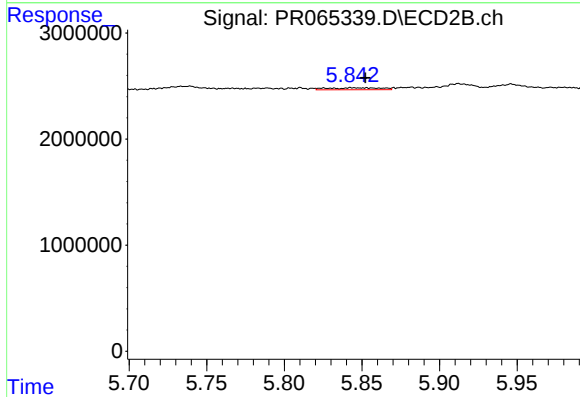


#29 AR-1254-4

R.T.: 5.843 min
Delta R.T.: -0.009 min
Response: 442552
Conc: 1.72 ng/ml

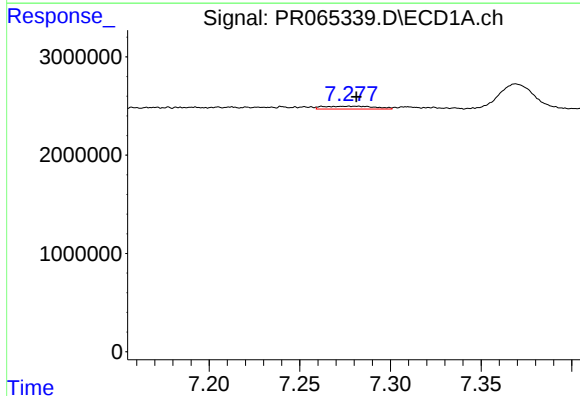


#30 AR-1254-5

R.T.: 7.278 min
Delta R.T.: -0.004 min
Response: 559520
Conc: 2.25 ng/ml

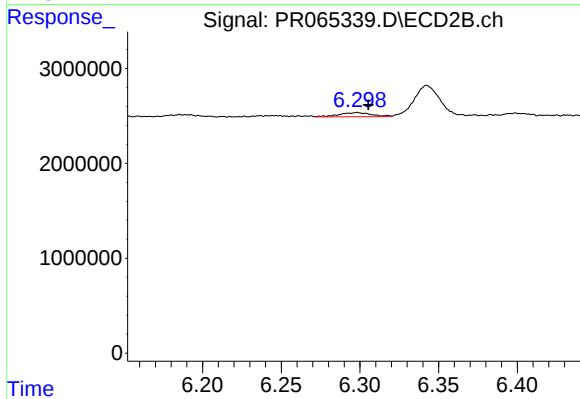

#30 AR-1254-5


R.T.: 6.298 min
Delta R.T.: -0.007 min
Response: 626812
Conc: 1.71 ng/ml

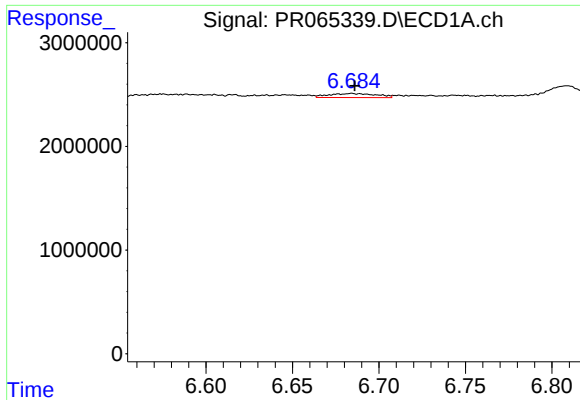

#31 AR-1260-1


R.T.: 6.684 min
Delta R.T.: -0.002 min
Response: 747283
Conc: 2.97 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

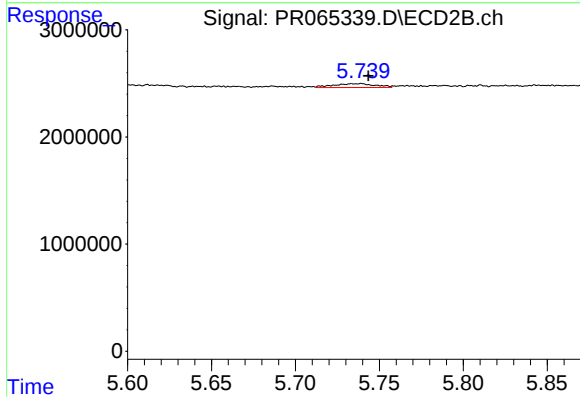


#31 AR-1260-1

R.T.: 5.739 min
Delta R.T.: -0.005 min
Response: 622576
Conc: 2.18 ng/ml

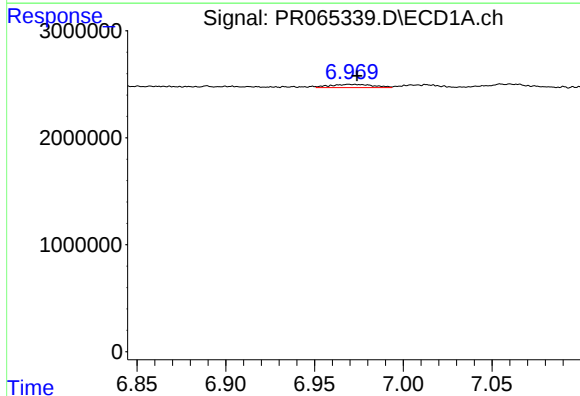


#32 AR-1260-2

R.T.: 6.970 min
Delta R.T.: -0.004 min
Response: 504506
Conc: 1.76 ng/ml

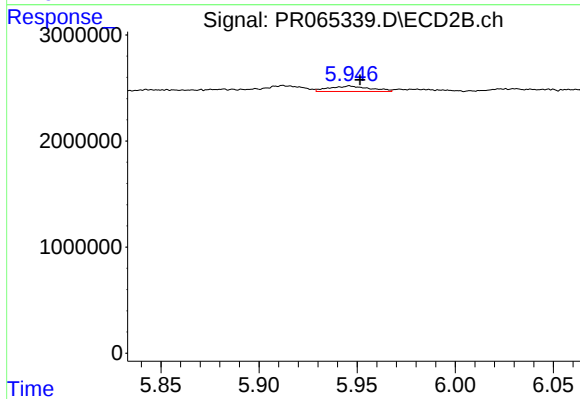

#32 AR-1260-2


R.T.: 5.946 min
Delta R.T.: -0.005 min
Response: 739331
Conc: 2.13 ng/ml

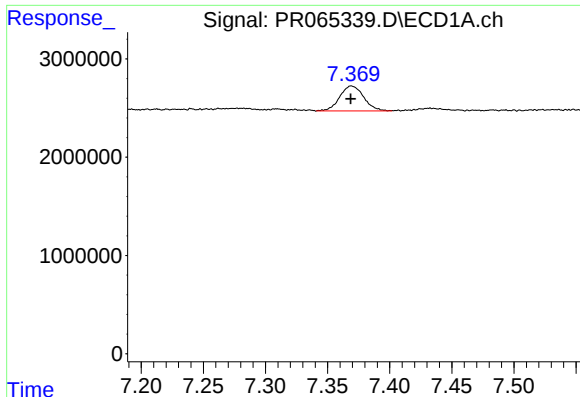

#33 AR-1260-3


R.T.: 7.369 min
Delta R.T.: 0.000 min
Response: 3430669
Conc: 16.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

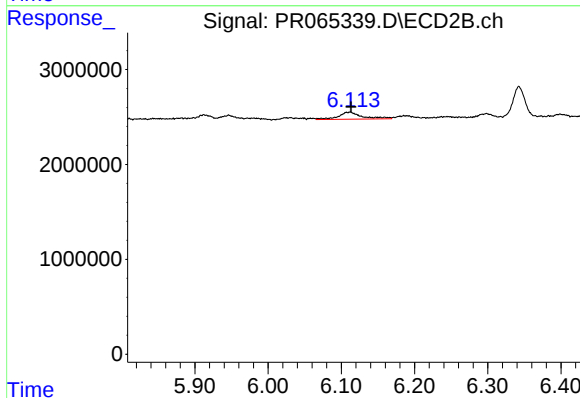


#33 AR-1260-3

R.T.: 6.112 min
Delta R.T.: -0.002 min
Response: 1666951
Conc: 5.13 ng/ml

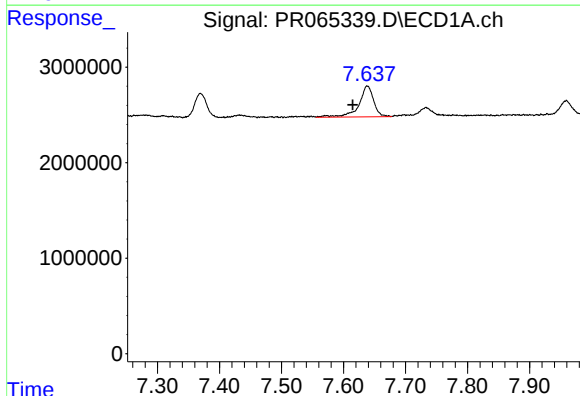


#34 AR-1260-4

R.T.: 7.638 min
Delta R.T.: 0.024 min
Response: 5366923
Conc: 22.74 ng/ml

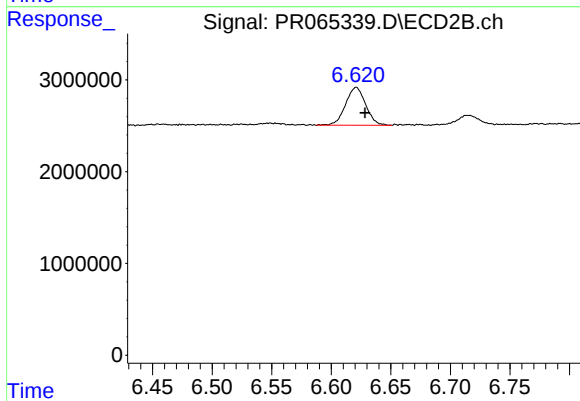

#34 AR-1260-4


R.T.: 6.621 min
Delta R.T.: -0.007 min
Response: 4844498
Conc: 18.34 ng/ml

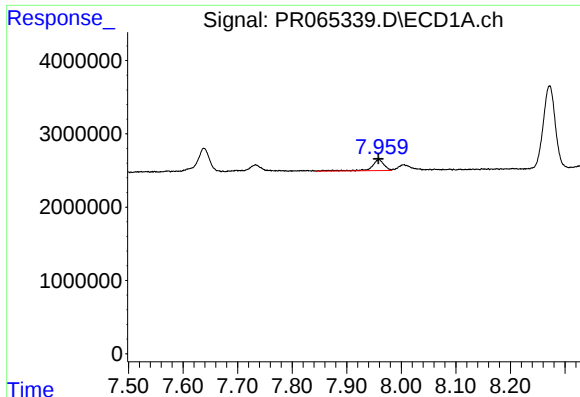

#35 AR-1260-5


R.T.: 7.959 min
Delta R.T.: 0.000 min
Response: 2391648
Conc: 5.44 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

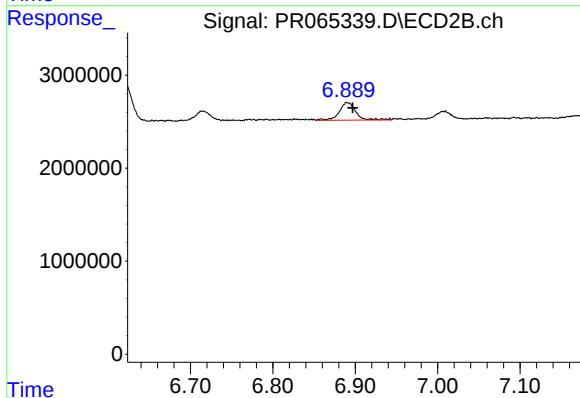


#35 AR-1260-5

R.T.: 6.890 min
Delta R.T.: -0.006 min
Response: 2632914
Conc: 4.27 ng/ml

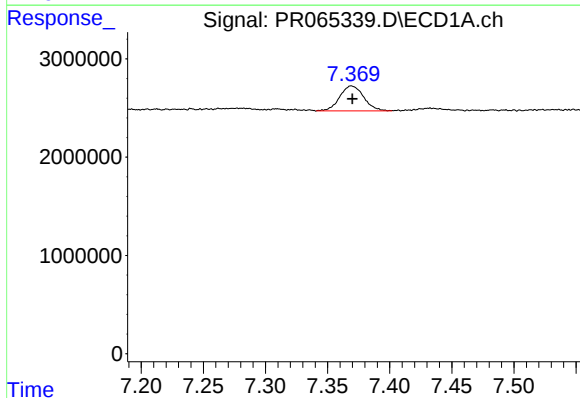


#36 AR-1262-1

R.T.: 7.369 min
Delta R.T.: 0.000 min
Response: 3430669
Conc: 10.14 ng/ml

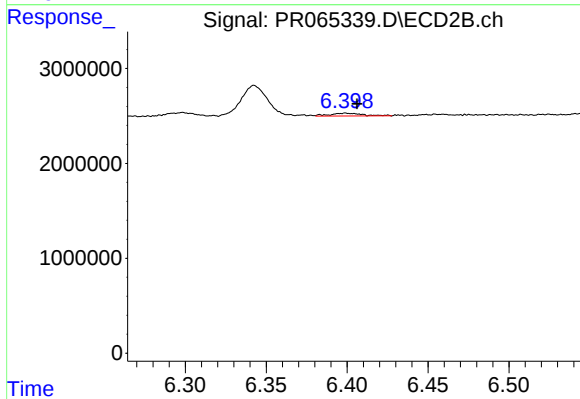

#36 AR-1262-1


R.T.: 6.399 min
Delta R.T.: -0.007 min
Response: 406054
Conc: 2.26 ng/ml

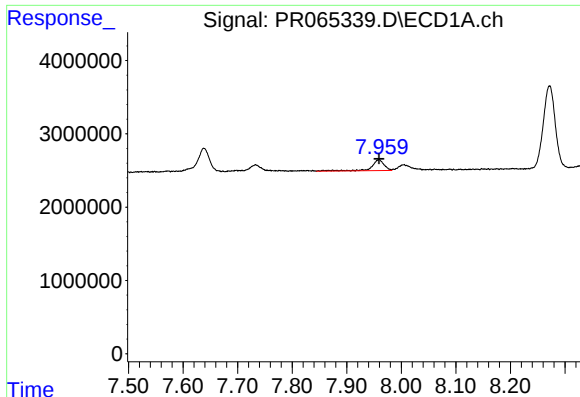

#37 AR-1262-2


R.T.: 7.959 min
Delta R.T.: 0.000 min
Response: 2391648
Conc: 4.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

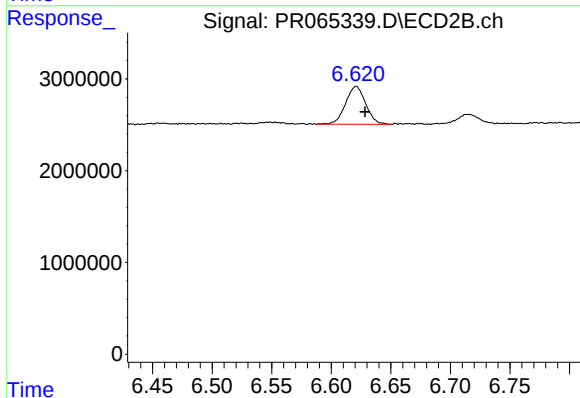


#37 AR-1262-2

R.T.: 6.621 min
Delta R.T.: -0.007 min
Response: 4844498
Conc: 12.45 ng/ml

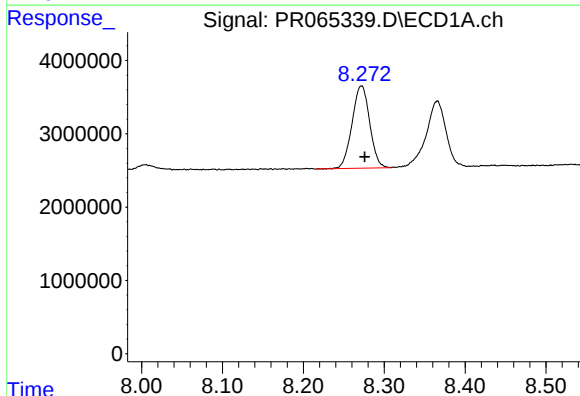


#38 AR-1262-3

R.T.: 8.272 min
Delta R.T.: -0.004 min
Response: 17044500
Conc: 44.79 ng/ml

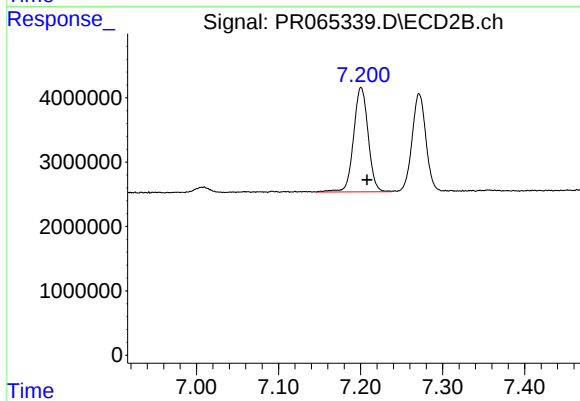

#38 AR-1262-3


R.T.: 7.201 min
Delta R.T.: -0.007 min
Response: 20002814
Conc: 70.57 ng/ml

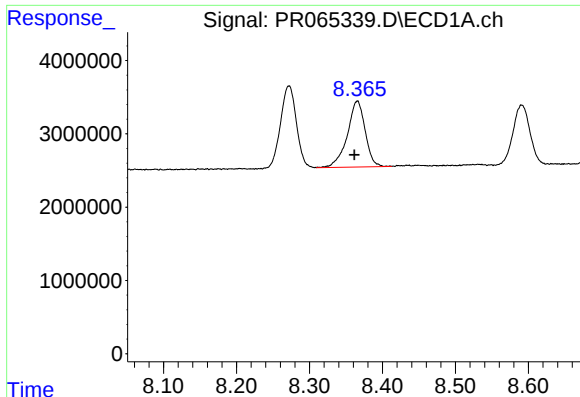

#39 AR-1262-4


R.T.: 8.365 min
Delta R.T.: 0.004 min
Response: 15335126
Conc: 52.35 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

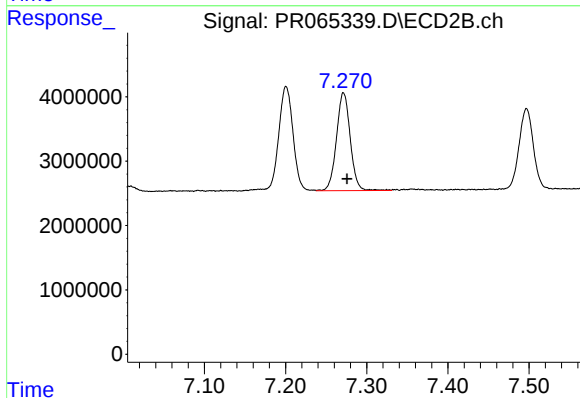


#39 AR-1262-4

R.T.: 7.271 min
Delta R.T.: -0.004 min
Response: 17961208
Conc: 31.19 ng/ml

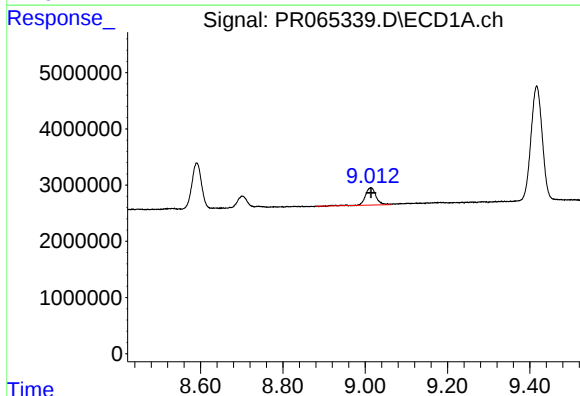


#40 AR-1262-5

R.T.: 9.014 min
Delta R.T.: 0.000 min
Response: 5567895
Conc: 27.78 ng/ml

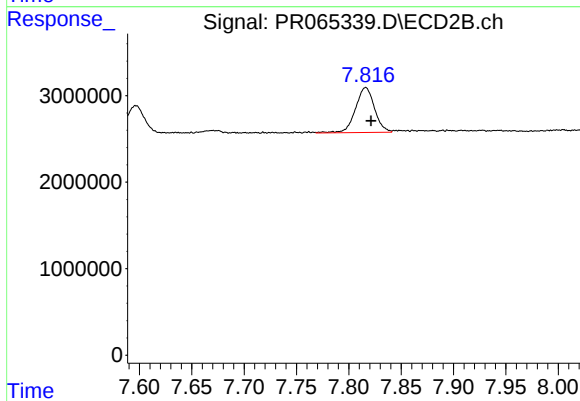

#40 AR-1262-5


R.T.: 7.816 min
Delta R.T.: -0.005 min
Response: 6576264
Conc: 25.27 ng/ml

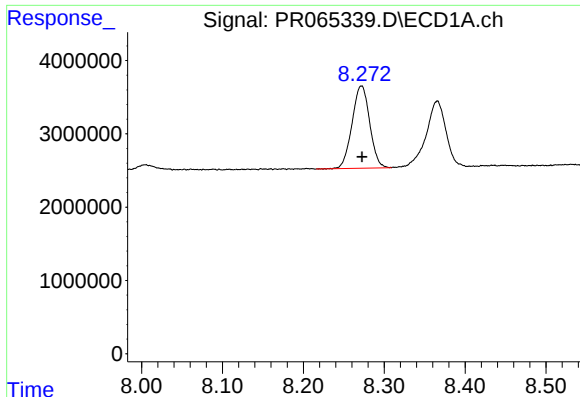

#41 AR-1268-1


R.T.: 8.272 min
Delta R.T.: -0.001 min
Response: 17044500
Conc: 28.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

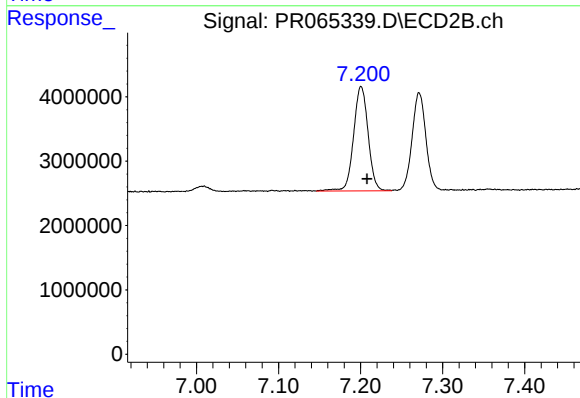


#41 AR-1268-1

R.T.: 7.201 min
Delta R.T.: -0.007 min
Response: 20002814
Conc: 25.21 ng/ml

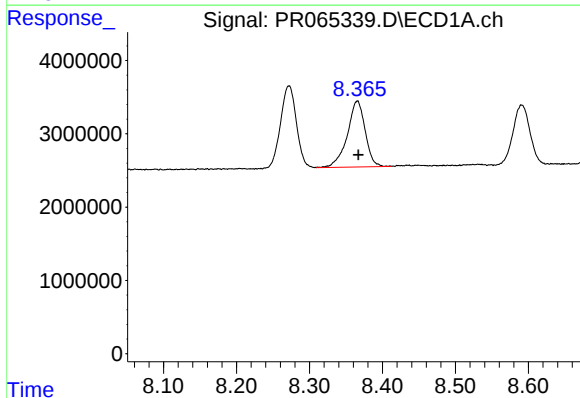


#42 AR-1268-2

R.T.: 8.365 min
Delta R.T.: -0.001 min
Response: 15335126
Conc: 28.03 ng/ml

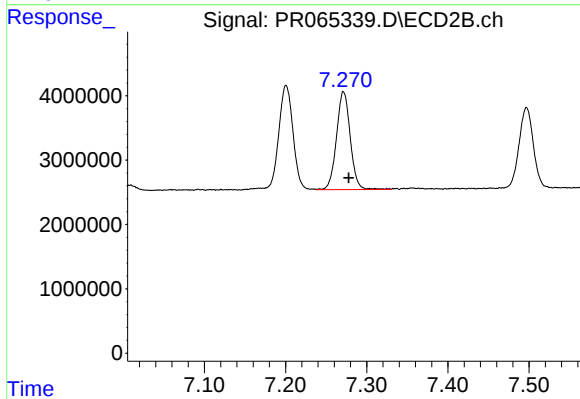

#42 AR-1268-2


R.T.: 7.271 min
Delta R.T.: -0.006 min
Response: 17961208
Conc: 24.13 ng/ml

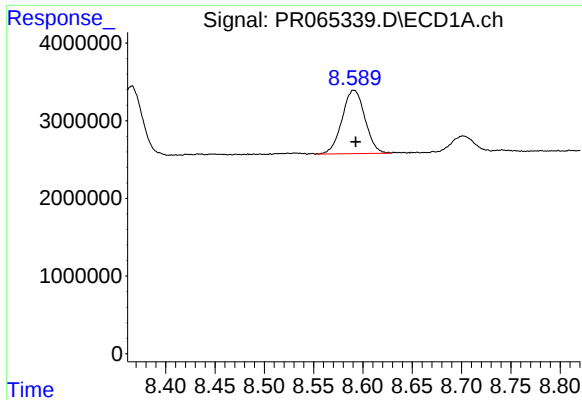

#43 AR-1268-3


R.T.: 8.591 min
Delta R.T.: -0.002 min
Response: 13145963
Conc: 27.71 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

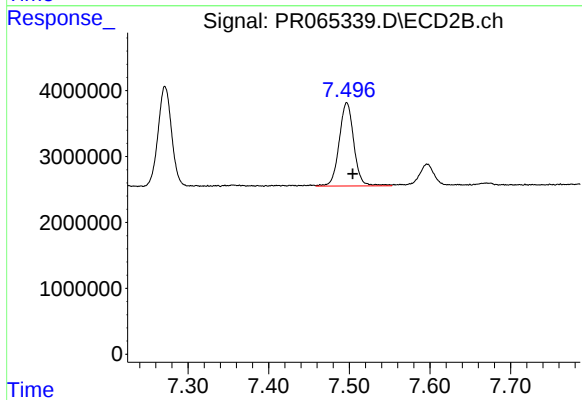


#43 AR-1268-3

R.T.: 7.497 min
Delta R.T.: -0.007 min
Response: 15970350
Conc: 25.21 ng/ml

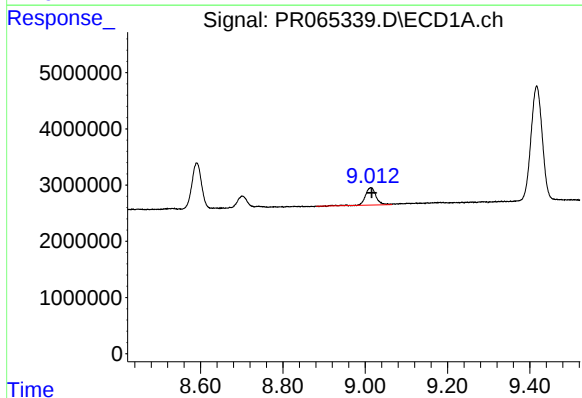


#44 AR-1268-4

R.T.: 9.014 min
Delta R.T.: -0.002 min
Response: 5567895
Conc: 27.36 ng/ml

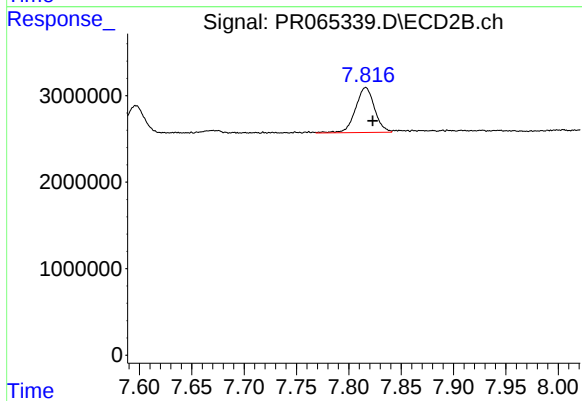

#44 AR-1268-4


R.T.: 7.816 min
Delta R.T.: -0.007 min
Response: 6576264
Conc: 25.07 ng/ml

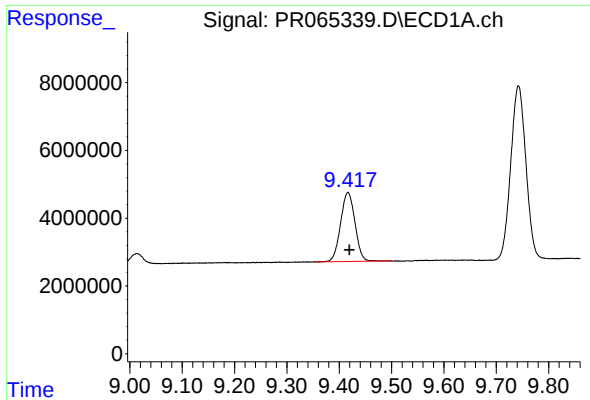

#45 AR-1268-5

R.T.: 9.417 min
Delta R.T.: -0.003 min
Response: 38788236
Conc: 26.61 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2024

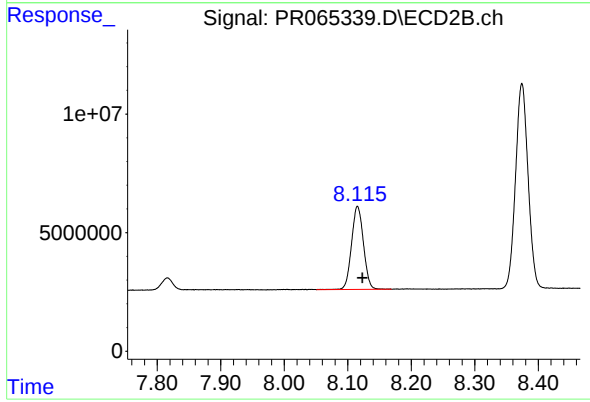

#45 AR-1268-5

R.T.: 8.116 min
Delta R.T.: -0.008 min
Response: 45655738
Conc: 23.85 ng/ml