

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR020522\
 Data File : PR053379.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 14:56
 Operator : AJ\MA
 Sample : N1323-13
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 23:24:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011022CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 11 05:43:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
28)	L6	AR-1254-3	7.332	0.000	250211	0	1.215 N.D. #
30)	L6	AR-1254-5	8.072f	6.957f	2777129	685786	16.362 3.202 #
31)	L7	AR-1260-1	7.462	0.000	45532	0	0.329 N.D. #
32)	L7	AR-1260-2	7.718	0.000	284460	0	1.712 N.D. #
33)	L7	AR-1260-3	8.072	0.000	2777129	0	21.632 N.D. #
36)	L8	AR-1262-1	8.072	6.957f	2777129	685786	13.134 5.768 #
38)	L8	AR-1262-3	9.013	0.000	460111	0	2.677 N.D. #
39)	L8	AR-1262-4	9.013f	0.000	460111	0	4.109 N.D. #
41)	L9	AR-1268-1	9.013	0.000	460111	0	1.052 N.D. #
43)	L9	AR-1268-3	9.263f	0.000	944990	0	2.736 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR020522\
Data File : PR053379.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 14:56
Operator : AJ\MA
Sample : N1323-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 23:24:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011022CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 11 05:43:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

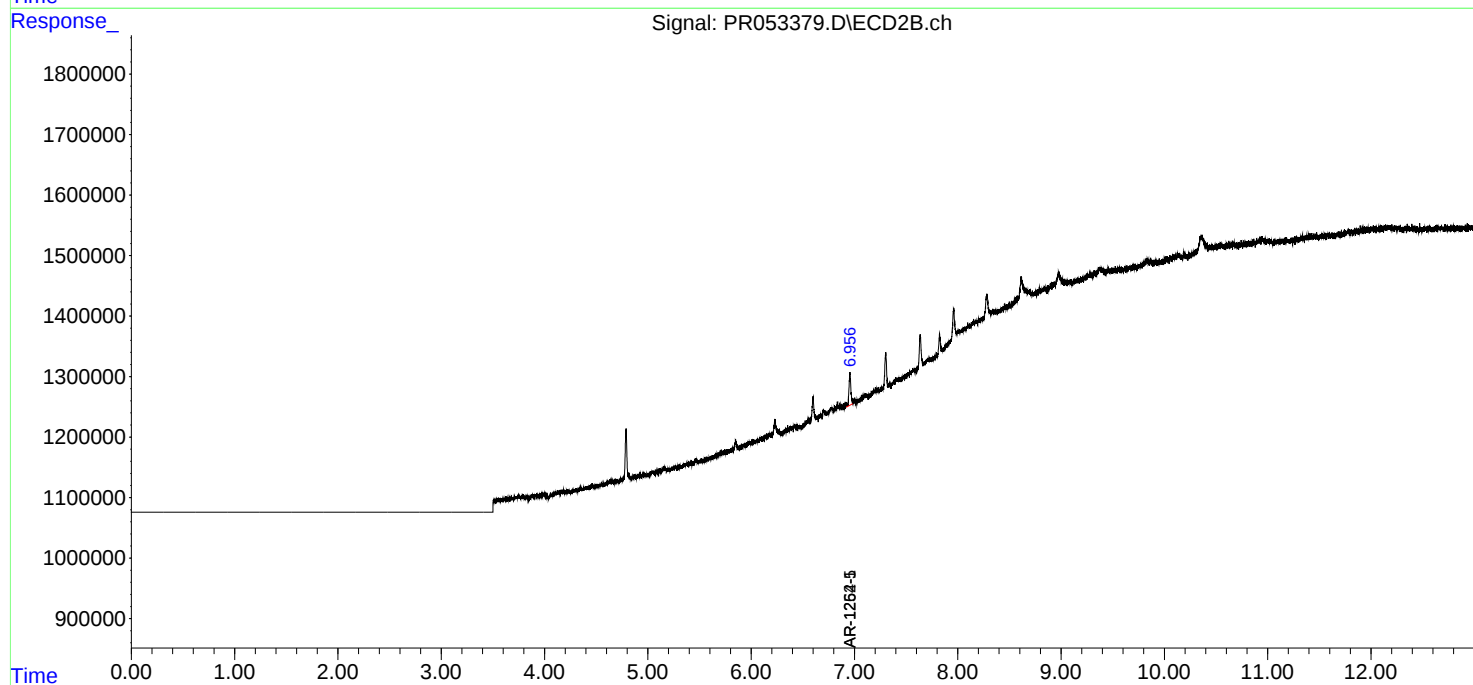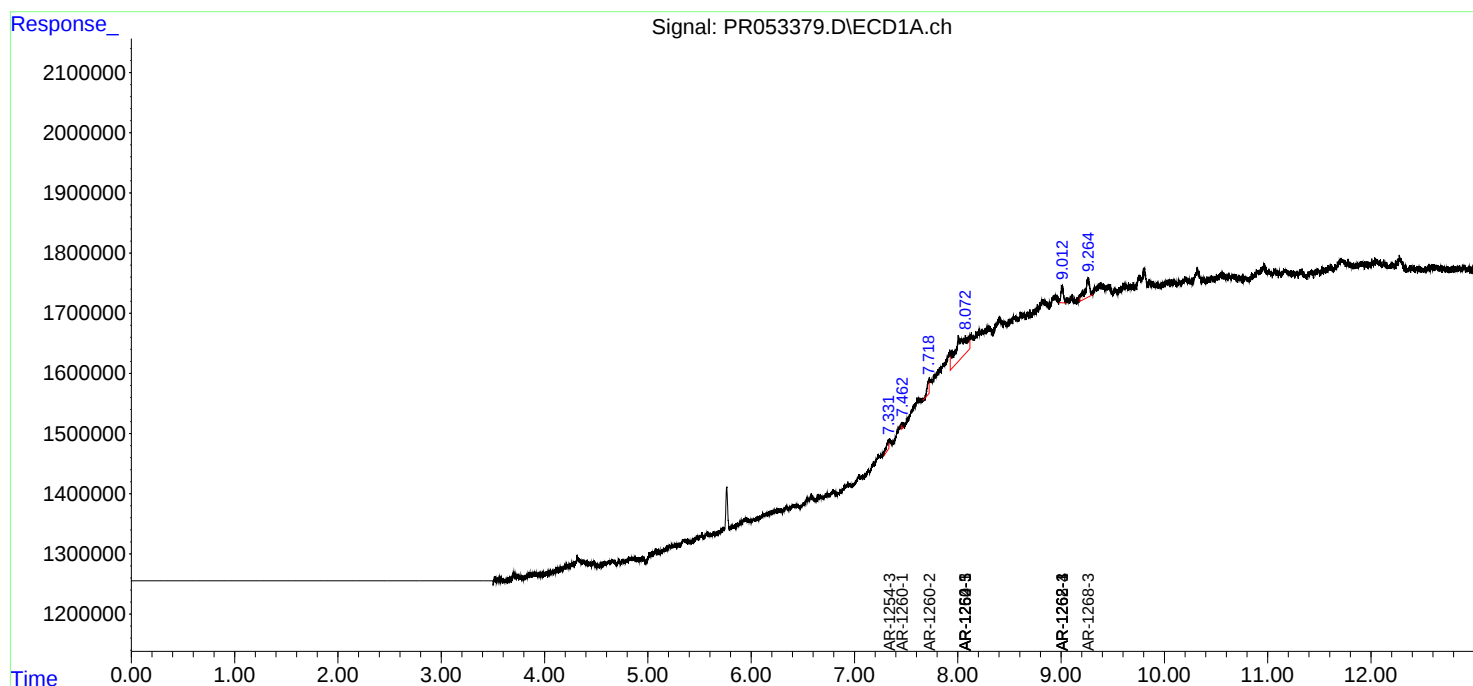


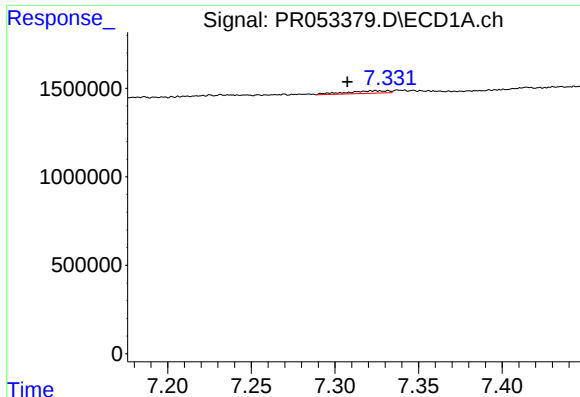

#28 AR-1254-3


R.T.: 7.332 min
Delta R.T.: 0.024 min
Response: 250211
Conc: 1.22 ng/ml

Instrument :
ECD_R
ClientSampleId :

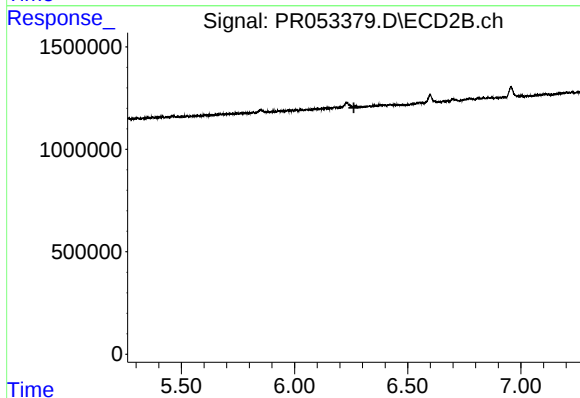


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.262 min
Response: 0
Conc: N.D.

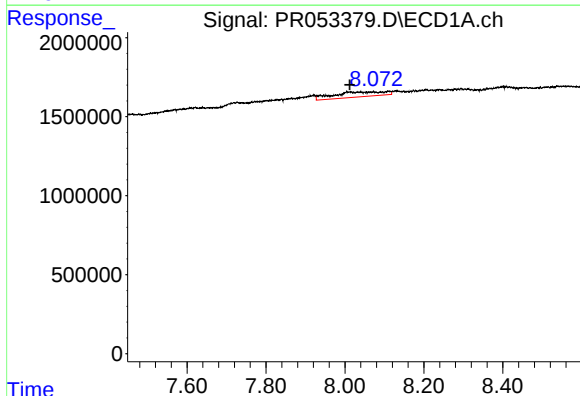


#30 AR-1254-5

R.T.: 8.072 min
Delta R.T.: 0.060 min
Response: 2777129
Conc: 16.36 ng/ml

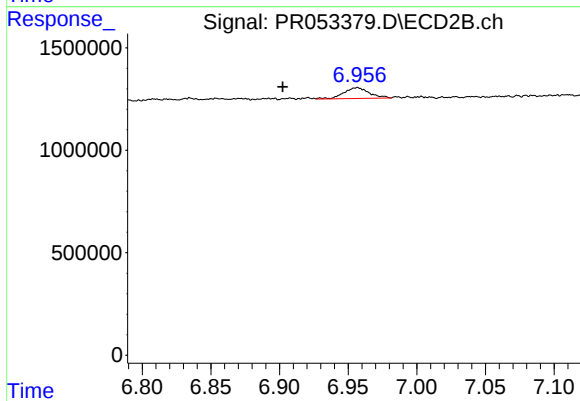

#30 AR-1254-5


R.T.: 6.957 min
Delta R.T.: 0.054 min
Response: 685786
Conc: 3.20 ng/ml

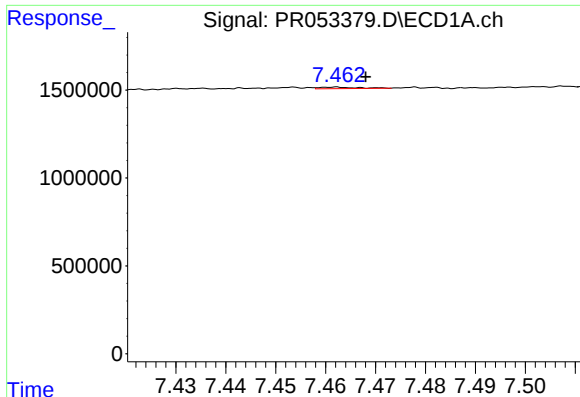

#31 AR-1260-1


R.T.: 7.462 min
Delta R.T.: -0.006 min
Response: 45532
Conc: 0.33 ng/ml

Instrument :
ECD_R
ClientSampleId :

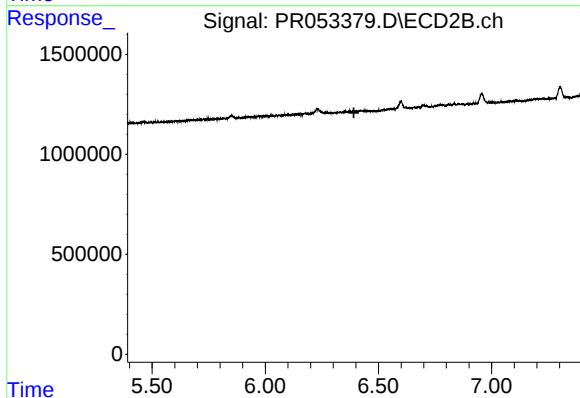


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.392 min
Response: 0
Conc: N.D.

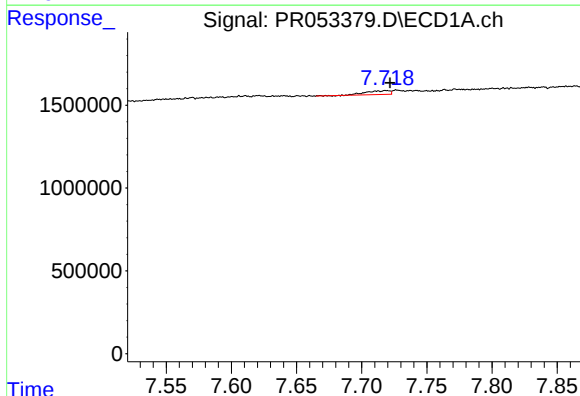


#32 AR-1260-2

R.T.: 7.718 min
Delta R.T.: -0.003 min
Response: 284460
Conc: 1.71 ng/ml

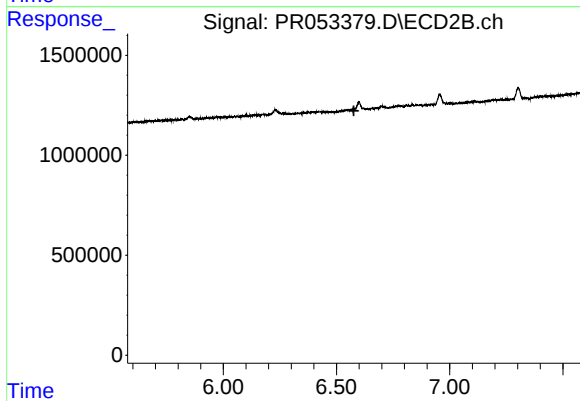

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.577 min
Response: 0
Conc: N.D.

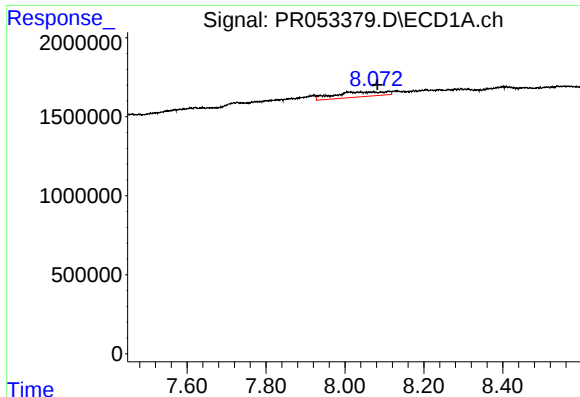

#33 AR-1260-3


R.T.: 8.072 min
Delta R.T.: -0.010 min
Response: 2777129
Conc: 21.63 ng/ml

Instrument :
ECD_R
ClientSampleId :

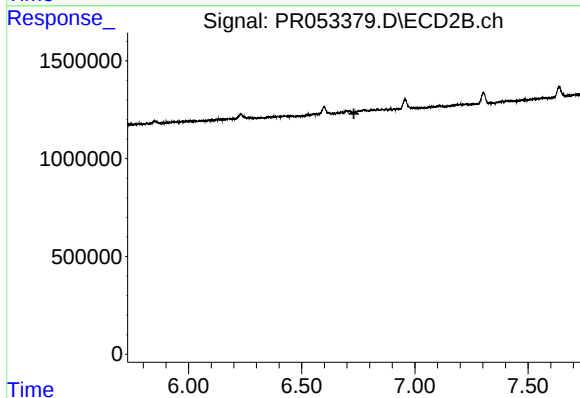


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.730 min
Response: 0
Conc: N.D.

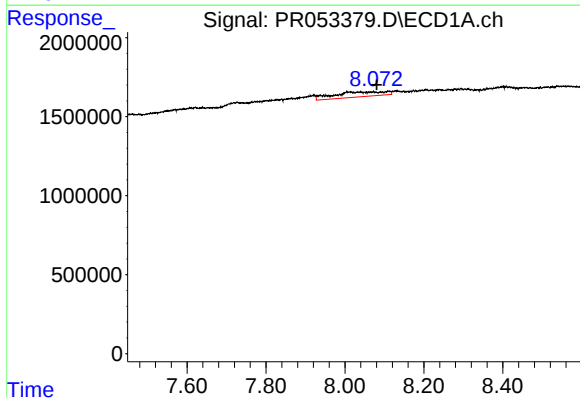


#36 AR-1262-1

R.T.: 8.072 min
Delta R.T.: -0.008 min
Response: 2777129
Conc: 13.13 ng/ml

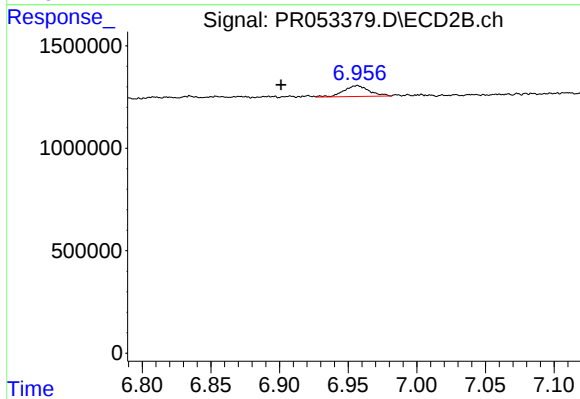

#36 AR-1262-1


R.T.: 6.957 min
Delta R.T.: 0.056 min
Response: 685786
Conc: 5.77 ng/ml

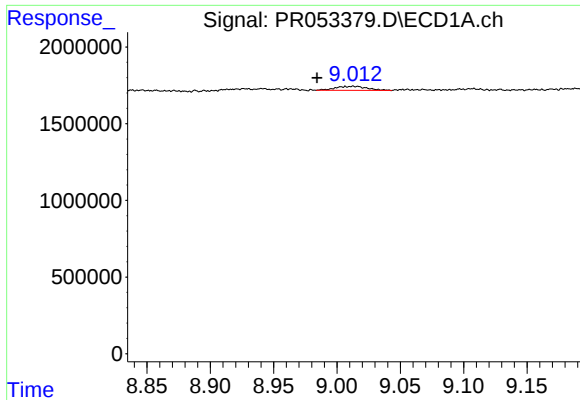

#38 AR-1262-3


R.T.: 9.013 min
Delta R.T.: 0.028 min
Response: 460111
Conc: 2.68 ng/ml

Instrument :
ECD_R
ClientSampleId :

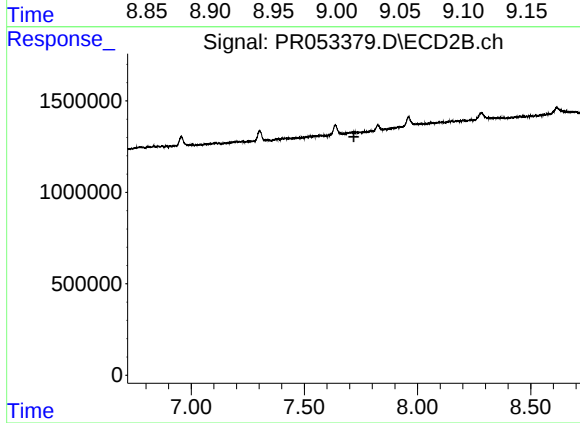


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 7.719 min
Response: 0
Conc: N.D.

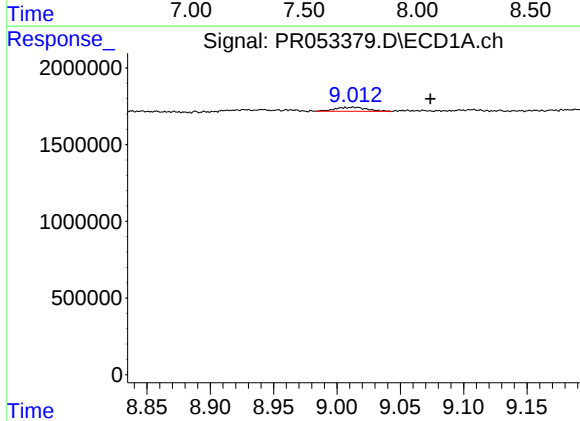


#39 AR-1262-4

R.T.: 9.013 min
Delta R.T.: -0.061 min
Response: 460111
Conc: 4.11 ng/ml

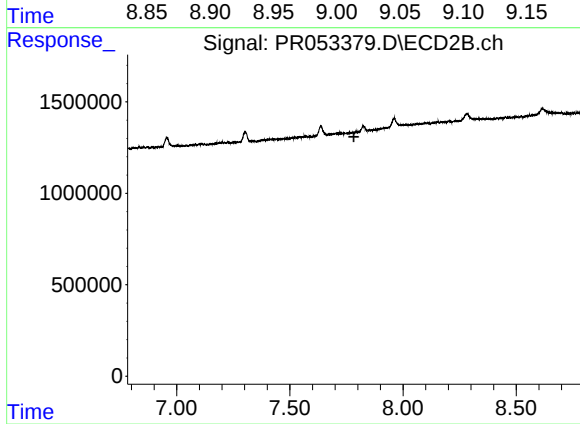

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 7.783 min
Response: 0
Conc: N.D.

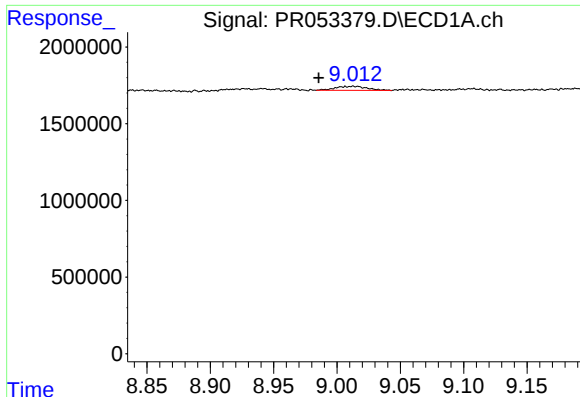

#41 AR-1268-1


R.T.: 9.013 min
Delta R.T.: 0.027 min
Response: 460111
Conc: 1.05 ng/ml

Instrument :
ECD_R
ClientSampleId :

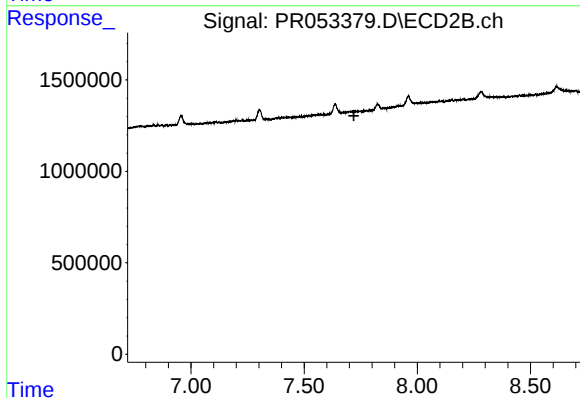


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.720 min
Response: 0
Conc: N.D.

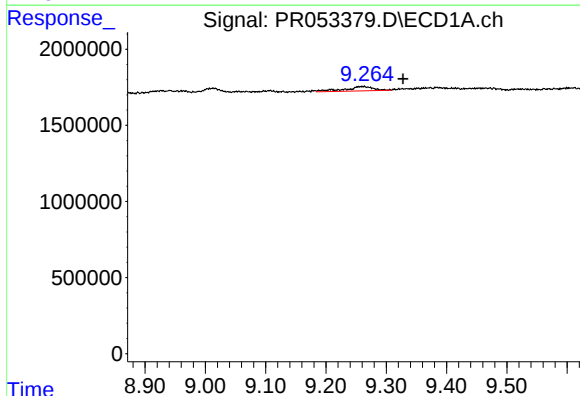

#43 AR-1268-3

R.T.: 9.263 min
Delta R.T.: -0.065 min
Response: 944990
Conc: 2.74 ng/ml

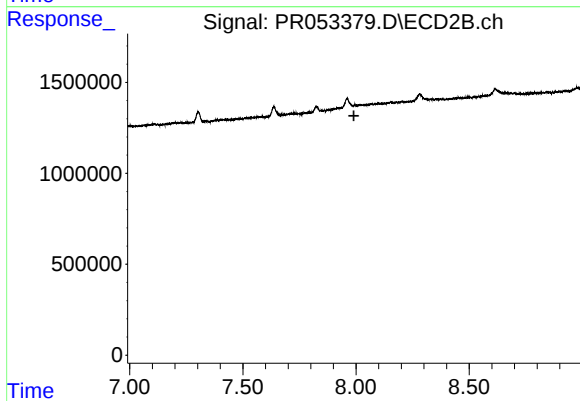

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.990 min
Response: 0
Conc: N.D.