

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR020724\
 Data File : PR065386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2024 12:28
 Operator : AJ\MA
 Sample : P1366-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 EB-1-0-2

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/08/2024
 Supervised By :Sohil Jodhani 02/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 20:58:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.700	3.003	120.2E6	123.0E6	20.130	22.488
2) SA Decachlor...	9.739	8.371	64744710	64813771	16.188	13.695m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR020724\
Data File : PR065386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2024 12:28
Operator : AJ\MA
Sample : P1366-03
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
EB-1-0-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/08/2024
Supervised By :Sohil Jodhani 02/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 20:58:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

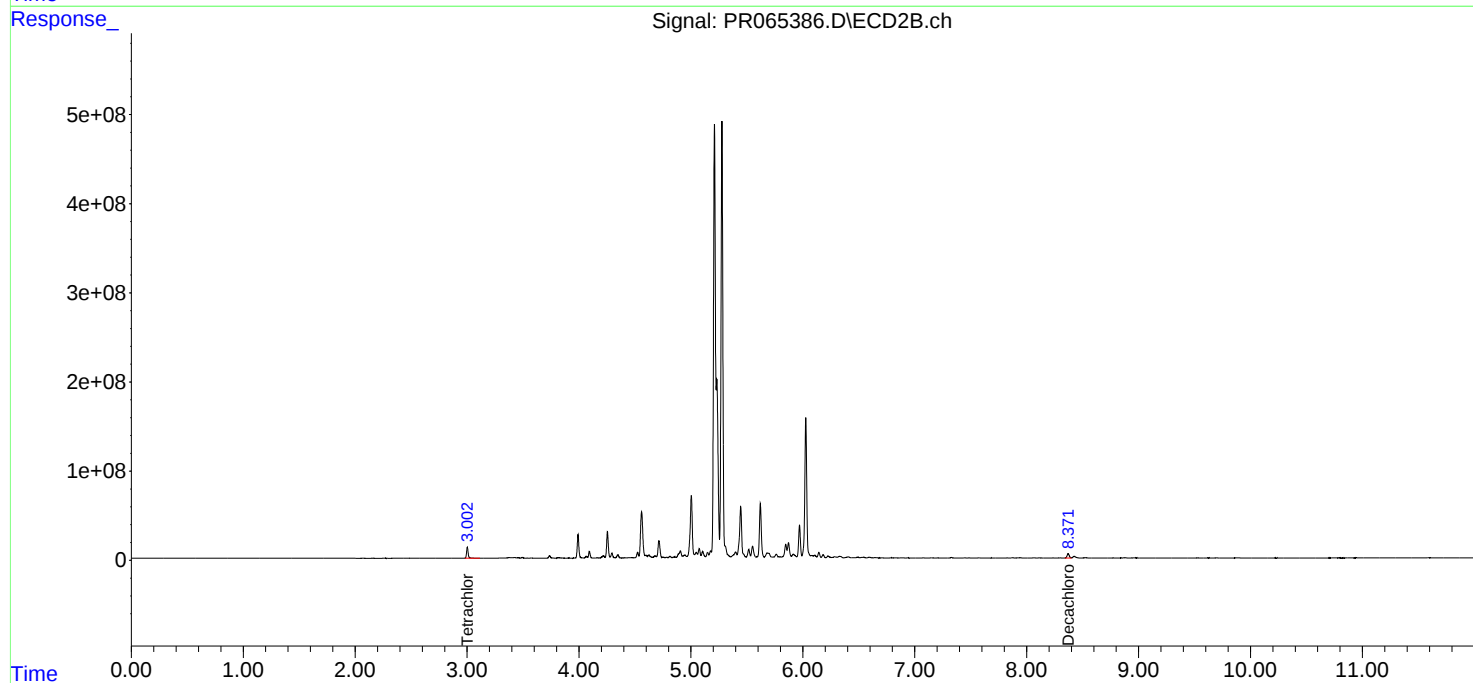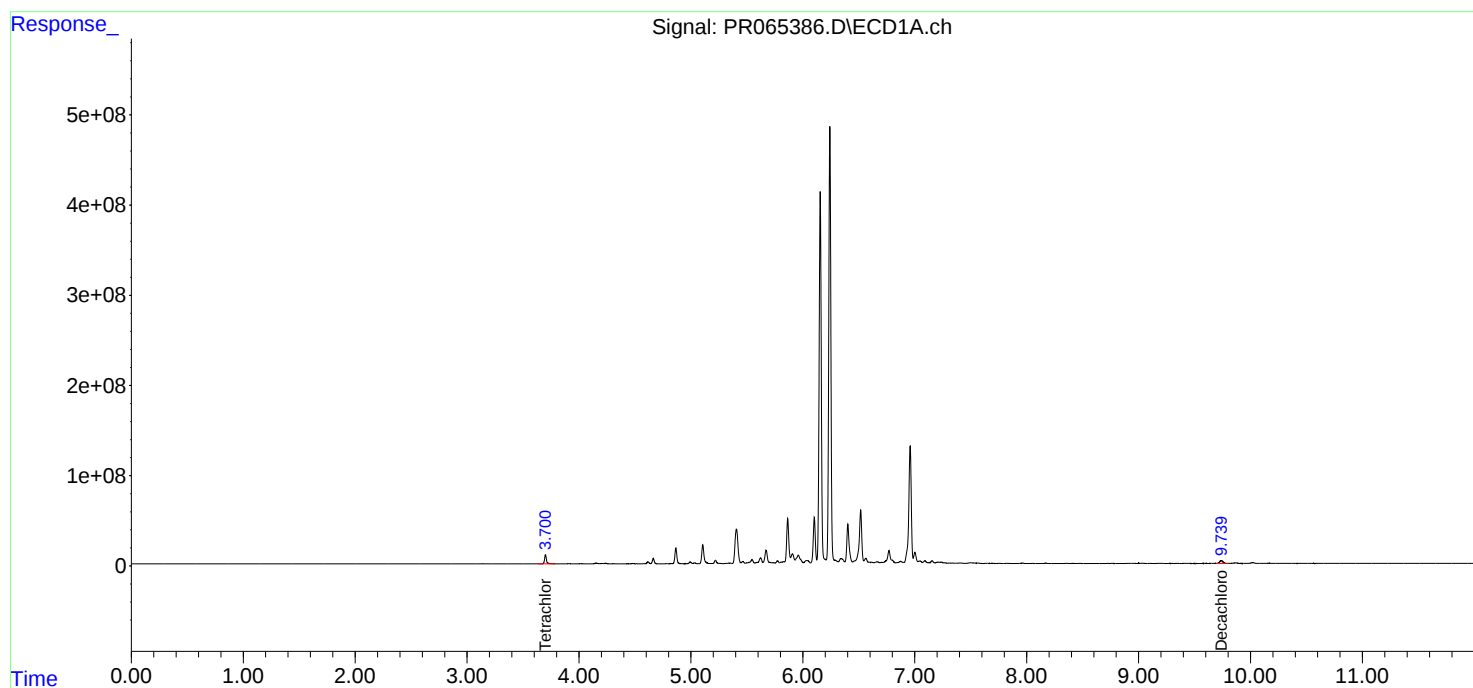

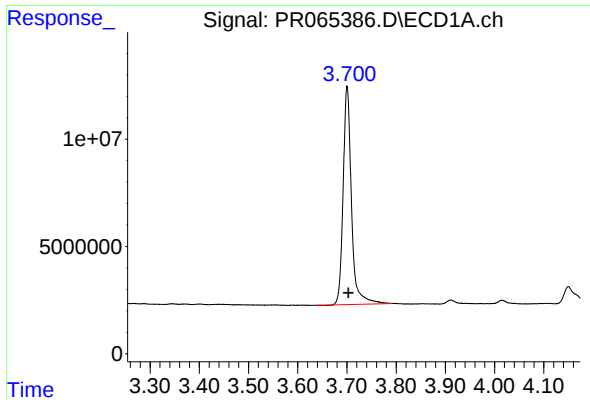


#1 Tetrachloro-m-xylene

R.T.: 3.700 min
Delta R.T.: -0.003 min
Response: 120160889
Conc: 20.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
EB-1-0-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/08/2024
Supervised By :Sohil Jodhani 02/08/2024

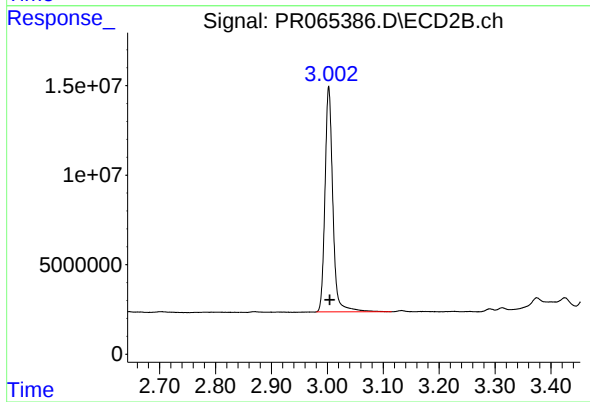


#1 Tetrachloro-m-xylene

R.T.: 3.003 min
Delta R.T.: -0.002 min
Response: 123002947
Conc: 22.49 ng/ml

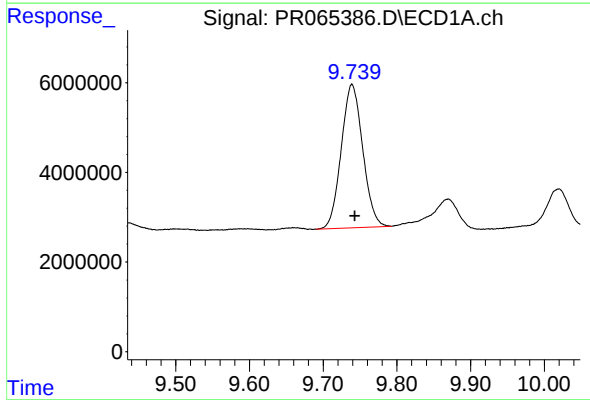

#2 Decachlorobiphenyl

R.T.: 9.739 min
Delta R.T.: -0.004 min
Response: 64744710
Conc: 16.19 ng/ml

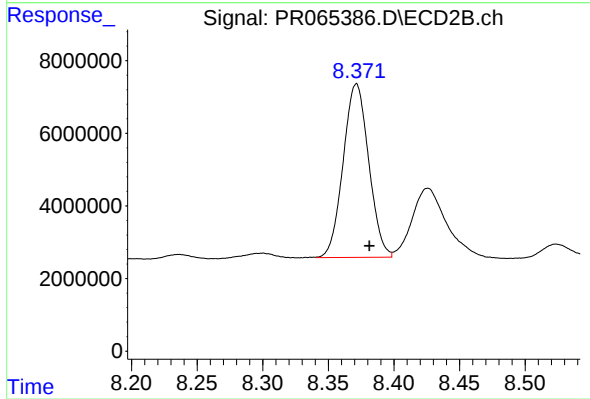

#2 Decachlorobiphenyl

R.T.: 8.371 min
Delta R.T.: -0.010 min
Response: 64813771
Conc: 13.69 ng/ml m