

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR020724\
 Data File : PR065387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2024 12:43
 Operator : AJ\MA
 Sample : P1366-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 EB-1-4-6

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/08/2024
 Supervised By :Sohil Jodhani 02/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 21:00:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.701	3.004	116.5E6	118.2E6	19.515	21.613
2) SA Decachlor...	9.738	8.371	67483559	67124942	16.873	14.183m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR020724\
Data File : PR065387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2024 12:43
Operator : AJ\MA
Sample : P1366-05
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
EB-1-4-6


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/08/2024
Supervised By :Sohil Jodhani 02/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 21:00:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

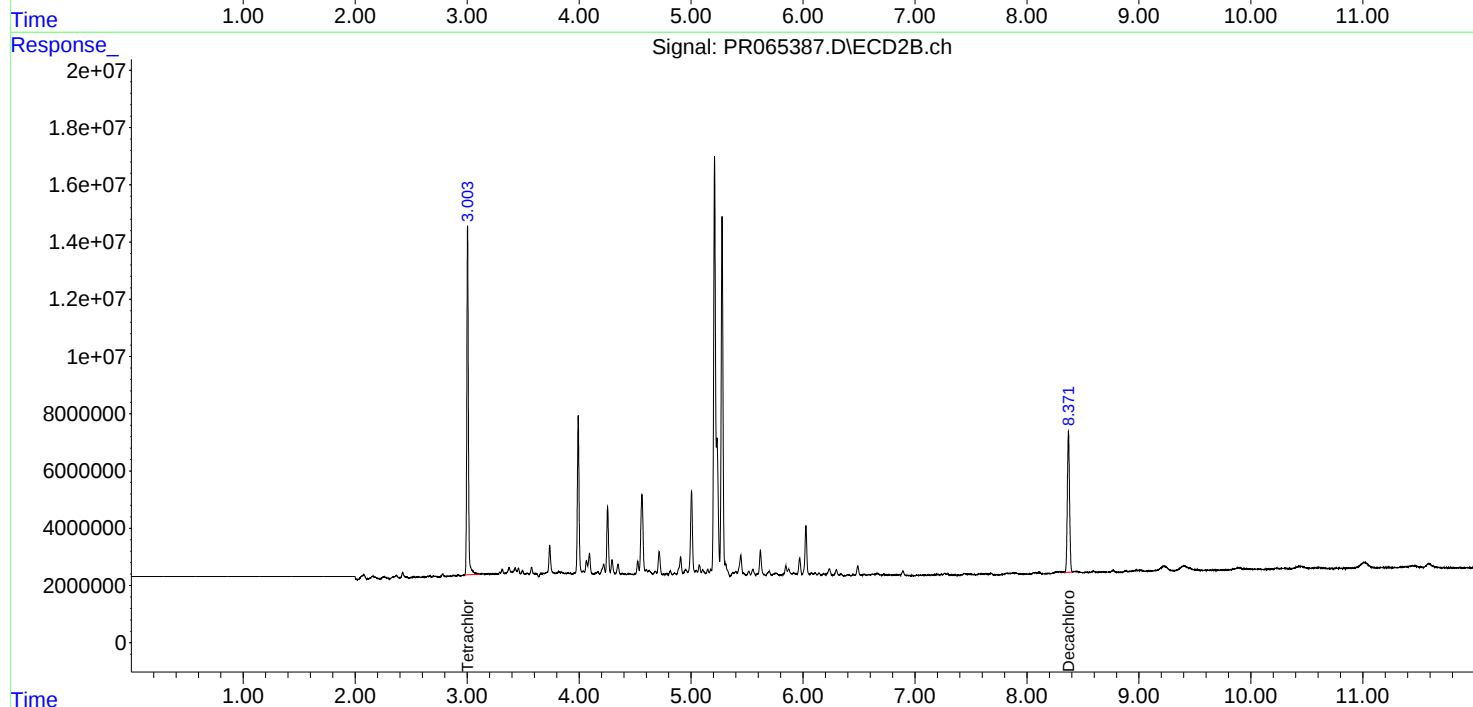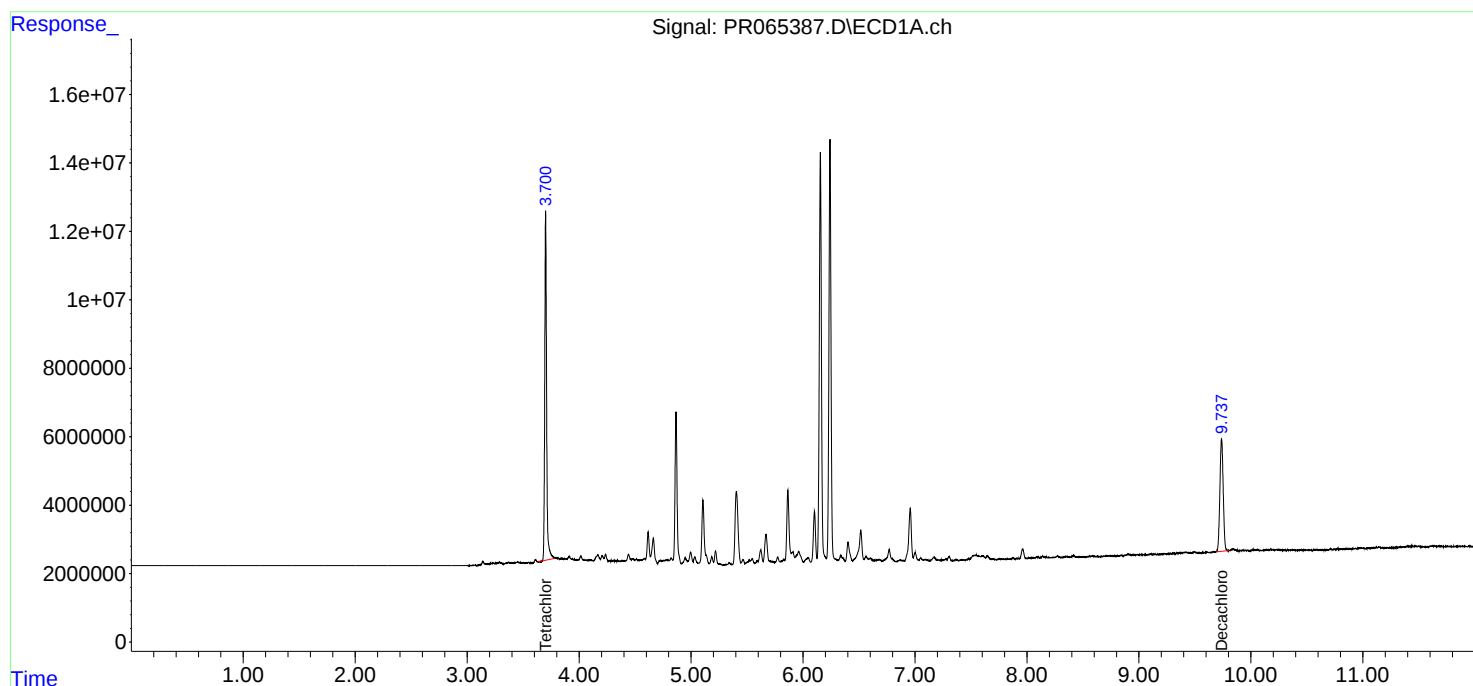

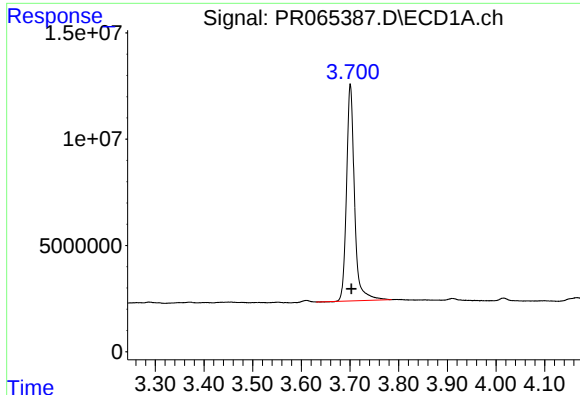


#1 Tetrachloro-m-xylene

R.T.: 3.701 min
Delta R.T.: -0.002 min
Response: 116488220
Conc: 19.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
EB-1-4-6


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/08/2024
Supervised By :Sohil Jodhani 02/08/2024

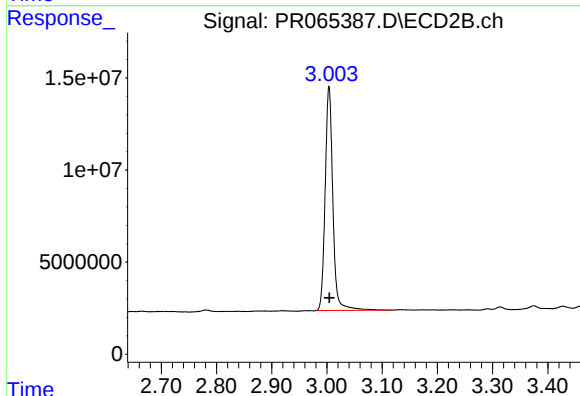


#1 Tetrachloro-m-xylene

R.T.: 3.004 min
Delta R.T.: 0.000 min
Response: 118216881
Conc: 21.61 ng/ml

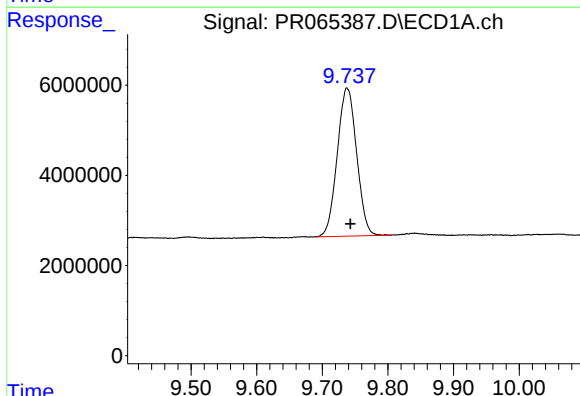

#2 Decachlorobiphenyl

R.T.: 9.738 min
Delta R.T.: -0.005 min
Response: 67483559
Conc: 16.87 ng/ml

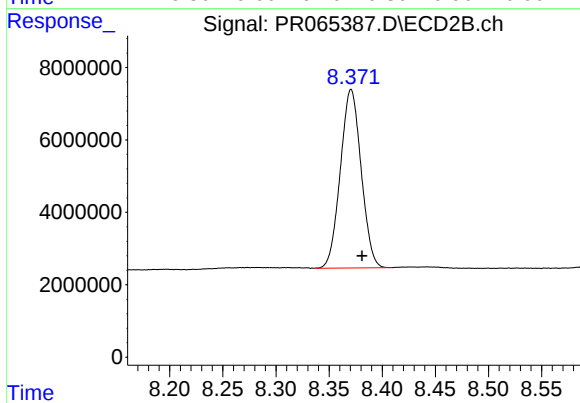

#2 Decachlorobiphenyl

R.T.: 8.371 min
Delta R.T.: -0.011 min
Response: 67124942
Conc: 14.18 ng/ml m