

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR020724\
 Data File : PR065396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2024 15:11
 Operator : AJ\MA
 Sample : P1367-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 EB-6-7-9

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/08/2024
 Supervised By :Sohil Jodhani 02/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 21:19:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 19 20:49:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.700	3.003	89002790	115.9E6	14.910	21.188 #
2) SA Decachlor...	9.739	8.371	56941759	52194262	14.237	11.029m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR020724\
Data File : PR065396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2024 15:11
Operator : AJ\MA
Sample : P1367-05
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
EB-6-7-9


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/08/2024
Supervised By :Sohil Jodhani 02/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 21:19:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR011924.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 19 20:49:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

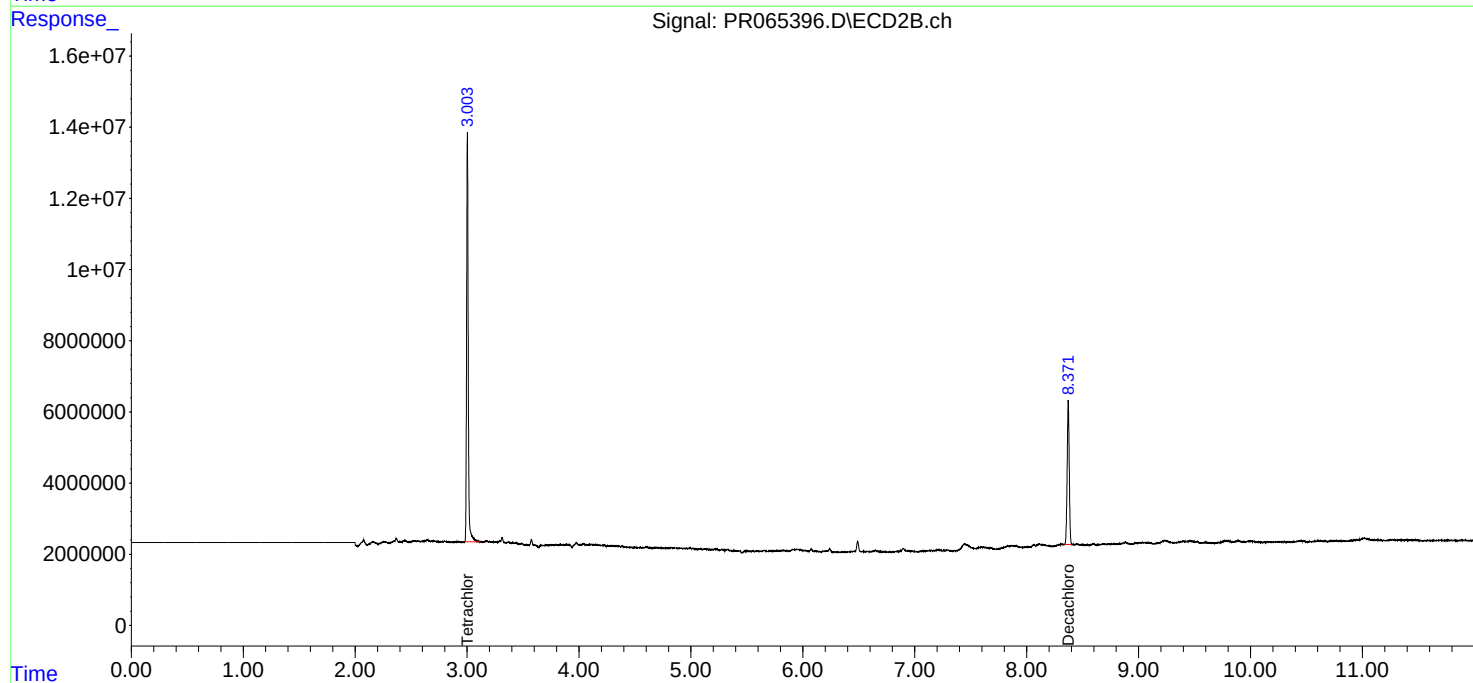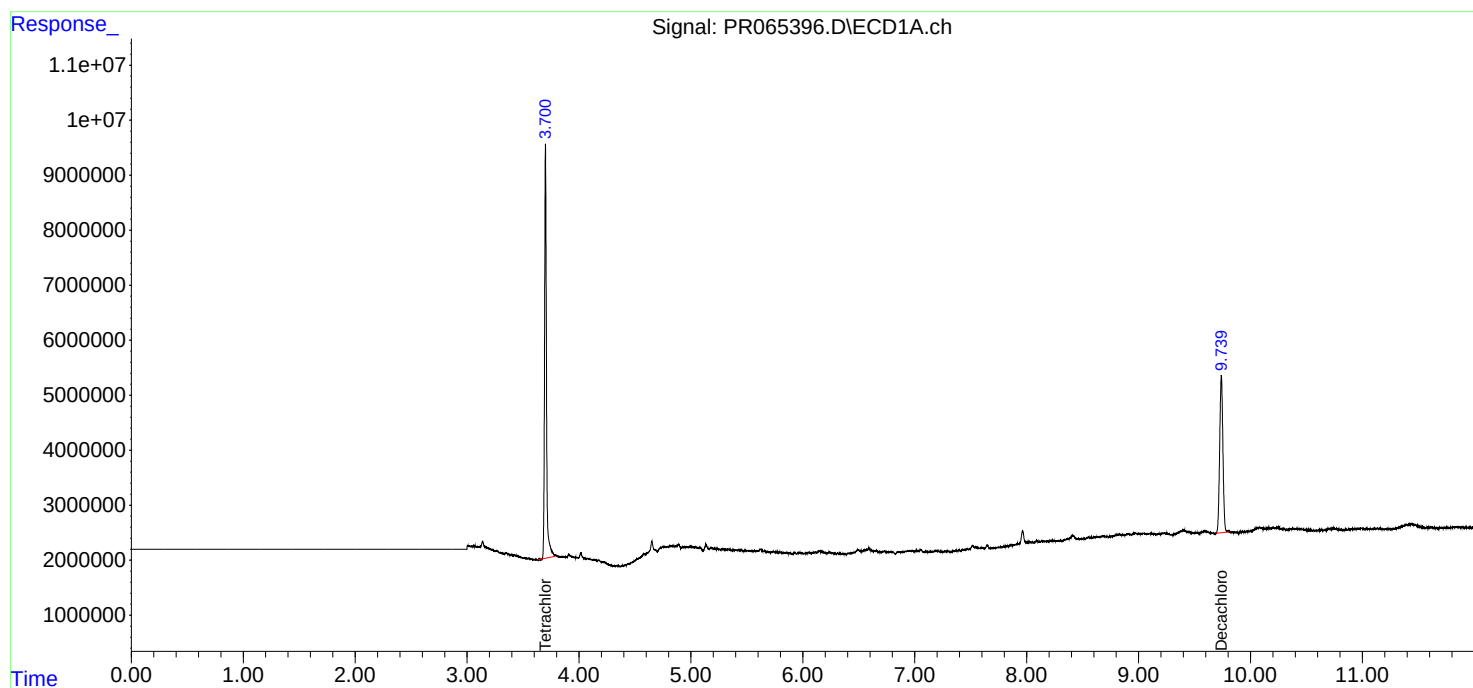

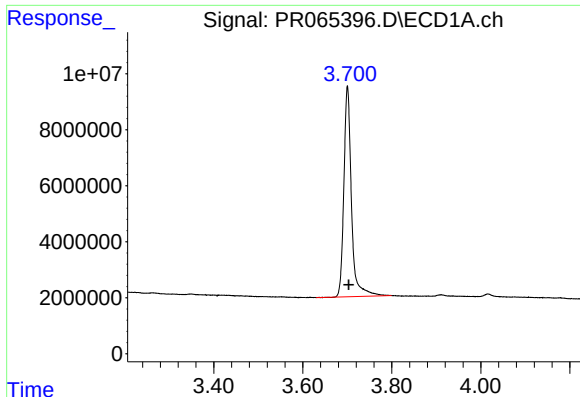


#1 Tetrachloro-m-xylene

R.T.: 3.700 min
Delta R.T.: -0.003 min
Response: 89002790
Conc: 14.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
EB-6-7-9


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/08/2024
Supervised By :Sohil Jodhani 02/08/2024

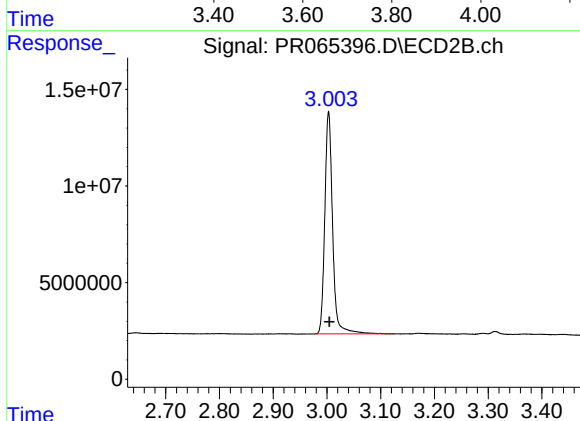


#1 Tetrachloro-m-xylene

R.T.: 3.003 min
Delta R.T.: -0.001 min
Response: 115895087
Conc: 21.19 ng/ml

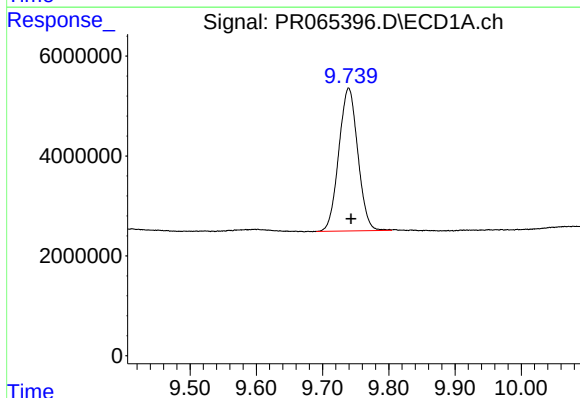

#2 Decachlorobiphenyl

R.T.: 9.739 min
Delta R.T.: -0.004 min
Response: 56941759
Conc: 14.24 ng/ml

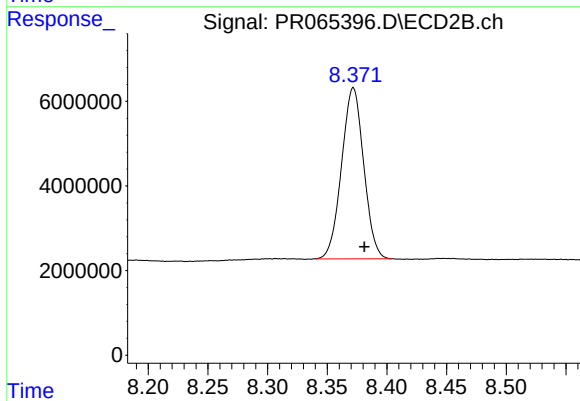

#2 Decachlorobiphenyl

R.T.: 8.371 min
Delta R.T.: -0.010 min
Response: 52194262
Conc: 11.03 ng/ml m