

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR021025\
 Data File : PR070266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2025 19:34
 Operator : AJ\MA
 Sample : Q1168-07
 Misc : AR1262 LOD 25 PPB
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 00:49:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 10 14:13:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.625	2.956	18574570	97611676	16.450	16.739
2) SA Decachlor...	9.510	8.224	13190431	74514241	18.451	18.199
Target Compounds						
3) L1 AR-1016-1	0.000	4.076	0	352507	N.D.	2.235 #
4) L1 AR-1016-2	0.000	4.087	0	239913	N.D.	1.007 #
5) L1 AR-1016-3	0.000	4.267	0	200454	N.D.	1.597 #
6) L1 AR-1016-4	0.000	4.319	0	307745	N.D.	2.800 #
7) L1 AR-1016-5	0.000	4.543	0	151966	N.D.	1.114 #
8) L2 AR-1221-1	3.834	0.000	210962	0	16.161	N.D. #
9) L2 AR-1221-2	3.934	3.260	302085	1241190	30.941	24.240
12) L3 AR-1232-2	0.000	4.087	0	239913	N.D.	2.161 #
13) L3 AR-1232-3	0.000	4.267	0	200454	N.D.	3.473 #
14) L3 AR-1232-4	0.000	4.371	0	175528	N.D.	3.308 #
15) L3 AR-1232-5	0.000	4.543	0	151966	N.D.	2.656 #
16) L4 AR-1242-1	0.000	4.076	0	352507	N.D.	2.726 #
17) L4 AR-1242-2	0.000	4.087	0	239913	N.D.	1.234 #
18) L4 AR-1242-3	0.000	4.267	0	200454	N.D.	1.926 #
19) L4 AR-1242-4	0.000	4.371	0	175528	N.D.	1.713 #
20) L4 AR-1242-5	0.000	4.910	0	905154	N.D.	7.899 #
21) L5 AR-1248-1	0.000	4.076	0	352507	N.D.	3.654 #
22) L5 AR-1248-2	0.000	4.319	0	307745	N.D.	2.121 #
23) L5 AR-1248-3	0.000	4.371	0	175528	N.D.	1.185 #
24) L5 AR-1248-4	5.751f	4.543	154313	151966	5.128	0.865 #
25) L5 AR-1248-5	0.000	4.948	0	299235	N.D.	1.993 #
26) L6 AR-1254-1	5.751	4.910	154313	905154	4.235	3.582
27) L6 AR-1254-2	5.987	5.071	135872	1148660	2.511	5.271 #
28) L6 AR-1254-3	6.371	5.515f	156175	2967008	2.923	9.296 #
29) L6 AR-1254-4	6.678	5.741	135090	253658	4.228	1.576 #
30) L6 AR-1254-5	7.143	6.187	967220	3200073	25.051	12.305 #
31) L7 AR-1260-1	6.559	5.635	907904	4204600	20.957	19.109
32) L7 AR-1260-2	6.841	5.842	1003901	4419455	22.200	17.948
33) L7 AR-1260-3	7.233	6.001	1384499	4923320	37.147	20.658 #
34) L7 AR-1260-4	7.477	6.506	1238581	6217352	31.096	31.562
35) L7 AR-1260-5	7.816	6.774	1751725	10316494	27.240	25.073
36) L8 AR-1262-1	7.477	6.232	1238581	6787417	24.556	22.047
37) L8 AR-1262-2	7.816	6.506	1751725	6217352	23.180	23.015
38) L8 AR-1262-3	8.122	7.078	1154181	3967176	21.627	20.225
39) L8 AR-1262-4	8.207	7.147	926052	7436574	21.038	20.633
40) L8 AR-1262-5	8.828	7.685	495987	3636042	20.511	23.843
41) L9 AR-1268-1	8.122	7.078	1154181	3967176	11.824	6.942 #
42) L9 AR-1268-2	8.207	7.147	926052	7436574	10.373	14.199 #
43) L9 AR-1268-3	0.000	7.371	0	595951	N.D.	1.219 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR021025\
Data File : PR070266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2025 19:34
Operator : AJ\MA
Sample : Q1168-07
Misc : AR1262 LOD 25 PPB
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 00:49:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021025.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 10 14:13:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44)	L9 AR-1268-4	8.828	7.685	495987	3636042	18.618	21.249
45)	L9 AR-1268-5	9.209	7.980	234091	1548420	1.108	1.116



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR021025\
Data File : PR070266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2025 19:34
Operator : AJ\MA
Sample : Q1168-07
Misc : AR1262 LOD 25 PPB
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 00:49:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021025.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 10 14:13:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

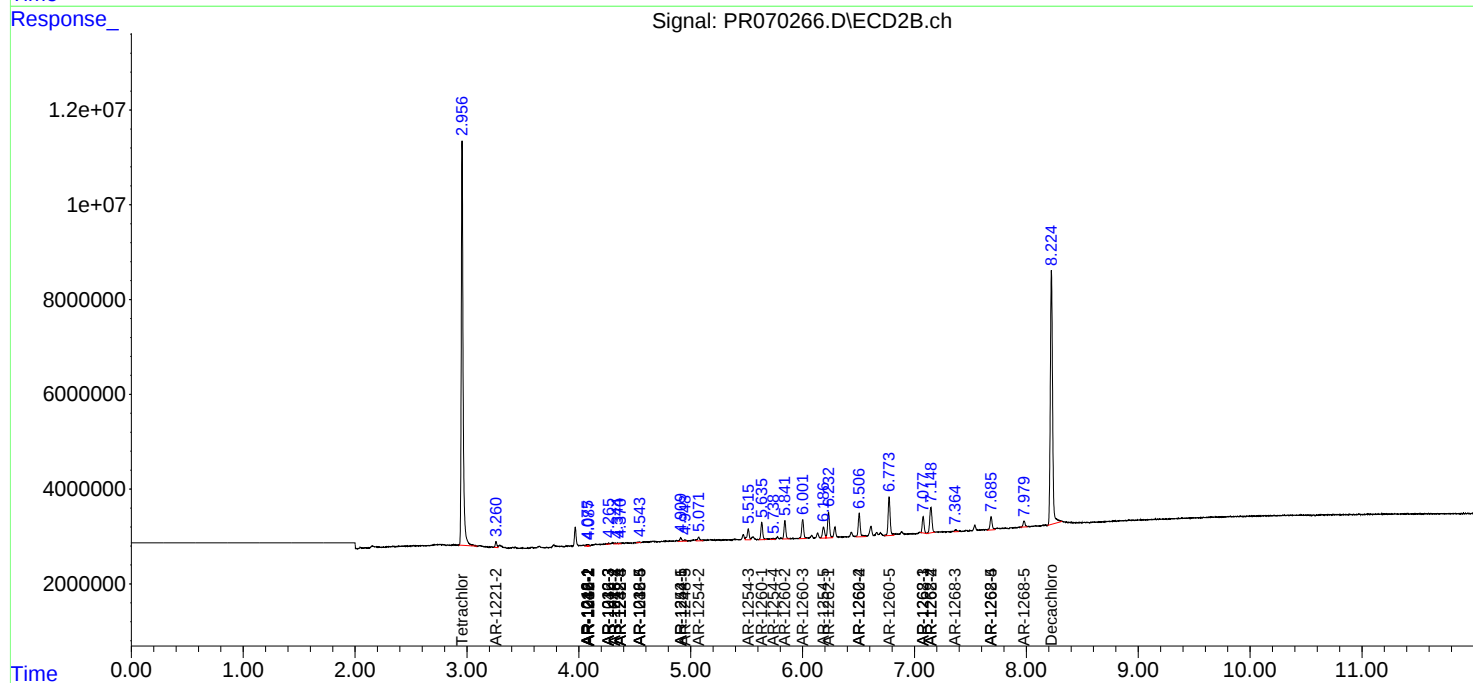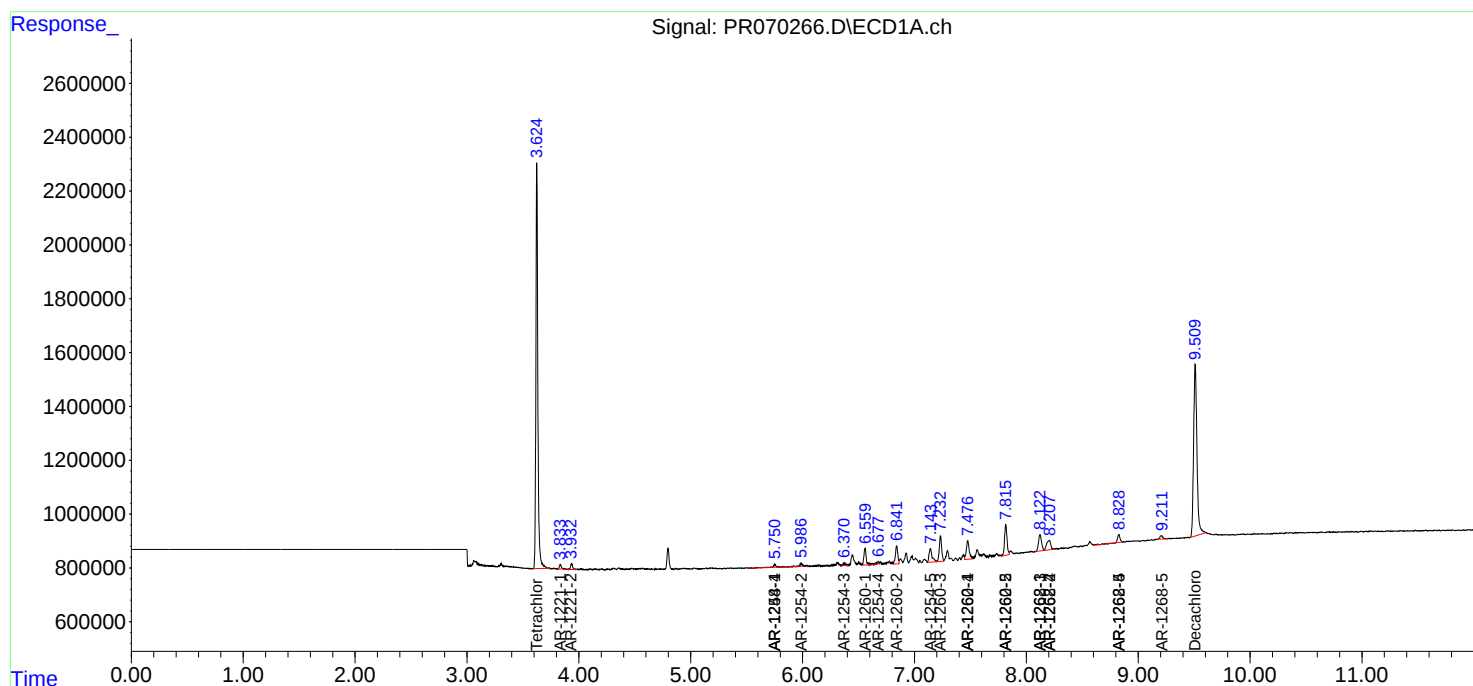


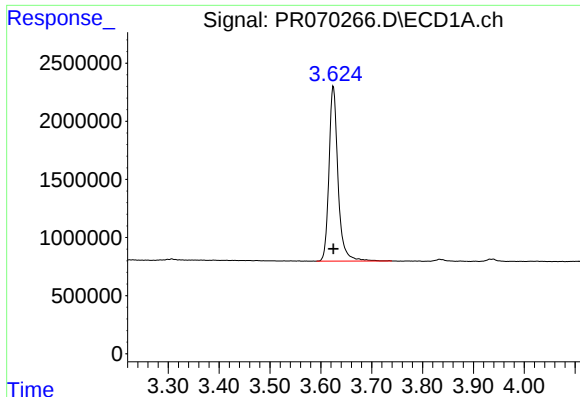

#1 Tetrachloro-m-xylene


R.T.: 3.625 min
Delta R.T.: 0.000 min
Response: 18574570
Conc: 16.45 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

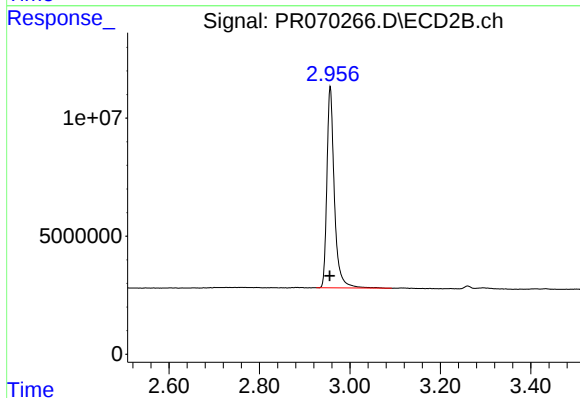


#1 Tetrachloro-m-xylene

R.T.: 2.956 min
Delta R.T.: 0.000 min
Response: 97611676
Conc: 16.74 ng/ml

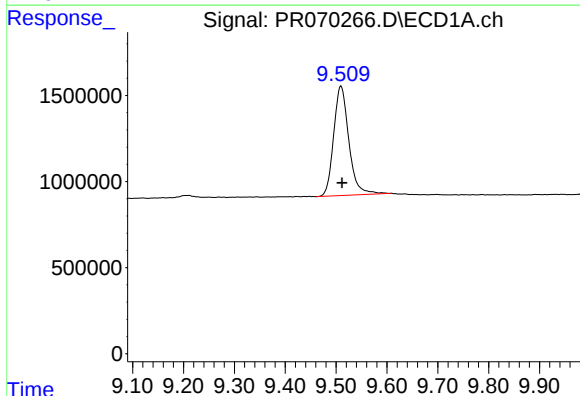


#2 Decachlorobiphenyl

R.T.: 9.510 min
Delta R.T.: -0.002 min
Response: 13190431
Conc: 18.45 ng/ml

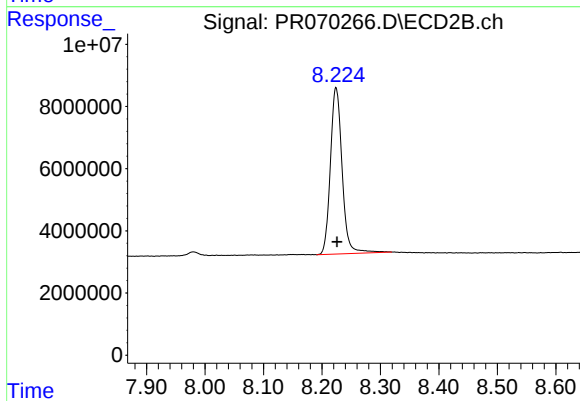

#2 Decachlorobiphenyl


R.T.: 8.224 min
Delta R.T.: -0.002 min
Response: 74514241
Conc: 18.20 ng/ml

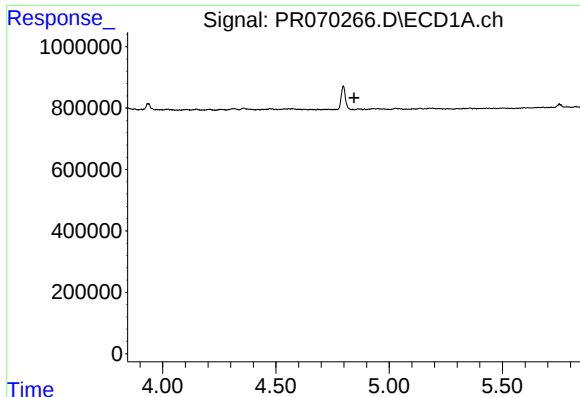

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 4.845 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

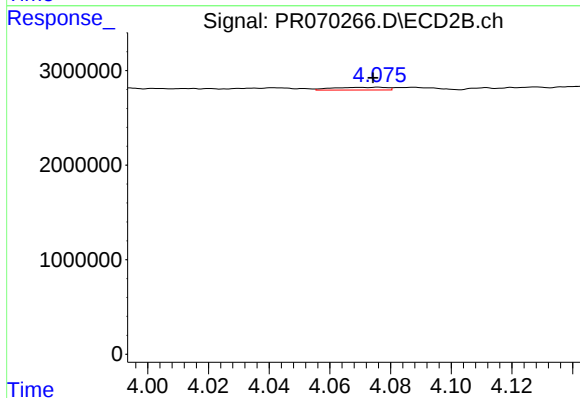


#3 AR-1016-1

R.T.: 4.076 min
Delta R.T.: 0.002 min
Response: 352507
Conc: 2.23 ng/ml

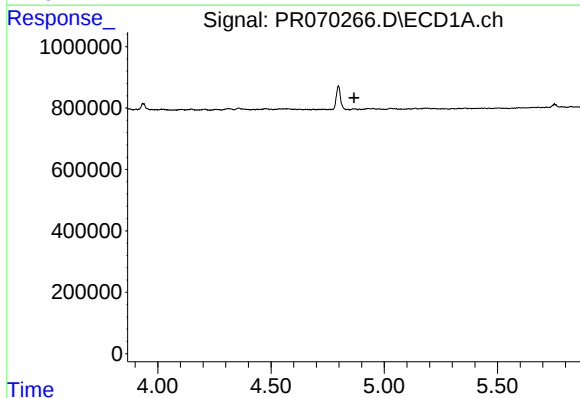


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 4.866 min
Response: 0
Conc: N.D.

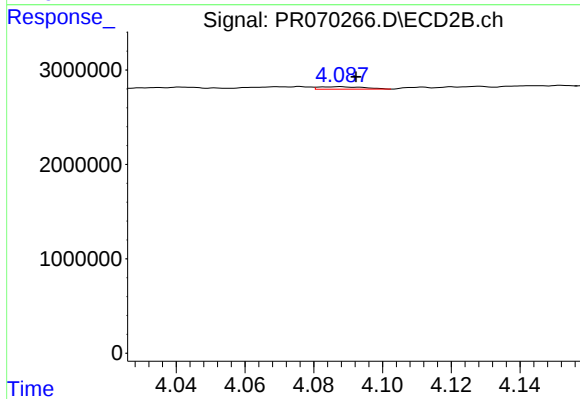

#4 AR-1016-2


R.T.: 4.087 min
Delta R.T.: -0.005 min
Response: 239913
Conc: 1.01 ng/ml

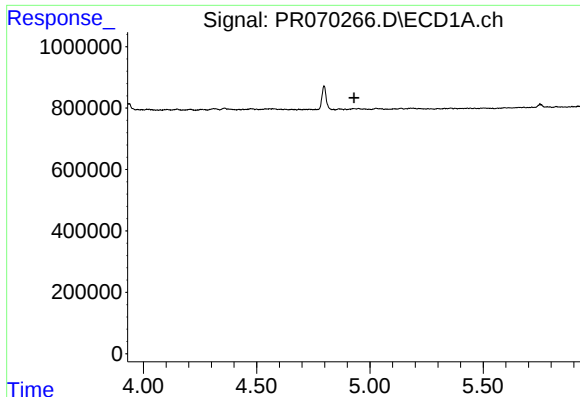

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 4.930 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

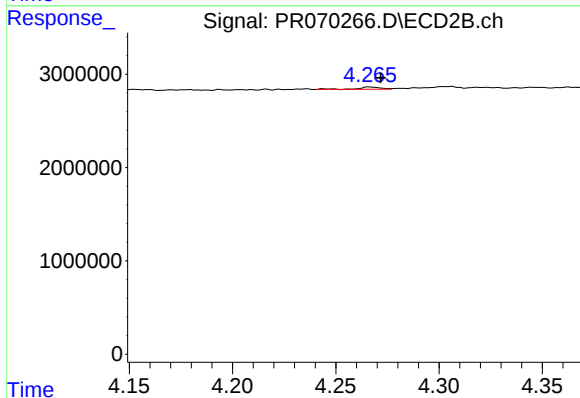


#5 AR-1016-3

R.T.: 4.267 min
Delta R.T.: -0.005 min
Response: 200454
Conc: 1.60 ng/ml

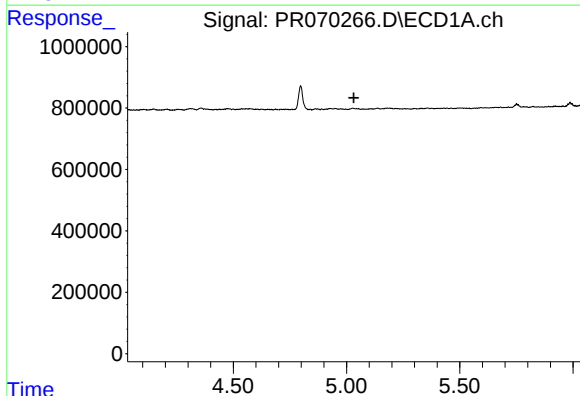


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.032 min
Response: 0
Conc: N.D.

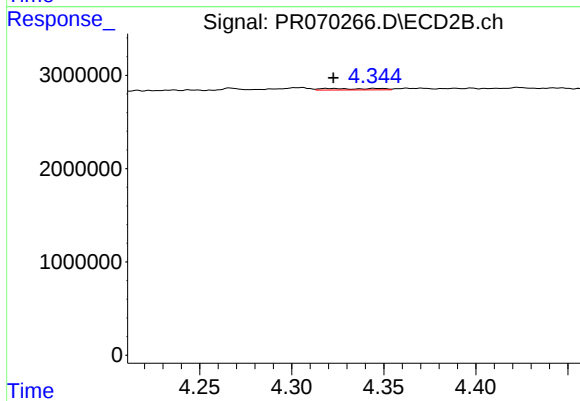

#6 AR-1016-4


R.T.: 4.319 min
Delta R.T.: -0.004 min
Response: 307745
Conc: 2.80 ng/ml

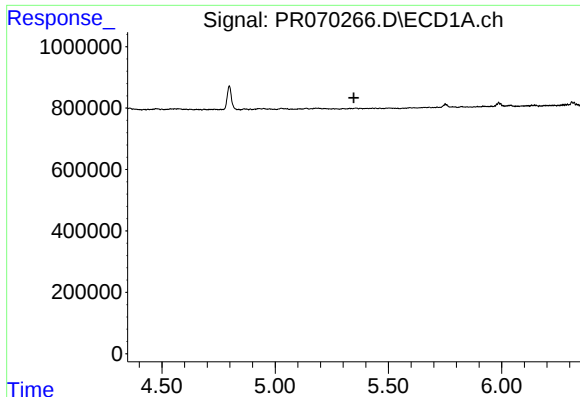

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

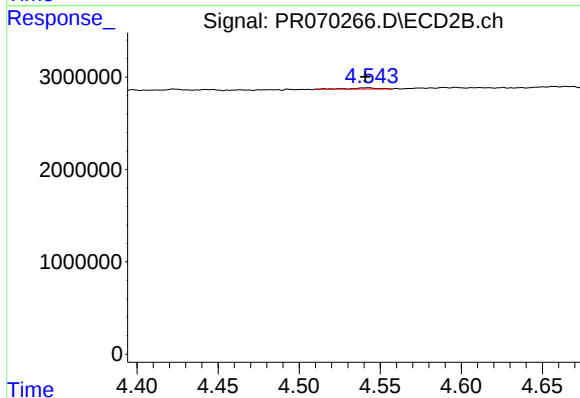


#7 AR-1016-5

R.T.: 4.543 min
Delta R.T.: 0.002 min
Response: 151966
Conc: 1.11 ng/ml

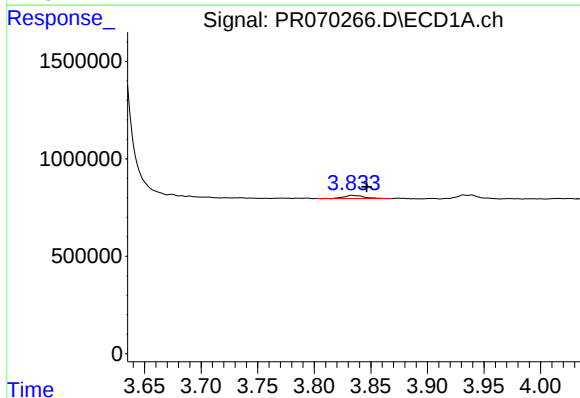


#8 AR-1221-1

R.T.: 3.834 min
Delta R.T.: -0.012 min
Response: 210962
Conc: 16.16 ng/ml

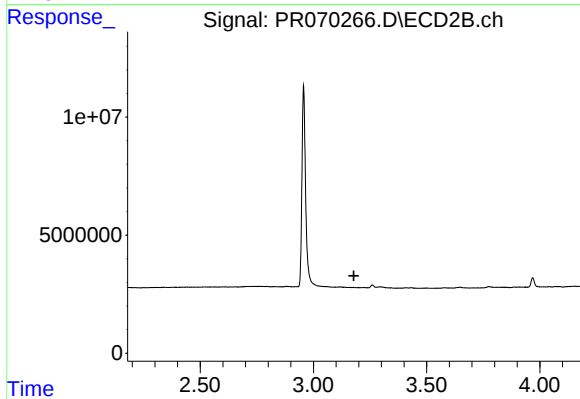

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 3.179 min
Response: 0
Conc: N.D.

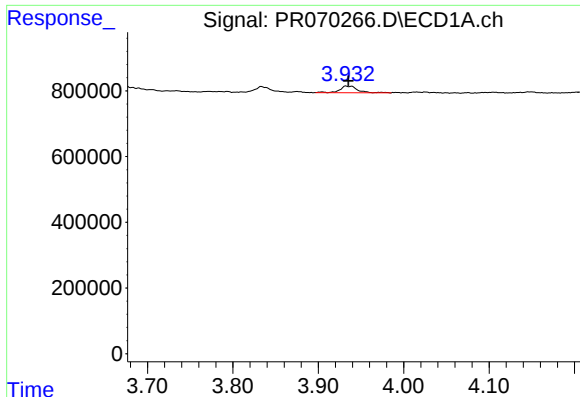

#9 AR-1221-2


R.T.: 3.934 min
Delta R.T.: 0.000 min
Response: 302085
Conc: 30.94 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

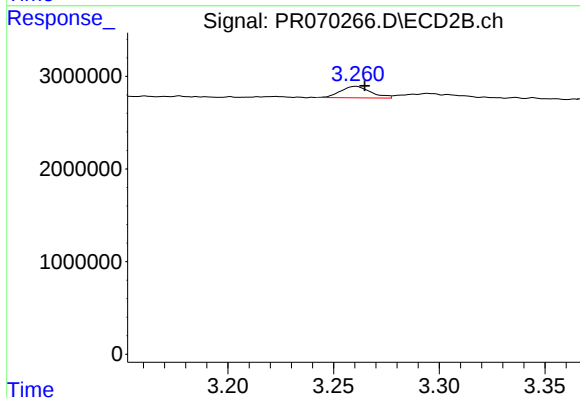


#9 AR-1221-2

R.T.: 3.260 min
Delta R.T.: -0.004 min
Response: 1241190
Conc: 24.24 ng/ml

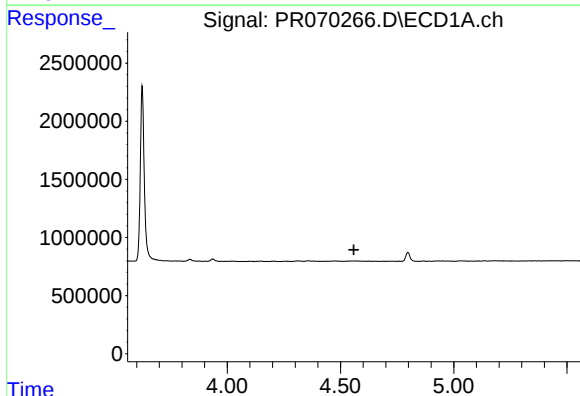


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.559 min
Response: 0
Conc: N.D.

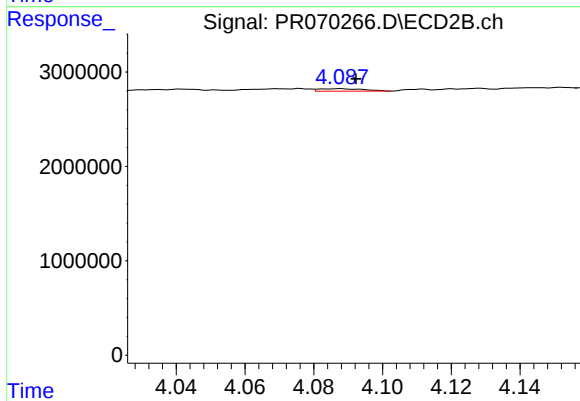

#12 AR-1232-2


R.T.: 4.087 min
Delta R.T.: -0.005 min
Response: 239913
Conc: 2.16 ng/ml

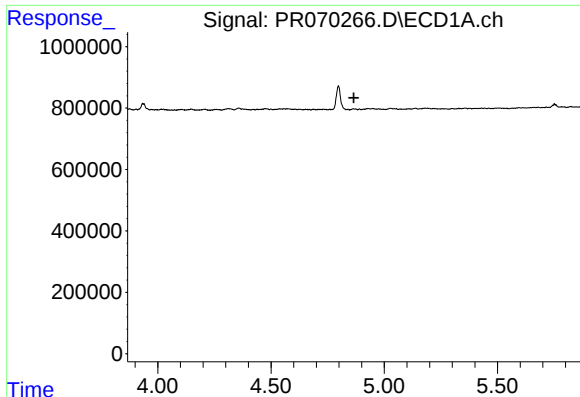

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 4.866 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

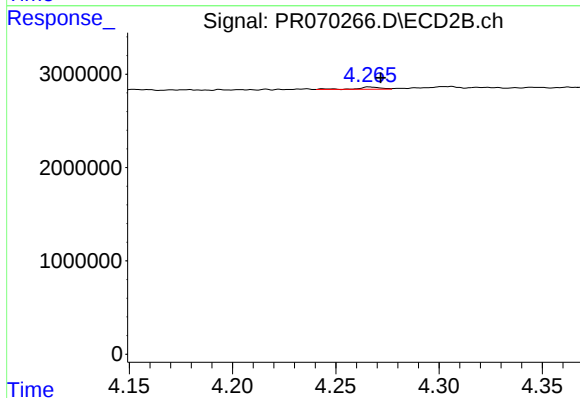


#13 AR-1232-3

R.T.: 4.267 min
Delta R.T.: -0.005 min
Response: 200454
Conc: 3.47 ng/ml

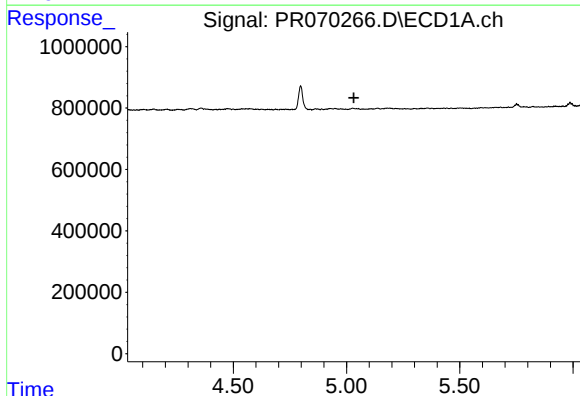


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.032 min
Response: 0
Conc: N.D.

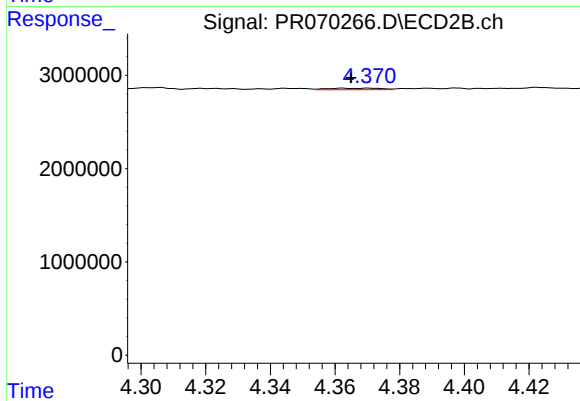

#14 AR-1232-4


R.T.: 4.371 min
Delta R.T.: 0.006 min
Response: 175528
Conc: 3.31 ng/ml

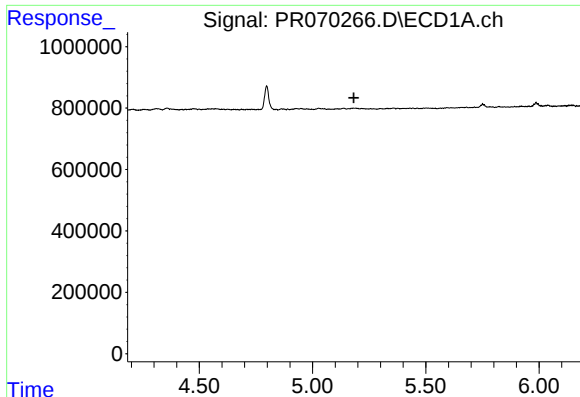

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

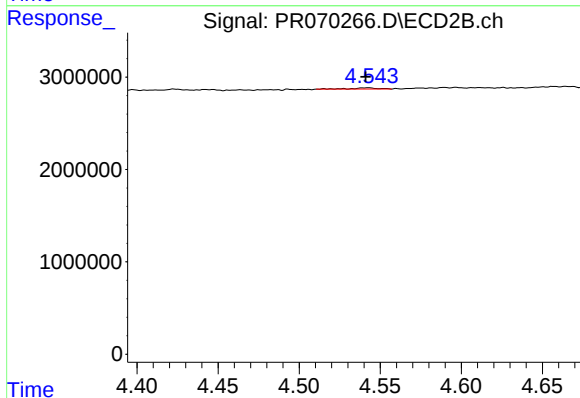


#15 AR-1232-5

R.T.: 4.543 min
Delta R.T.: 0.002 min
Response: 151966
Conc: 2.66 ng/ml

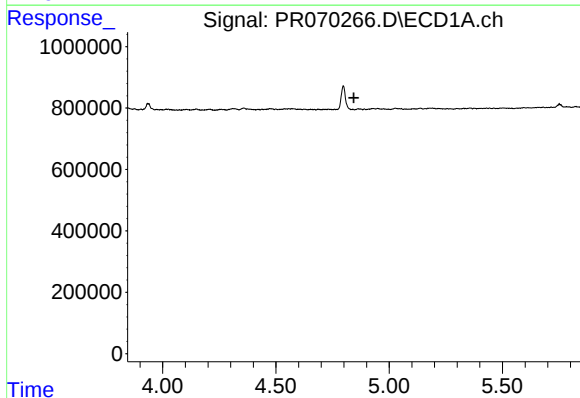


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 4.844 min
Response: 0
Conc: N.D.

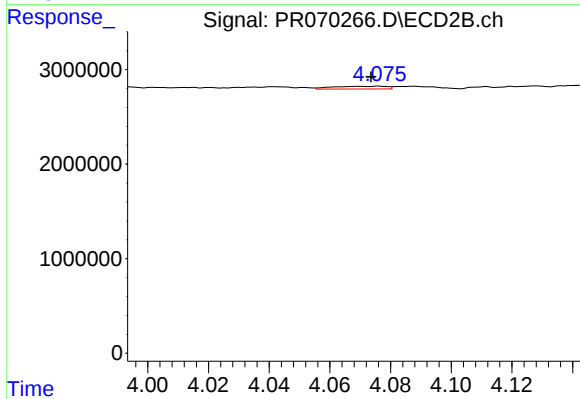

#16 AR-1242-1


R.T.: 4.076 min
Delta R.T.: 0.002 min
Response: 352507
Conc: 2.73 ng/ml

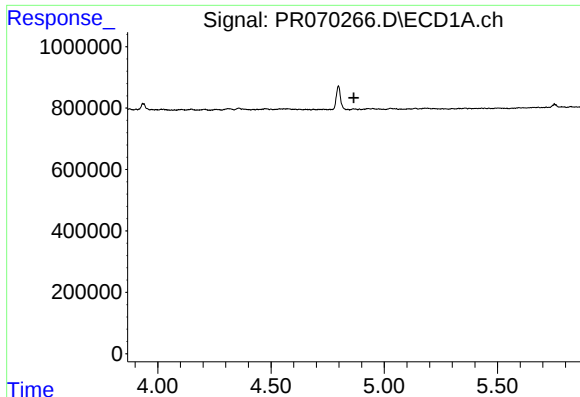

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 4.866 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

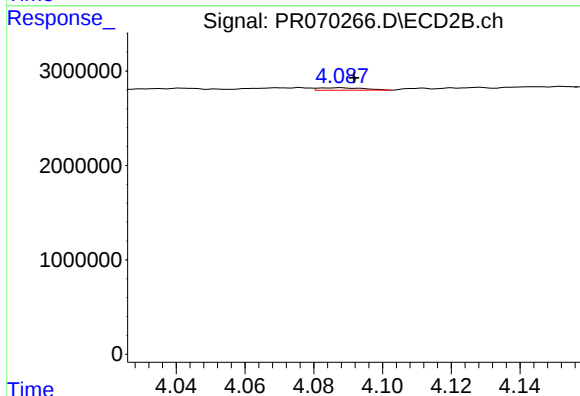


#17 AR-1242-2

R.T.: 4.087 min
Delta R.T.: -0.004 min
Response: 239913
Conc: 1.23 ng/ml

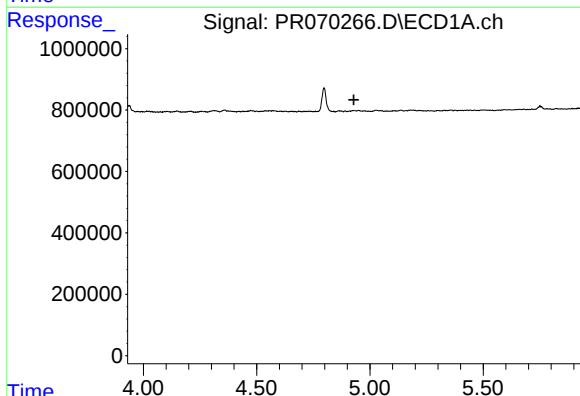


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 4.930 min
Response: 0
Conc: N.D.

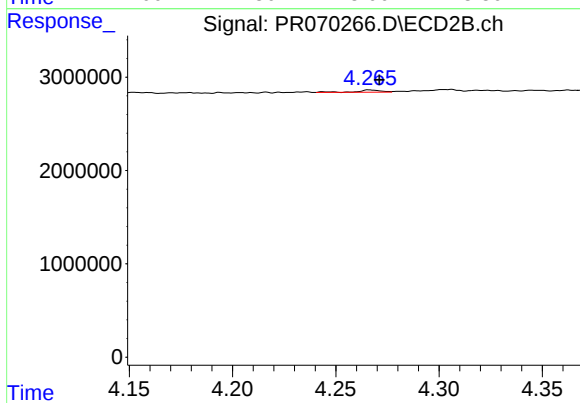

#18 AR-1242-3


R.T.: 4.267 min
Delta R.T.: -0.005 min
Response: 200454
Conc: 1.93 ng/ml

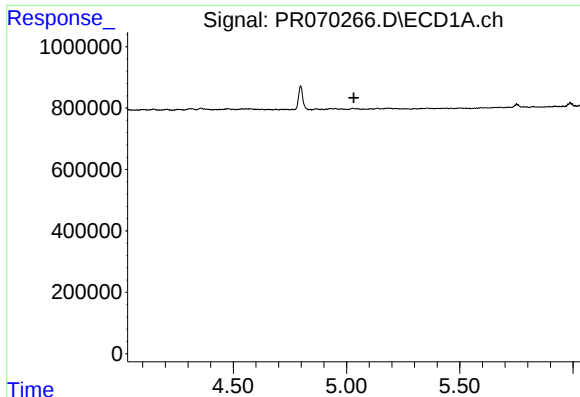

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.032 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

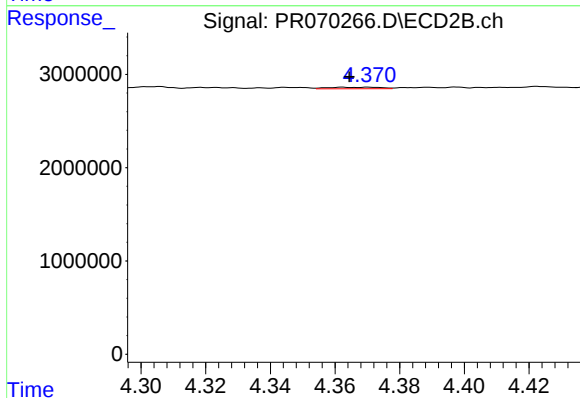


#19 AR-1242-4

R.T.: 4.371 min
Delta R.T.: 0.006 min
Response: 175528
Conc: 1.71 ng/ml

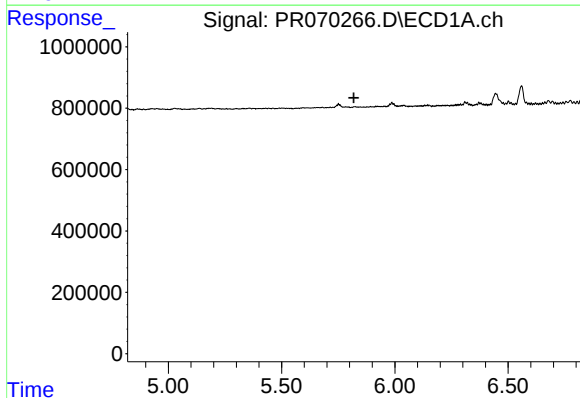


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 5.819 min
Response: 0
Conc: N.D.

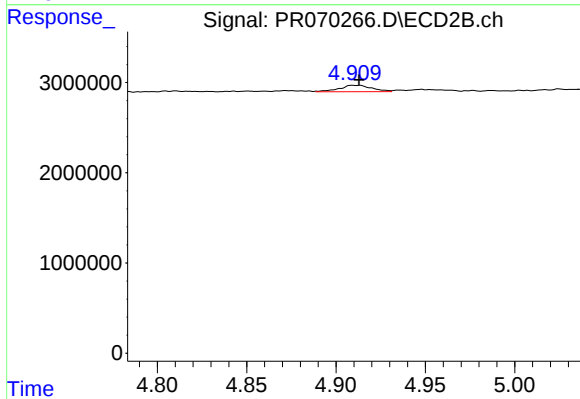

#20 AR-1242-5


R.T.: 4.910 min
Delta R.T.: -0.003 min
Response: 905154
Conc: 7.90 ng/ml

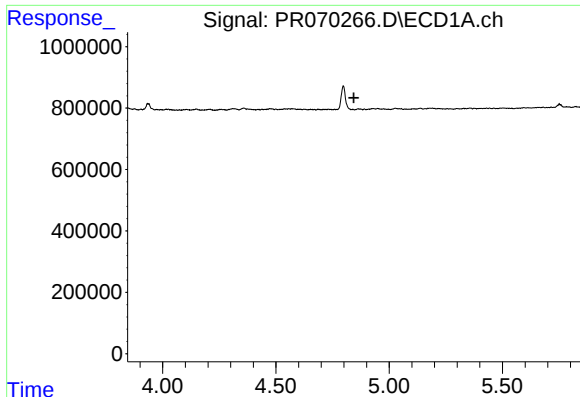

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 4.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

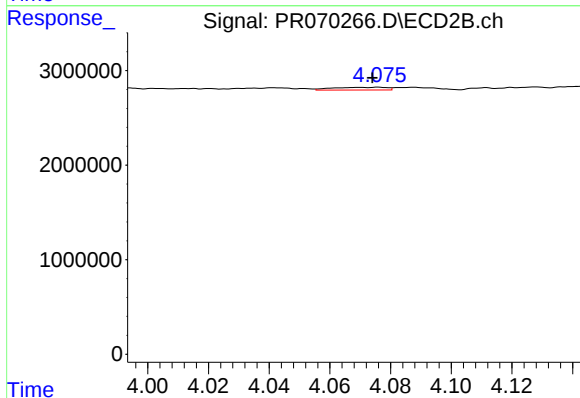


#21 AR-1248-1

R.T.: 4.076 min
Delta R.T.: 0.002 min
Response: 352507
Conc: 3.65 ng/ml

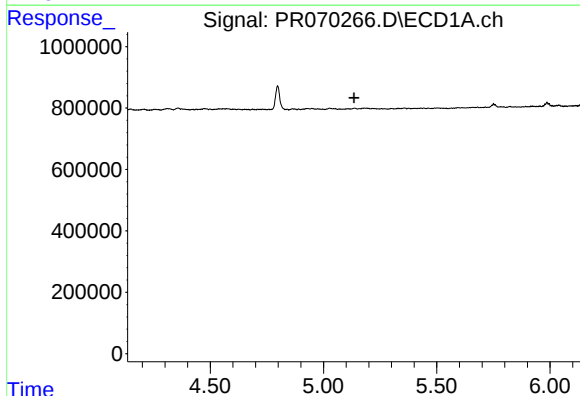


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.135 min
Response: 0
Conc: N.D.

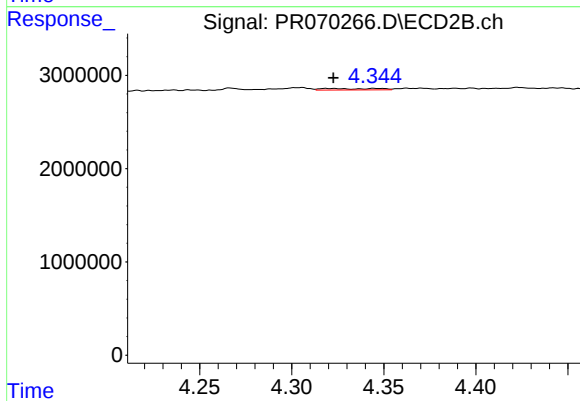

#22 AR-1248-2


R.T.: 4.319 min
Delta R.T.: -0.004 min
Response: 307745
Conc: 2.12 ng/ml

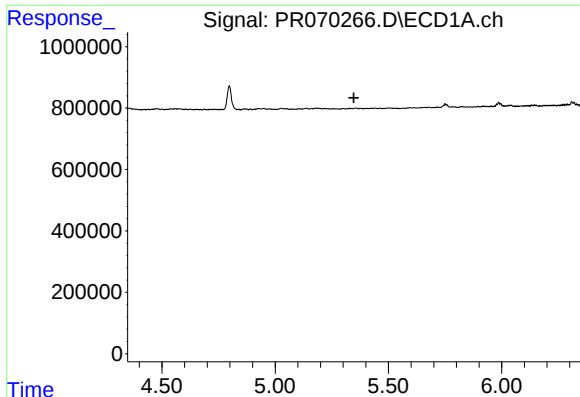

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

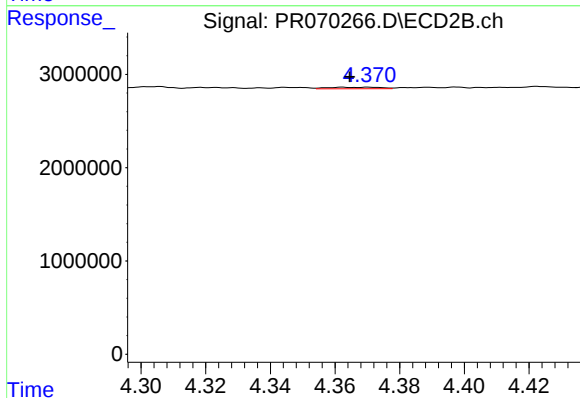


#23 AR-1248-3

R.T.: 4.371 min
Delta R.T.: 0.006 min
Response: 175528
Conc: 1.19 ng/ml

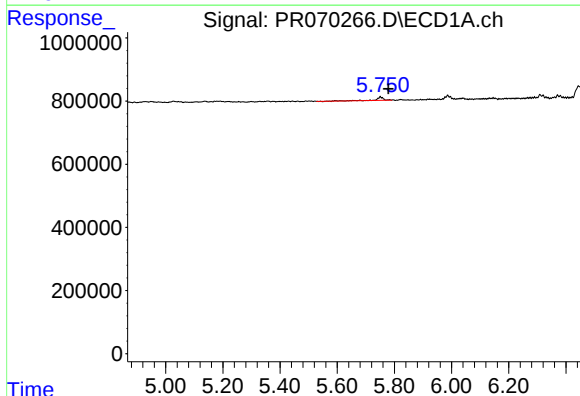


#24 AR-1248-4

R.T.: 5.751 min
Delta R.T.: -0.028 min
Response: 154313
Conc: 5.13 ng/ml

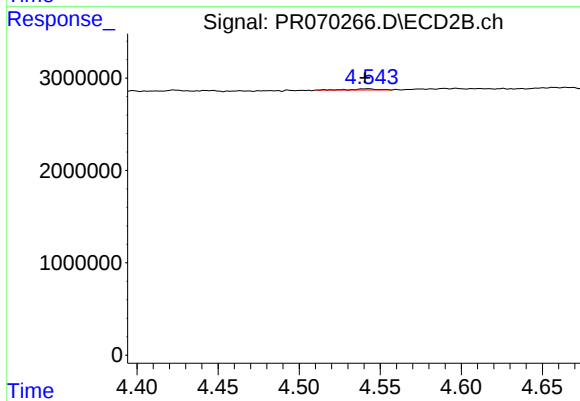

#24 AR-1248-4


R.T.: 4.543 min
Delta R.T.: 0.002 min
Response: 151966
Conc: 0.86 ng/ml

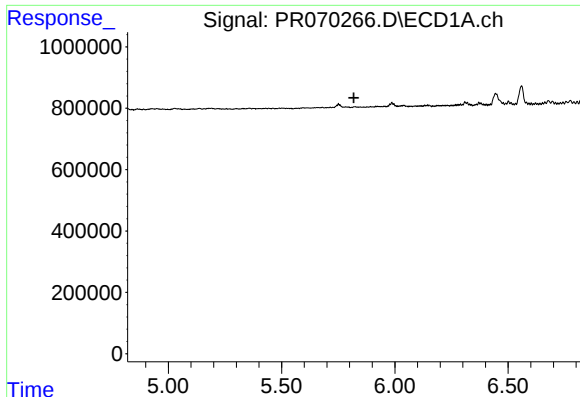

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 5.819 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

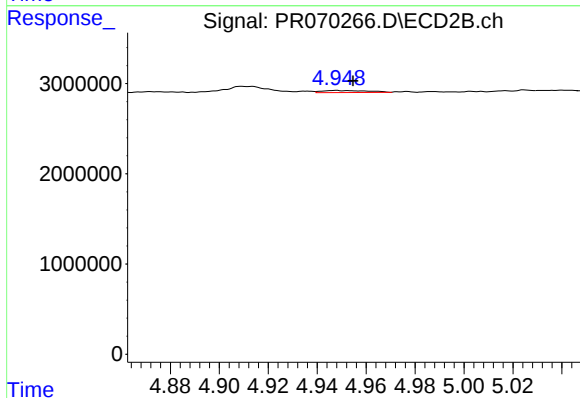


#25 AR-1248-5

R.T.: 4.948 min
Delta R.T.: -0.007 min
Response: 299235
Conc: 1.99 ng/ml

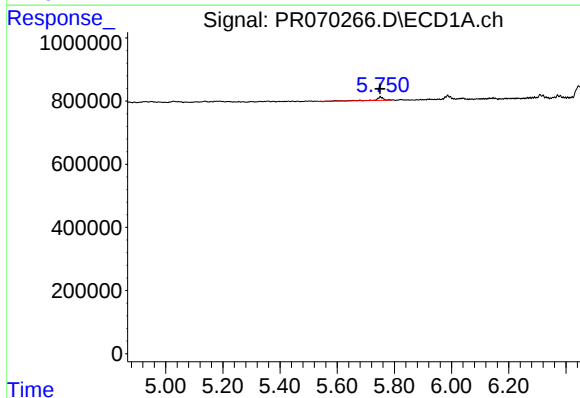


#26 AR-1254-1

R.T.: 5.751 min
Delta R.T.: 0.001 min
Response: 154313
Conc: 4.23 ng/ml

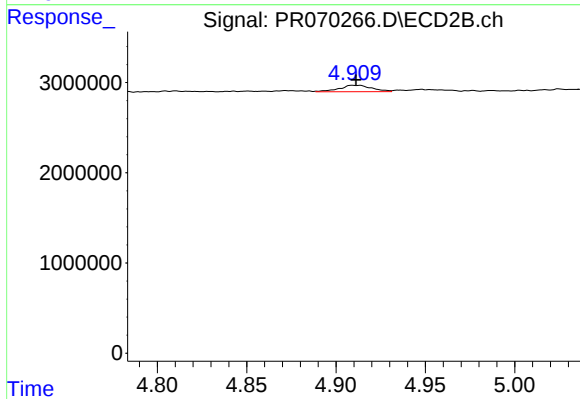

#26 AR-1254-1


R.T.: 4.910 min
Delta R.T.: 0.000 min
Response: 905154
Conc: 3.58 ng/ml

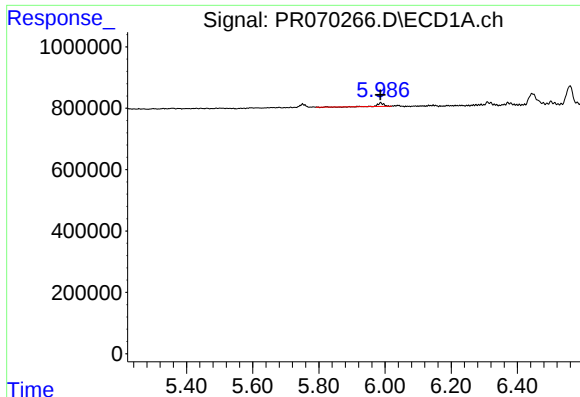

#27 AR-1254-2


R.T.: 5.987 min
Delta R.T.: 0.000 min
Response: 135872
Conc: 2.51 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

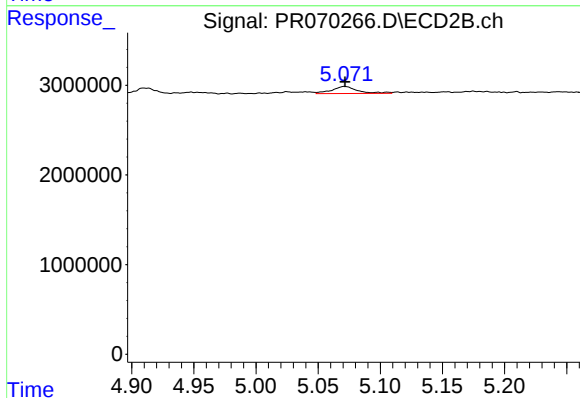


#27 AR-1254-2

R.T.: 5.071 min
Delta R.T.: 0.000 min
Response: 1148660
Conc: 5.27 ng/ml

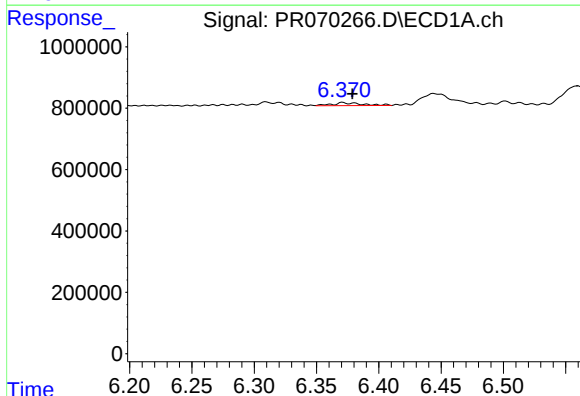


#28 AR-1254-3

R.T.: 6.371 min
Delta R.T.: -0.008 min
Response: 156175
Conc: 2.92 ng/ml

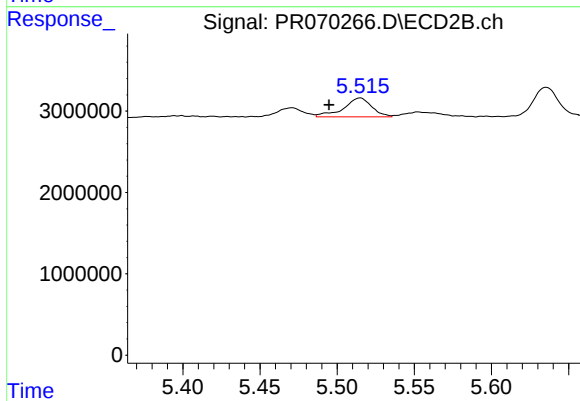

#28 AR-1254-3


R.T.: 5.515 min
Delta R.T.: 0.020 min
Response: 2967008
Conc: 9.30 ng/ml

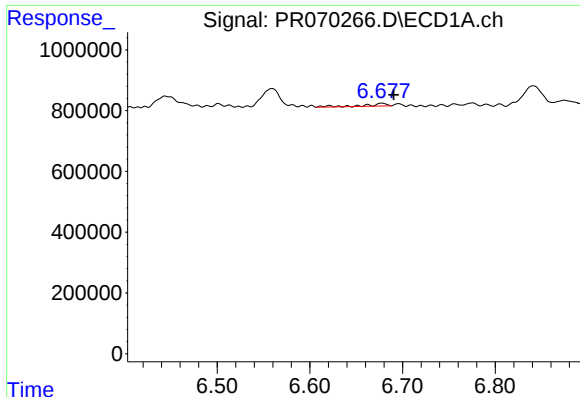

#29 AR-1254-4


R.T.: 6.678 min
Delta R.T.: -0.013 min
Response: 135090
Conc: 4.23 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

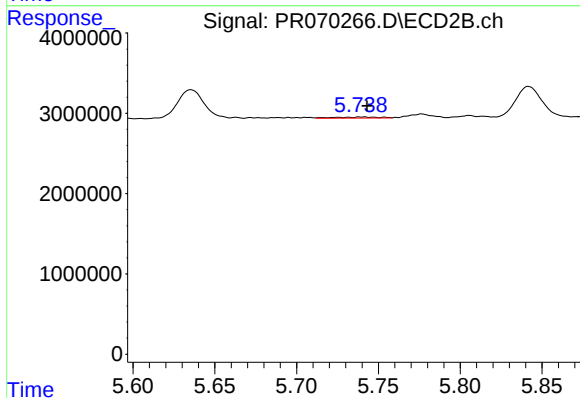


#29 AR-1254-4

R.T.: 5.741 min
Delta R.T.: -0.002 min
Response: 253658
Conc: 1.58 ng/ml

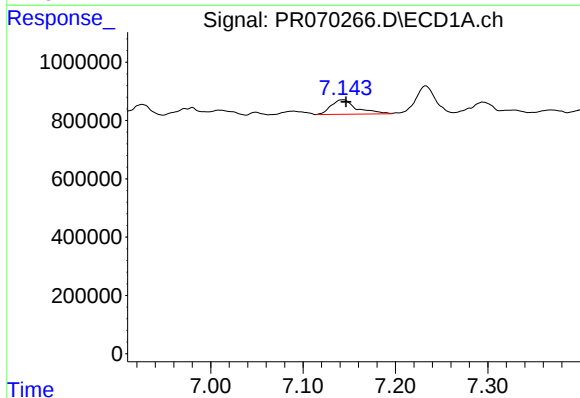


#30 AR-1254-5

R.T.: 7.143 min
Delta R.T.: -0.004 min
Response: 967220
Conc: 25.05 ng/ml

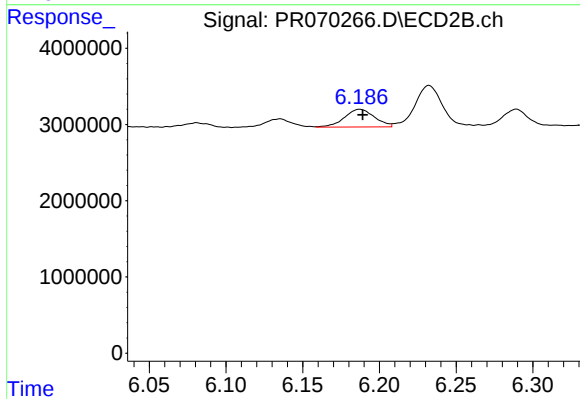

#30 AR-1254-5


R.T.: 6.187 min
Delta R.T.: -0.002 min
Response: 3200073
Conc: 12.30 ng/ml

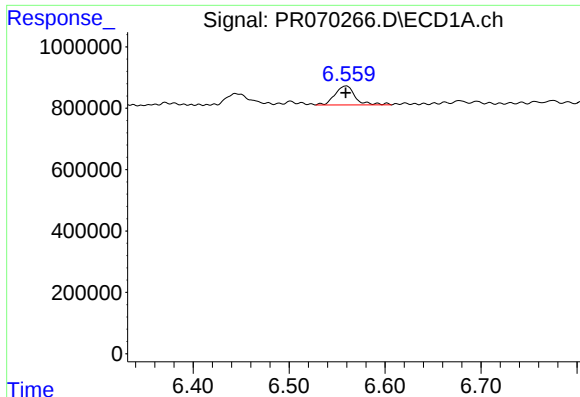

#31 AR-1260-1


R.T.: 6.559 min
Delta R.T.: 0.000 min
Response: 907904
Conc: 20.96 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

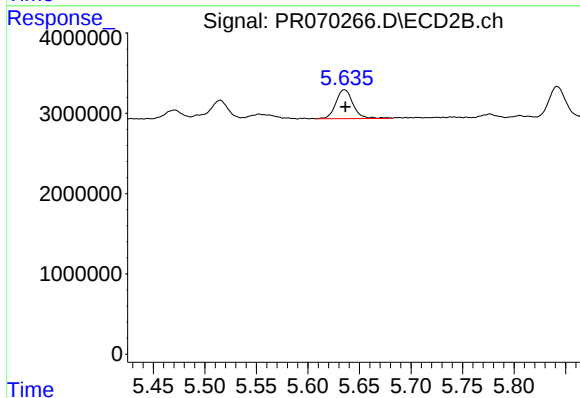


#31 AR-1260-1

R.T.: 5.635 min
Delta R.T.: 0.000 min
Response: 4204600
Conc: 19.11 ng/ml

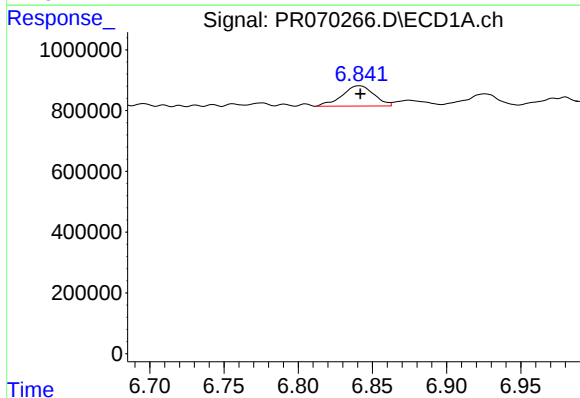


#32 AR-1260-2

R.T.: 6.841 min
Delta R.T.: 0.000 min
Response: 1003901
Conc: 22.20 ng/ml

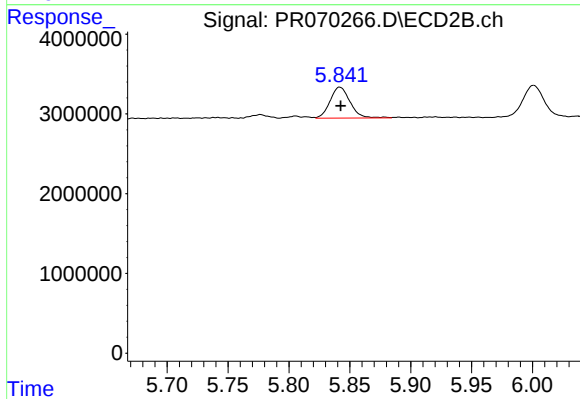

#32 AR-1260-2


R.T.: 5.842 min
Delta R.T.: 0.000 min
Response: 4419455
Conc: 17.95 ng/ml

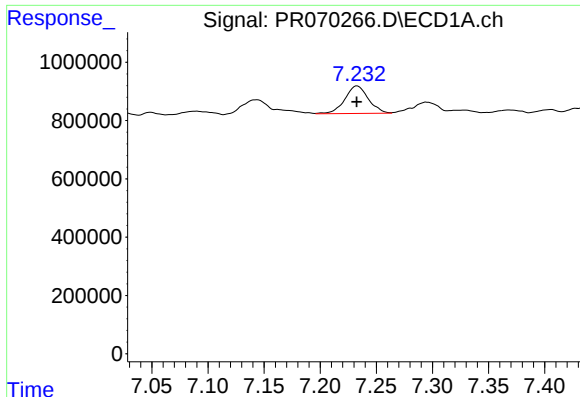

#33 AR-1260-3


R.T.: 7.233 min
Delta R.T.: 0.000 min
Response: 1384499
Conc: 37.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

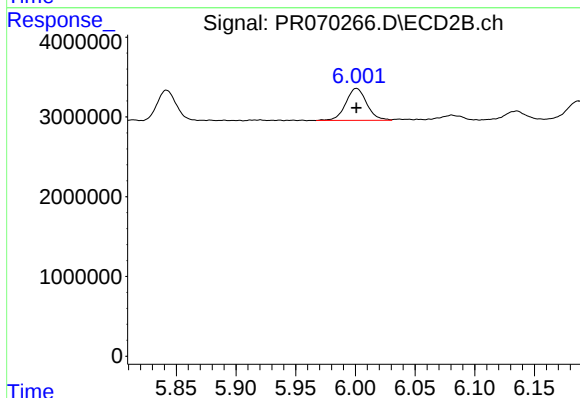


#33 AR-1260-3

R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 4923320
Conc: 20.66 ng/ml

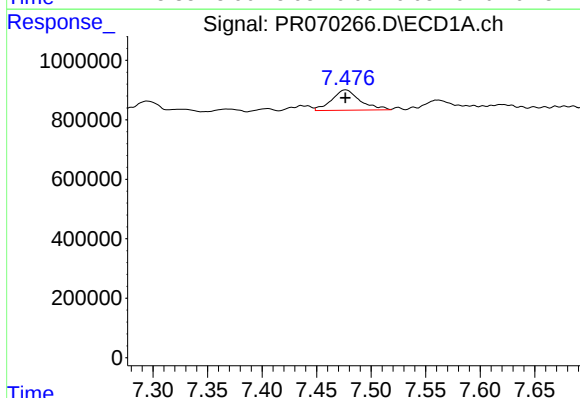


#34 AR-1260-4

R.T.: 7.477 min
Delta R.T.: 0.000 min
Response: 1238581
Conc: 31.10 ng/ml

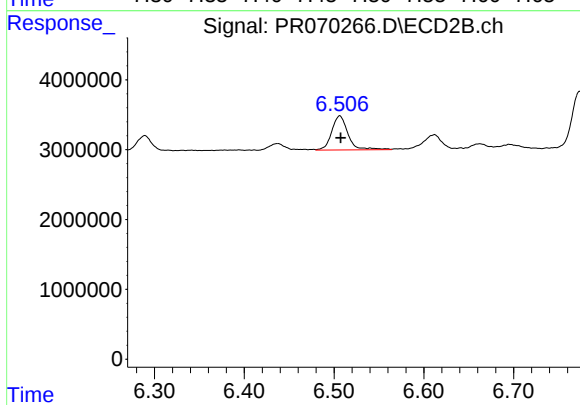

#34 AR-1260-4


R.T.: 6.506 min
Delta R.T.: -0.001 min
Response: 6217352
Conc: 31.56 ng/ml

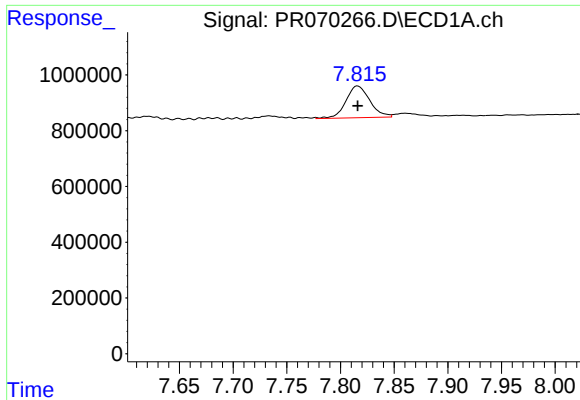

#35 AR-1260-5


R.T.: 7.816 min
Delta R.T.: 0.000 min
Response: 1751725
Conc: 27.24 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

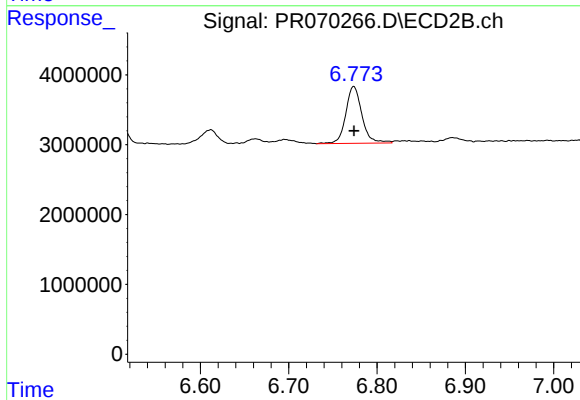


#35 AR-1260-5

R.T.: 6.774 min
Delta R.T.: 0.000 min
Response: 10316494
Conc: 25.07 ng/ml

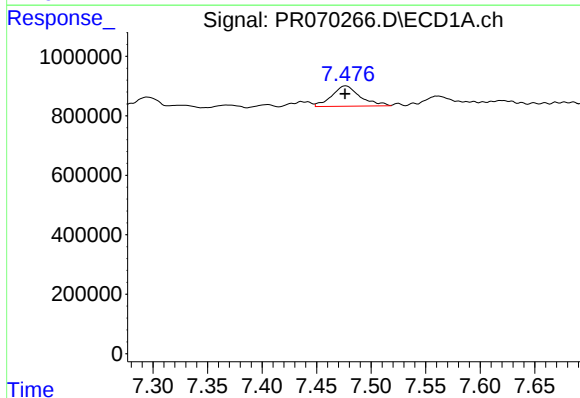


#36 AR-1262-1

R.T.: 7.477 min
Delta R.T.: 0.000 min
Response: 1238581
Conc: 24.56 ng/ml

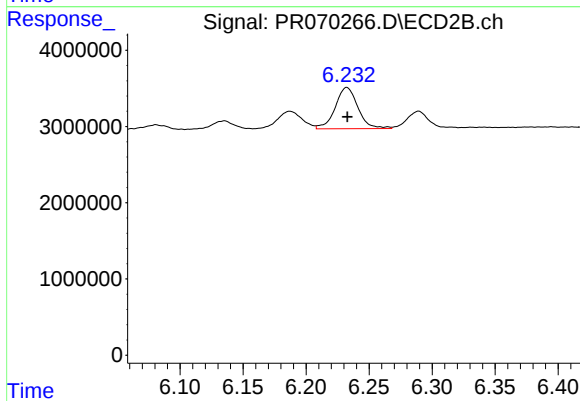

#36 AR-1262-1


R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 6787417
Conc: 22.05 ng/ml

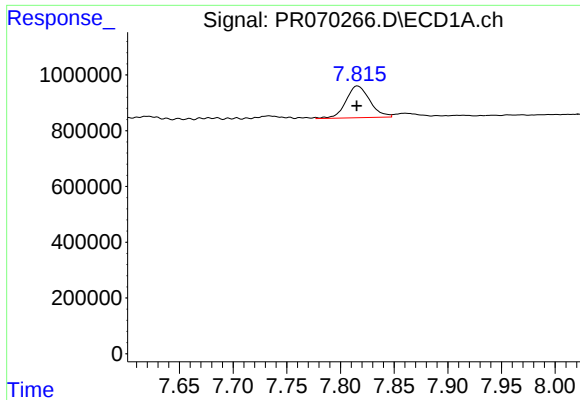

#37 AR-1262-2


R.T.: 7.816 min
Delta R.T.: 0.000 min
Response: 1751725
Conc: 23.18 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

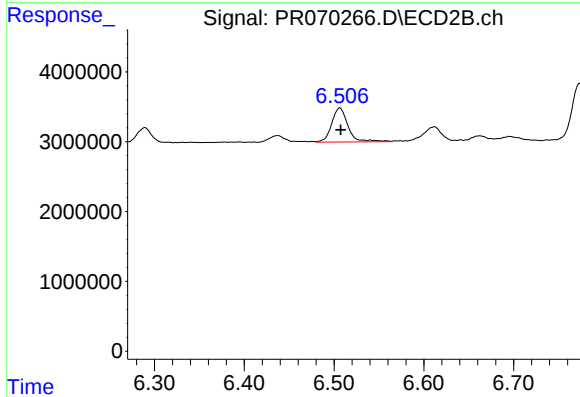


#37 AR-1262-2

R.T.: 6.506 min
Delta R.T.: 0.000 min
Response: 6217352
Conc: 23.02 ng/ml

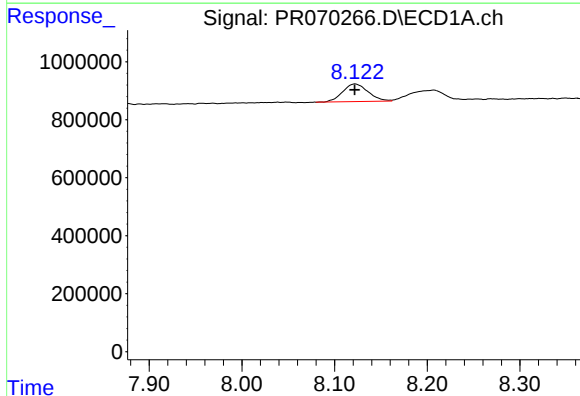


#38 AR-1262-3

R.T.: 8.122 min
Delta R.T.: 0.000 min
Response: 1154181
Conc: 21.63 ng/ml

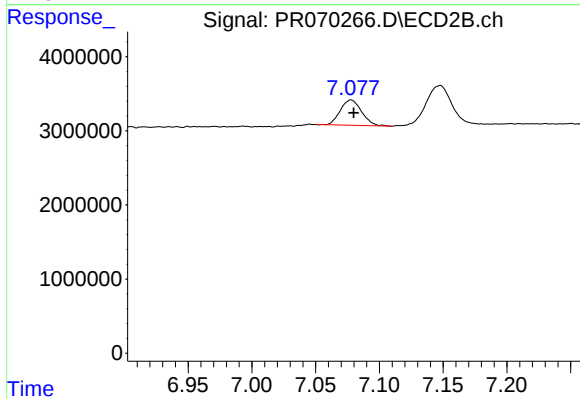

#38 AR-1262-3


R.T.: 7.078 min
Delta R.T.: -0.002 min
Response: 3967176
Conc: 20.23 ng/ml

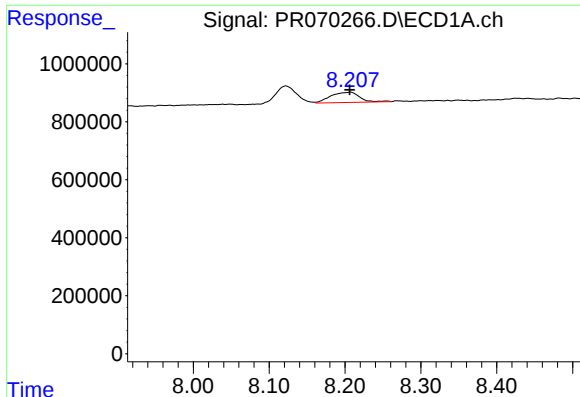

#39 AR-1262-4


R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 926052
Conc: 21.04 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

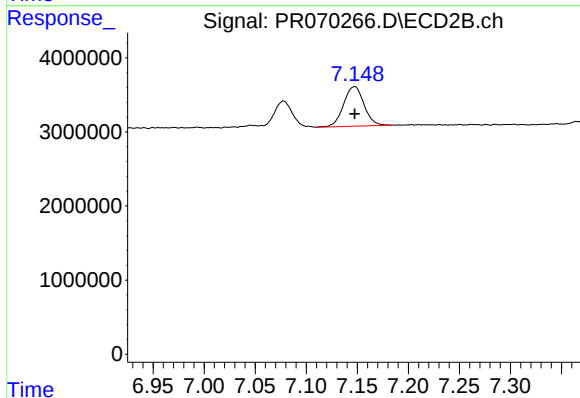


#39 AR-1262-4

R.T.: 7.147 min
Delta R.T.: 0.000 min
Response: 7436574
Conc: 20.63 ng/ml

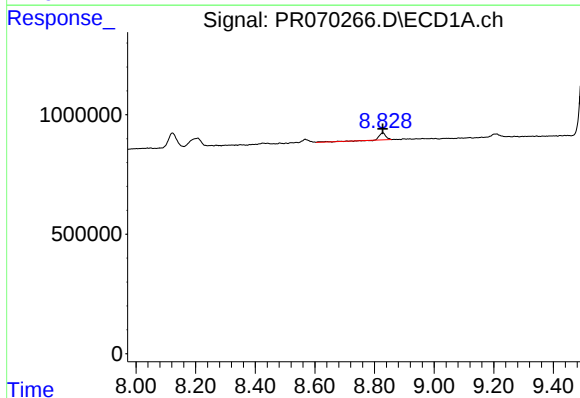


#40 AR-1262-5

R.T.: 8.828 min
Delta R.T.: 0.000 min
Response: 495987
Conc: 20.51 ng/ml

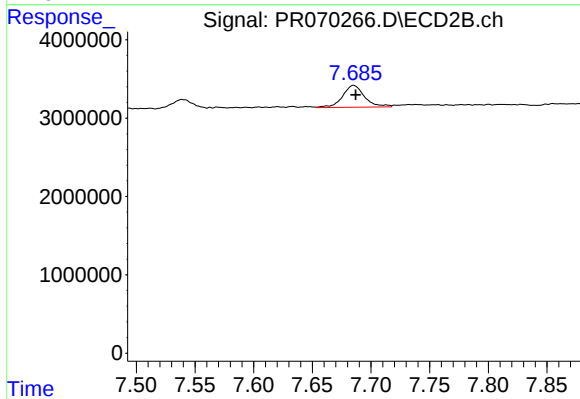

#40 AR-1262-5


R.T.: 7.685 min
Delta R.T.: -0.002 min
Response: 3636042
Conc: 23.84 ng/ml

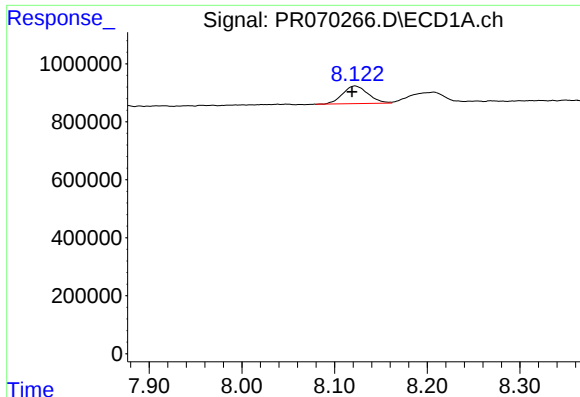

#41 AR-1268-1


R.T.: 8.122 min
Delta R.T.: 0.004 min
Response: 1154181
Conc: 11.82 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

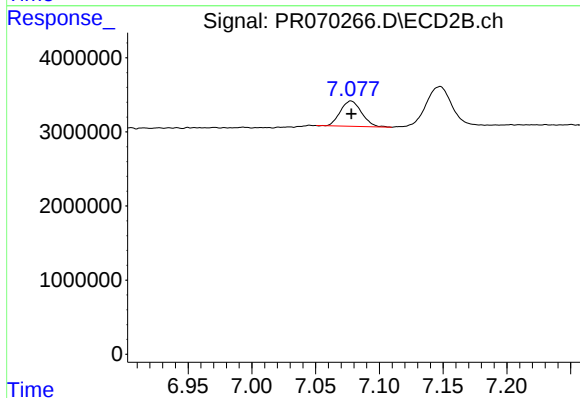


#41 AR-1268-1

R.T.: 7.078 min
Delta R.T.: 0.000 min
Response: 3967176
Conc: 6.94 ng/ml

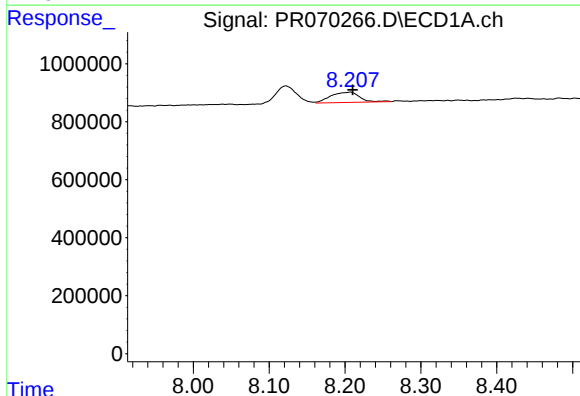


#42 AR-1268-2

R.T.: 8.207 min
Delta R.T.: -0.003 min
Response: 926052
Conc: 10.37 ng/ml

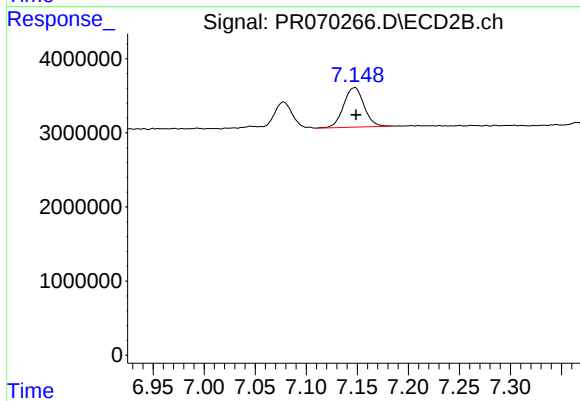

#42 AR-1268-2


R.T.: 7.147 min
Delta R.T.: -0.002 min
Response: 7436574
Conc: 14.20 ng/ml

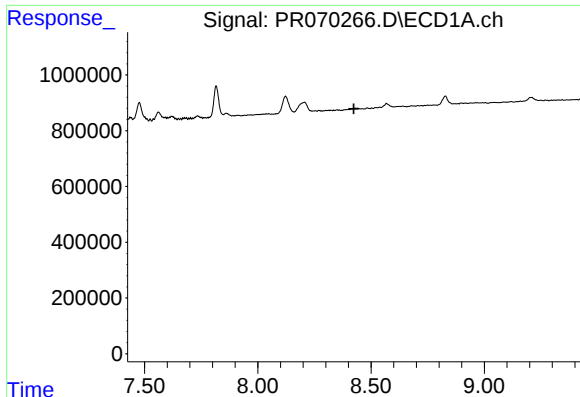

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

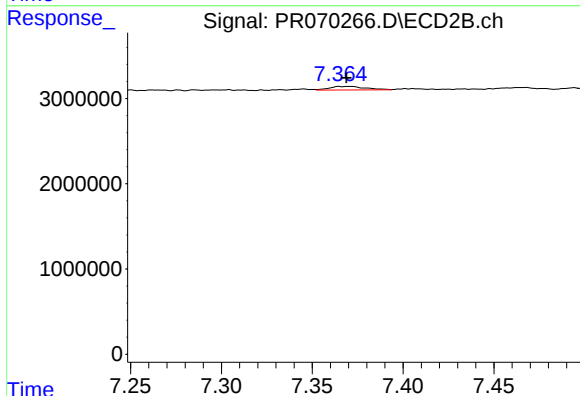


#43 AR-1268-3

R.T.: 7.371 min
Delta R.T.: 0.002 min
Response: 595951
Conc: 1.22 ng/ml

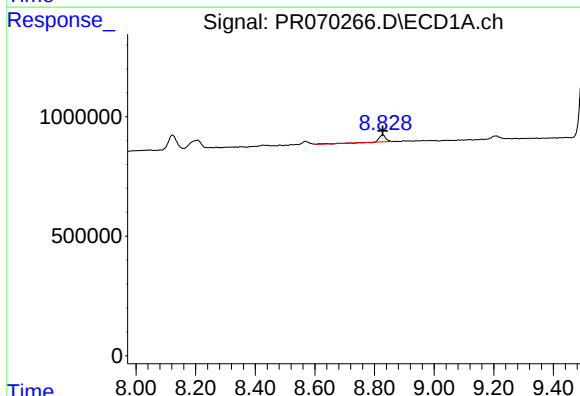


#44 AR-1268-4

R.T.: 8.828 min
Delta R.T.: 0.000 min
Response: 495987
Conc: 18.62 ng/ml

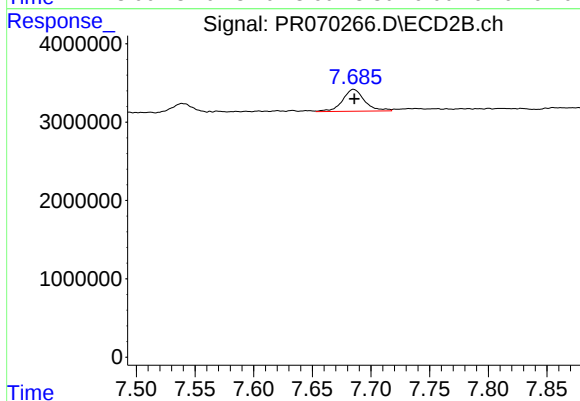

#44 AR-1268-4


R.T.: 7.685 min
Delta R.T.: 0.000 min
Response: 3636042
Conc: 21.25 ng/ml

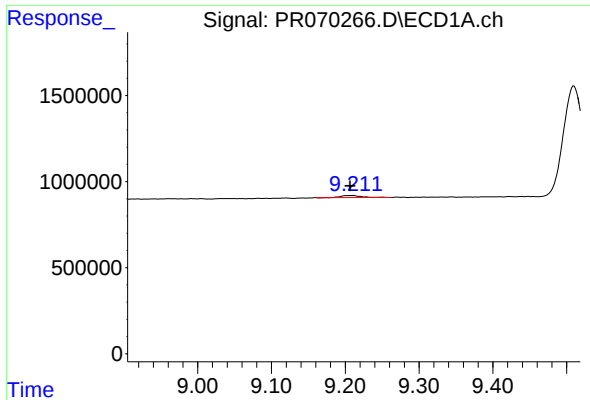

#45 AR-1268-5

R.T.: 9.209 min
Delta R.T.: 0.002 min
Response: 234091
Conc: 1.11 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

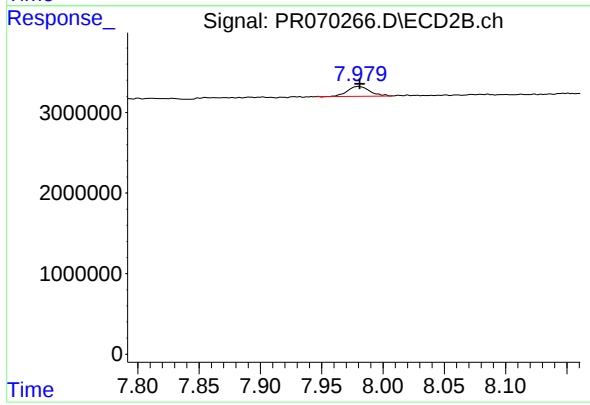

#45 AR-1268-5

R.T.: 7.980 min
Delta R.T.: -0.001 min
Response: 1548420
Conc: 1.12 ng/ml