

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR021025\
 Data File : PR070281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2025 23:15
 Operator : AJ\MA
 Sample : Q1168-07
 Misc : AR1221 LOD 40 PPB
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 00:52:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 10 14:13:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.624	2.956	19099319	98342787	16.914	16.865
2)	SA Decachlor...	9.508	8.223	13725665	77271495	19.200	18.872
Target Compounds							
3)	L1 AR-1016-1	0.000	4.074	0	403103	N.D.	2.556 #
4)	L1 AR-1016-2	0.000	4.091	0	702496	N.D.	2.949 #
5)	L1 AR-1016-3	0.000	4.269	0	313492	N.D.	2.498 #
6)	L1 AR-1016-4	0.000	4.325	0	132350	N.D.	1.204 #
7)	L1 AR-1016-5	0.000	4.539	0	347070	N.D.	2.544 #
8)	L2 AR-1221-1	3.840	3.178	692266	2308569	53.032	33.727 #
9)	L2 AR-1221-2	3.935	3.263	561064	2442578	57.468	47.703
10)	L2 AR-1221-3	4.012	3.342	1061913	4759191	34.723	30.568
11)	L3 AR-1232-1	4.012	3.342	1061913	4759191	44.775	39.800
12)	L3 AR-1232-2	0.000	4.091	0	702496	N.D.	6.328 #
13)	L3 AR-1232-3	0.000	4.269	0	313492	N.D.	5.432 #
14)	L3 AR-1232-4	0.000	4.366	0	115220	N.D.	2.171 #
15)	L3 AR-1232-5	0.000	4.539	0	347070	N.D.	6.066 #
16)	L4 AR-1242-1	0.000	4.074	0	403103	N.D.	3.117 #
17)	L4 AR-1242-2	0.000	4.091	0	702496	N.D.	3.612 #
18)	L4 AR-1242-3	0.000	4.269	0	313492	N.D.	3.012 #
19)	L4 AR-1242-4	0.000	4.366	0	115220	N.D.	1.124 #
20)	L4 AR-1242-5	0.000	4.914	0	711164	N.D.	6.206 #
21)	L5 AR-1248-1	0.000	4.074	0	403103	N.D.	4.178 #
22)	L5 AR-1248-2	0.000	4.325	0	132350	N.D.	0.912 #
23)	L5 AR-1248-3	0.000	4.366	0	115220	N.D.	0.778 #
24)	L5 AR-1248-4	0.000	4.539	0	347070	N.D.	1.975 #
25)	L5 AR-1248-5	0.000	4.951	0	1536267	N.D.	10.231 #
26)	L6 AR-1254-1	5.745	4.914	127125	711164	3.489	2.814
27)	L6 AR-1254-2	0.000	5.064	0	618184	N.D.	2.837 #
28)	L6 AR-1254-3	6.372	5.517f	131907	176143	2.469	0.552 #
29)	L6 AR-1254-4	6.674f	5.755	348286	156798	10.900	0.974 #
30)	L6 AR-1254-5	0.000	6.178	0	609438	N.D.	2.343 #
31)	L7 AR-1260-1	0.000	5.635	0	243414	N.D.	1.106 #
32)	L7 AR-1260-2	0.000	5.849	0	186272	N.D.	0.756 #
33)	L7 AR-1260-3	0.000	6.005	0	1768670	N.D.	7.421 #
34)	L7 AR-1260-4	0.000	6.505	0	486810	N.D.	2.471 #
35)	L7 AR-1260-5	0.000	6.771	0	653697	N.D.	1.589 #
36)	L8 AR-1262-1	0.000	6.229	0	237530	N.D.	0.772 #
37)	L8 AR-1262-2	0.000	6.505	0	486810	N.D.	1.802 #
38)	L8 AR-1262-3	0.000	7.063f	0	106127	N.D.	0.541 #
39)	L8 AR-1262-4	0.000	7.163f	0	207161	N.D.	0.575 #
41)	L9 AR-1268-1	0.000	7.063	0	106127	N.D.	0.186 #
42)	L9 AR-1268-2	0.000	7.163	0	207161	N.D.	0.396 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR021025\
 Data File : PR070281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Feb 2025 23:15
 Operator : AJ\MA
 Sample : Q1168-07
 Misc : AR1221 LOD 40 PPB
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 11 00:52:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 10 14:13:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	7.374	0	83930	N.D.	0.172 #
45) L9	AR-1268-5	0.000	7.981	0	439670	N.D.	0.317 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR021025\
Data File : PR070281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Feb 2025 23:15
Operator : AJ\MA
Sample : Q1168-07
Misc : AR1221 LOD 40 PPB
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 11 00:52:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021025.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 10 14:13:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

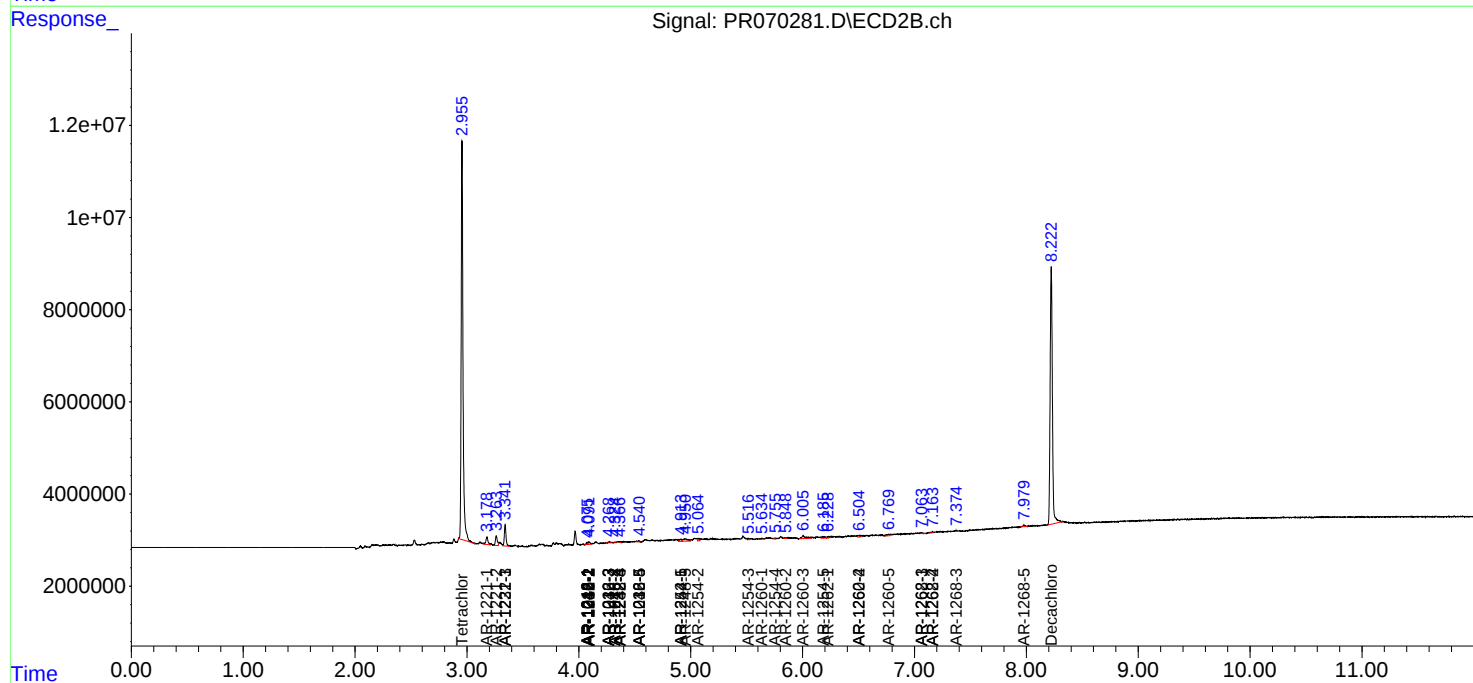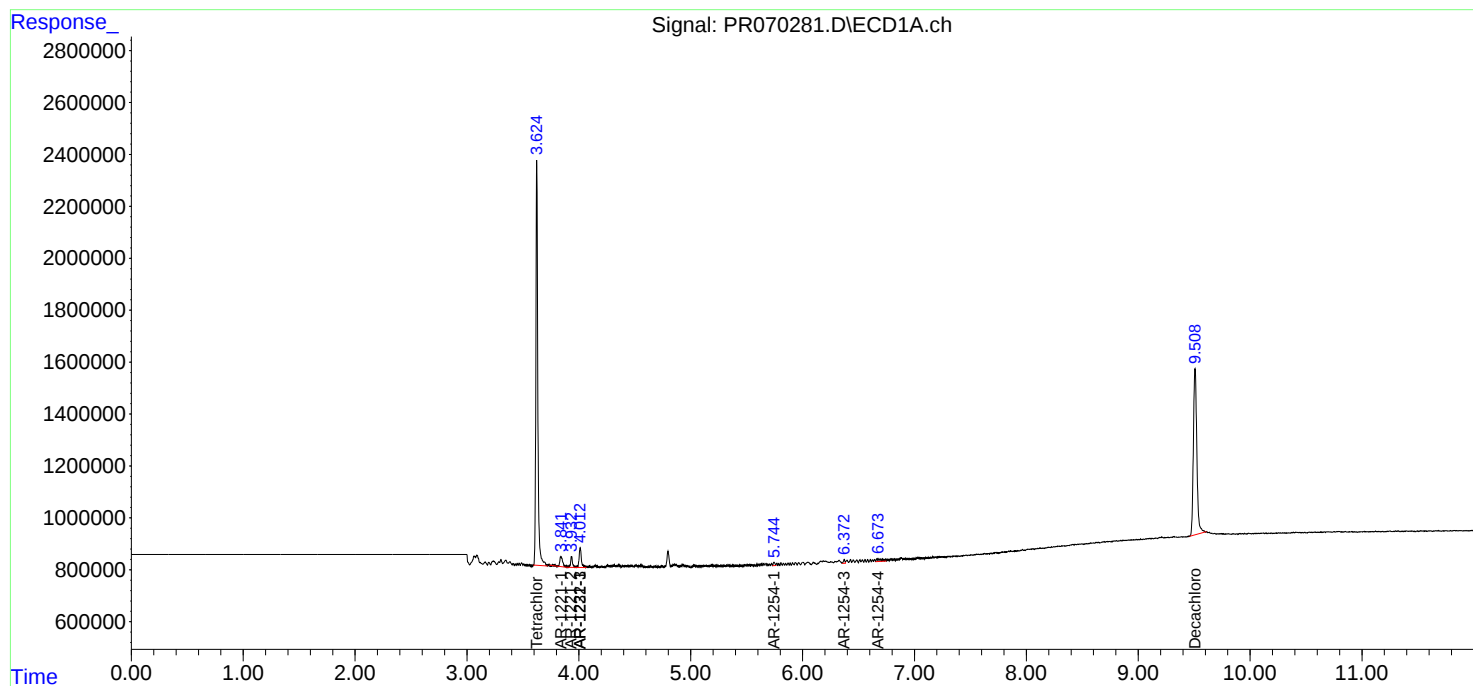


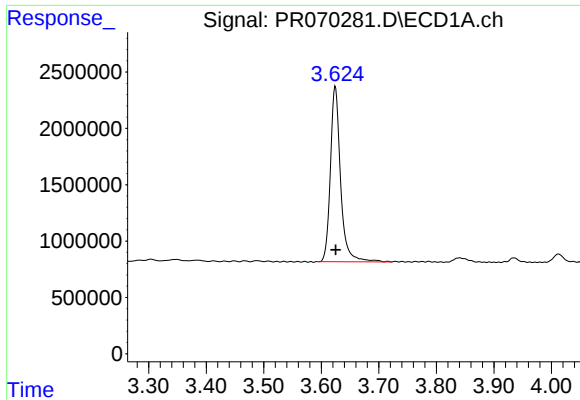

#1 Tetrachloro-m-xylene


R.T.: 3.624 min
Delta R.T.: 0.000 min
Response: 19099319
Conc: 16.91 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

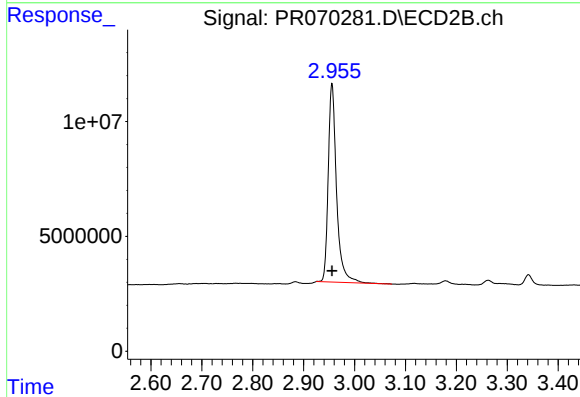


#1 Tetrachloro-m-xylene

R.T.: 2.956 min
Delta R.T.: 0.000 min
Response: 98342787
Conc: 16.86 ng/ml

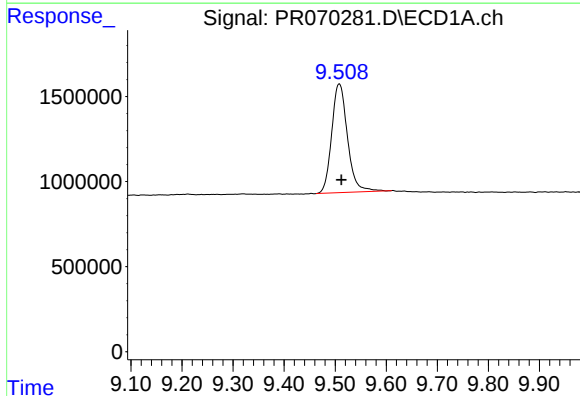


#2 Decachlorobiphenyl

R.T.: 9.508 min
Delta R.T.: -0.004 min
Response: 13725665
Conc: 19.20 ng/ml

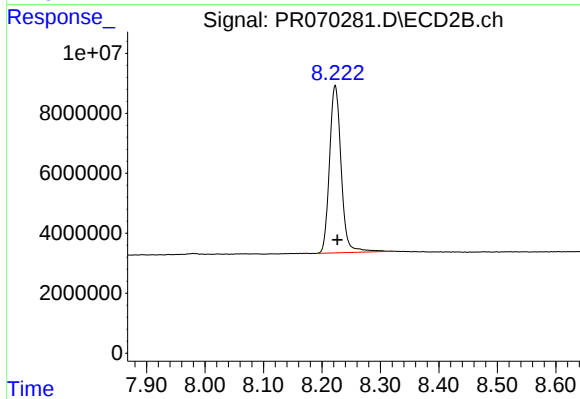

#2 Decachlorobiphenyl


R.T.: 8.223 min
Delta R.T.: -0.003 min
Response: 77271495
Conc: 18.87 ng/ml

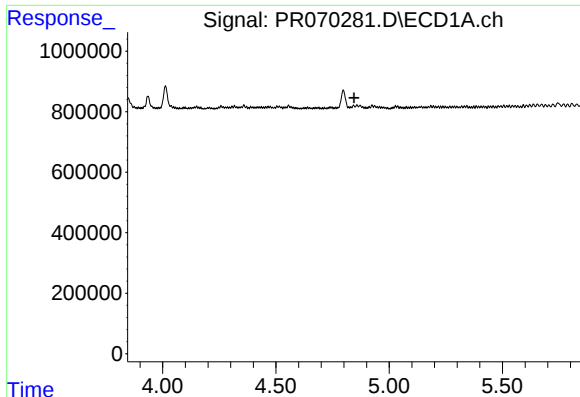

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 4.845 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

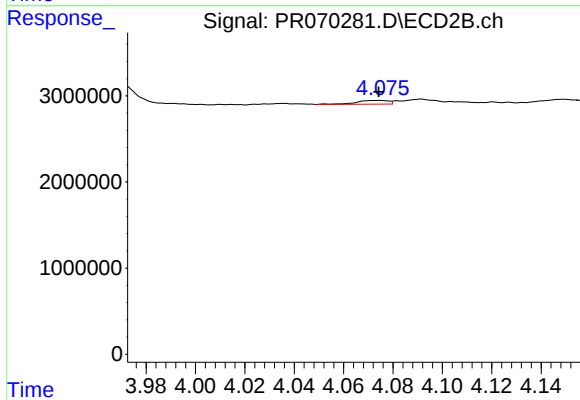


#3 AR-1016-1

R.T.: 4.074 min
Delta R.T.: 0.000 min
Response: 403103
Conc: 2.56 ng/ml

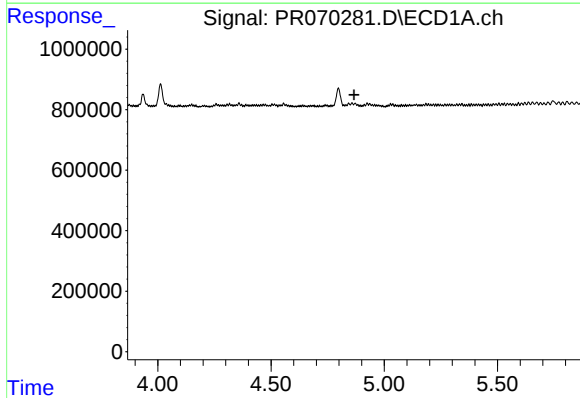


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 4.866 min
Response: 0
Conc: N.D.

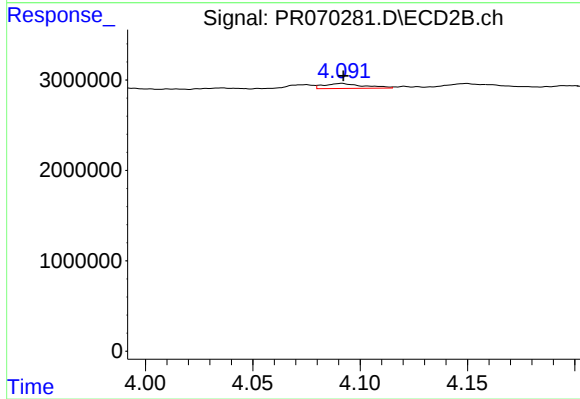

#4 AR-1016-2


R.T.: 4.091 min
Delta R.T.: 0.000 min
Response: 702496
Conc: 2.95 ng/ml

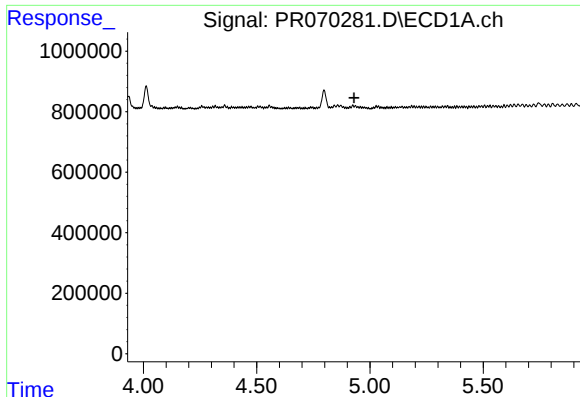

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 4.930 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

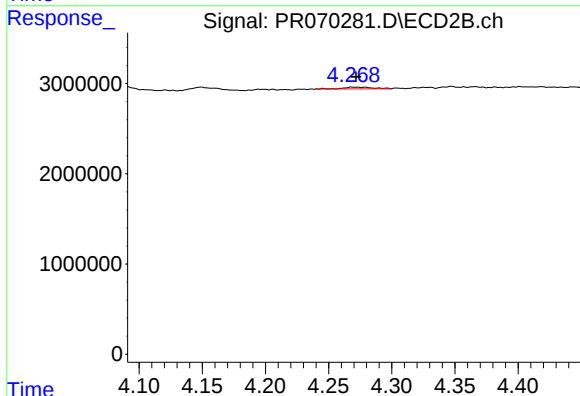


#5 AR-1016-3

R.T.: 4.269 min
Delta R.T.: -0.003 min
Response: 313492
Conc: 2.50 ng/ml

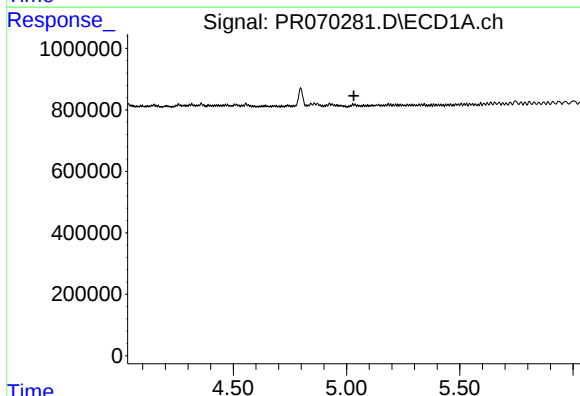


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.032 min
Response: 0
Conc: N.D.

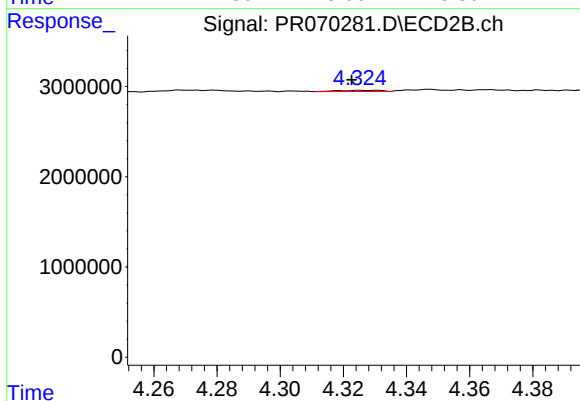

#6 AR-1016-4


R.T.: 4.325 min
Delta R.T.: 0.003 min
Response: 132350
Conc: 1.20 ng/ml

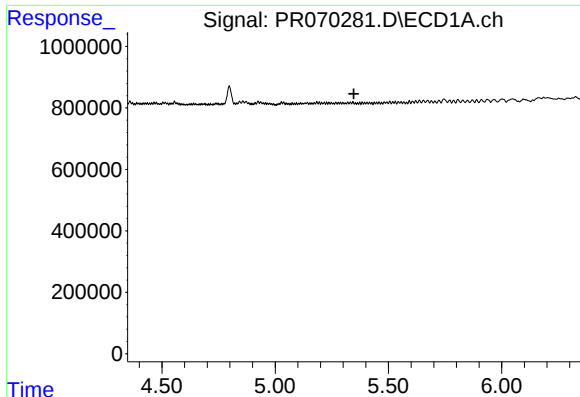

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

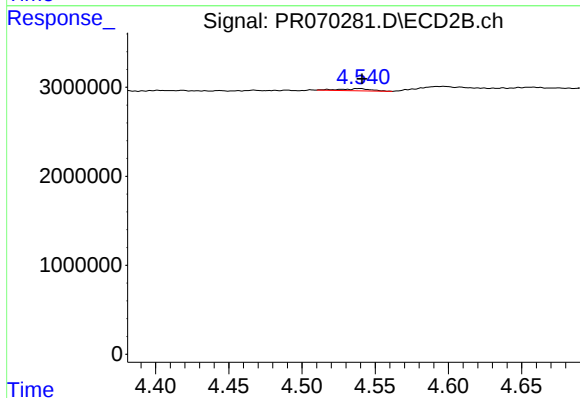


#7 AR-1016-5

R.T.: 4.539 min
Delta R.T.: -0.002 min
Response: 347070
Conc: 2.54 ng/ml

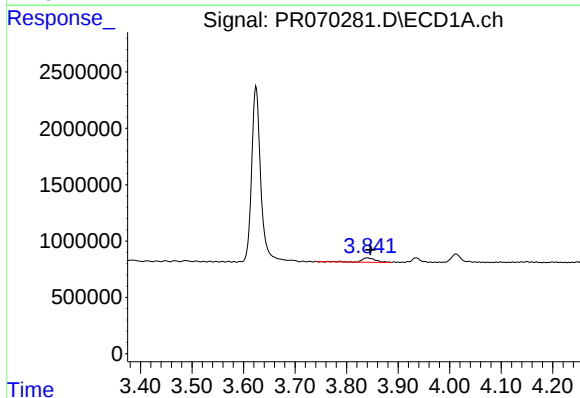


#8 AR-1221-1

R.T.: 3.840 min
Delta R.T.: -0.006 min
Response: 692266
Conc: 53.03 ng/ml

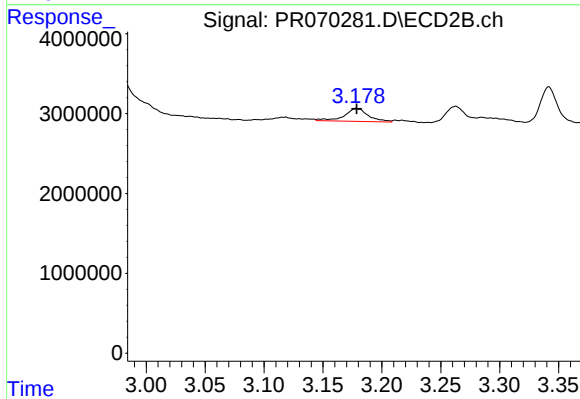

#8 AR-1221-1


R.T.: 3.178 min
Delta R.T.: 0.000 min
Response: 2308569
Conc: 33.73 ng/ml

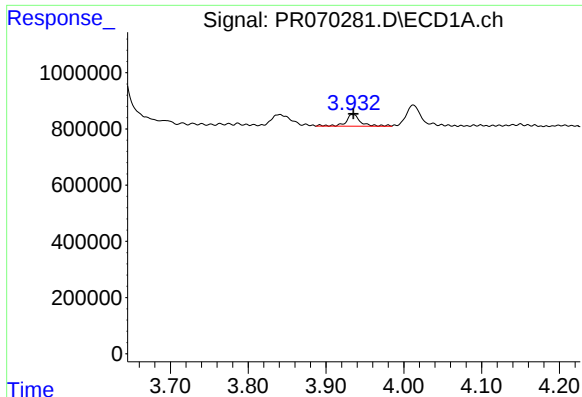

#9 AR-1221-2


R.T.: 3.935 min
Delta R.T.: 0.000 min
Response: 561064
Conc: 57.47 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

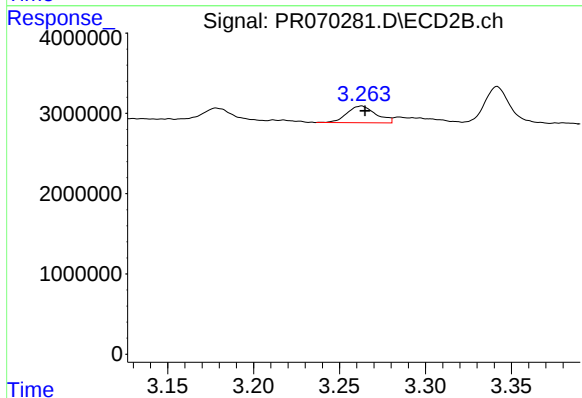


#9 AR-1221-2

R.T.: 3.263 min
Delta R.T.: -0.002 min
Response: 2442578
Conc: 47.70 ng/ml

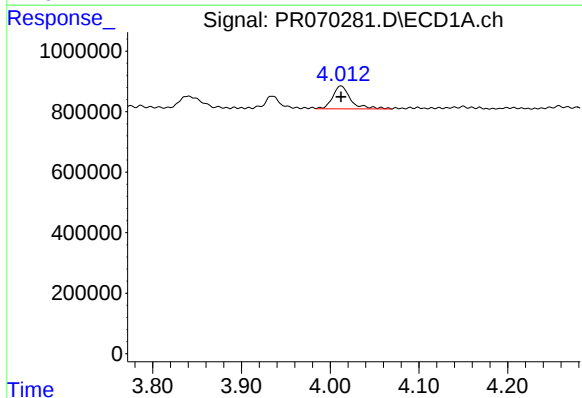


#10 AR-1221-3

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 1061913
Conc: 34.72 ng/ml

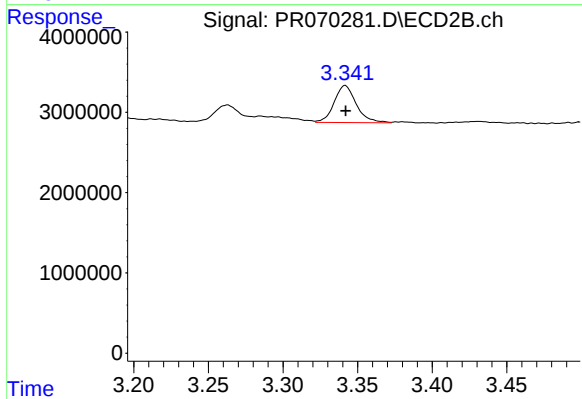

#10 AR-1221-3


R.T.: 3.342 min
Delta R.T.: 0.000 min
Response: 4759191
Conc: 30.57 ng/ml

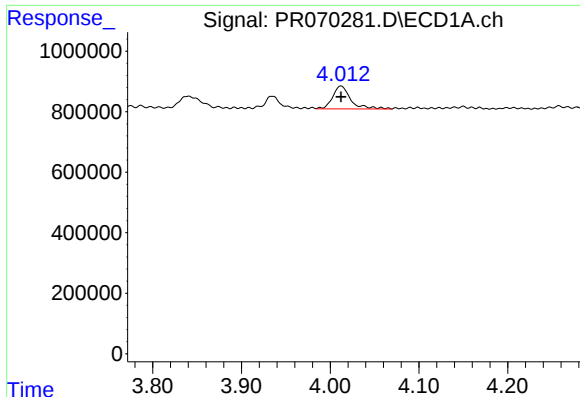

#11 AR-1232-1


R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 1061913
Conc: 44.78 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

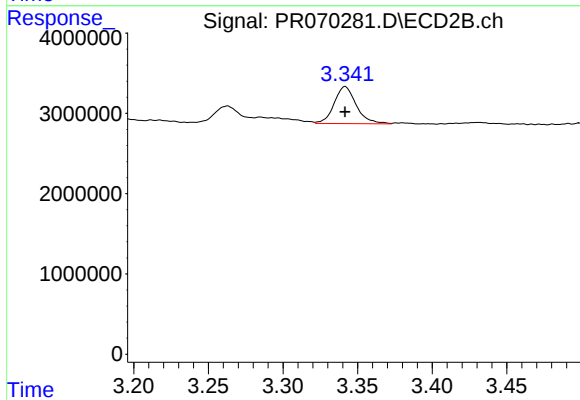


#11 AR-1232-1

R.T.: 3.342 min
Delta R.T.: 0.000 min
Response: 4759191
Conc: 39.80 ng/ml

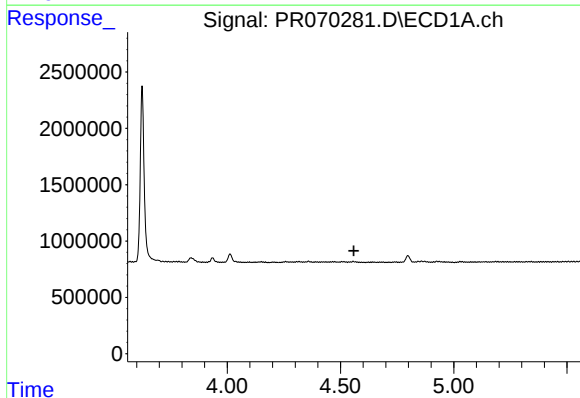


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.559 min
Response: 0
Conc: N.D.

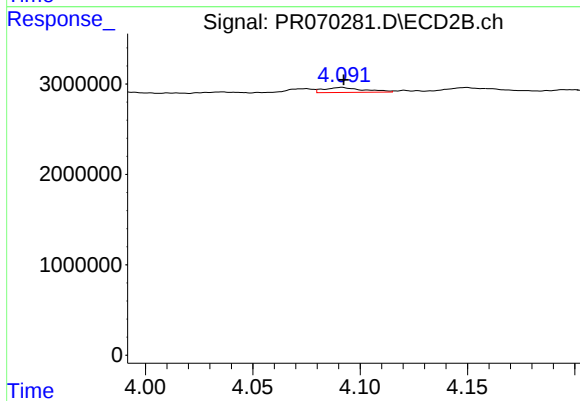

#12 AR-1232-2


R.T.: 4.091 min
Delta R.T.: -0.001 min
Response: 702496
Conc: 6.33 ng/ml

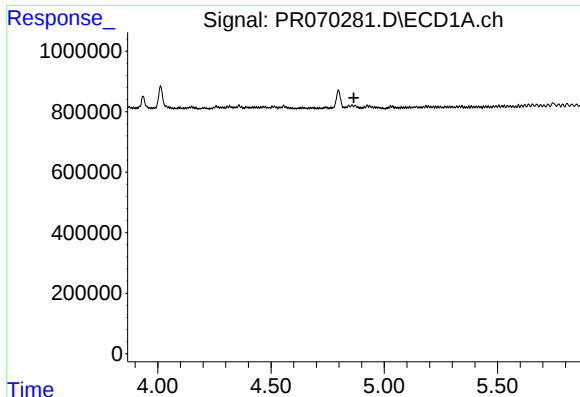

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 4.866 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

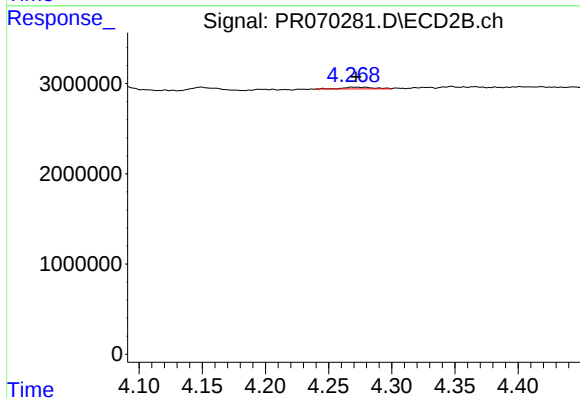


#13 AR-1232-3

R.T.: 4.269 min
Delta R.T.: -0.003 min
Response: 313492
Conc: 5.43 ng/ml

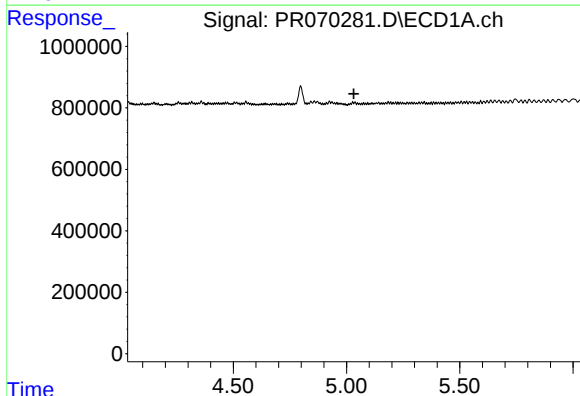


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T.: 5.032 min
Response: 0
Conc: N.D.

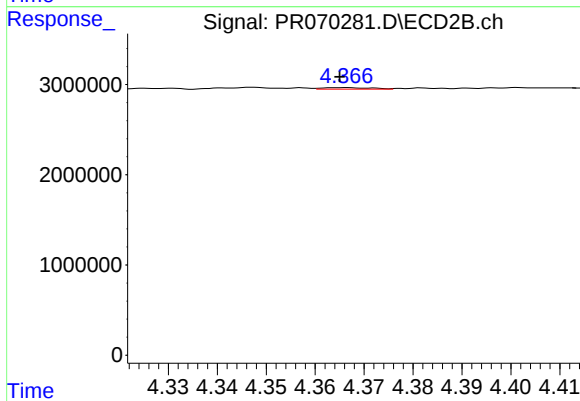

#14 AR-1232-4


R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 115220
Conc: 2.17 ng/ml

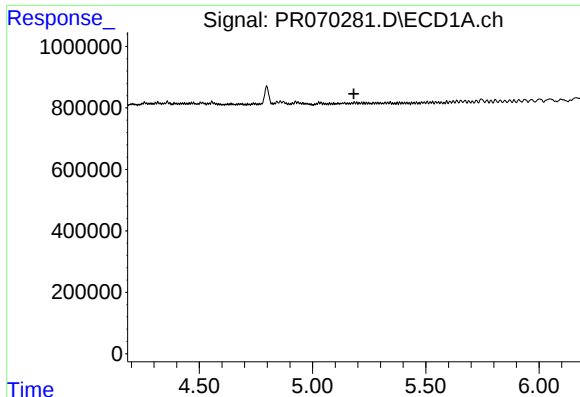

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

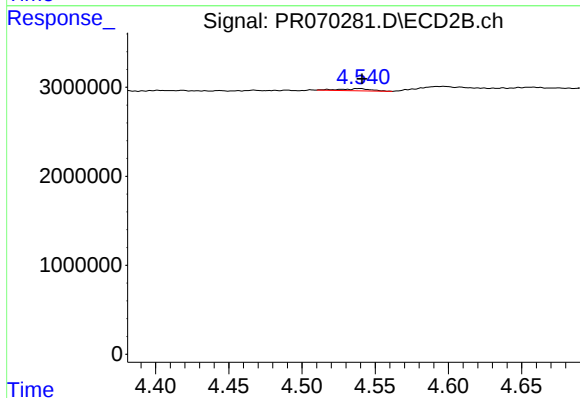


#15 AR-1232-5

R.T.: 4.539 min
Delta R.T.: -0.002 min
Response: 347070
Conc: 6.07 ng/ml

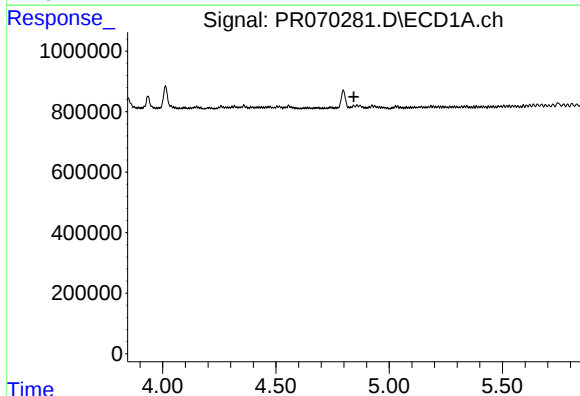


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T.: 4.844 min
Response: 0
Conc: N.D.

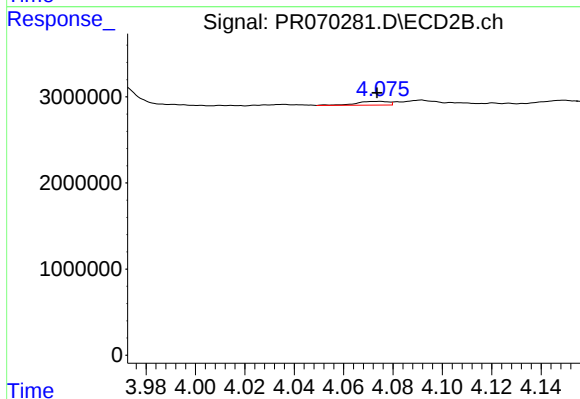

#16 AR-1242-1


R.T.: 4.074 min
Delta R.T.: 0.000 min
Response: 403103
Conc: 3.12 ng/ml

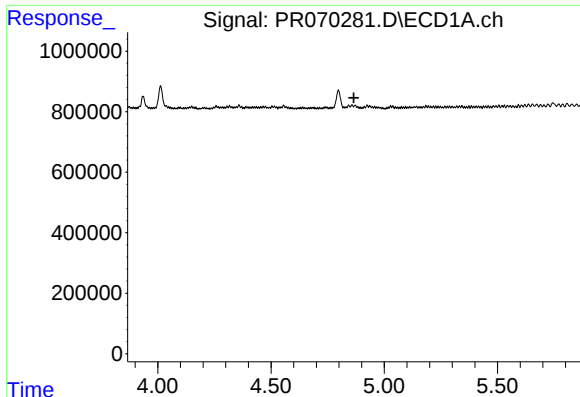

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 4.866 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

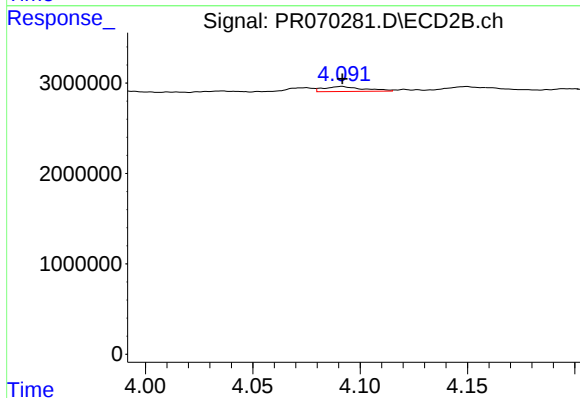


#17 AR-1242-2

R.T.: 4.091 min
Delta R.T.: 0.000 min
Response: 702496
Conc: 3.61 ng/ml

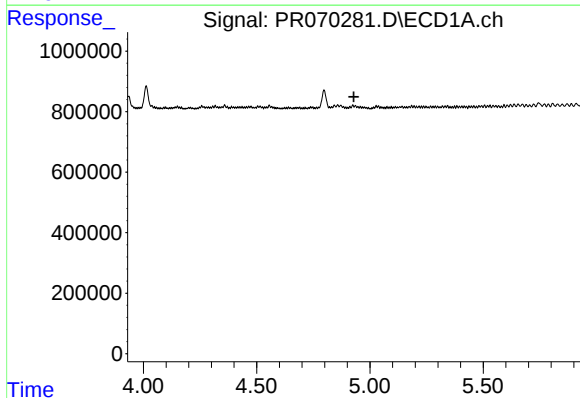


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 4.930 min
Response: 0
Conc: N.D.

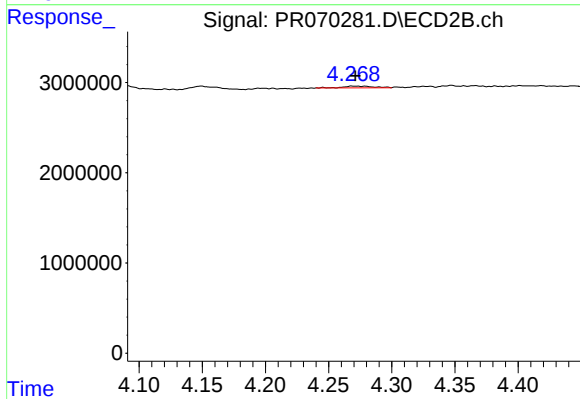

#18 AR-1242-3


R.T.: 4.269 min
Delta R.T.: -0.002 min
Response: 313492
Conc: 3.01 ng/ml

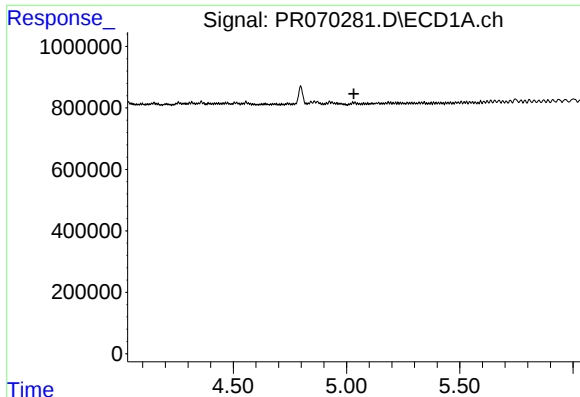

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.032 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

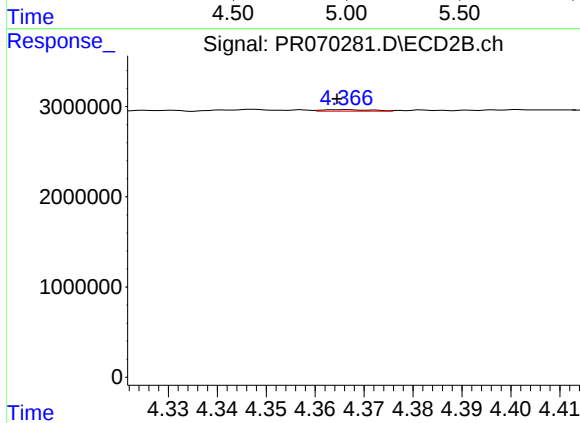


#19 AR-1242-4

R.T.: 4.366 min
Delta R.T.: 0.001 min
Response: 115220
Conc: 1.12 ng/ml

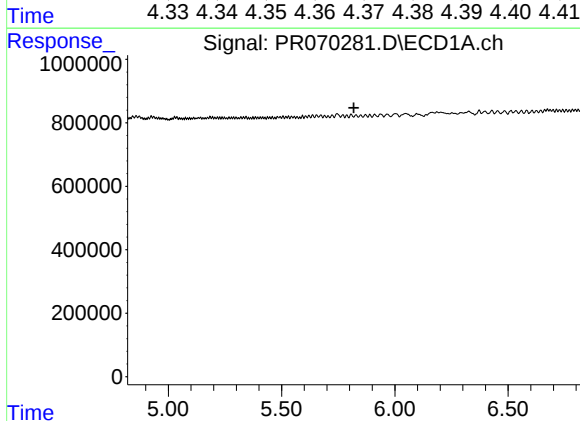


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 5.819 min
Response: 0
Conc: N.D.

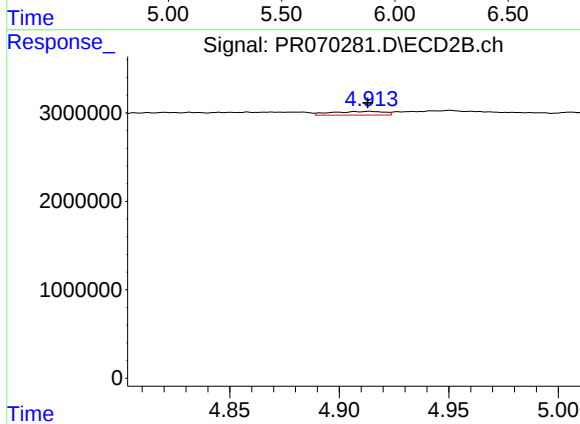

#20 AR-1242-5


R.T.: 4.914 min
Delta R.T.: 0.001 min
Response: 711164
Conc: 6.21 ng/ml

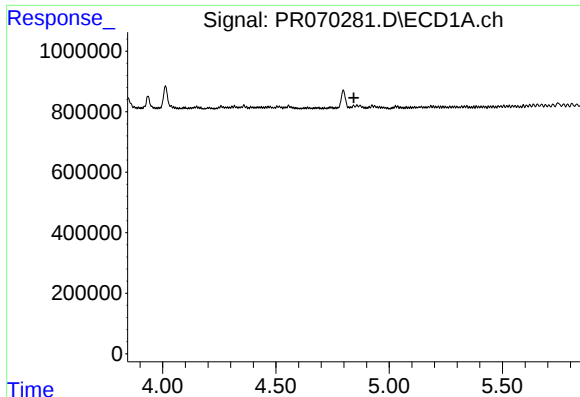

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 4.844 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

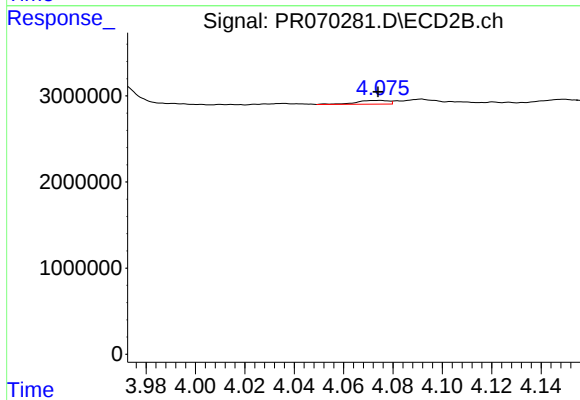


#21 AR-1248-1

R.T.: 4.074 min
Delta R.T.: 0.000 min
Response: 403103
Conc: 4.18 ng/ml

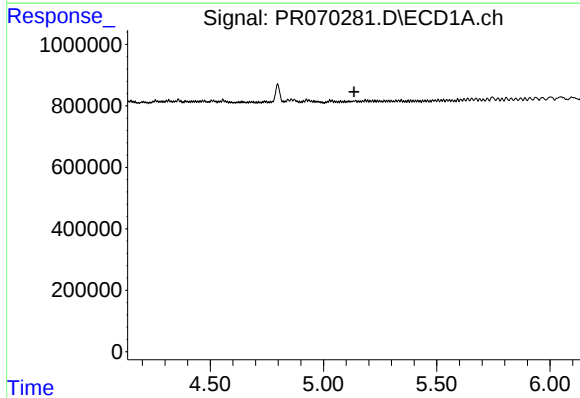


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 5.135 min
Response: 0
Conc: N.D.

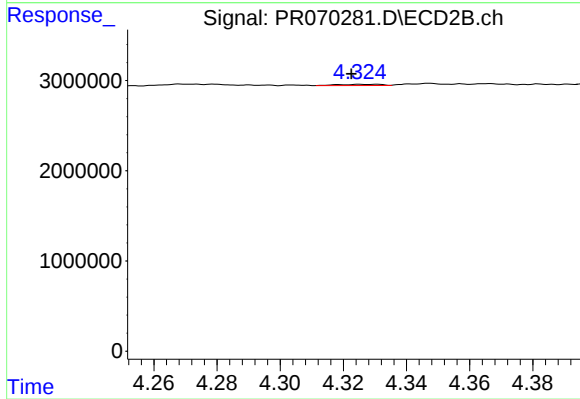

#22 AR-1248-2


R.T.: 4.325 min
Delta R.T.: 0.003 min
Response: 132350
Conc: 0.91 ng/ml

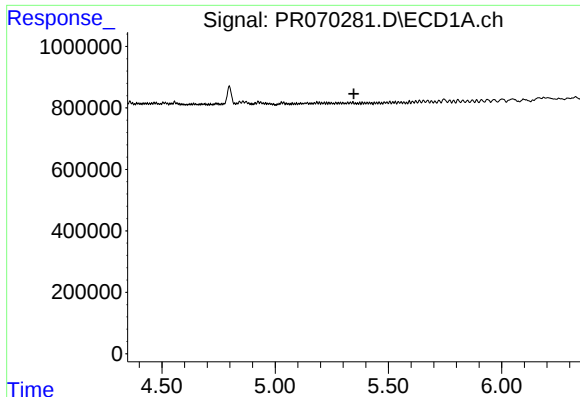

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.347 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

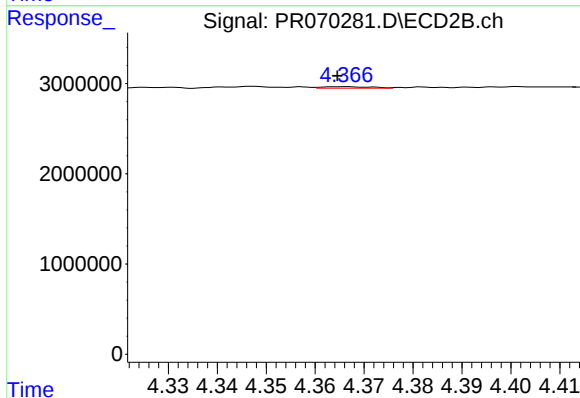


#23 AR-1248-3

R.T.: 4.366 min
Delta R.T.: 0.001 min
Response: 115220
Conc: 0.78 ng/ml

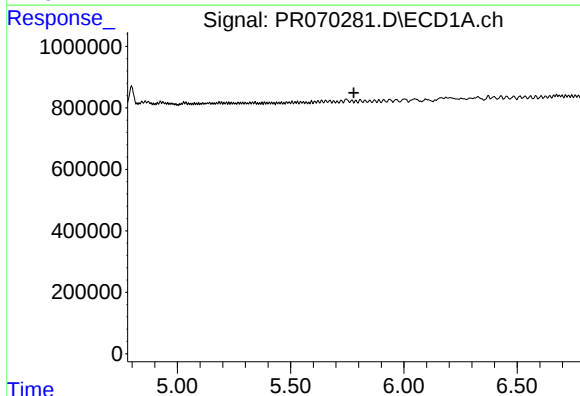


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 5.779 min
Response: 0
Conc: N.D.

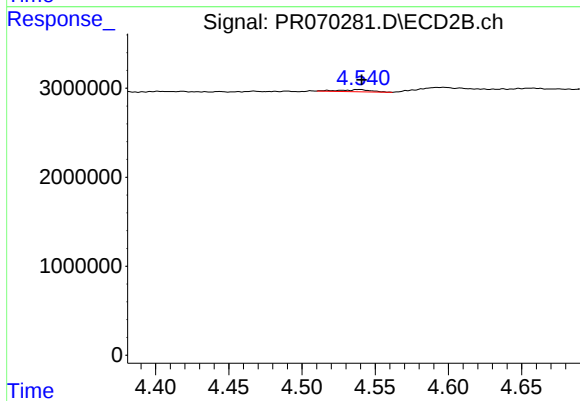

#24 AR-1248-4


R.T.: 4.539 min
Delta R.T.: -0.002 min
Response: 347070
Conc: 1.97 ng/ml

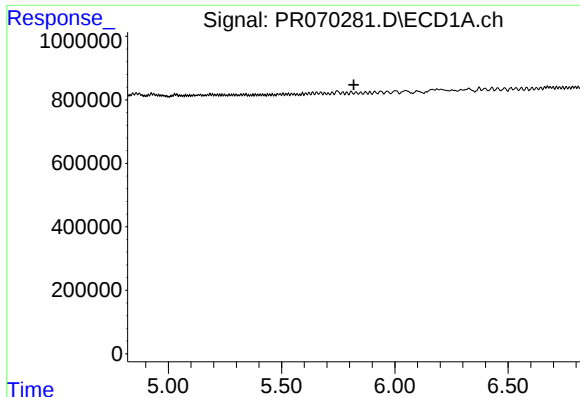

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 5.819 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

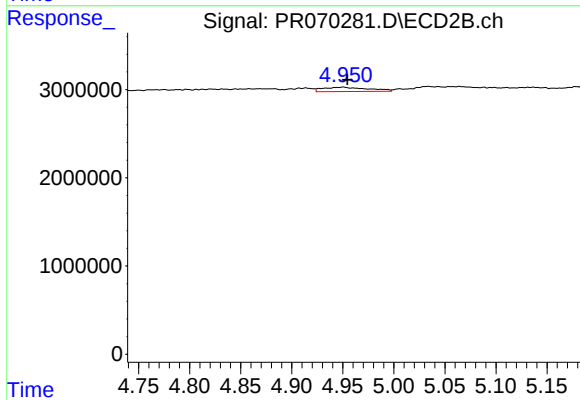


#25 AR-1248-5

R.T.: 4.951 min
Delta R.T.: -0.004 min
Response: 1536267
Conc: 10.23 ng/ml

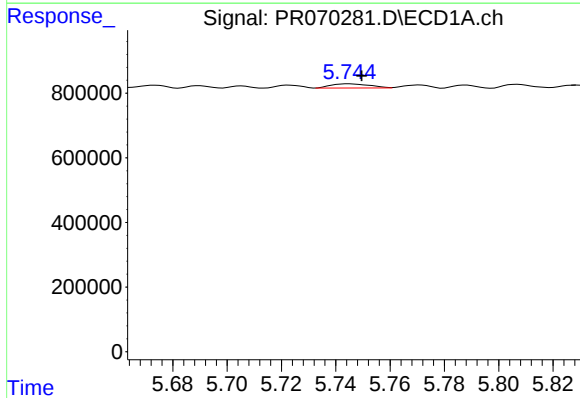


#26 AR-1254-1

R.T.: 5.745 min
Delta R.T.: -0.005 min
Response: 127125
Conc: 3.49 ng/ml

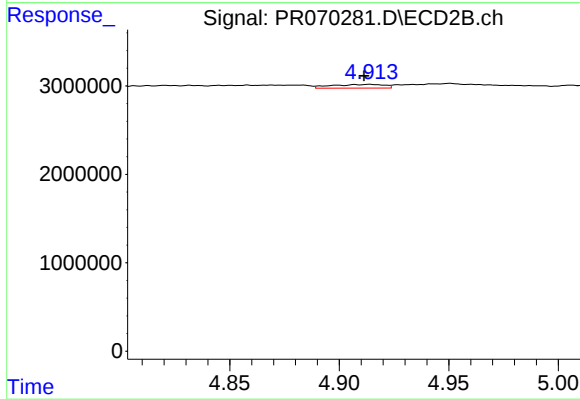

#26 AR-1254-1


R.T.: 4.914 min
Delta R.T.: 0.003 min
Response: 711164
Conc: 2.81 ng/ml

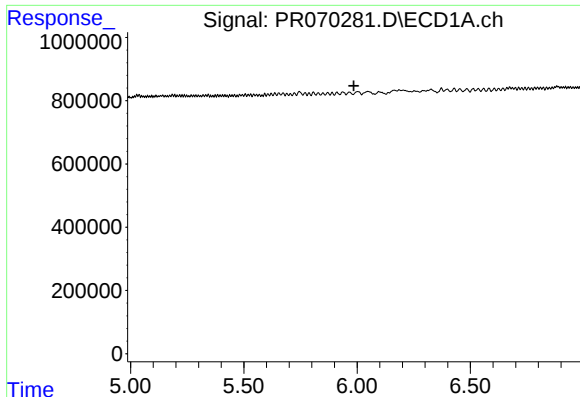

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 5.986 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

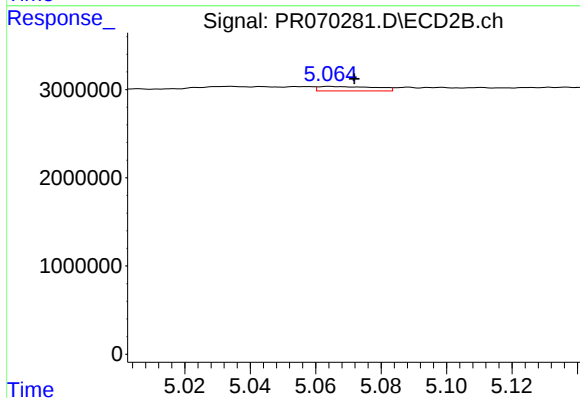


#27 AR-1254-2

R.T.: 5.064 min
Delta R.T.: -0.008 min
Response: 618184
Conc: 2.84 ng/ml

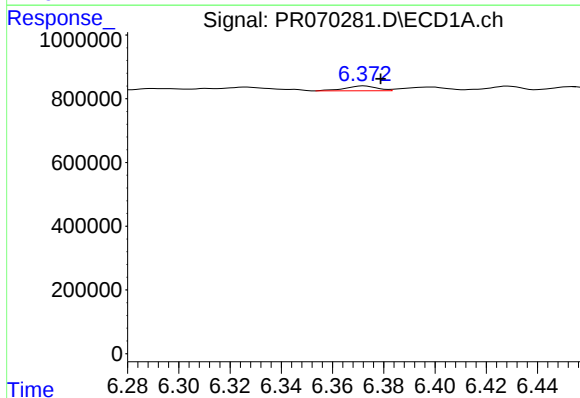


#28 AR-1254-3

R.T.: 6.372 min
Delta R.T.: -0.007 min
Response: 131907
Conc: 2.47 ng/ml

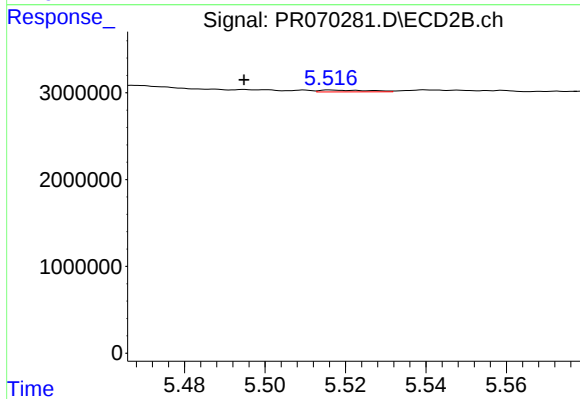

#28 AR-1254-3


R.T.: 5.517 min
Delta R.T.: 0.022 min
Response: 176143
Conc: 0.55 ng/ml

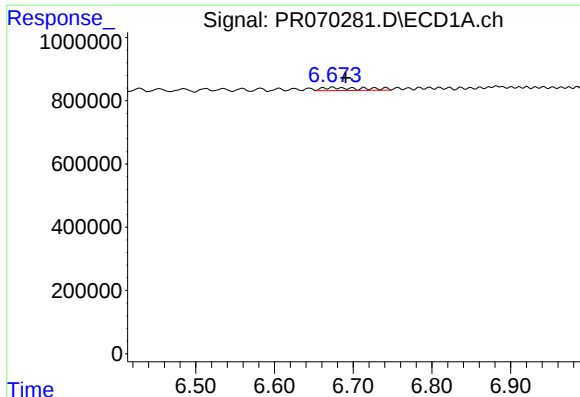

#29 AR-1254-4


R.T.: 6.674 min
Delta R.T.: -0.017 min
Response: 348286
Conc: 10.90 ng/ml

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

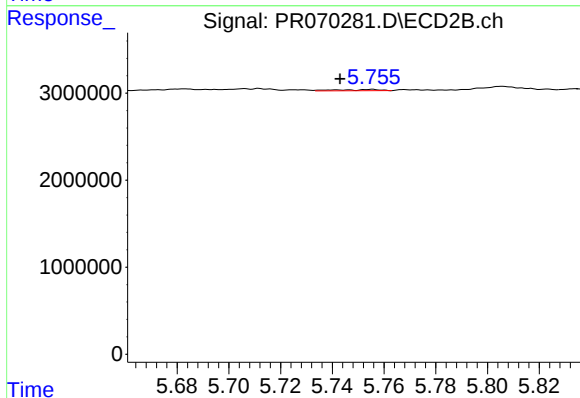


#29 AR-1254-4

R.T.: 5.755 min
Delta R.T.: 0.012 min
Response: 156798
Conc: 0.97 ng/ml

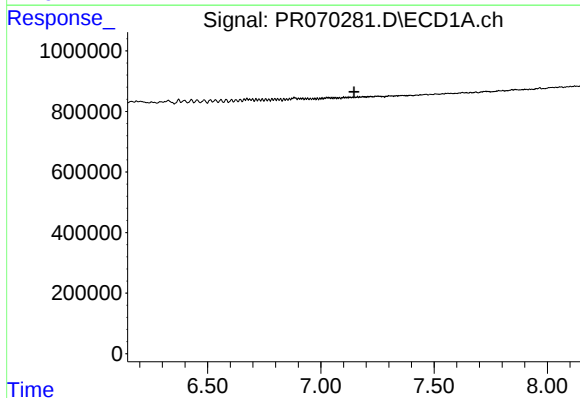


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.147 min
Response: 0
Conc: N.D.

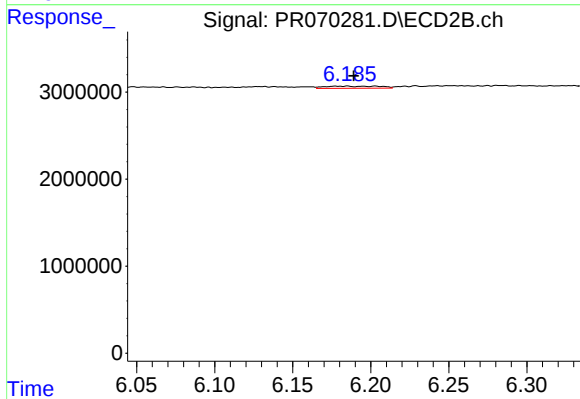

#30 AR-1254-5


R.T.: 6.178 min
Delta R.T.: -0.012 min
Response: 609438
Conc: 2.34 ng/ml

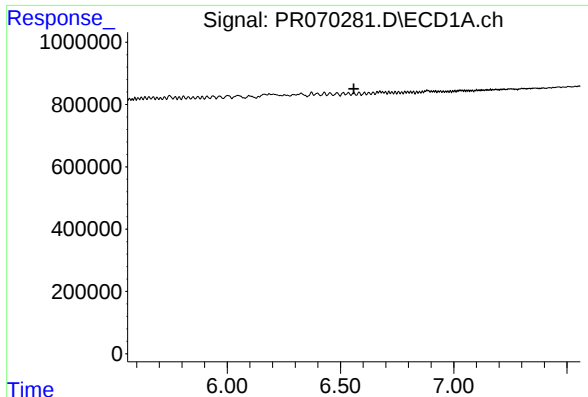

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 6.559 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

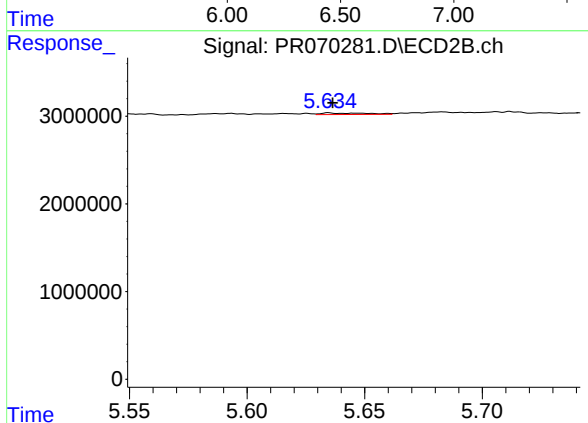


#31 AR-1260-1

R.T.: 5.635 min
Delta R.T.: -0.002 min
Response: 243414
Conc: 1.11 ng/ml

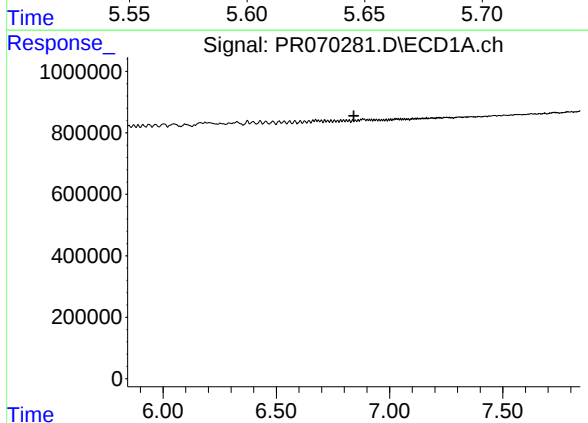


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 6.842 min
Response: 0
Conc: N.D.

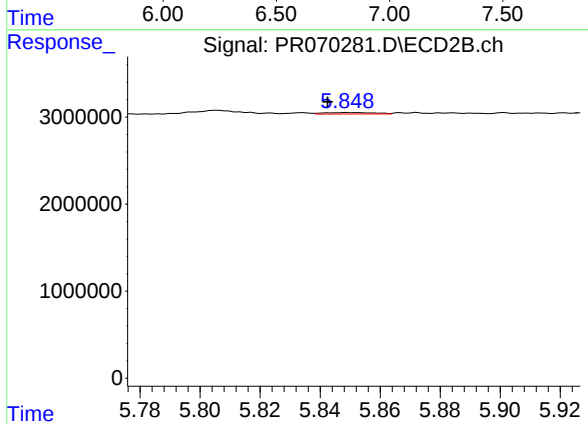

#32 AR-1260-2


R.T.: 5.849 min
Delta R.T.: 0.007 min
Response: 186272
Conc: 0.76 ng/ml

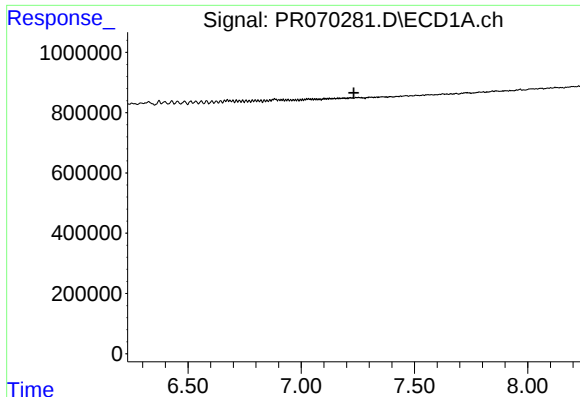

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.233 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

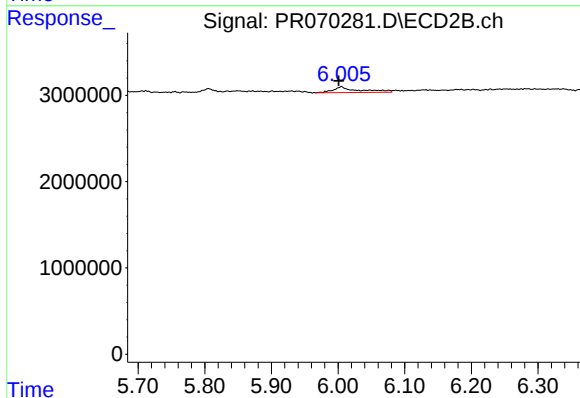


#33 AR-1260-3

R.T.: 6.005 min
Delta R.T.: 0.004 min
Response: 1768670
Conc: 7.42 ng/ml

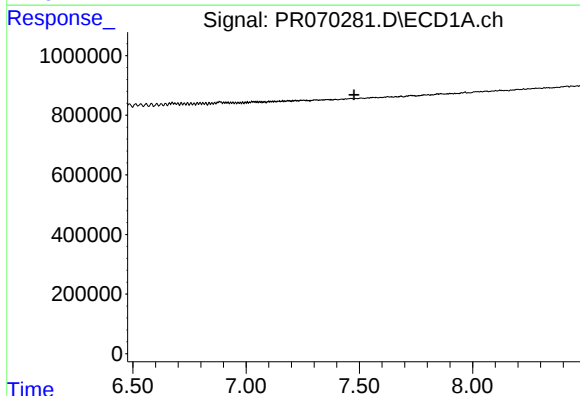


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.476 min
Response: 0
Conc: N.D.

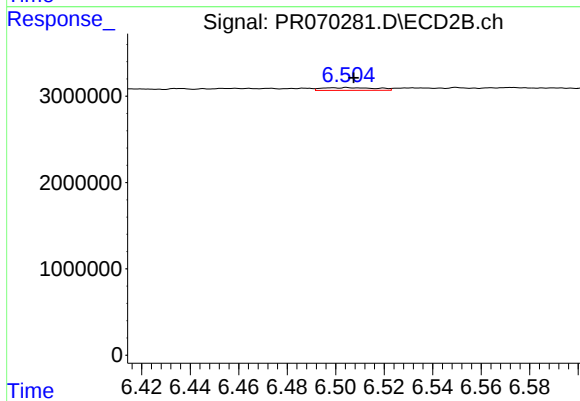

#34 AR-1260-4


R.T.: 6.505 min
Delta R.T.: -0.003 min
Response: 486810
Conc: 2.47 ng/ml

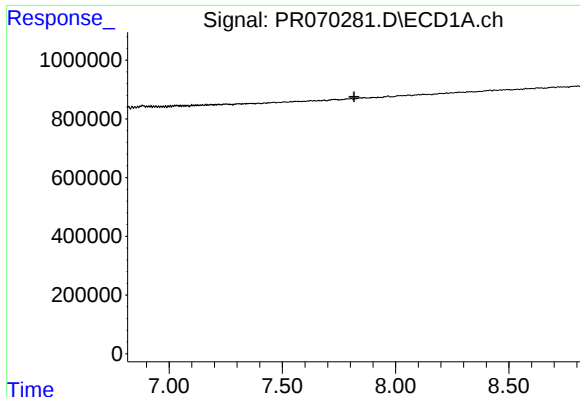

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.816 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

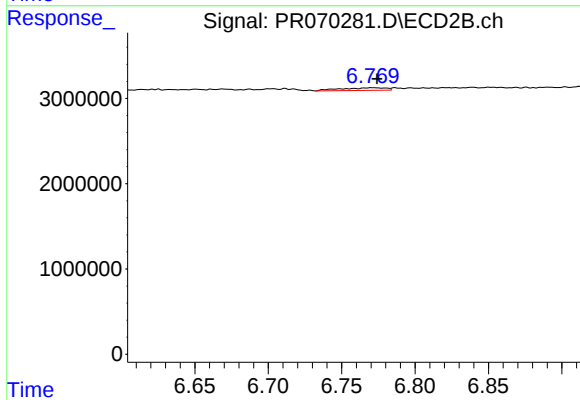


#35 AR-1260-5

R.T.: 6.771 min
Delta R.T.: -0.003 min
Response: 653697
Conc: 1.59 ng/ml

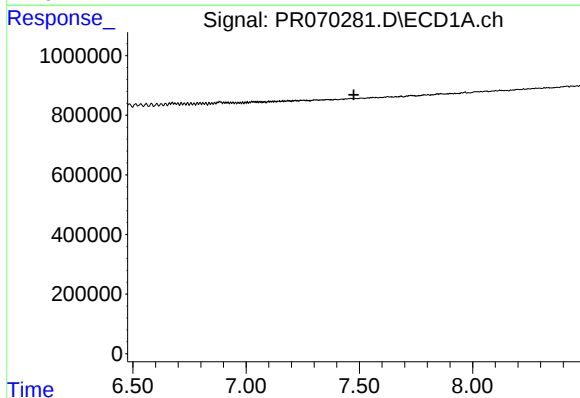


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.476 min
Response: 0
Conc: N.D.

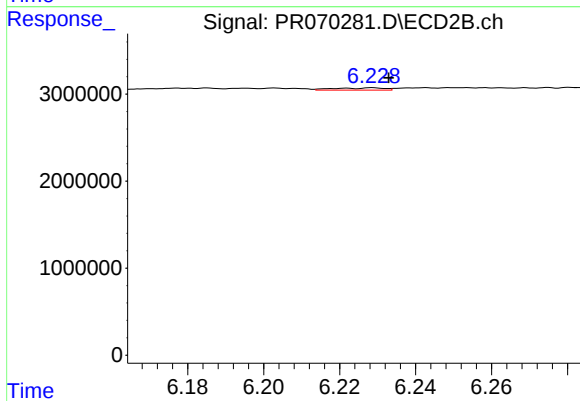

#36 AR-1262-1


R.T.: 6.229 min
Delta R.T.: -0.004 min
Response: 237530
Conc: 0.77 ng/ml

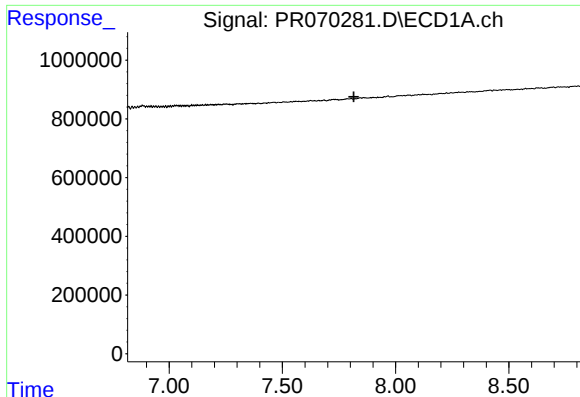

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 7.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

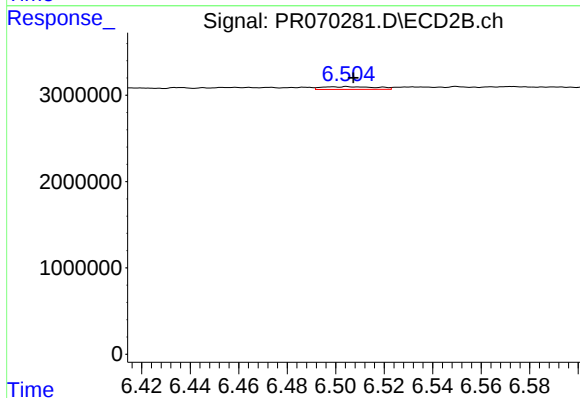


#37 AR-1262-2

R.T.: 6.505 min
Delta R.T.: -0.003 min
Response: 486810
Conc: 1.80 ng/ml

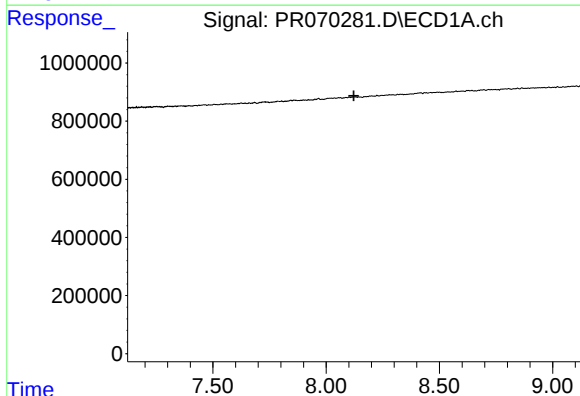


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.122 min
Response: 0
Conc: N.D.

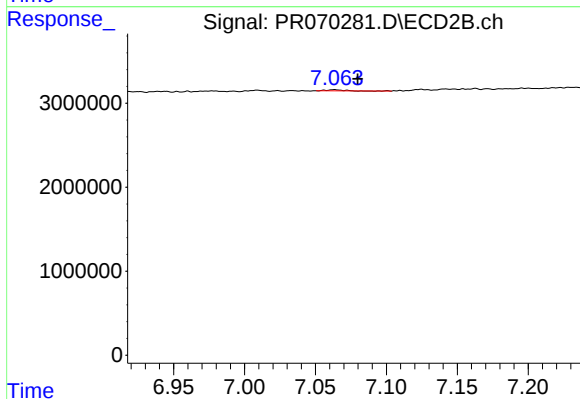

#38 AR-1262-3


R.T.: 7.063 min
Delta R.T.: -0.016 min
Response: 106127
Conc: 0.54 ng/ml

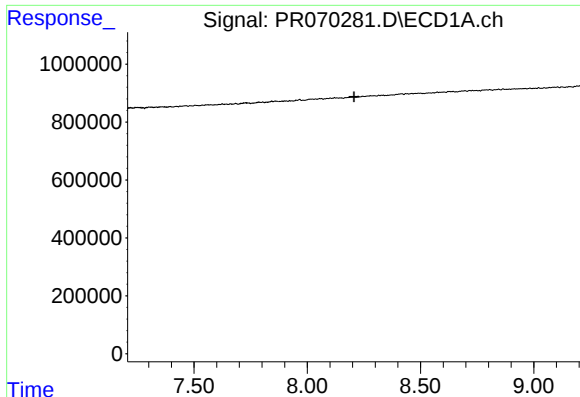

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

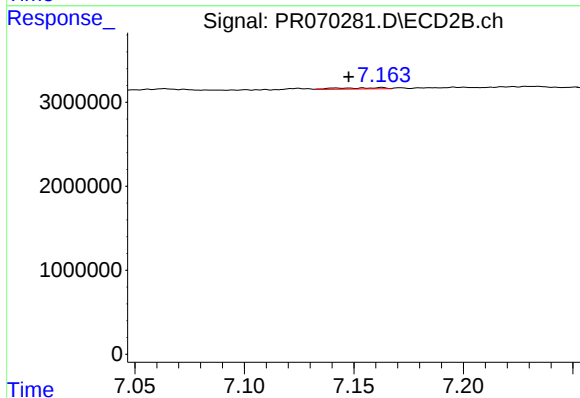


#39 AR-1262-4

R.T.: 7.163 min
Delta R.T.: 0.015 min
Response: 207161
Conc: 0.57 ng/ml

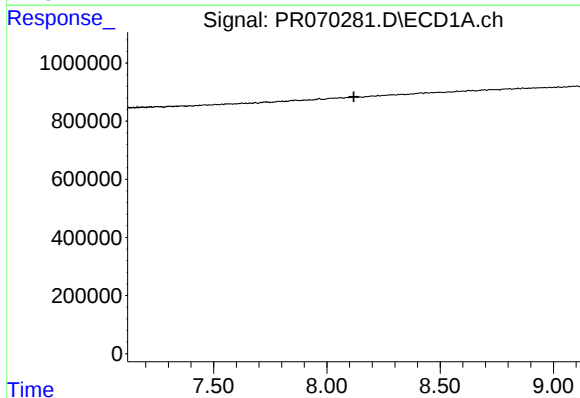


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.119 min
Response: 0
Conc: N.D.

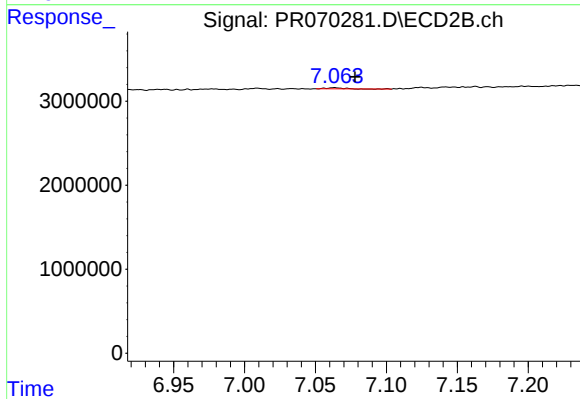

#41 AR-1268-1


R.T.: 7.063 min
Delta R.T.: -0.015 min
Response: 106127
Conc: 0.19 ng/ml

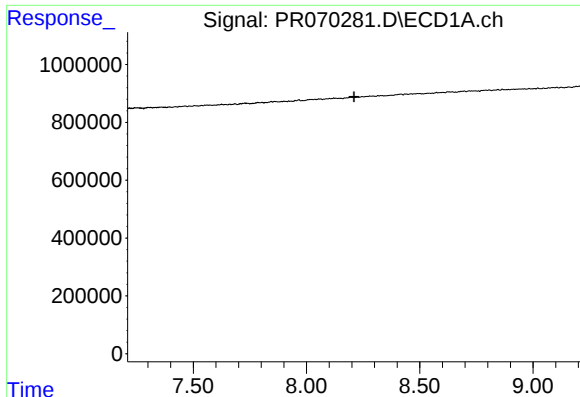

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

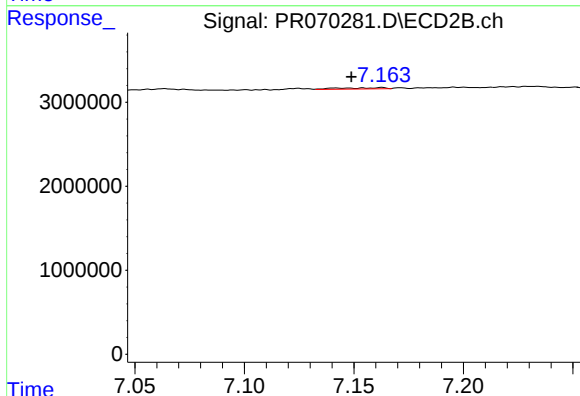


#42 AR-1268-2

R.T.: 7.163 min
Delta R.T.: 0.014 min
Response: 207161
Conc: 0.40 ng/ml

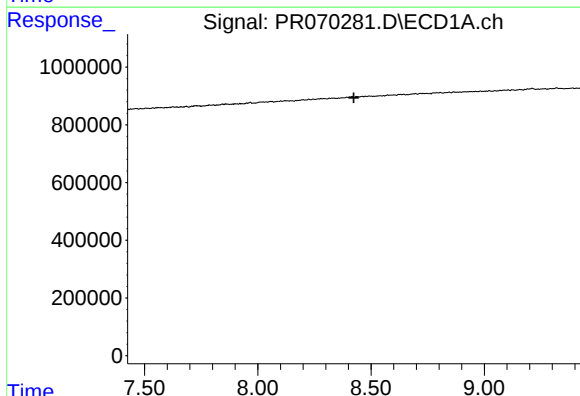


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 8.424 min
Response: 0
Conc: N.D.

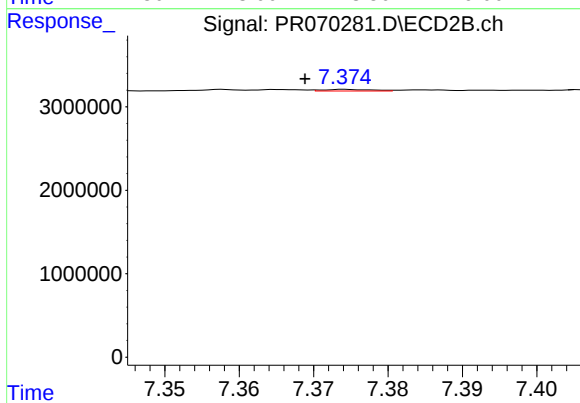

#43 AR-1268-3


R.T.: 7.374 min
Delta R.T.: 0.005 min
Response: 83930
Conc: 0.17 ng/ml

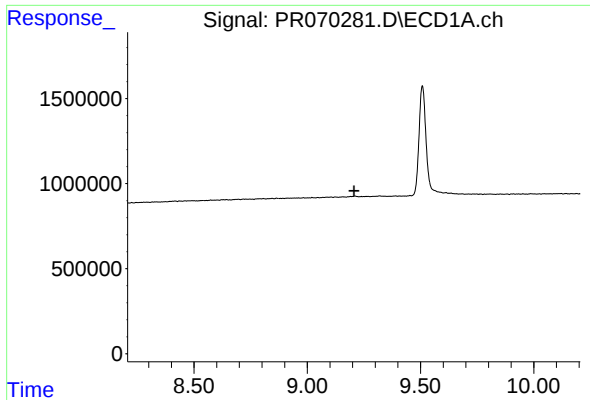

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
LOD-MDL-WATER-01-QT1-2025

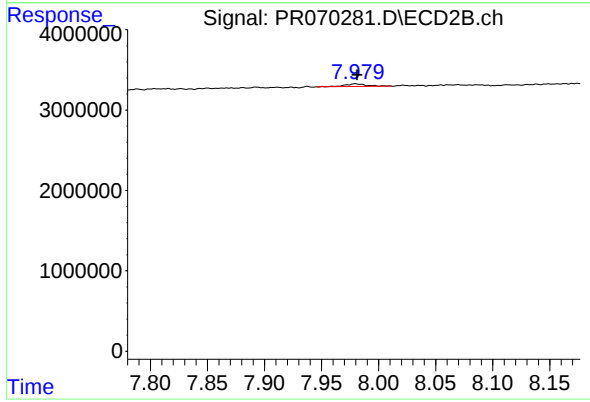

#45 AR-1268-5

R.T.: 7.981 min
Delta R.T.: 0.000 min
Response: 439670
Conc: 0.32 ng/ml