
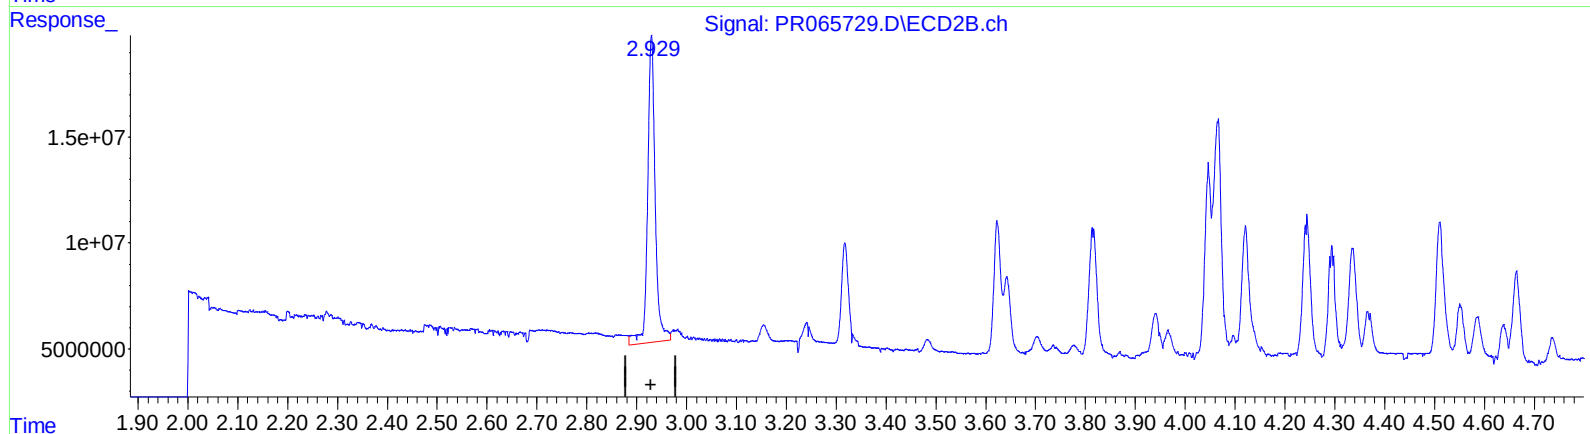


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022124\
Data File : PR065729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 12:08
Operator : AJ\MA
Sample : P1501-04MSD
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 22:07:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021624CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 17 06:03:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

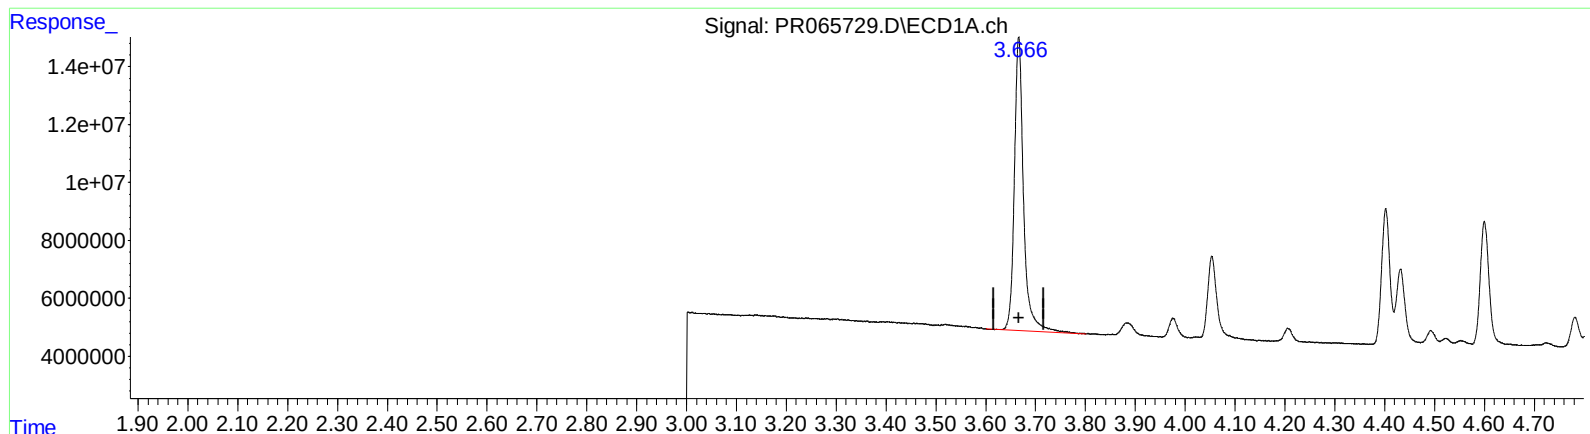

QEdit

(1) Tetrachloro-m-xylene (SA)

3.666min 22.895 ng/ml

response 130089406

(1) Tetrachloro-m-xylene #2 (SA)



2.930min 24.478 ng/ml

response 153207318

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022124\
Data File : PR065729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 12:08
Operator : AJ\MA
Sample : P1501-04MSD
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 22:07:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021624CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 17 06:03:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

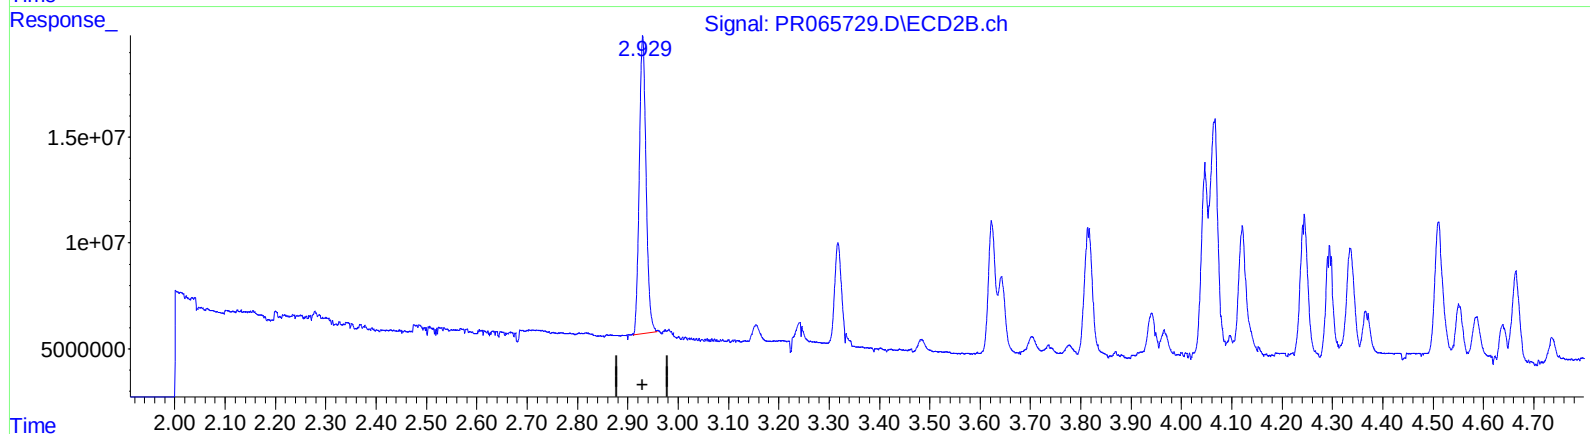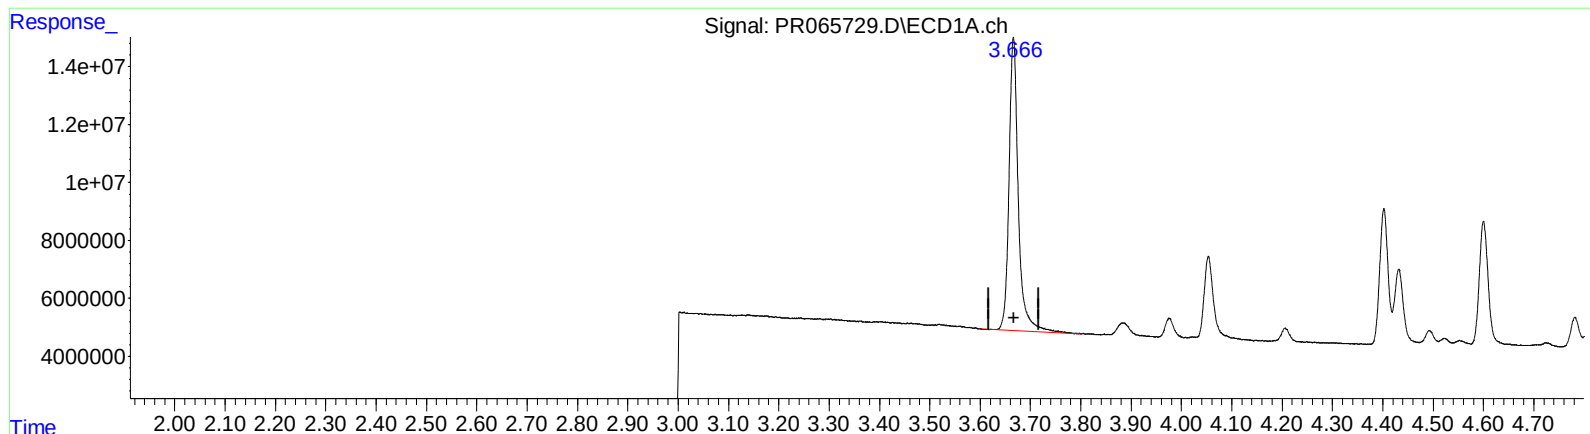

QEdit

(1) Tetrachloro-m-xylene (SA)

3.666min 22.895 ng/ml

response 130089406

(1) Tetrachloro-m-xylene #2 (SA)



2.929min 21.135 ng/ml m

response 132283726

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022124\
Data File : PR065729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 12:08
Operator : AJ\MA
Sample : P1501-04MSD
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 22:07:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021624CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 17 06:03:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

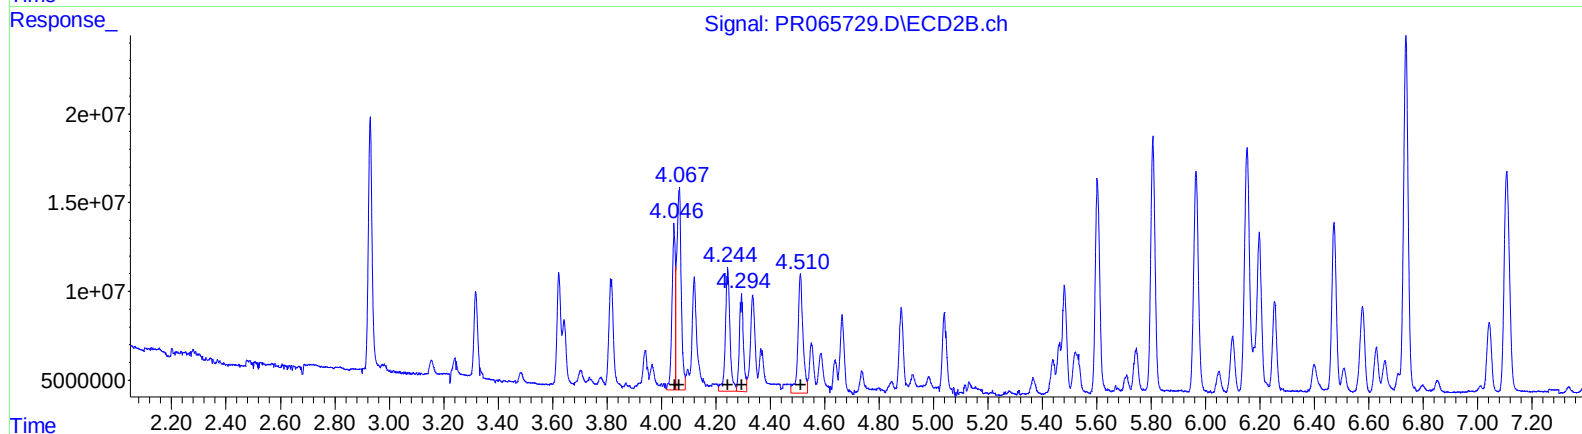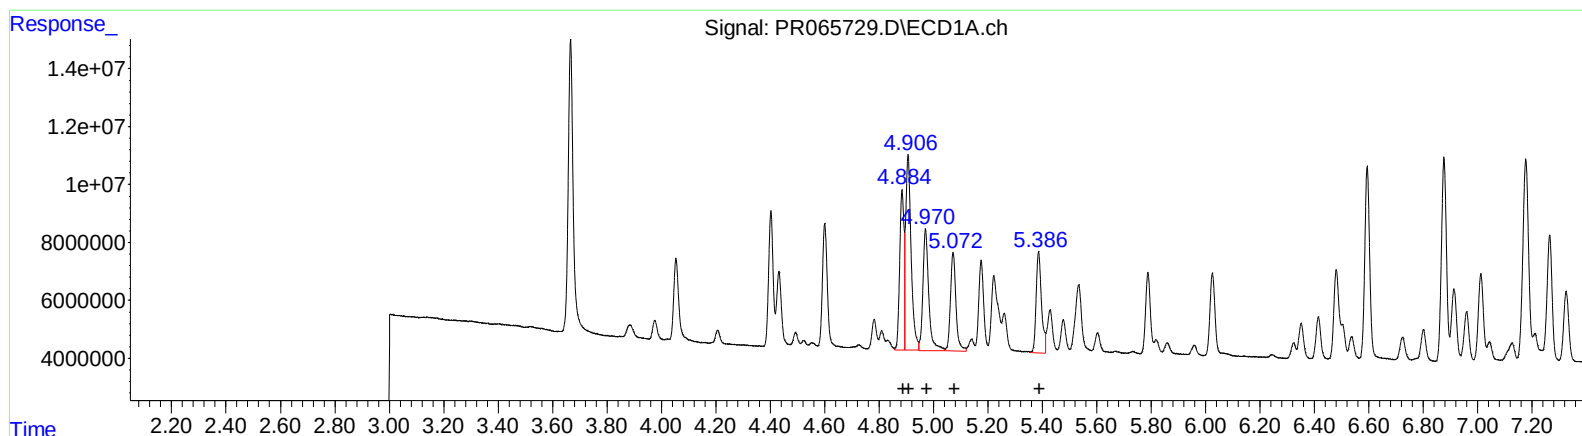

QEdit

(3) AR-1016-1 (L1)

R.T.	Response	Conc
4.88	60073845	495.70
4.91	94655636	465.26
4.97	62038151	457.84
5.07	47994058	460.06
5.39	47856077	473.36

(3) AR-1016-1 #2 (L1)


R.T.	Response	Conc
4.05	78989564	403.85
4.07	128533759	460.76
4.24	80757810	525.41
4.29	56536578	460.59
4.51	85317694	534.96

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022124\
Data File : PR065729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 12:08
Operator : AJ\MA
Sample : P1501-04MSD
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 22:07:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021624CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 17 06:03:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

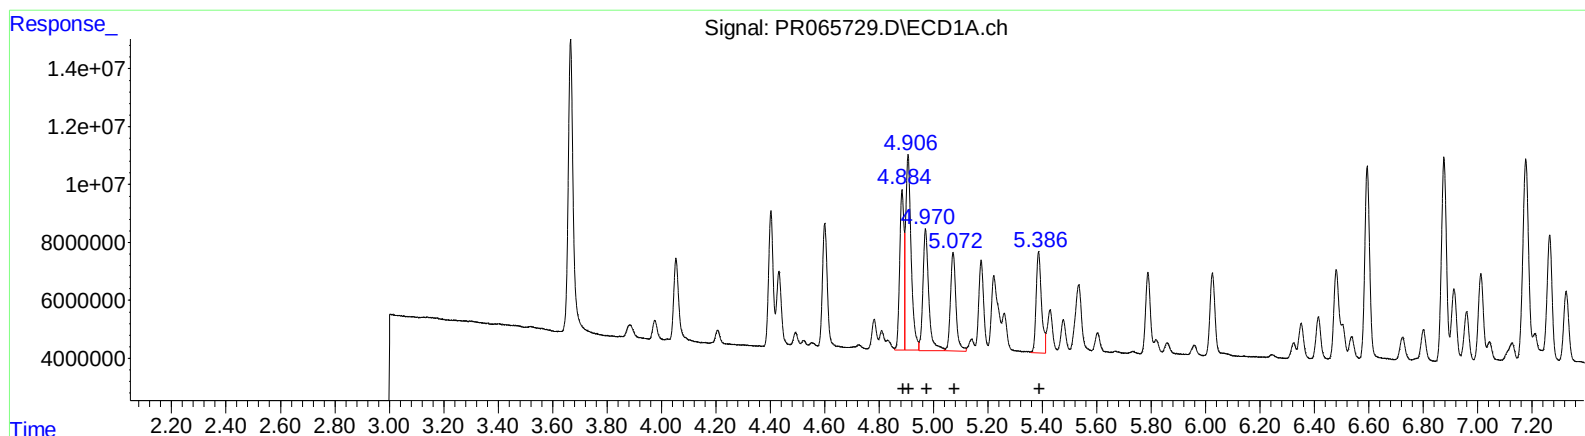

QEdit

(3) AR-1016-1 (L1)

R.T.	Response	Conc
4.88	60073845	495.70
4.91	94655636	465.26
4.97	62038151	457.84
5.07	47994058	460.06
5.39	47856077	473.36

(3) AR-1016-1 #2 (L1)

R.T.	Response	Conc
4.05	78989564	403.85
4.07	128533759	460.76
4.24	73903179	480.81
4.29	52322612	426.26
4.51	69998581	438.91

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022124\
 Data File : PR065729.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2024 12:08
 Operator : AJ\MA
 Sample : P1501-04MSD
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 22:07:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021624CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Feb 17 06:03:42 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.666	2.929	130.1E6	132.3E6	22.895	21.135m
2) SA Decachlor...	9.542	8.188	74203577	123.8E6	54.977	55.860
Target Compounds						
3) L1 AR-1016-1	4.884	4.047	60073845	78989564	495.701	403.845
4) L1 AR-1016-2	4.907	4.066	94655636	128.5E6	465.257	460.760
5) L1 AR-1016-3	4.971	4.244	62038151	73903179	457.842	480.811m
6) L1 AR-1016-4	5.072	4.294	47994058	52322612	460.058	426.262m
7) L1 AR-1016-5	5.386	4.510	47856077	69998581	473.359	438.907m
31) L7 AR-1260-1	6.594	5.602	84867073	140.1E6	486.132	473.514
32) L7 AR-1260-2	6.876	5.806	90302896	166.2E6	504.045	493.358
33) L7 AR-1260-3	7.264	5.965	60851351	157.8E6	430.166	485.118
34) L7 AR-1260-4	7.505	6.472	71308550	114.9E6	465.811	444.290
35) L7 AR-1260-5	7.841	6.736	119.4E6	238.4E6	468.355	446.845

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022124\
Data File : PR065729.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 12:08
Operator : AJ\MA
Sample : P1501-04MSD
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 22:07:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021624CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 17 06:03:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

