

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022124\
Data File : PR065730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 12:23
Operator : AJ\MA
Sample : P1501-05
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
E10A1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/22/2024
Supervised By :Ankita Jodhani 02/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 22:08:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021624CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 17 06:03:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

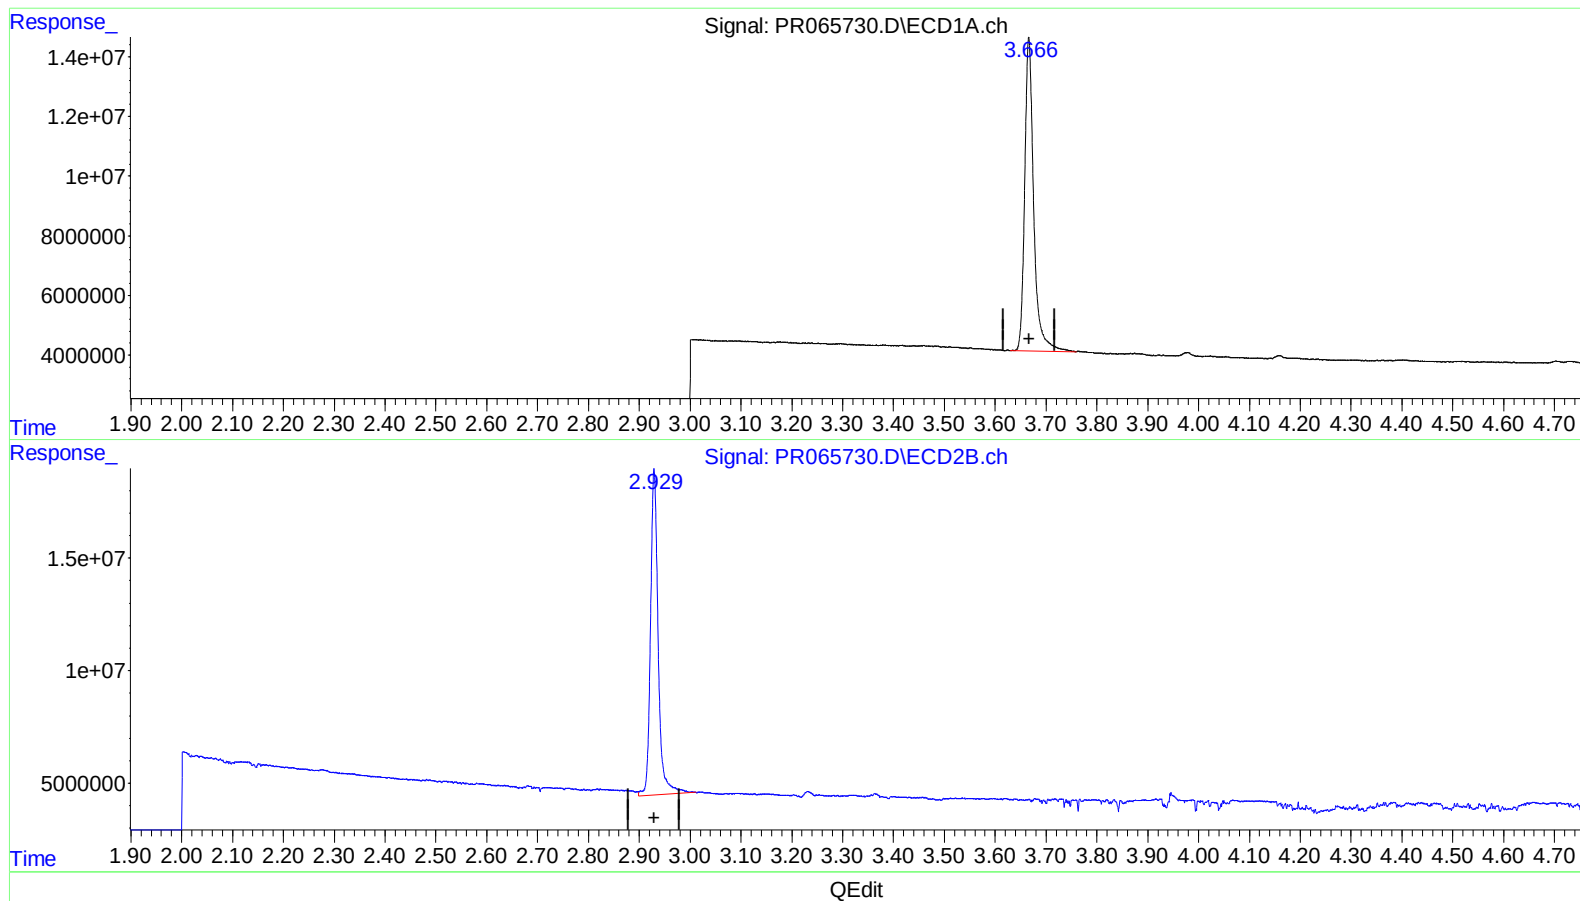

(1) Tetrachloro-m-xylene (SA)

3.666min 22.720 ng/ml

response 129095926

(1) Tetrachloro-m-xylene #2 (SA)

2.929min 24.303 ng/ml

response 152115254

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022124\
Data File : PR065730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2024 12:23
Operator : AJ\MA
Sample : P1501-05
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
E10A1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/22/2024
Supervised By :Ankita Jodhani 02/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 22:08:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR021624CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Feb 17 06:03:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

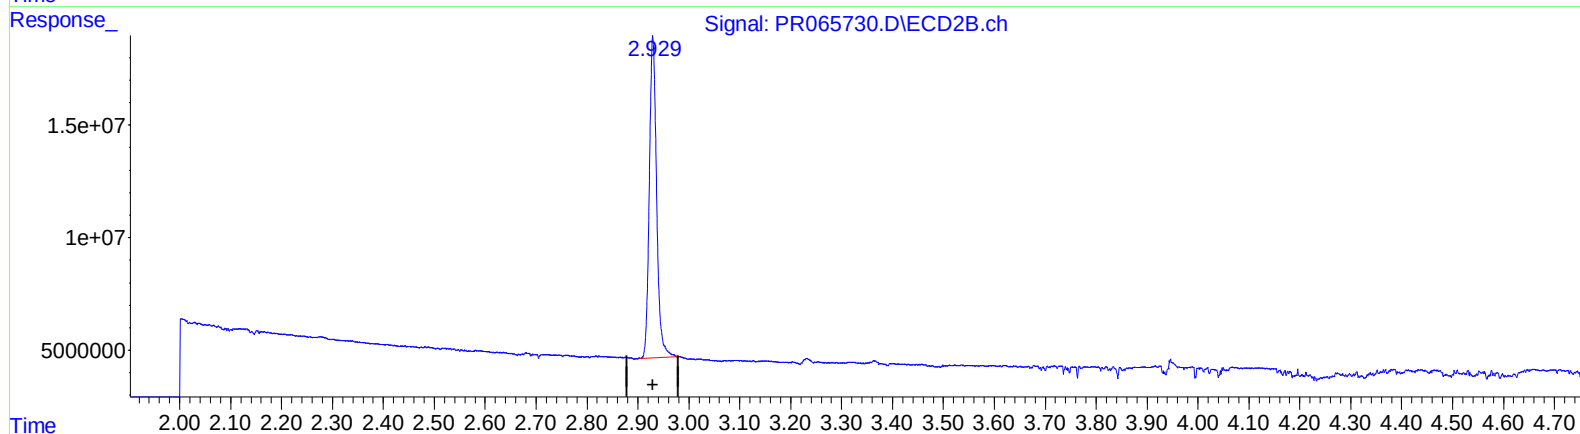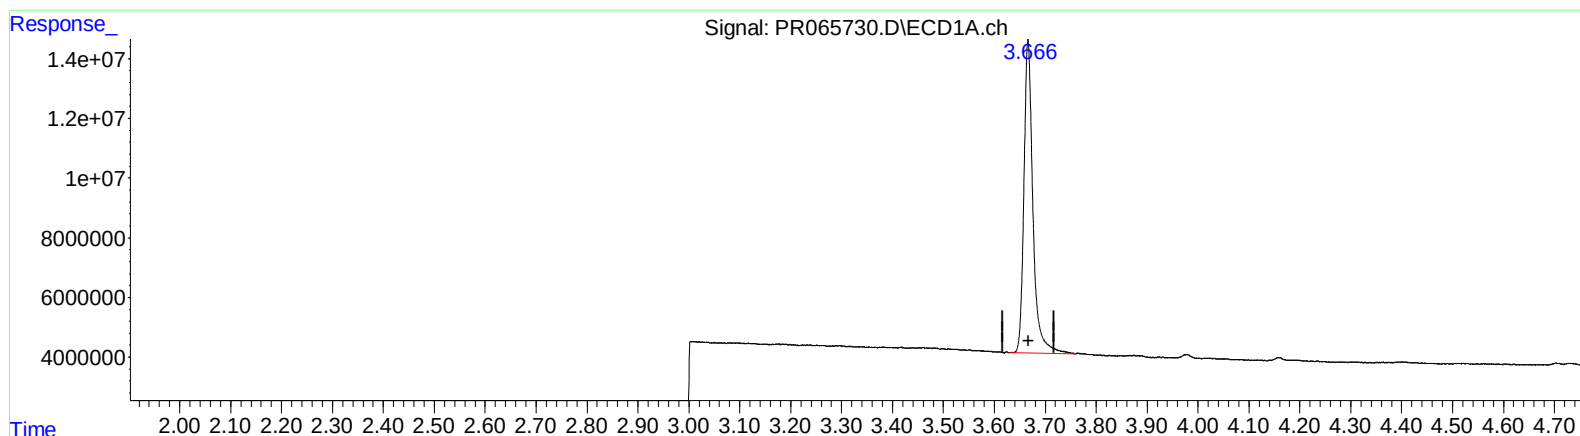

QEdit

(1) Tetrachloro-m-xylene (SA)

3.666min 22.720 ng/ml

response 129095926

(1) Tetrachloro-m-xylene #2 (SA)

2.929min 22.621 ng/ml m

response 141585195

(+) = Expected Retention Time