

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022219\
 Data File : PR035767.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Feb 2019 21:34
 Operator : SM\SJ
 Sample : AIBLK55
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 AIBLK55

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 22 22:58:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR022119CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 22 02:53:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.422	3.496	25698070	79187237	20.417	23.749
2)	SA Decachlor...	10.091	8.373	52112034	202.9E6	29.275	34.314
Target Compounds							
9)	L2 AR-1221-2	4.727	3.789	494913	1218480	43.575	35.754
10)	L2 AR-1221-3	4.727f	0.000	494913	0	12.677	N.D. #
11)	L3 AR-1232-1	4.727f	0.000	494913	0	18.738	N.D. #
29)	L6 AR-1254-4	0.000	6.049f	0	2586794	N.D.	8.123 #
31)	L7 AR-1260-1	0.000	6.049f	0	2586794	N.D.	5.180 #
32)	L7 AR-1260-2	0.000	6.179	0	2053399	N.D.	2.868 #
43)	L9 AR-1268-3	8.945	7.583	481100	1094154	1.635	0.733 #
45)	L9 AR-1268-5	9.765	8.143	527042	1218939	0.600	0.307 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022219\
Data File : PR035767.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Feb 2019 21:34
Operator : SM\SJ
Sample : AIBLK55
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
AIBLK55

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 22 22:58:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR022119CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 22 02:53:40 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

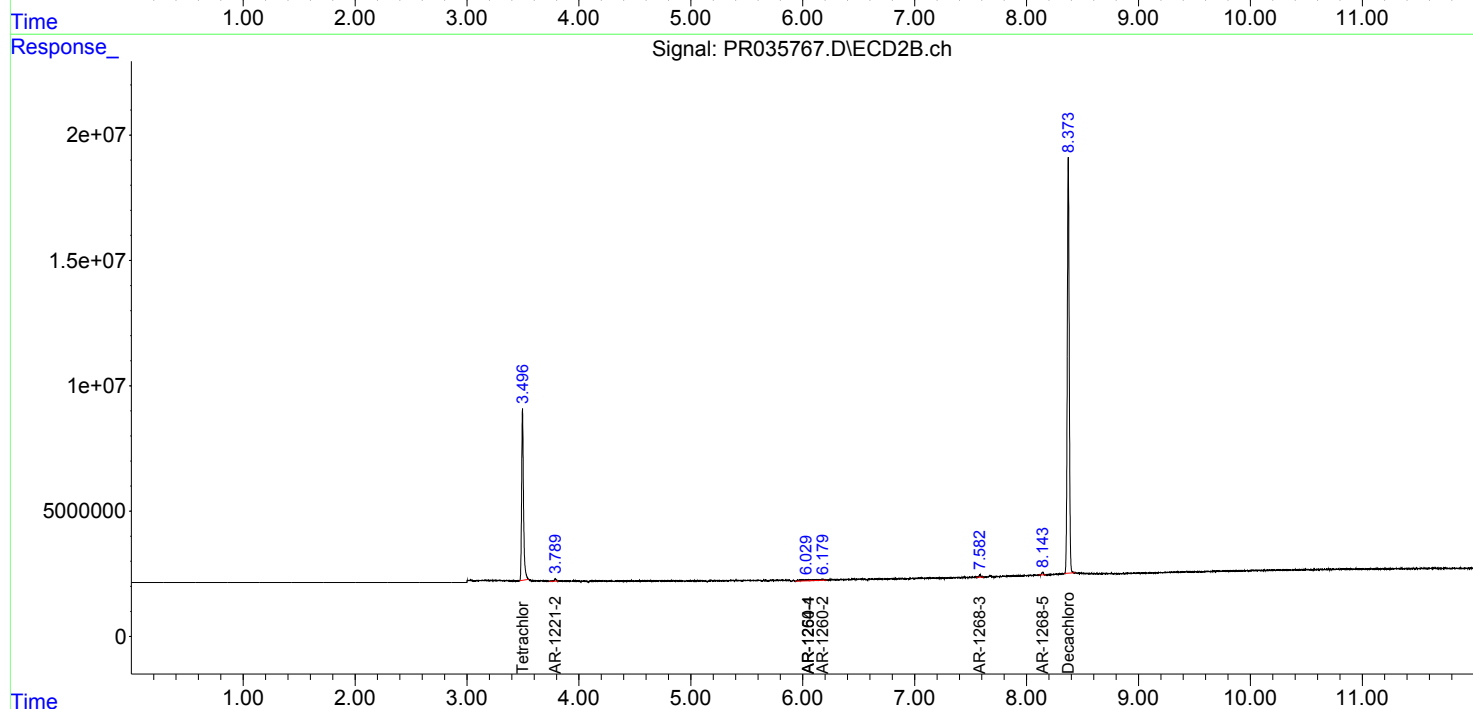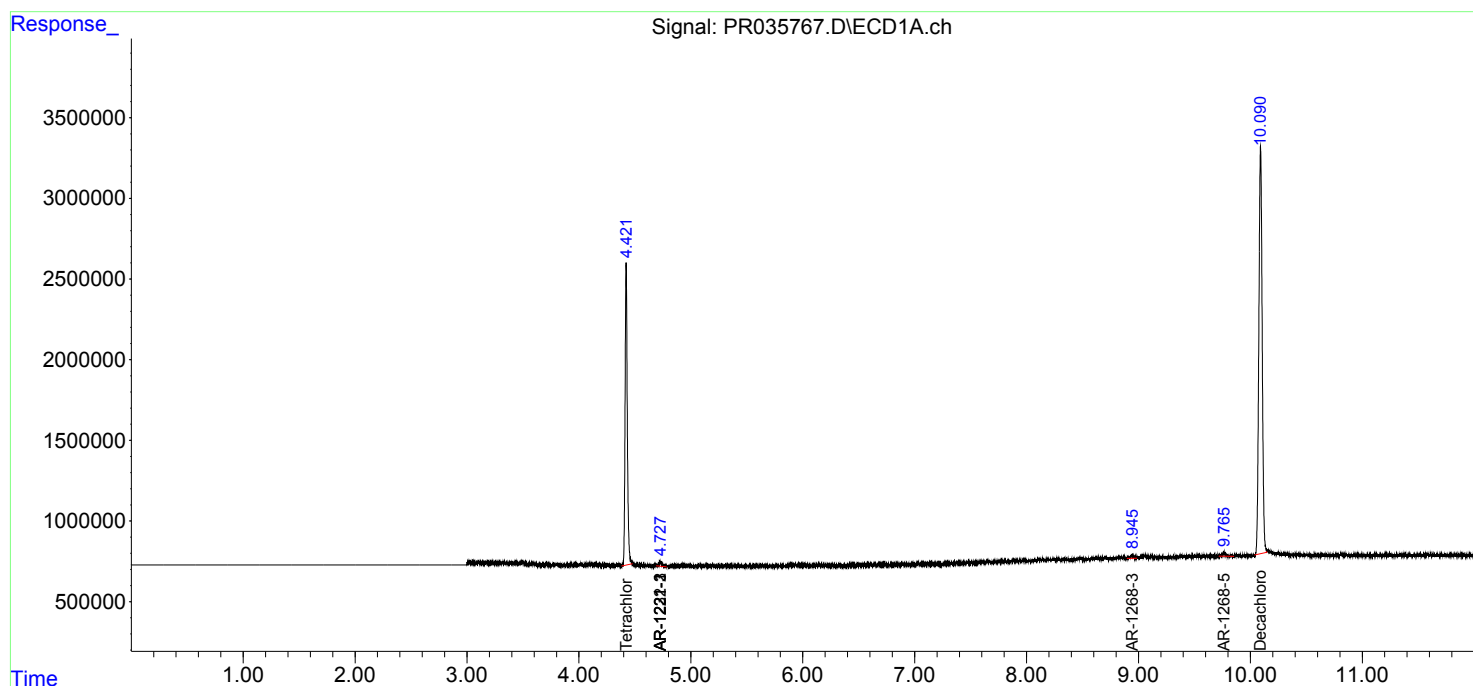


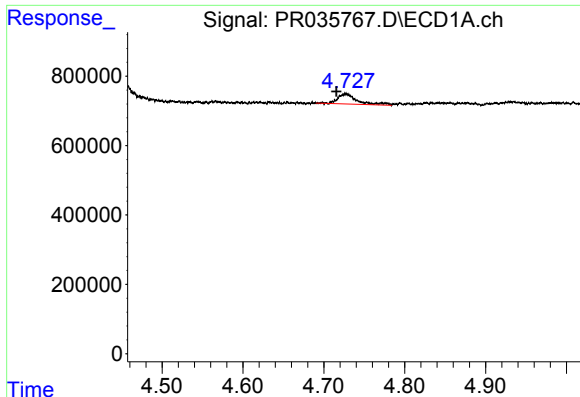

#9 AR-1221-2


R.T.: 4.727 min
Delta R.T.: 0.012 min
Response: 494913
Conc: 43.57 ng/ml

Instrument :
ECD_R
ClientSampleId :
AIBLK55

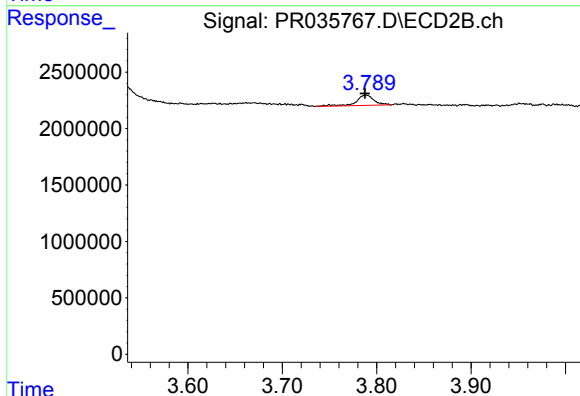


#9 AR-1221-2

R.T.: 3.789 min
Delta R.T.: 0.001 min
Response: 1218480
Conc: 35.75 ng/ml

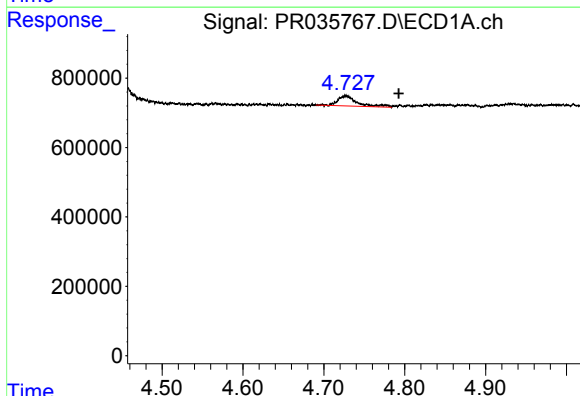


#10 AR-1221-3

R.T.: 4.727 min
Delta R.T.: -0.065 min
Response: 494913
Conc: 12.68 ng/ml

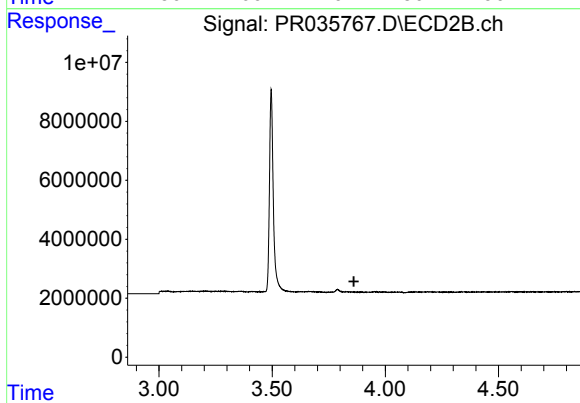

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 3.861 min
Response: 0
Conc: N.D.

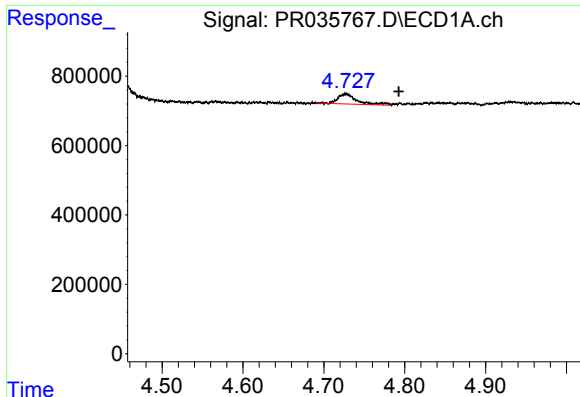

#11 AR-1232-1


R.T.: 4.727 min
Delta R.T.: -0.066 min
Response: 494913
Conc: 18.74 ng/ml

Instrument :
ECD_R
ClientSampleId :
AIBLK55

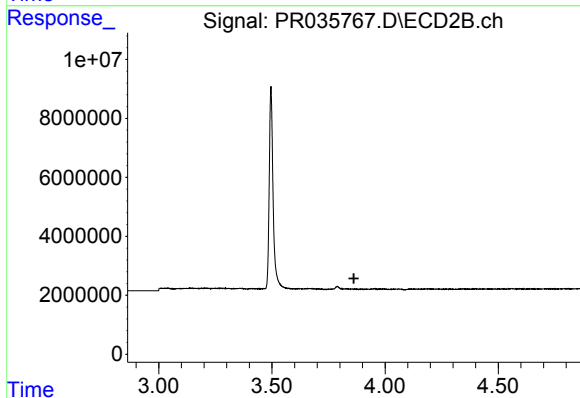


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.862 min
Response: 0
Conc: N.D.

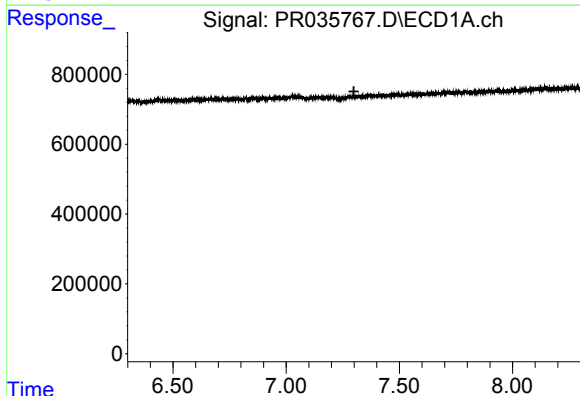


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.299 min
Response: 0
Conc: N.D.

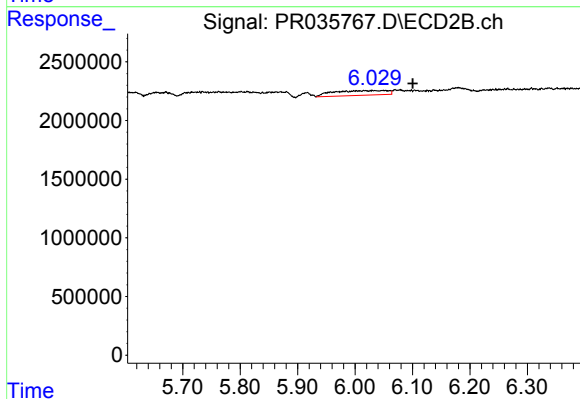

#29 AR-1254-4


R.T.: 6.049 min
Delta R.T.: -0.052 min
Response: 2586794
Conc: 8.12 ng/ml

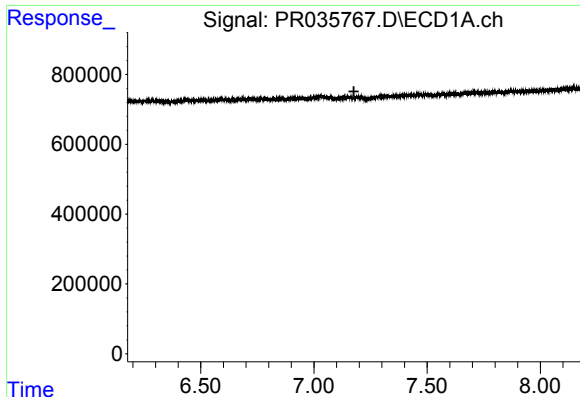

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.176 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
AIBLK55

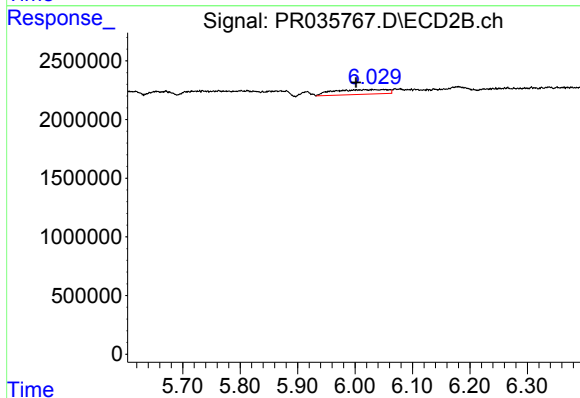


#31 AR-1260-1

R.T.: 6.049 min
Delta R.T.: 0.047 min
Response: 2586794
Conc: 5.18 ng/ml

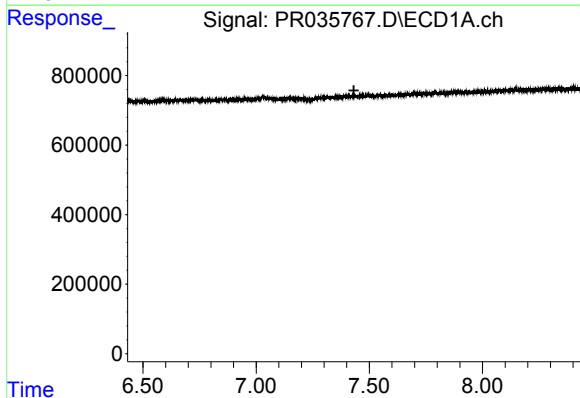


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

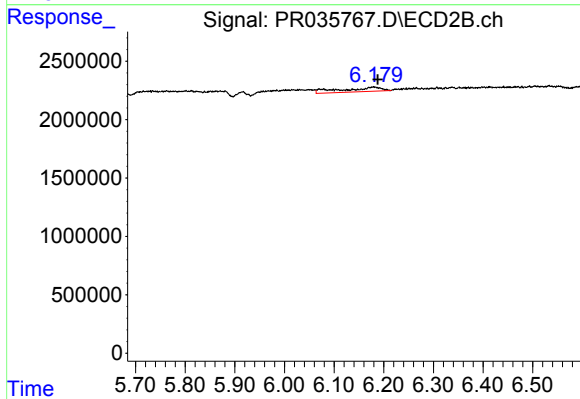

#32 AR-1260-2


R.T.: 6.179 min
Delta R.T.: -0.009 min
Response: 2053399
Conc: 2.87 ng/ml

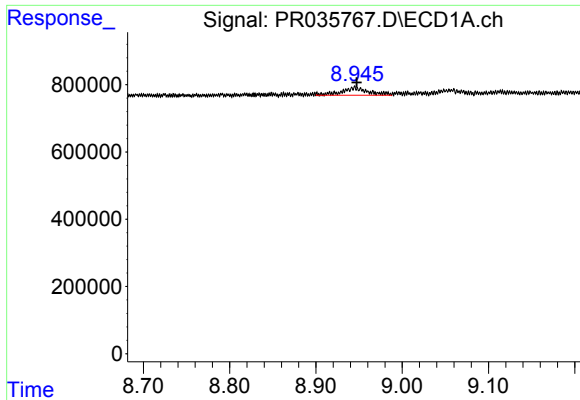

#43 AR-1268-3


R.T.: 8.945 min
Delta R.T.: -0.002 min
Response: 481100
Conc: 1.64 ng/ml

Instrument :
ECD_R
ClientSampleId :
AIBLK55

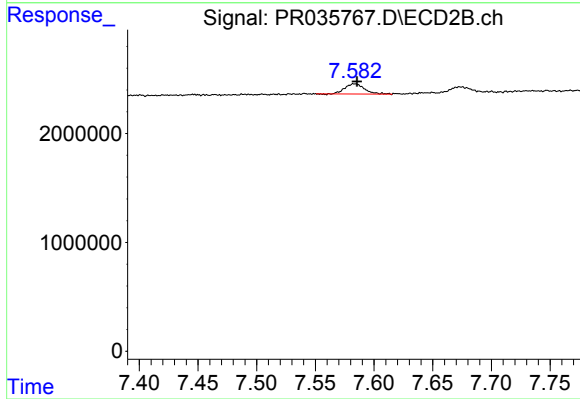


#43 AR-1268-3

R.T.: 7.583 min
Delta R.T.: -0.002 min
Response: 1094154
Conc: 0.73 ng/ml

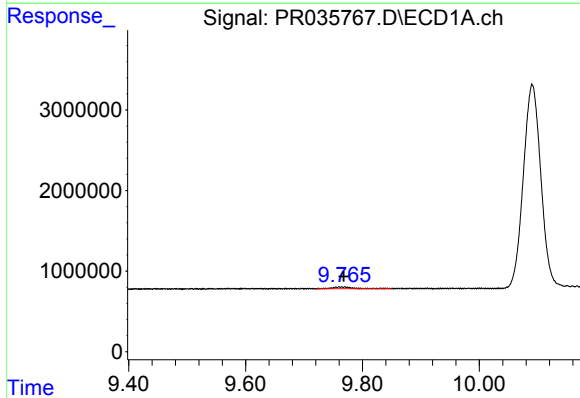

#45 AR-1268-5

R.T.: 9.765 min
Delta R.T.: -0.003 min
Response: 527042
Conc: 0.60 ng/ml

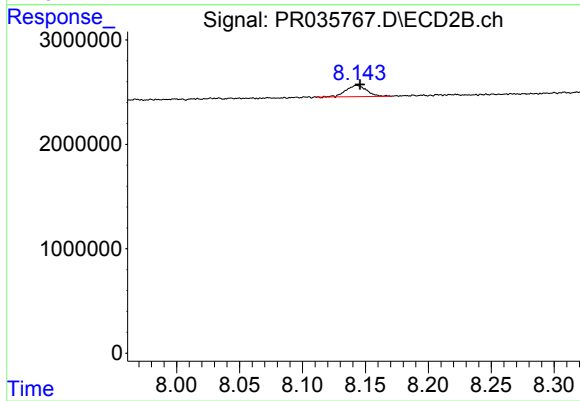

#45 AR-1268-5

R.T.: 8.143 min
Delta R.T.: -0.003 min
Response: 1218939
Conc: 0.31 ng/ml