

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022423\
 Data File : PR059793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2023 08:00
 Operator : YP\AJ
 Sample : 01627-09 (Sig #1); 01627-08 (Sig #2)
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 05:01:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR022423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 24 12:41:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.690	2.906	58743400	84820724	19.662	19.596
2) SA Decachlor...	9.658	8.137	52921087	75933202	23.072	21.524
Target Compounds						
11) L3 AR-1232-1	4.082	3.291	2091321	2433097	30.068	26.299
12) L3 AR-1232-2	4.636	4.034	899608	2421831	27.653	27.477
13) L3 AR-1232-3	4.947	4.212	1687892	1225429	28.839	27.430
14) L3 AR-1232-4	5.114	4.304	791203	1146269	26.706	28.540
15) L3 AR-1232-5	5.217	4.478	587103	1227366	26.127m	26.855



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022423\
Data File : PR059793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2023 08:00
Operator : YP\AJ
Sample : 01627-09 (Sig #1); 01627-08 (Sig #2)
Misc : AR1232 MDL 25 PPB
ALS Vial : 66 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 05:01:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR022423.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 24 12:41:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

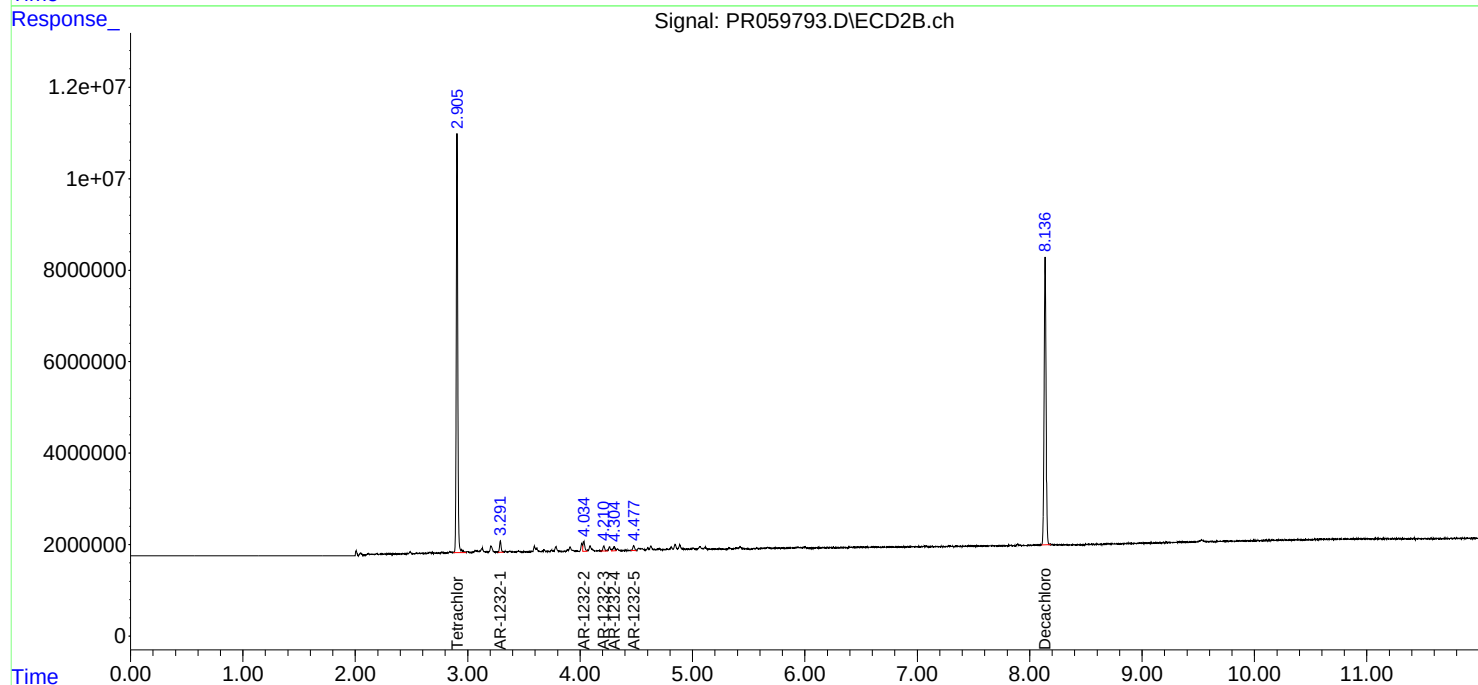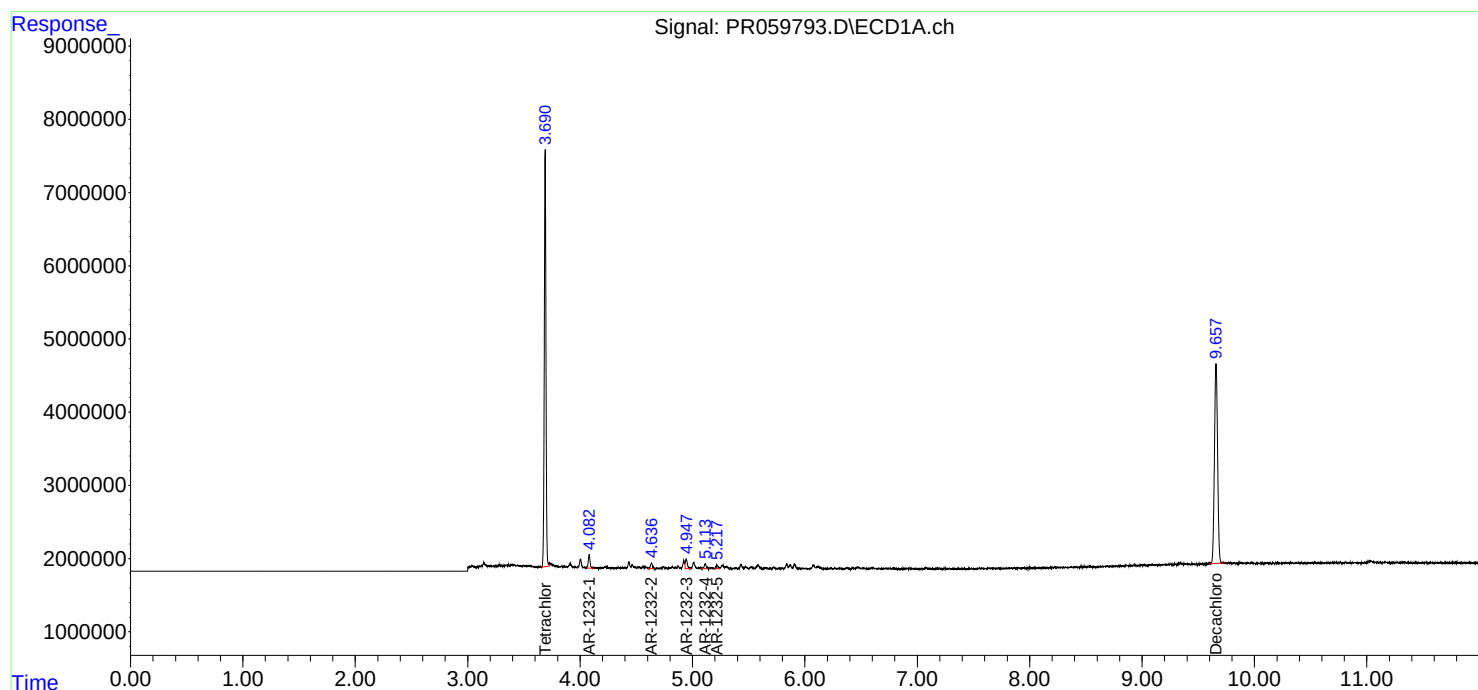


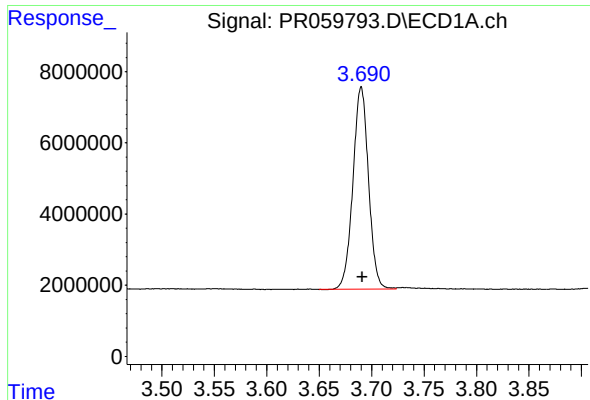

#1 Tetrachloro-m-xylene


R.T.: 3.690 min
Delta R.T.: 0.000 min
Response: 58743400
Conc: 19.66 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2023

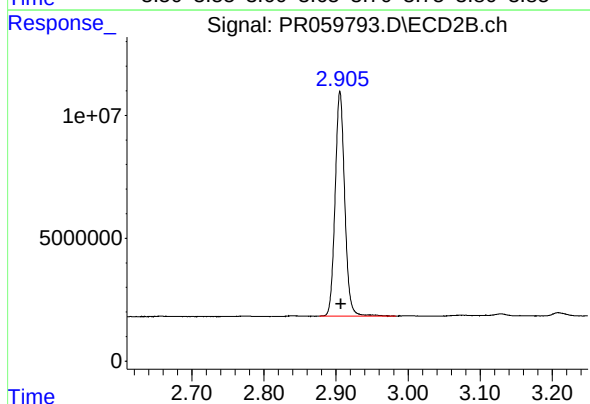


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 84820724
Conc: 19.60 ng/ml

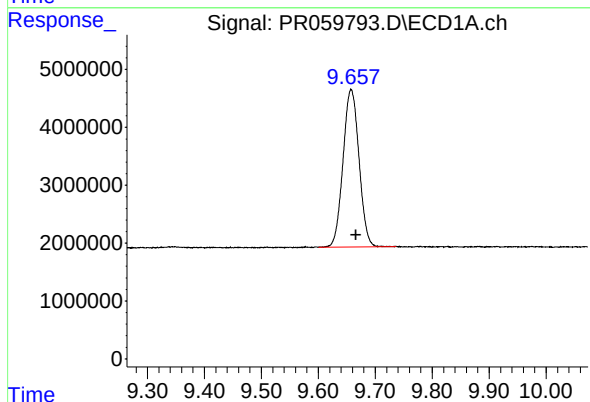


#2 Decachlorobiphenyl

R.T.: 9.658 min
Delta R.T.: -0.008 min
Response: 52921087
Conc: 23.07 ng/ml

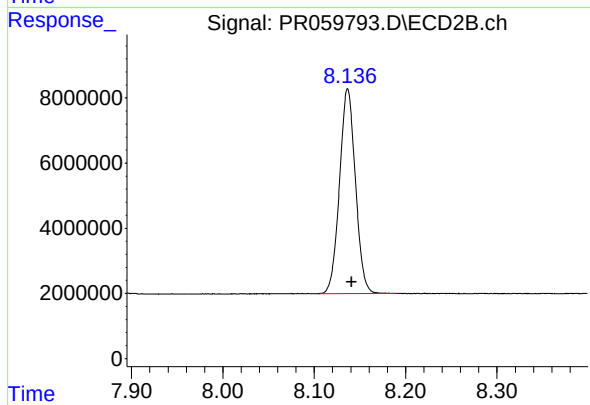

#2 Decachlorobiphenyl


R.T.: 8.137 min
Delta R.T.: -0.004 min
Response: 75933202
Conc: 21.52 ng/ml

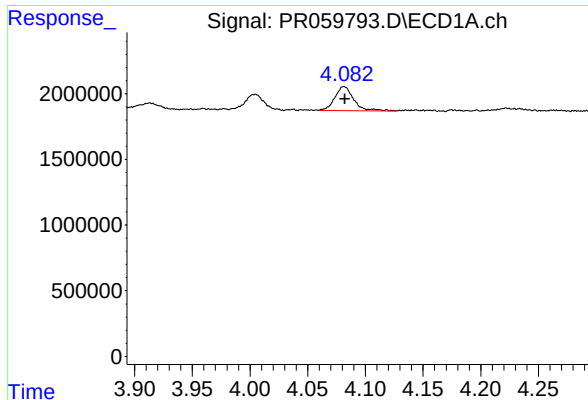

#11 AR-1232-1


R.T.: 4.082 min
Delta R.T.: 0.000 min
Response: 2091321
Conc: 30.07 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2023

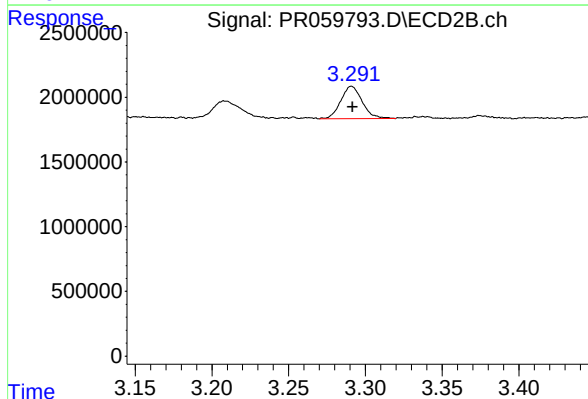


#11 AR-1232-1

R.T.: 3.291 min
Delta R.T.: 0.000 min
Response: 2433097
Conc: 26.30 ng/ml

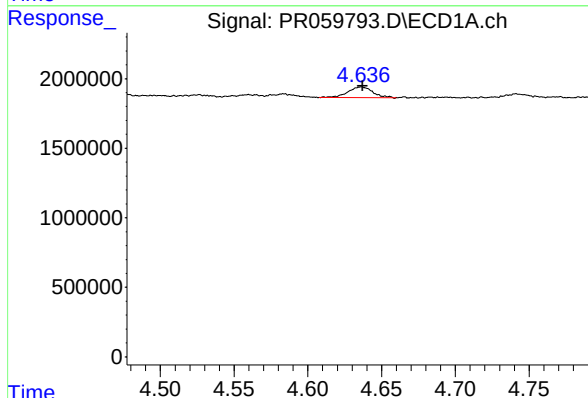


#12 AR-1232-2

R.T.: 4.636 min
Delta R.T.: 0.000 min
Response: 899608
Conc: 27.65 ng/ml

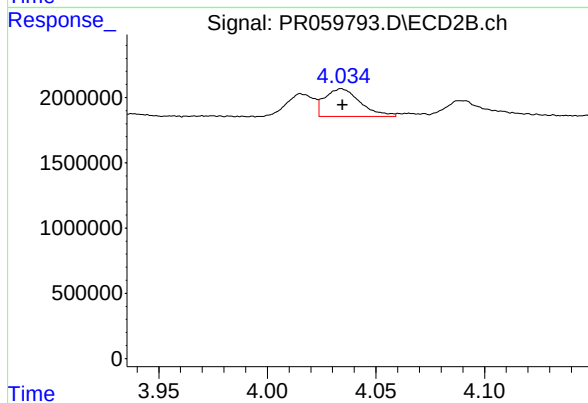

#12 AR-1232-2


R.T.: 4.034 min
Delta R.T.: 0.000 min
Response: 2421831
Conc: 27.48 ng/ml

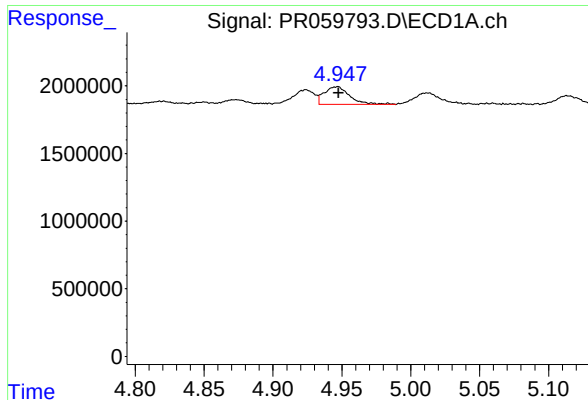

#13 AR-1232-3


R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 1687892
Conc: 28.84 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2023

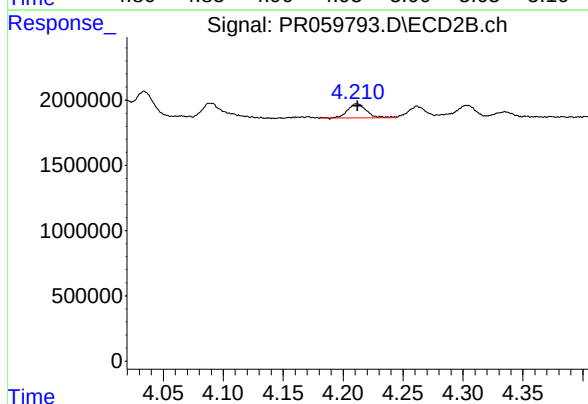


#13 AR-1232-3

R.T.: 4.212 min
Delta R.T.: 0.000 min
Response: 1225429
Conc: 27.43 ng/ml

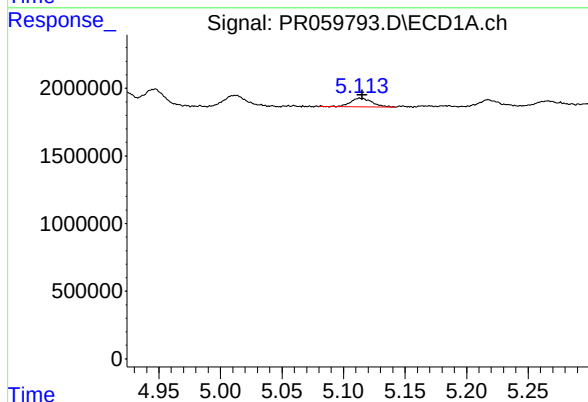


#14 AR-1232-4

R.T.: 5.114 min
Delta R.T.: -0.002 min
Response: 791203
Conc: 26.71 ng/ml

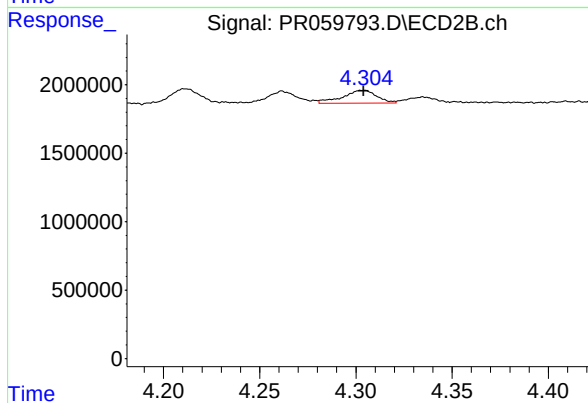

#14 AR-1232-4


R.T.: 4.304 min
Delta R.T.: 0.000 min
Response: 1146269
Conc: 28.54 ng/ml

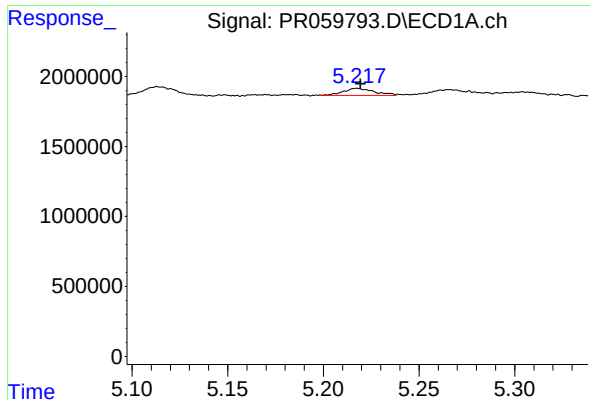

#15 AR-1232-5

R.T.: 5.217 min
Delta R.T.: -0.002 min
Response: 587103
Conc: 26.13 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2023

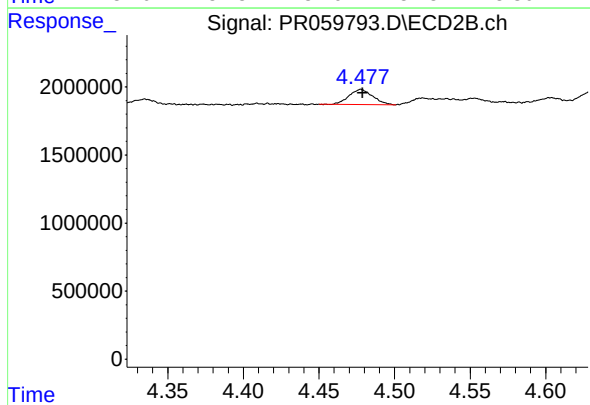

#15 AR-1232-5

R.T.: 4.478 min
Delta R.T.: 0.000 min
Response: 1227366
Conc: 26.85 ng/ml