

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022423\
 Data File : PR059796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2023 08:44
 Operator : YP\AJ
 Sample : 01627-09 (Sig #1); 01627-08 (Sig #2)
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 MDL-WATER-03-QT1-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 05:06:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR022423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 24 12:41:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.689	2.906	58198140	84136679	19.479	19.438
2) SA Decachlor...	9.658	8.137	51310117	75155571	22.370	21.304
Target Compounds						
26) L6 AR-1254-1	5.839	4.846	3179479	6182963	34.148	27.242
27) L6 AR-1254-2	6.078	5.004	4785439	5478454	33.859	28.105
28) L6 AR-1254-3	6.473	5.424	4687730	8387666	31.916	26.989
29) L6 AR-1254-4	6.787	5.670	3282916	5028190	30.960	27.869
30) L6 AR-1254-5	7.245	6.113	3746231	7403519	31.491	26.911



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR022423\
Data File : PR059796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2023 08:44
Operator : YP\AJ
Sample : 01627-09 (Sig #1); 01627-08 (Sig #2)
Misc : AR1254 MDL 25 PPB
ALS Vial : 69 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 05:06:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR022423.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 24 12:41:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

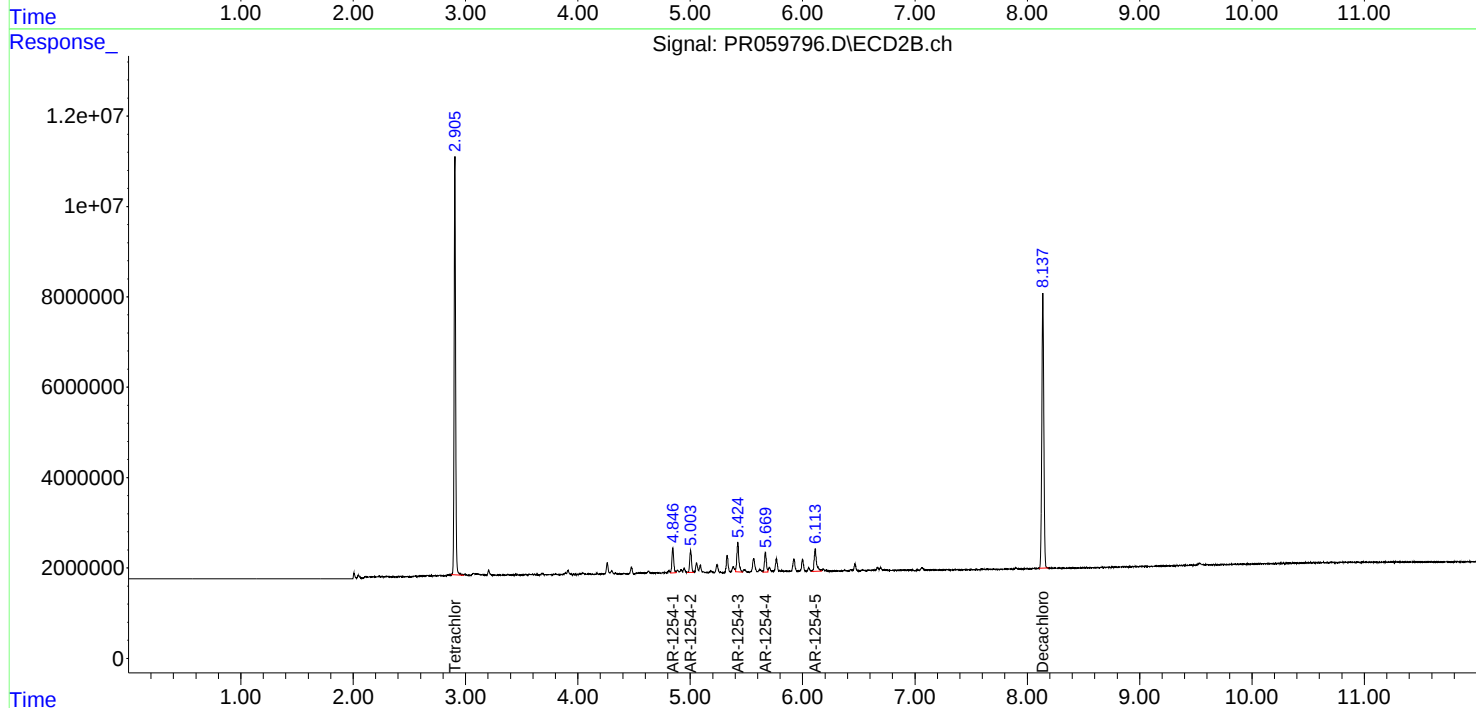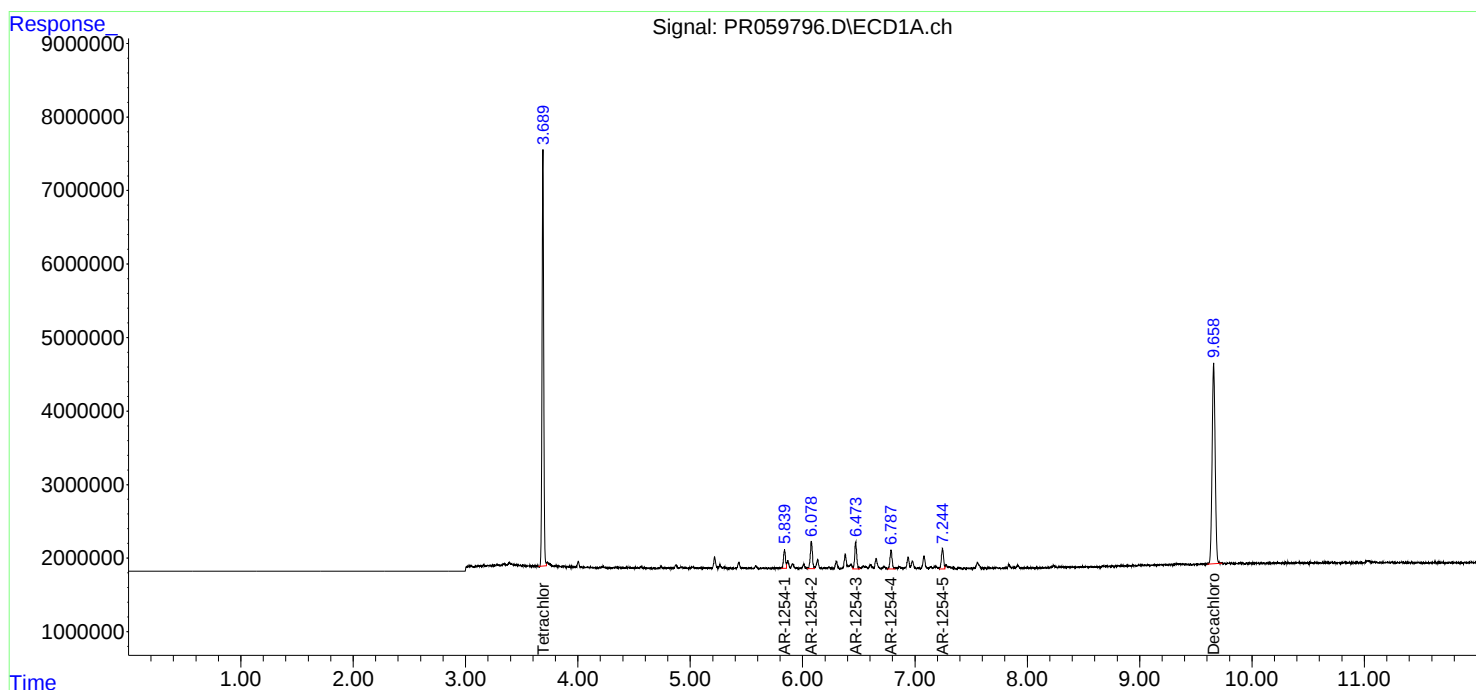


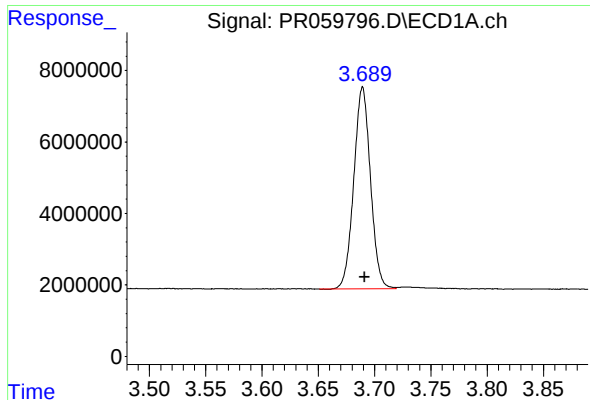

#1 Tetrachloro-m-xylene


R.T.: 3.689 min
Delta R.T.: -0.002 min
Response: 58198140
Conc: 19.48 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2023

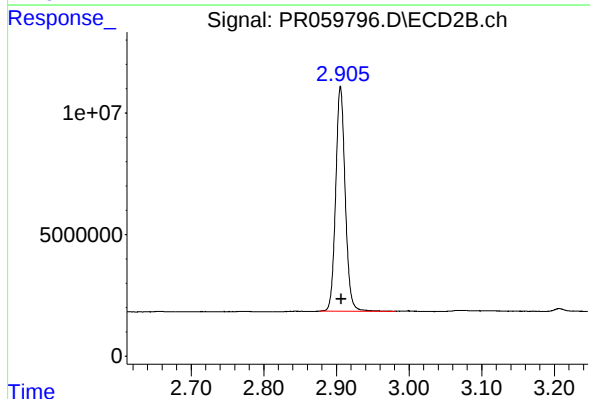


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 84136679
Conc: 19.44 ng/ml

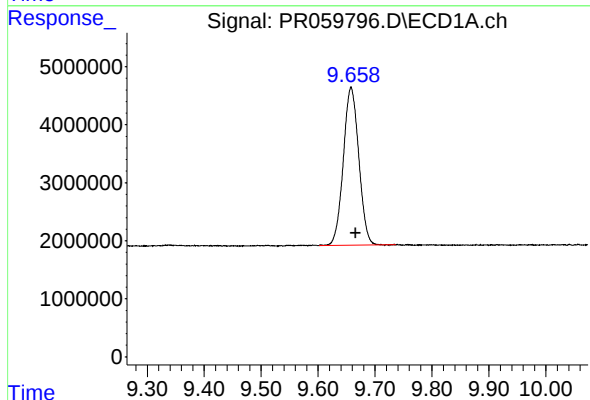


#2 Decachlorobiphenyl

R.T.: 9.658 min
Delta R.T.: -0.008 min
Response: 51310117
Conc: 22.37 ng/ml

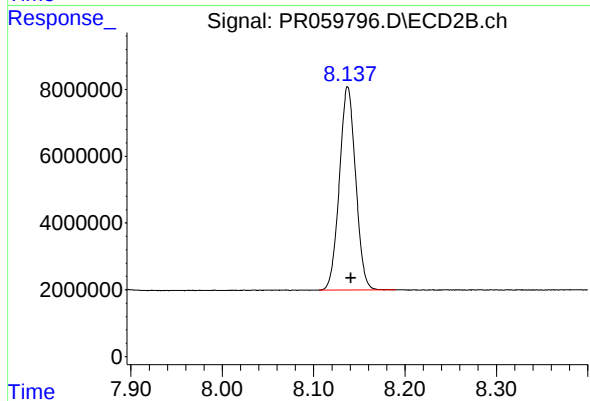

#2 Decachlorobiphenyl


R.T.: 8.137 min
Delta R.T.: -0.004 min
Response: 75155571
Conc: 21.30 ng/ml

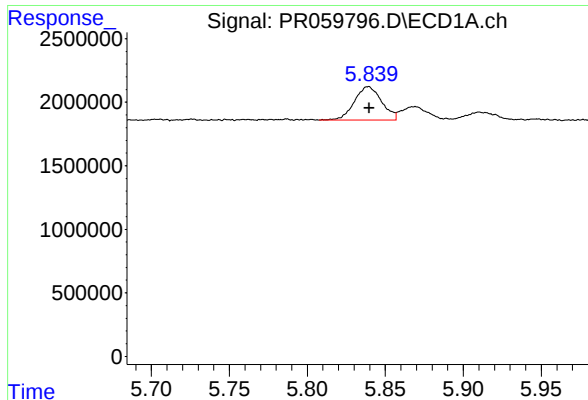

#26 AR-1254-1


R.T.: 5.839 min
Delta R.T.: 0.000 min
Response: 3179479
Conc: 34.15 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2023

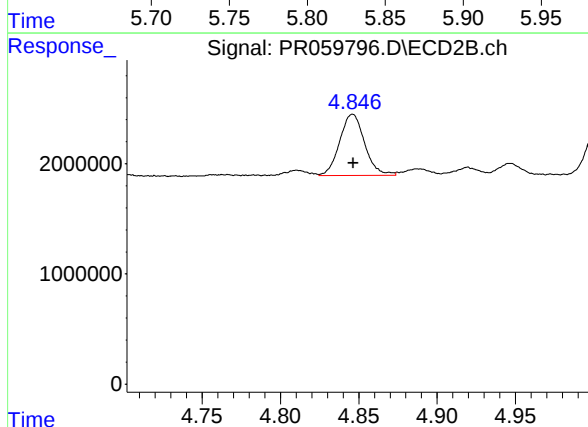


#26 AR-1254-1

R.T.: 4.846 min
Delta R.T.: 0.000 min
Response: 6182963
Conc: 27.24 ng/ml

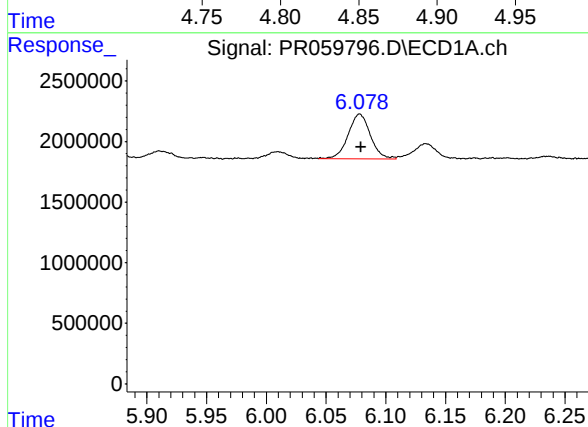


#27 AR-1254-2

R.T.: 6.078 min
Delta R.T.: -0.001 min
Response: 4785439
Conc: 33.86 ng/ml

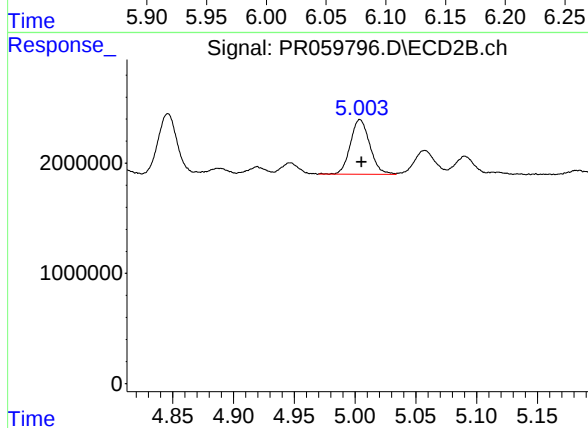

#27 AR-1254-2


R.T.: 5.004 min
Delta R.T.: -0.001 min
Response: 5478454
Conc: 28.11 ng/ml

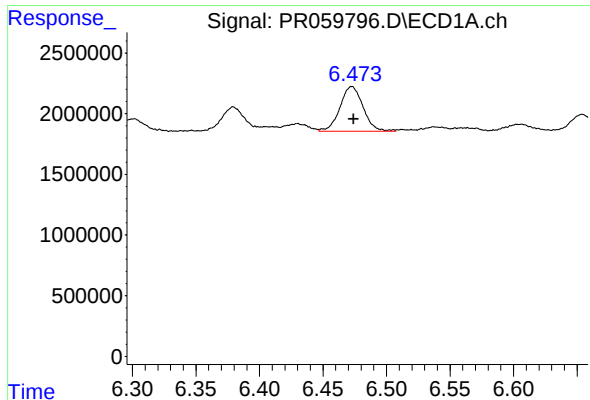

#28 AR-1254-3


R.T.: 6.473 min
Delta R.T.: -0.001 min
Response: 4687730
Conc: 31.92 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2023

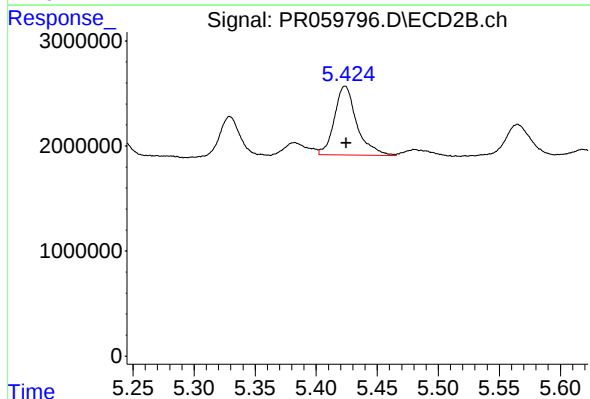


#28 AR-1254-3

R.T.: 5.424 min
Delta R.T.: -0.001 min
Response: 8387666
Conc: 26.99 ng/ml

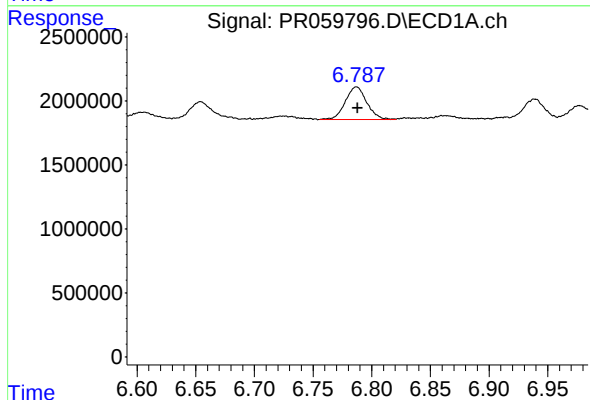


#29 AR-1254-4

R.T.: 6.787 min
Delta R.T.: 0.000 min
Response: 3282916
Conc: 30.96 ng/ml

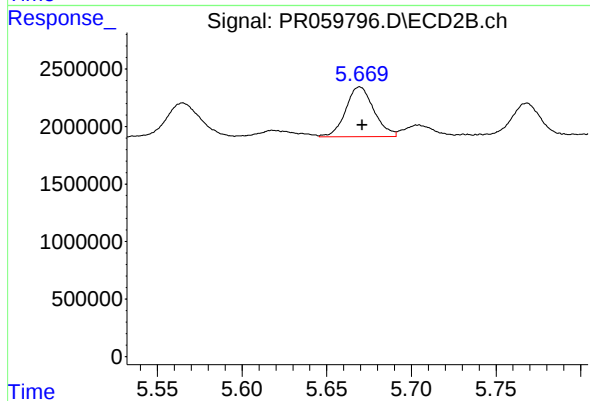

#29 AR-1254-4


R.T.: 5.670 min
Delta R.T.: -0.001 min
Response: 5028190
Conc: 27.87 ng/ml

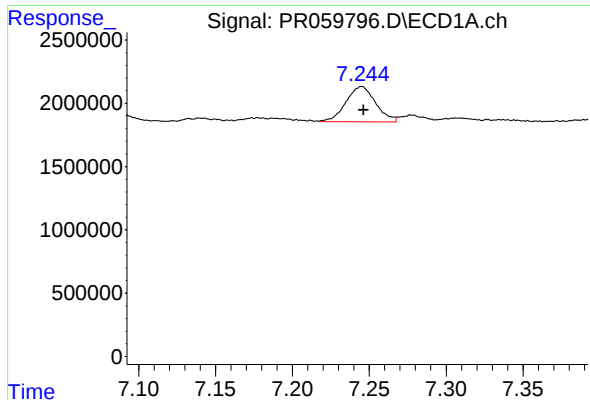

#30 AR-1254-5

R.T.: 7.245 min
Delta R.T.: -0.001 min
Response: 3746231
Conc: 31.49 ng/ml

Instrument :
ECD_R
ClientSampleId :
MDL-WATER-03-QT1-2023

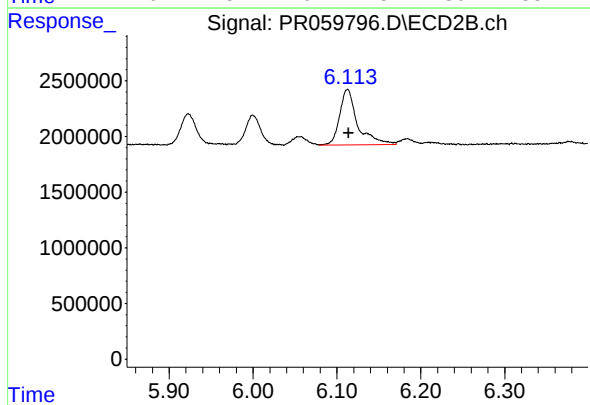

#30 AR-1254-5

R.T.: 6.113 min
Delta R.T.: -0.001 min
Response: 7403519
Conc: 26.91 ng/ml